

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
 Data File : PS000726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 19:19
 Operator : UA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:48:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.817	11.201	281.4E6	256.4E6	747.166	753.509
Target Compounds							
1) T	Dalapon	3.174	2.554	350.3E6	301.0E6	684.971	690.508
2) T	3,5-DICHL...	10.232	9.345	385.5E6	327.8E6	714.253	712.612
3) T	4-Nitroph...	11.415	10.348	157.7E6	132.8E6	670.925	677.487
5) T	DICAMBA	12.136	11.490	1047.7E6	932.5E6	741.203	752.639
6) T	MCPD	12.474	11.716	78440500	65940769	69.268	68.727
7) T	MCPA	12.726	12.094	117.3E6	94511395	66.720	68.242
8) T	DICHLORPROP	13.328	12.614	267.1E6	232.6E6	709.999	722.502
9) T	2,4-D	13.686	13.086	345.4E6	311.0E6	722.088	731.770
10) T	Pentachlo...	14.084	13.649	3932.4E6	3638.4E6	749.024	769.101
11) T	2,4,5-TP ...	14.949	14.258	1621.8E6	1481.4E6	747.076	761.263
12) T	2,4,5-T	15.347	14.833	1594.0E6	1110.1E6	740.288	656.446
13) T	2,4-DB	16.100	15.478	208.2E6	178.0E6	707.011	718.980
14) T	DINOSEB	17.611	15.911	1080.0E6	967.5E6	725.240	741.612
15) T	Picloram	17.368	17.155	1790.7E6	1565.6E6	613.153	627.656
16) T	DCPA	17.949	17.097	1924.5E6	1792.4E6	751.027	777.296



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070218\
Data File : PS000726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 19:19
Operator : UA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:48:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

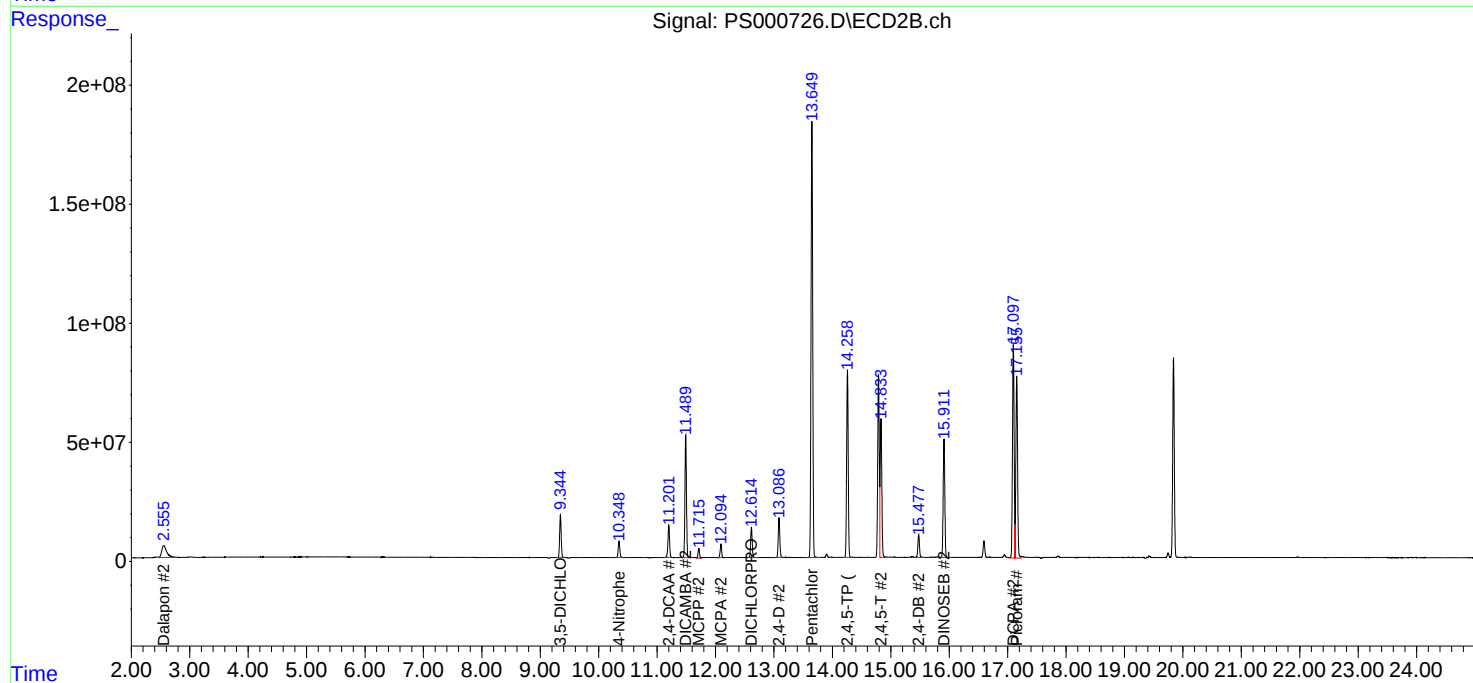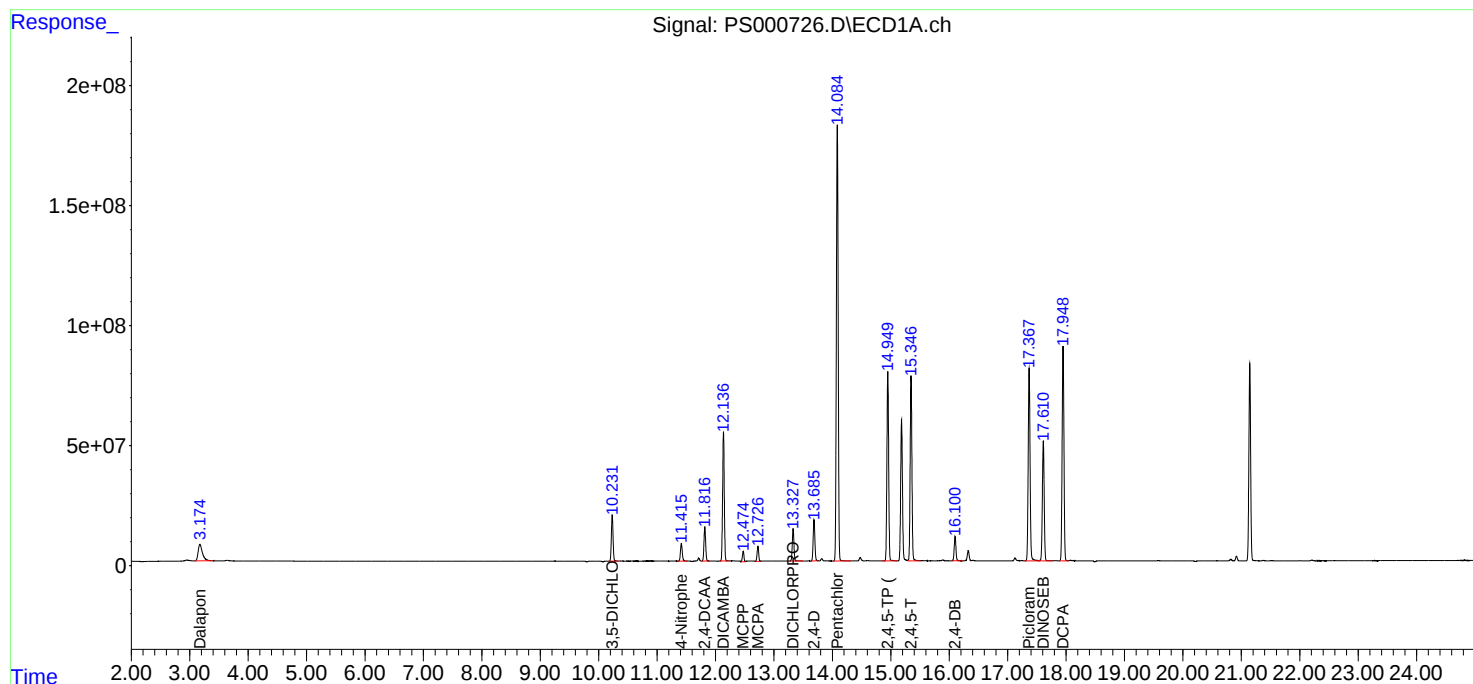


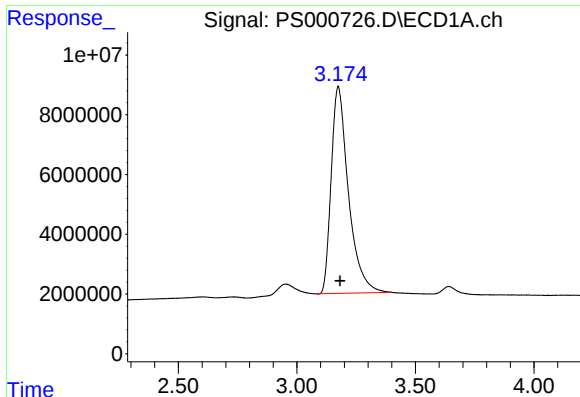

#1 Dalapon


R.T.: 3.174 min
Delta R.T.: -0.008 min
Response: 350335732
Conc: 684.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

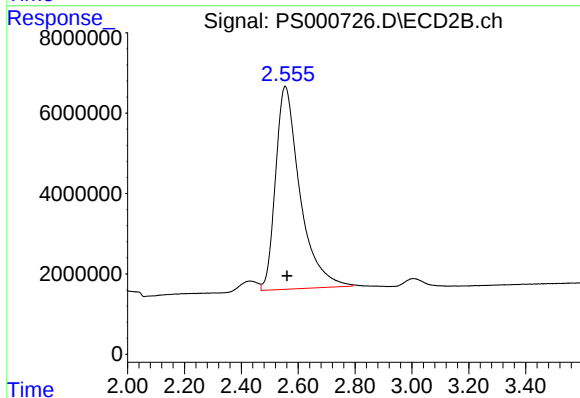


#1 Dalapon

R.T.: 2.554 min
Delta R.T.: -0.006 min
Response: 301014846
Conc: 690.51 ng/ml

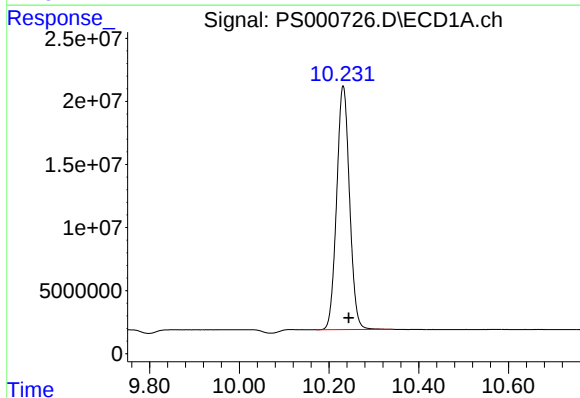


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.232 min
Delta R.T.: -0.012 min
Response: 385465548
Conc: 714.25 ng/ml

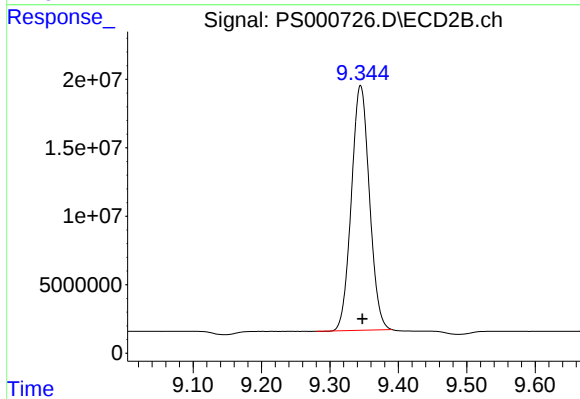

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.345 min
Delta R.T.: -0.003 min
Response: 327830794
Conc: 712.61 ng/ml

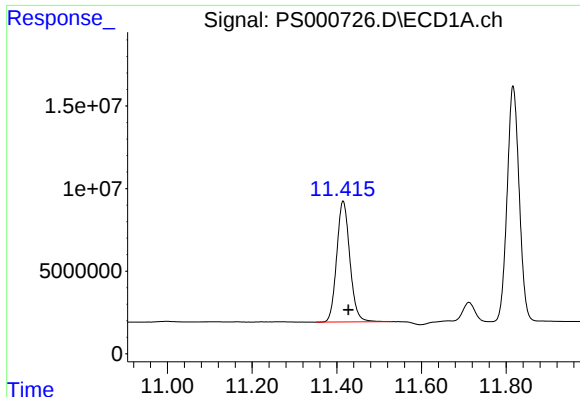

#3 4-Nitrophenol


R.T.: 11.415 min
Delta R.T.: -0.013 min
Response: 157714750
Conc: 670.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

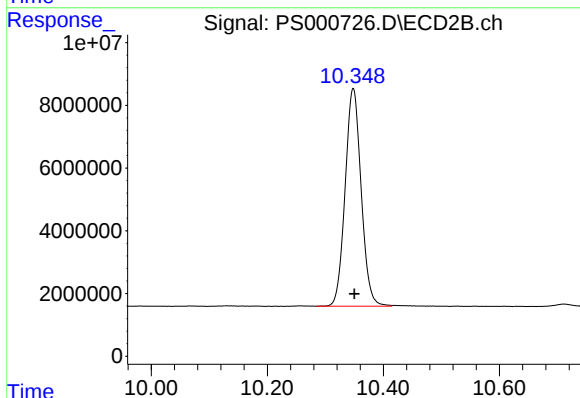


#3 4-Nitrophenol

R.T.: 10.348 min
Delta R.T.: -0.002 min
Response: 132761522
Conc: 677.49 ng/ml

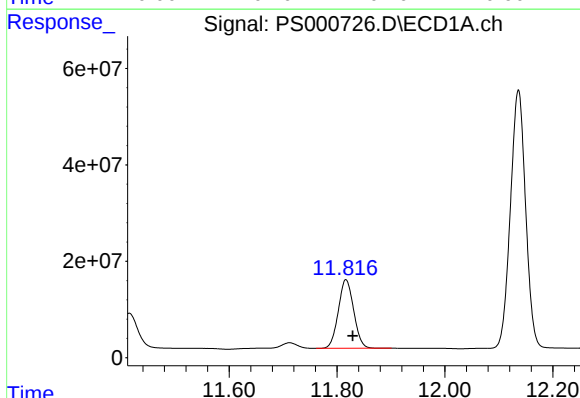


#4 2,4-DCAA

R.T.: 11.817 min
Delta R.T.: -0.013 min
Response: 281423750
Conc: 747.17 ng/ml

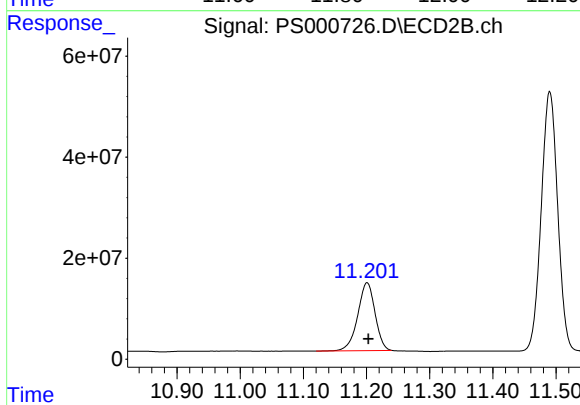

#4 2,4-DCAA


R.T.: 11.201 min
Delta R.T.: -0.002 min
Response: 256425889
Conc: 753.51 ng/ml

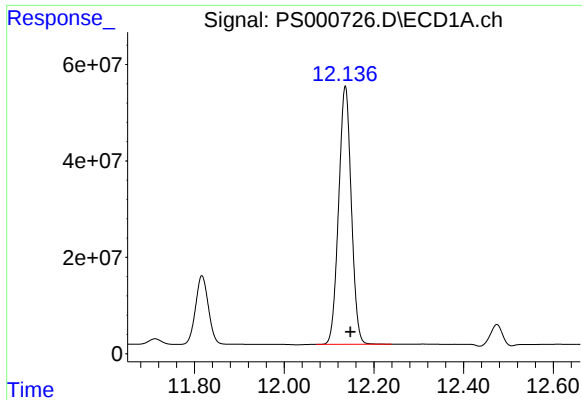

#5 DICAMBA


R.T.: 12.136 min
Delta R.T.: -0.011 min
Response: 1047654646
Conc: 741.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

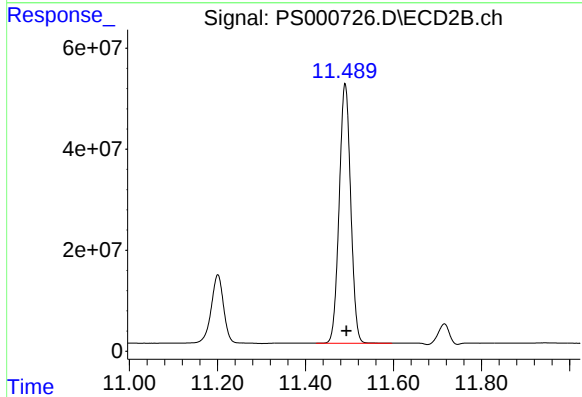


#5 DICAMBA

R.T.: 11.490 min
Delta R.T.: -0.003 min
Response: 932489437
Conc: 752.64 ng/ml

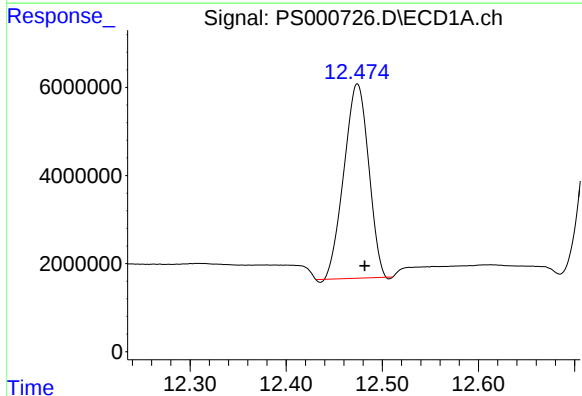


#6 MCP

R.T.: 12.474 min
Delta R.T.: -0.008 min
Response: 78440500
Conc: 69.27 ug/ml

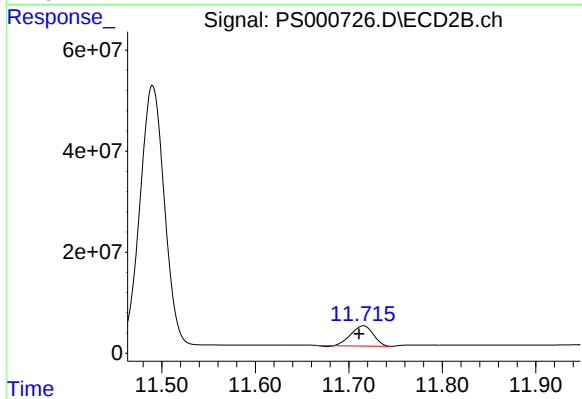

#6 MCP


R.T.: 11.716 min
Delta R.T.: 0.005 min
Response: 65940769
Conc: 68.73 ug/ml

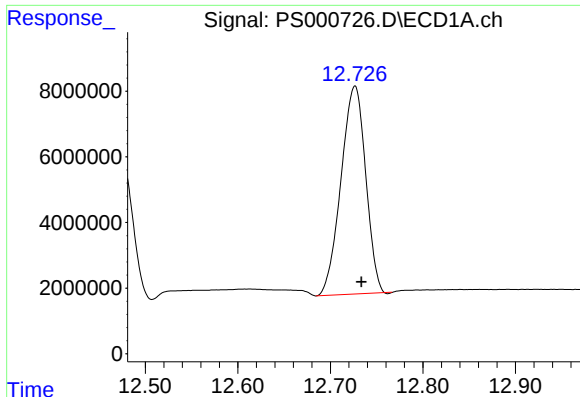

#7 MCPA


R.T.: 12.726 min
Delta R.T.: -0.007 min
Response: 117273693
Conc: 66.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

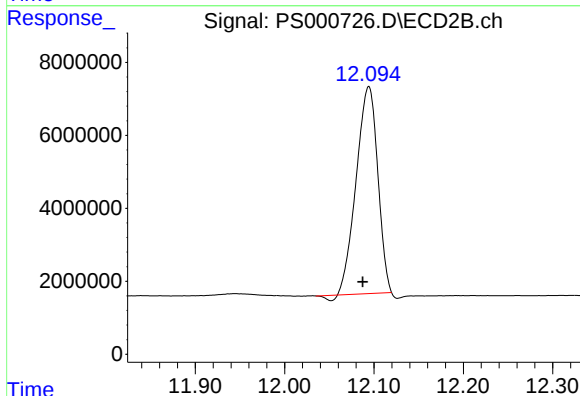


#7 MCPA

R.T.: 12.094 min
Delta R.T.: 0.007 min
Response: 94511395
Conc: 68.24 ug/ml

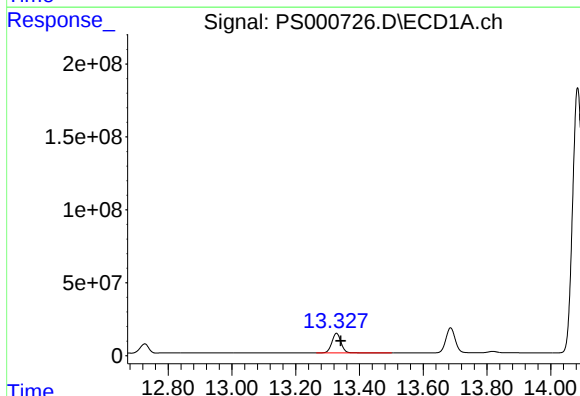


#8 DICHLORPROP

R.T.: 13.328 min
Delta R.T.: -0.013 min
Response: 267072592
Conc: 710.00 ng/ml

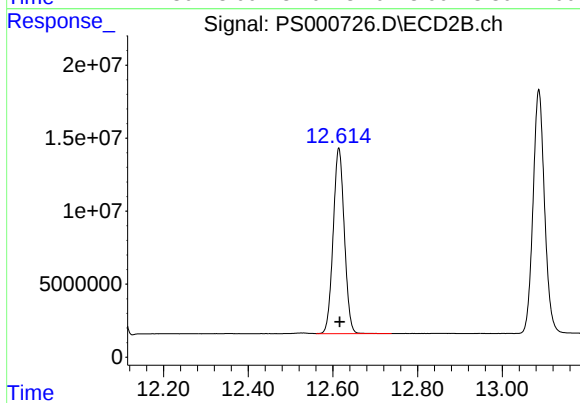

#8 DICHLORPROP


R.T.: 12.614 min
Delta R.T.: -0.002 min
Response: 232625069
Conc: 722.50 ng/ml

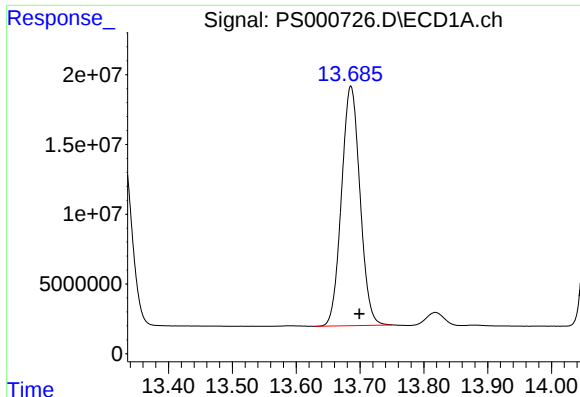

#9 2,4-D


R.T.: 13.686 min
Delta R.T.: -0.013 min
Response: 345378062
Conc: 722.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

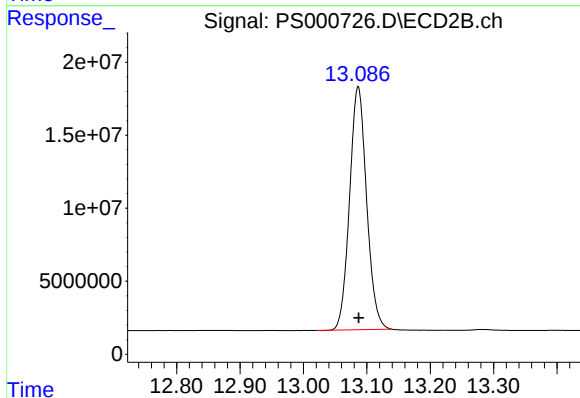


#9 2,4-D

R.T.: 13.086 min
Delta R.T.: -0.001 min
Response: 311001786
Conc: 731.77 ng/ml

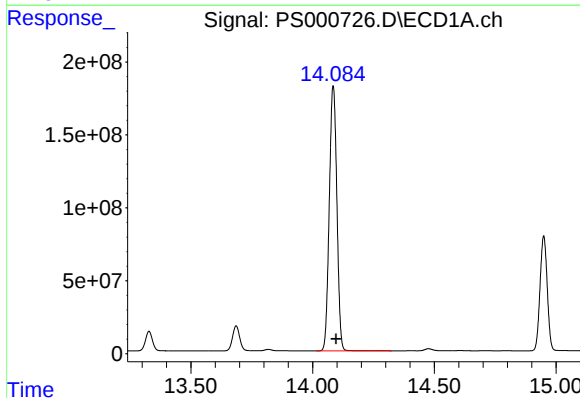


#10 Pentachlorophenol

R.T.: 14.084 min
Delta R.T.: -0.012 min
Response: 3932351391
Conc: 749.02 ng/ml

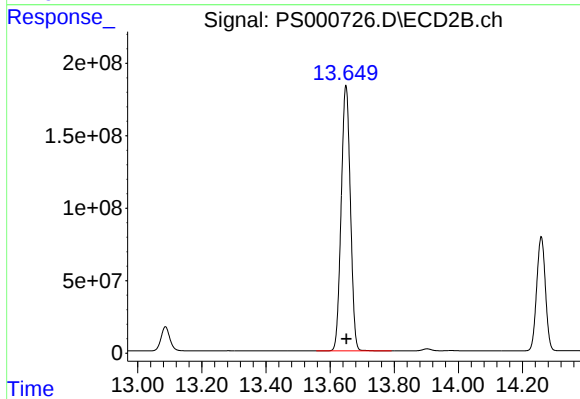

#10 Pentachlorophenol


R.T.: 13.649 min
Delta R.T.: -0.002 min
Response: 3638362068
Conc: 769.10 ng/ml

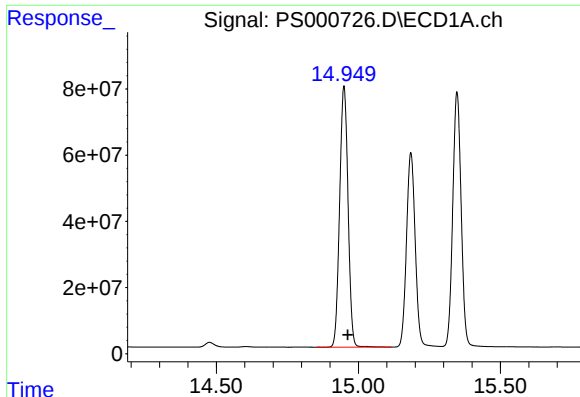

#11 2,4,5-TP (SILVEX)


R.T.: 14.949 min
Delta R.T.: -0.013 min
Response: 1621781956
Conc: 747.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

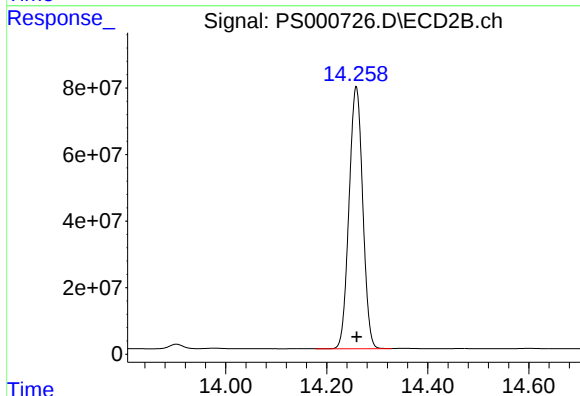


#11 2,4,5-TP (SILVEX)

R.T.: 14.258 min
Delta R.T.: 0.000 min
Response: 1481427720
Conc: 761.26 ng/ml

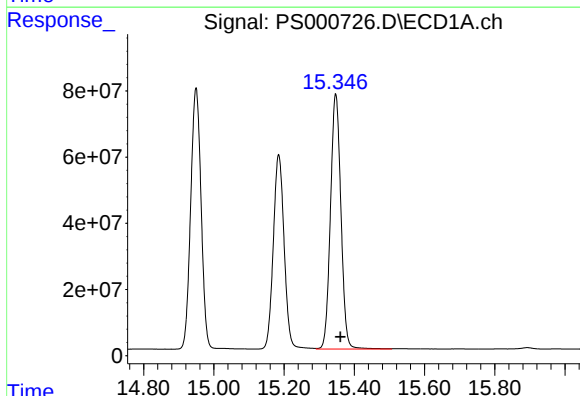


#12 2,4,5-T

R.T.: 15.347 min
Delta R.T.: -0.013 min
Response: 1594045352
Conc: 740.29 ng/ml

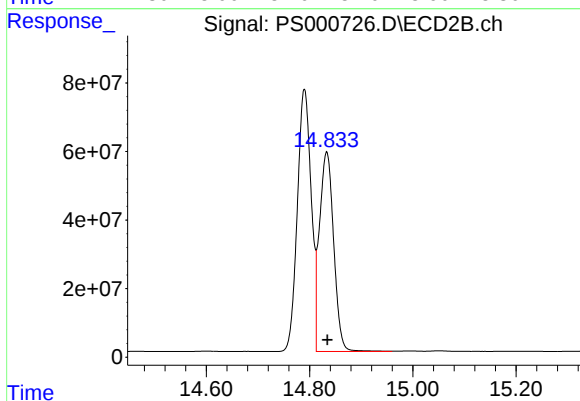

#12 2,4,5-T


R.T.: 14.833 min
Delta R.T.: -0.001 min
Response: 1110137666
Conc: 656.45 ng/ml

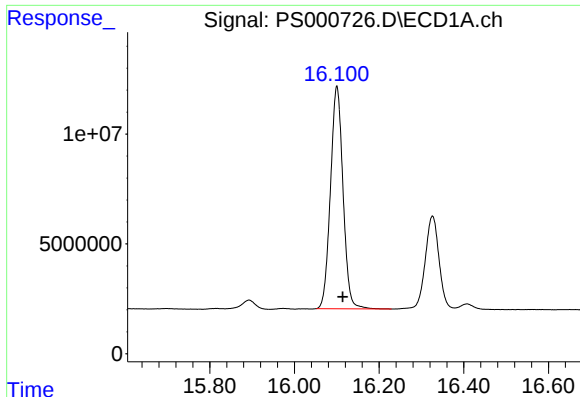

#13 2,4-DB


R.T.: 16.100 min
Delta R.T.: -0.014 min
Response: 208156996
Conc: 707.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

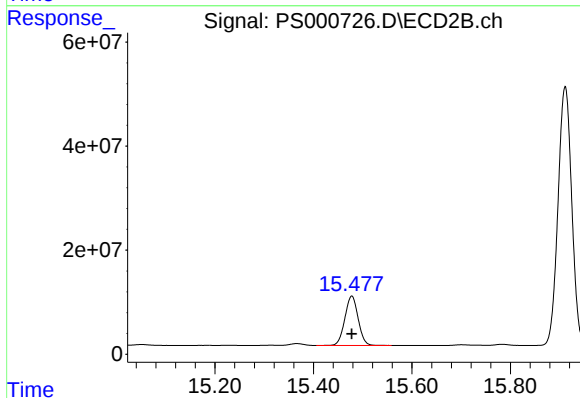


#13 2,4-DB

R.T.: 15.478 min
Delta R.T.: 0.000 min
Response: 177981701
Conc: 718.98 ng/ml

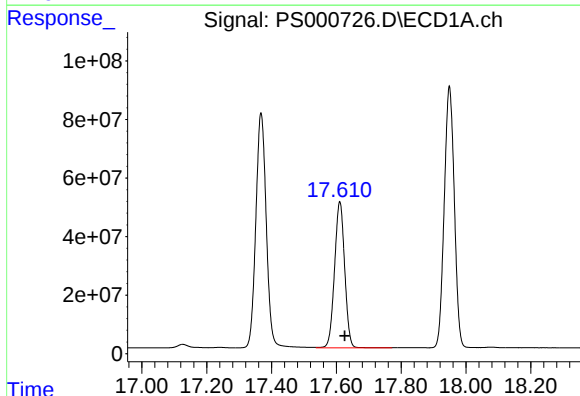


#14 DINOSEB

R.T.: 17.611 min
Delta R.T.: -0.015 min
Response: 1079971081
Conc: 725.24 ng/ml

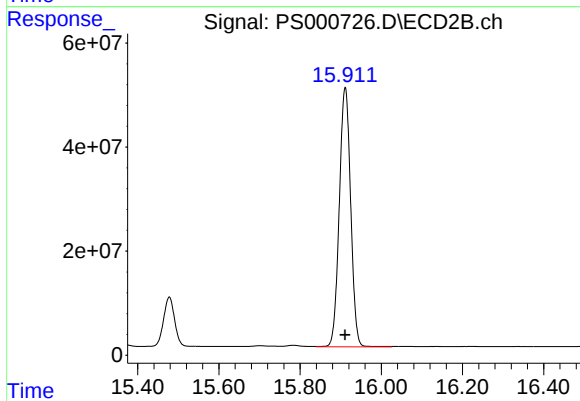

#14 DINOSEB


R.T.: 15.911 min
Delta R.T.: 0.000 min
Response: 967484592
Conc: 741.61 ng/ml

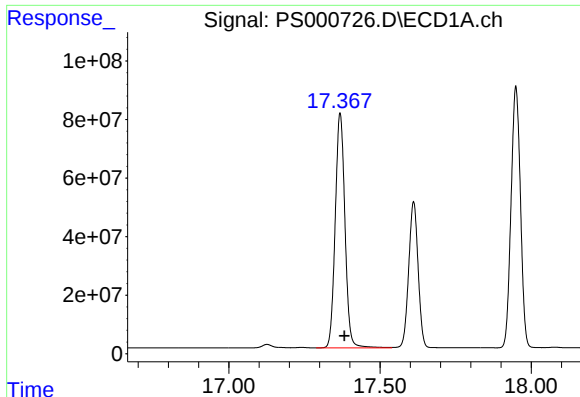

#15 Picloram


R.T.: 17.368 min
Delta R.T.: -0.014 min
Response: 1790699502
Conc: 613.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

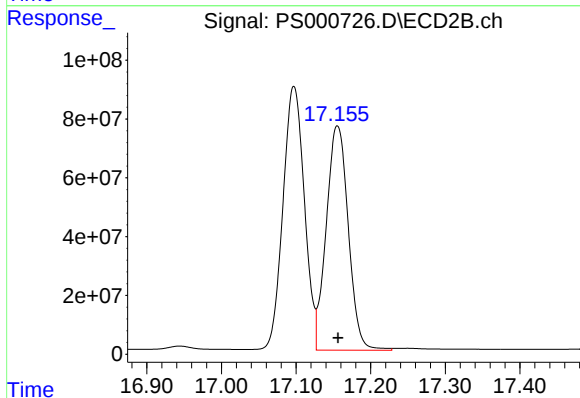


#15 Picloram

R.T.: 17.155 min
Delta R.T.: 0.000 min
Response: 1565597893
Conc: 627.66 ng/ml

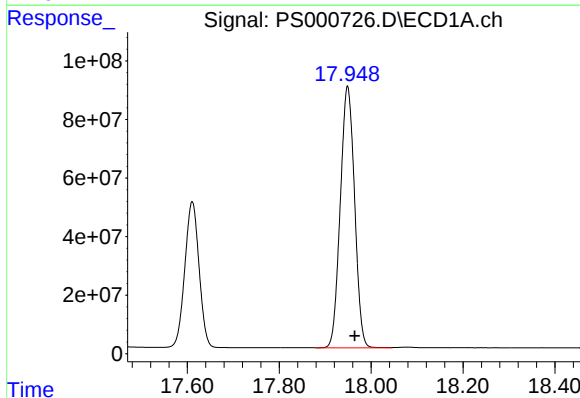

#16 DCPA

R.T.: 17.949 min
Delta R.T.: -0.015 min
Response: 1924483795
Conc: 751.03 ng/ml

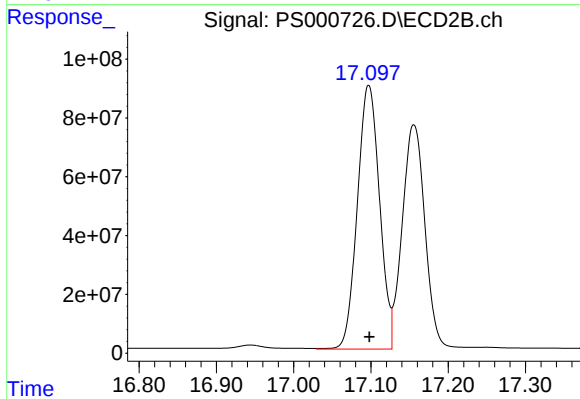

#16 DCPA

R.T.: 17.097 min
Delta R.T.: 0.000 min
Response: 1792416277
Conc: 777.30 ng/ml