

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
 Data File : PS005354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2019 20:01
 Operator : SM\AJ
 Sample : K3160-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-01-062819-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 00:43:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.569	5.284	371.8E6	252.5E6	253.260	251.907
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0 84624898		N.D.	64.173
5) T	DICAMBA	5.669	0.000	5707398	0	1.000	N.D. #
8) T	DICHLORPROP	6.309	5.971	8339727	117.3E6	5.832	121.519 #
9) T	2,4-D	0.000	6.274	0 35025187		N.D.	31.405
11) T	2,4,5-TP ...	0.000	6.939	0 88101209		N.D.	16.544
12) T	2,4,5-T	7.589	0.000	105.5E6	0	13.109	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
Data File : PS005354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2019 20:01
Operator : SM\AJ
Sample : K3160-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 00:43:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

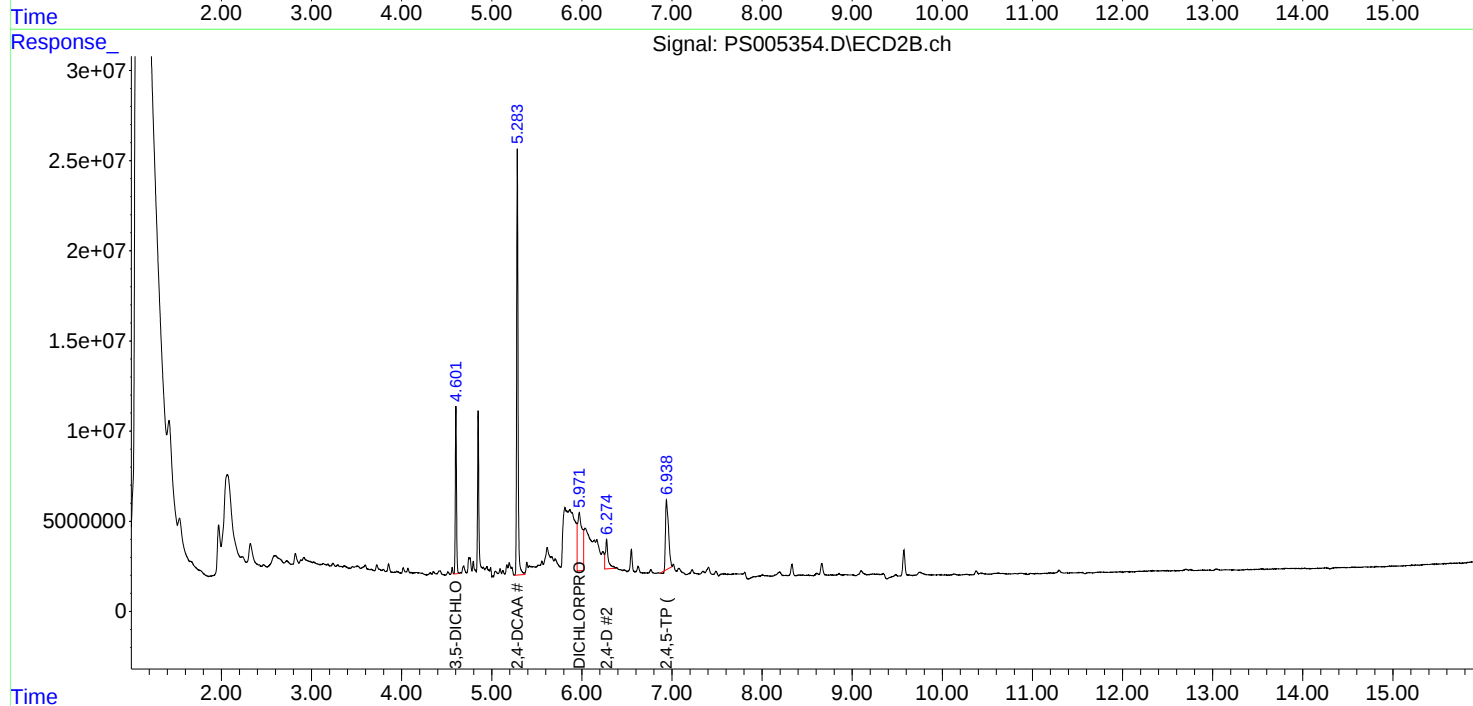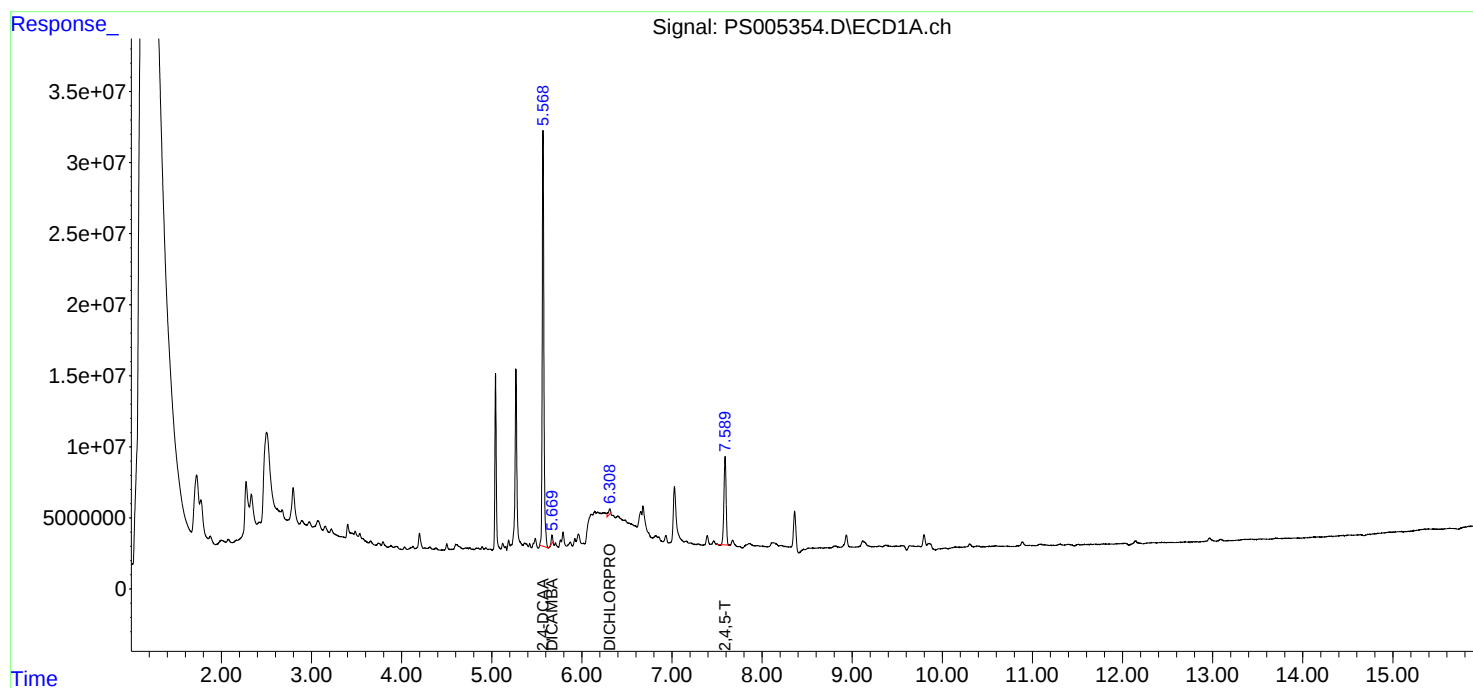


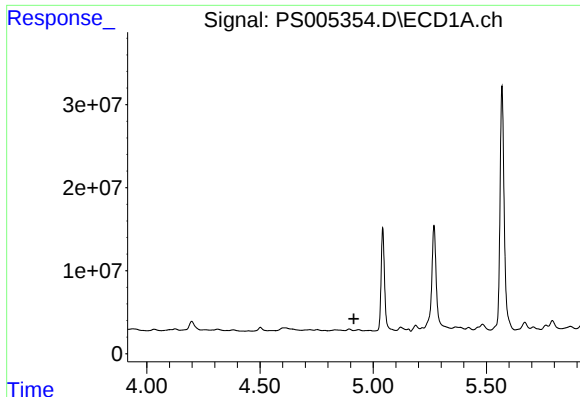

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-A

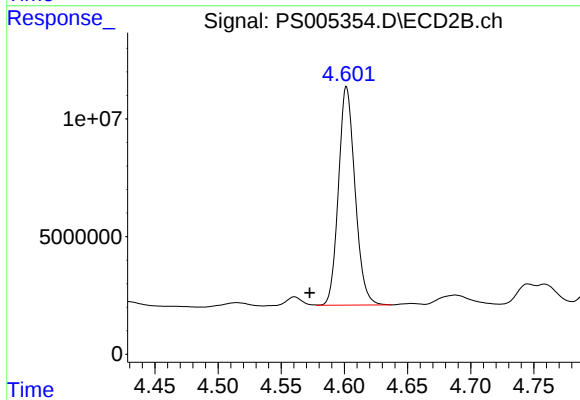


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.029 min
Response: 84624898
Conc: 64.17 ng/ml

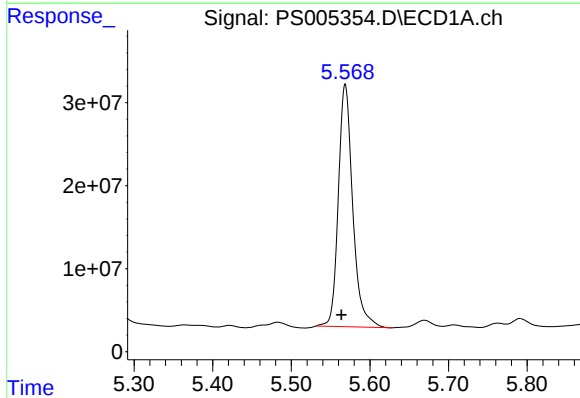


#4 2,4-DCAA

R.T.: 5.569 min
Delta R.T.: 0.005 min
Response: 371757954
Conc: 253.26 ng/ml

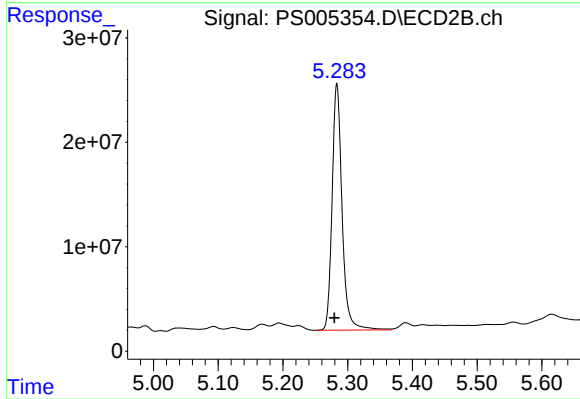

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: 0.004 min
Response: 252503778
Conc: 251.91 ng/ml

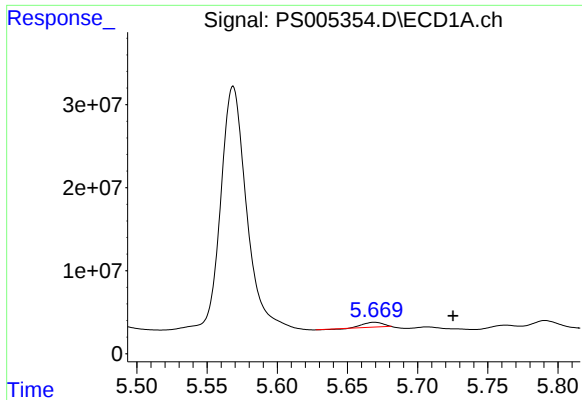

#5 DICAMBA


R.T.: 5.669 min
Delta R.T.: -0.056 min
Response: 5707398
Conc: 1.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-A

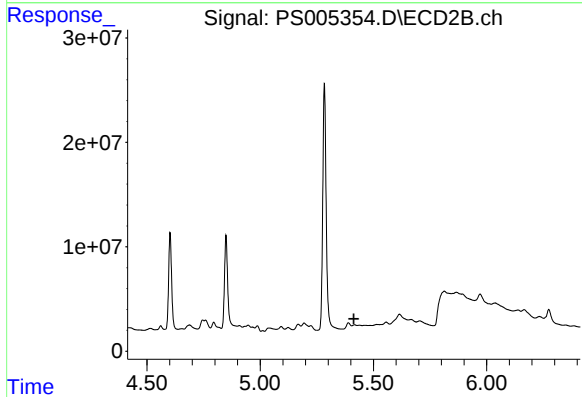


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

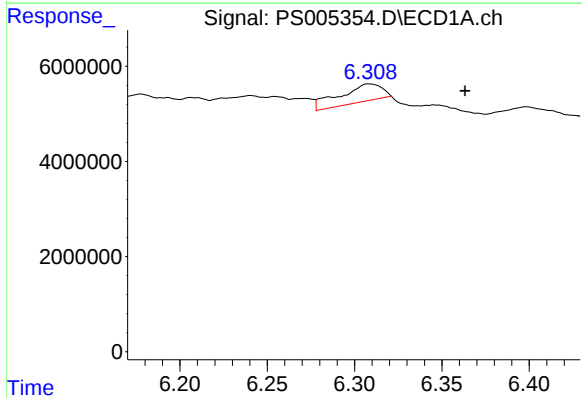


#8 DICHLORPROP

R.T.: 6.309 min
Delta R.T.: -0.054 min
Response: 8339727
Conc: 5.83 ng/ml

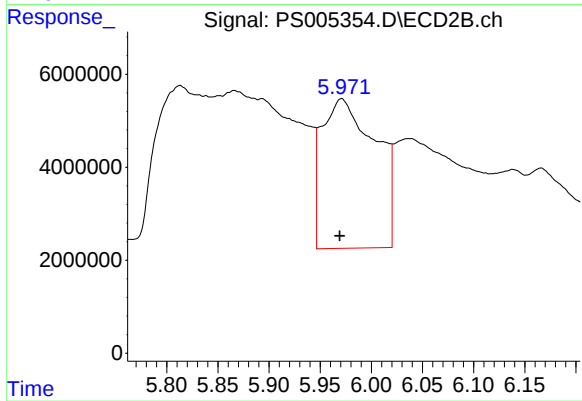

#8 DICHLORPROP


R.T.: 5.971 min
Delta R.T.: 0.002 min
Response: 117331501
Conc: 121.52 ng/ml

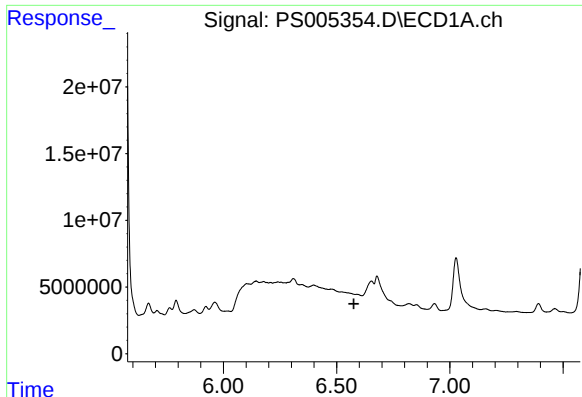

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-A

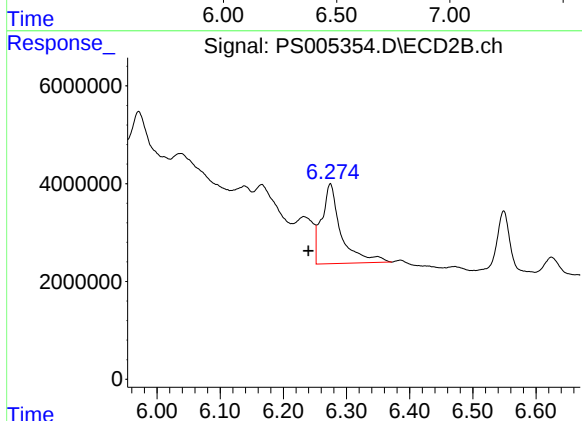


#9 2,4-D

R.T.: 6.274 min
Delta R.T.: 0.035 min
Response: 35025187
Conc: 31.40 ng/ml

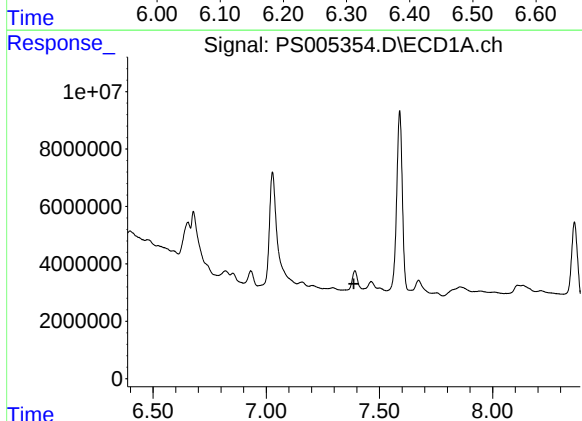


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

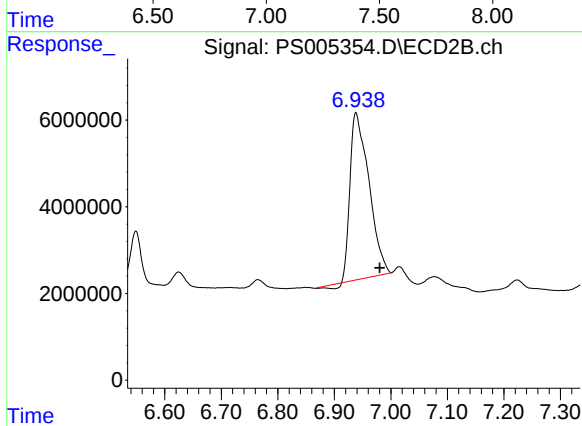

#11 2,4,5-TP (SILVEX)


R.T.: 6.939 min
Delta R.T.: -0.042 min
Response: 88101209
Conc: 16.54 ng/ml

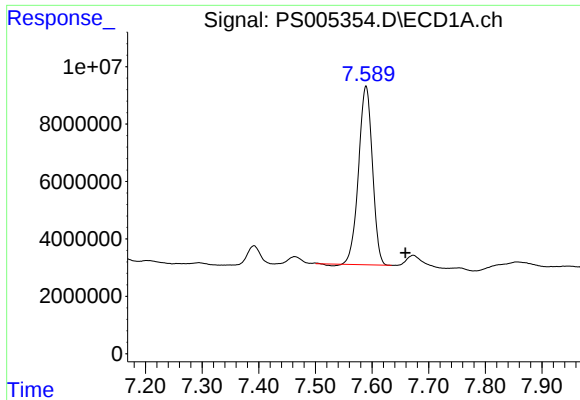

#12 2,4,5-T

R.T.: 7.589 min
Delta R.T.: -0.069 min
Response: 105501654
Conc: 13.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-A

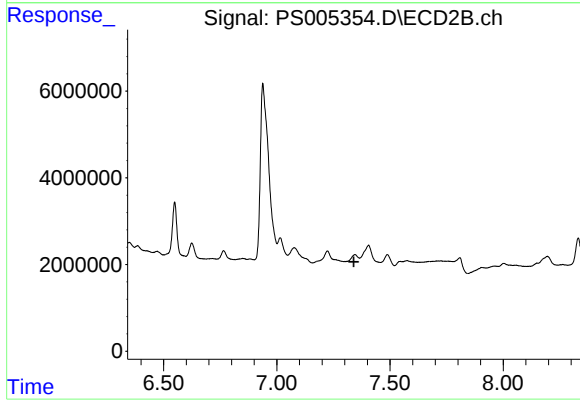

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.