

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
 Data File : PS005355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2019 20:23
 Operator : SM\AJ
 Sample : K3160-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-01-062819-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 00:43:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.569	5.284	361.6E6	246.2E6	246.342	245.599
Target Compounds							
2) T	3,5-DICHL...	0.000	4.602	0	195.1E6	N.D.	147.929
5) T	DICAMBA	5.766	5.390	13258659	15523748	2.324	4.147 #
6) T	MCP	5.922	0.000	7429697	0	1.697	N.D. #
8) T	DICHLORPROP	6.309	5.972	99788117	54710652	69.779	56.663
11) T	2,4,5-TP ...	0.000	6.937	0	115.0E6	N.D.	21.587
12) T	2,4,5-T	7.592	0.000	201.5E6	0	25.038	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
Data File : PS005355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2019 20:23
Operator : SM\AJ
Sample : K3160-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 00:43:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

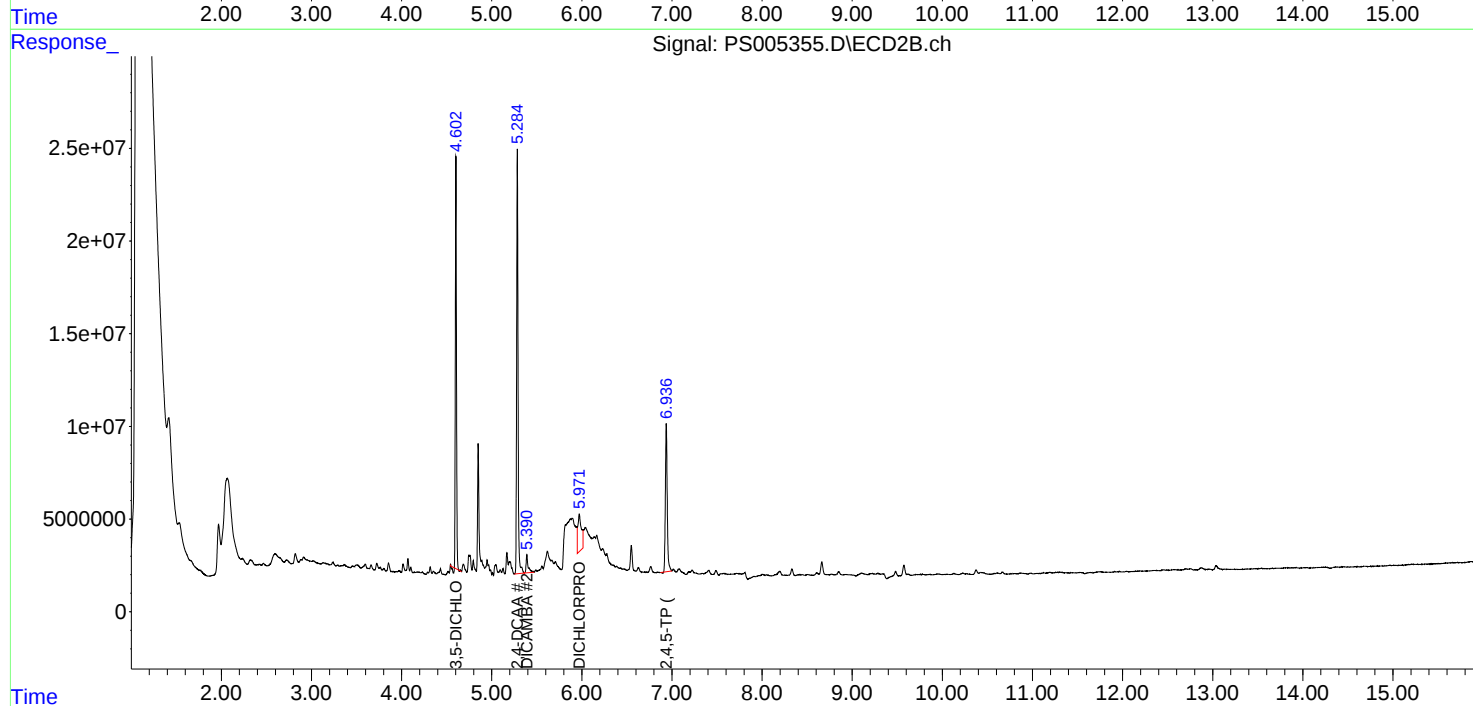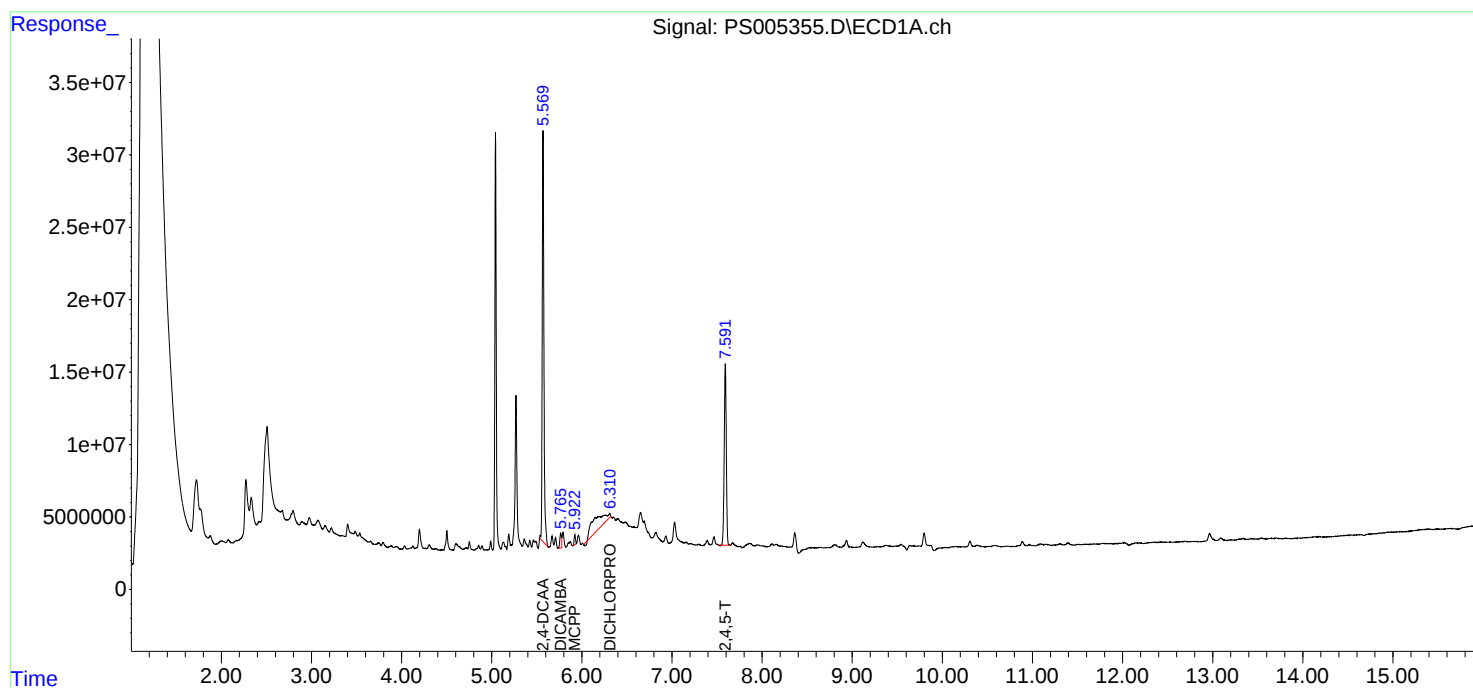


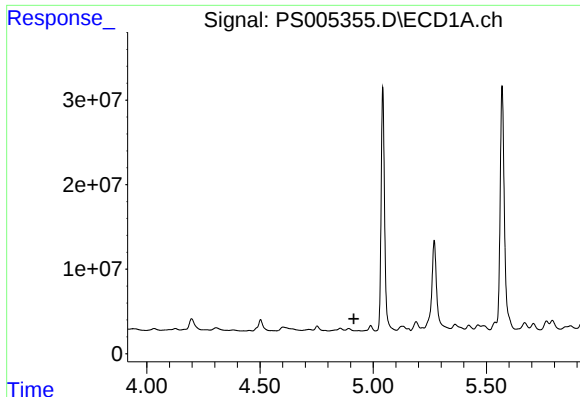

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-B

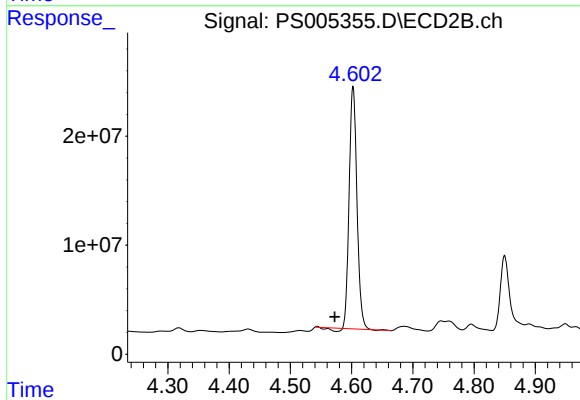


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.602 min
Delta R.T.: 0.030 min
Response: 195075780
Conc: 147.93 ng/ml

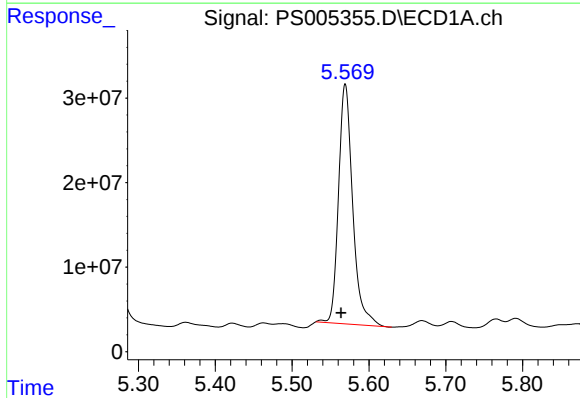


#4 2,4-DCAA

R.T.: 5.569 min
Delta R.T.: 0.006 min
Response: 361603219
Conc: 246.34 ng/ml

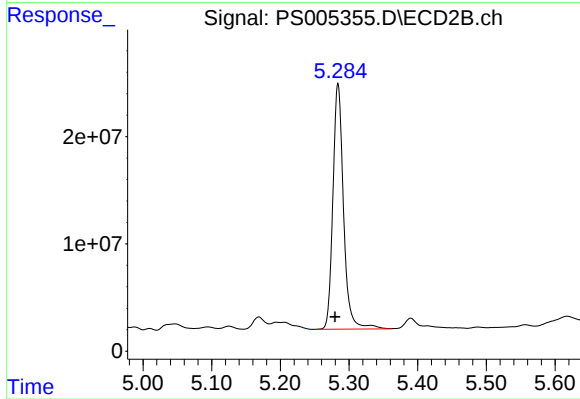

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: 0.005 min
Response: 246180313
Conc: 245.60 ng/ml

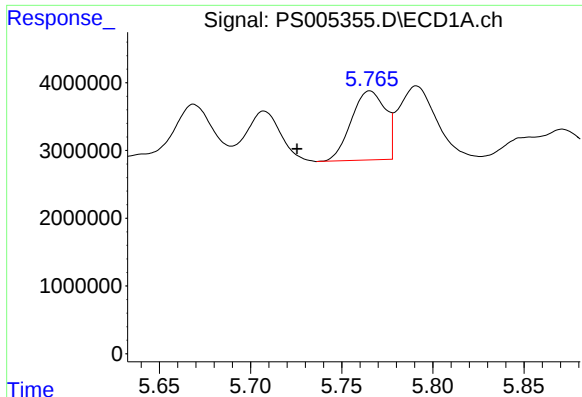

#5 DICAMBA


R.T.: 5.766 min
Delta R.T.: 0.040 min
Response: 13258659
Conc: 2.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-B

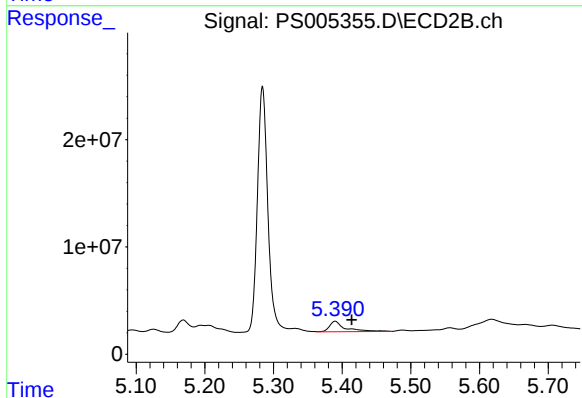


#5 DICAMBA

R.T.: 5.390 min
Delta R.T.: -0.024 min
Response: 15523748
Conc: 4.15 ng/ml

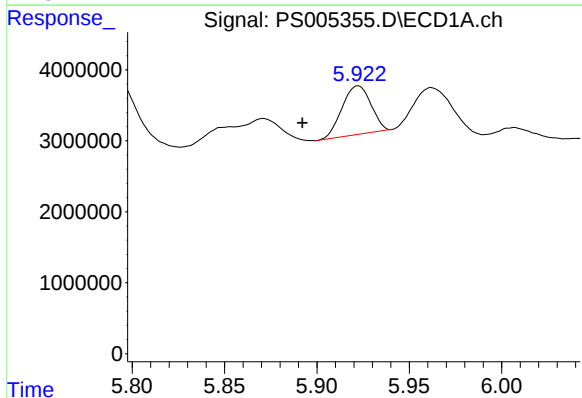


#6 MCP

R.T.: 5.922 min
Delta R.T.: 0.030 min
Response: 7429697
Conc: 1.70 ug/ml

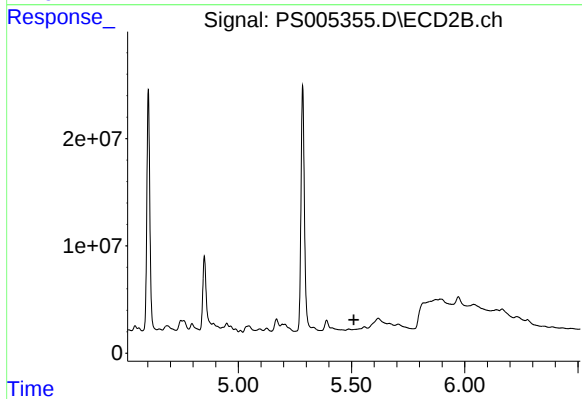

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

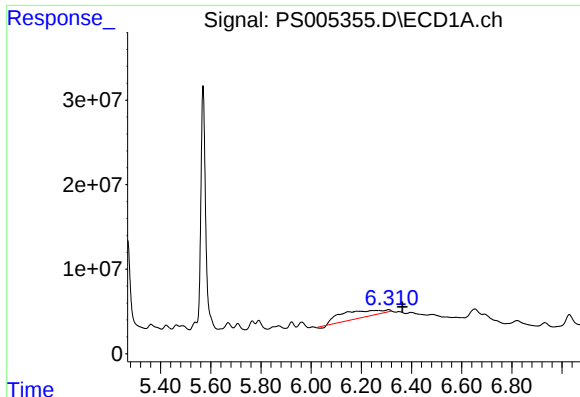

#8 DICHLORPROP


R.T.: 6.309 min
Delta R.T.: -0.054 min
Response: 99788117
Conc: 69.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-B

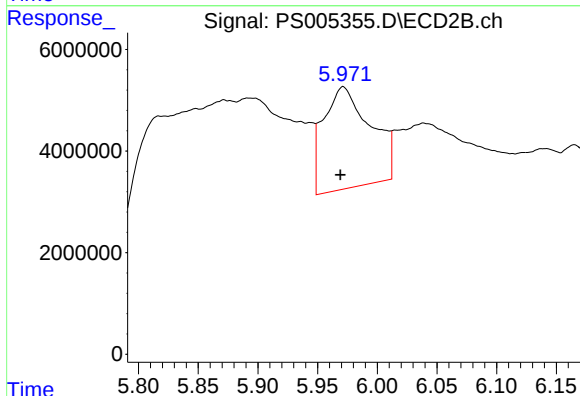


#8 DICHLORPROP

R.T.: 5.972 min
Delta R.T.: 0.003 min
Response: 54710652
Conc: 56.66 ng/ml

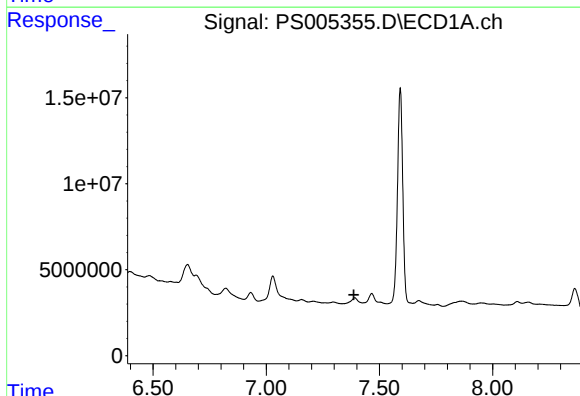


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

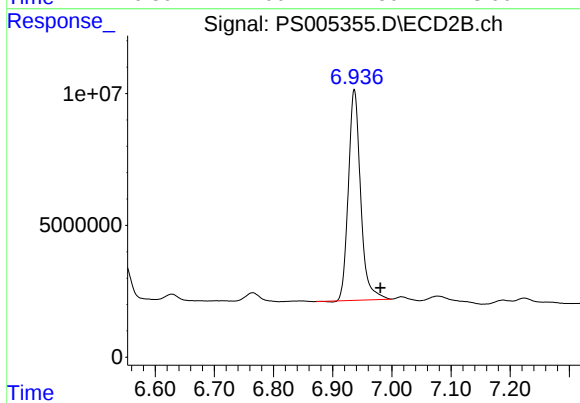

#11 2,4,5-TP (SILVEX)


R.T.: 6.937 min
Delta R.T.: -0.044 min
Response: 114956881
Conc: 21.59 ng/ml

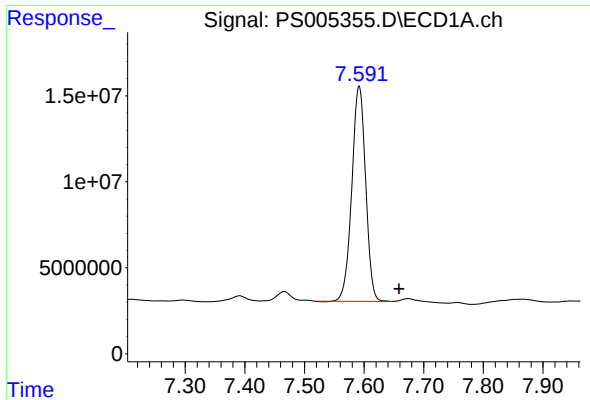

#12 2,4,5-T

R.T.: 7.592 min
Delta R.T.: -0.067 min
Response: 201503898
Conc: 25.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-062819-B

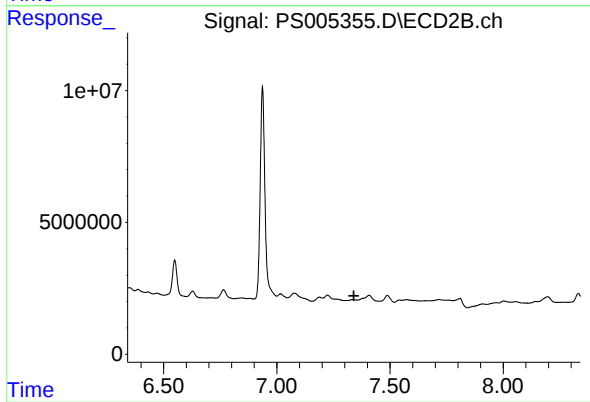

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.