

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
 Data File : PS005360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2019 22:13
 Operator : SM\AJ
 Sample : K3606-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HJDC-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 00:45:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.592	5.307	355.9E6	236.3E6	242.425	235.701
Target Compounds							
2) T	3,5-DICHL...	0.000	4.625	0	226.5E6	N.D.	171.791
5) T	DICAMBA	0.000	5.413	0	8776050	N.D.	2.344
6) T	MCP	5.944	0.000	12649803	0	2.890	N.D. #
7) T	MCPA	5.986	0.000	11780965	0	1.876	N.D. #
8) T	DICHLORPROP	0.000	5.995	0	85061484	N.D.	88.097
9) T	2,4-D	0.000	6.190	0	34645753	N.D.	31.065
10) T	Pentachlo...	6.877	6.646	23911218	15284731	1.215	1.189
11) T	2,4,5-TP ...	0.000	6.960	0	69007561	N.D.	12.958
12) T	2,4,5-T	7.613	0.000	194.8E6	0	24.211	N.D. #
15) T	Picloram	9.160	9.118	209.1E6	145.6E6	18.195	19.287



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
Data File : PS005360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2019 22:13
Operator : SM\AJ
Sample : K3606-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
HJDC-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 00:45:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

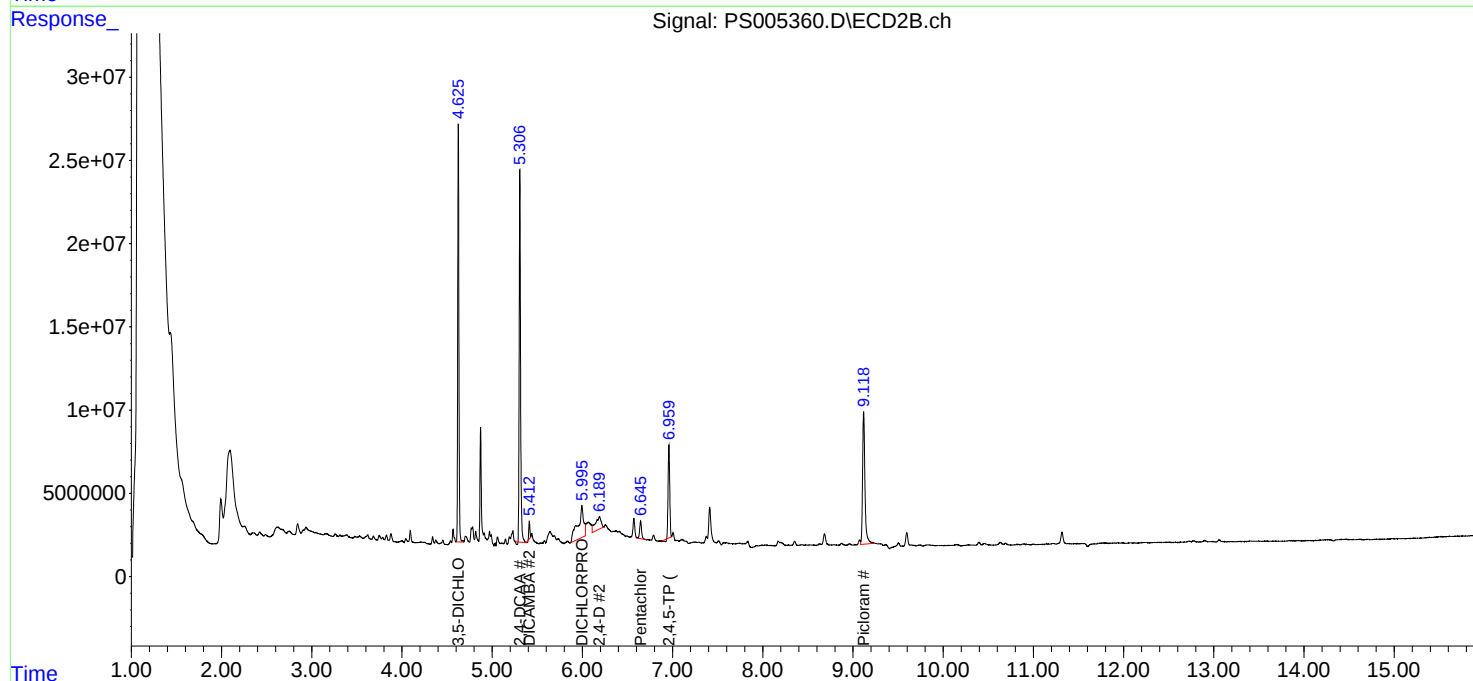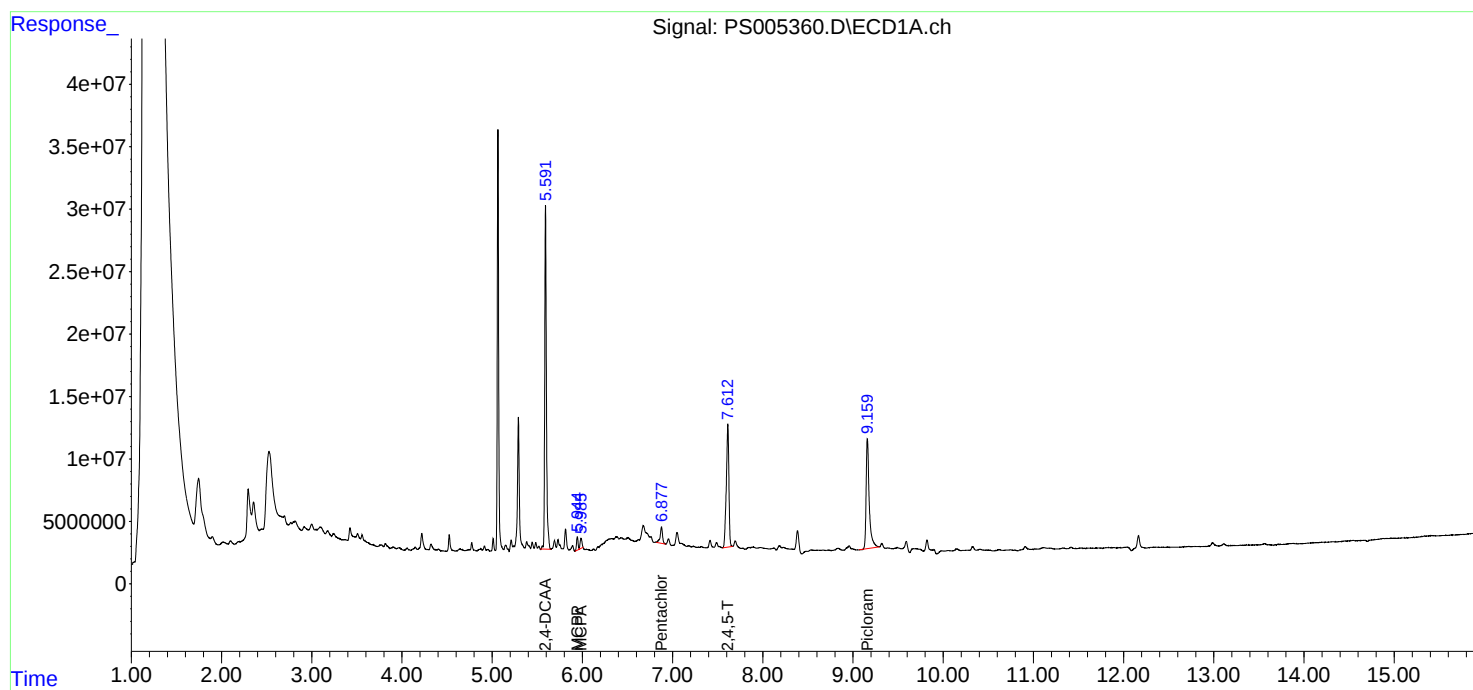


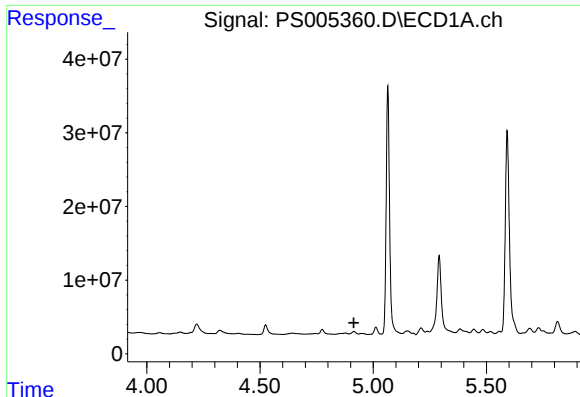

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

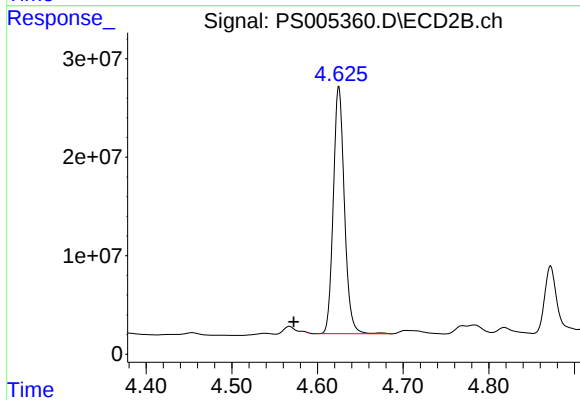


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.625 min
Delta R.T.: 0.053 min
Response: 226542121
Conc: 171.79 ng/ml

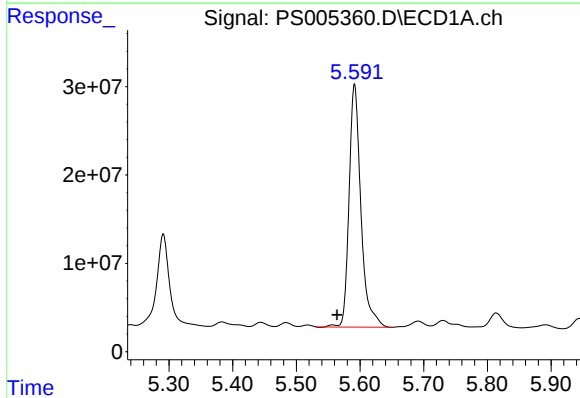


#4 2,4-DCAA

R.T.: 5.592 min
Delta R.T.: 0.028 min
Response: 355853700
Conc: 242.42 ng/ml

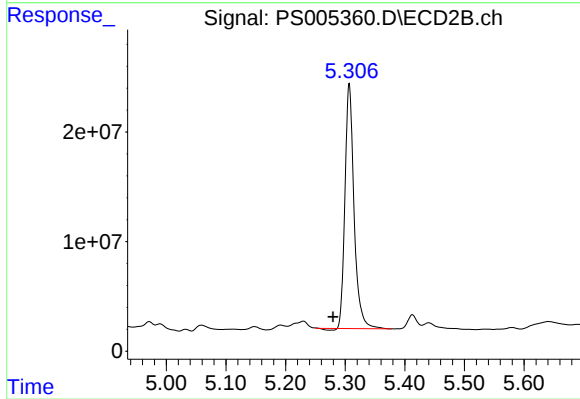

#4 2,4-DCAA


R.T.: 5.307 min
Delta R.T.: 0.027 min
Response: 236259606
Conc: 235.70 ng/ml

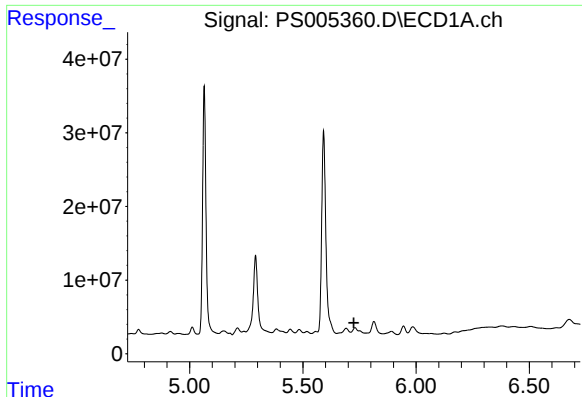

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

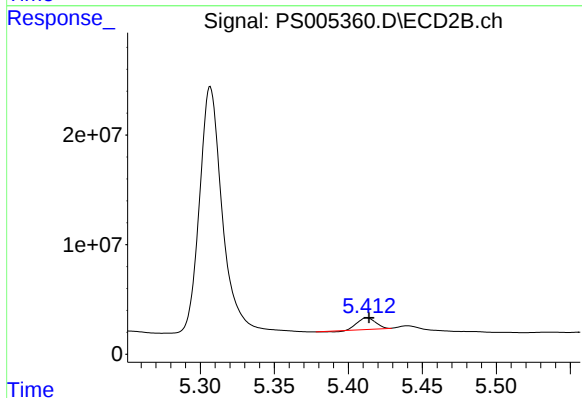


#5 DICAMBA

R.T.: 5.413 min
Delta R.T.: -0.001 min
Response: 8776050
Conc: 2.34 ng/ml

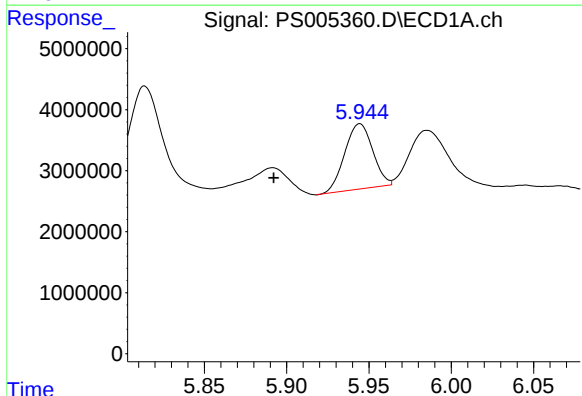


#6 MCP

R.T.: 5.944 min
Delta R.T.: 0.052 min
Response: 12649803
Conc: 2.89 ug/ml

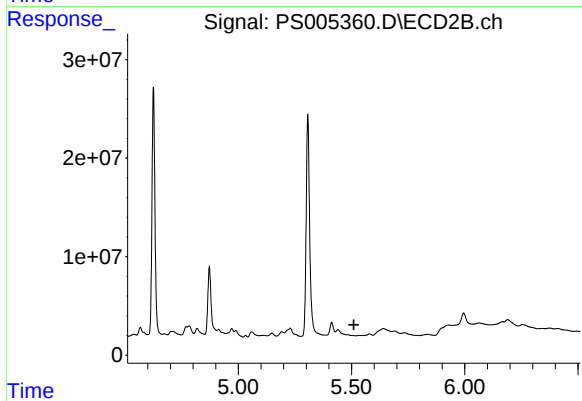

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

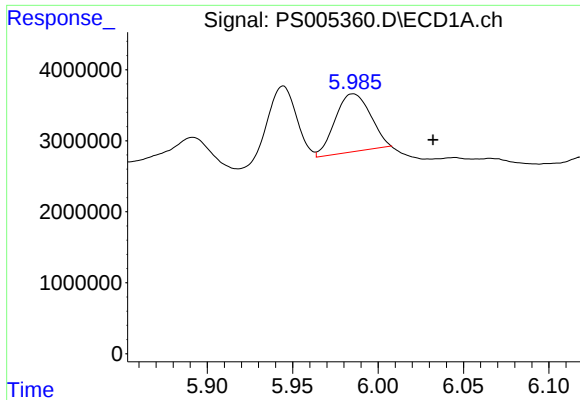

#7 MCPA


R.T.: 5.986 min
Delta R.T.: -0.047 min
Response: 11780965
Conc: 1.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

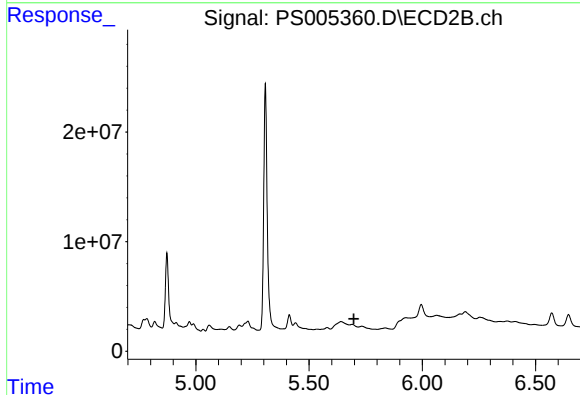


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.698 min
Response: 0
Conc: N.D.

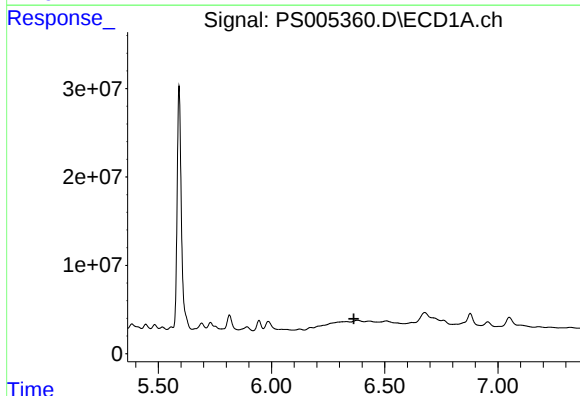


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

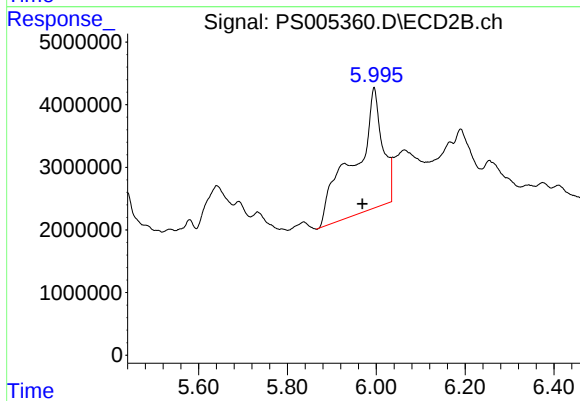

#8 DICHLORPROP


R.T.: 5.995 min
Delta R.T.: 0.026 min
Response: 85061484
Conc: 88.10 ng/ml

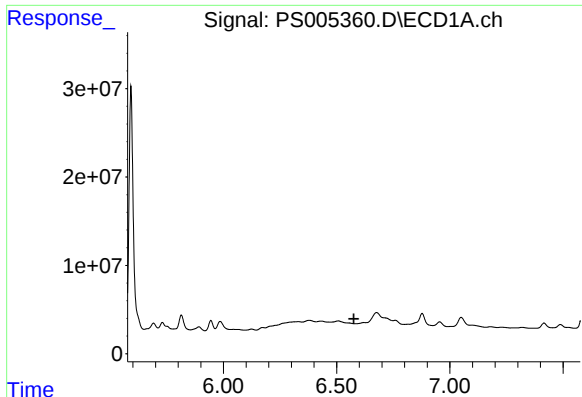

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

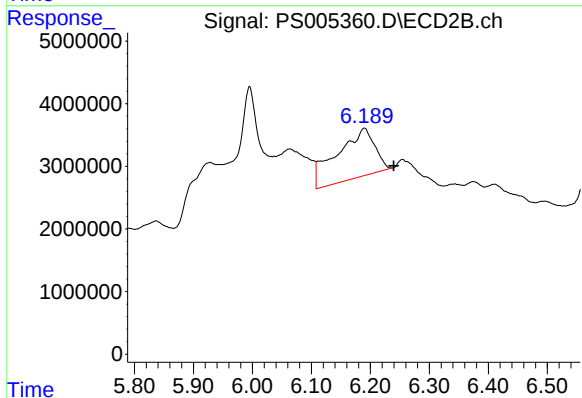


#9 2,4-D

R.T.: 6.190 min
Delta R.T.: -0.050 min
Response: 34645753
Conc: 31.06 ng/ml

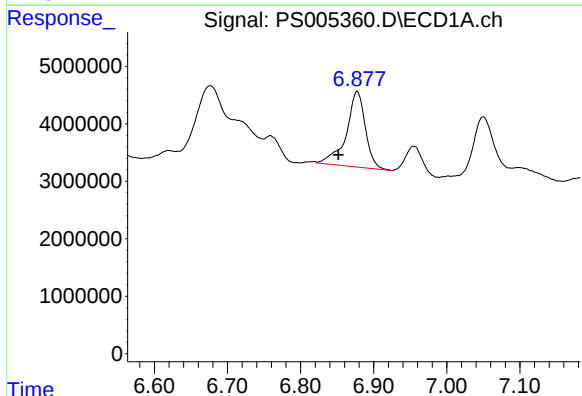


#10 Pentachlorophenol

R.T.: 6.877 min
Delta R.T.: 0.026 min
Response: 23911218
Conc: 1.22 ng/ml

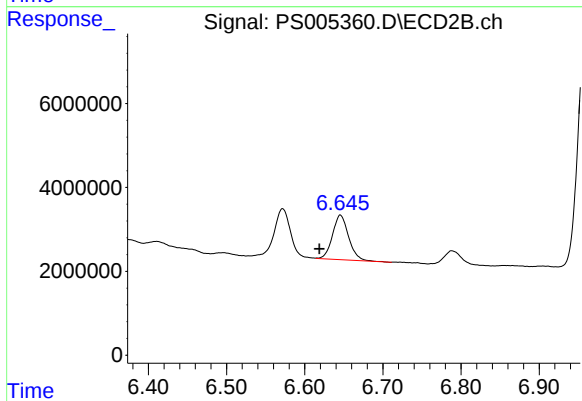

#10 Pentachlorophenol


R.T.: 6.646 min
Delta R.T.: 0.027 min
Response: 15284731
Conc: 1.19 ng/ml

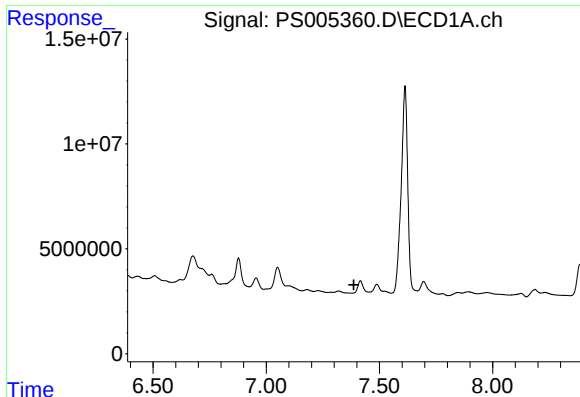

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

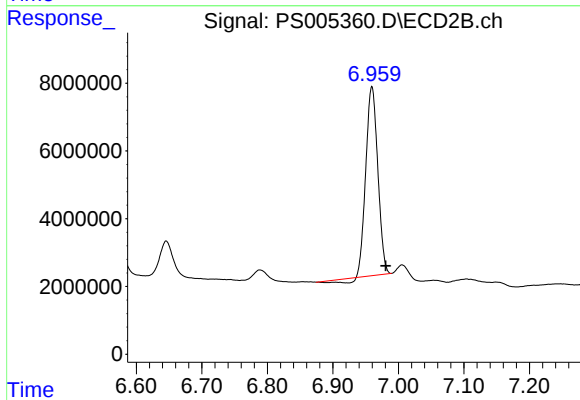


#11 2,4,5-TP (SILVEX)

R.T.: 6.960 min
Delta R.T.: -0.021 min
Response: 69007561
Conc: 12.96 ng/ml

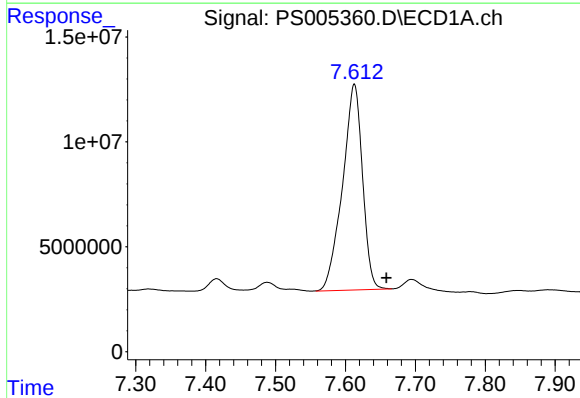


#12 2,4,5-T

R.T.: 7.613 min
Delta R.T.: -0.046 min
Response: 194846147
Conc: 24.21 ng/ml

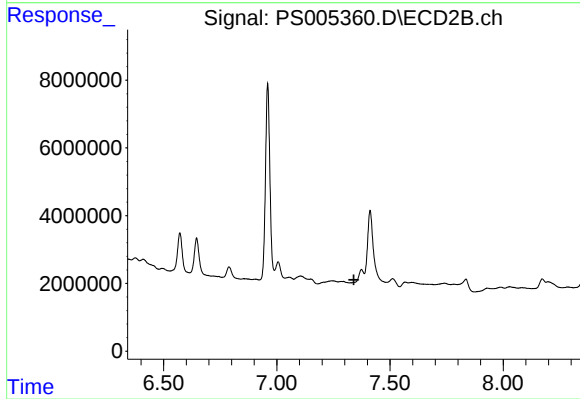

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.341 min
Response: 0
Conc: N.D.

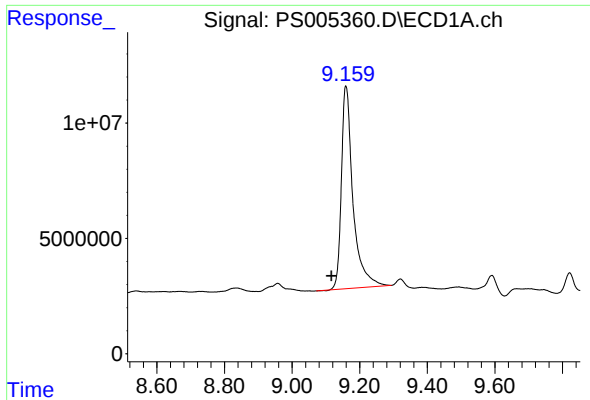

#15 Picloram

R.T.: 9.160 min
Delta R.T.: 0.043 min
Response: 209081137
Conc: 18.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-1

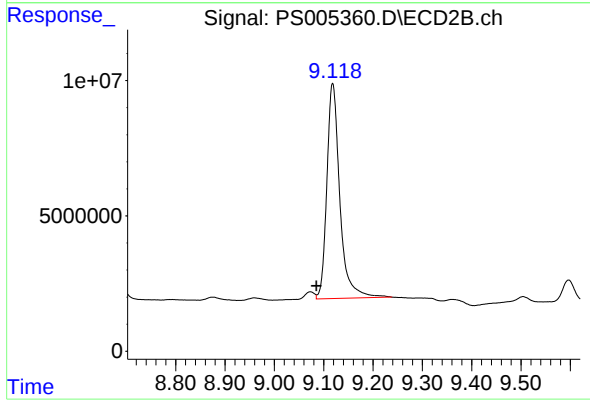

#15 Picloram

R.T.: 9.118 min
Delta R.T.: 0.033 min
Response: 145550621
Conc: 19.29 ng/ml