

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
 Data File : PS005362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2019 22:57
 Operator : SM\AJ
 Sample : K3634-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HJDC-COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 00:46:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.308	316.6E6	205.4E6	215.693	204.876
Target Compounds							
2) T	3,5-DICHL...	0.000	4.626	0	231.1E6	N.D.	175.231
5) T	DICAMBA	0.000	5.413	0	17432582	N.D.	4.657
6) T	MCP	5.946	0.000	8281307	0	1.892	N.D. #
7) T	MCPA	5.986	5.641	9784162	23914600	1.558	5.904 #
8) T	DICHLORPROP	0.000	5.995	0	75861236	N.D.	78.569
10) T	Pentachlo...	0.000	6.573	0	16425700	N.D.	1.278
11) T	2,4,5-TP ...	0.000	6.960	0	113.7E6	N.D.	21.345
12) T	2,4,5-T	7.616	0.000	204.4E6	0	25.394	N.D. #
13) T	2,4-DB	8.158	0.000	23173691	0	19.951	N.D. #
15) T	Picloram	9.140	0.000	29222281	0	2.543	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070219\
Data File : PS005362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2019 22:57
Operator : SM\AJ
Sample : K3634-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 00:46:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

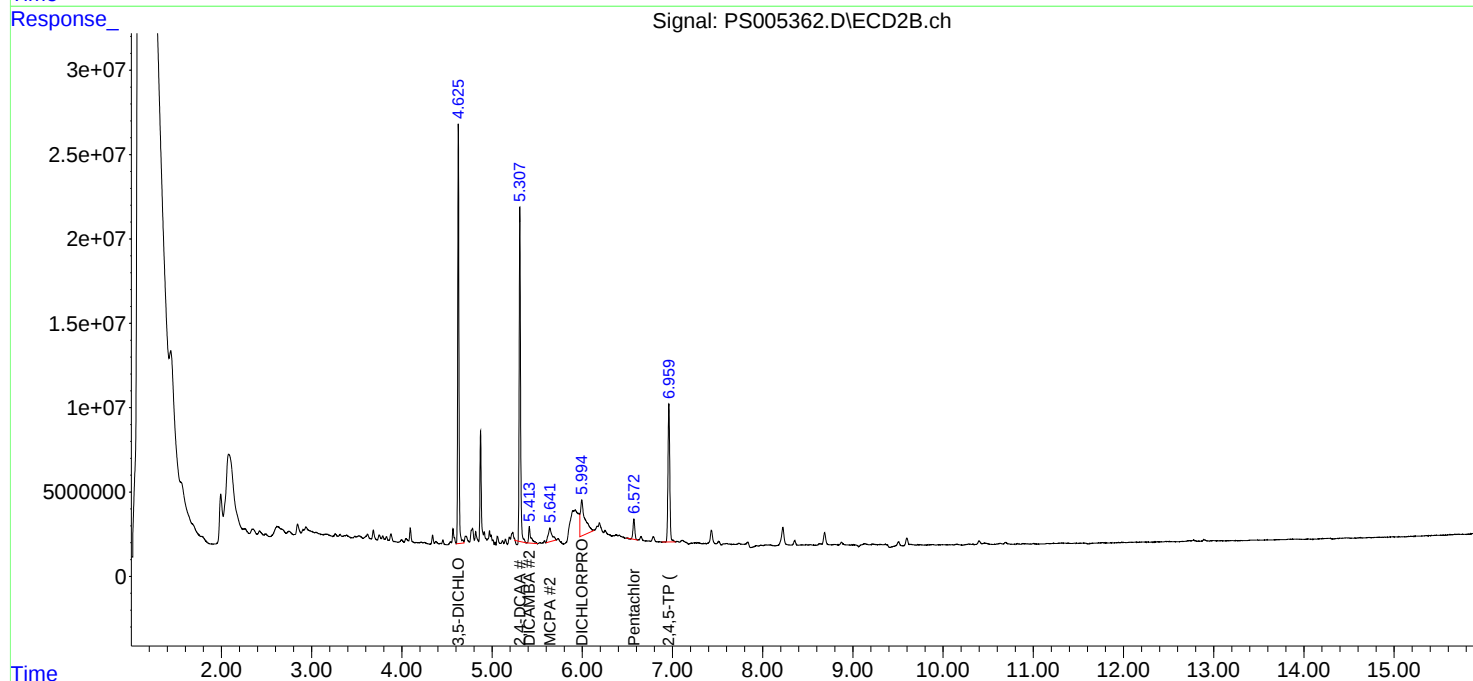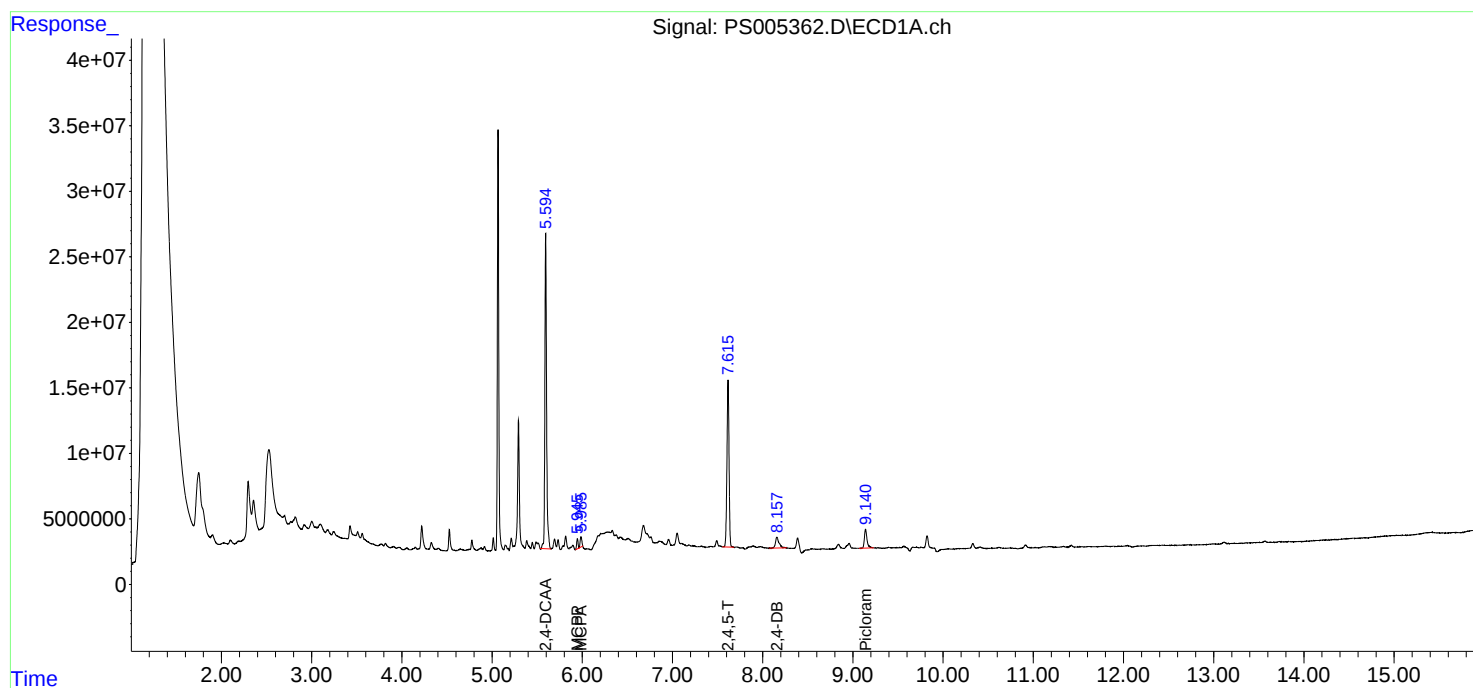


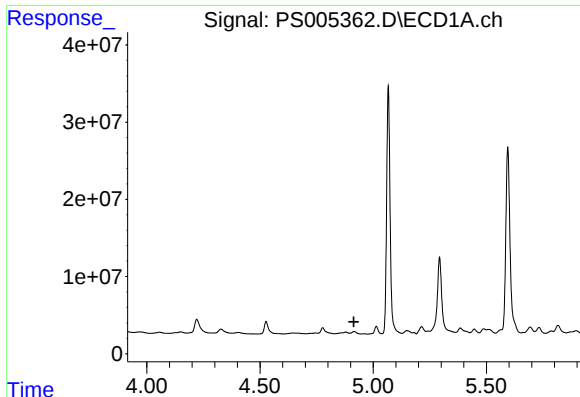

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

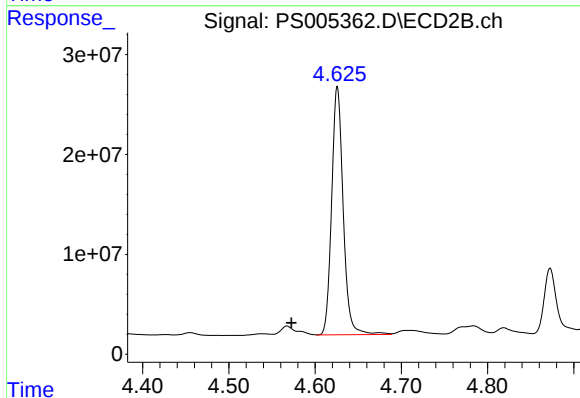


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.626 min
Delta R.T.: 0.053 min
Response: 231078244
Conc: 175.23 ng/ml

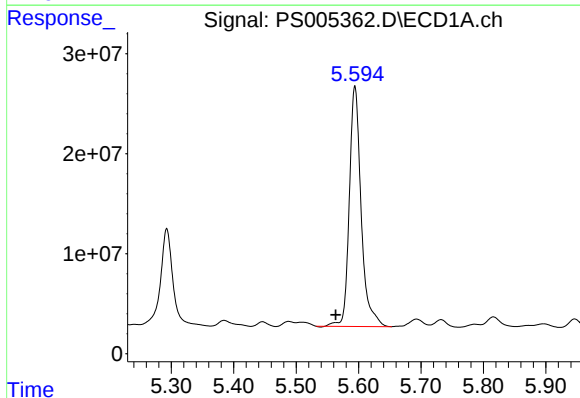


#4 2,4-DCAA

R.T.: 5.594 min
Delta R.T.: 0.031 min
Response: 316613551
Conc: 215.69 ng/ml

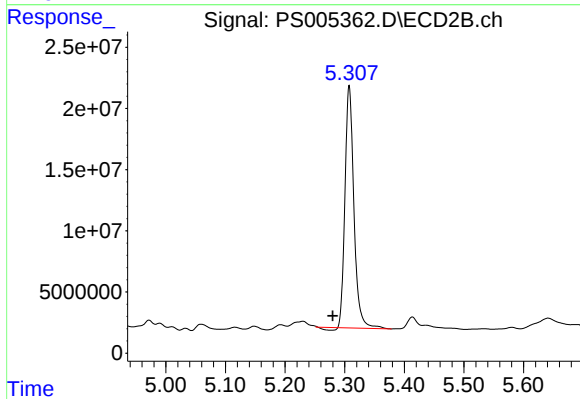

#4 2,4-DCAA


R.T.: 5.308 min
Delta R.T.: 0.028 min
Response: 205361046
Conc: 204.88 ng/ml

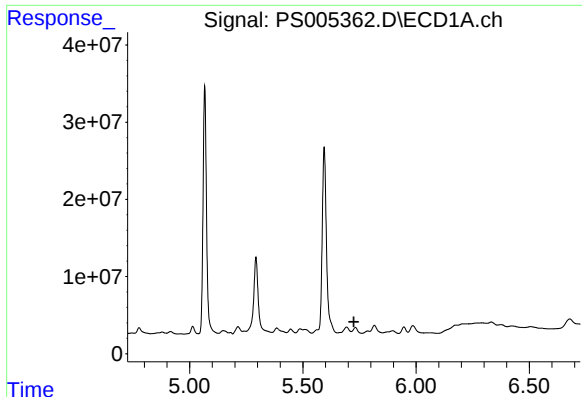

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.725 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

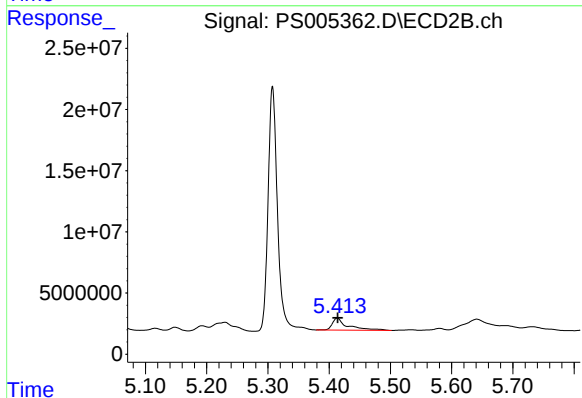


#5 DICAMBA

R.T.: 5.413 min
Delta R.T.: 0.000 min
Response: 17432582
Conc: 4.66 ng/ml

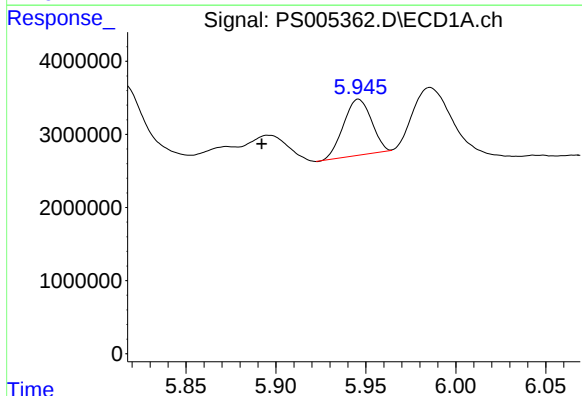


#6 MCP

R.T.: 5.946 min
Delta R.T.: 0.054 min
Response: 8281307
Conc: 1.89 ug/ml

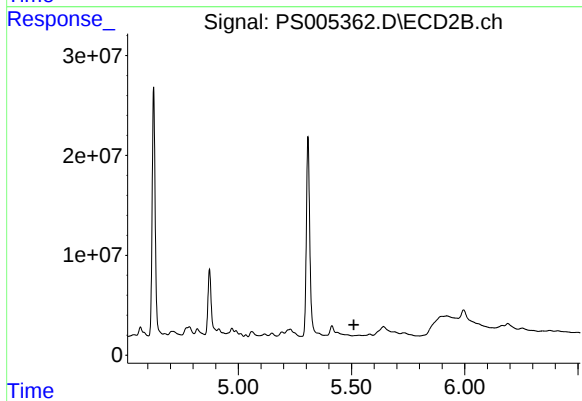

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.511 min
Response: 0
Conc: N.D.

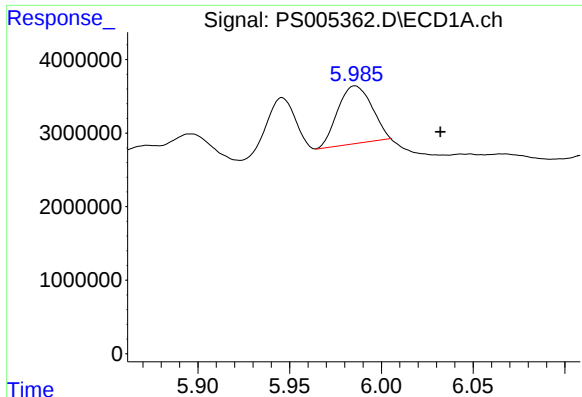

#7 MCPA


R.T.: 5.986 min
Delta R.T.: -0.046 min
Response: 9784162
Conc: 1.56 ug/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

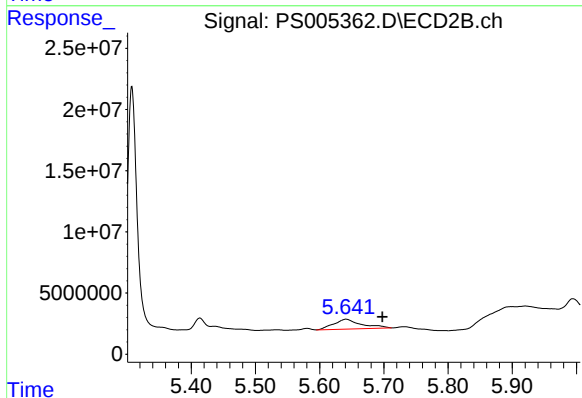


#7 MCPA

R.T.: 5.641 min
Delta R.T.: -0.057 min
Response: 23914600
Conc: 5.90 ug/ml

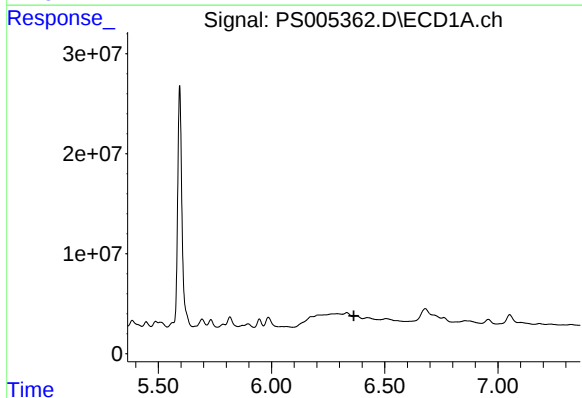


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

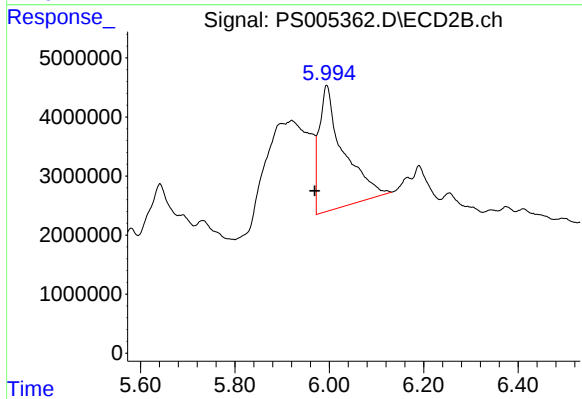

#8 DICHLORPROP


R.T.: 5.995 min
Delta R.T.: 0.026 min
Response: 75861236
Conc: 78.57 ng/ml

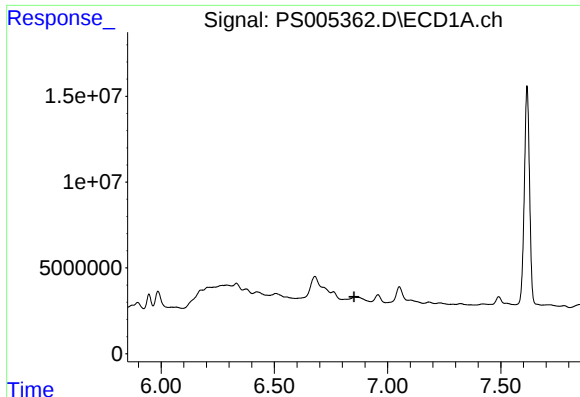

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

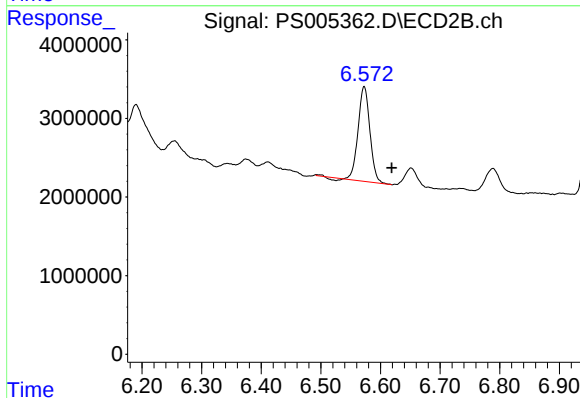


#10 Pentachlorophenol

R.T.: 6.573 min
Delta R.T.: -0.046 min
Response: 16425700
Conc: 1.28 ng/ml

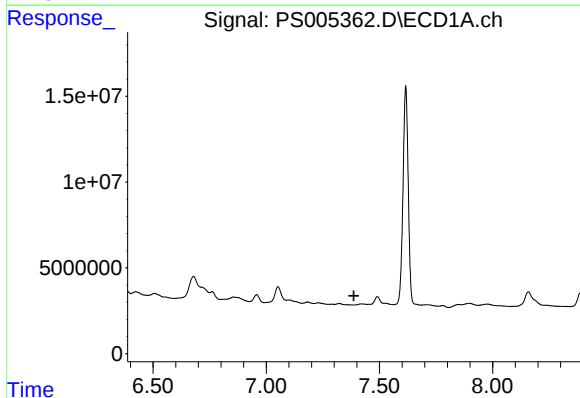


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

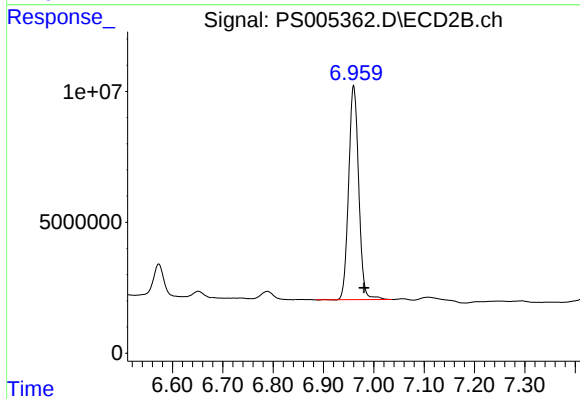

#11 2,4,5-TP (SILVEX)


R.T.: 6.960 min
Delta R.T.: -0.021 min
Response: 113667738
Conc: 21.34 ng/ml

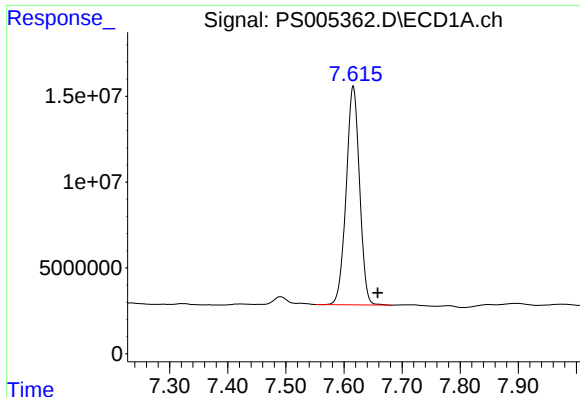

#12 2,4,5-T


R.T.: 7.616 min
Delta R.T.: -0.043 min
Response: 204366348
Conc: 25.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

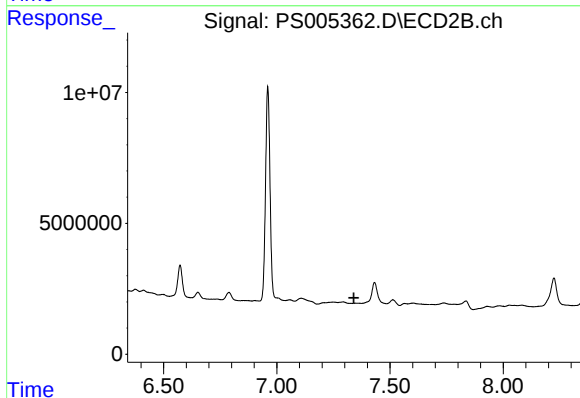


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.

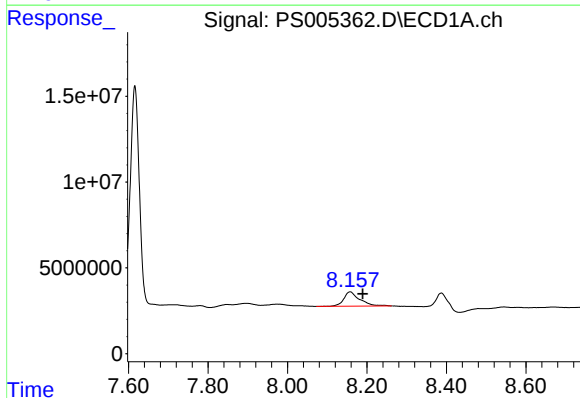


#13 2,4-DB

R.T.: 8.158 min
Delta R.T.: -0.032 min
Response: 23173691
Conc: 19.95 ng/ml

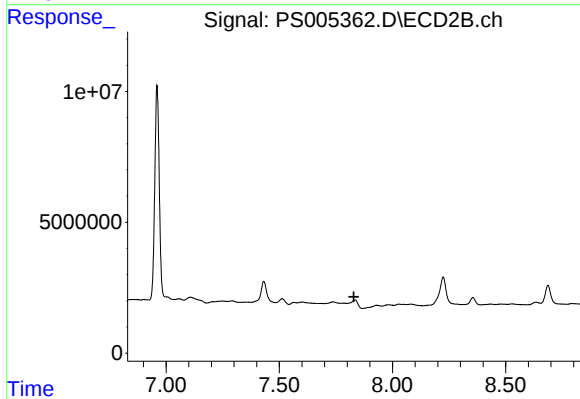

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.830 min
Response: 0
Conc: N.D.

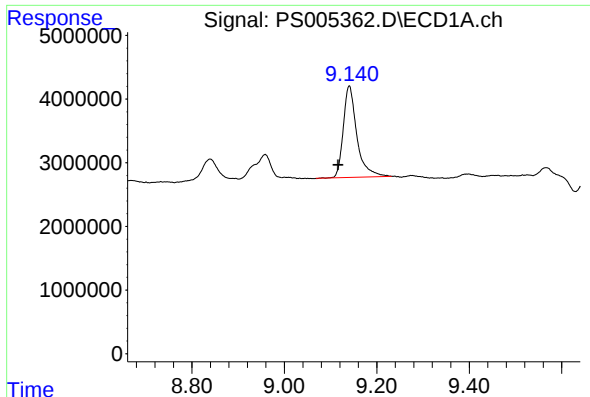

#15 Picloram

R.T.: 9.140 min
Delta R.T.: 0.024 min
Response: 29222281
Conc: 2.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HJDC-COMP-2

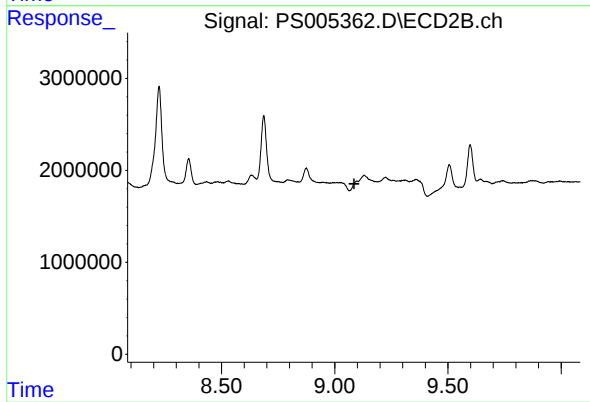

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.