

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
 Data File : PS011076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 20:01
 Operator : DD\AJ
 Sample : PB129944TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:08:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.920	283.3E6	206.7E6	312.460	373.006
Target Compounds							
1) T	Dalapon	2.996	2.585	35078330	82415716	31.328	109.252 #
2) T	3,5-DICHL...	0.000	6.100	0	88443592	N.D.	106.197
5) T	DICAMBA	7.409	0.000	8352234	0	2.291	N.D. #
6) T	MCPD	7.641	0.000	7071407	0	2.480	N.D. #
7) T	MCPA	7.693	7.462	121.2E6	101.6E6	30.446	36.822
8) T	DICHLORPROP	0.000	7.741	0	10781936	N.D.	18.364
10) T	Pentachlo...	8.709	0.000	7761092	0	<MDL	N.D. #
12) T	2,4,5-T	9.425	9.248	33671759	11398057	7.229	3.828 #
14) T	DINOSEB	0.000	10.065	0	12188074	N.D.	5.854
15) T	Picloram	10.999	0.000	20929338	0	3.733	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
Data File : PS011076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 20:01
Operator : DD\AJ
Sample : PB129944TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:08:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

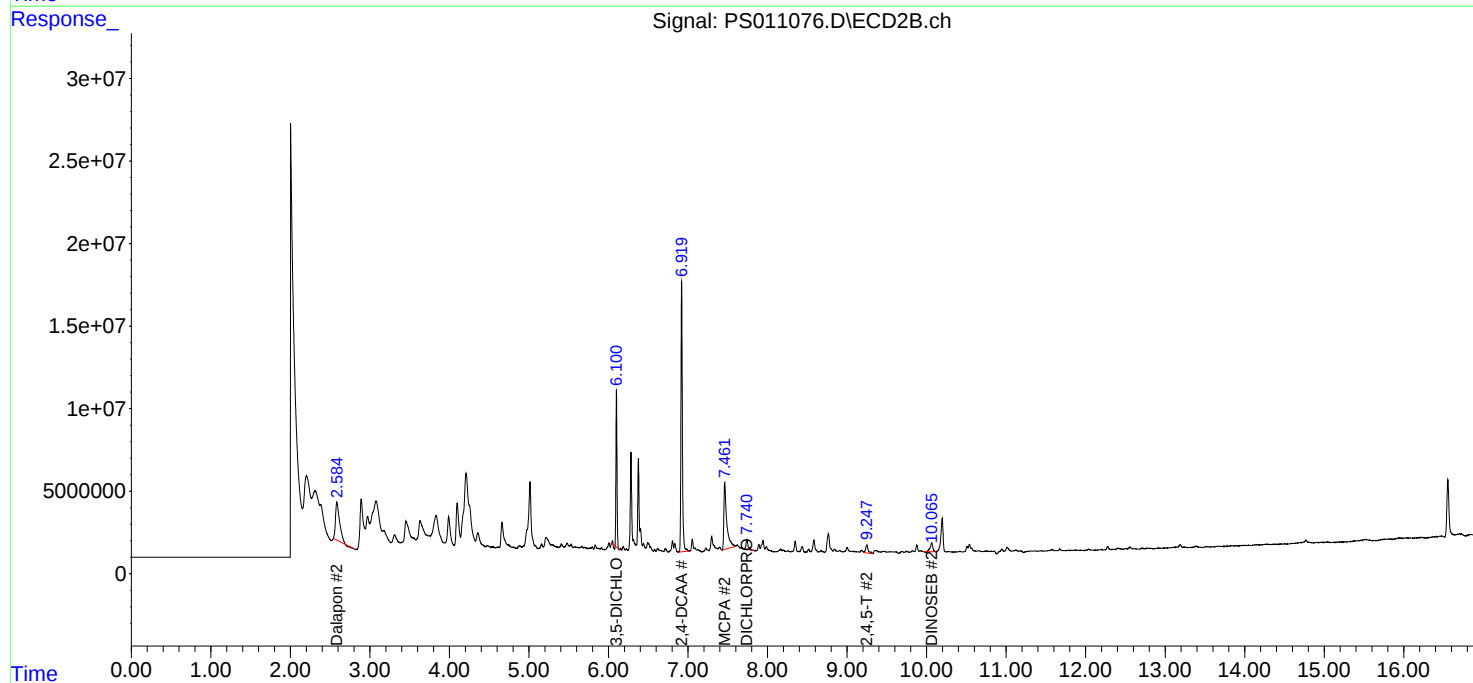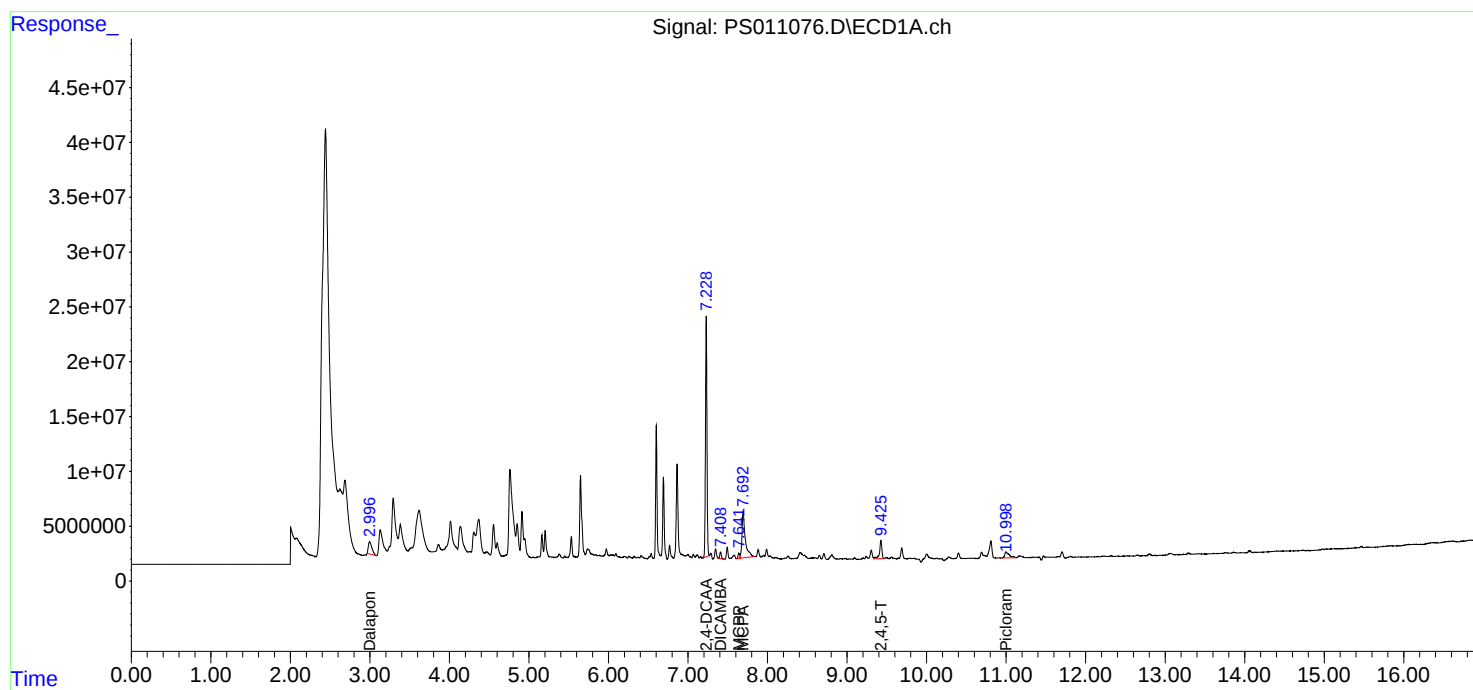


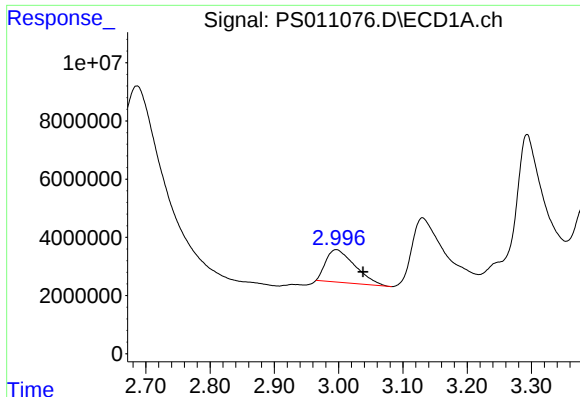

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 35078330
Conc: 31.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

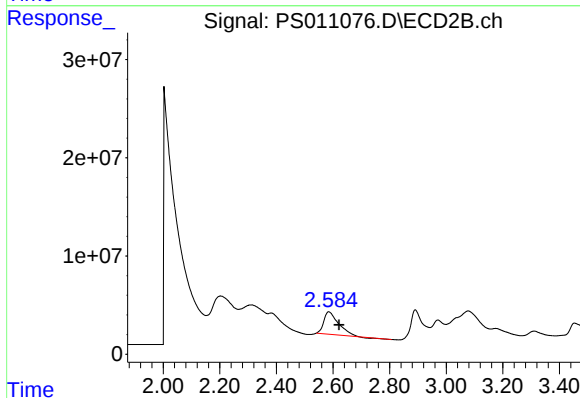


#1 Dalapon

R.T.: 2.585 min
Delta R.T.: -0.037 min
Response: 82415716
Conc: 109.25 ng/ml

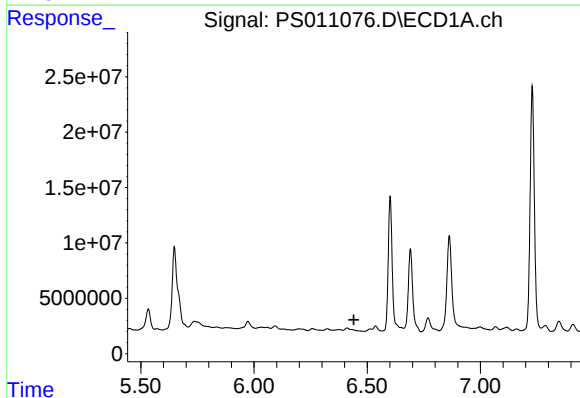


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

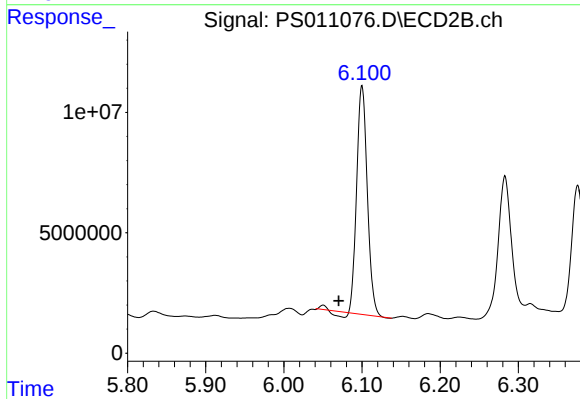

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 88443592
Conc: 106.20 ng/ml

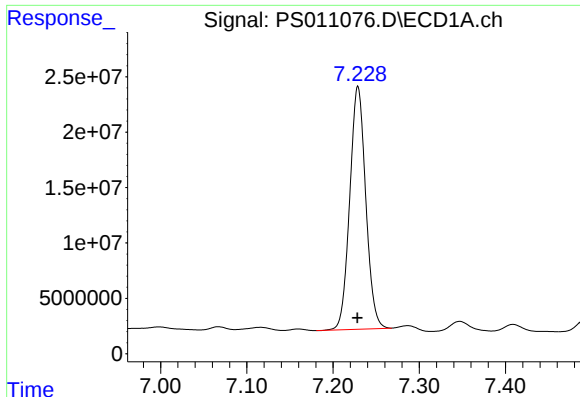

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 283344294
Conc: 312.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

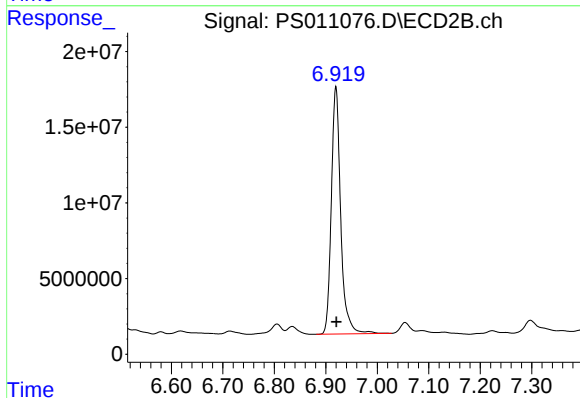


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 206673667
Conc: 373.01 ng/ml

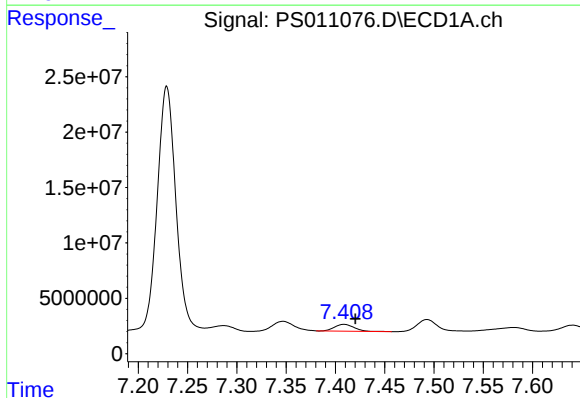


#5 DICAMBA

R.T.: 7.409 min
Delta R.T.: -0.012 min
Response: 8352234
Conc: 2.29 ng/ml

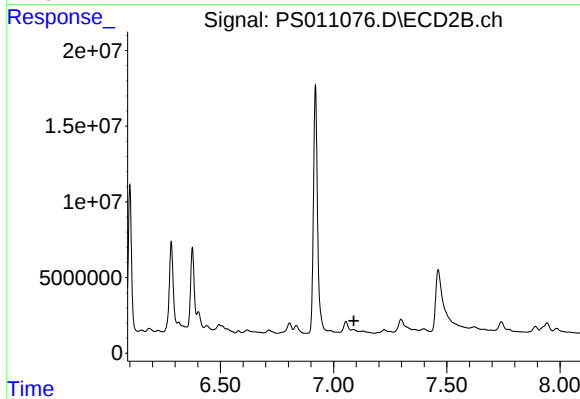

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

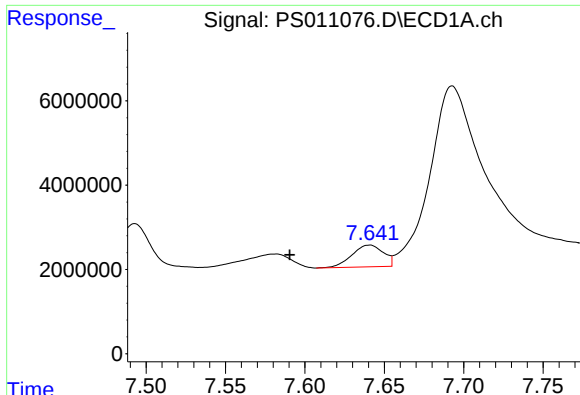

#6 MCPP


R.T.: 7.641 min
Delta R.T.: 0.050 min
Response: 7071407
Conc: 2.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

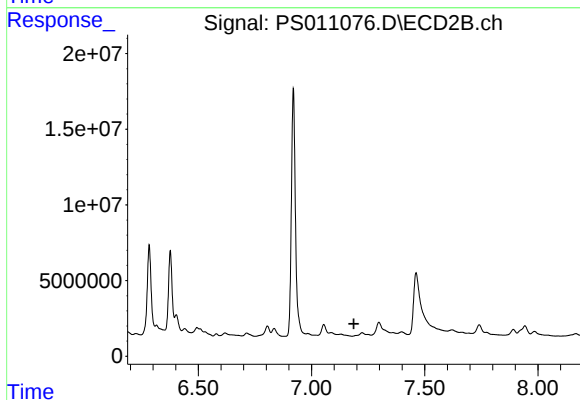


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

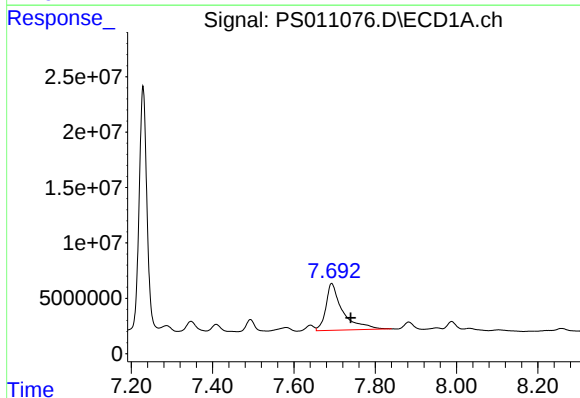


#7 MCPA

R.T.: 7.693 min
Delta R.T.: -0.047 min
Response: 121248766
Conc: 30.45 ug/ml

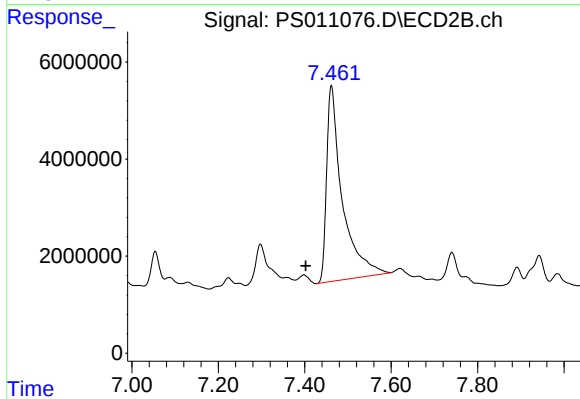

#7 MCPA


R.T.: 7.462 min
Delta R.T.: 0.059 min
Response: 101628793
Conc: 36.82 ug/ml

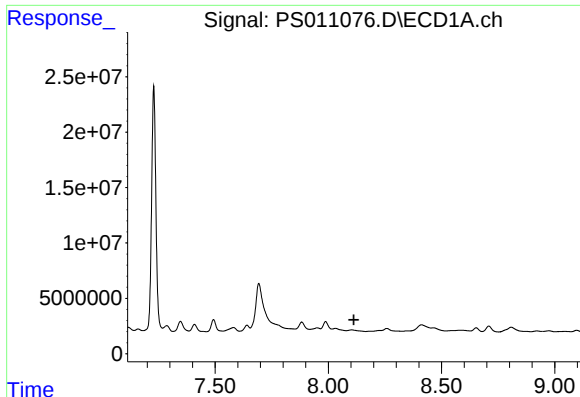

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

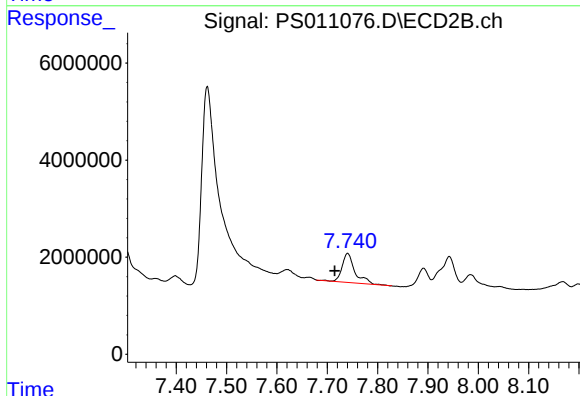


#8 DICHLORPROP

R.T.: 7.741 min
Delta R.T.: 0.025 min
Response: 10781936
Conc: 18.36 ng/ml

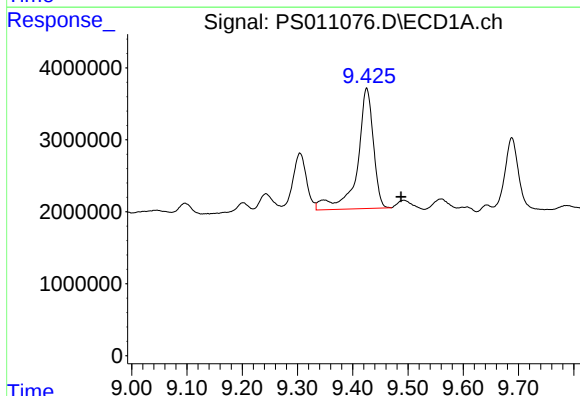


#12 2,4,5-T

R.T.: 9.425 min
Delta R.T.: -0.062 min
Response: 33671759
Conc: 7.23 ng/ml

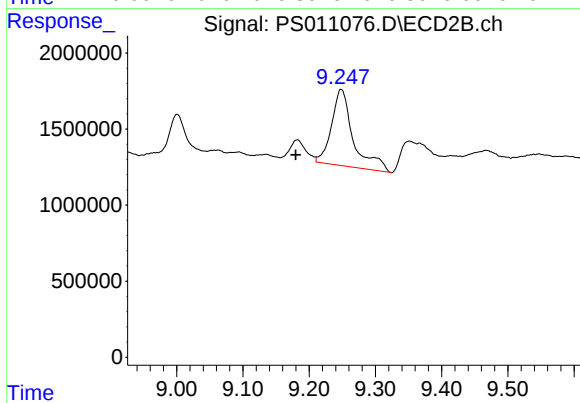

#12 2,4,5-T


R.T.: 9.248 min
Delta R.T.: 0.069 min
Response: 11398057
Conc: 3.83 ng/ml

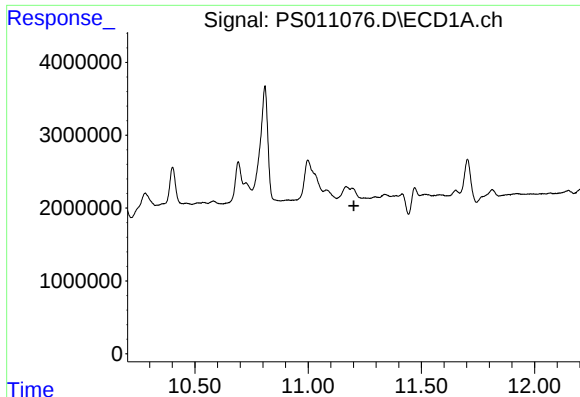

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

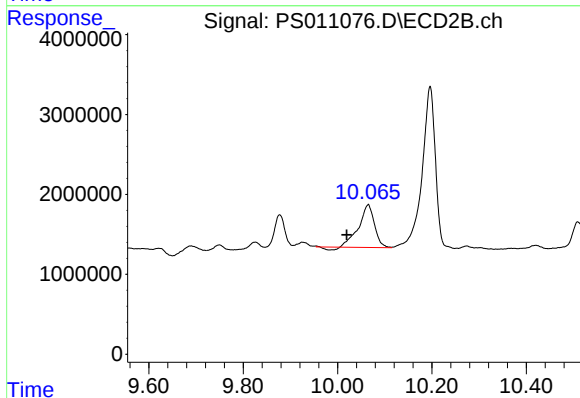


#14 DINOSEB

R.T.: 10.065 min
Delta R.T.: 0.045 min
Response: 12188074
Conc: 5.85 ng/ml

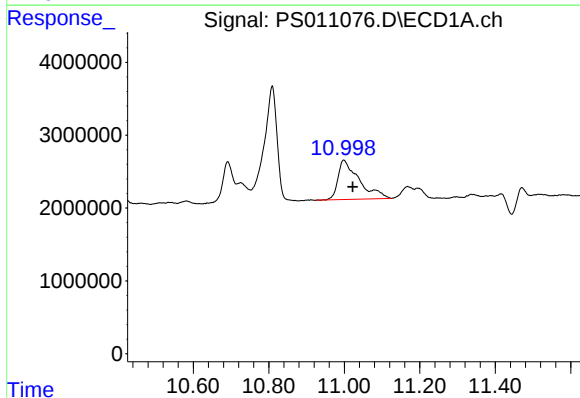

#15 Picloram

R.T.: 10.999 min
Delta R.T.: -0.024 min
Response: 20929338
Conc: 3.73 ng/ml

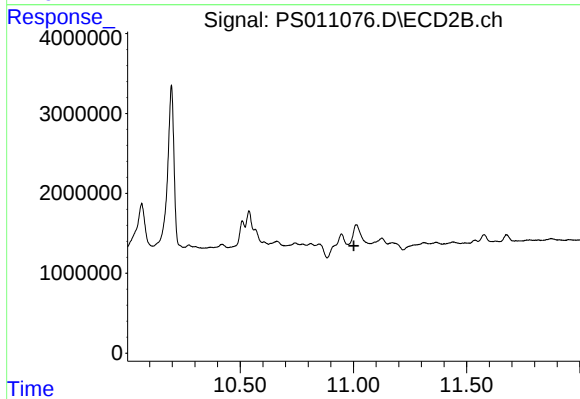

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.