

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS070220\  
 Data File : PS011085.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 02 Jul 2020 23:28  
 Operator : DD\AJ  
 Sample : L2188-01  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 03 02:10:57 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS062420.M  
 Quant Title : 8080.M  
 QLast Update : Thu Jun 25 02:45:12 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|--------|--------|----------|----------|---------|----------|
| -----                       |              |        |        |          |          |         |          |
| System Monitoring Compounds |              |        |        |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 7.228  | 6.919  | 161.5E6  | 99836232 | 178.069 | 180.185  |
| Target Compounds            |              |        |        |          |          |         |          |
| 1) T                        | Dalapon      | 2.993  | 2.581  | 26757990 | 38772558 | 23.897  | 51.398 # |
| 2) T                        | 3,5-DICHL... | 6.508  | 6.100  | 5755566  | 47448210 | 4.575   | 56.973 # |
| 5) T                        | DICAMBA      | 0.000  | 7.123  | 0        | 6100609  | N.D.    | 2.686    |
| 6) T                        | MCP          | 0.000  | 7.123  | 0        | 6100609  | N.D.    | 3.223    |
| 7) T                        | MCPA         | 7.741  | 7.383  | 26750005 | 20352450 | 6.717   | 7.374    |
| 8) T                        | DICHLORPROP  | 0.000  | 7.666  | 0        | 3617176  | N.D.    | 6.161    |
| 10) T                       | Pentachlo... | 8.713  | 0.000  | 14507523 | 0        | 1.167   | N.D. #   |
| 12) T                       | 2,4,5-T      | 9.509  | 0.000  | 5323557  | 0        | 1.143   | N.D. #   |
| 14) T                       | DINOSEB      | 11.170 | 10.032 | -4217972 | 33275999 | N.D.    | 15.982   |
| 15) T                       | Picloram     | 10.992 | 11.001 | 33531447 | 16729606 | 5.981   | 3.993 #  |
| 16) T                       | DCPA         | 0.000  | 11.001 | 0        | 16729606 | N.D.    | 4.492    |
| -----                       |              |        |        |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS070220\  
Data File : PS011085.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 02 Jul 2020 23:28  
Operator : DD\AJ  
Sample : L2188-01  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 03 02:10:57 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS062420.M  
Quant Title : 8080.M  
QLast Update : Thu Jun 25 02:45:12 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

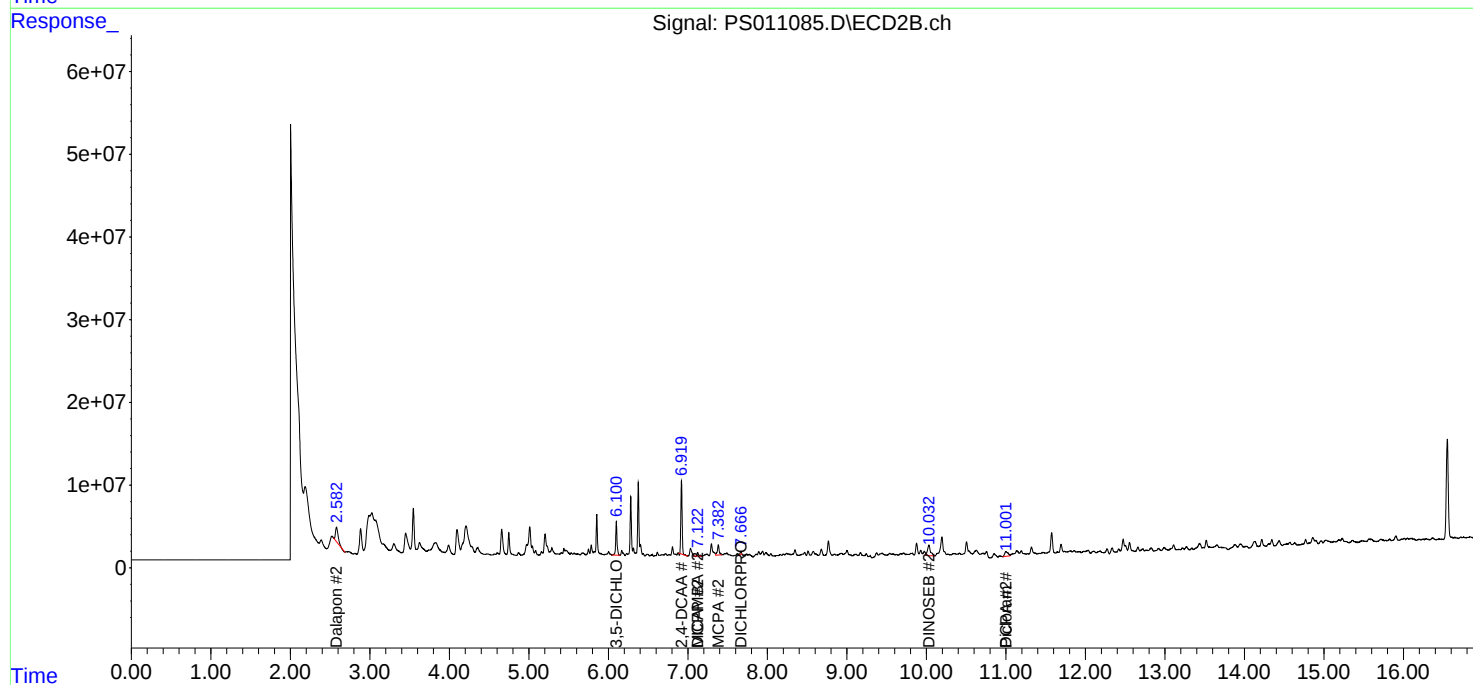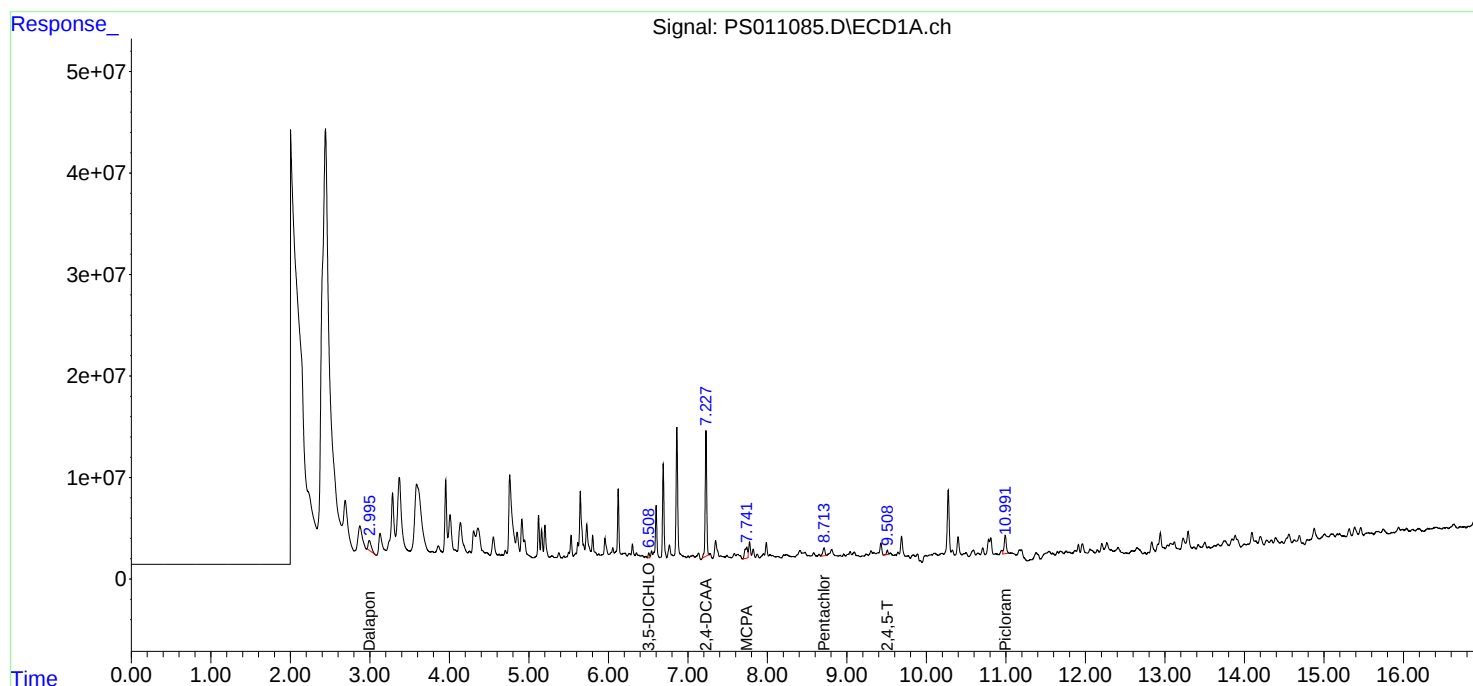


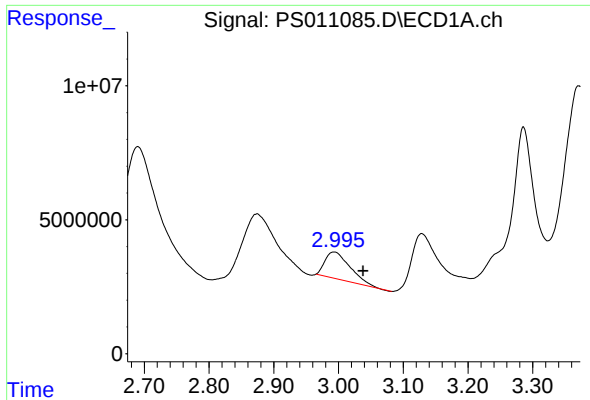

#1 Dalapon


R.T.: 2.993 min  
Delta R.T.: -0.045 min  
Response: 26757990  
Conc: 23.90 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

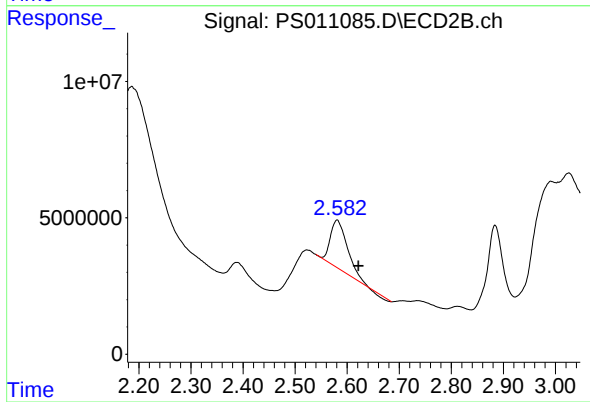


#1 Dalapon

R.T.: 2.581 min  
Delta R.T.: -0.041 min  
Response: 38772558  
Conc: 51.40 ng/ml

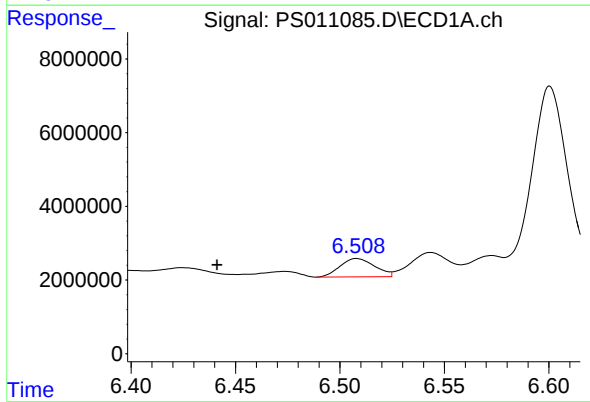


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.508 min  
Delta R.T.: 0.067 min  
Response: 5755566  
Conc: 4.57 ng/ml

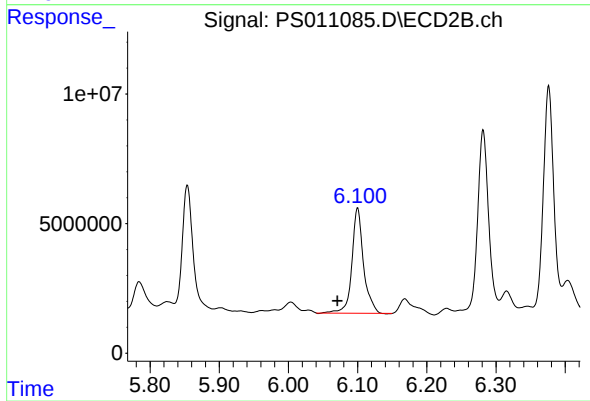

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min  
Delta R.T.: 0.030 min  
Response: 47448210  
Conc: 56.97 ng/ml

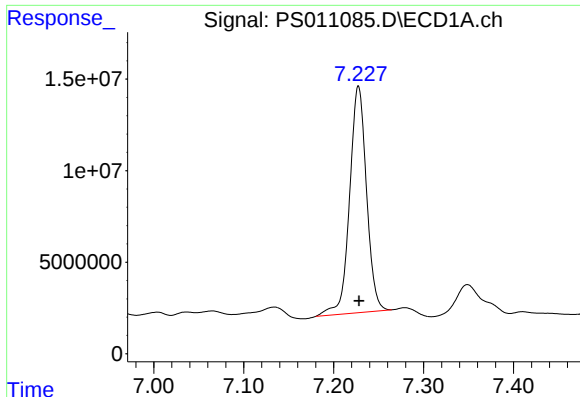

#4 2,4-DCAA


R.T.: 7.228 min  
Delta R.T.: 0.000 min  
Response: 161476023  
Conc: 178.07 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

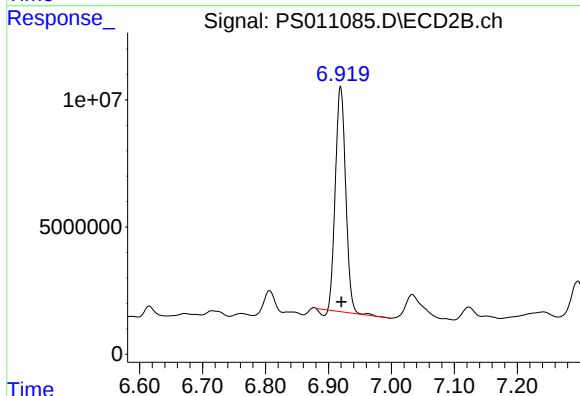


#4 2,4-DCAA

R.T.: 6.919 min  
Delta R.T.: -0.001 min  
Response: 99836232  
Conc: 180.19 ng/ml

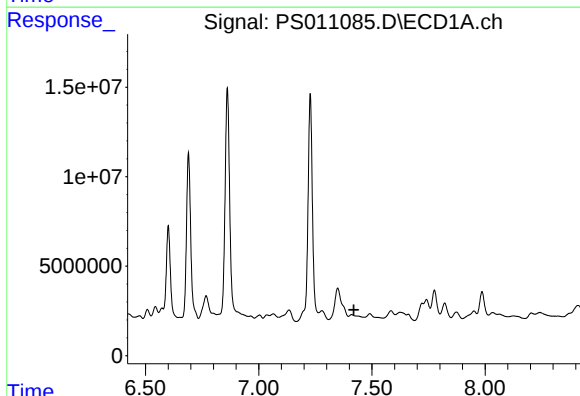


#5 DICAMBA

R.T.: 0.000 min  
Exp R.T. : 7.420 min  
Response: 0  
Conc: N.D.

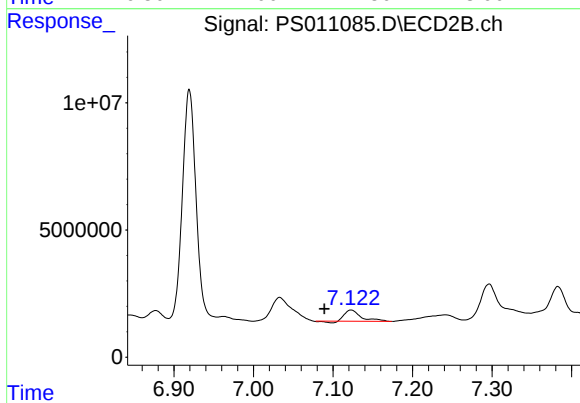

#5 DICAMBA


R.T.: 7.123 min  
Delta R.T.: 0.034 min  
Response: 6100609  
Conc: 2.69 ng/ml

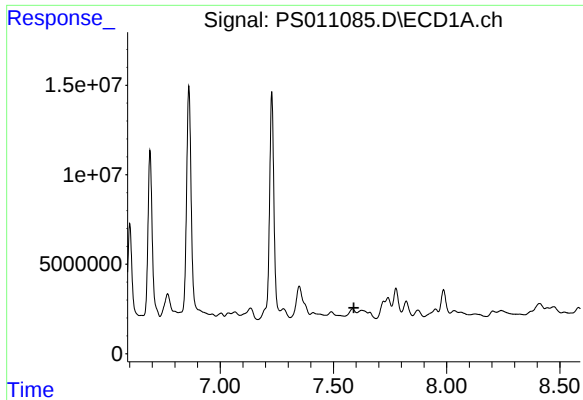

#6 MCPP


R.T.: 0.000 min  
Exp R.T.: 7.590 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

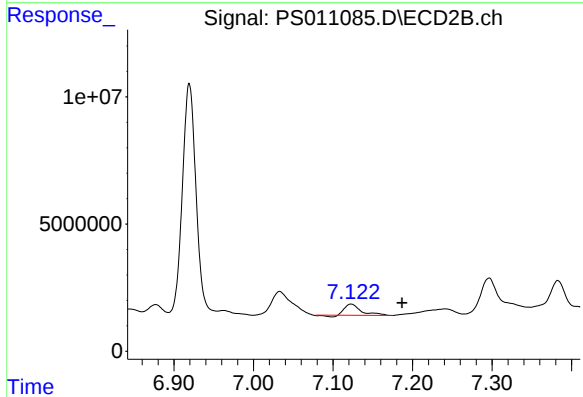


#6 MCPP

R.T.: 7.123 min  
Delta R.T.: -0.064 min  
Response: 6100609  
Conc: 3.22 ug/ml

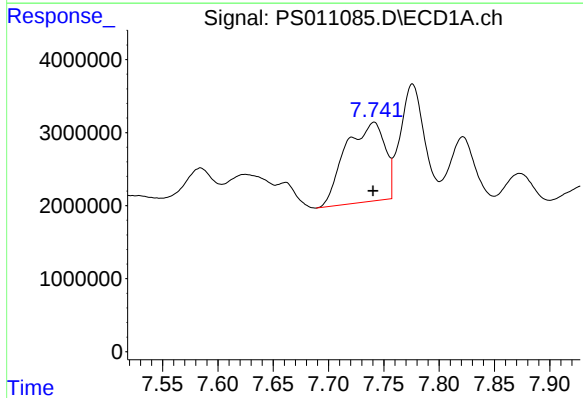


#7 MCPA

R.T.: 7.741 min  
Delta R.T.: 0.000 min  
Response: 26750005  
Conc: 6.72 ug/ml

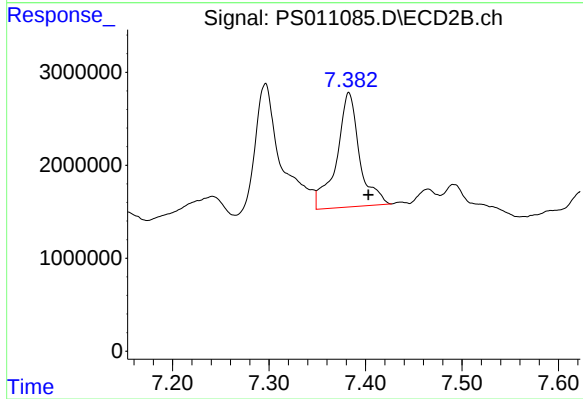

#7 MCPA


R.T.: 7.383 min  
Delta R.T.: -0.020 min  
Response: 20352450  
Conc: 7.37 ug/ml

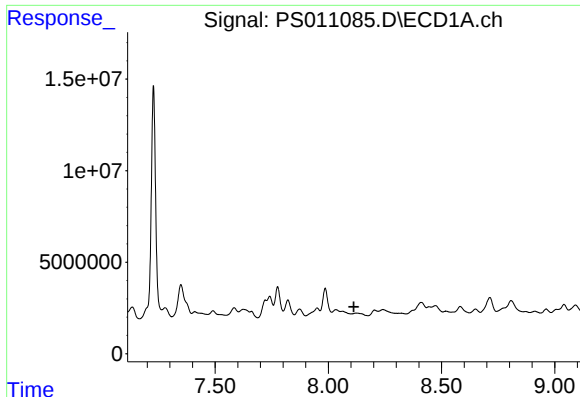

#8 DICHLORPROP


R.T.: 0.000 min  
Exp R.T.: 8.113 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

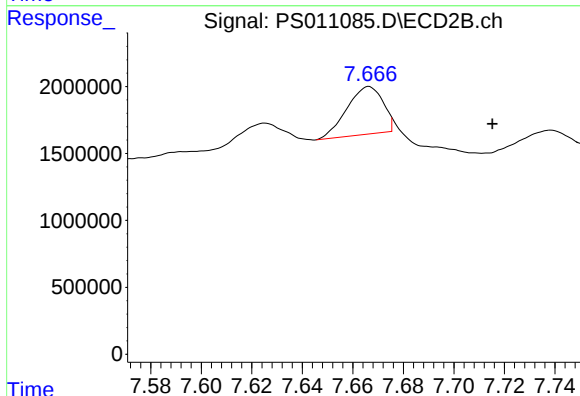


#8 DICHLORPROP

R.T.: 7.666 min  
Delta R.T.: -0.049 min  
Response: 3617176  
Conc: 6.16 ng/ml

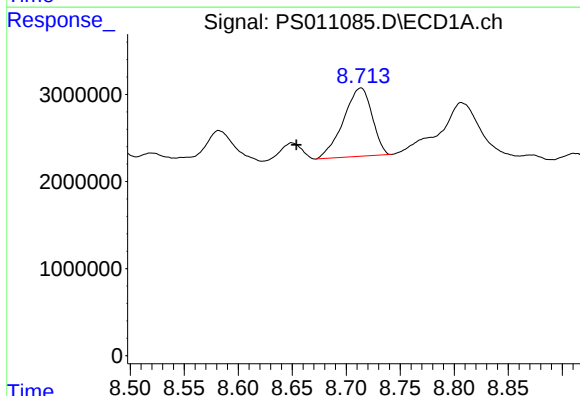


#10 Pentachlorophenol

R.T.: 8.713 min  
Delta R.T.: 0.059 min  
Response: 14507523  
Conc: 1.17 ng/ml

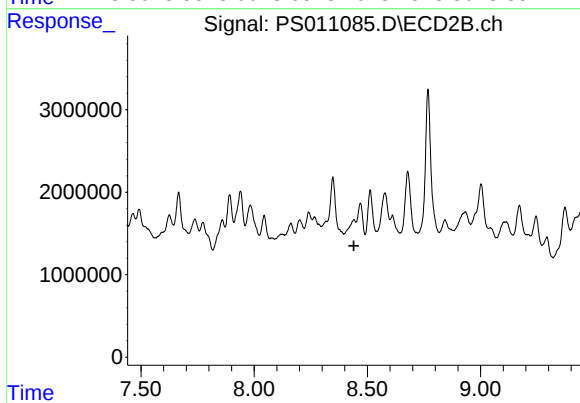

#10 Pentachlorophenol


R.T.: 0.000 min  
Exp R.T.: 8.440 min  
Response: 0  
Conc: N.D.

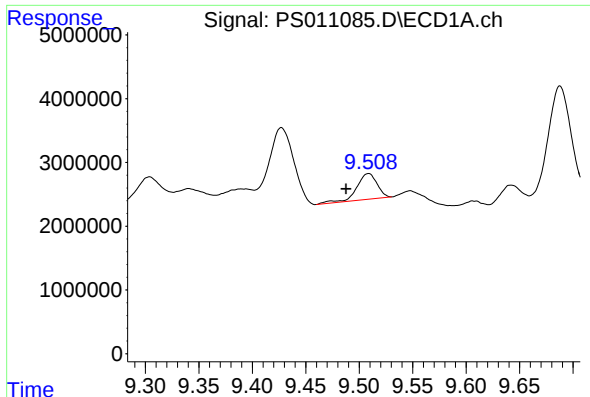

#12 2,4,5-T


R.T.: 9.509 min  
Delta R.T.: 0.021 min  
Response: 5323557  
Conc: 1.14 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

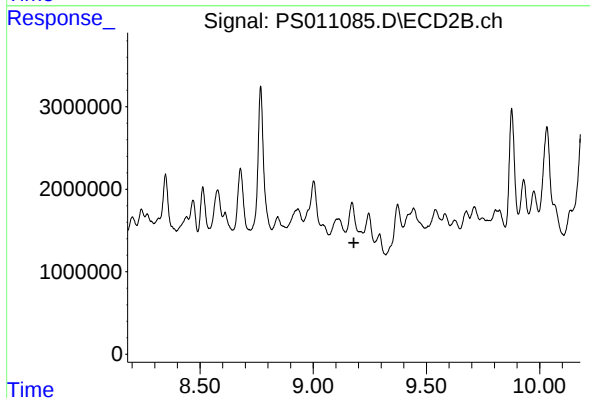


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 9.179 min  
Response: 0  
Conc: N.D.

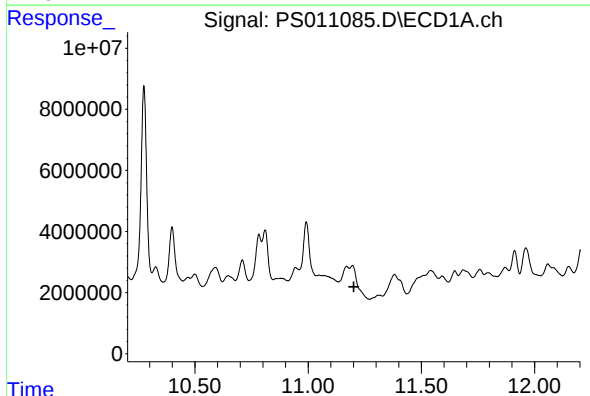


#14 DINOSEB

R.T.: 11.170 min  
Delta R.T.: -0.032 min  
Response: -4217972  
Conc: N.D.

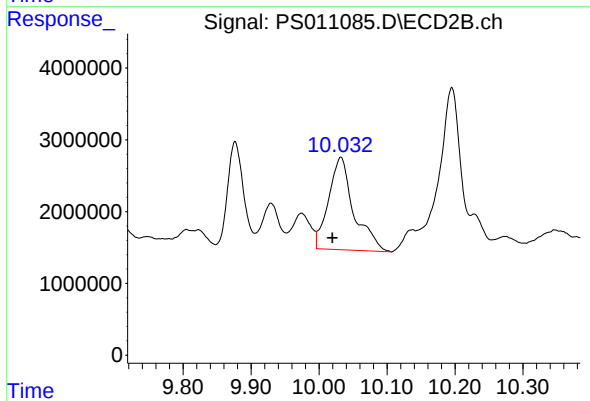

#14 DINOSEB


R.T.: 10.032 min  
Delta R.T.: 0.012 min  
Response: 33275999  
Conc: 15.98 ng/ml

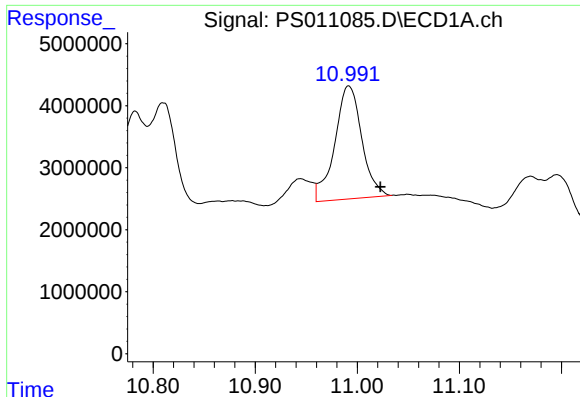

#15 Picloram


R.T.: 10.992 min  
Delta R.T.: -0.031 min  
Response: 33531447  
Conc: 5.98 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

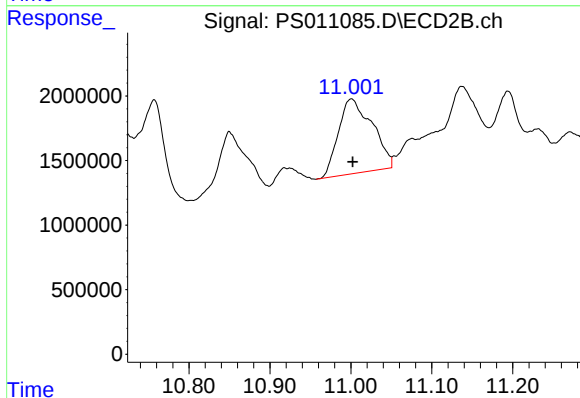


#15 Picloram

R.T.: 11.001 min  
Delta R.T.: -0.001 min  
Response: 16729606  
Conc: 3.99 ng/ml

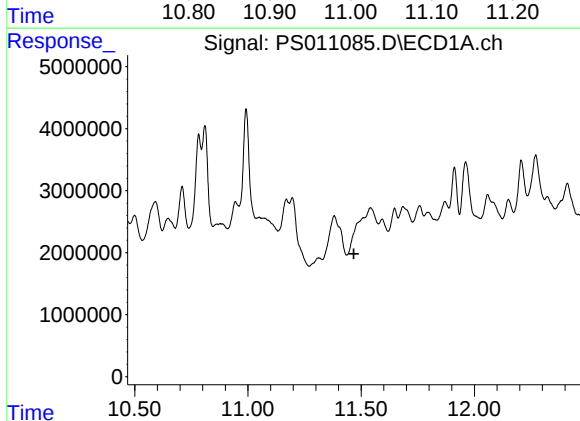

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 11.468 min  
Response: 0  
Conc: N.D.

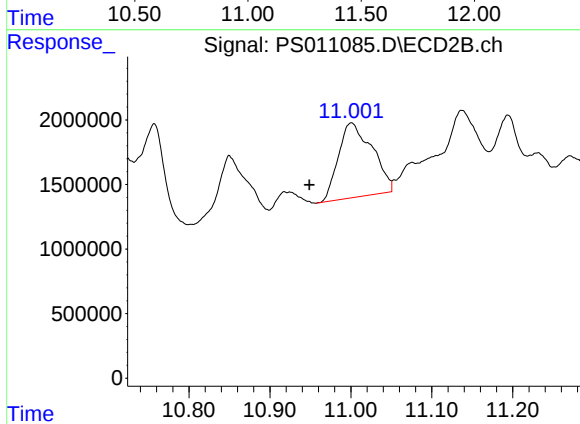

#16 DCPA

R.T.: 11.001 min  
Delta R.T.: 0.052 min  
Response: 16729606  
Conc: 4.49 ng/ml