

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
 Data File : PS011087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2020 00:14
 Operator : DD\AJ
 Sample : L3197-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:11:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	789.0E6	435.0E6	870.054	785.016
Target Compounds							
2) T	3,5-DICHL...	0.000	6.100	0	42903610	N.D.	51.516
3) T	4-Nitroph...	7.052	0.000	15182126	0	38.034	N.D. #
5) T	DICAMBA	7.417	0.000	1451496	0	<MDL	N.D. #
6) T	MCP	7.621	0.000	32577778	0	11.425	N.D. #
7) T	MCPA	7.719	7.412	66793984	14721408	16.772	5.334 #
8) T	DICHLORPROP	0.000	7.667	0	15491615	N.D.	26.385
10) T	Pentachlo...	8.638	0.000	27645855	0	2.223	N.D. #
11) T	2,4,5-TP ...	9.230	0.000	26670512	0	5.371	N.D. #
12) T	2,4,5-T	9.510	0.000	7299222	0	1.567	N.D. #
13) T	2,4-DB	9.992	9.693	7898465	8154835	13.290	19.842 #
14) T	DINOSEB	11.167	10.037	11703713	17813189	3.268	8.555 #
15) T	Picloram	10.993	0.000	62414693	0	11.133	N.D. #
16) T	DCPA	11.536	10.925	26063398	9511451	4.263	2.554 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
Data File : PS011087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2020 00:14
Operator : DD\AJ
Sample : L3197-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:11:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

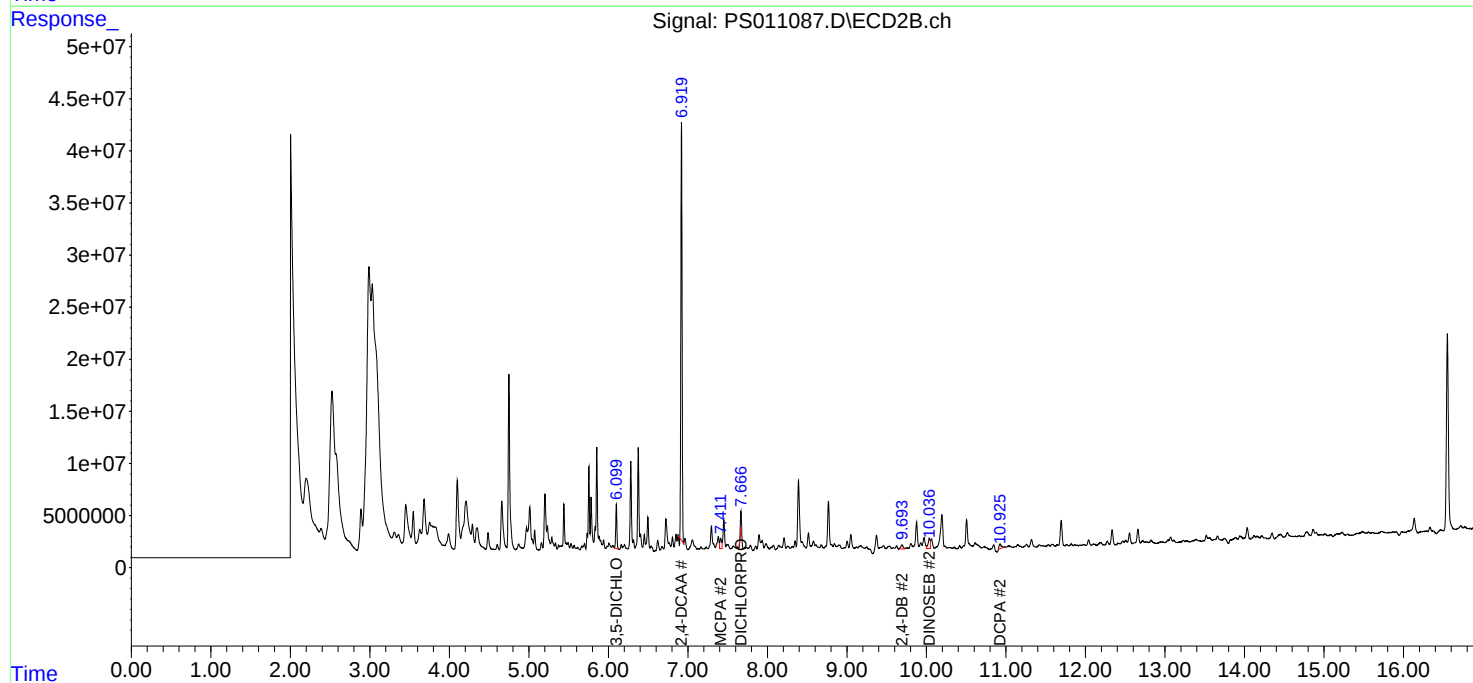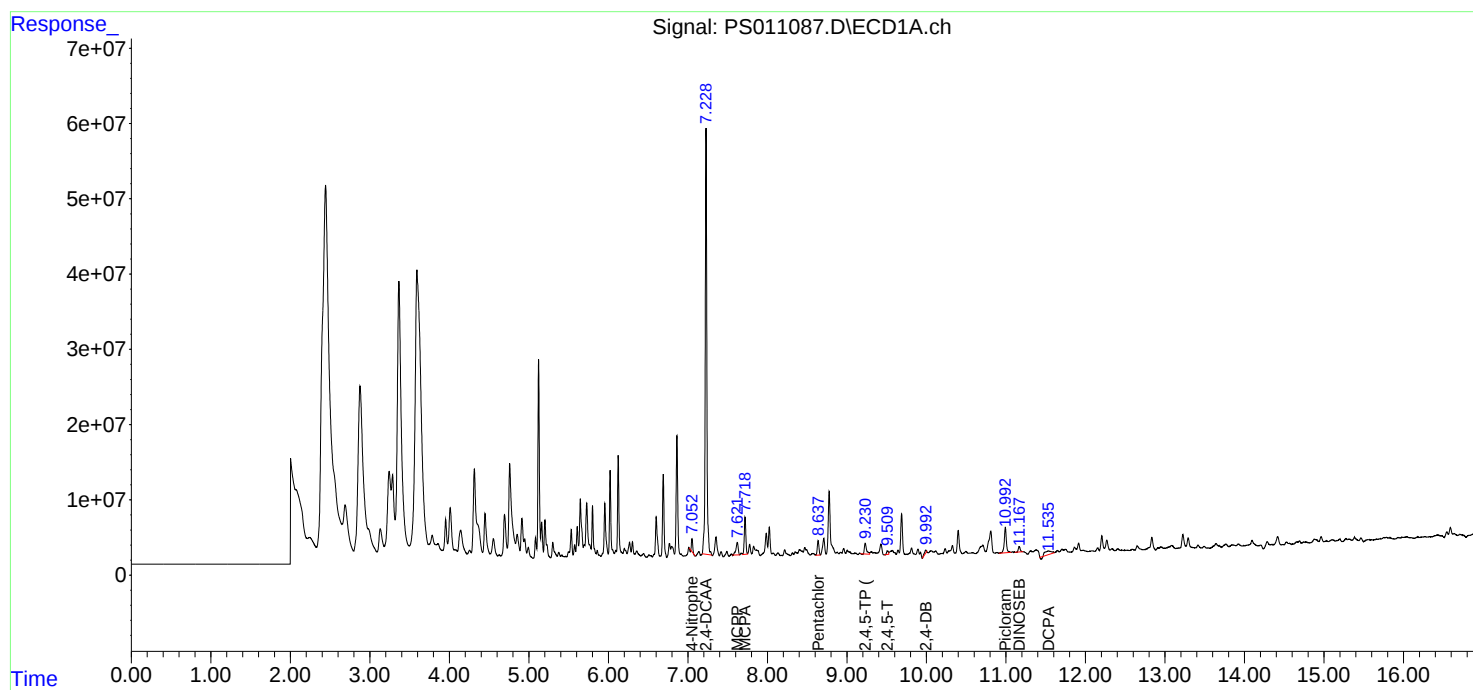


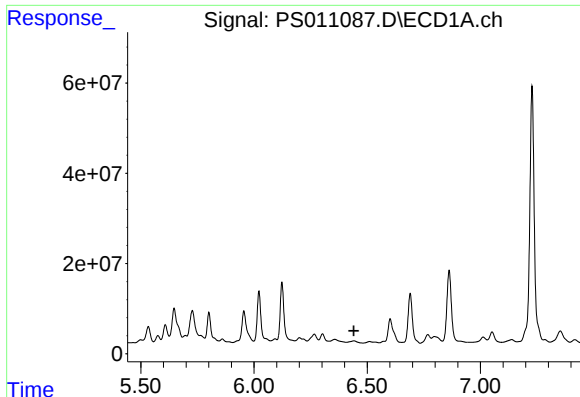

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

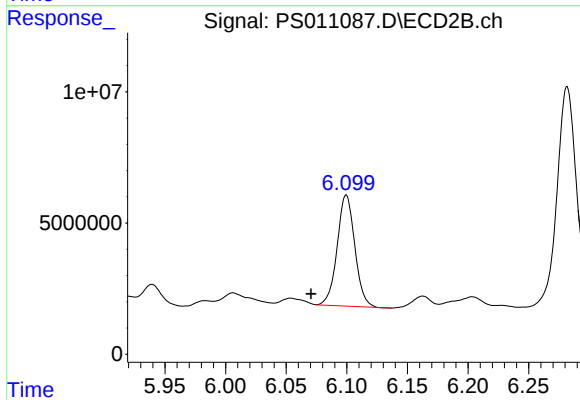


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 42903610
Conc: 51.52 ng/ml

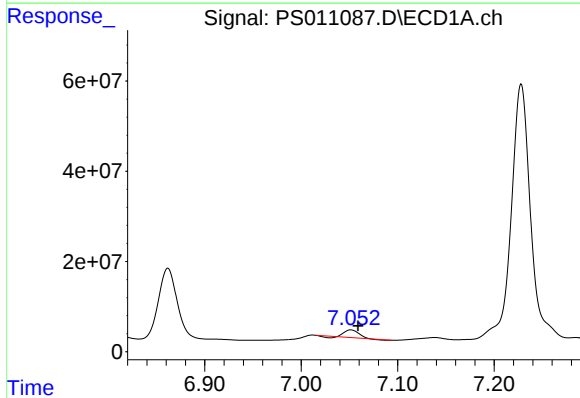


#3 4-Nitrophenol

R.T.: 7.052 min
Delta R.T.: -0.007 min
Response: 15182126
Conc: 38.03 ng/ml

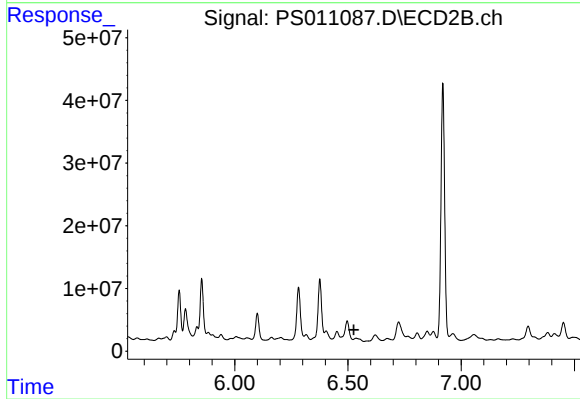

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.526 min
Response: 0
Conc: N.D.

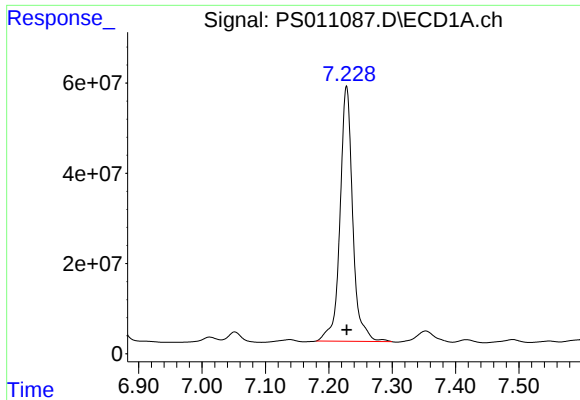

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 788980836
Conc: 870.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

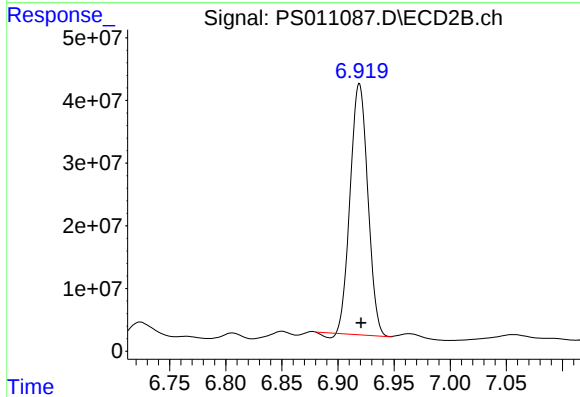


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 434958819
Conc: 785.02 ng/ml

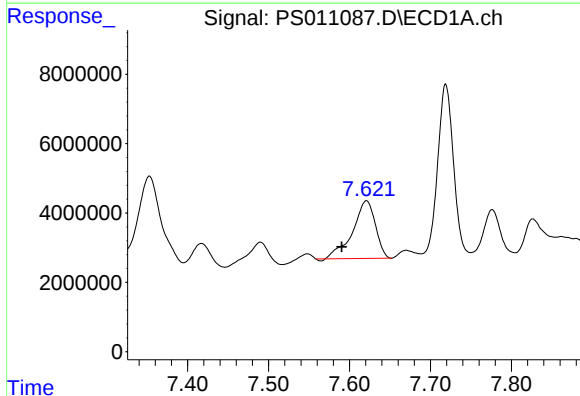


#6 MCPP

R.T.: 7.621 min
Delta R.T.: 0.030 min
Response: 32577778
Conc: 11.42 ug/ml

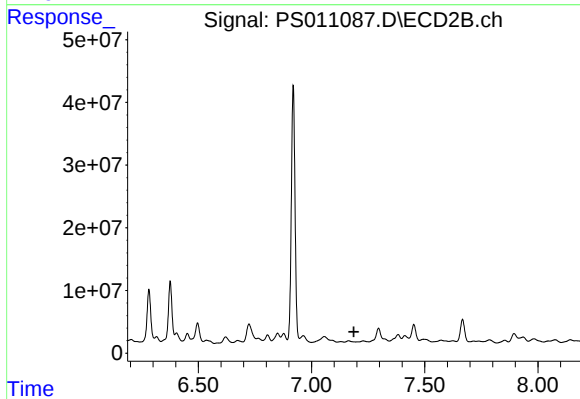

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

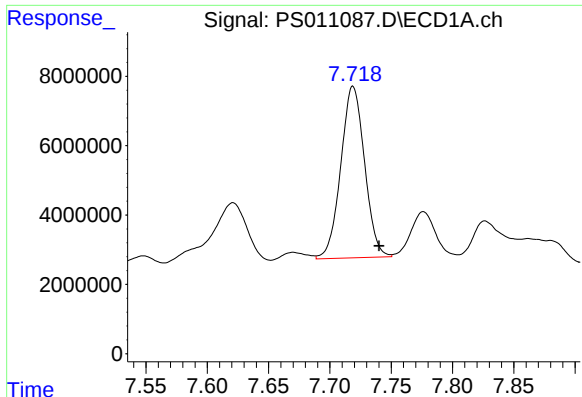

#7 MCPA


R.T.: 7.719 min
Delta R.T.: -0.021 min
Response: 66793984
Conc: 16.77 ug/ml

Instrument :
ECD_S
ClientSampleId :

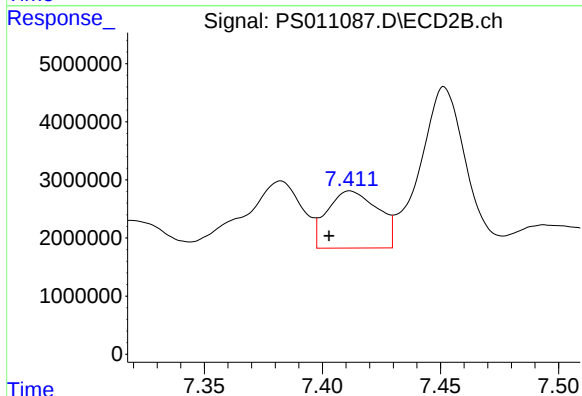


#7 MCPA

R.T.: 7.412 min
Delta R.T.: 0.009 min
Response: 14721408
Conc: 5.33 ug/ml

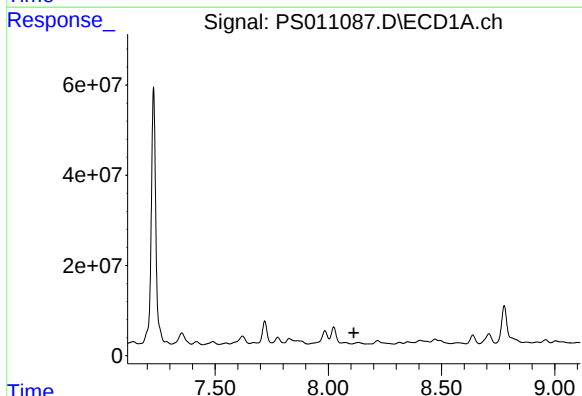


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

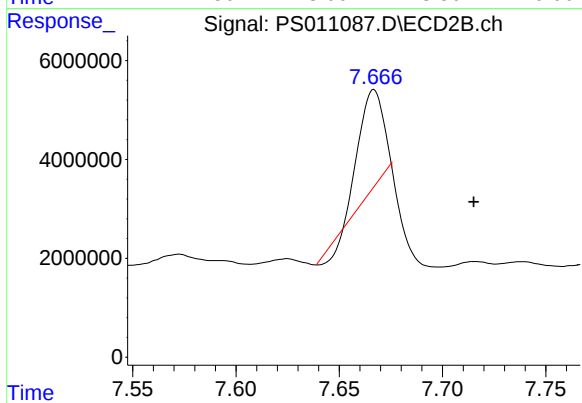

#8 DICHLORPROP


R.T.: 7.667 min
Delta R.T.: -0.048 min
Response: 15491615
Conc: 26.39 ng/ml

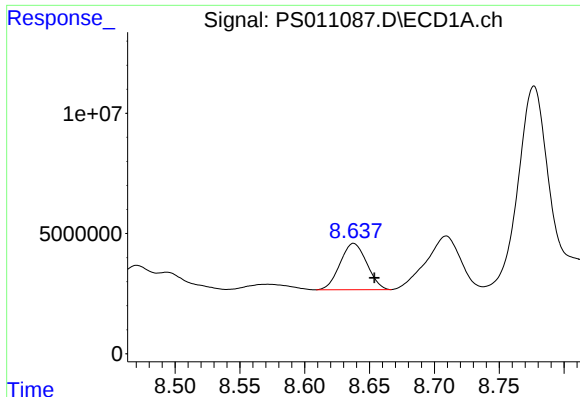

#10 Pentachlorophenol


R.T.: 8.638 min
Delta R.T.: -0.016 min
Response: 27645855
Conc: 2.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

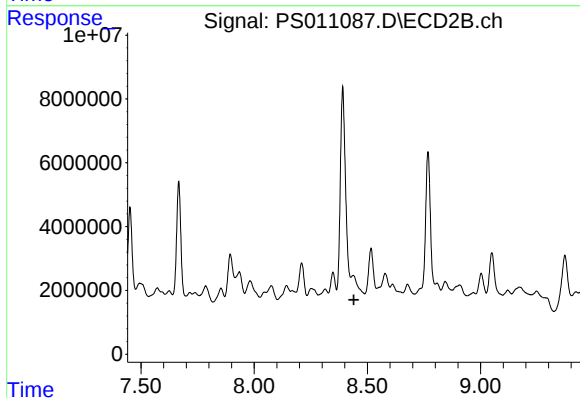


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

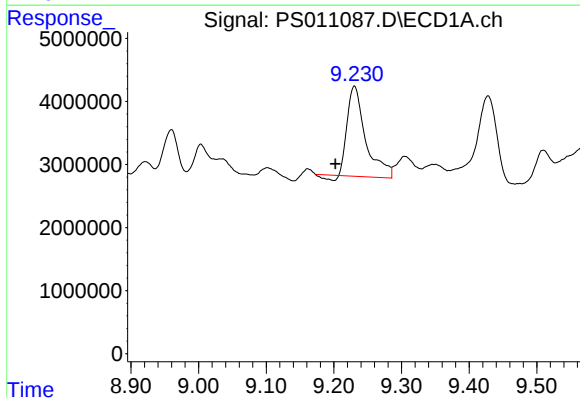


#11 2,4,5-TP (SILVEX)

R.T.: 9.230 min
Delta R.T.: 0.028 min
Response: 26670512
Conc: 5.37 ng/ml

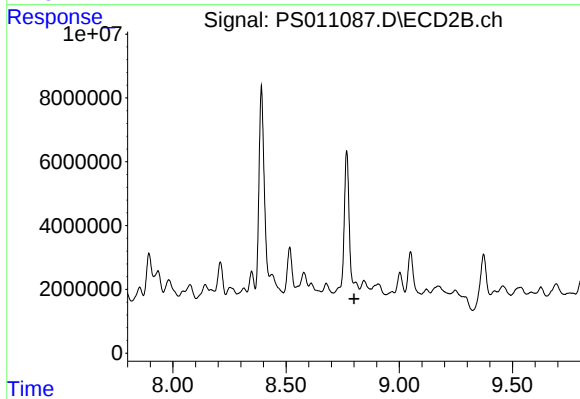

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.800 min
Response: 0
Conc: N.D.

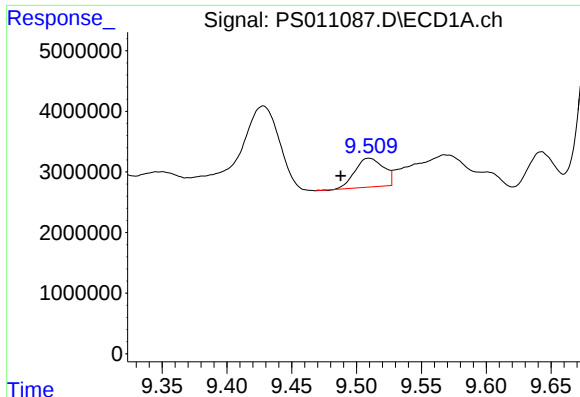

#12 2,4,5-T


R.T.: 9.510 min
Delta R.T.: 0.022 min
Response: 7299222
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

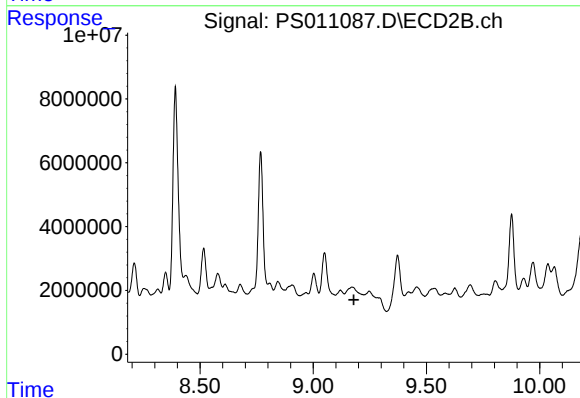


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

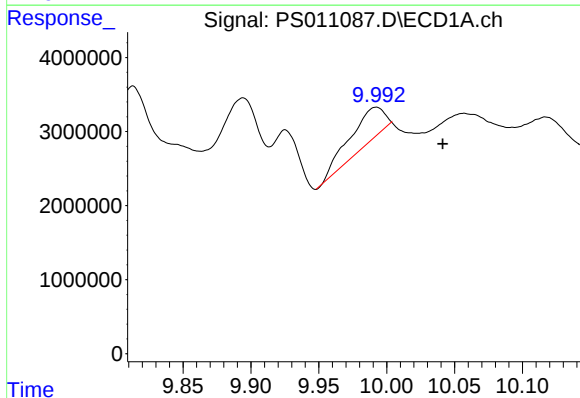


#13 2,4-DB

R.T.: 9.992 min
Delta R.T.: -0.049 min
Response: 7898465
Conc: 13.29 ng/ml

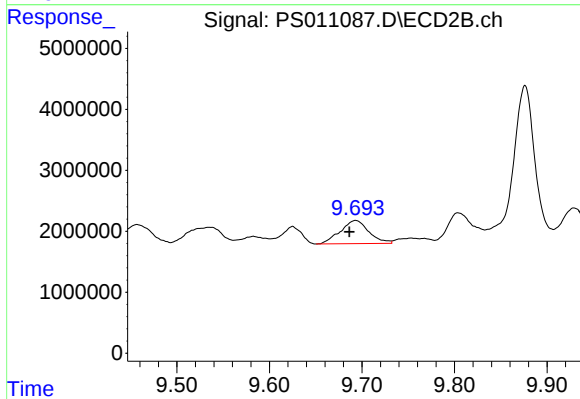

#13 2,4-DB


R.T.: 9.693 min
Delta R.T.: 0.007 min
Response: 8154835
Conc: 19.84 ng/ml

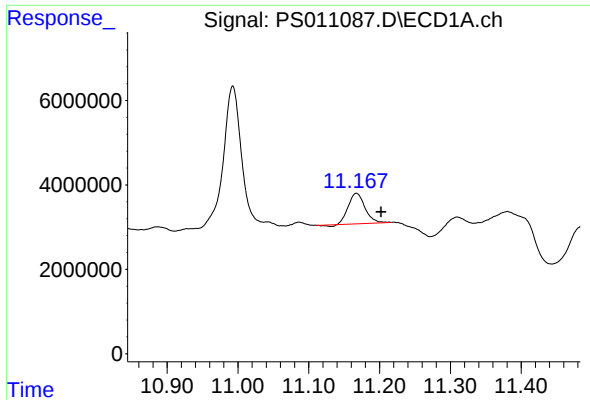

#14 DINOSEB


R.T.: 11.167 min
Delta R.T.: -0.035 min
Response: 11703713
Conc: 3.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

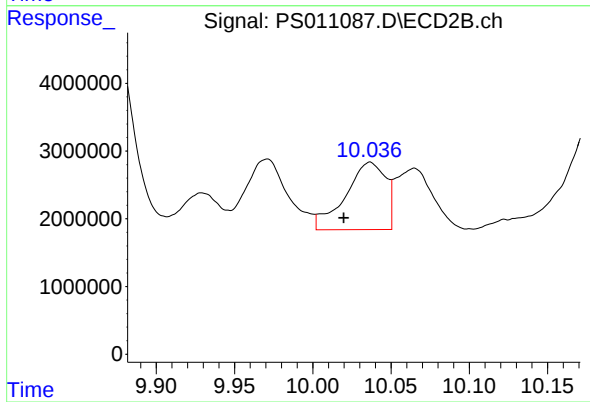


#14 DINOSEB

R.T.: 10.037 min
Delta R.T.: 0.017 min
Response: 17813189
Conc: 8.56 ng/ml

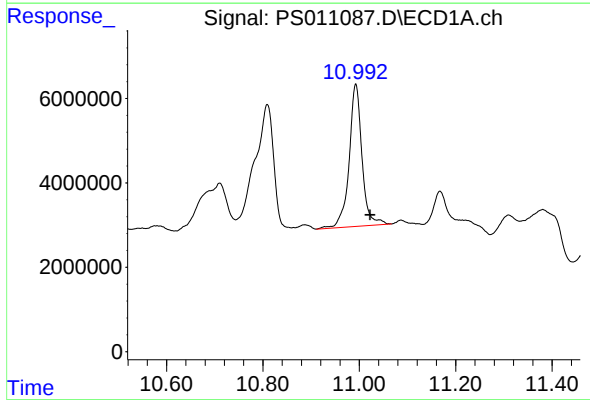


#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.030 min
Response: 62414693
Conc: 11.13 ng/ml

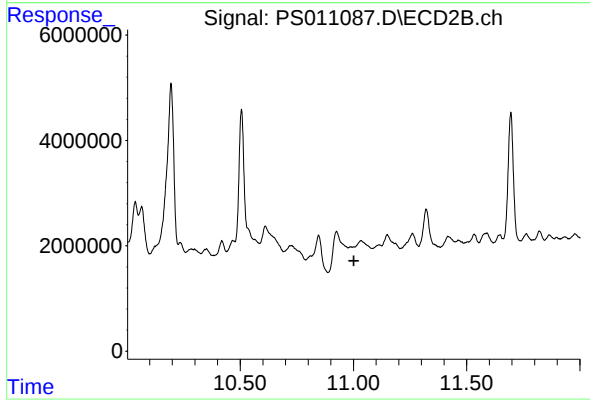

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.

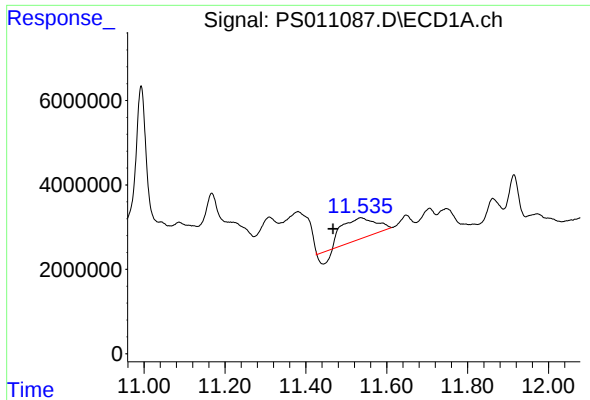

#16 DCPA

R.T.: 11.536 min
Delta R.T.: 0.068 min
Response: 26063398
Conc: 4.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

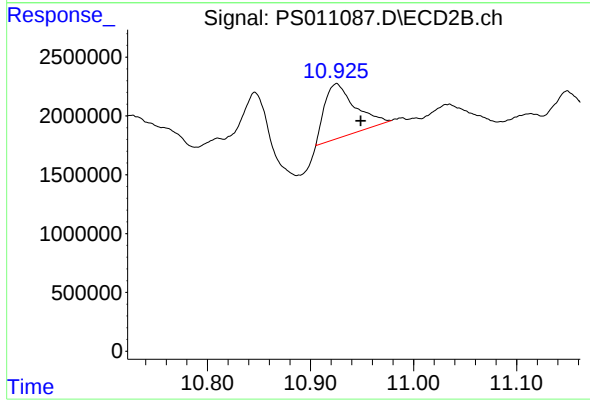

#16 DCPA

R.T.: 10.925 min
Delta R.T.: -0.023 min
Response: 9511451
Conc: 2.55 ng/ml