

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
 Data File : PS011087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2020 00:14
 Operator : DD\AJ
 Sample : L3197-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 MH-2-COMP

Manual Integrations
 APPROVED

Ankita
 7/6/2020 1:42:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:11:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	789.0E6	453.6E6	870.054	818.603m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070220\
Data File : PS011087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2020 00:14
Operator : DD\AJ
Sample : L3197-08
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
MH-2-COMP


Manual Integrations
APPROVED

Ankita
7/6/2020 1:42:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:11:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

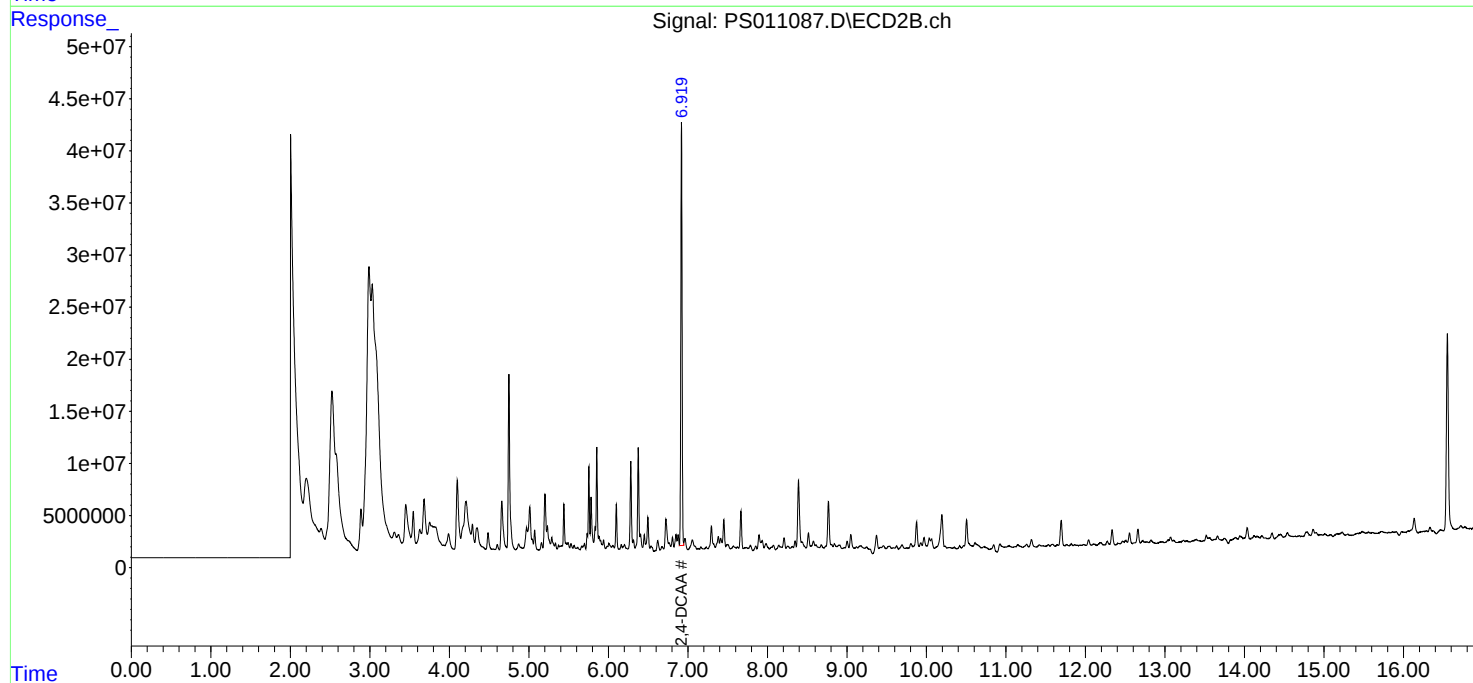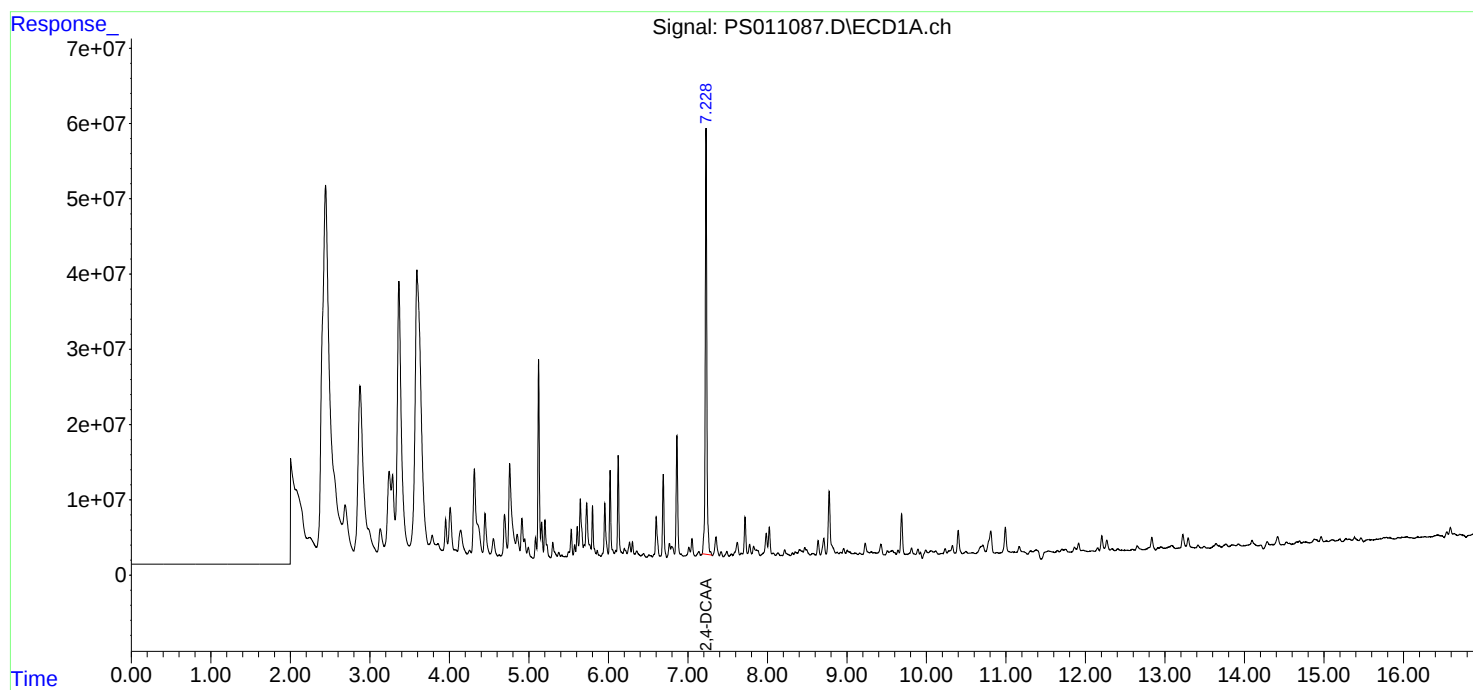

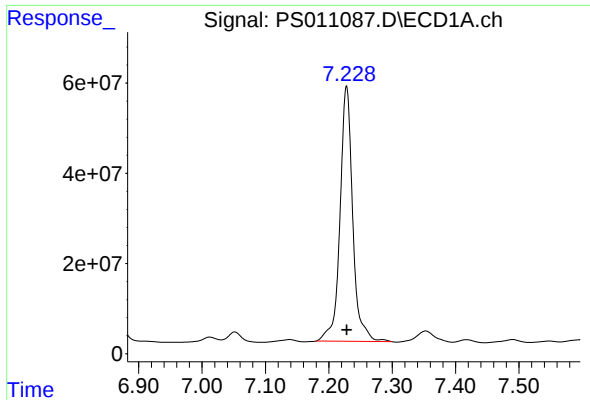


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 788980836
Conc: 870.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
MH-2-COMP

Manual Integrations
APPROVED

Ankita
7/6/2020 1:42:29 PM

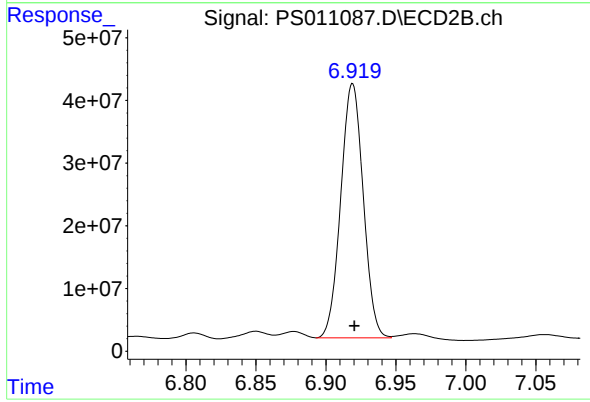

#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.002 min
Response: 453568249
Conc: 818.60 ng/ml m