

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
 Data File : PS000749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 09:01
 Operator : UA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:52:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	11.192	0	32923	N.D.	0.097 #
Target Compounds							
1) T	Dalapon	0.000	2.555	0	36712	N.D.	0.084 #
5) T	DICAMBA	0.000	11.485	0	29759	N.D.	0.024 #
6) T	MCPD	0.000	11.722	0	164062	N.D.	0.171 #
10) T	Pentachlo...	0.000	13.646	0	352122	N.D.	0.074 #
11) T	2,4,5-TP ...	0.000	14.254	0	678200	N.D.	0.349 #
12) T	2,4,5-T	0.000	14.836	0	388071	N.D.	0.229 #
14) T	DINOSEB	0.000	15.909	0	633350	N.D.	0.485 #
15) T	Picloram	0.000	17.152	0	2886221	N.D.	1.157 #
16) T	DCPA	0.000	17.087	0	3447714	N.D.	1.495 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
Data File : PS000749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 09:01
Operator : UA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:52:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

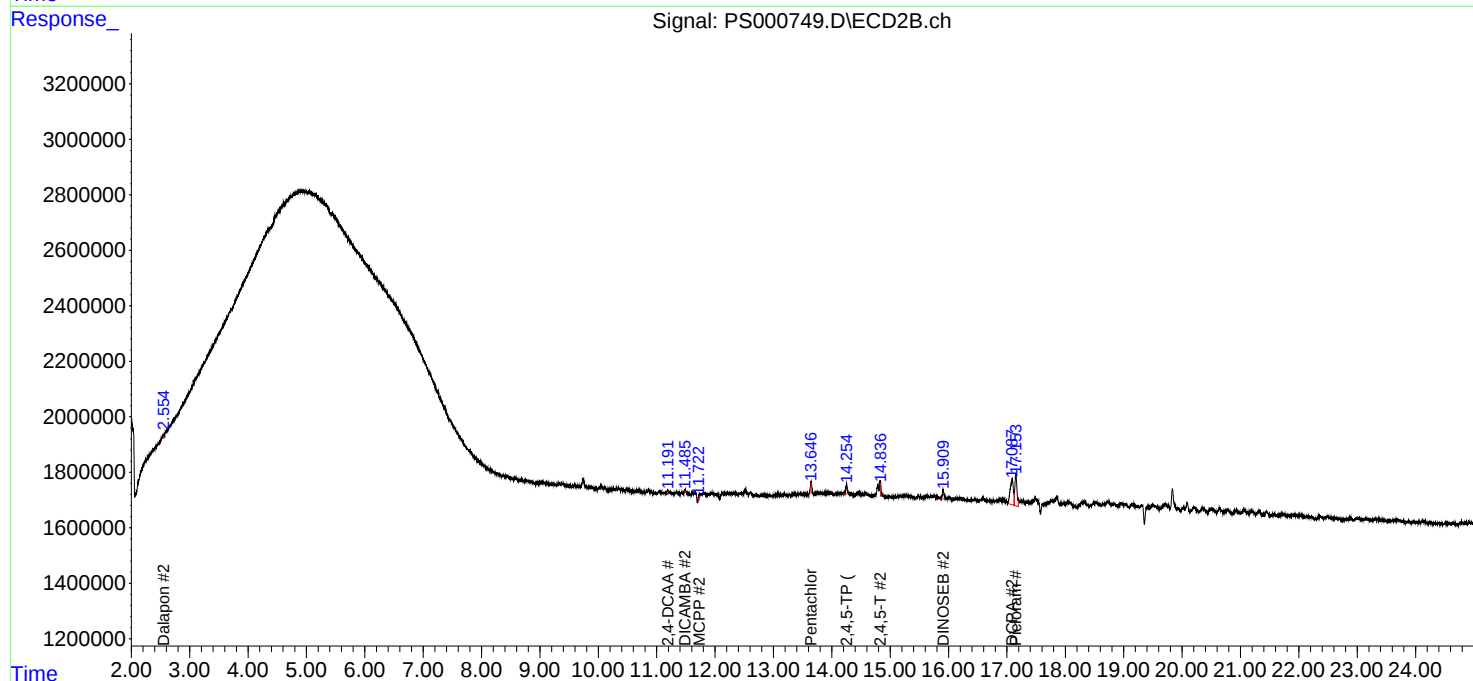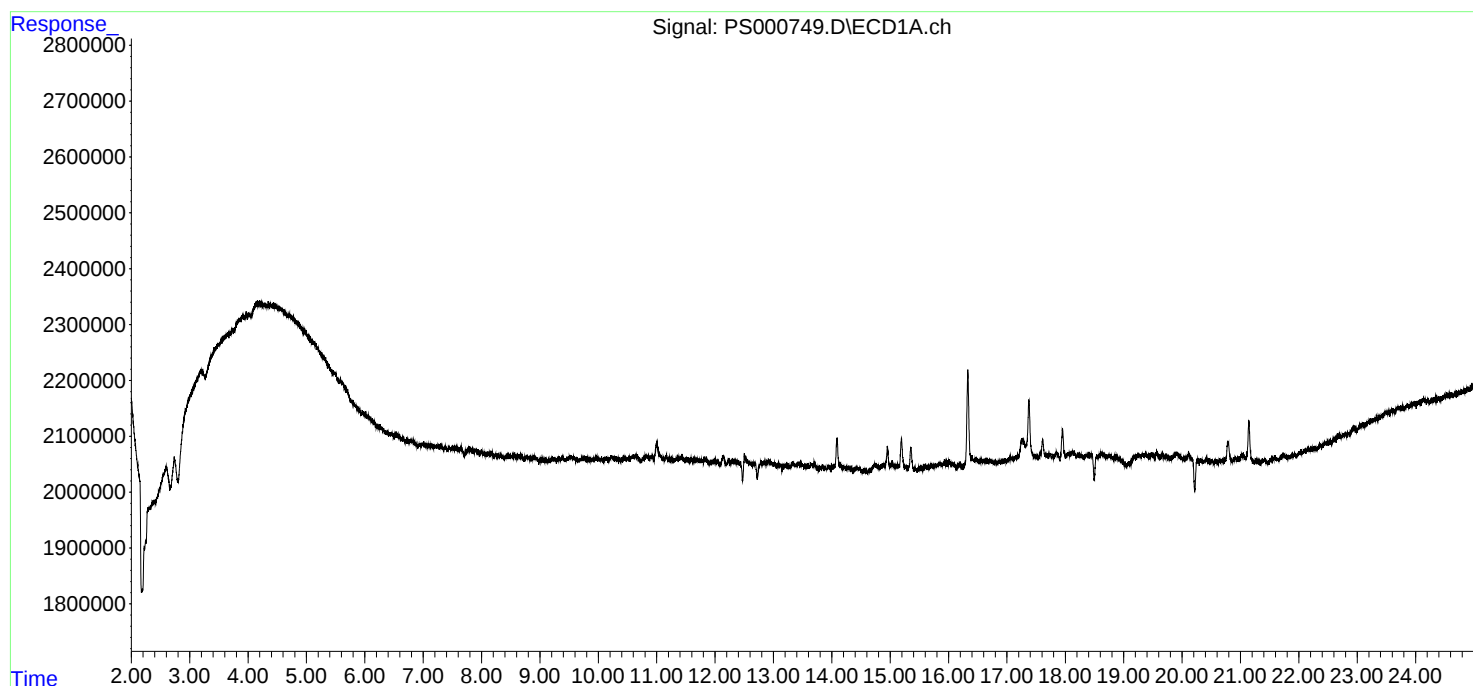


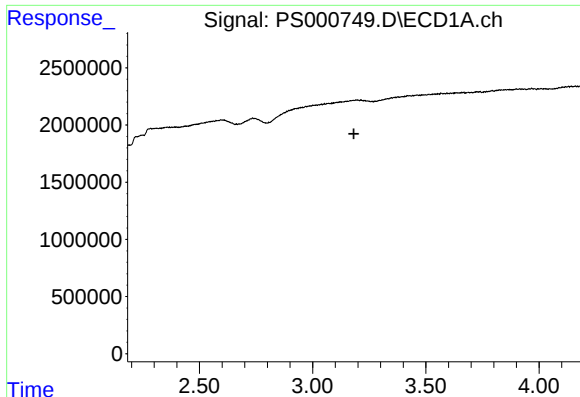

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

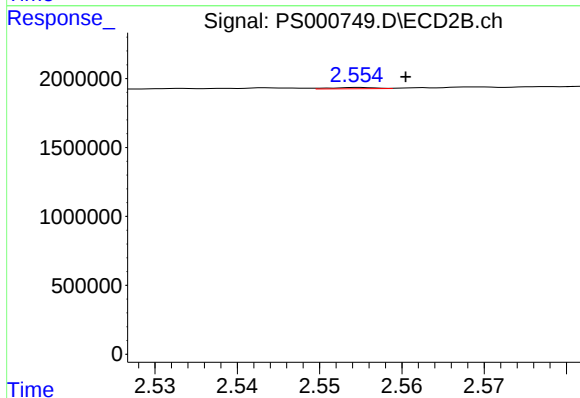


#1 Dalapon

R.T.: 2.555 min
Delta R.T.: -0.006 min
Response: 36712
Conc: 0.08 ng/ml

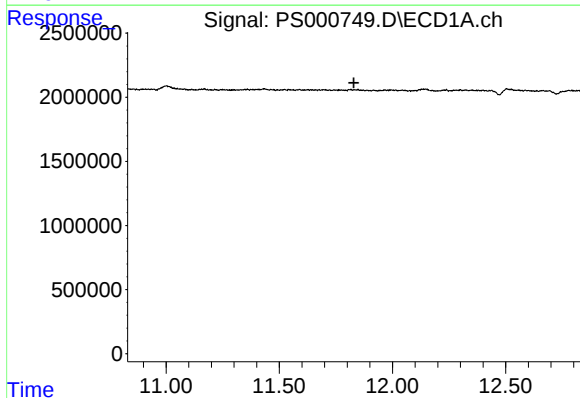


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.829 min
Response: 0
Conc: N.D.

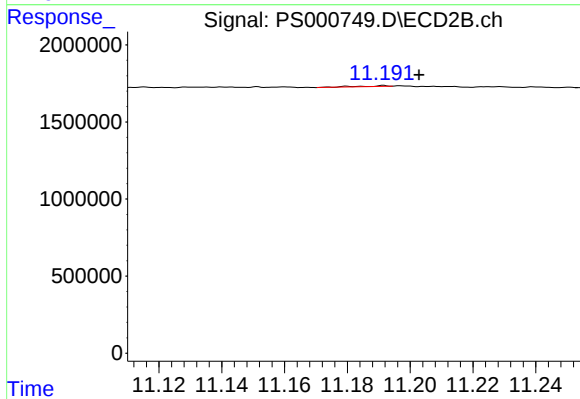

#4 2,4-DCAA


R.T.: 11.192 min
Delta R.T.: -0.011 min
Response: 32923
Conc: 0.10 ng/ml

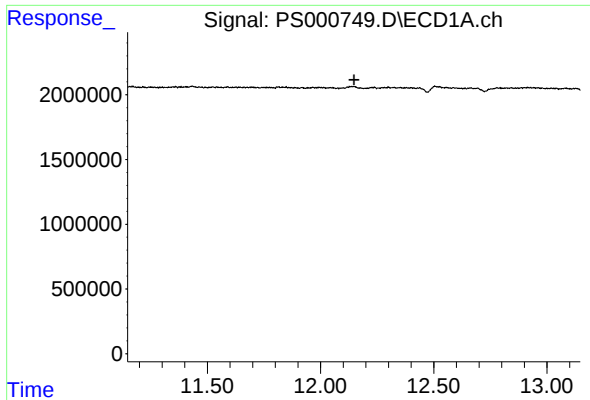

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

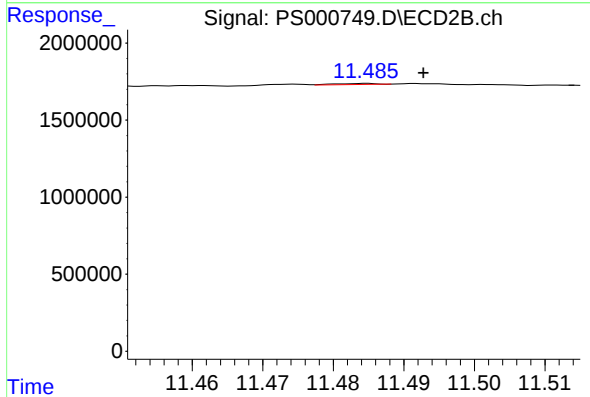


#5 DICAMBA

R.T.: 11.485 min
Delta R.T.: -0.008 min
Response: 29759
Conc: 0.02 ng/ml

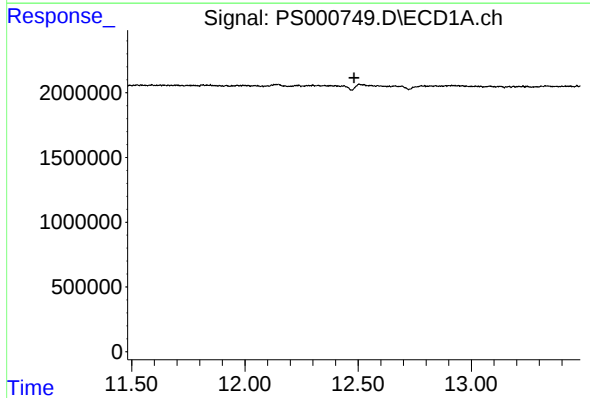


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.482 min
Response: 0
Conc: N.D.

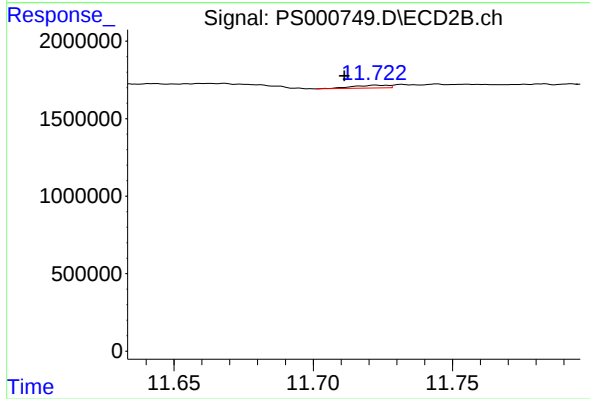

#6 MCPP


R.T.: 11.722 min
Delta R.T.: 0.011 min
Response: 164062
Conc: 0.17 ug/ml

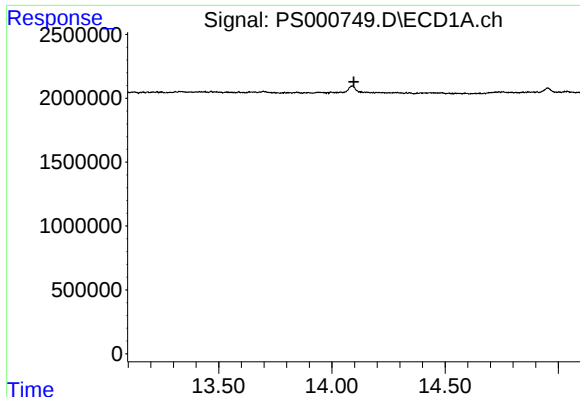

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 14.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

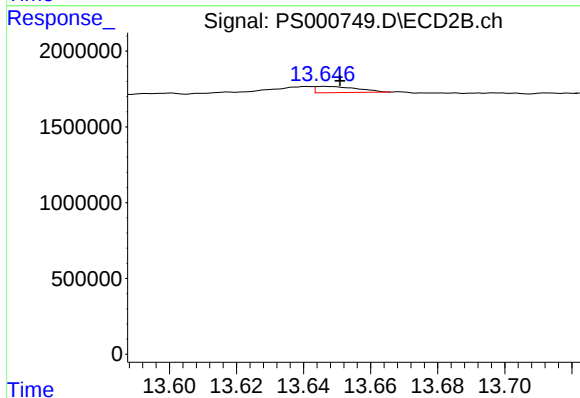


#10 Pentachlorophenol

R.T.: 13.646 min
Delta R.T.: -0.005 min
Response: 352122
Conc: 0.07 ng/ml

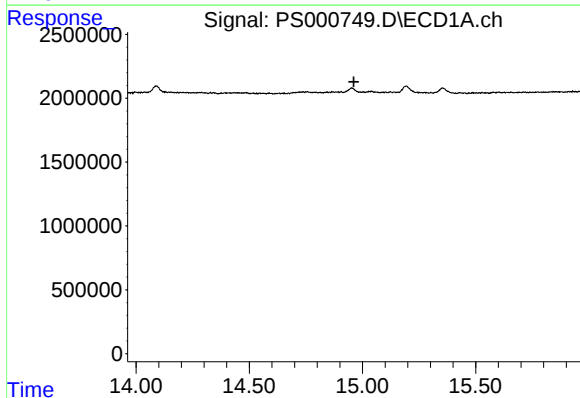


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.962 min
Response: 0
Conc: N.D.

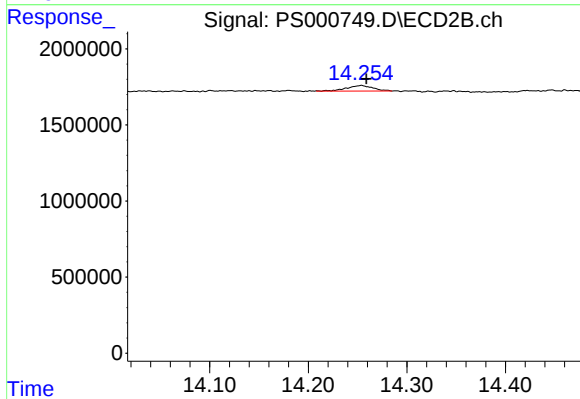

#11 2,4,5-TP (SILVEX)


R.T.: 14.254 min
Delta R.T.: -0.005 min
Response: 678200
Conc: 0.35 ng/ml

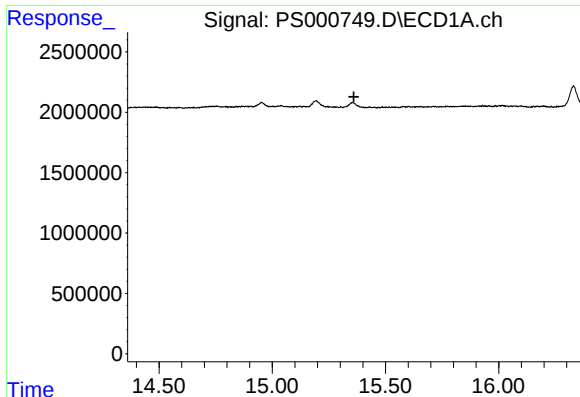

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.360 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

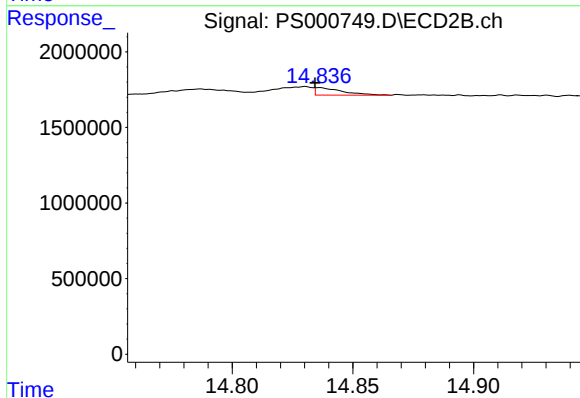


#12 2,4,5-T

R.T.: 14.836 min
Delta R.T.: 0.002 min
Response: 388071
Conc: 0.23 ng/ml

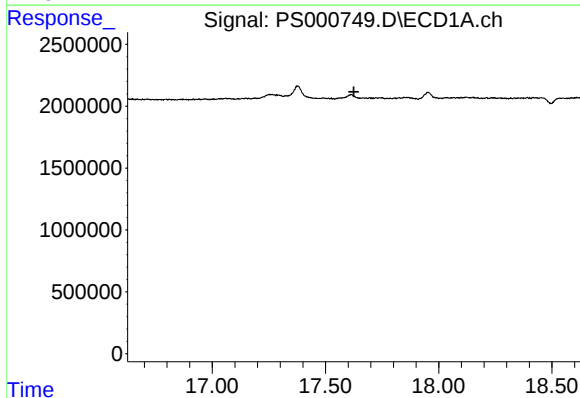


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.625 min
Response: 0
Conc: N.D.

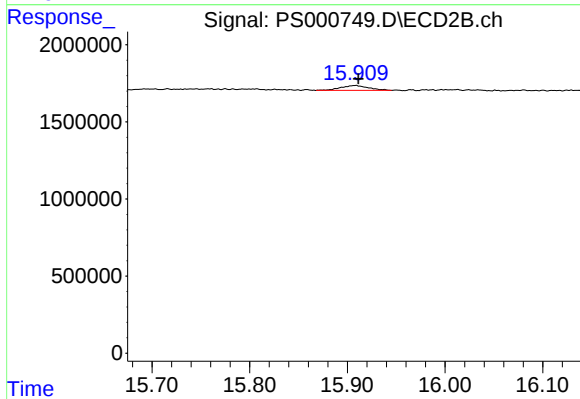

#14 DINOSEB


R.T.: 15.909 min
Delta R.T.: -0.002 min
Response: 633350
Conc: 0.49 ng/ml

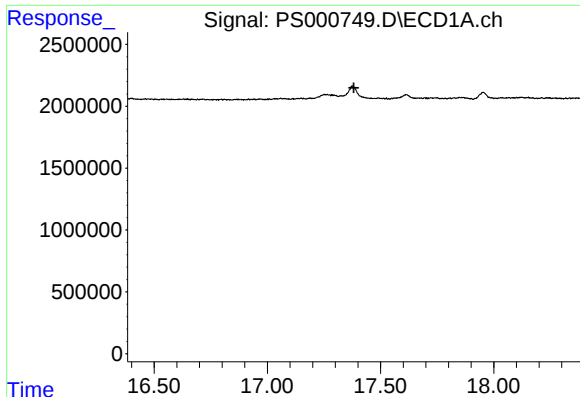

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

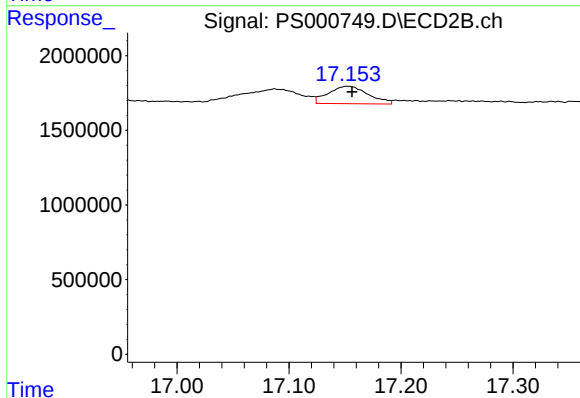


#15 Picloram

R.T.: 17.152 min
Delta R.T.: -0.004 min
Response: 2886221
Conc: 1.16 ng/ml

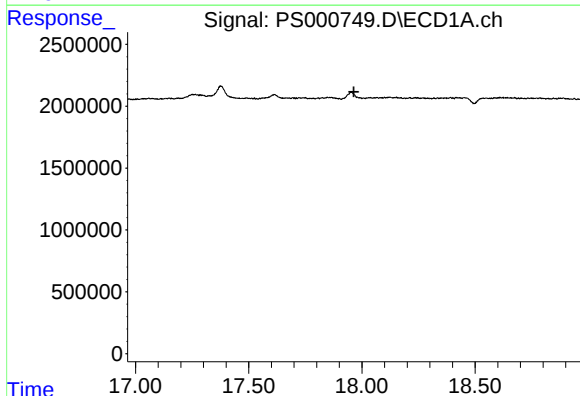

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.964 min
Response: 0
Conc: N.D.

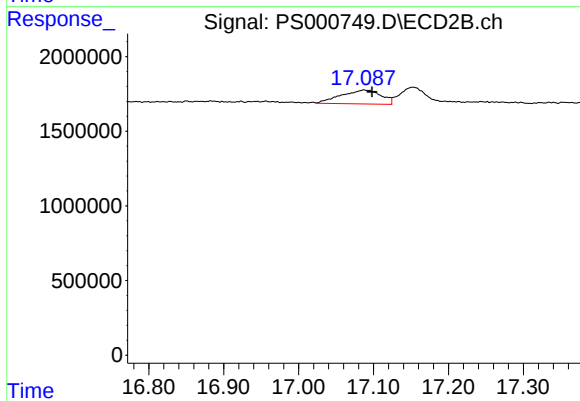

#16 DCPA

R.T.: 17.087 min
Delta R.T.: -0.011 min
Response: 3447714
Conc: 1.50 ng/ml