

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
 Data File : PS000750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 09:32
 Operator : UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:53:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.813	11.196	184.9E6	156.8E6	490.933	460.819
Target Compounds							
1) T	Dalapon	3.181	0.000	13819144	0	27.019	N.D. #
6) T	MCP	0.000	11.737	0	72217	N.D.	0.075 #
10) T	Pentachlo...	0.000	13.643	0	31043	N.D.	0.007 #
15) T	Picloram	0.000	17.164	0	708501	N.D.	0.284 #
16) T	DCPA	0.000	17.164	0	708501	N.D.	0.307 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
Data File : PS000750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 09:32
Operator : UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:53:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

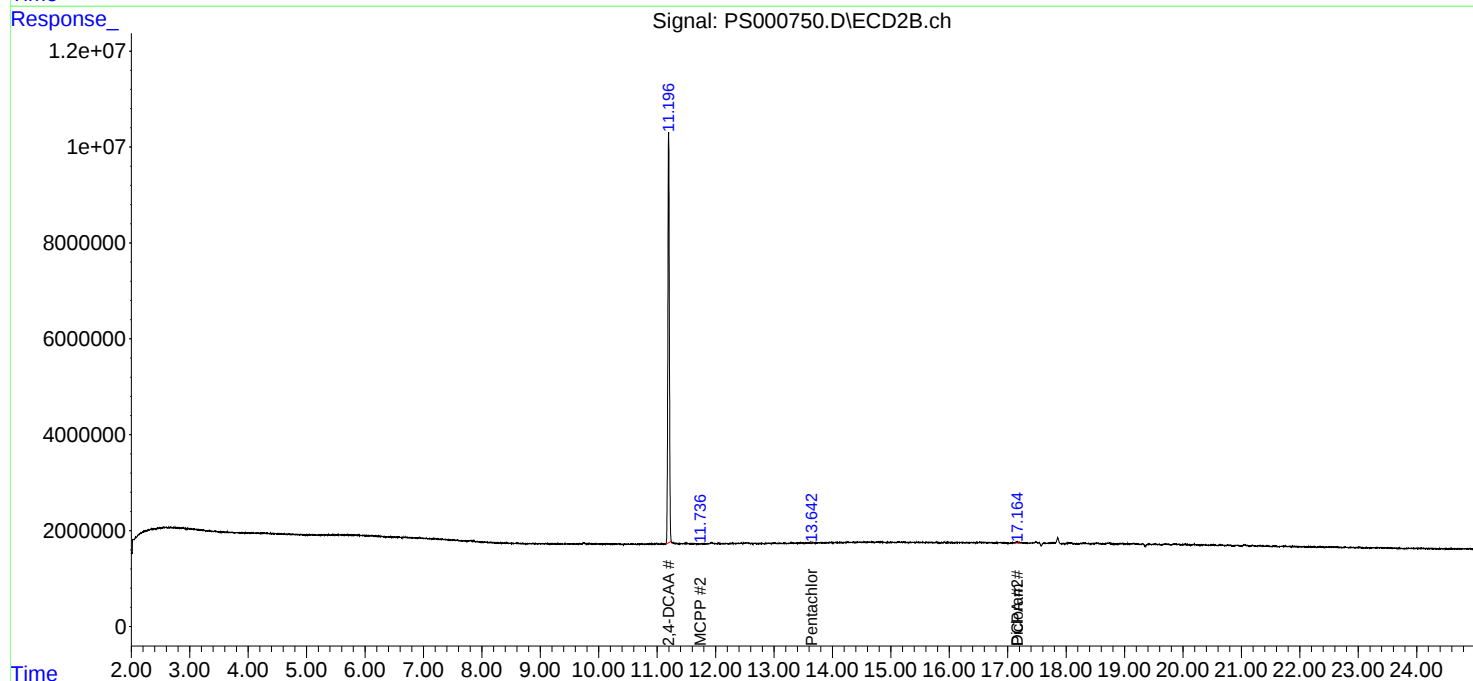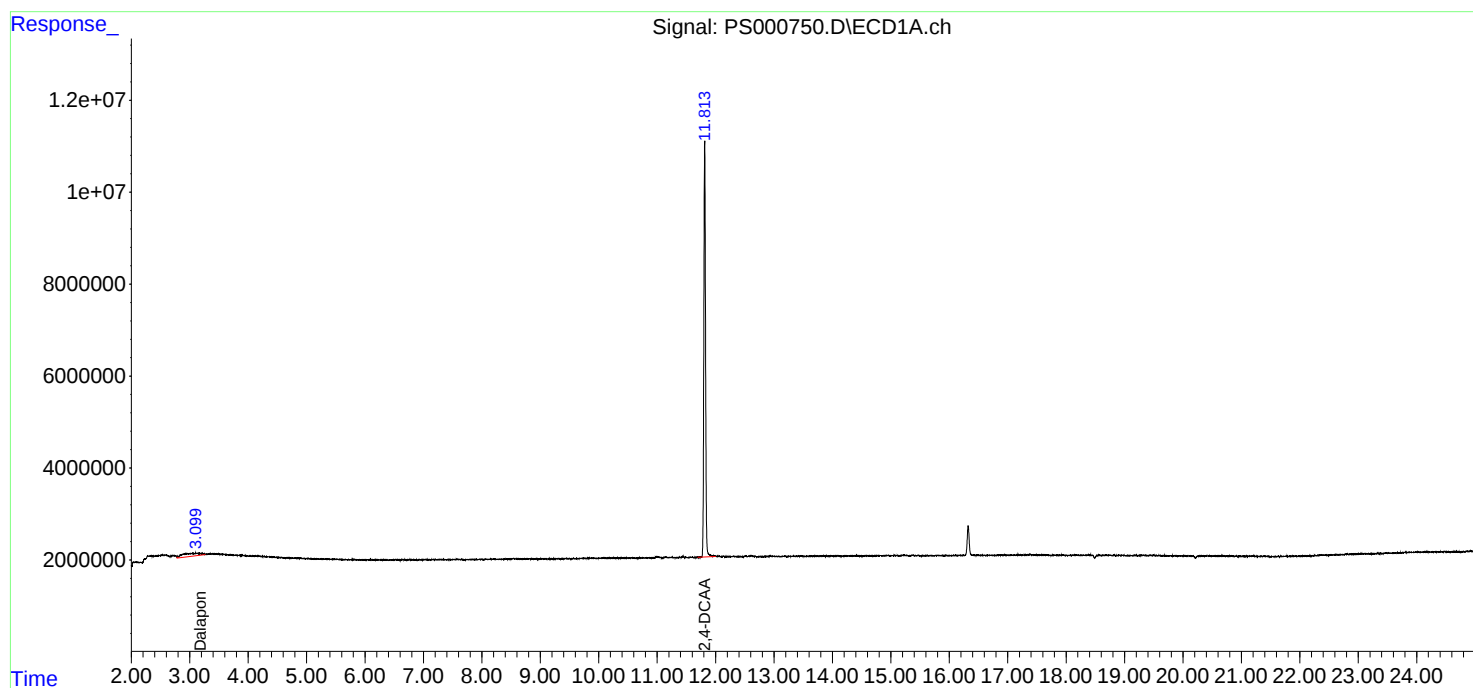


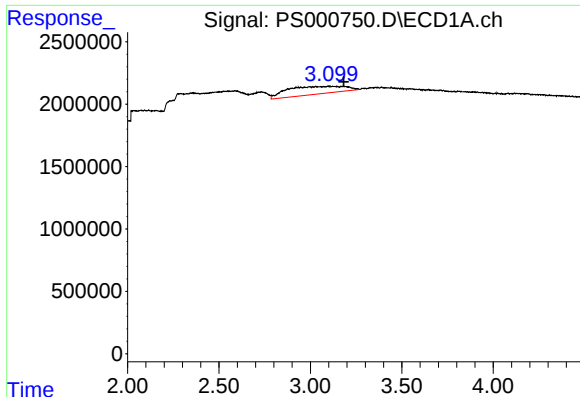

#1 Dalapon


R.T.: 3.181 min
Delta R.T.: -0.001 min
Response: 13819144
Conc: 27.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

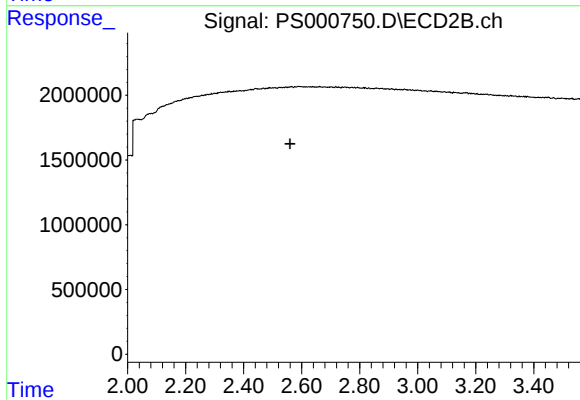


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.560 min
Response: 0
Conc: N.D.

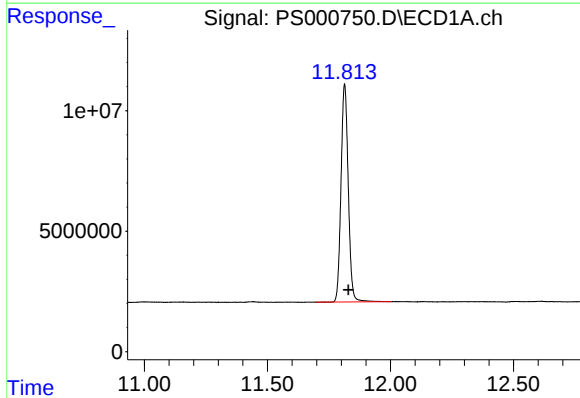


#4 2,4-DCAA

R.T.: 11.813 min
Delta R.T.: -0.016 min
Response: 184912130
Conc: 490.93 ng/ml

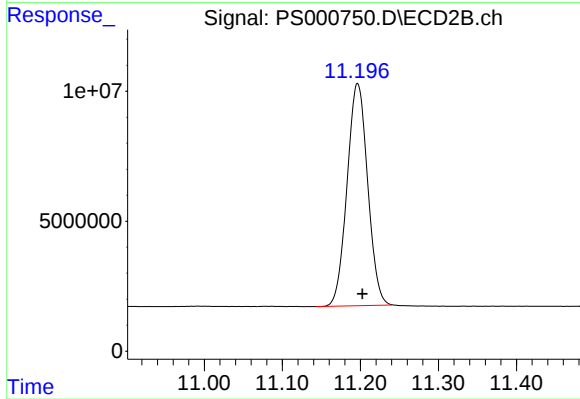

#4 2,4-DCAA


R.T.: 11.196 min
Delta R.T.: -0.007 min
Response: 156820991
Conc: 460.82 ng/ml

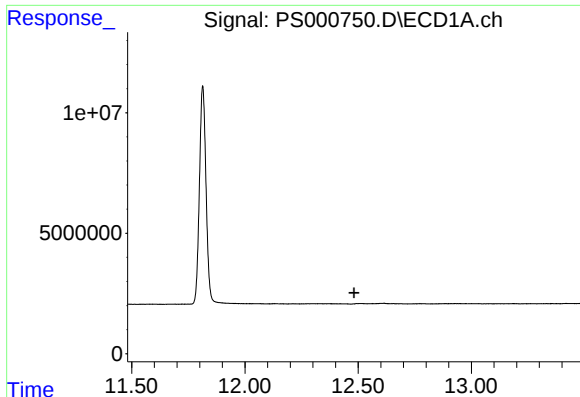

#6 MCP


R.T.: 0.000 min
Exp R.T.: 12.482 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

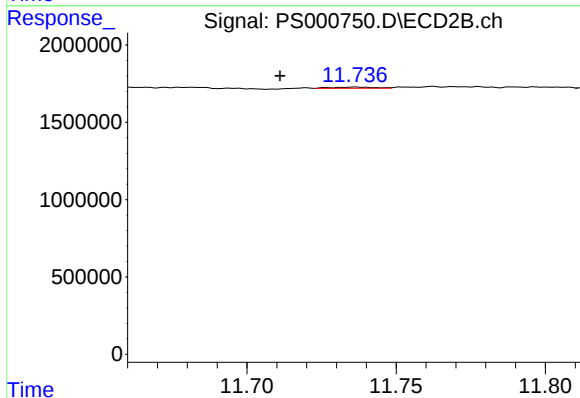


#6 MCP

R.T.: 11.737 min
Delta R.T.: 0.025 min
Response: 72217
Conc: 0.08 ug/ml

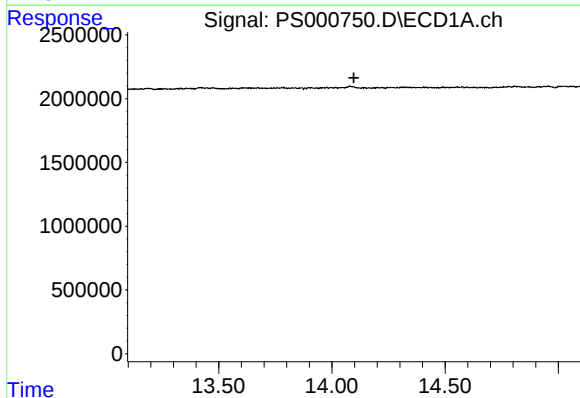


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 14.097 min
Response: 0
Conc: N.D.

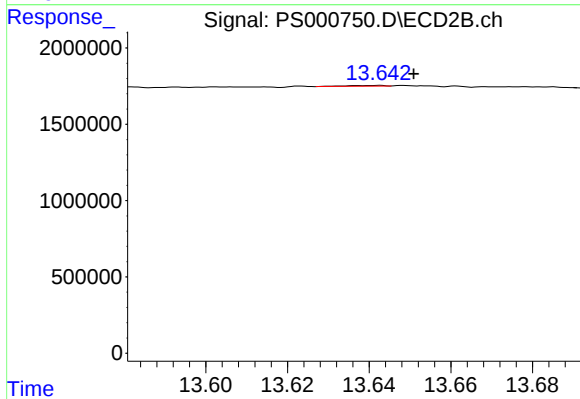

#10 Pentachlorophenol


R.T.: 13.643 min
Delta R.T.: -0.008 min
Response: 31043
Conc: 0.01 ng/ml

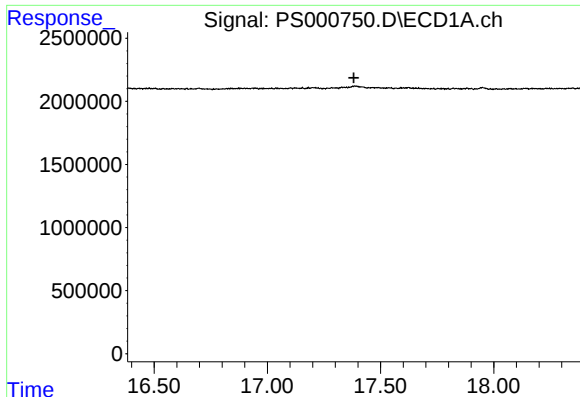

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

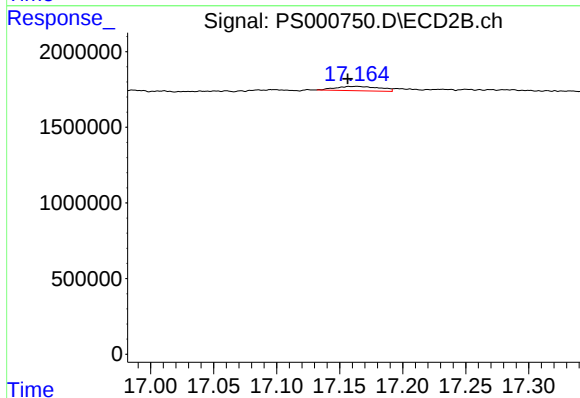


#15 Picloram

R.T.: 17.164 min
Delta R.T.: 0.008 min
Response: 708501
Conc: 0.28 ng/ml

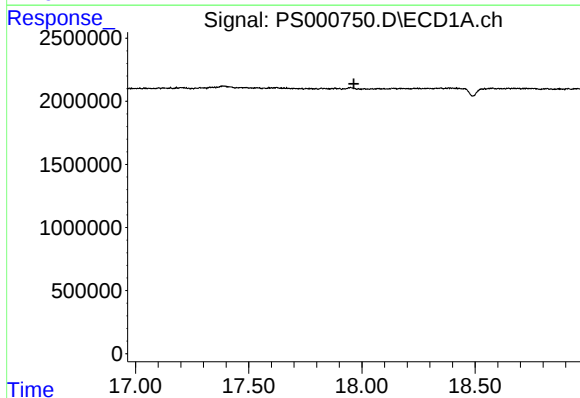

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.964 min
Response: 0
Conc: N.D.

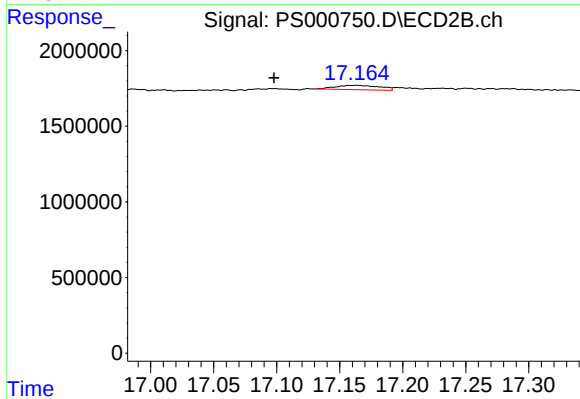

#16 DCPA

R.T.: 17.164 min
Delta R.T.: 0.066 min
Response: 708501
Conc: 0.31 ng/ml