

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
 Data File : PS000760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 16:27
 Operator : UA
 Sample : J3243-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 22:56:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.799	11.183	152.6E6	122.7E6	405.095	360.589
Target Compounds							
1) T	Dalapon	0.000	2.494	0	1026532	N.D.	2.355 #
2) T	3,5-DICHL...	0.000	9.330	0	1088705	N.D.	2.367 #
3) T	4-Nitroph...	11.457	10.341	3209317	4309350	13.653	21.991 #
5) T	DICAMBA	0.000	11.497	0	296161	N.D.	0.239 #
6) T	MCP	12.495	11.695	11533716	282178	10.185	0.294 #
8) T	DICHLORPROP	0.000	12.626	0	78768	N.D.	0.245 #
11) T	2,4,5-TP ...	0.000	14.266	0	2446782	N.D.	1.257 #
12) T	2,4,5-T	0.000	14.827	0	853647	N.D.	0.505 #
13) T	2,4-DB	0.000	15.449	0	55724	N.D.	0.225 #
14) T	DINOSEB	0.000	15.917	0	1220069	N.D.	0.935 #
15) T	Picloram	0.000	17.166	0	636712	N.D.	0.255 #
16) T	DCPA	0.000	17.103	0	730677	N.D.	0.317 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
Data File : PS000760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 16:27
Operator : UA
Sample : J3243-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 22:56:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

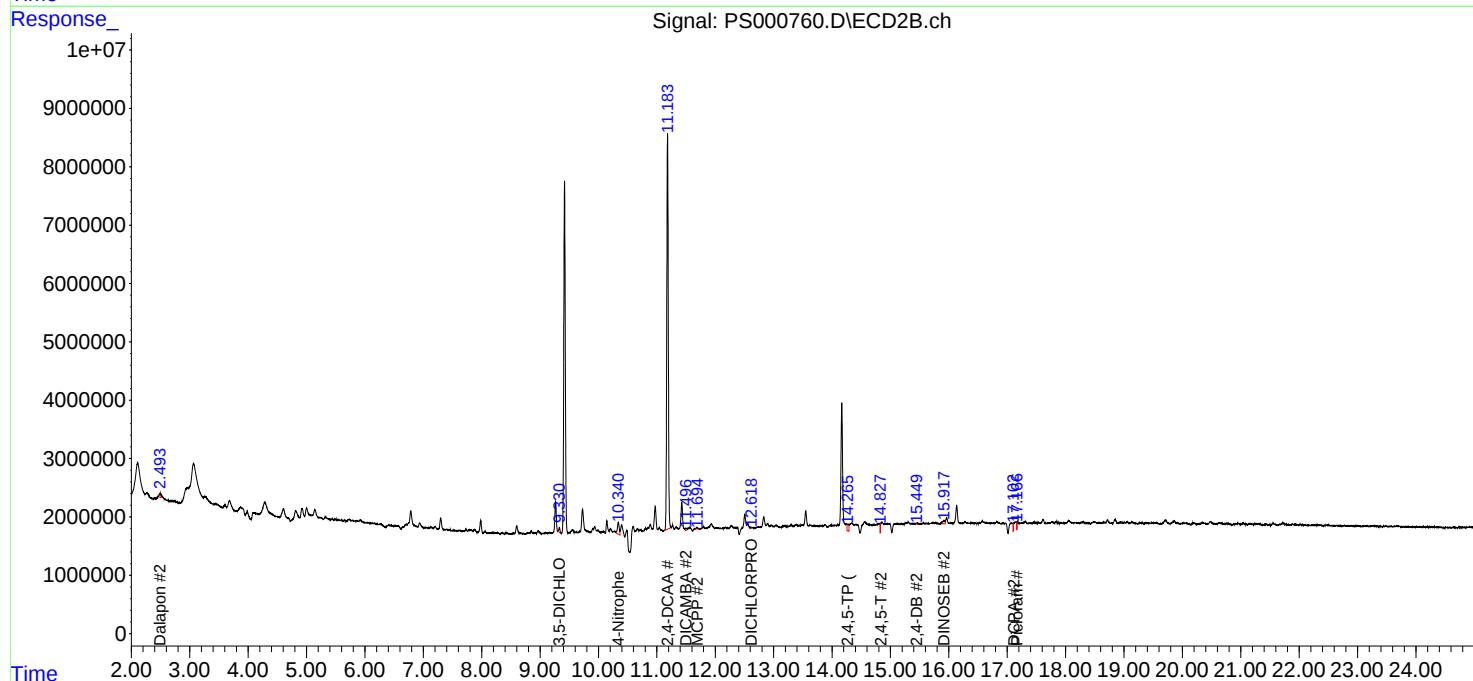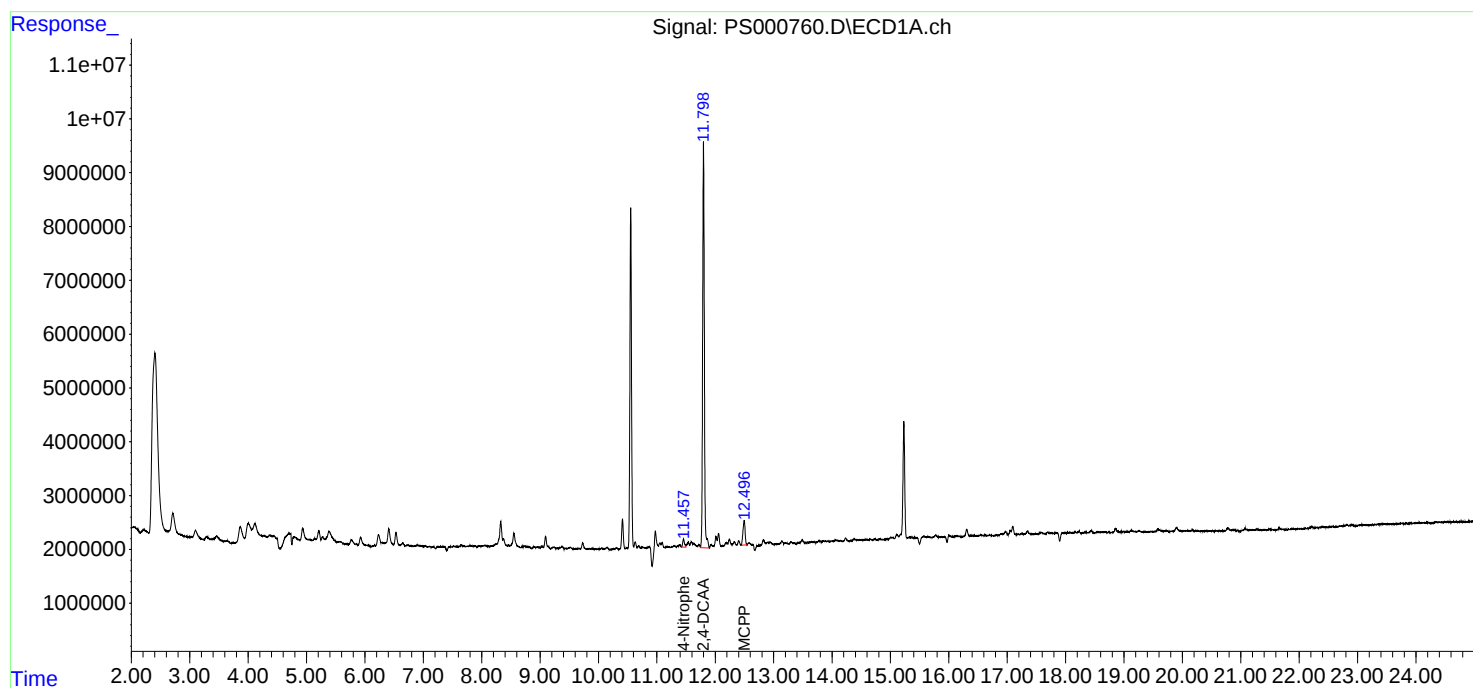


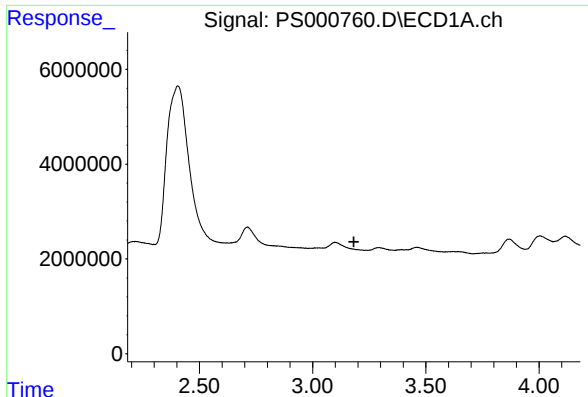

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

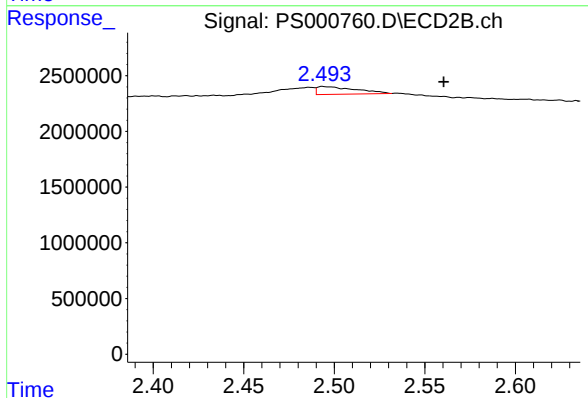


#1 Dalapon

R.T.: 2.494 min
Delta R.T.: -0.067 min
Response: 1026532
Conc: 2.35 ng/ml

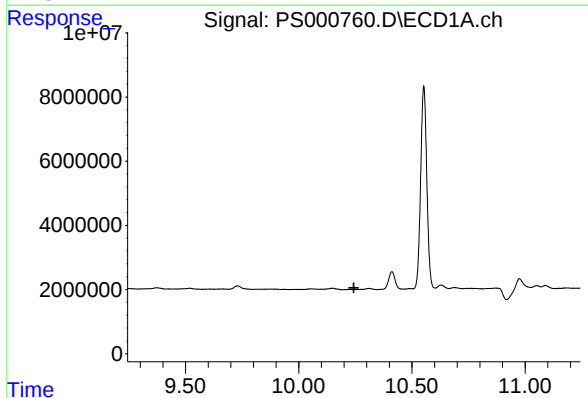


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.244 min
Response: 0
Conc: N.D.

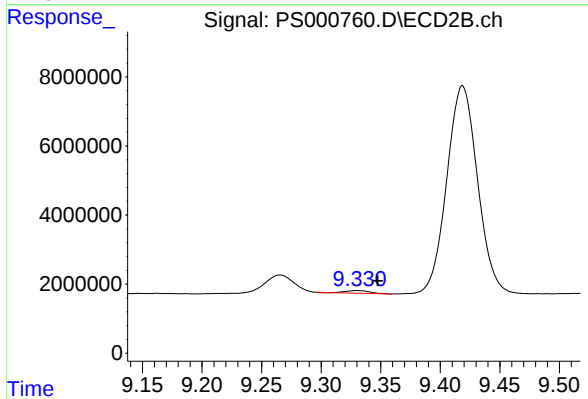

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.330 min
Delta R.T.: -0.017 min
Response: 1088705
Conc: 2.37 ng/ml

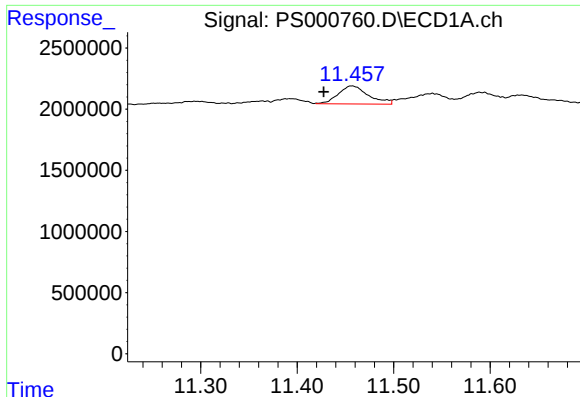

#3 4-Nitrophenol


R.T.: 11.457 min
Delta R.T.: 0.029 min
Response: 3209317
Conc: 13.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

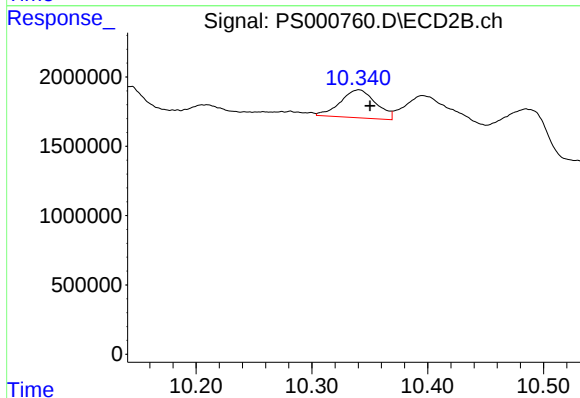


#3 4-Nitrophenol

R.T.: 10.341 min
Delta R.T.: -0.010 min
Response: 4309350
Conc: 21.99 ng/ml

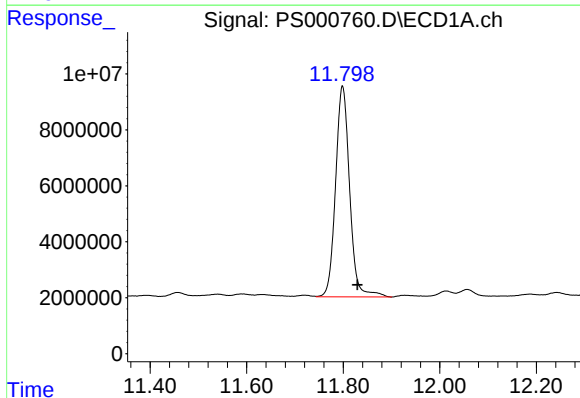


#4 2,4-DCAA

R.T.: 11.799 min
Delta R.T.: -0.031 min
Response: 152580855
Conc: 405.09 ng/ml

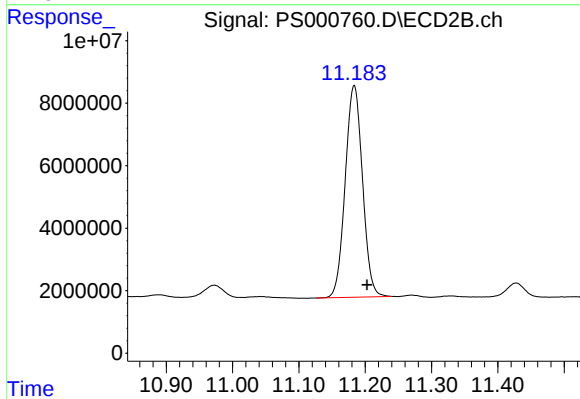

#4 2,4-DCAA


R.T.: 11.183 min
Delta R.T.: -0.019 min
Response: 122711629
Conc: 360.59 ng/ml

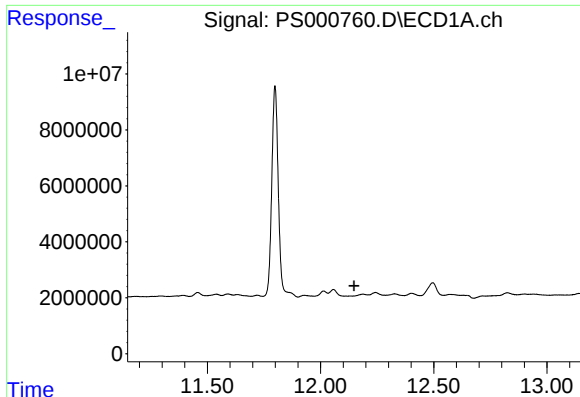

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

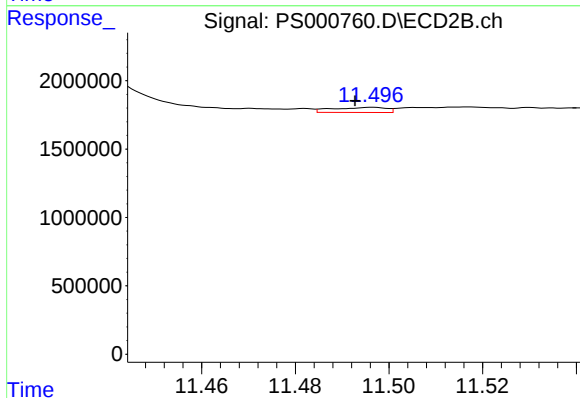


#5 DICAMBA

R.T.: 11.497 min
Delta R.T.: 0.004 min
Response: 296161
Conc: 0.24 ng/ml

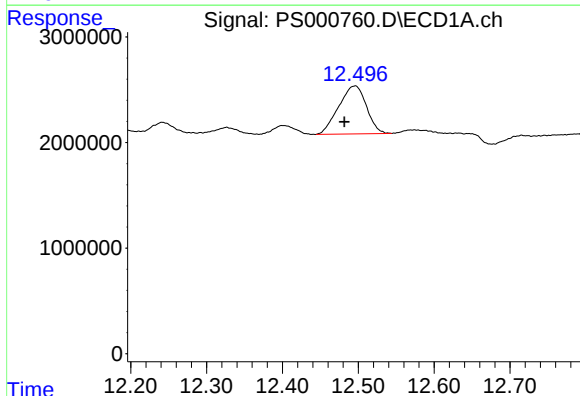


#6 MCP

R.T.: 12.495 min
Delta R.T.: 0.013 min
Response: 11533716
Conc: 10.19 ug/ml

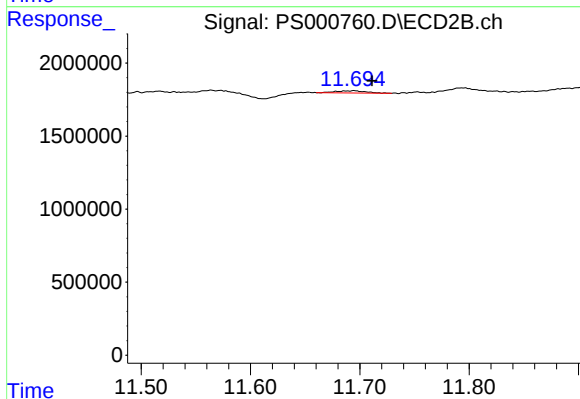

#6 MCP


R.T.: 11.695 min
Delta R.T.: -0.017 min
Response: 282178
Conc: 0.29 ug/ml

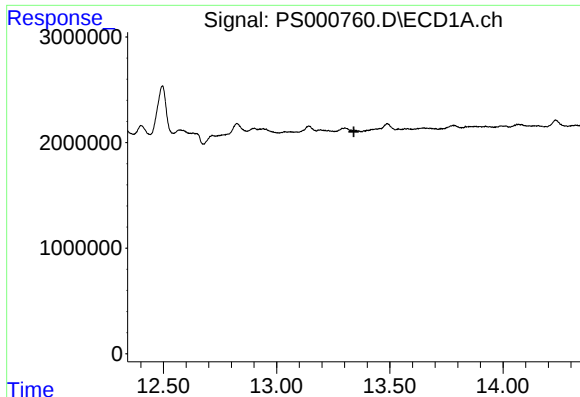

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

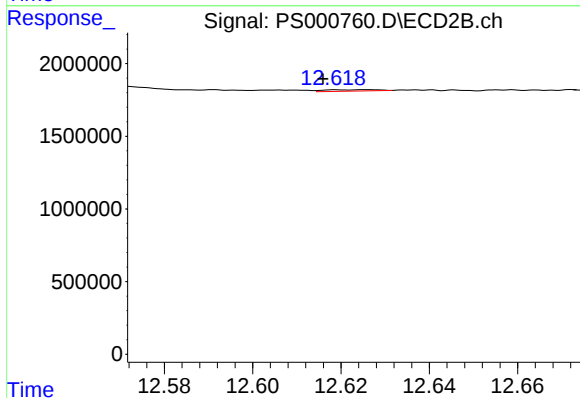


#8 DICHLORPROP

R.T.: 12.626 min
Delta R.T.: 0.010 min
Response: 78768
Conc: 0.24 ng/ml

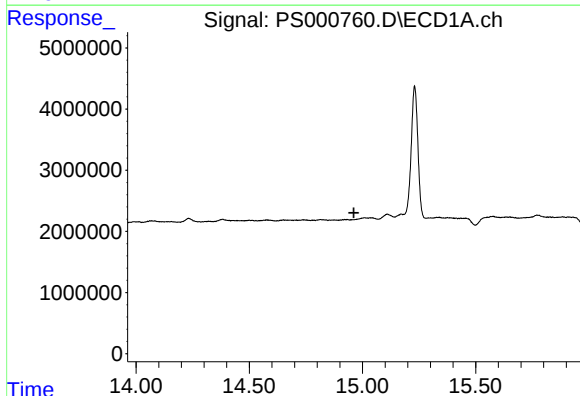


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.962 min
Response: 0
Conc: N.D.

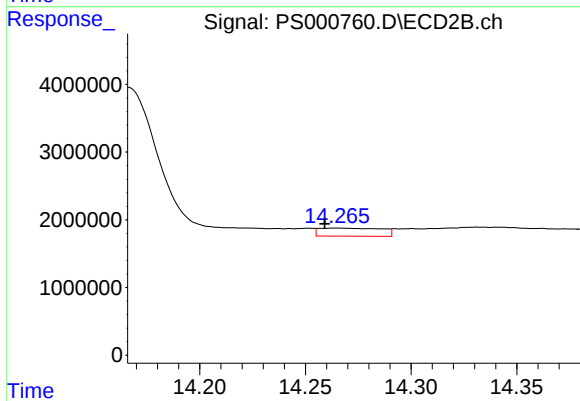

#11 2,4,5-TP (SILVEX)


R.T.: 14.266 min
Delta R.T.: 0.006 min
Response: 2446782
Conc: 1.26 ng/ml

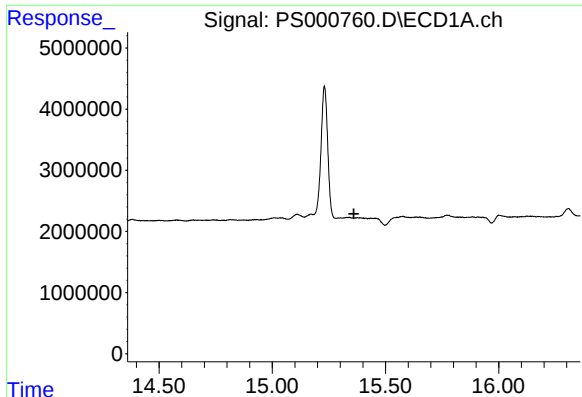

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.360 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

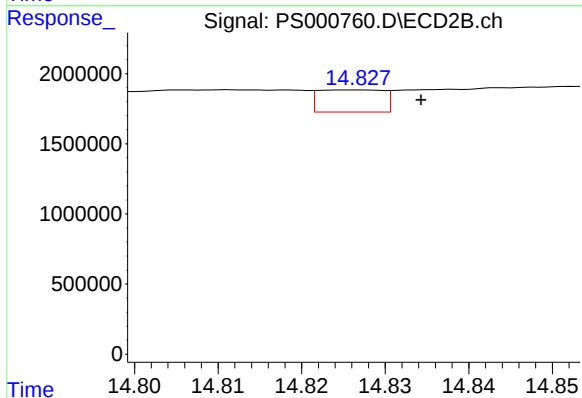


#12 2,4,5-T

R.T.: 14.827 min
Delta R.T.: -0.007 min
Response: 853647
Conc: 0.50 ng/ml

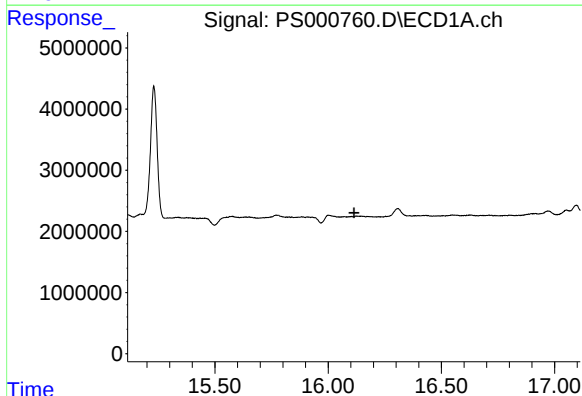


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 16.114 min
Response: 0
Conc: N.D.

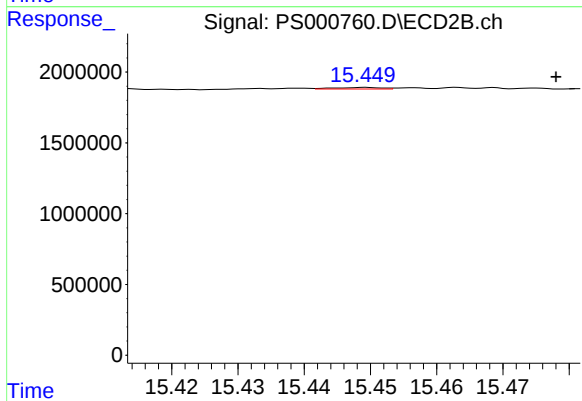

#13 2,4-DB


R.T.: 15.449 min
Delta R.T.: -0.029 min
Response: 55724
Conc: 0.23 ng/ml

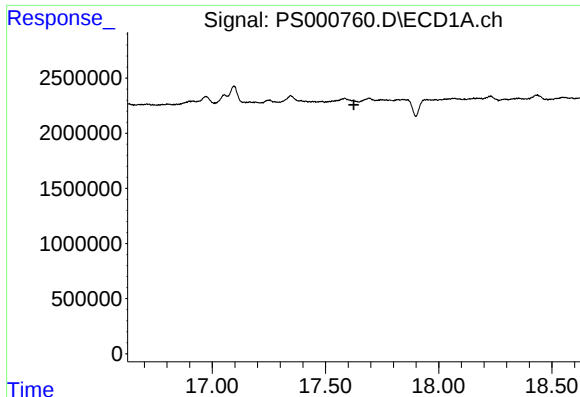

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.625 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

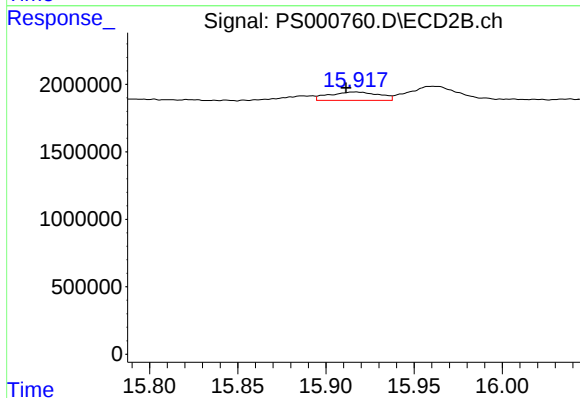


#14 DINOSEB

R.T.: 15.917 min
Delta R.T.: 0.006 min
Response: 1220069
Conc: 0.94 ng/ml

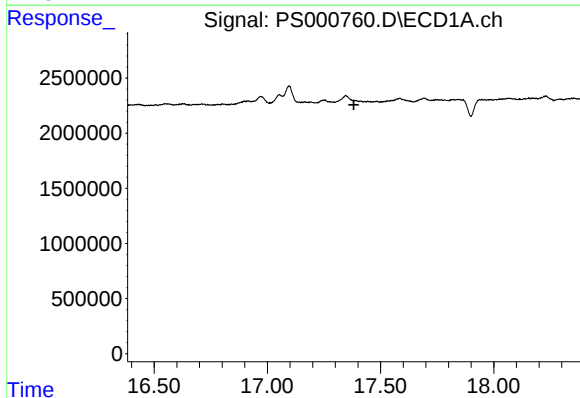


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

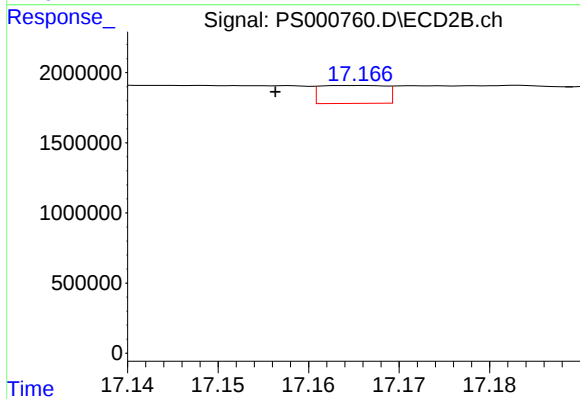

#15 Picloram


R.T.: 17.166 min
Delta R.T.: 0.010 min
Response: 636712
Conc: 0.26 ng/ml

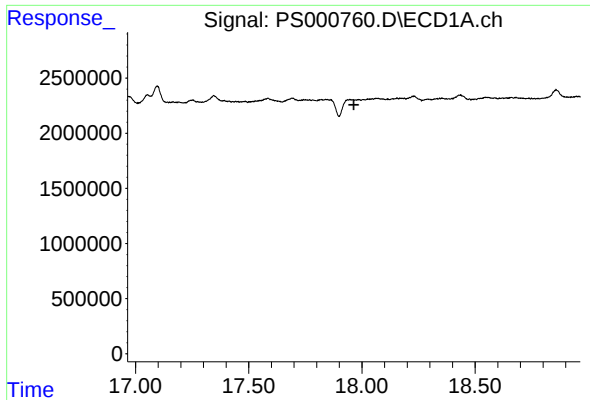

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.964 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

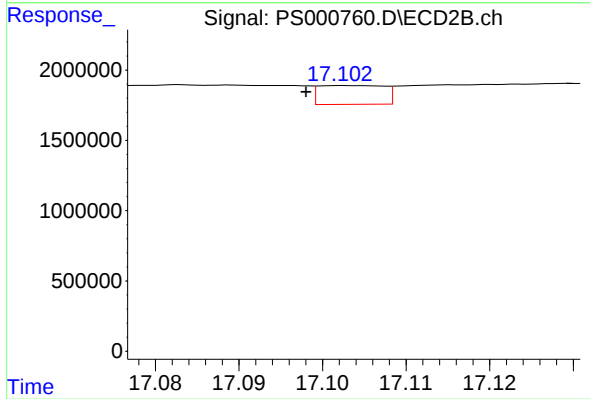

#16 DCPA

R.T.: 17.103 min
Delta R.T.: 0.005 min
Response: 730677
Conc: 0.32 ng/ml