

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS070318\  
 Data File : PS000762.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 03 Jul 2018 17:29  
 Operator : UA  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 03 22:57:43 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS061718.M  
 Quant Title : 8080.M  
 QLast Update : Mon Jun 18 00:27:44 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|--------|--------|---------|---------|---------|---------|
| -----                       |          |        |        |         |         |         |         |
| System Monitoring Compounds |          |        |        |         |         |         |         |
| 4) S                        | 2,4-DCAA | 11.822 | 11.208 | 188.2E6 | 152.1E6 | 499.771 | 447.069 |
| Target Compounds            |          |        |        |         |         |         |         |
| 1) T                        | Dalapon  | 0.000  | 2.557  | 0       | 303951  | N.D.    | 0.697 # |
| 15) T                       | Picloram | 0.000  | 17.104 | 0       | 27177   | N.D.    | 0.011 # |
| 16) T                       | DCPA     | 0.000  | 17.104 | 0       | 27177   | N.D.    | 0.012 # |
| -----                       |          |        |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS070318\  
Data File : PS000762.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 03 Jul 2018 17:29  
Operator : UA  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 03 22:57:43 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS061718.M  
Quant Title : 8080.M  
QLast Update : Mon Jun 18 00:27:44 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

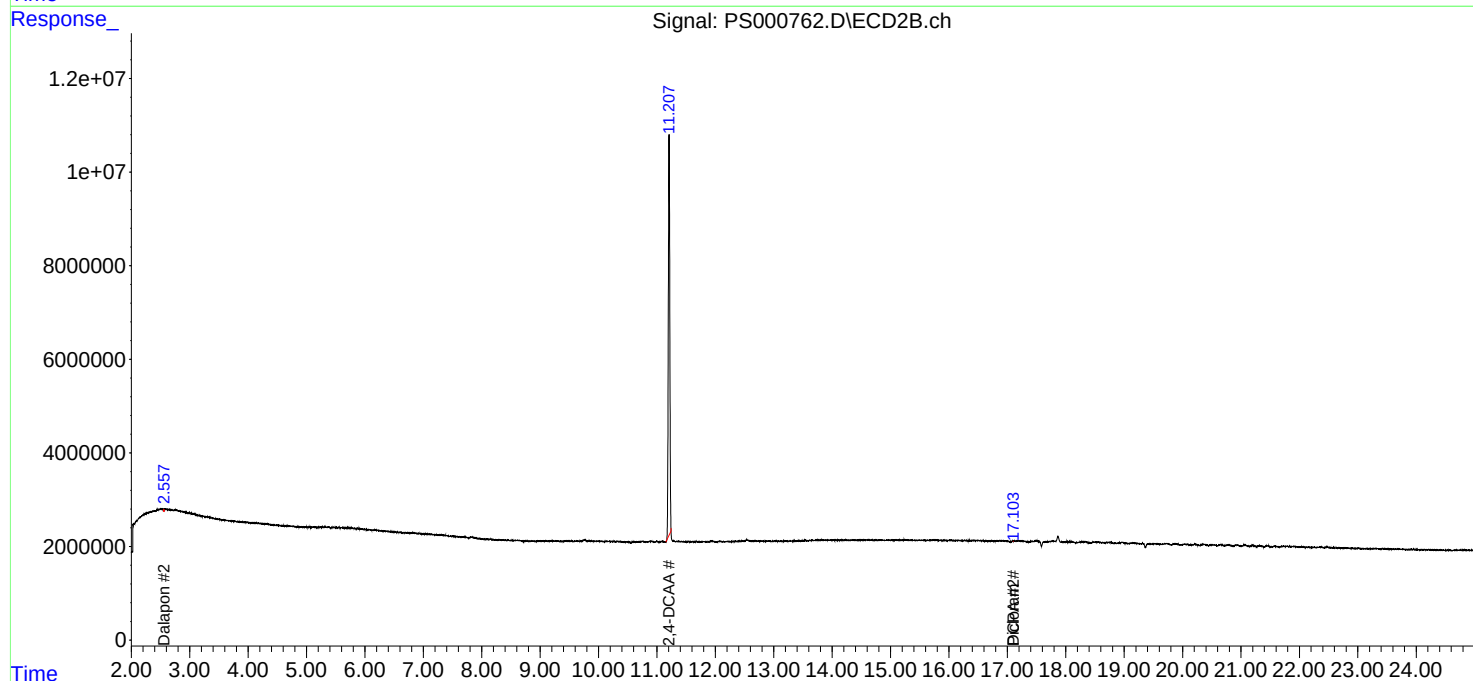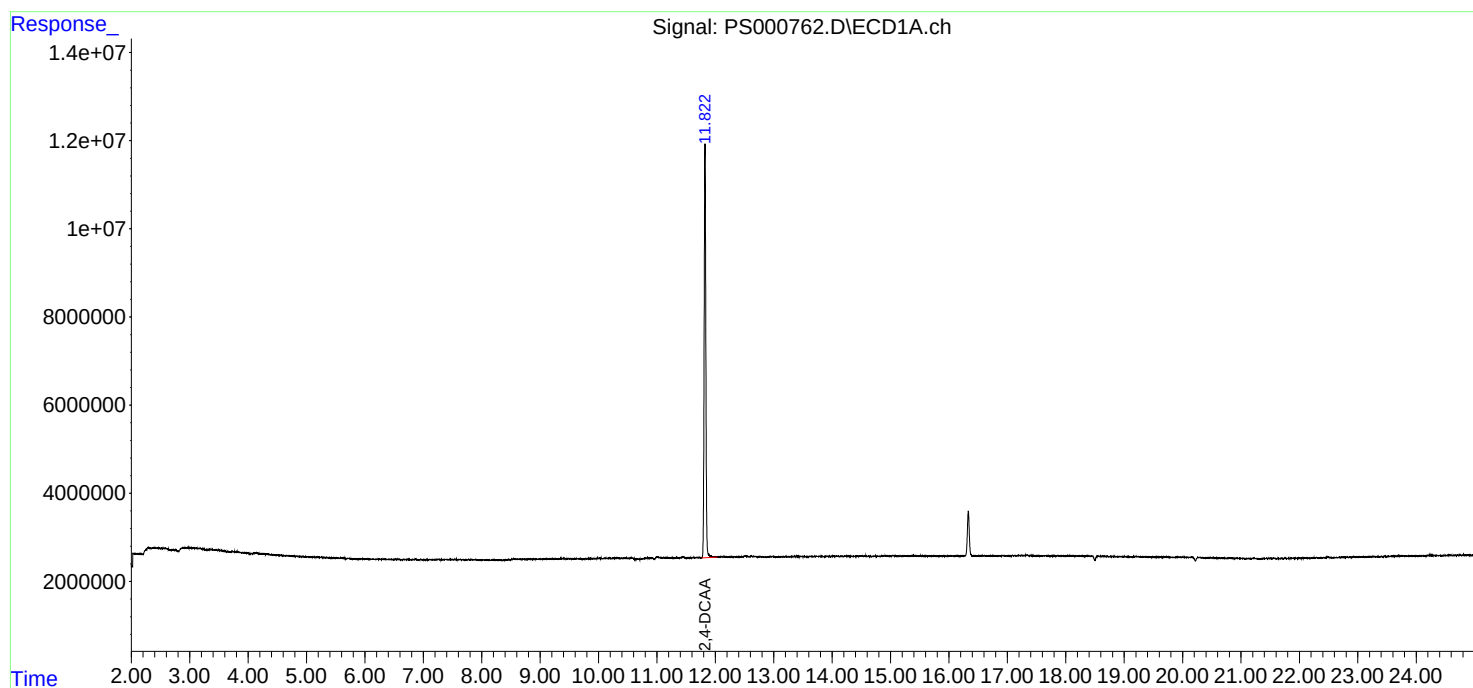


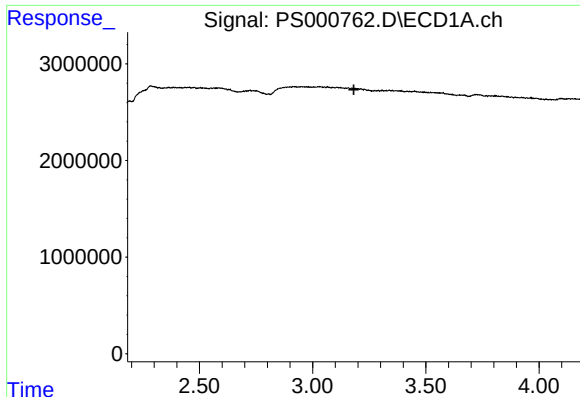

#1 Dalapon


R.T.: 0.000 min  
Exp R.T.: 3.182 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

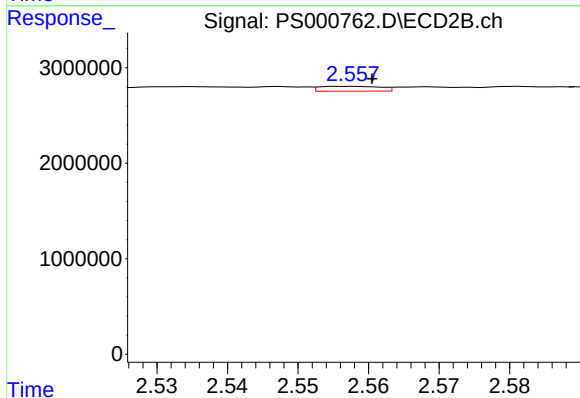


#1 Dalapon

R.T.: 2.557 min  
Delta R.T.: -0.003 min  
Response: 303951  
Conc: 0.70 ng/ml

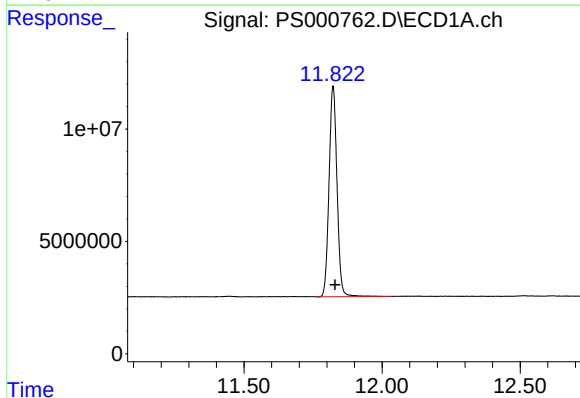


#4 2,4-DCAA

R.T.: 11.822 min  
Delta R.T.: -0.007 min  
Response: 188241115  
Conc: 499.77 ng/ml

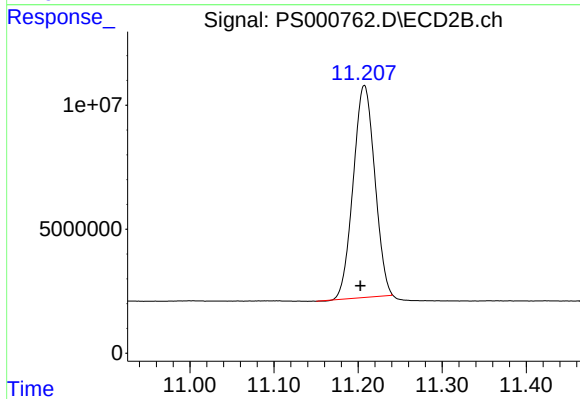

#4 2,4-DCAA


R.T.: 11.208 min  
Delta R.T.: 0.005 min  
Response: 152141671  
Conc: 447.07 ng/ml

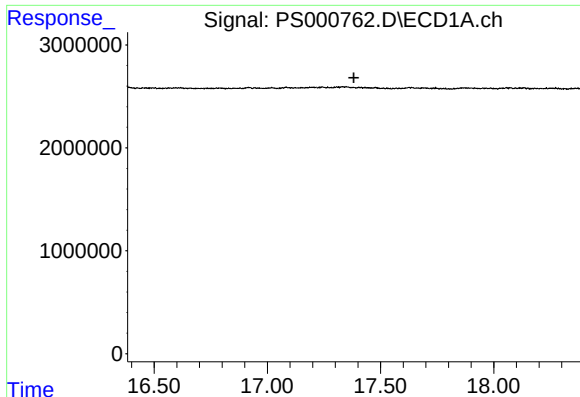

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 17.382 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

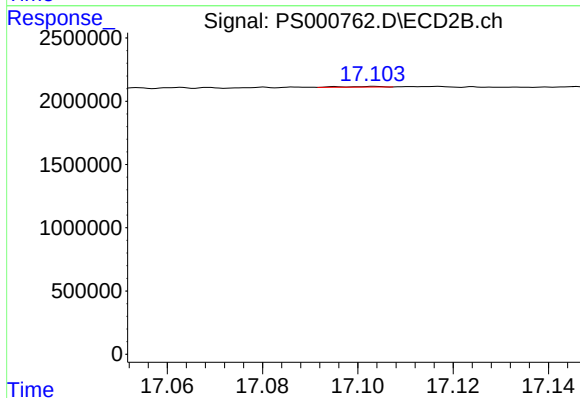


#15 Picloram

R.T.: 17.104 min  
Delta R.T.: -0.053 min  
Response: 27177  
Conc: 0.01 ng/ml

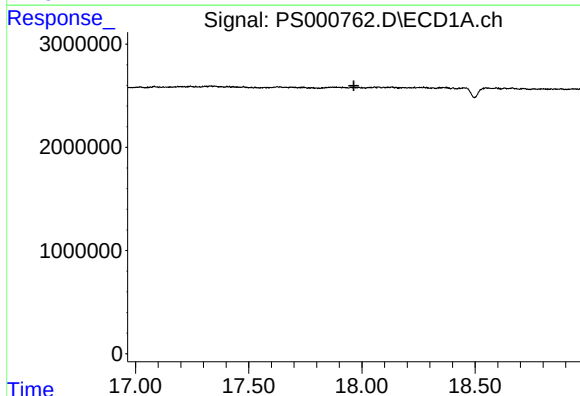

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 17.964 min  
Response: 0  
Conc: N.D.

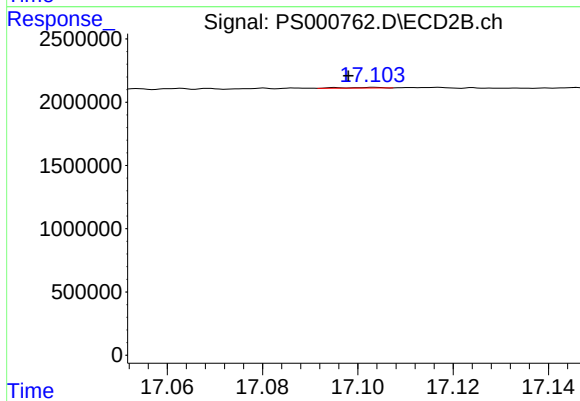

#16 DCPA

R.T.: 17.104 min  
Delta R.T.: 0.006 min  
Response: 27177  
Conc: 0.01 ng/ml