

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
 Data File : PS000770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2018 21:37
 Operator : UA
 Sample : J3840-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 23:00:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 18 00:27:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.814	11.200	120.5E6	95614897	319.961	280.965
Target Compounds							
1) T	Dalapon	0.000	2.528	0	33351	N.D.	0.077 #
2) T	3,5-DICHL...	0.000	9.348	0	758978	N.D.	1.650 #
3) T	4-Nitroph...	11.472	10.357	3203635	4819036	13.628	24.592 #
5) T	DICAMBA	0.000	11.532	0	97854	N.D.	0.079 #
6) T	MCP	12.510	11.709	11377934	212125	10.047	0.221 #
8) T	DICHLORPROP	0.000	12.618	0	984671	N.D.	3.058 #
9) T	2,4-D	0.000	13.061	0	358782	N.D.	0.844 #
11) T	2,4,5-TP ...	0.000	14.283	0	1541347	N.D.	0.792 #
12) T	2,4,5-T	0.000	14.826	0	1242851	N.D.	0.735 #
13) T	2,4-DB	0.000	15.480	0	238125	N.D.	0.962 #
14) T	DINOSEB	0.000	15.916	0	596192	N.D.	0.457 #
15) T	Picloram	0.000	17.161	0	1108774	N.D.	0.445 #
16) T	DCPA	17.959	17.116	5415536	6560586	2.113	2.845 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070318\
Data File : PS000770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2018 21:37
Operator : UA
Sample : J3840-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 23:00:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061718.M
Quant Title : 8080.M
QLast Update : Mon Jun 18 00:27:44 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

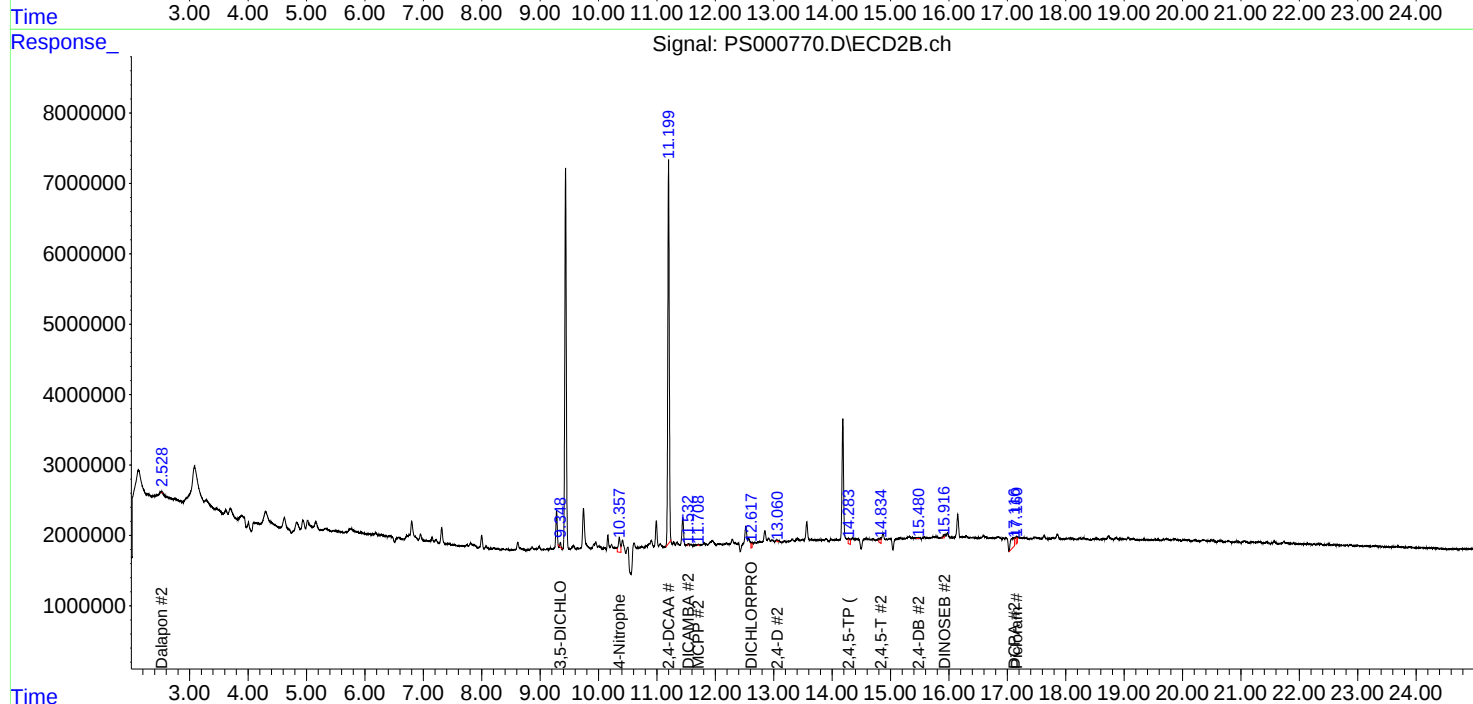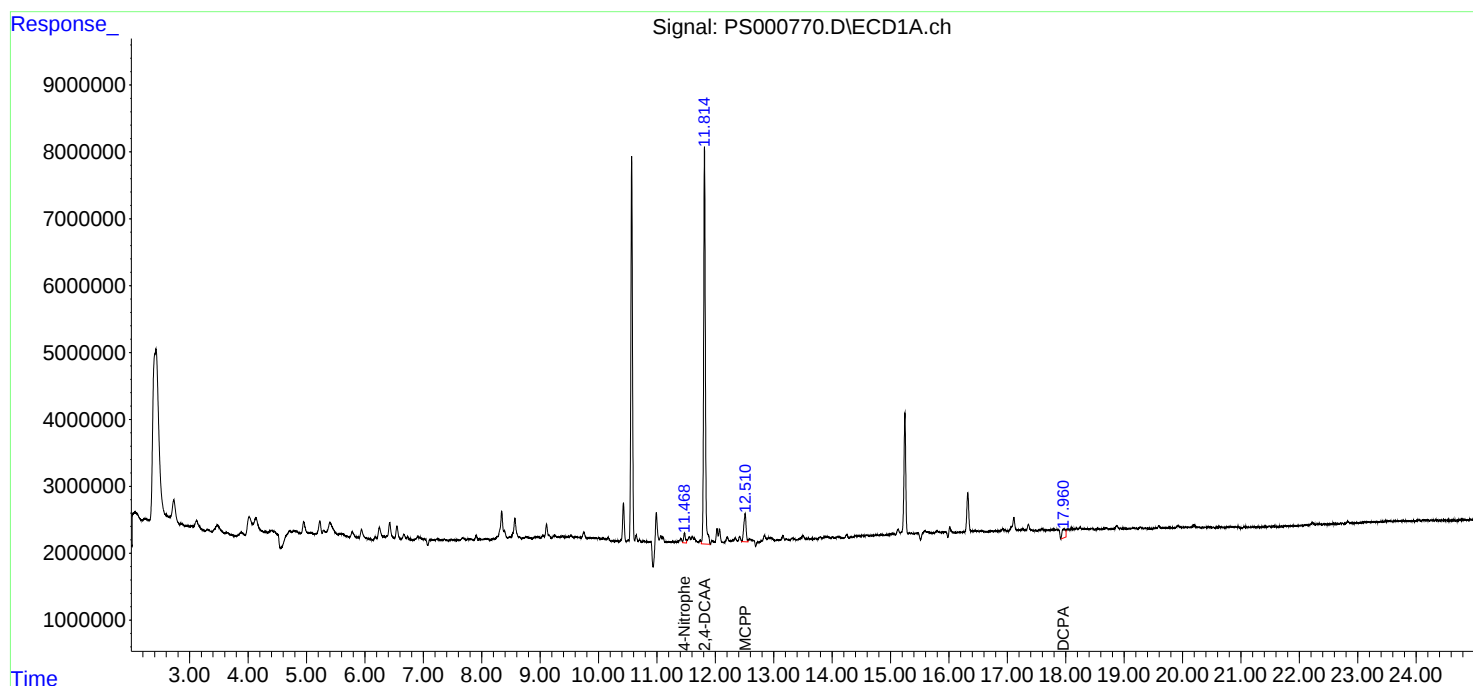


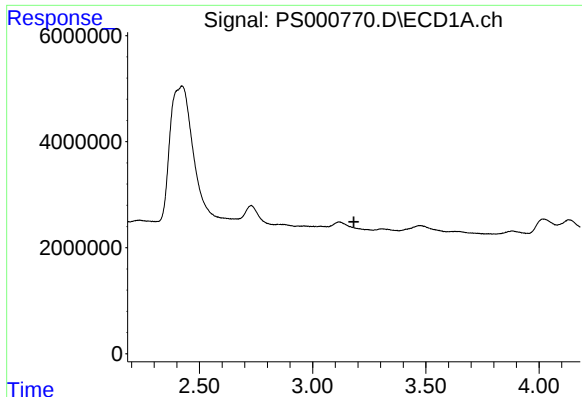

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

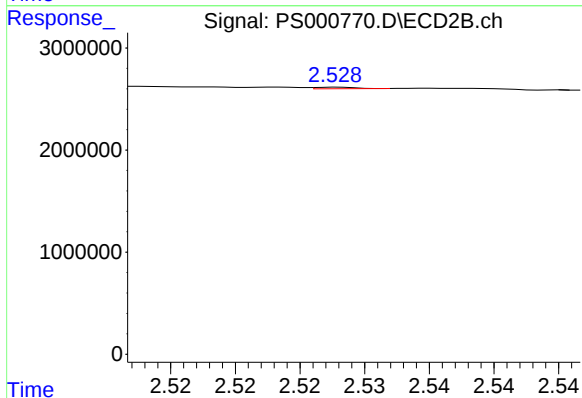


#1 Dalapon

R.T.: 2.528 min
Delta R.T.: -0.033 min
Response: 33351
Conc: 0.08 ng/ml

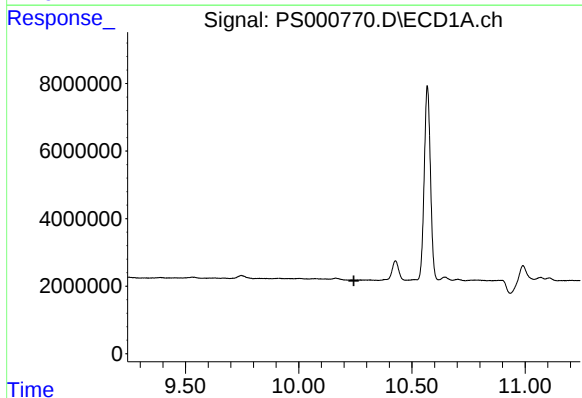


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.244 min
Response: 0
Conc: N.D.

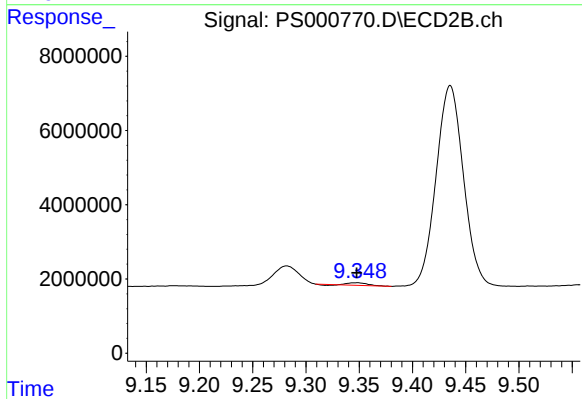

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.348 min
Delta R.T.: 0.000 min
Response: 758978
Conc: 1.65 ng/ml

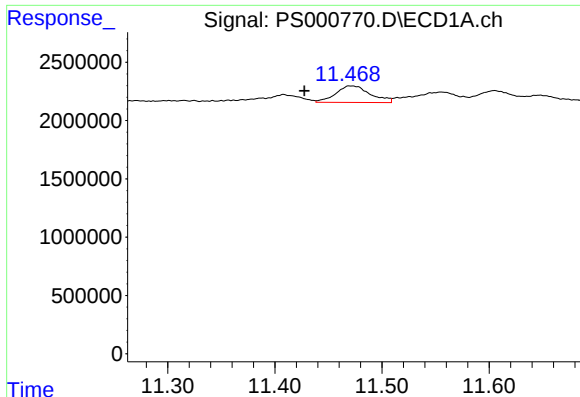

#3 4-Nitrophenol


R.T.: 11.472 min
Delta R.T.: 0.044 min
Response: 3203635
Conc: 13.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

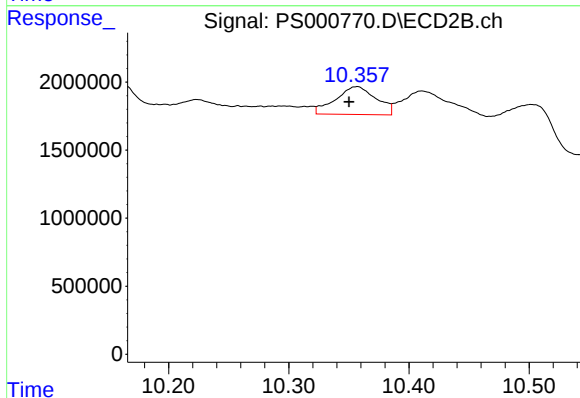


#3 4-Nitrophenol

R.T.: 10.357 min
Delta R.T.: 0.007 min
Response: 4819036
Conc: 24.59 ng/ml

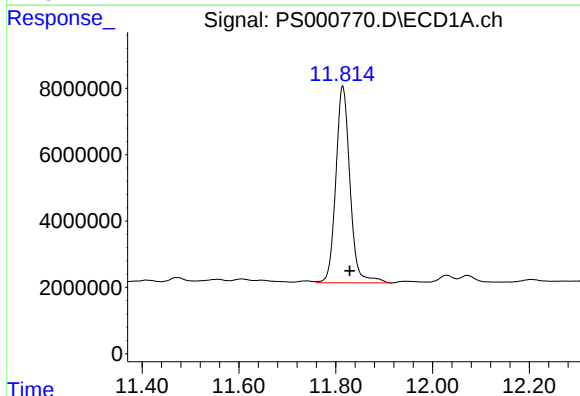


#4 2,4-DCAA

R.T.: 11.814 min
Delta R.T.: -0.015 min
Response: 120514971
Conc: 319.96 ng/ml

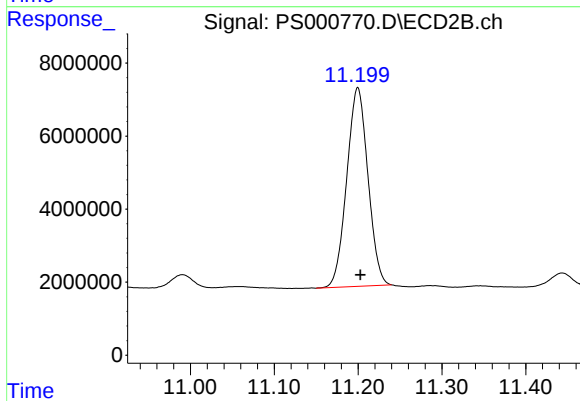

#4 2,4-DCAA


R.T.: 11.200 min
Delta R.T.: -0.003 min
Response: 95614897
Conc: 280.96 ng/ml

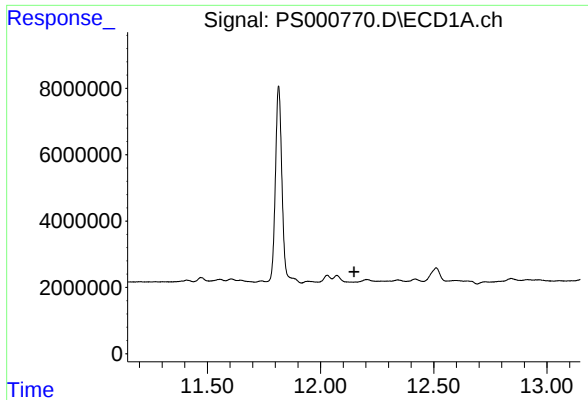

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 12.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

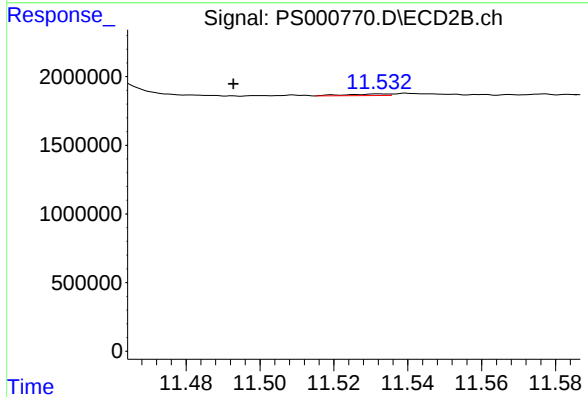


#5 DICAMBA

R.T.: 11.532 min
Delta R.T.: 0.040 min
Response: 97854
Conc: 0.08 ng/ml

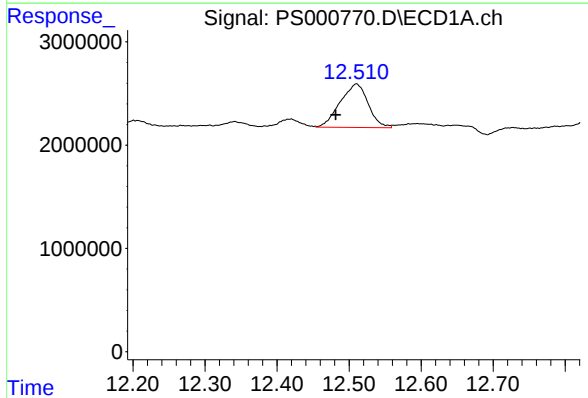


#6 MCP

R.T.: 12.510 min
Delta R.T.: 0.028 min
Response: 11377934
Conc: 10.05 ug/ml

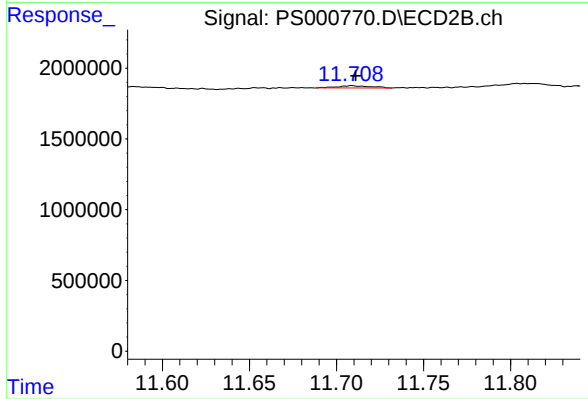

#6 MCP


R.T.: 11.709 min
Delta R.T.: -0.002 min
Response: 212125
Conc: 0.22 ug/ml

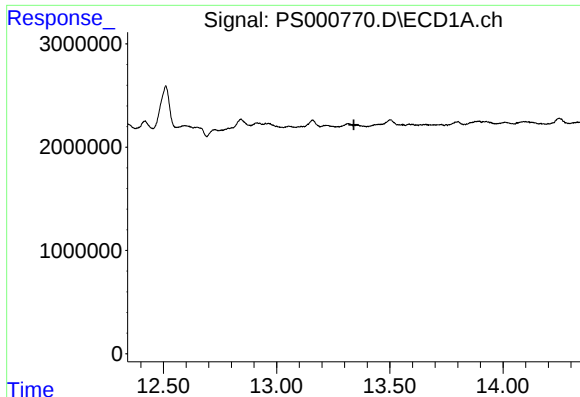

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

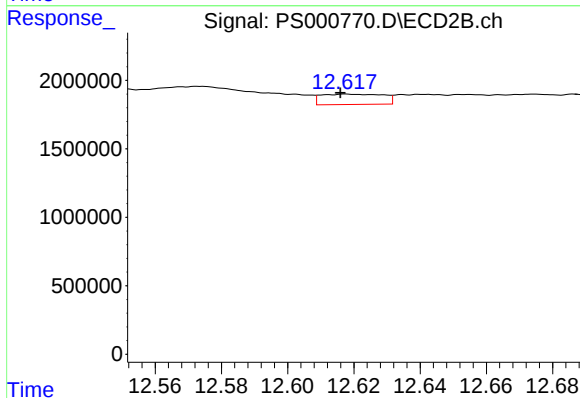


#8 DICHLORPROP

R.T.: 12.618 min
Delta R.T.: 0.002 min
Response: 984671
Conc: 3.06 ng/ml

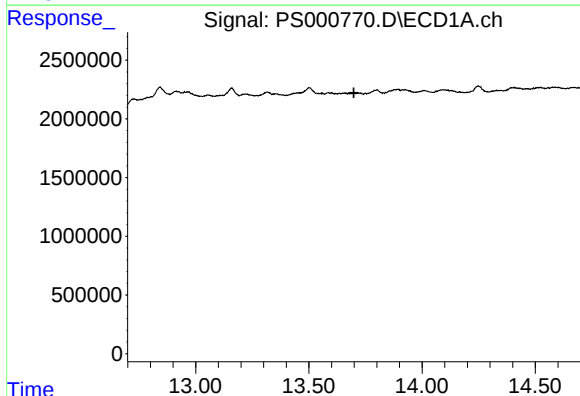


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.699 min
Response: 0
Conc: N.D.

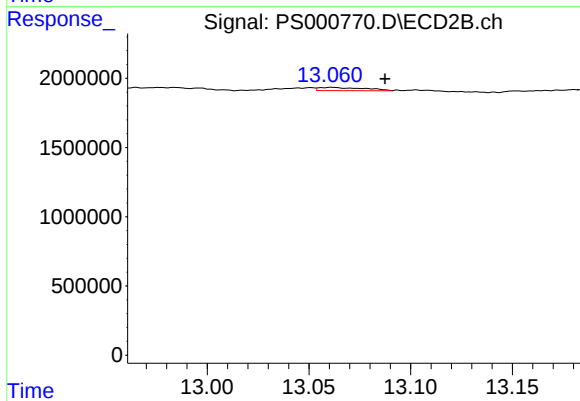

#9 2,4-D


R.T.: 13.061 min
Delta R.T.: -0.026 min
Response: 358782
Conc: 0.84 ng/ml

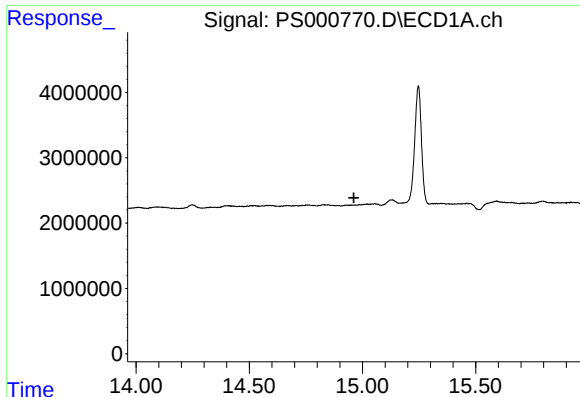

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.962 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

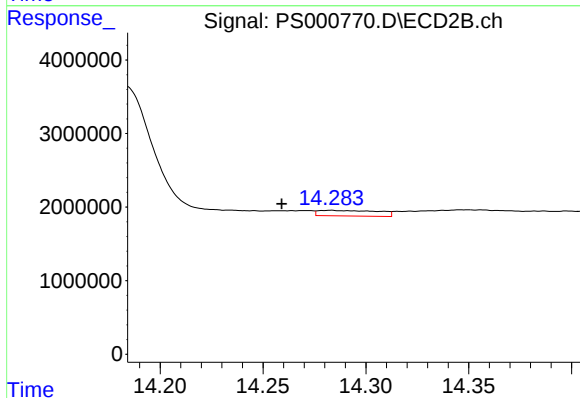


#11 2,4,5-TP (SILVEX)

R.T.: 14.283 min
Delta R.T.: 0.024 min
Response: 1541347
Conc: 0.79 ng/ml

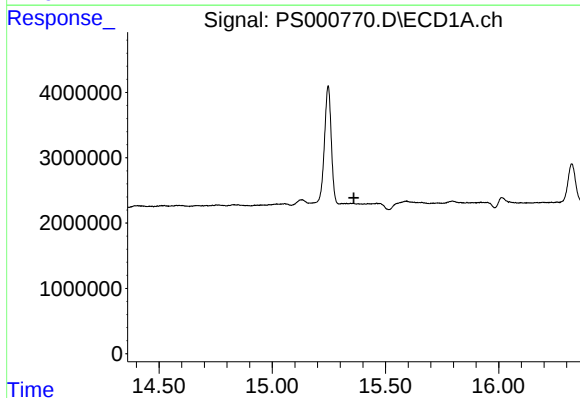


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.360 min
Response: 0
Conc: N.D.

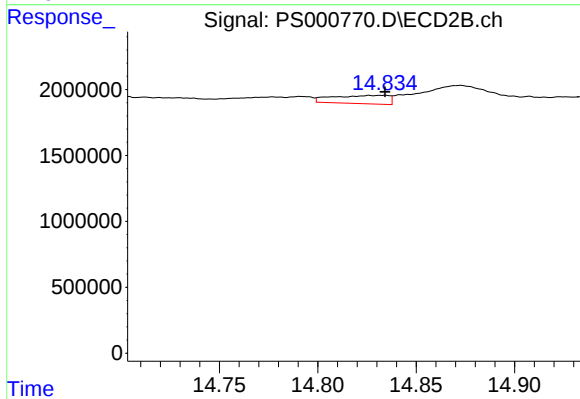

#12 2,4,5-T


R.T.: 14.826 min
Delta R.T.: -0.008 min
Response: 1242851
Conc: 0.73 ng/ml

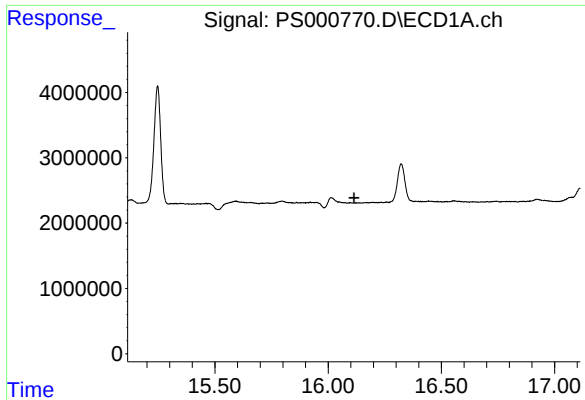

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

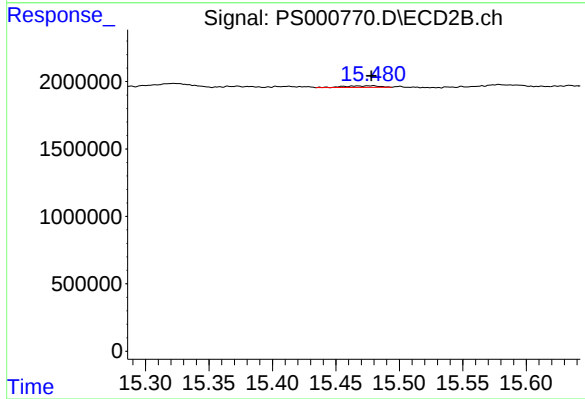


#13 2,4-DB

R.T.: 15.480 min
Delta R.T.: 0.002 min
Response: 238125
Conc: 0.96 ng/ml

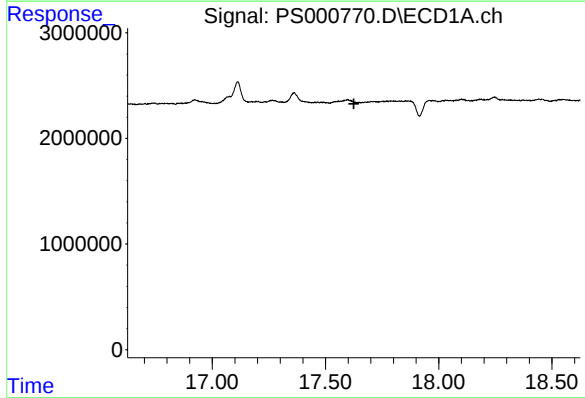


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.625 min
Response: 0
Conc: N.D.

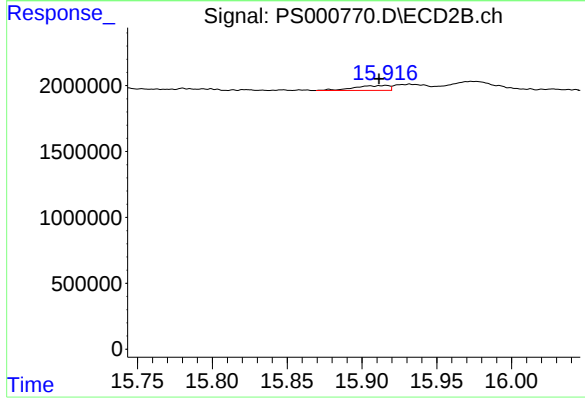

#14 DINOSEB


R.T.: 15.916 min
Delta R.T.: 0.005 min
Response: 596192
Conc: 0.46 ng/ml

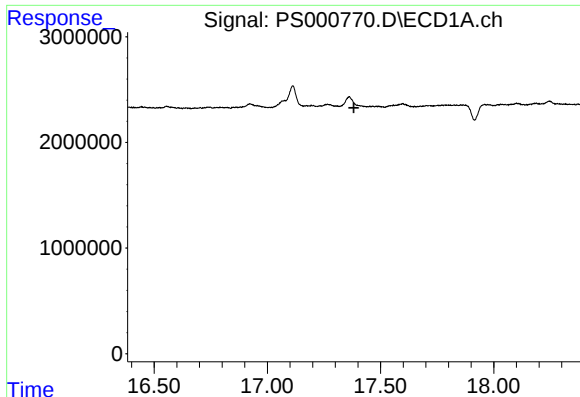

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

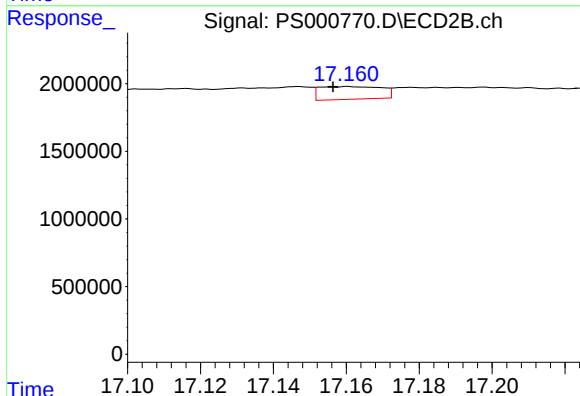


#15 Picloram

R.T.: 17.161 min
Delta R.T.: 0.004 min
Response: 1108774
Conc: 0.44 ng/ml

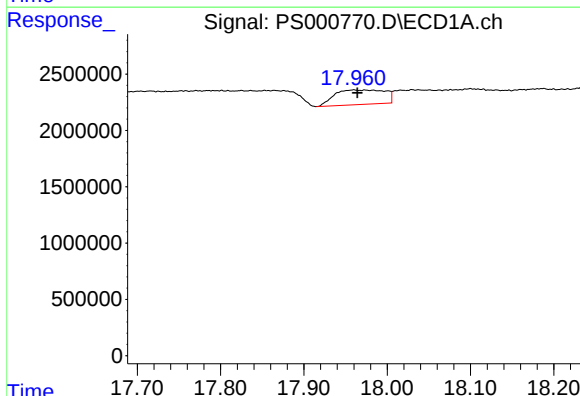

#16 DCPA

R.T.: 17.959 min
Delta R.T.: -0.005 min
Response: 5415536
Conc: 2.11 ng/ml

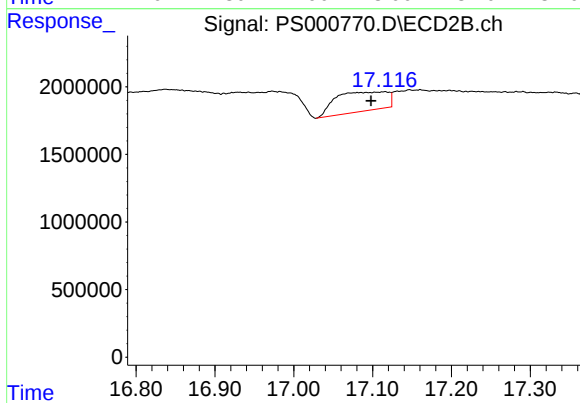

#16 DCPA

R.T.: 17.116 min
Delta R.T.: 0.018 min
Response: 6560586
Conc: 2.85 ng/ml