

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070323\
 Data File : PS023598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2023 12:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 21:33:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.482	0.000	2407486	0	1.361	N.D.	#
Target Compounds								
1) T	Dalapon	2.587	2.599	24923006	300698	13.630	<MDL	#
2) T	3,5-DICHL...	5.828	0.000	309605	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.326	6.525f	10424044	1103654	8.088	3.235	#
5) T	DICAMBA	6.632	0.000	1691951	0	<MDL	N.D.	#
6) T	MCPD	6.752	0.000	56204	0	<MDL	N.D.	#
7) T	MCPA	6.933	0.000	118276	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.201	0.000	45315910	0	21.960	N.D.	#
9) T	2,4-D	7.461	0.000	49758266	0	20.365	N.D.	#
10) T	Pentachlo...	7.686	0.000	496761	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	8.194	8.706	1455814	730768	<MDL	<MDL	#
12) T	2,4,5-T	8.471	9.077	466634	585033	<MDL	<MDL	#
13) T	2,4-DB	8.997	9.592	9855602	326993	4.187	<MDL	#
14) T	DINOSEB	10.055	0.000	806361	0	<MDL	N.D.	#
15) T	Picloram	9.910	10.877	63289245	14341172	3.647	3.142	
16) T	DCPA	10.322	10.877	616911	14341172	<MDL	3.575	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070323\
Data File : PS023598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2023 12:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 21:33:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

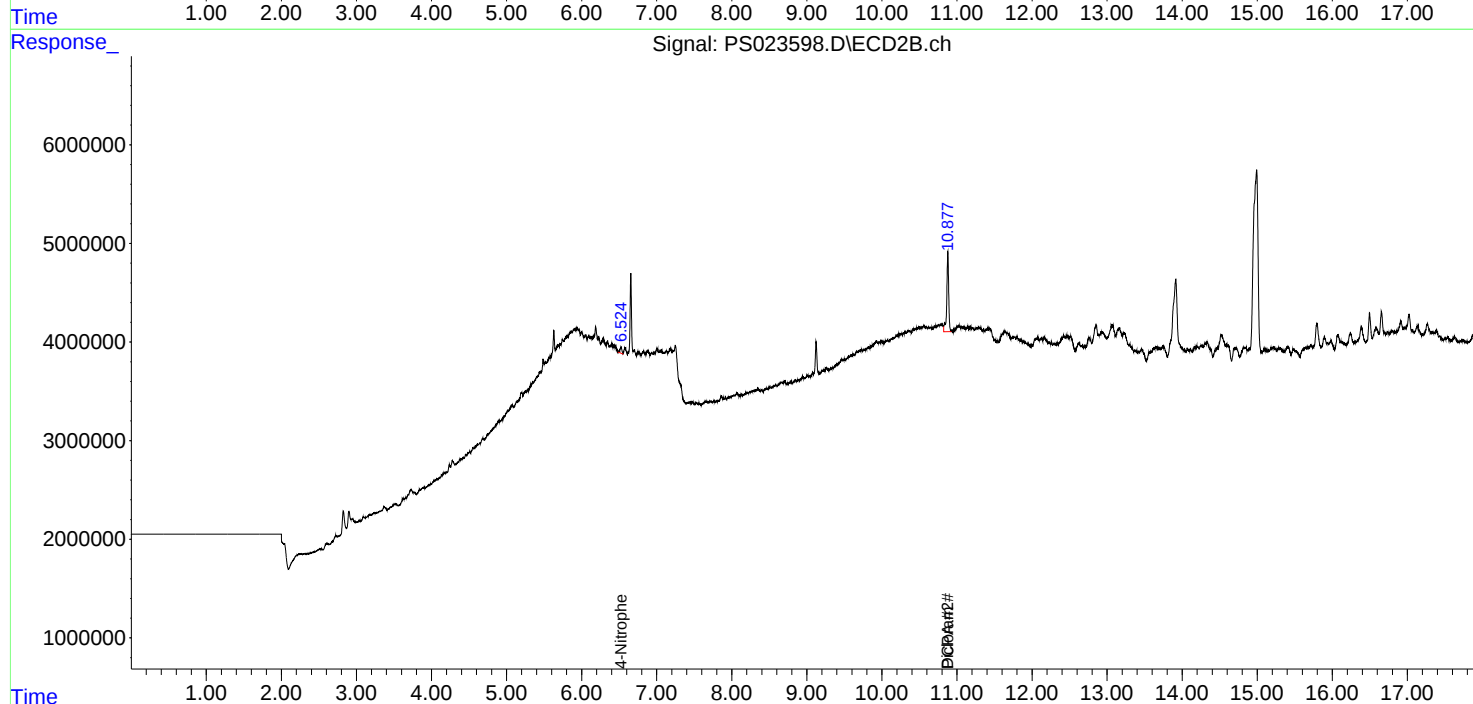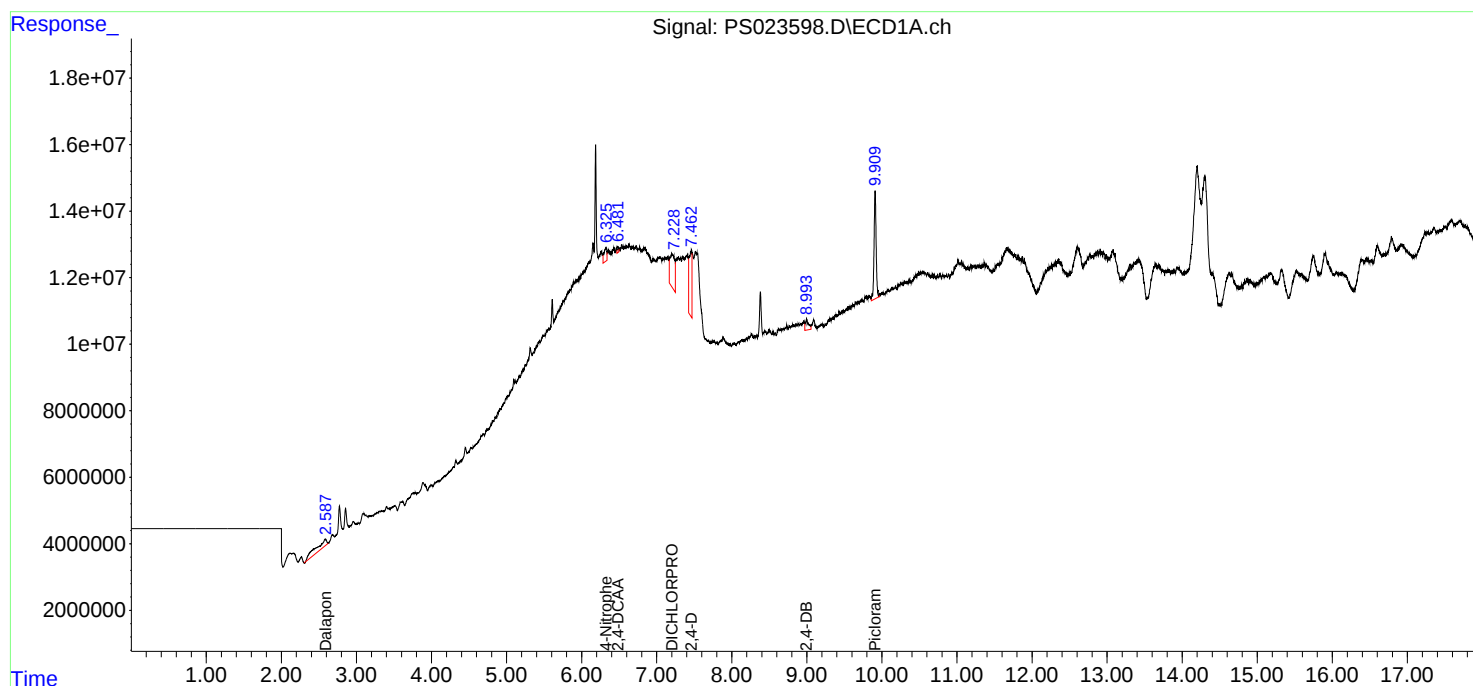


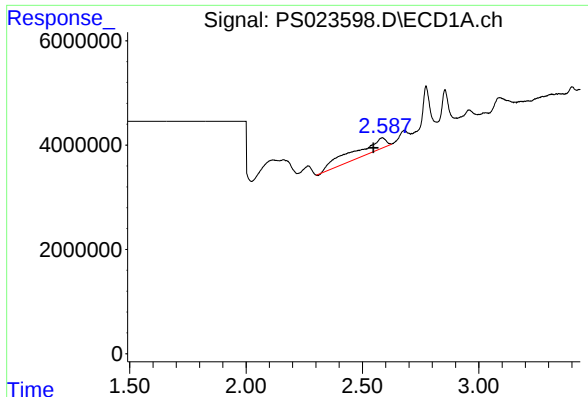

#1 Dalapon


R.T.: 2.587 min
Delta R.T.: 0.040 min
Response: 24923006
Conc: 13.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

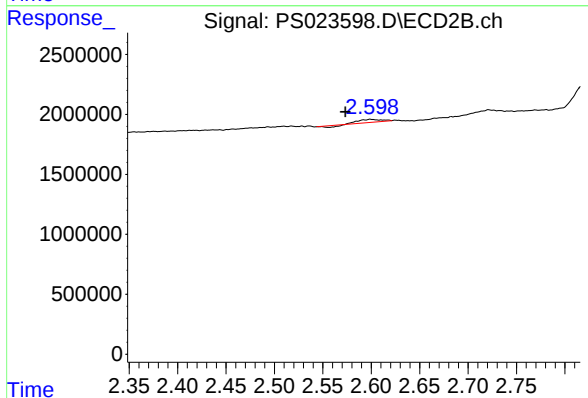


#1 Dalapon

R.T.: 2.599 min
Delta R.T.: 0.025 min
Response: 300698
Conc: N.D.

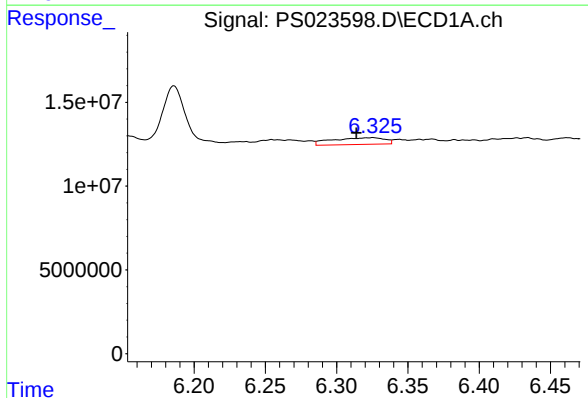


#3 4-Nitrophenol

R.T.: 6.326 min
Delta R.T.: 0.012 min
Response: 10424044
Conc: 8.09 ng/ml

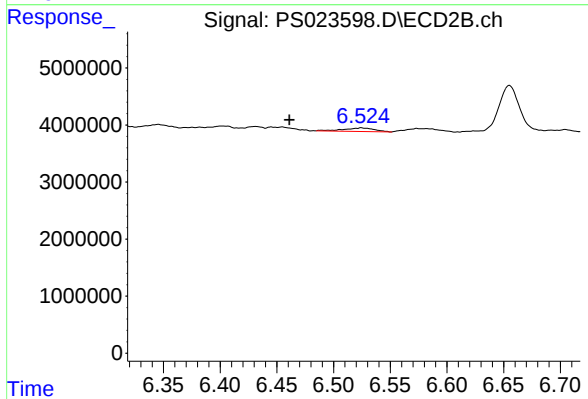

#3 4-Nitrophenol


R.T.: 6.525 min
Delta R.T.: 0.063 min
Response: 1103654
Conc: 3.24 ng/ml

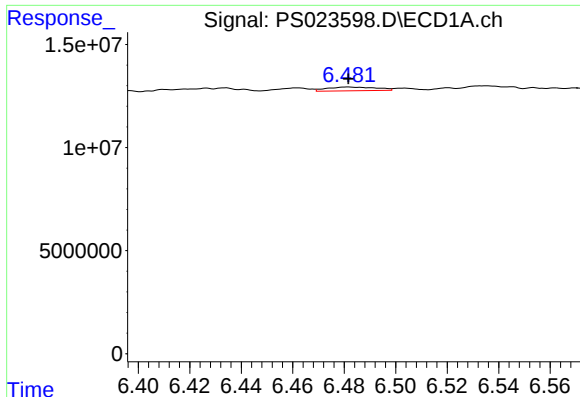

#4 2,4-DCAA


R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 2407486
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

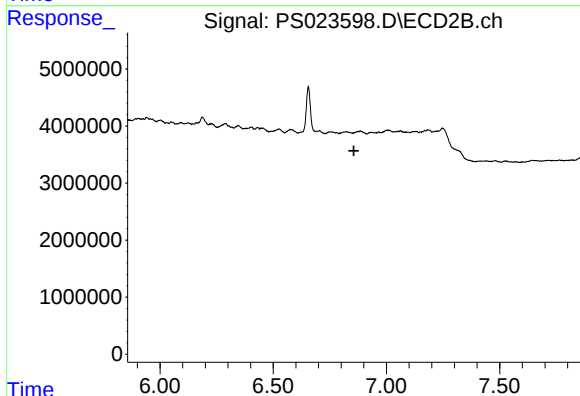


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.856 min
Response: 0
Conc: N.D.

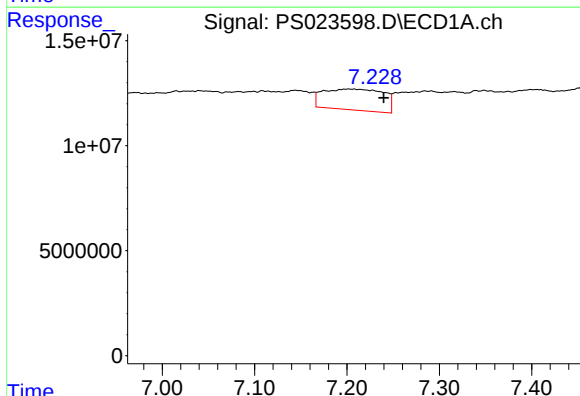


#8 DICHLORPROP

R.T.: 7.201 min
Delta R.T.: -0.038 min
Response: 45315910
Conc: 21.96 ng/ml

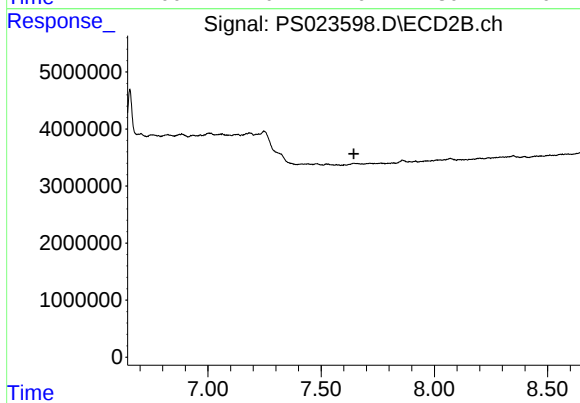

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.645 min
Response: 0
Conc: N.D.

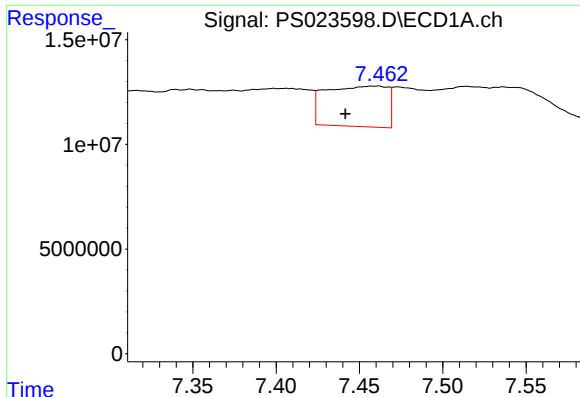

#9 2,4-D


R.T.: 7.461 min
Delta R.T.: 0.019 min
Response: 49758266
Conc: 20.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

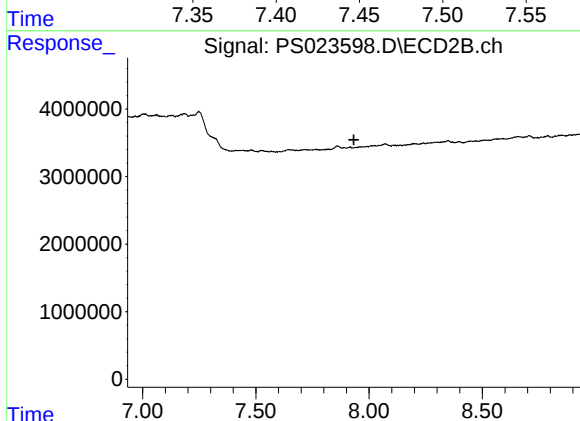


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.933 min
Response: 0
Conc: N.D.

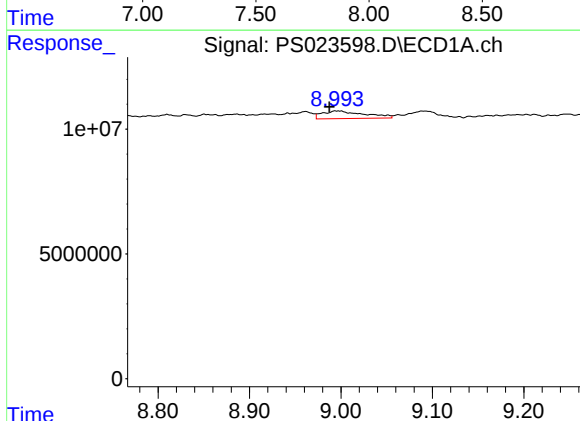


#13 2,4-DB

R.T.: 8.997 min
Delta R.T.: 0.009 min
Response: 9855602
Conc: 4.19 ng/ml

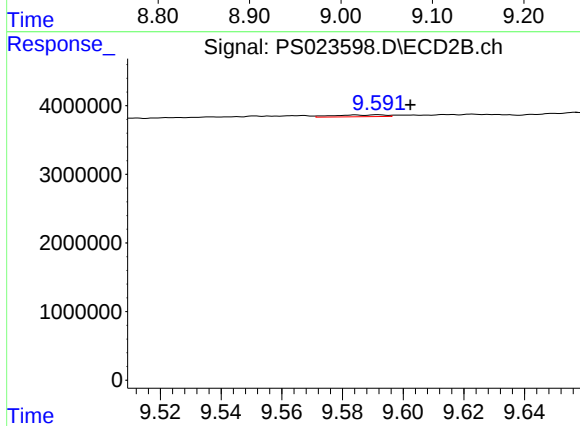

#13 2,4-DB


R.T.: 9.592 min
Delta R.T.: -0.011 min
Response: 326993
Conc: N.D.

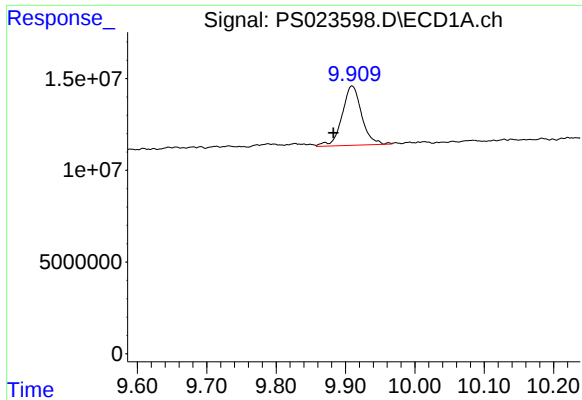

#15 Picloram


R.T.: 9.910 min
Delta R.T.: 0.027 min
Response: 63289245
Conc: 3.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

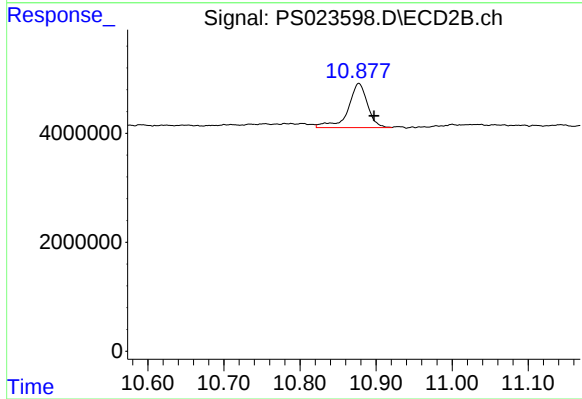


#15 Picloram

R.T.: 10.877 min
Delta R.T.: -0.020 min
Response: 14341172
Conc: 3.14 ng/ml

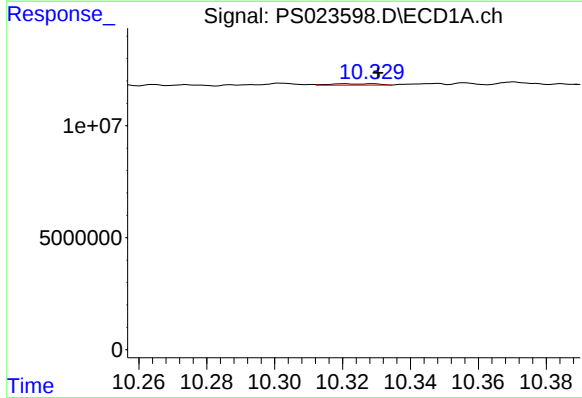

#16 DCPA

R.T.: 10.322 min
Delta R.T.: -0.009 min
Response: 616911
Conc: N.D.

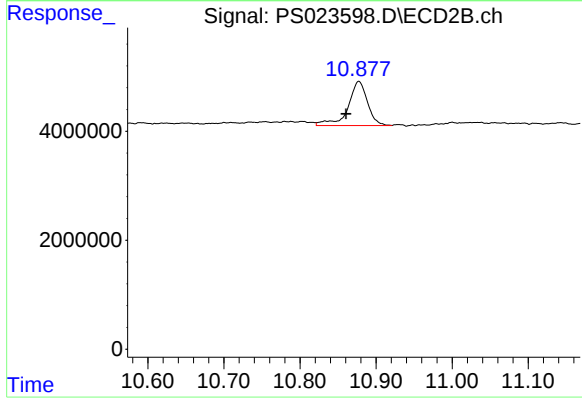

#16 DCPA

R.T.: 10.877 min
Delta R.T.: 0.017 min
Response: 14341172
Conc: 3.57 ng/ml