

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070323\
 Data File : PS023599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2023 12:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 21:34:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
 Quant Title : 8080.M
 QLast Update : Tue Jun 06 13:00:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.479	6.843	926.1E6	219.2E6	523.419	386.180 #
Target Compounds							
1) T	Dalapon	2.557	0.000	3487610	0	1.907	N.D. #
2) T	3,5-DICHL...	5.799	0.000	164088	0	<MDL	N.D. #
3) T	4-Nitroph...	6.315	0.000	5113259	0	3.967	N.D. #
6) T	MCP	6.818	0.000	272163	0	<MDL	N.D. #
7) T	MCPA	6.853f	7.292	-3710627	13121792	N.D.	4.882
8) T	DICHLORPROP	7.289f	0.000	1433708	0	<MDL	N.D. #
10) T	Pentachlo...	7.668	0.000	825750	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.210	0.000	3627271	0	<MDL	N.D. #
12) T	2,4,5-T	8.475	9.127	2890641	2971142	<MDL	<MDL #
13) T	2,4-DB	8.974	9.663f	4024391	1103881	1.710	2.977 #
14) T	DINOSEB	10.056	0.000	517659	0	<MDL	N.D. #
15) T	Picloram	9.890	10.879	45460855	13193630	2.620	2.891
16) T	DCPA	10.329	10.879	2153022	13193630	<MDL	3.289 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070323\
Data File : PS023599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2023 12:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 21:34:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS060623.M
Quant Title : 8080.M
QLast Update : Tue Jun 06 13:00:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

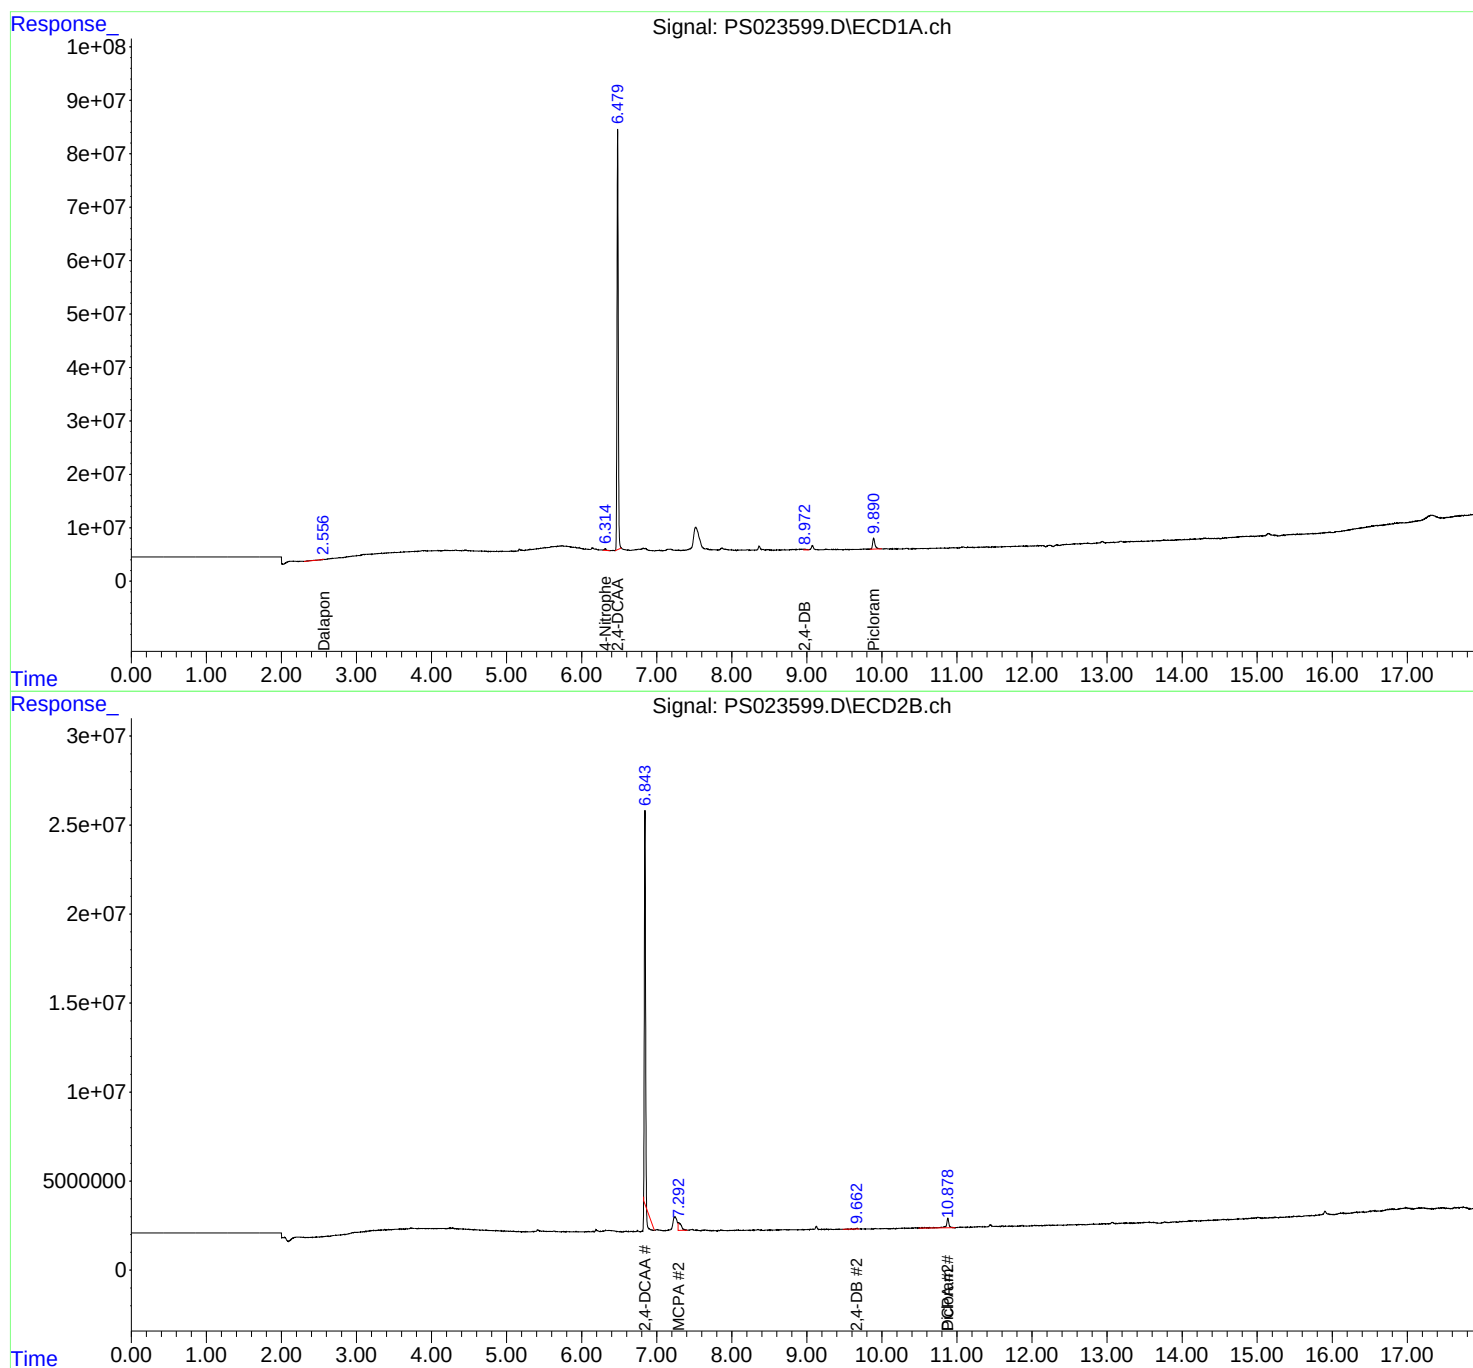


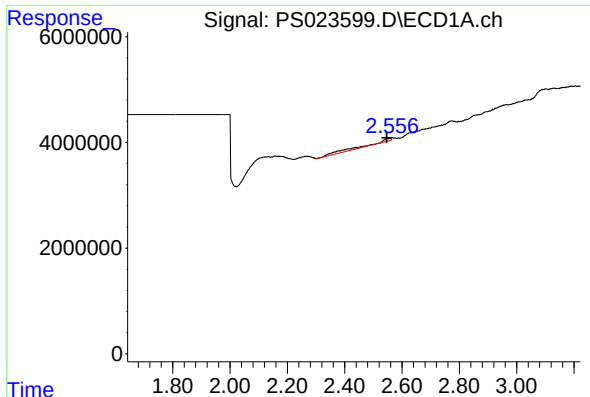

#1 Dalapon


R.T.: 2.557 min
Delta R.T.: 0.010 min
Response: 3487610
Conc: 1.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

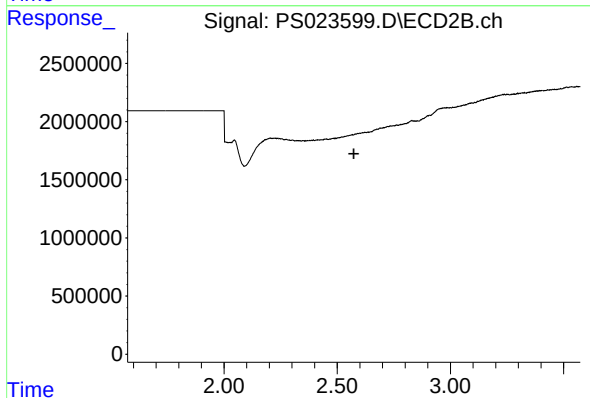


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.574 min
Response: 0
Conc: N.D.

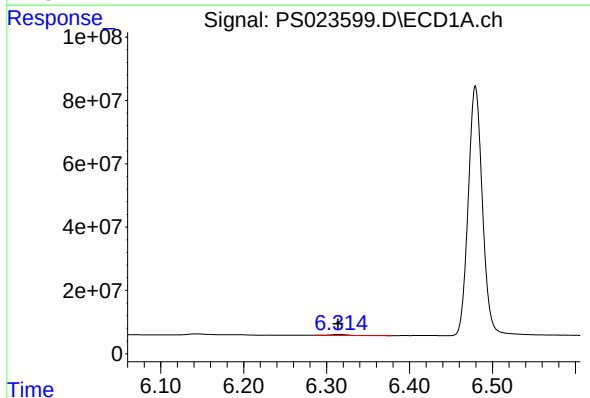


#3 4-Nitrophenol

R.T.: 6.315 min
Delta R.T.: 0.001 min
Response: 5113259
Conc: 3.97 ng/ml

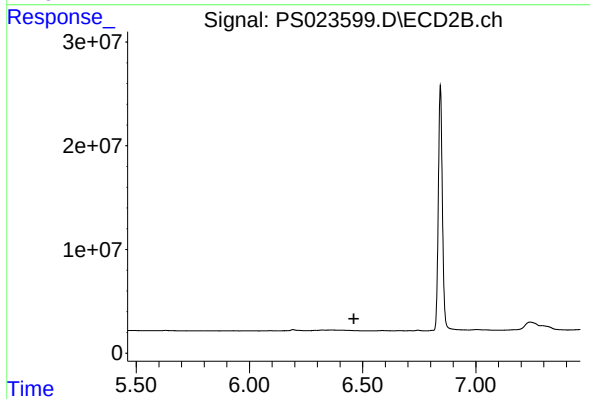

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.461 min
Response: 0
Conc: N.D.

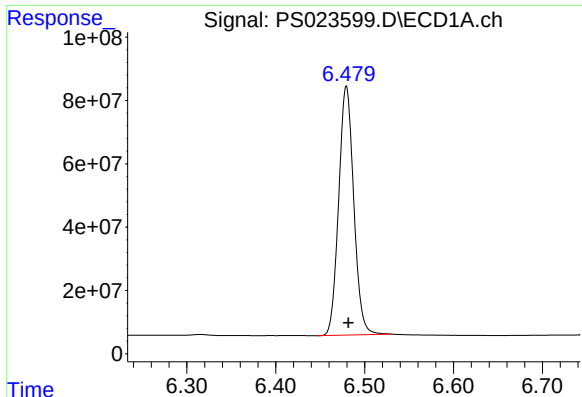

#4 2,4-DCAA


R.T.: 6.479 min
Delta R.T.: -0.002 min
Response: 926062072
Conc: 523.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

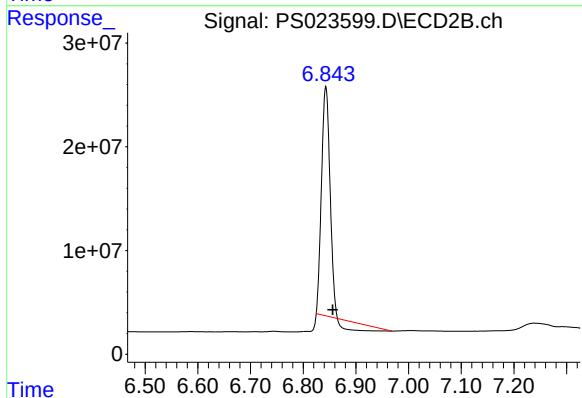


#4 2,4-DCAA

R.T.: 6.843 min
Delta R.T.: -0.013 min
Response: 219232435
Conc: 386.18 ng/ml

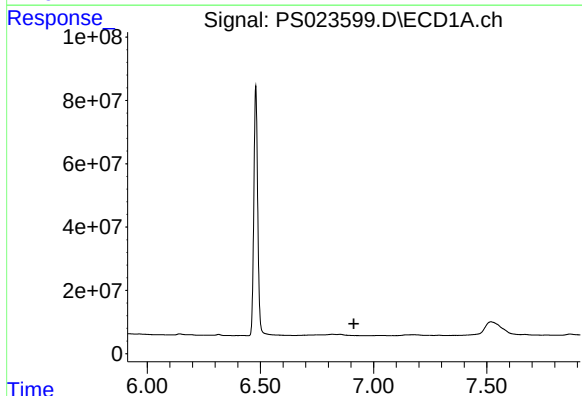


#7 MCPA

R.T.: 6.853 min
Delta R.T.: -0.060 min
Response: -3710627
Conc: N.D.

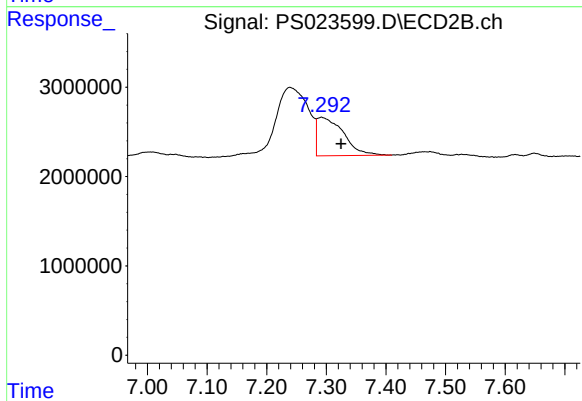

#7 MCPA


R.T.: 7.292 min
Delta R.T.: -0.033 min
Response: 13121792
Conc: 4.88 ug/ml

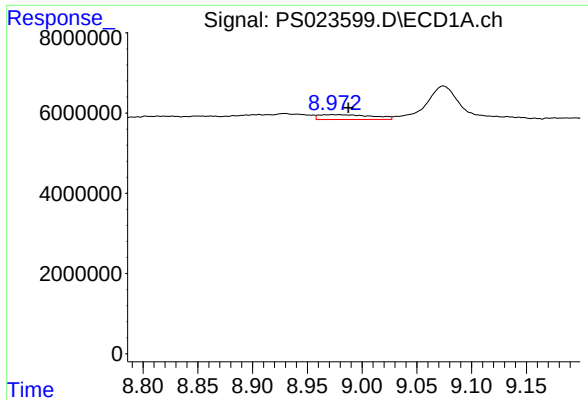

#13 2,4-DB


R.T.: 8.974 min
Delta R.T.: -0.014 min
Response: 4024391
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

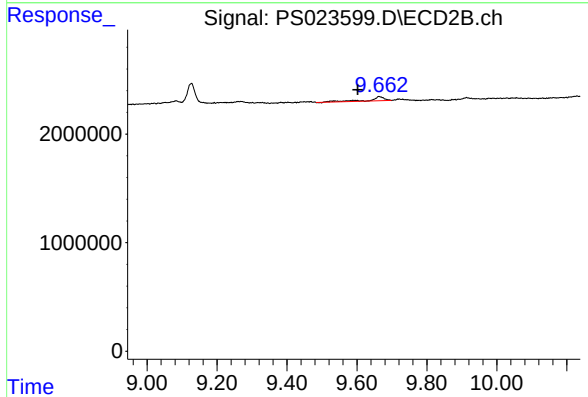


#13 2,4-DB

R.T.: 9.663 min
Delta R.T.: 0.060 min
Response: 1103881
Conc: 2.98 ng/ml

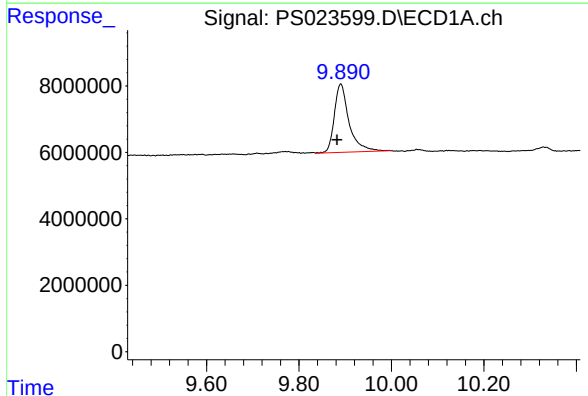


#15 Picloram

R.T.: 9.890 min
Delta R.T.: 0.008 min
Response: 45460855
Conc: 2.62 ng/ml

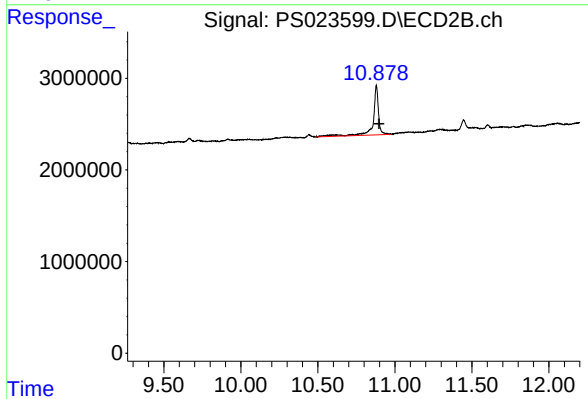

#15 Picloram


R.T.: 10.879 min
Delta R.T.: -0.018 min
Response: 13193630
Conc: 2.89 ng/ml

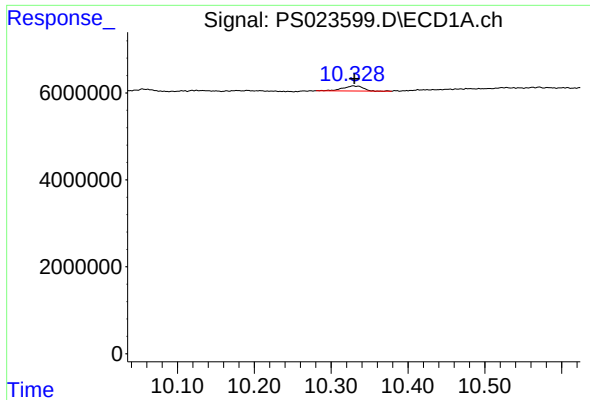

#16 DCPA

R.T.: 10.329 min
Delta R.T.: 0.000 min
Response: 2153022
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

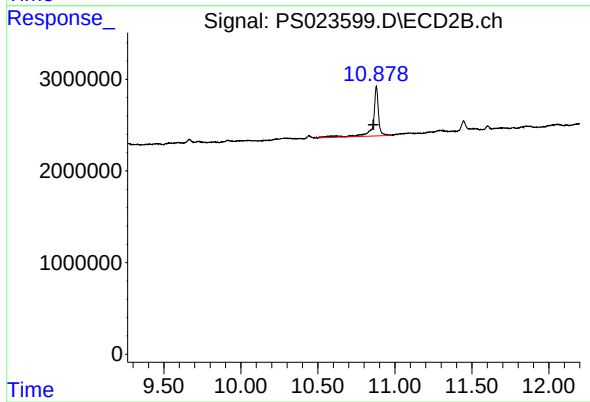

#16 DCPA

R.T.: 10.879 min
Delta R.T.: 0.019 min
Response: 13193630
Conc: 3.29 ng/ml