

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070522\
 Data File : PS019871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jul 2022 12:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 06:19:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.199	6.778	1069.1E6	370.4E6	412.206	456.070
Target Compounds							
3) T	4-Nitroph...	0.000	6.412	0	8547654	N.D.	19.763
6) T	MCP	7.518	7.056	113282	1145844	<MDL	<MDL #
7) T	MCPA	7.728	0.000	35751324	0	3.051	N.D. #
8) T	DICHLORPROP	8.103	0.000	7436913	0	2.747	N.D. #
9) T	2,4-D	8.318	7.864	21997301	335317	7.406	<MDL #
10) T	Pentachlo...	8.618	0.000	430485	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.196	8.625	2569662	76993	<MDL	<MDL #
14) T	DINOSEB	11.103f	0.000	42960790	0	2.642	N.D. #
15) T	Picloram	10.961	10.783f	412895	785040	<MDL	<MDL #
16) T	DCPA	11.423	10.783	1874570	785040	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070522\
Data File : PS019871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jul 2022 12:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 06:19:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

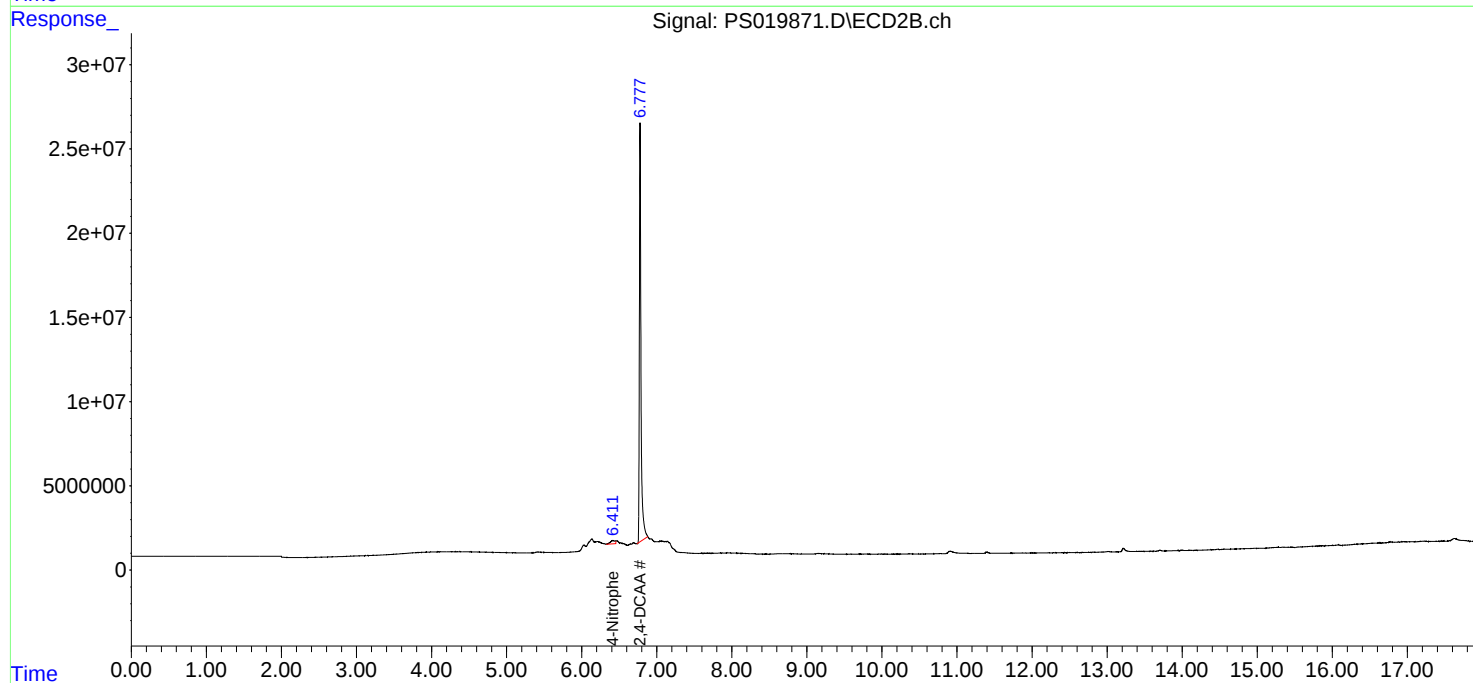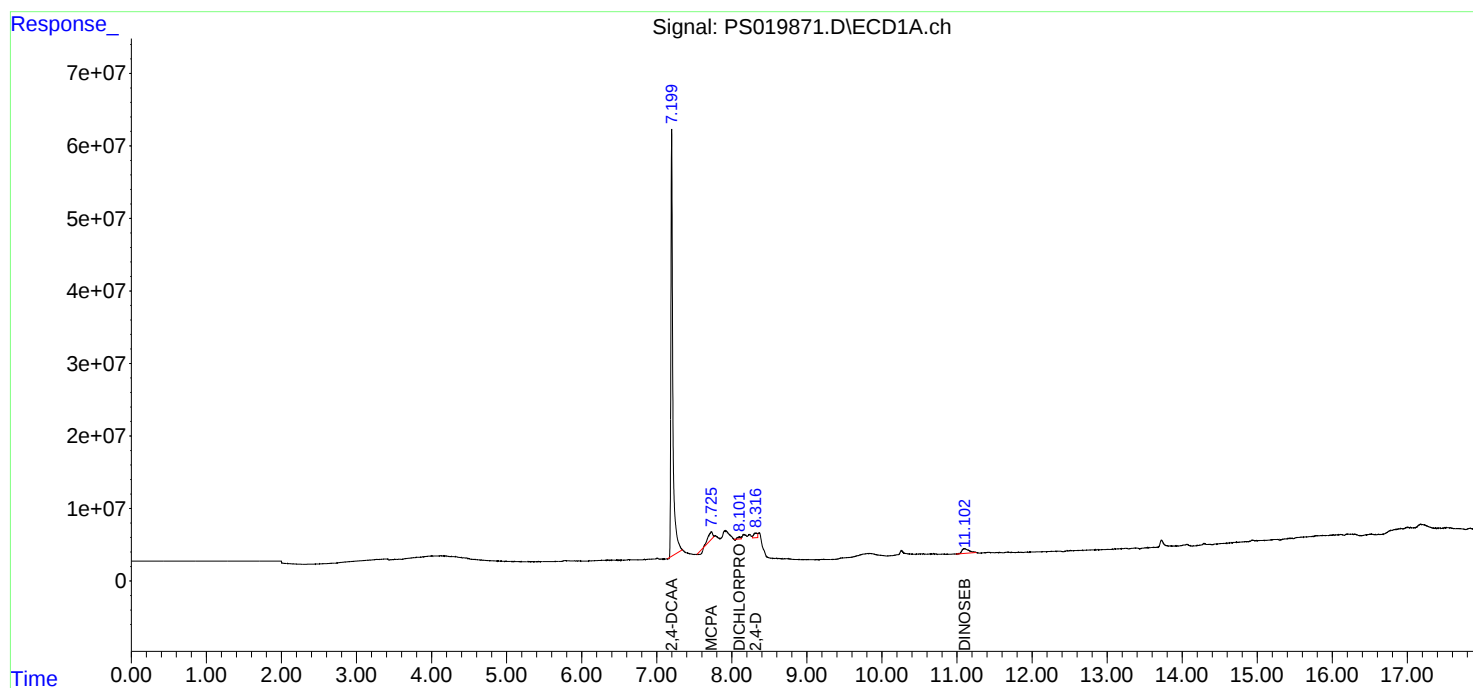


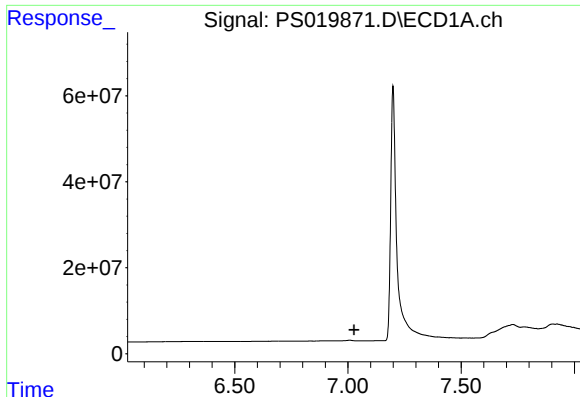

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.027 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

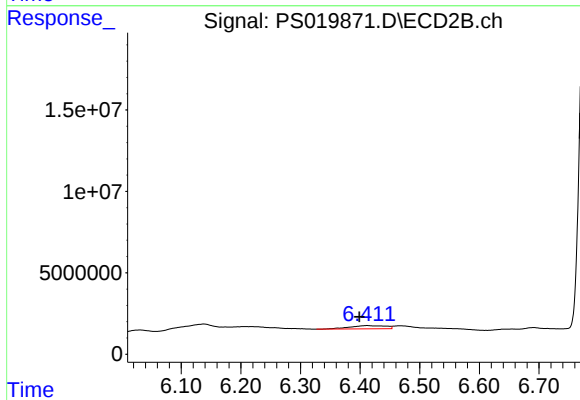


#3 4-Nitrophenol

R.T.: 6.412 min
Delta R.T.: 0.013 min
Response: 8547654
Conc: 19.76 ng/ml

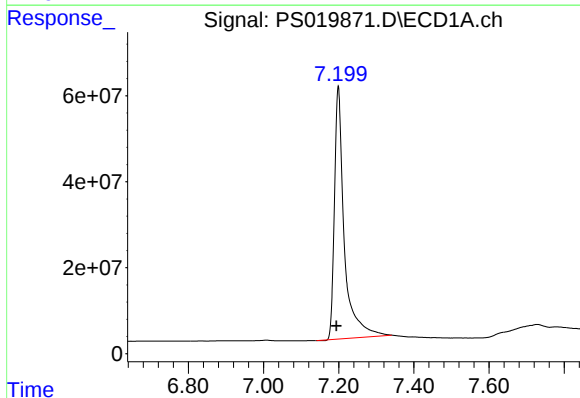


#4 2,4-DCAA

R.T.: 7.199 min
Delta R.T.: 0.005 min
Response: 1069118280
Conc: 412.21 ng/ml

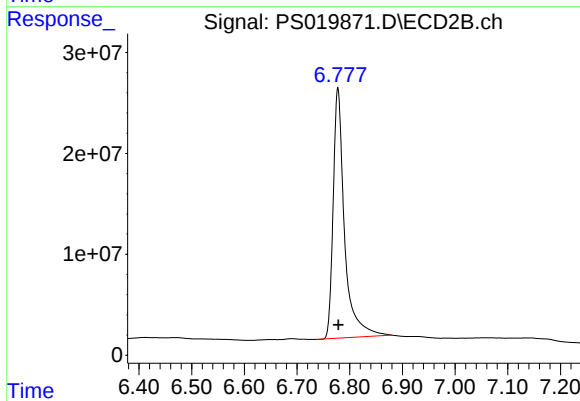

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: -0.001 min
Response: 370395268
Conc: 456.07 ng/ml

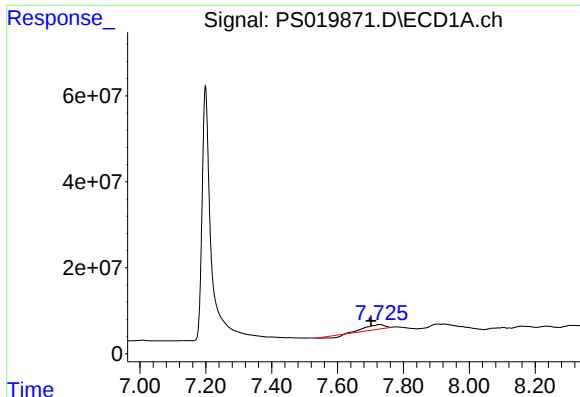

#7 MCPA


R.T.: 7.728 min
Delta R.T.: 0.026 min
Response: 35751324
Conc: 3.05 ug/ml

Instrument :
ECD_S
ClientSampleId :

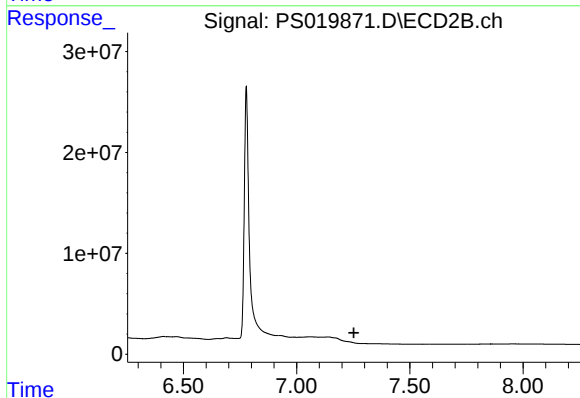


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.253 min
Response: 0
Conc: N.D.

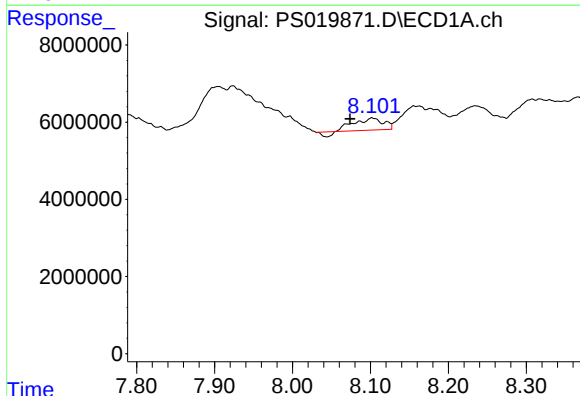


#8 DICHLORPROP

R.T.: 8.103 min
Delta R.T.: 0.029 min
Response: 7436913
Conc: 2.75 ng/ml

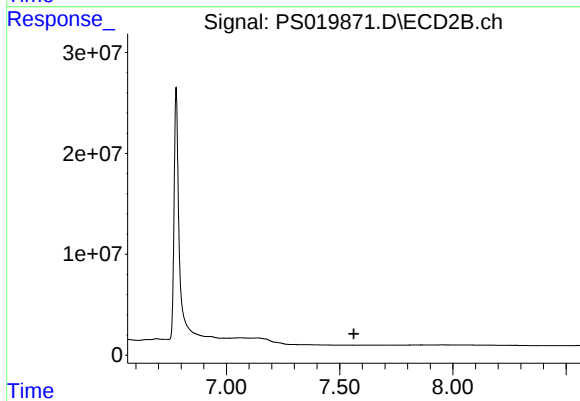

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 7.563 min
Response: 0
Conc: N.D.

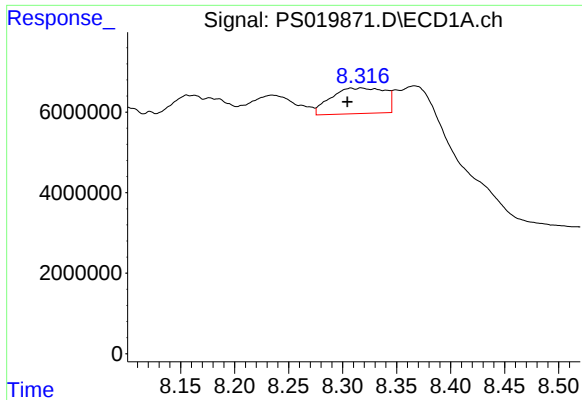

#9 2,4-D


R.T.: 8.318 min
Delta R.T.: 0.013 min
Response: 21997301
Conc: 7.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

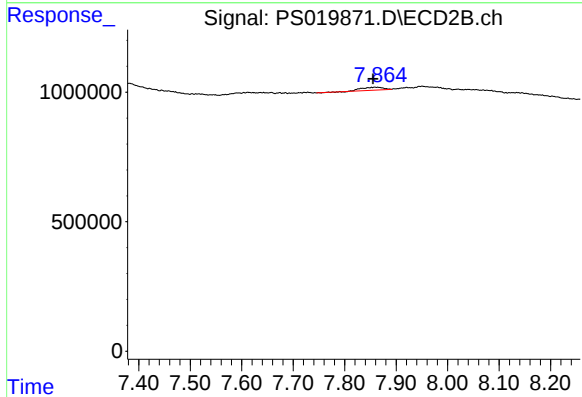


#9 2,4-D

R.T.: 7.864 min
Delta R.T.: 0.009 min
Response: 335317
Conc: N.D.

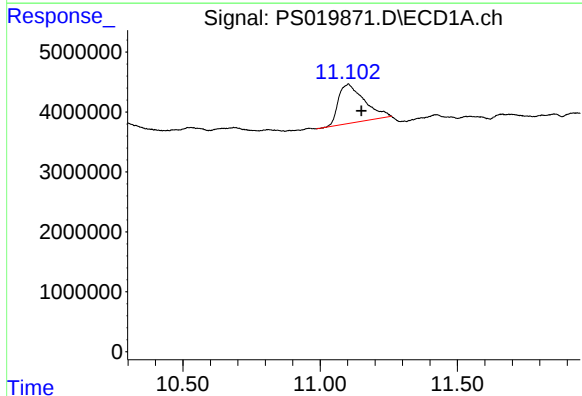

#14 DINOSEB

R.T.: 11.103 min
Delta R.T.: -0.049 min
Response: 42960790
Conc: 2.64 ng/ml

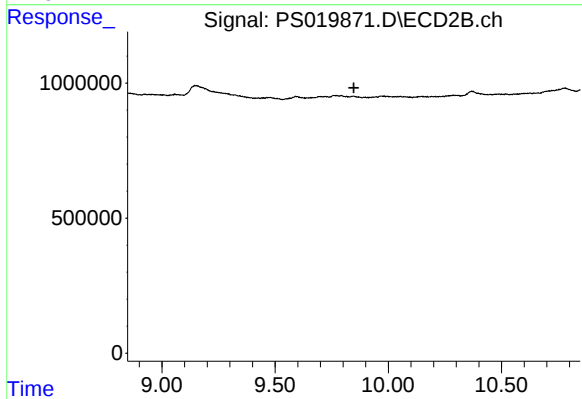

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.848 min
Response: 0
Conc: N.D.