

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070618\
 Data File : PS000805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 20:36
 Operator : UA
 Sample : J3853-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 23:12:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070618.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 06 19:07:49 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.634	11.069	94555897	62028133	270.234	253.352
Target Compounds							
1) T	Dalapon	2.983	0.000	7691229	0	18.043	N.D. #
3) T	4-Nitroph...	11.228	0.000	5928554	0	28.264	N.D. #
5) T	DICAMBA	0.000	11.313	0	7257509	N.D.	7.908 #
7) T	MCPA	12.463	0.000	1593265	0	0.913	N.D. #
10) T	Pentachlo...	13.889	0.000	8817926	0	2.016	N.D. #
11) T	2,4,5-TP ...	0.000	14.049	0	24787356	N.D.	16.887 #
12) T	2,4,5-T	15.203	0.000	3860619	0	2.444	N.D. #
14) T	DINOSEB	17.390	0.000	2790951	0	3.909	N.D. #
16) T	DCPA	17.750	0.000	2676845	0	1.905	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070618\
Data File : PS000805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 20:36
Operator : UA
Sample : J3853-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 23:12:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070618.M
Quant Title : 8080.M
QLast Update : Fri Jul 06 19:07:49 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

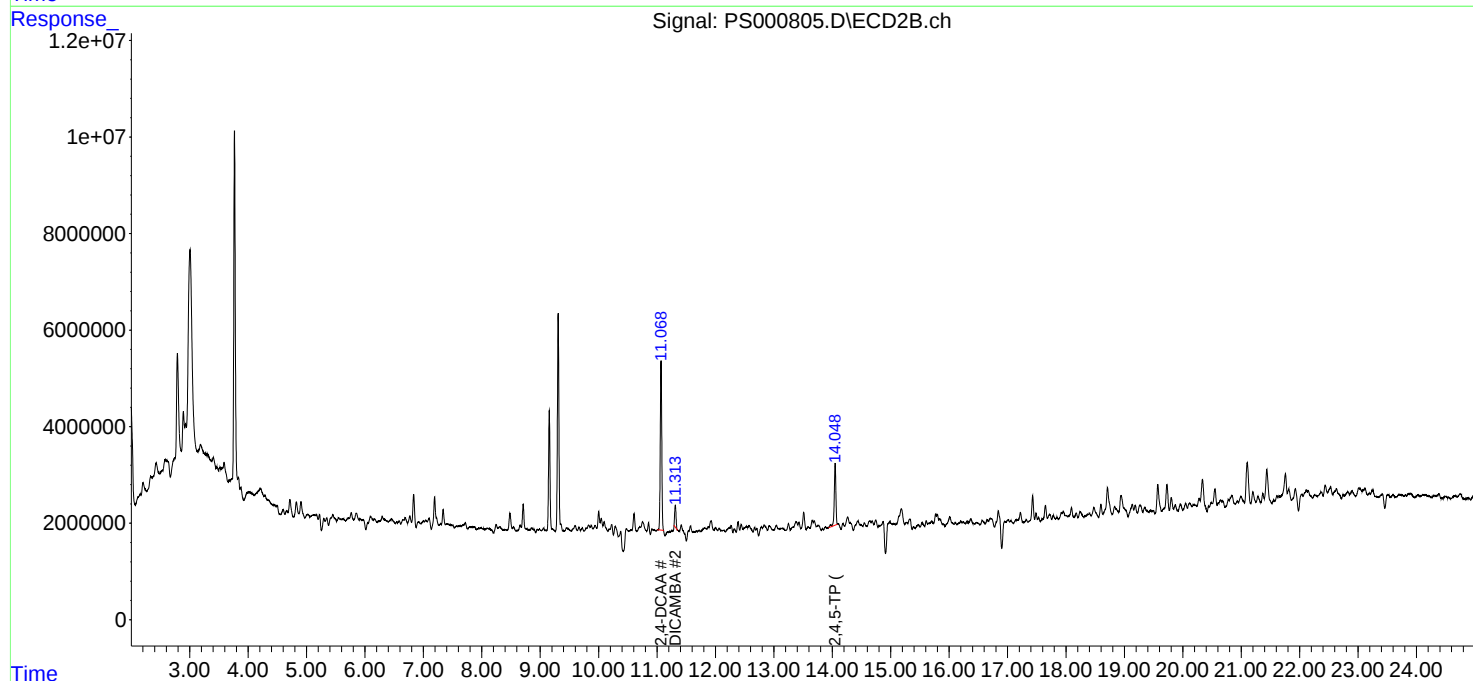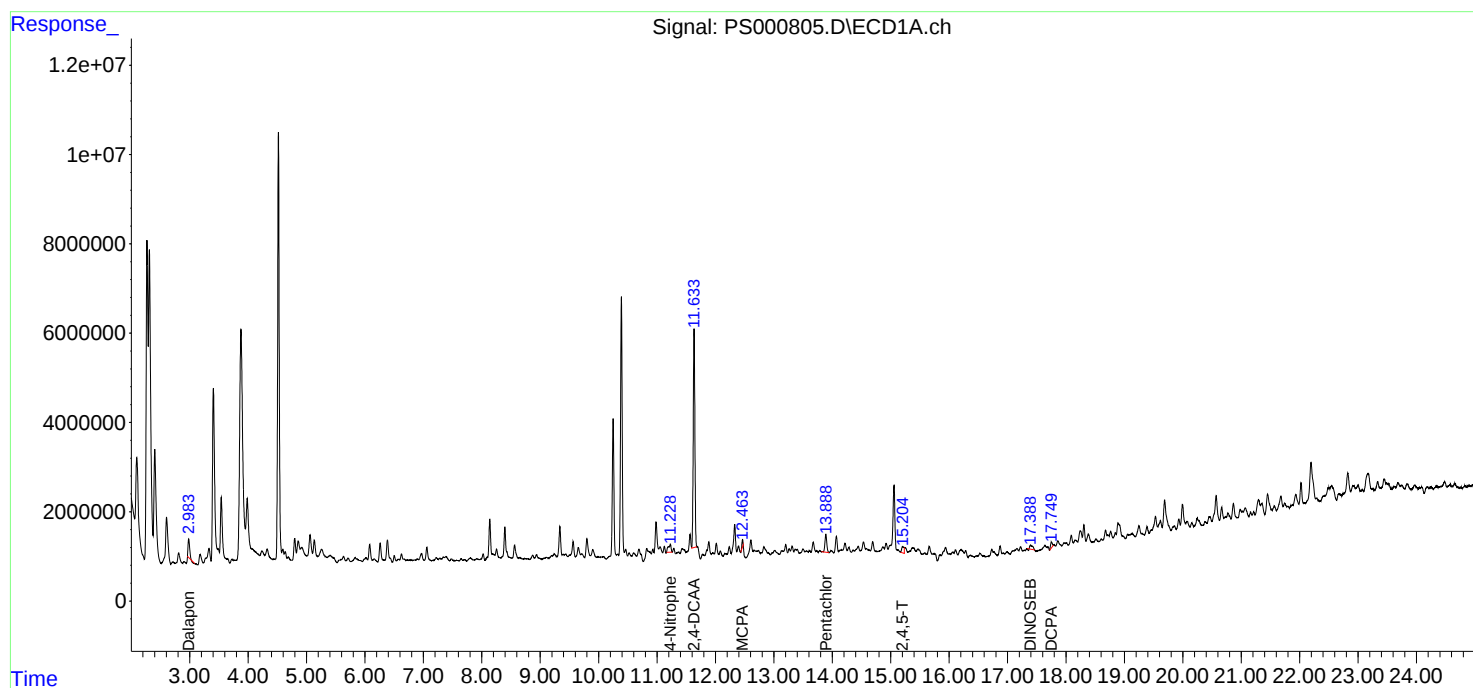


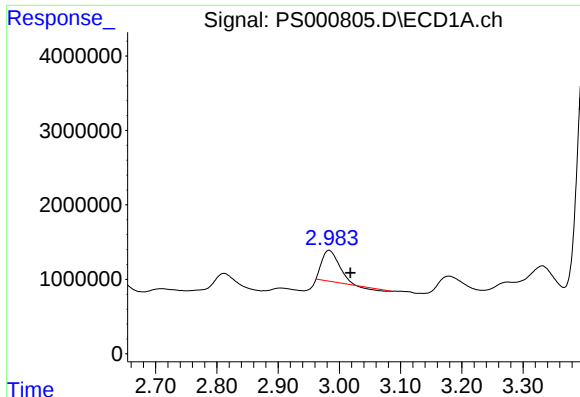

#1 Dalapon


R.T.: 2.983 min
Delta R.T.: -0.035 min
Response: 7691229
Conc: 18.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

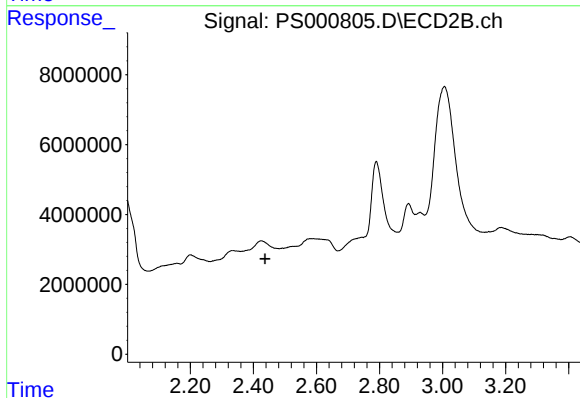


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.437 min
Response: 0
Conc: N.D.

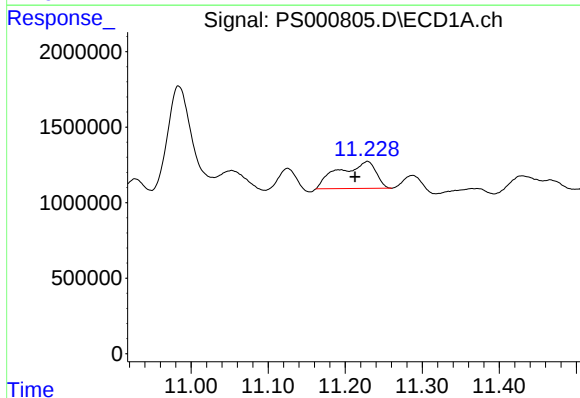


#3 4-Nitrophenol

R.T.: 11.228 min
Delta R.T.: 0.016 min
Response: 5928554
Conc: 28.26 ng/ml

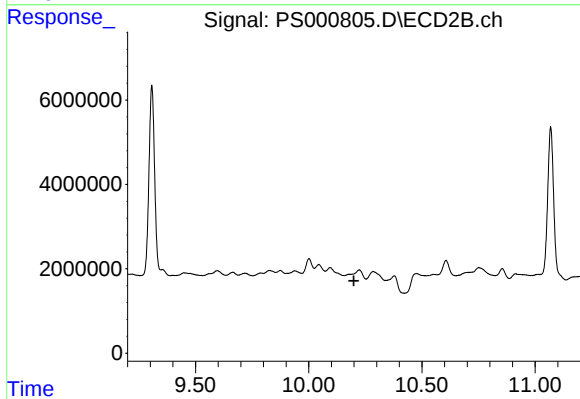

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.200 min
Response: 0
Conc: N.D.

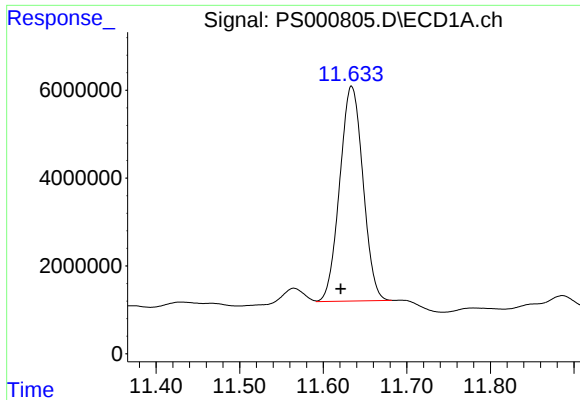

#4 2,4-DCAA


R.T.: 11.634 min
Delta R.T.: 0.013 min
Response: 94555897
Conc: 270.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

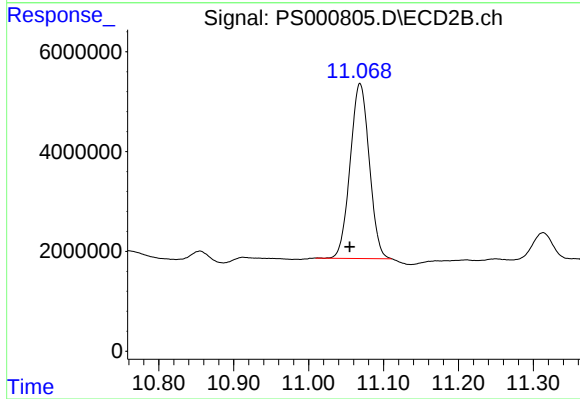


#4 2,4-DCAA

R.T.: 11.069 min
Delta R.T.: 0.014 min
Response: 62028133
Conc: 253.35 ng/ml

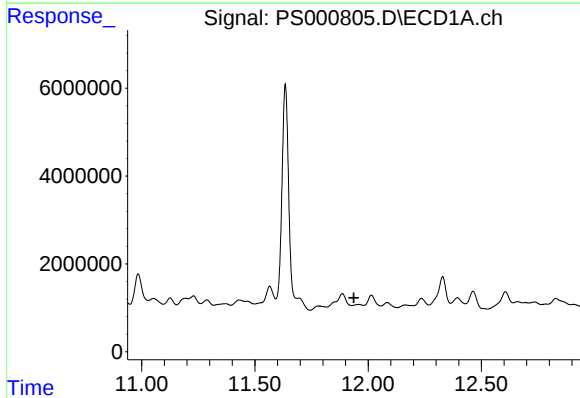


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.937 min
Response: 0
Conc: N.D.

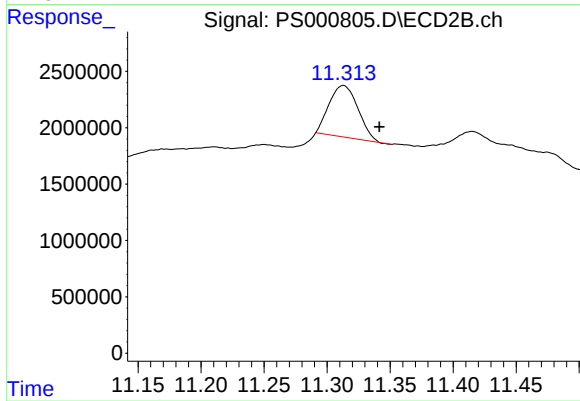

#5 DICAMBA


R.T.: 11.313 min
Delta R.T.: -0.029 min
Response: 7257509
Conc: 7.91 ng/ml

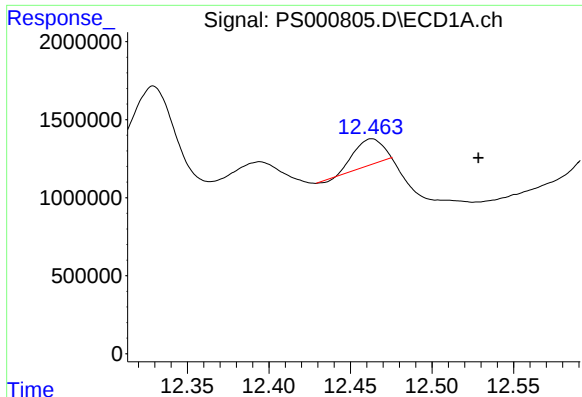

#7 MCPA


R.T.: 12.463 min
Delta R.T.: -0.066 min
Response: 1593265
Conc: 0.91 ug/ml

Instrument :
ECD_S
ClientSampleId :

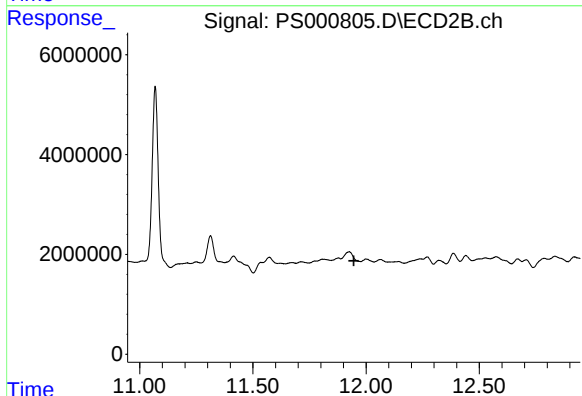


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.946 min
Response: 0
Conc: N.D.

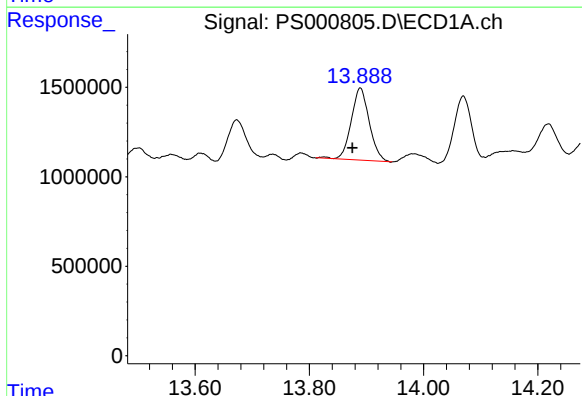


#10 Pentachlorophenol

R.T.: 13.889 min
Delta R.T.: 0.014 min
Response: 8817926
Conc: 2.02 ng/ml

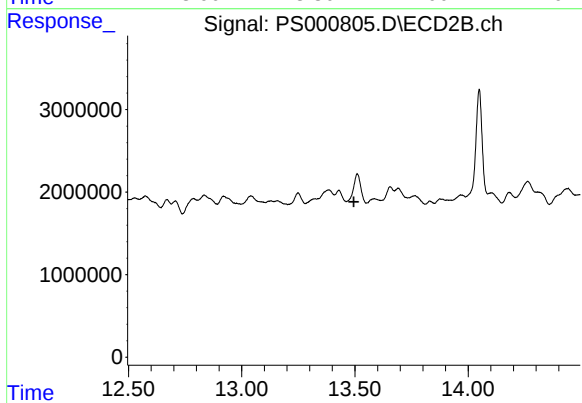

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.495 min
Response: 0
Conc: N.D.

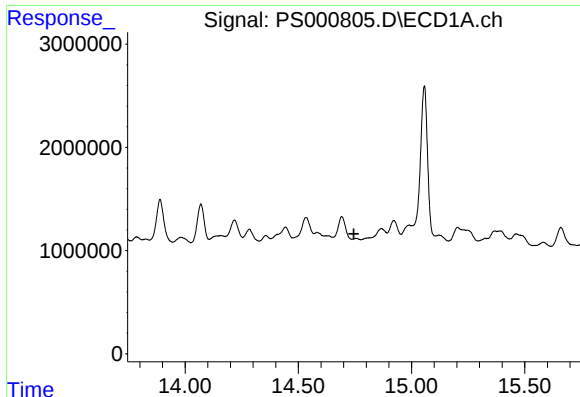

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

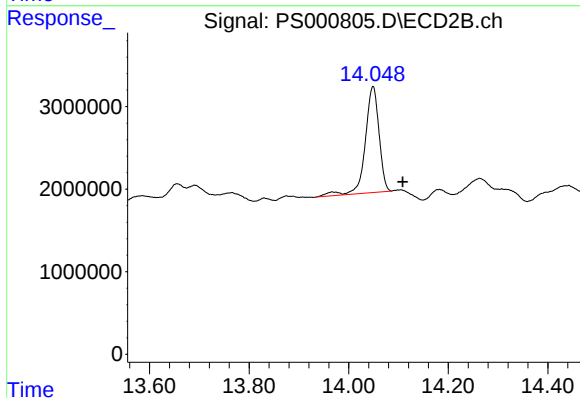


#11 2,4,5-TP (SILVEX)

R.T.: 14.049 min
Delta R.T.: -0.060 min
Response: 24787356
Conc: 16.89 ng/ml

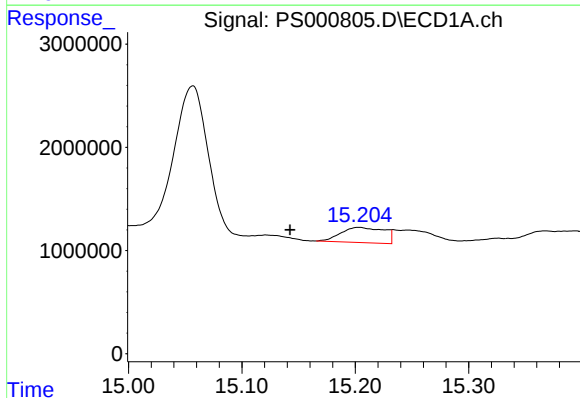


#12 2,4,5-T

R.T.: 15.203 min
Delta R.T.: 0.061 min
Response: 3860619
Conc: 2.44 ng/ml

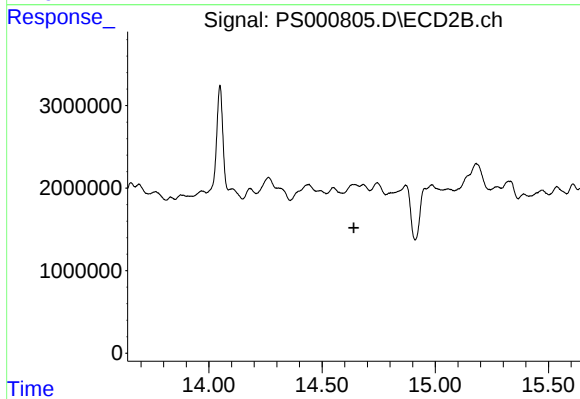

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.641 min
Response: 0
Conc: N.D.

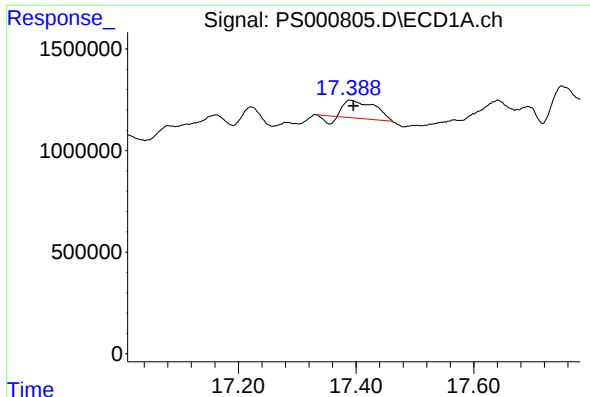

#14 DINOSEB


R.T.: 17.390 min
Delta R.T.: -0.005 min
Response: 2790951
Conc: 3.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

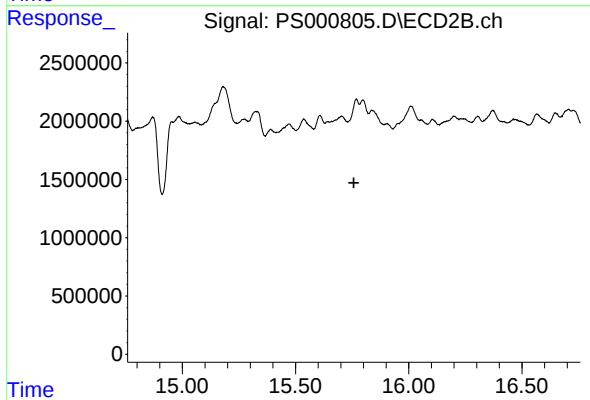


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.758 min
Response: 0
Conc: N.D.

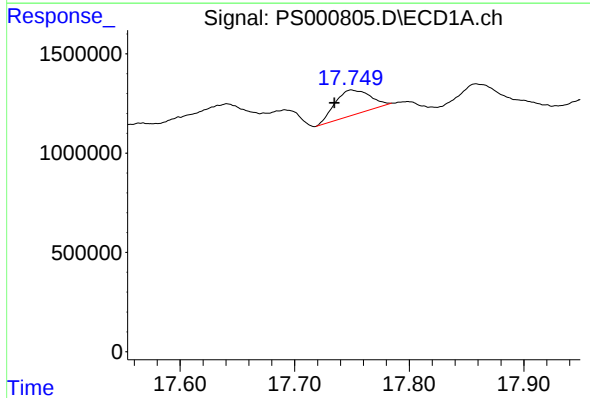

#16 DCPA

R.T.: 17.750 min
Delta R.T.: 0.015 min
Response: 2676845
Conc: 1.91 ng/ml

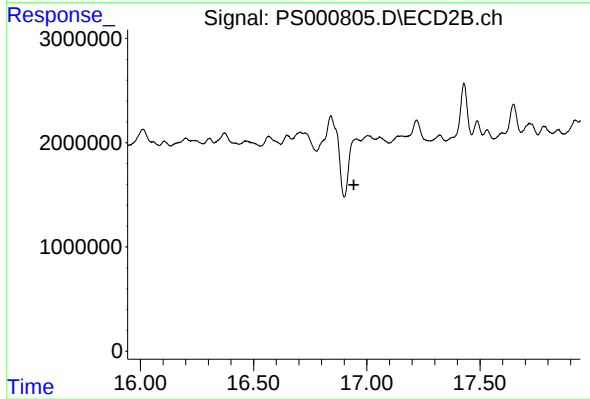

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.943 min
Response: 0
Conc: N.D.