

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070618\
 Data File : PS000798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2018 16:28
 Operator : UA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 19:01:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070618.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 06 18:59:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.621	11.055	278.2E6	188.5E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.018	2.437	304.8E6	225.3E6	682.500	682.500
2) T	3,5-DICHL...	10.038	9.201	368.2E6	243.1E6	697.500	697.500
3) T	4-Nitroph...	11.213	10.200	149.5E6	95983262	682.500	682.500
5) T	DICAMBA	11.937	11.342	966.0E6	670.9E6	705.000	705.000
6) T	MCPD	12.278	11.569	83732115	48188956	70.500	70.500
7) T	MCPA	12.528	11.946	126.8E6	69916488	69.750	69.750
8) T	DICHLORPROP	13.129	12.467	255.7E6	168.3E6	705.000	705.000
9) T	2,4-D	13.486	12.938	327.2E6	232.2E6	705.000	705.000
10) T	Pentachlo...	13.875	13.495	3282.3E6	2669.5E6	712.500	712.500
11) T	2,4,5-TP ...	14.746	14.109	1330.5E6	1084.1E6	712.500	712.500
12) T	2,4,5-T	15.142	14.641	1219.5E6	1066.7E6	712.500	712.500
13) T	2,4-DB	15.893	15.326	131.3E6	123.9E6	712.500	712.500
14) T	DINOSEB	17.395	15.758	515.0E6	711.6E6	705.000	705.000
15) T	Picloram	17.152	16.999	1022.8E6	1520.5E6	712.500	712.500
16) T	DCPA	17.735	16.943	1046.9E6	1300.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070618\
Data File : PS000798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2018 16:28
Operator : UA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 19:01:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070618.M
Quant Title : 8080.M
QLast Update : Fri Jul 06 18:59:57 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

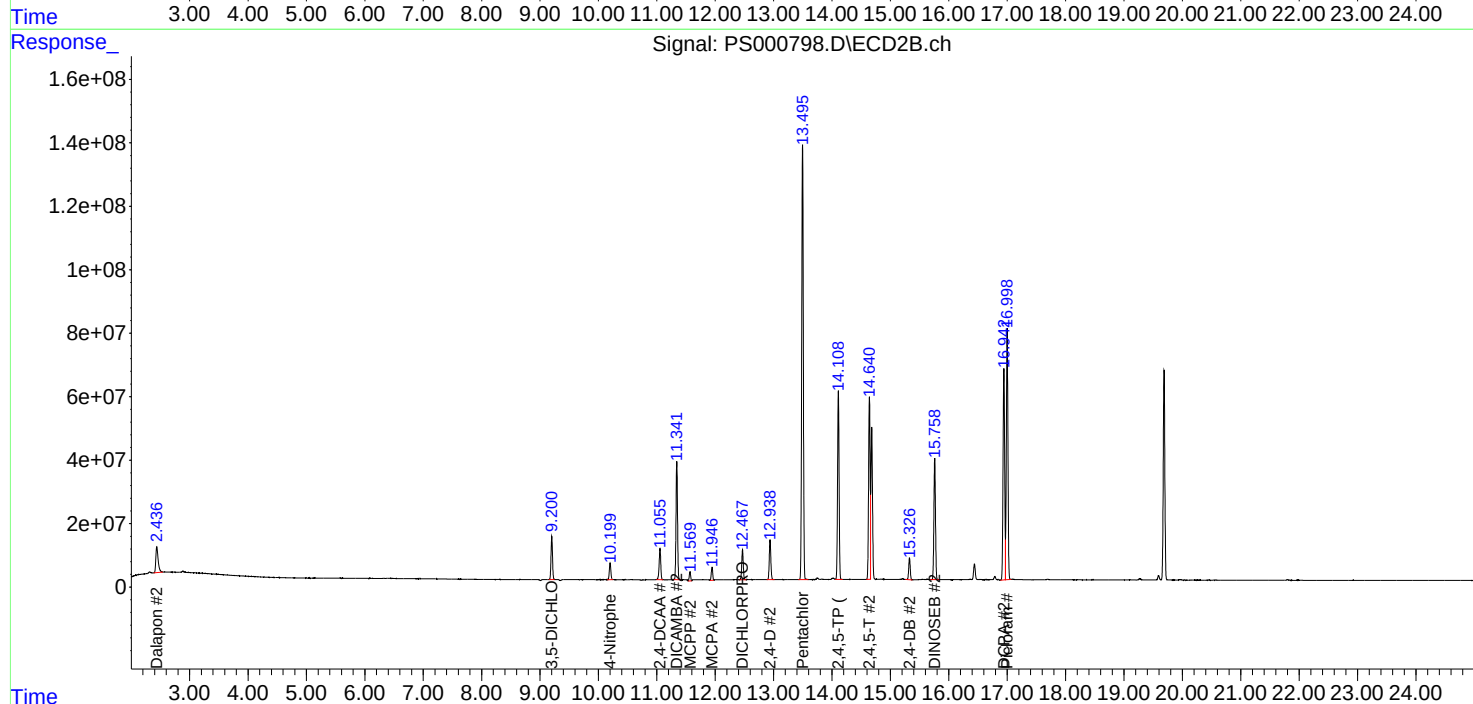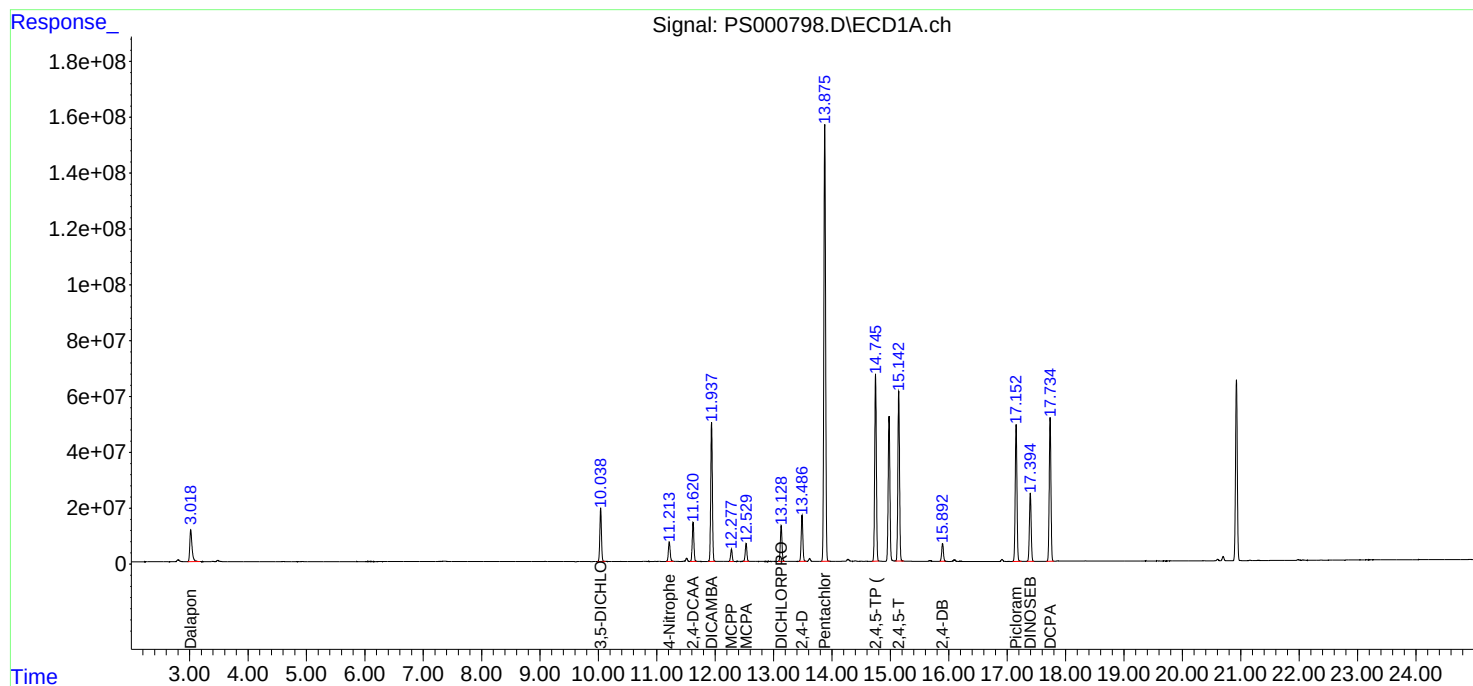


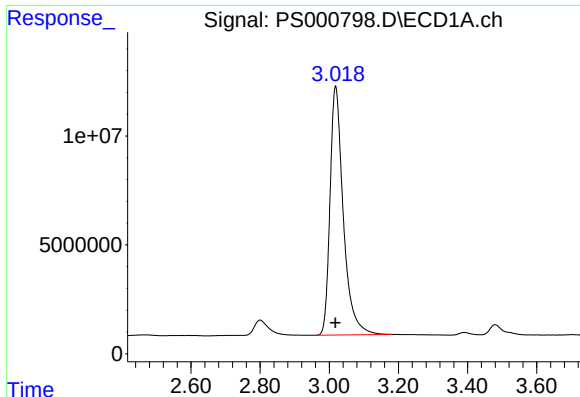

#1 Dalapon


R.T.: 3.018 min
Delta R.T.: 0.000 min
Response: 304826466
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

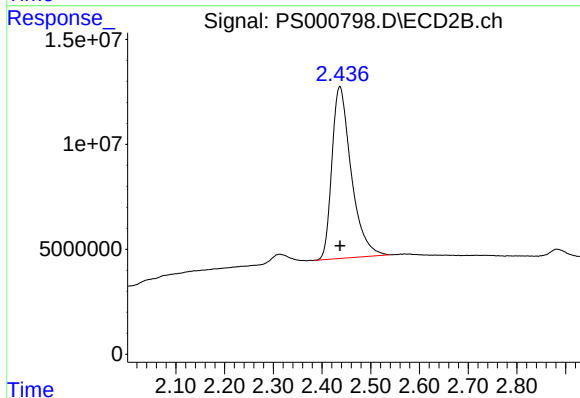


#1 Dalapon

R.T.: 2.437 min
Delta R.T.: 0.000 min
Response: 225259709
Conc: 682.50 ng/ml

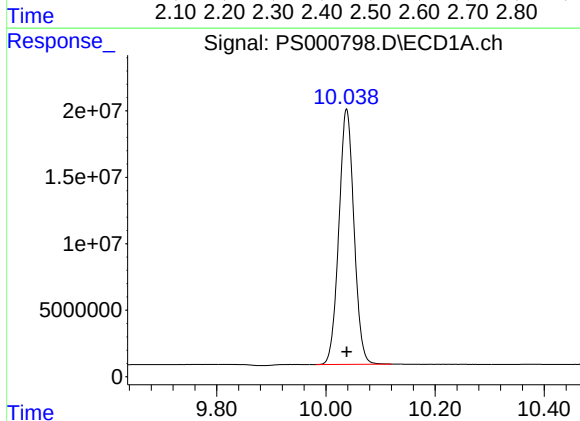


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.038 min
Delta R.T.: 0.000 min
Response: 368222598
Conc: 697.50 ng/ml

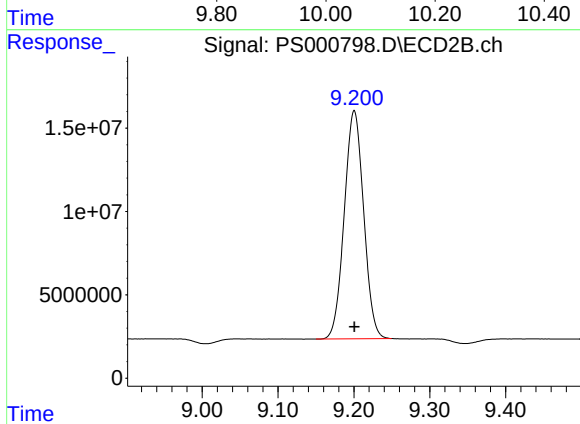

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 243147036
Conc: 697.50 ng/ml

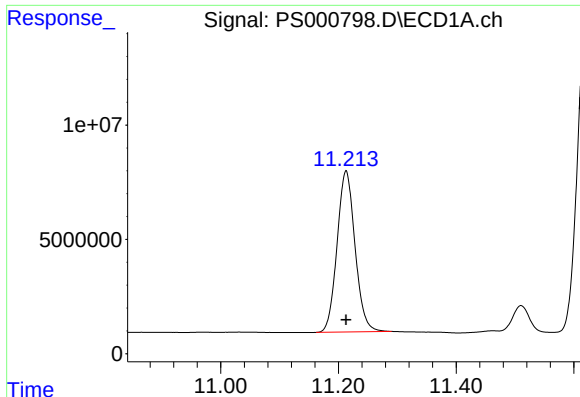

#3 4-Nitrophenol


R.T.: 11.213 min
Delta R.T.: 0.000 min
Response: 149459244
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

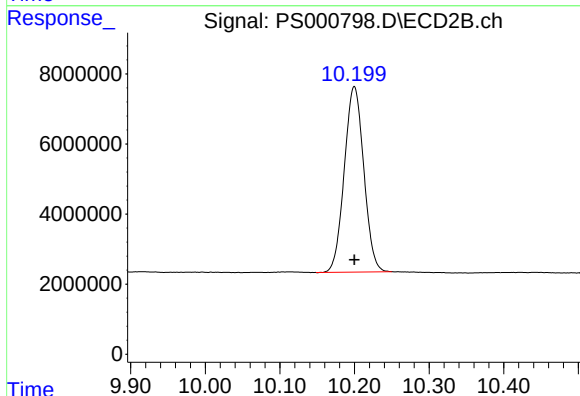


#3 4-Nitrophenol

R.T.: 10.200 min
Delta R.T.: 0.000 min
Response: 95983262
Conc: 682.50 ng/ml

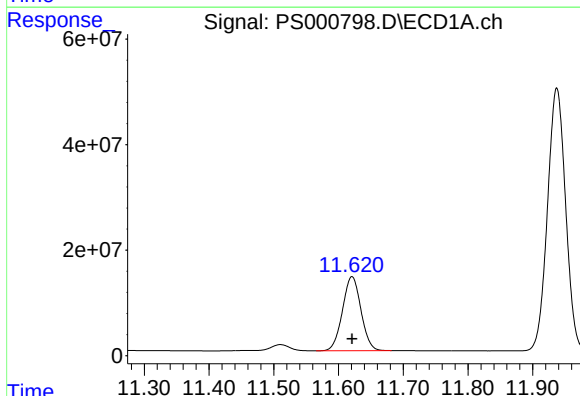


#4 2,4-DCAA

R.T.: 11.621 min
Delta R.T.: 0.000 min
Response: 278200821
Conc: 750.00 ng/ml

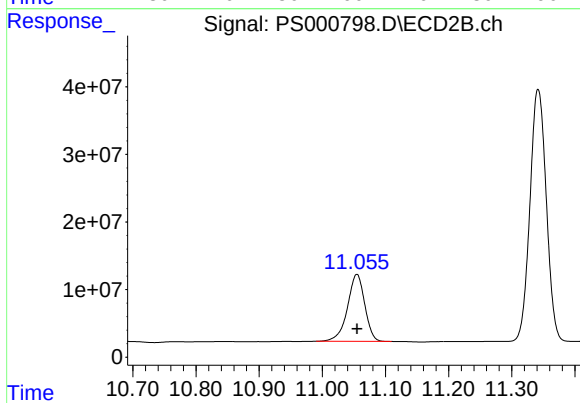

#4 2,4-DCAA


R.T.: 11.055 min
Delta R.T.: 0.000 min
Response: 188496053
Conc: 750.00 ng/ml

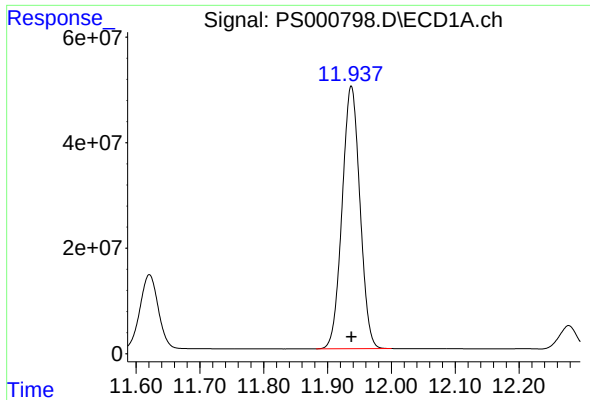

#5 DICAMBA


R.T.: 11.937 min
Delta R.T.: 0.000 min
Response: 966038569
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

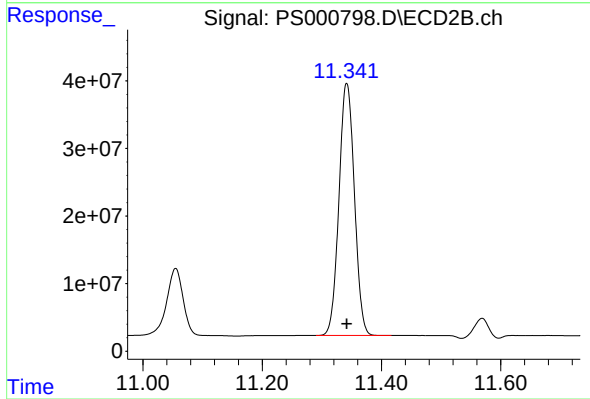


#5 DICAMBA

R.T.: 11.342 min
Delta R.T.: 0.000 min
Response: 670942747
Conc: 705.00 ng/ml

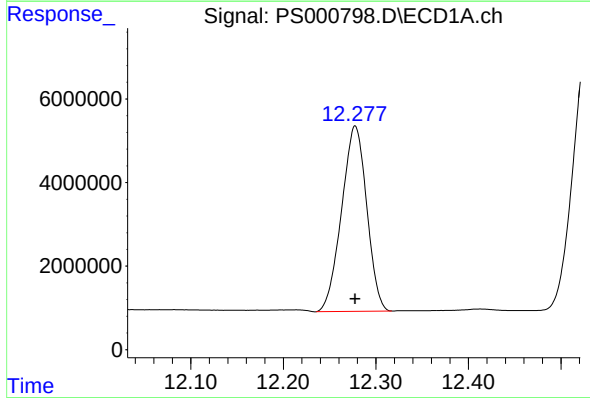


#6 MCP

R.T.: 12.278 min
Delta R.T.: 0.000 min
Response: 83732115
Conc: 70.50 ug/ml

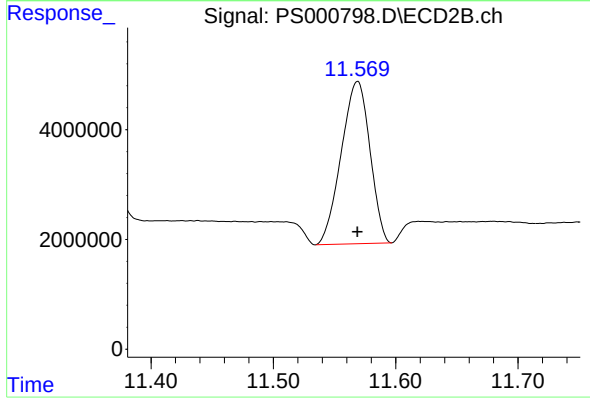

#6 MCP


R.T.: 11.569 min
Delta R.T.: 0.000 min
Response: 48188956
Conc: 70.50 ug/ml

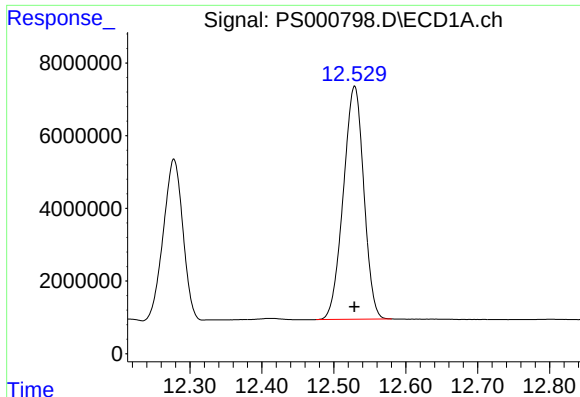

#7 MCPA


R.T.: 12.528 min
Delta R.T.: 0.000 min
Response: 126802704
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

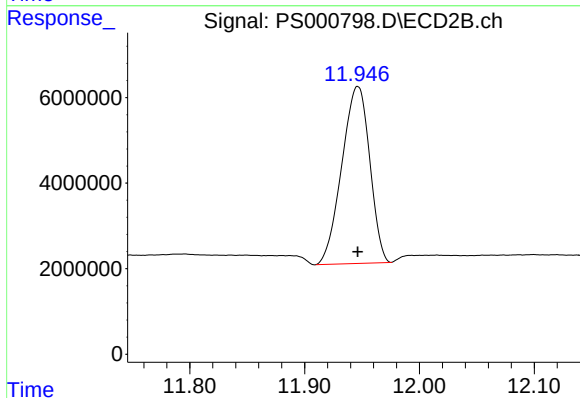


#7 MCPA

R.T.: 11.946 min
Delta R.T.: 0.000 min
Response: 69916488
Conc: 69.75 ug/ml

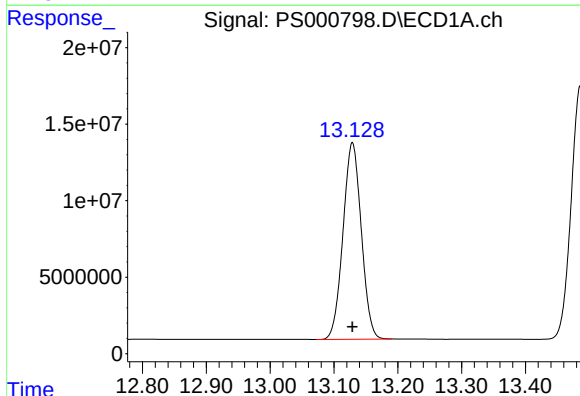


#8 DICHLORPROP

R.T.: 13.129 min
Delta R.T.: 0.000 min
Response: 255721105
Conc: 705.00 ng/ml

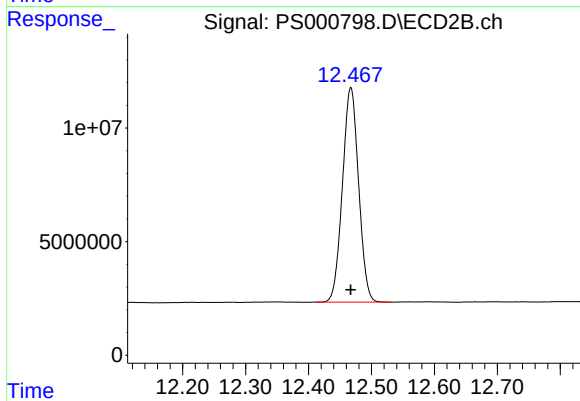

#8 DICHLORPROP


R.T.: 12.467 min
Delta R.T.: 0.000 min
Response: 168310647
Conc: 705.00 ng/ml

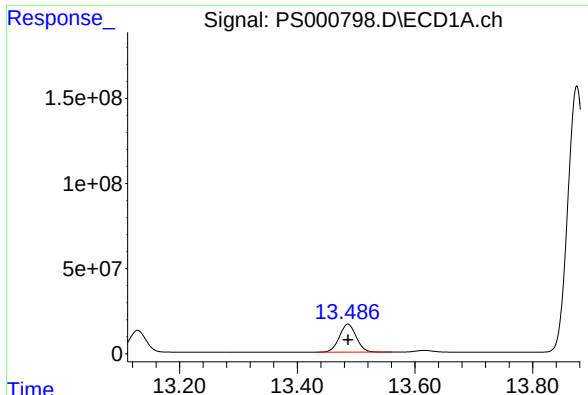

#9 2,4-D


R.T.: 13.486 min
Delta R.T.: 0.000 min
Response: 327179954
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

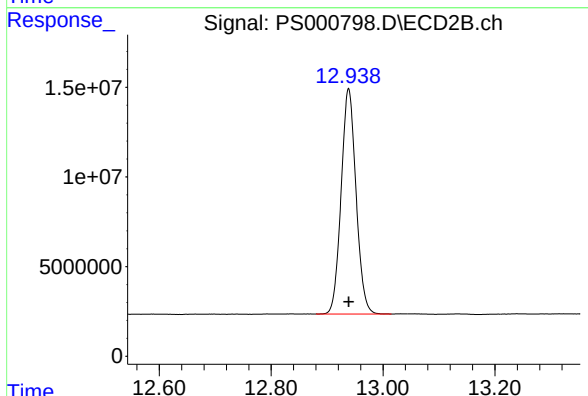


#9 2,4-D

R.T.: 12.938 min
Delta R.T.: 0.000 min
Response: 232223560
Conc: 705.00 ng/ml

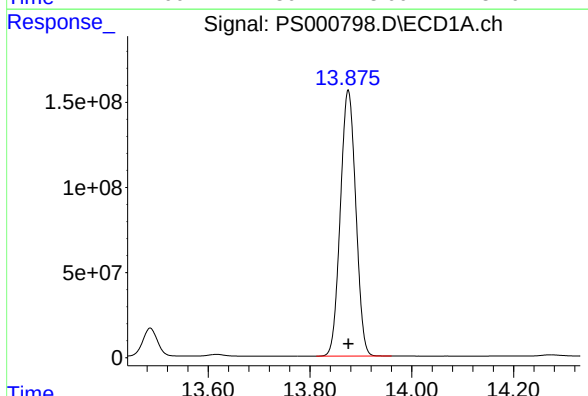


#10 Pentachlorophenol

R.T.: 13.875 min
Delta R.T.: 0.000 min
Response: 3282270461
Conc: 712.50 ng/ml

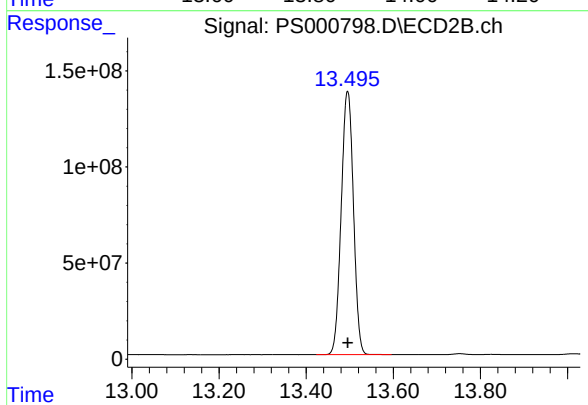

#10 Pentachlorophenol


R.T.: 13.495 min
Delta R.T.: 0.000 min
Response: 2669494990
Conc: 712.50 ng/ml

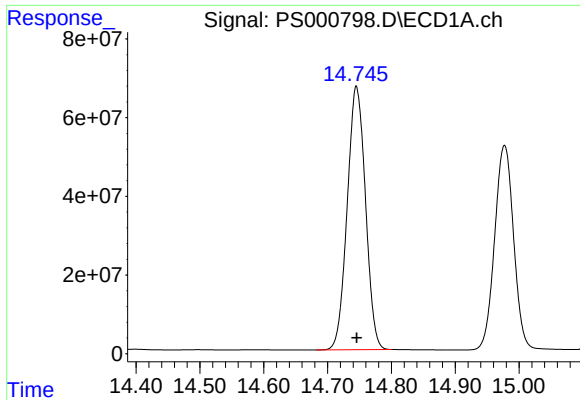

#11 2,4,5-TP (SILVEX)


R.T.: 14.746 min
Delta R.T.: 0.000 min
Response: 1330518344
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

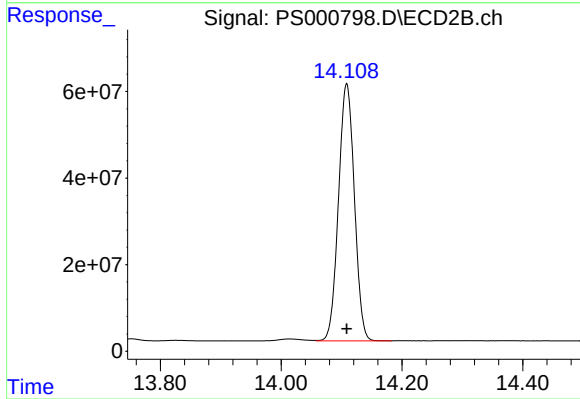


#11 2,4,5-TP (SILVEX)

R.T.: 14.109 min
Delta R.T.: 0.000 min
Response: 1084137914
Conc: 712.50 ng/ml

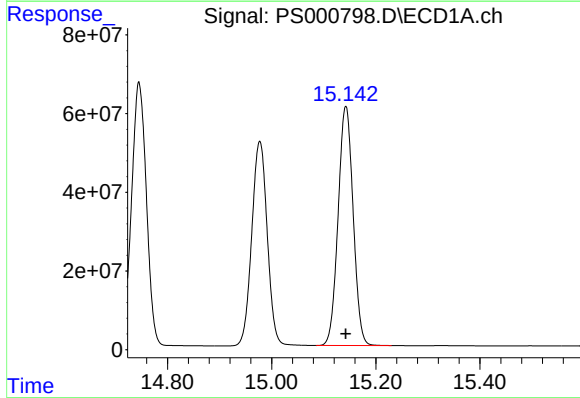


#12 2,4,5-T

R.T.: 15.142 min
Delta R.T.: 0.000 min
Response: 1219465744
Conc: 712.50 ng/ml

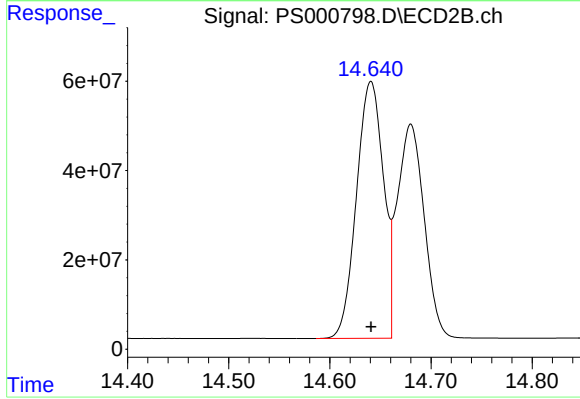

#12 2,4,5-T


R.T.: 14.641 min
Delta R.T.: 0.000 min
Response: 1066691280
Conc: 712.50 ng/ml

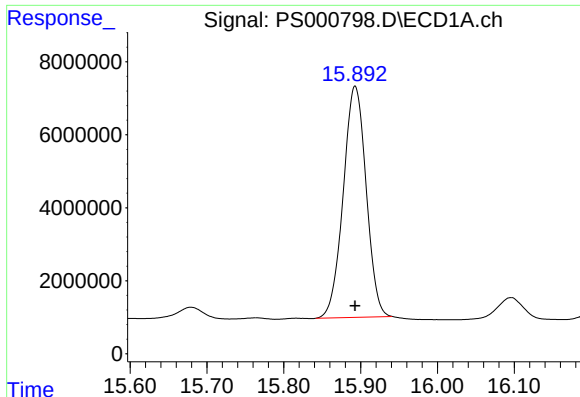

#13 2,4-DB


R.T.: 15.893 min
Delta R.T.: 0.000 min
Response: 131257786
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

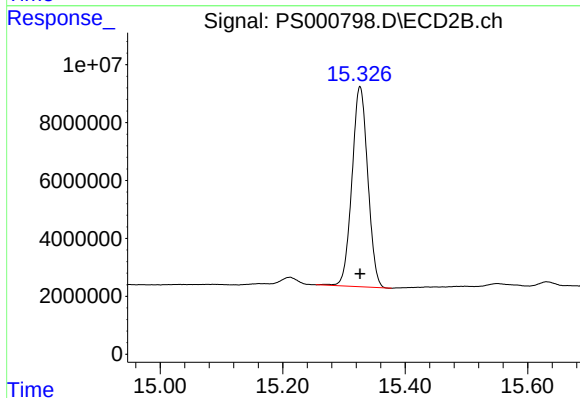


#13 2,4-DB

R.T.: 15.326 min
Delta R.T.: 0.000 min
Response: 123916389
Conc: 712.50 ng/ml

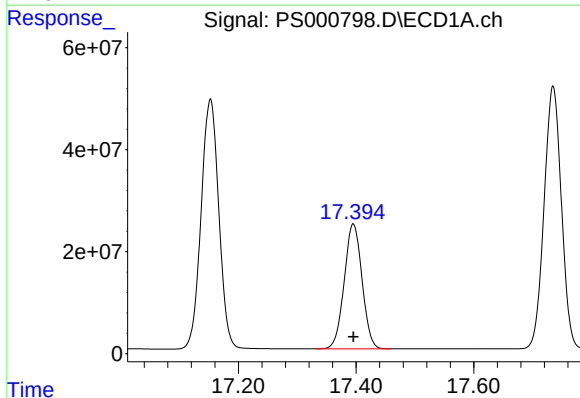


#14 DINOSEB

R.T.: 17.395 min
Delta R.T.: 0.000 min
Response: 514955141
Conc: 705.00 ng/ml

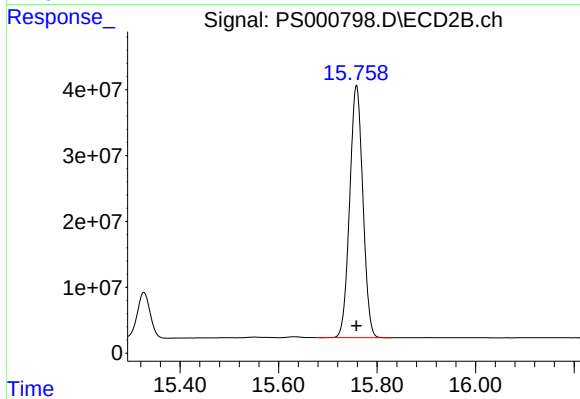

#14 DINOSEB


R.T.: 15.758 min
Delta R.T.: 0.000 min
Response: 711640091
Conc: 705.00 ng/ml

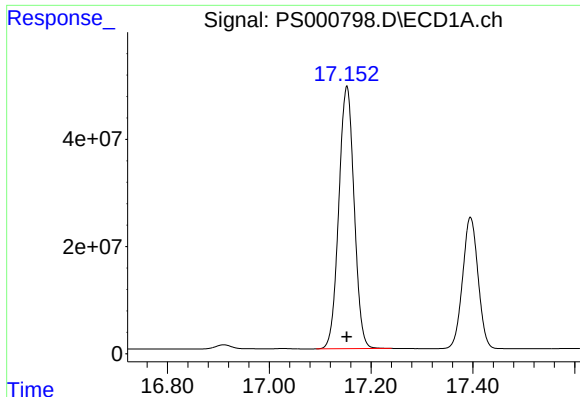

#15 Picloram


R.T.: 17.152 min
Delta R.T.: 0.000 min
Response: 1022843773
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

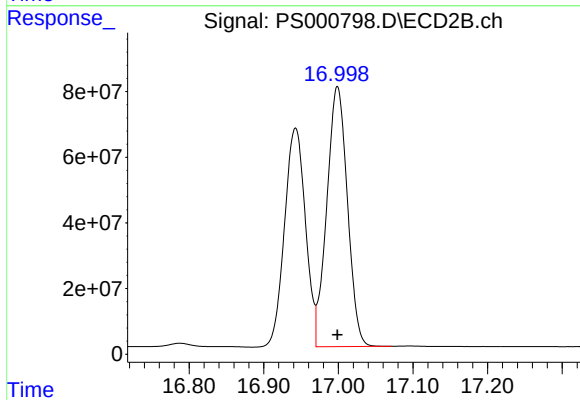


#15 Picloram

R.T.: 16.999 min
Delta R.T.: 0.000 min
Response: 1520502992
Conc: 712.50 ng/ml

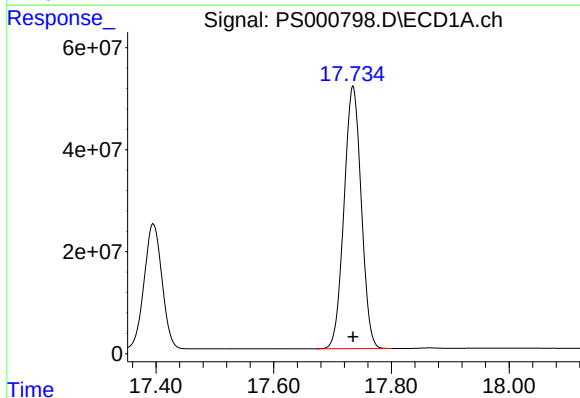

#16 DCPA

R.T.: 17.735 min
Delta R.T.: 0.000 min
Response: 1046866279
Conc: 720.00 ng/ml

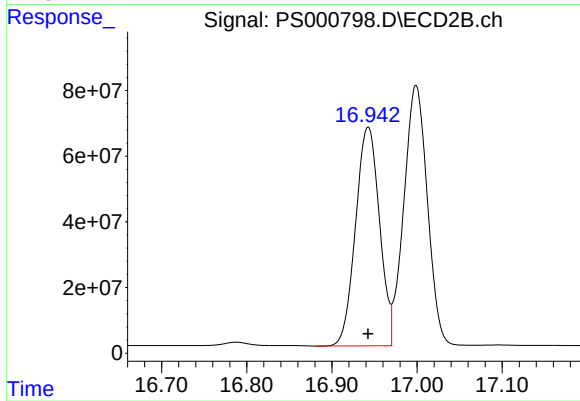

#16 DCPA

R.T.: 16.943 min
Delta R.T.: 0.000 min
Response: 1300862149
Conc: 720.00 ng/ml