

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070620\
 Data File : PS011097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2020 16:15
 Operator : DD\AJ
 Sample : L3188-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 18:53:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	424.6E6	265.5E6	468.221	479.153
Target Compounds							
1) T	Dalapon	2.994	2.583	30812855	37676293	27.518	49.945 #
2) T	3,5-DICHL...	6.508	6.100	7194609	53269077	5.719	63.962 #
6) T	MCP	7.583	7.123	8401360	-3695450	2.946	N.D. #
7) T	MCPA	7.740	7.383	27661295	24087122	6.946	8.727 #
8) T	DICHLORPROP	0.000	7.666	0	3176956	N.D.	5.411
10) T	Pentachlo...	8.713	8.469	14466817	9051213	1.163	1.302
12) T	2,4,5-T	9.509	0.000	4573715	0	<MDL	N.D. #
14) T	DINOSEB	11.168	10.033	58103463	32301458	16.223	15.514
15) T	Picloram	10.990	11.002	99360246	13803168	17.723	3.295 #
16) T	DCPA	0.000	11.002	0	13803168	N.D.	3.706



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070620\
Data File : PS011097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2020 16:15
Operator : DD\AJ
Sample : L3188-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 18:53:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

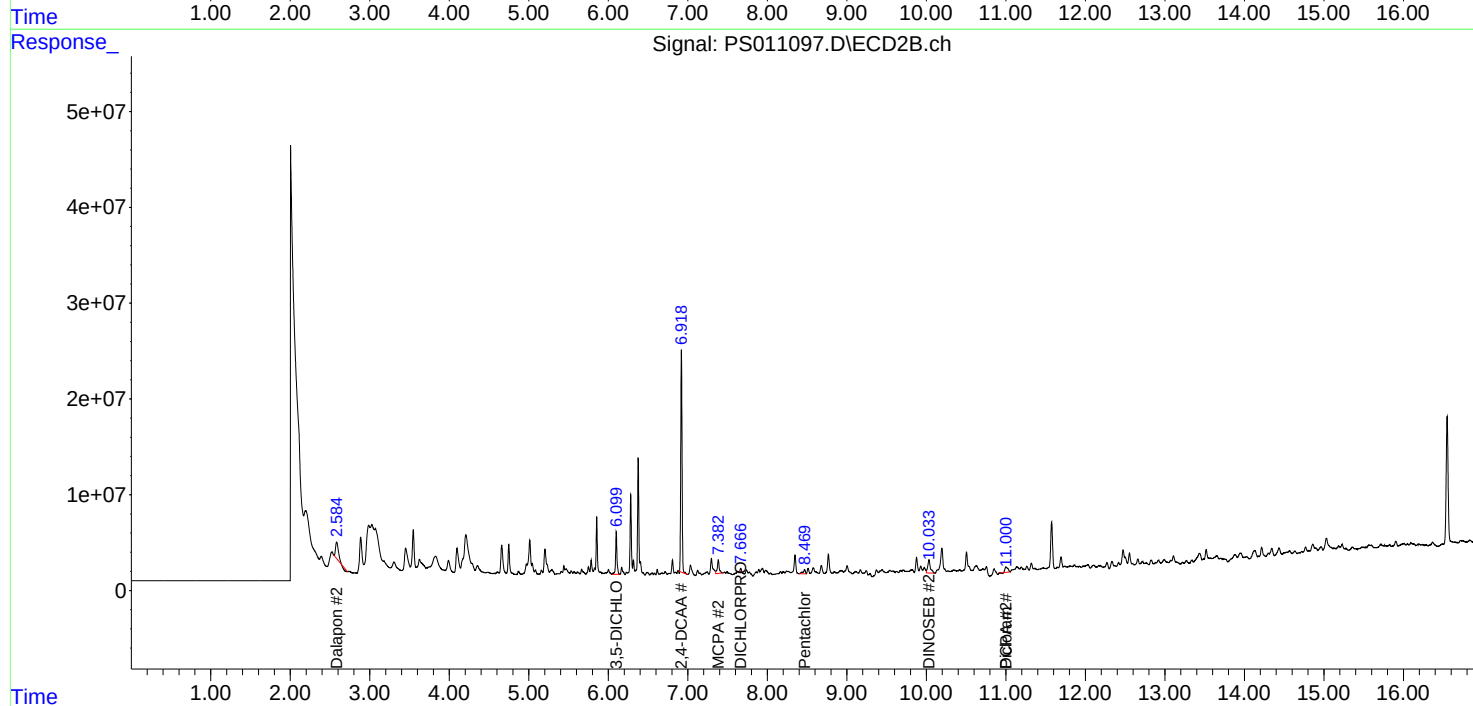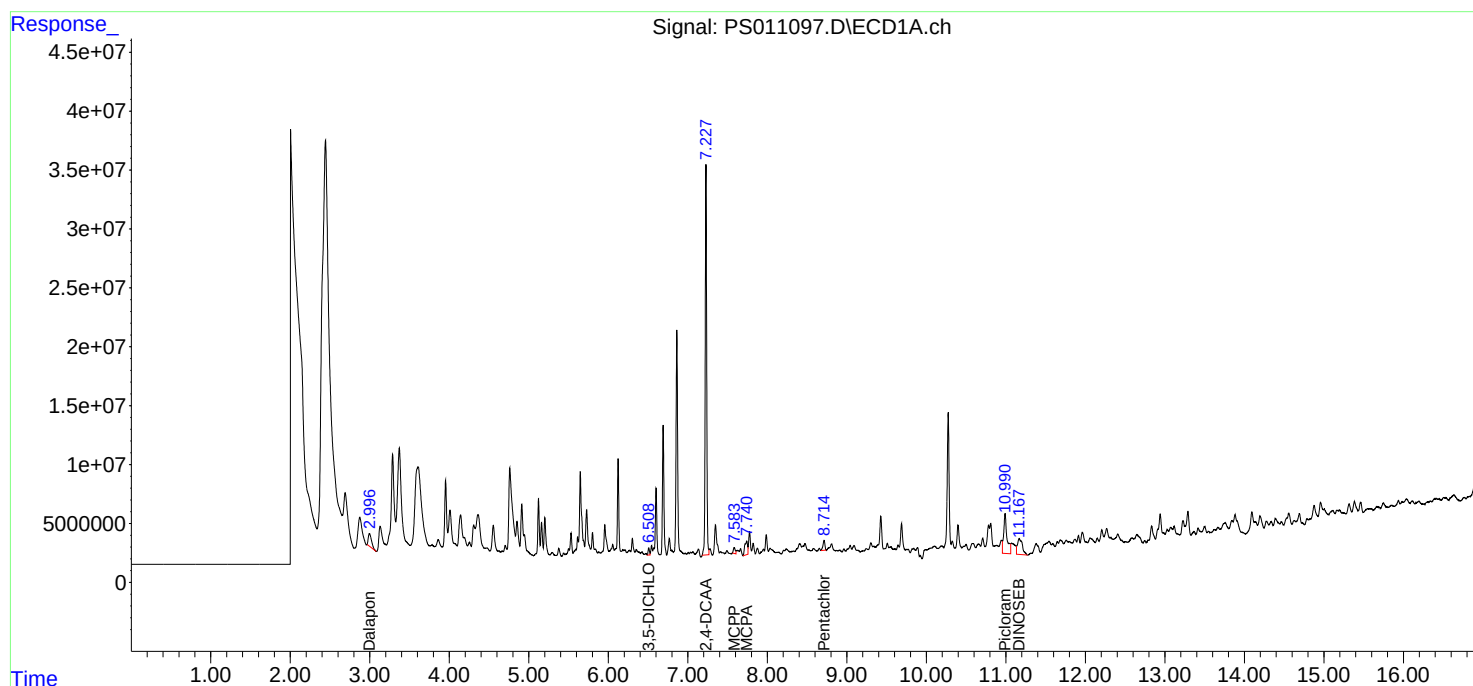


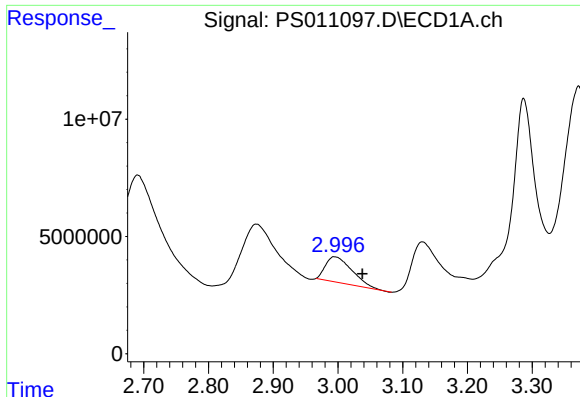

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.044 min
Response: 30812855
Conc: 27.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

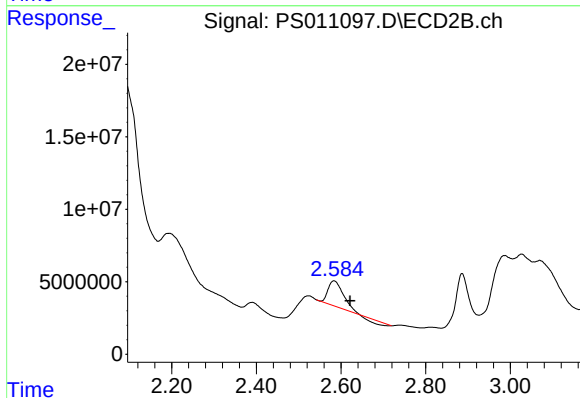


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: -0.038 min
Response: 37676293
Conc: 49.94 ng/ml

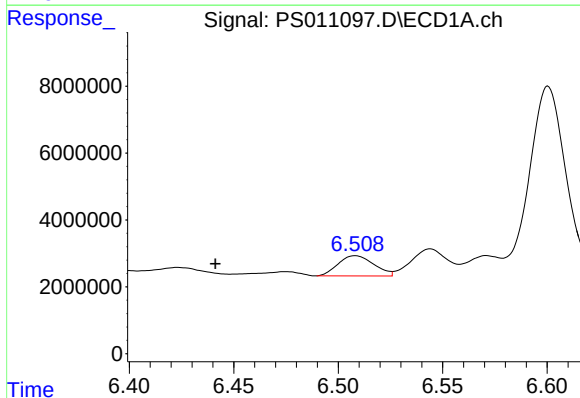


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.508 min
Delta R.T.: 0.067 min
Response: 7194609
Conc: 5.72 ng/ml

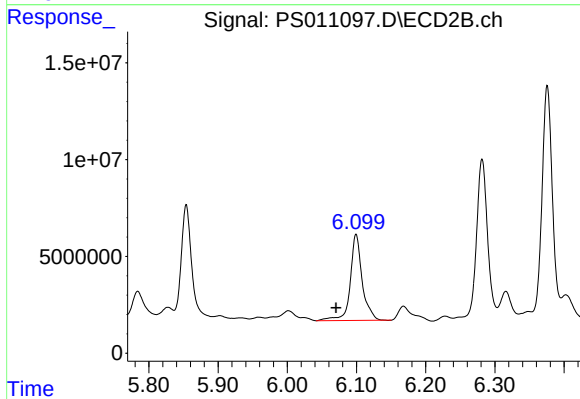

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 53269077
Conc: 63.96 ng/ml

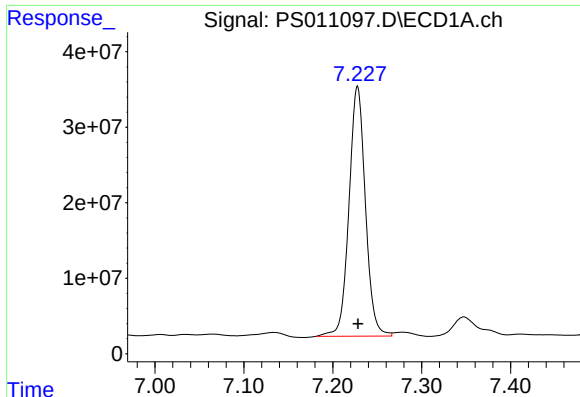

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 424591700
Conc: 468.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

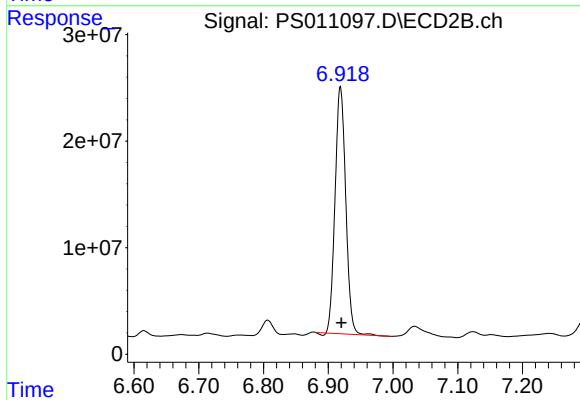


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.002 min
Response: 265487479
Conc: 479.15 ng/ml

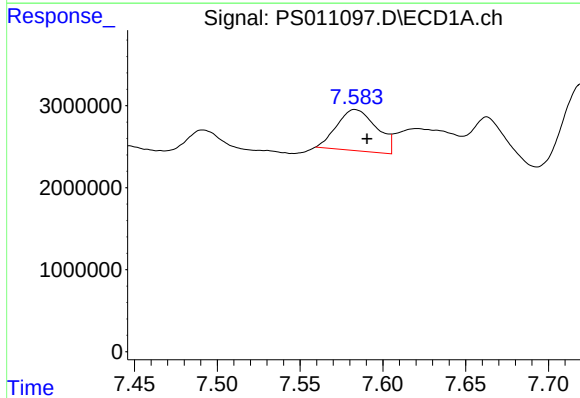


#6 MCP

R.T.: 7.583 min
Delta R.T.: -0.007 min
Response: 8401360
Conc: 2.95 ug/ml

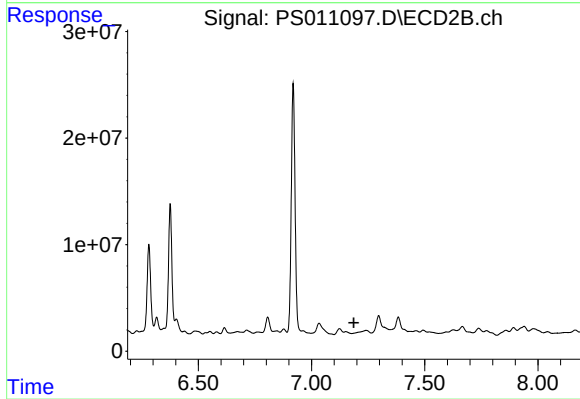

#6 MCP


R.T.: 7.123 min
Delta R.T.: -0.063 min
Response: -3695450
Conc: N.D.

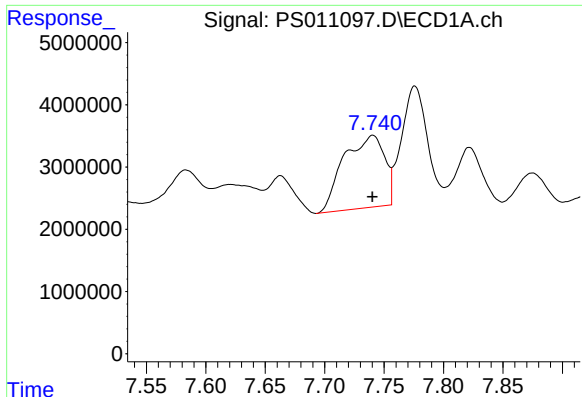

#7 MCPA


R.T.: 7.740 min
Delta R.T.: 0.000 min
Response: 27661295
Conc: 6.95 ug/ml

Instrument :
ECD_S
ClientSampleId :

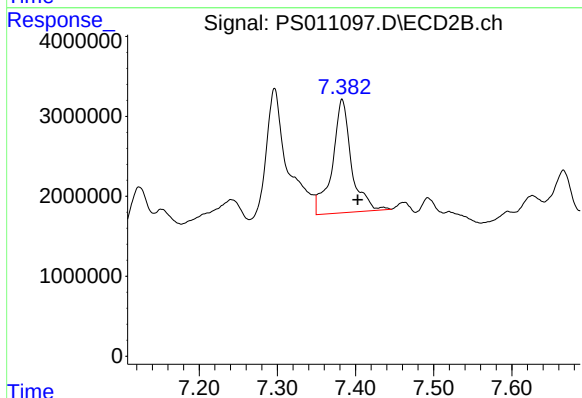


#7 MCPA

R.T.: 7.383 min
Delta R.T.: -0.020 min
Response: 24087122
Conc: 8.73 ug/ml

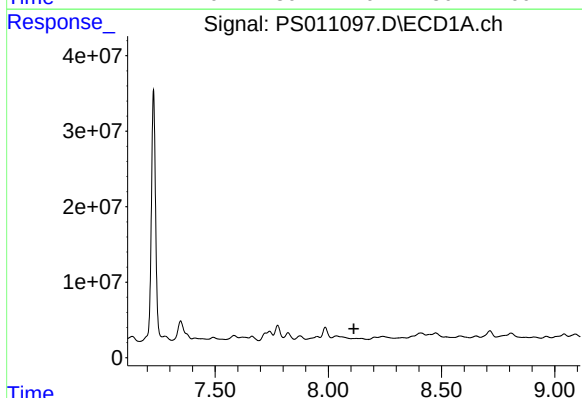


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

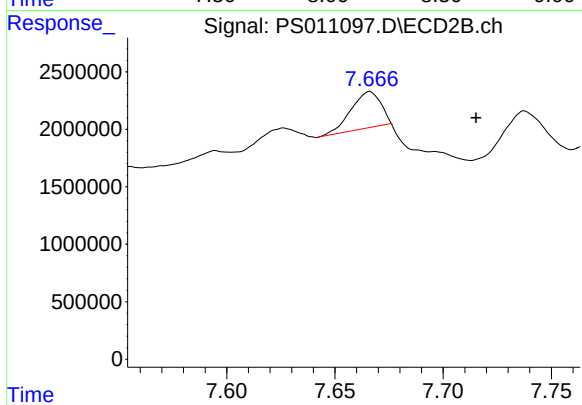

#8 DICHLORPROP


R.T.: 7.666 min
Delta R.T.: -0.049 min
Response: 3176956
Conc: 5.41 ng/ml

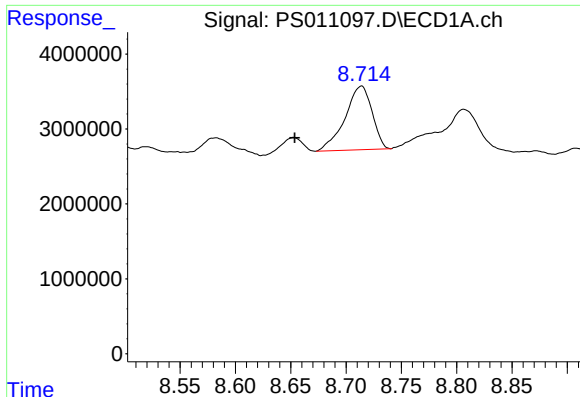

#10 Pentachlorophenol


R.T.: 8.713 min
Delta R.T.: 0.060 min
Response: 14466817
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

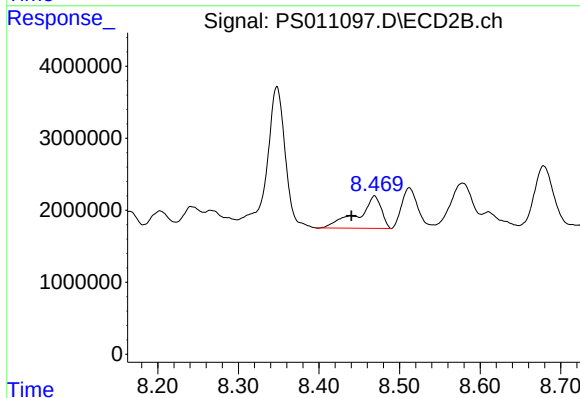


#10 Pentachlorophenol

R.T.: 8.469 min
Delta R.T.: 0.029 min
Response: 9051213
Conc: 1.30 ng/ml

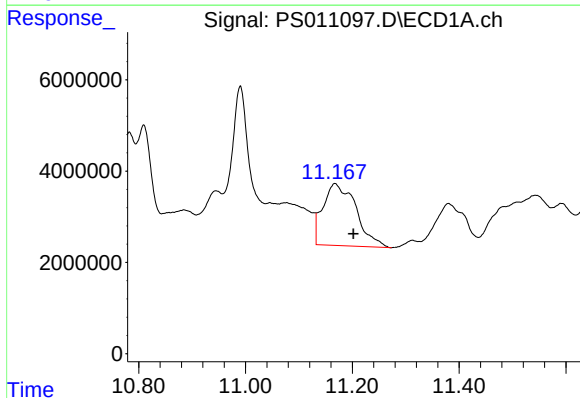


#14 DINOSEB

R.T.: 11.168 min
Delta R.T.: -0.035 min
Response: 58103463
Conc: 16.22 ng/ml

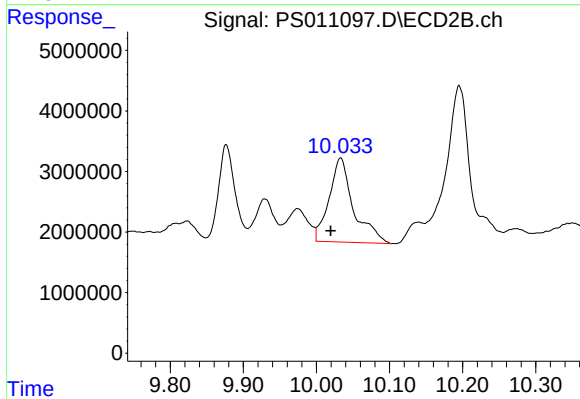

#14 DINOSEB


R.T.: 10.033 min
Delta R.T.: 0.013 min
Response: 32301458
Conc: 15.51 ng/ml

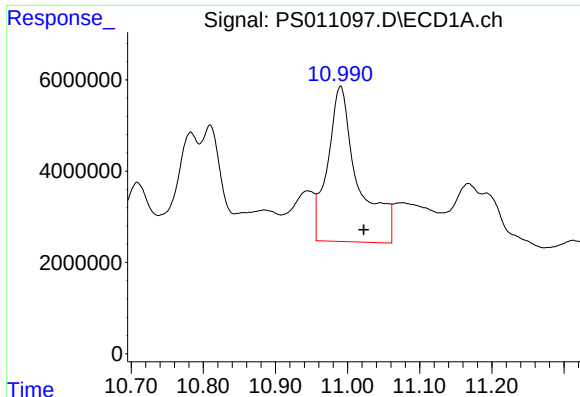

#15 Picloram


R.T.: 10.990 min
Delta R.T.: -0.032 min
Response: 99360246
Conc: 17.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

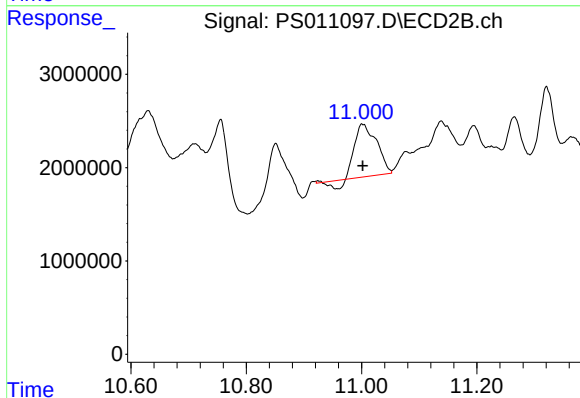


#15 Picloram

R.T.: 11.002 min
Delta R.T.: 0.000 min
Response: 13803168
Conc: 3.29 ng/ml

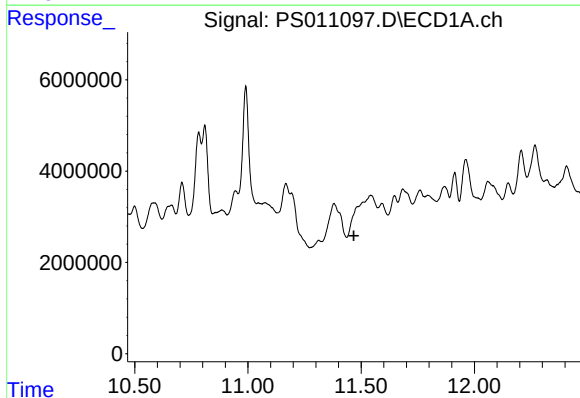

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

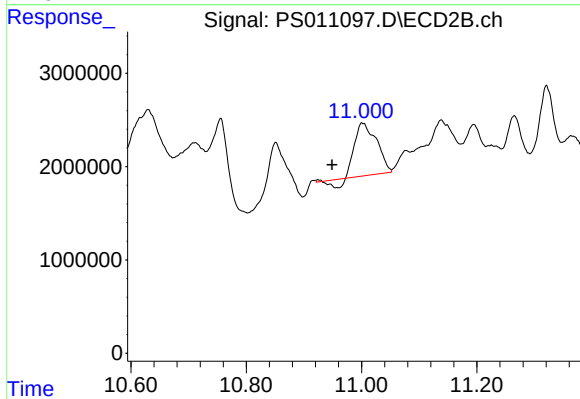

#16 DCPA

R.T.: 11.002 min
Delta R.T.: 0.053 min
Response: 13803168
Conc: 3.71 ng/ml