

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070622\
 Data File : PS019890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jul 2022 09:16
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 03:45:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.770	0	619468	N.D.	<MDL
Target Compounds							
1) T	Dalapon	3.014	0.000	226546	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.371	5.956	286739	226709	<MDL	<MDL #
3) T	4-Nitroph...	6.987	6.409	868329	125525	<MDL	<MDL #
5) T	DICAMBA	7.394	6.942	36725850	1244864	3.579	<MDL #
6) T	MCPD	7.542	7.036	668432	1397179	<MDL	<MDL #
7) T	MCPA	7.688	0.000	1305717	0	<MDL	N.D. #
8) T	DICHLORPROP	8.099	0.000	6387236	0	2.359	N.D. #
9) T	2,4-D	8.297	7.787f	18751098	135744	6.313	<MDL #
13) T	2,4-DB	9.979	9.500	86307679	107694	21.568	<MDL #
14) T	DINOSEB	0.000	9.851	0	3972354	N.D.	1.115
15) T	Picloram	10.967	10.887f	55712099	49493973	1.787	7.610 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070622\
Data File : PS019890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jul 2022 09:16
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 03:45:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

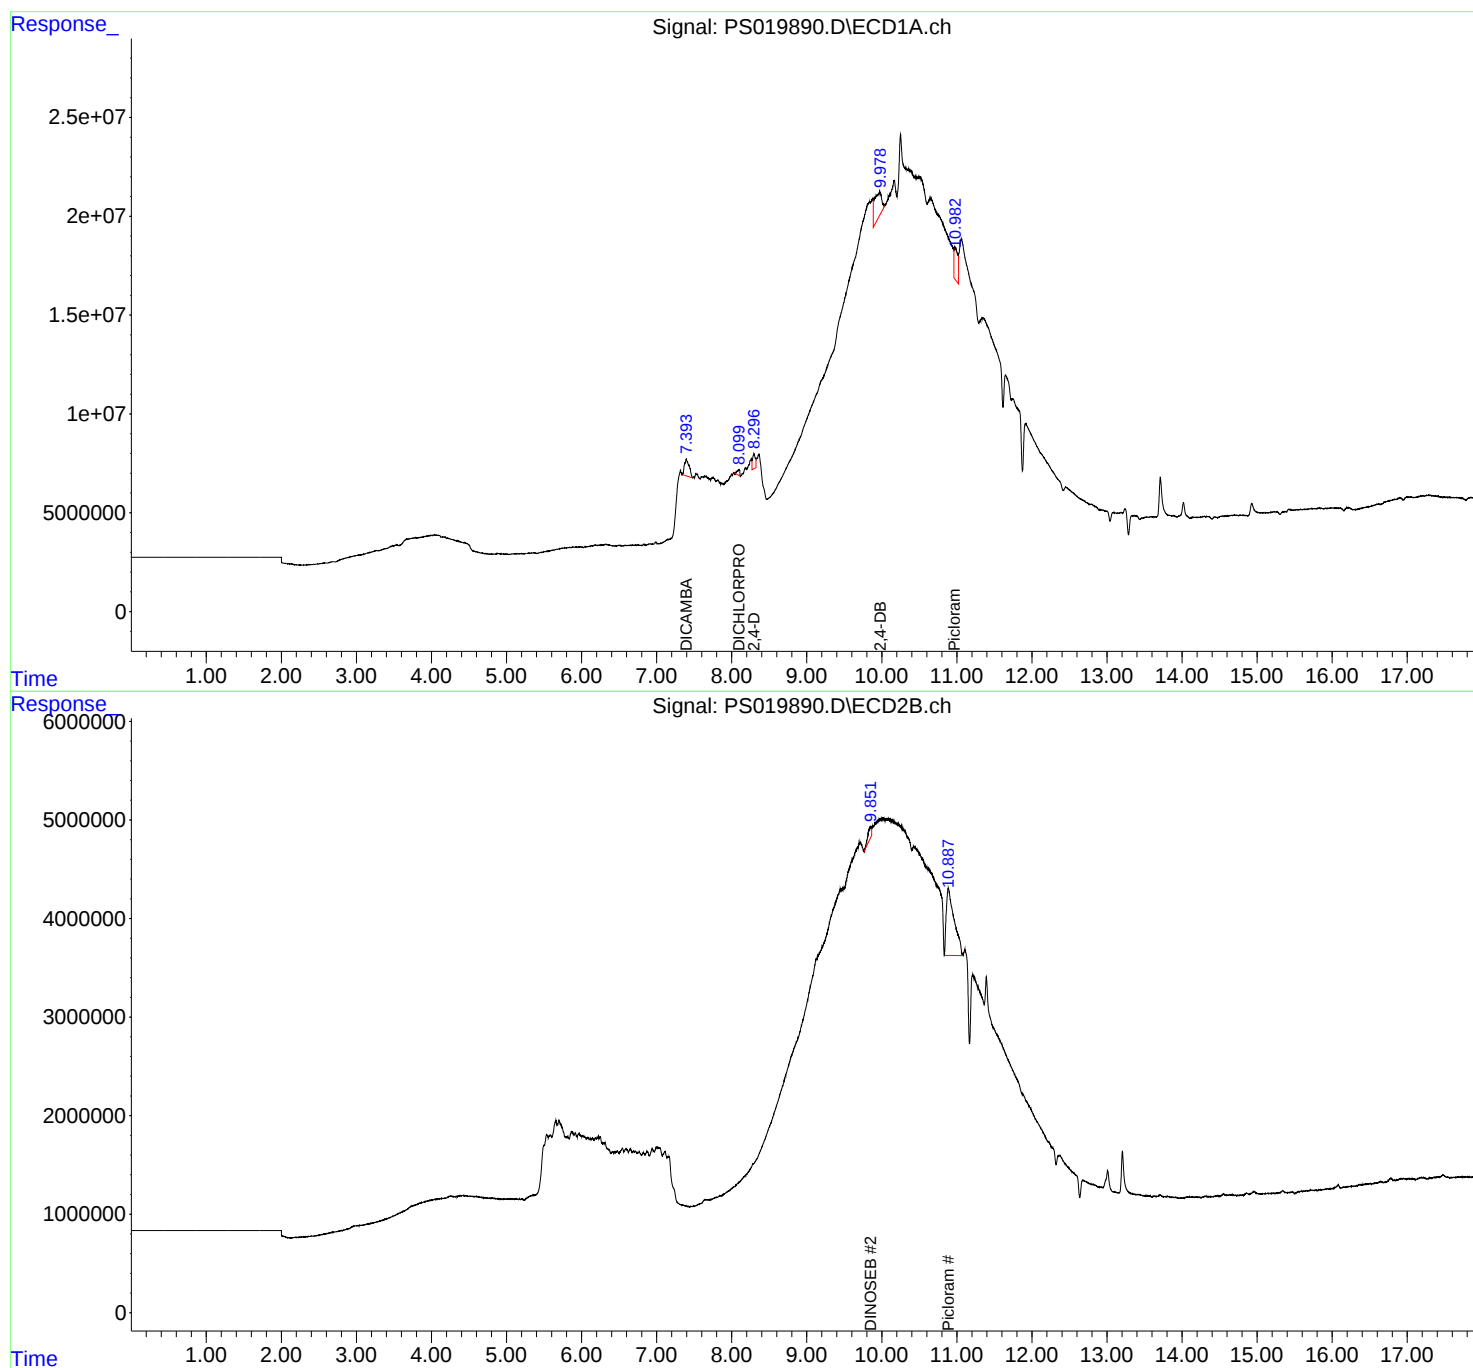


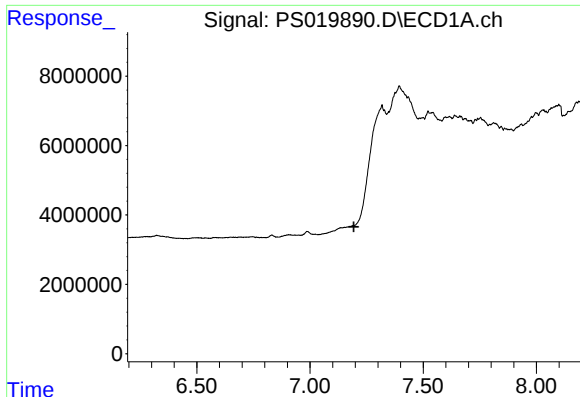

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.194 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

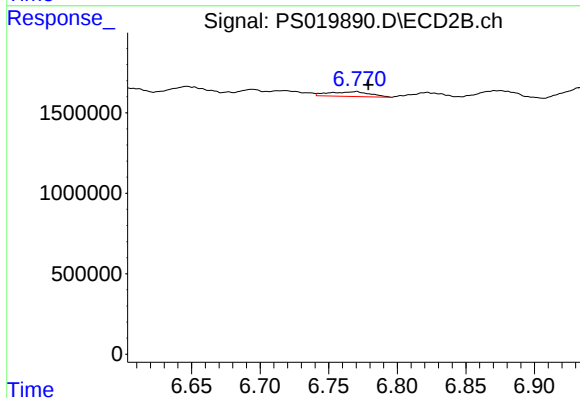


#4 2,4-DCAA

R.T.: 6.770 min
Delta R.T.: -0.009 min
Response: 619468
Conc: N.D.

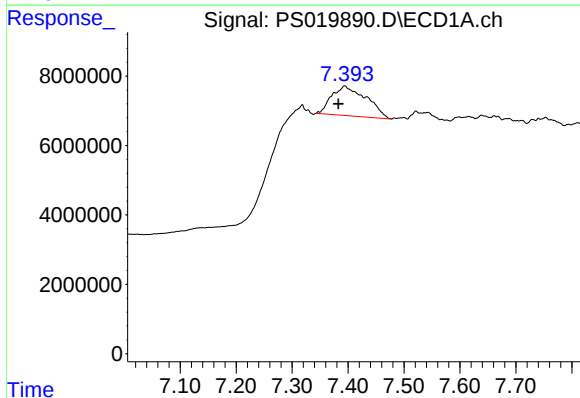


#5 DICAMBA

R.T.: 7.394 min
Delta R.T.: 0.011 min
Response: 36725850
Conc: 3.58 ng/ml

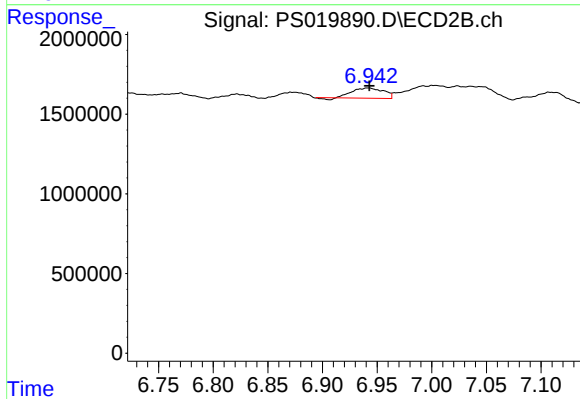

#5 DICAMBA


R.T.: 6.942 min
Delta R.T.: -0.001 min
Response: 1244864
Conc: N.D.

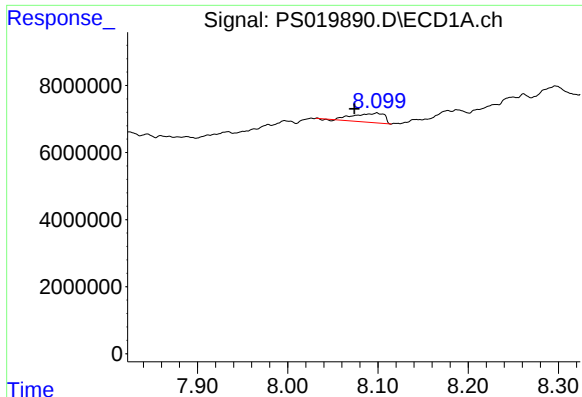

#8 DICHLORPROP


R.T.: 8.099 min
Delta R.T.: 0.025 min
Response: 6387236
Conc: 2.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

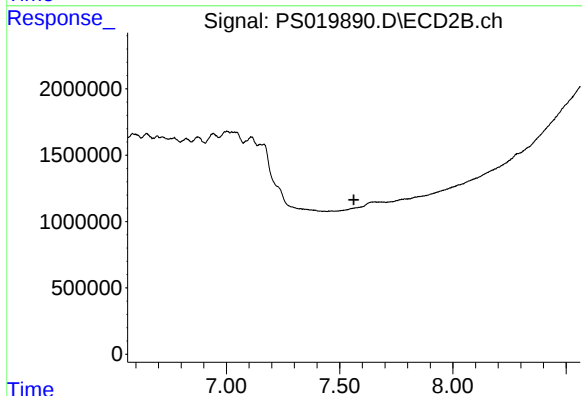


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.563 min
Response: 0
Conc: N.D.

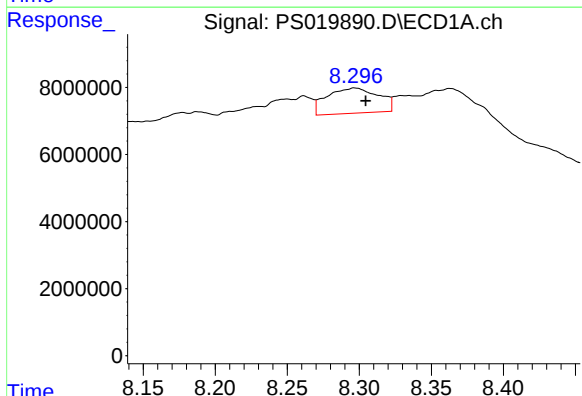


#9 2,4-D

R.T.: 8.297 min
Delta R.T.: -0.008 min
Response: 18751098
Conc: 6.31 ng/ml

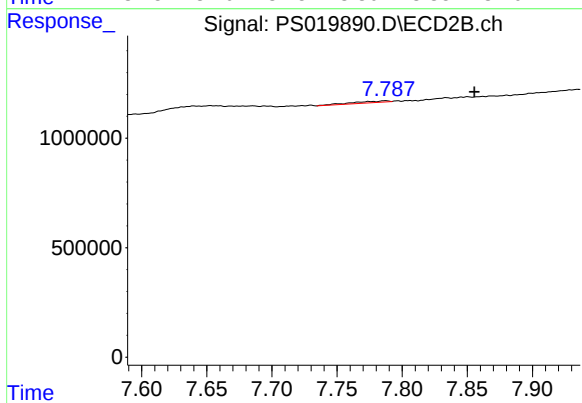

#9 2,4-D


R.T.: 7.787 min
Delta R.T.: -0.068 min
Response: 135744
Conc: N.D.

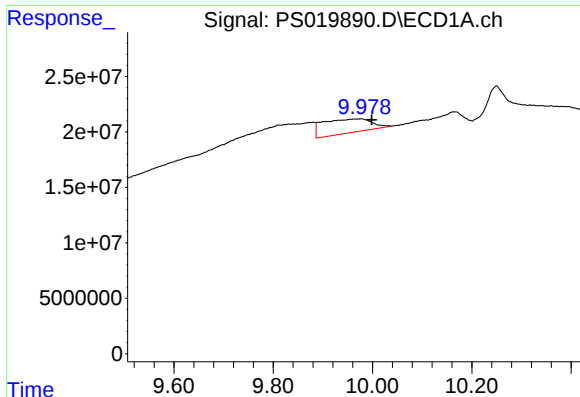

#13 2,4-DB


R.T.: 9.979 min
Delta R.T.: -0.020 min
Response: 86307679
Conc: 21.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

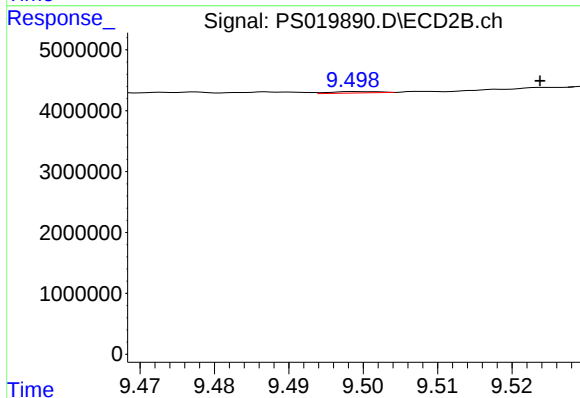


#13 2,4-DB

R.T.: 9.500 min
Delta R.T.: -0.024 min
Response: 107694
Conc: N.D.

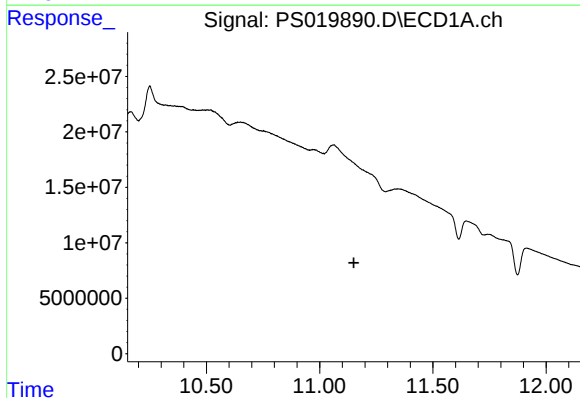


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.151 min
Response: 0
Conc: N.D.

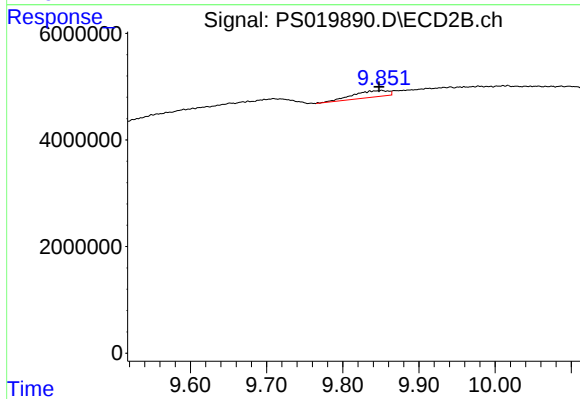

#14 DINOSEB


R.T.: 9.851 min
Delta R.T.: 0.003 min
Response: 3972354
Conc: 1.11 ng/ml

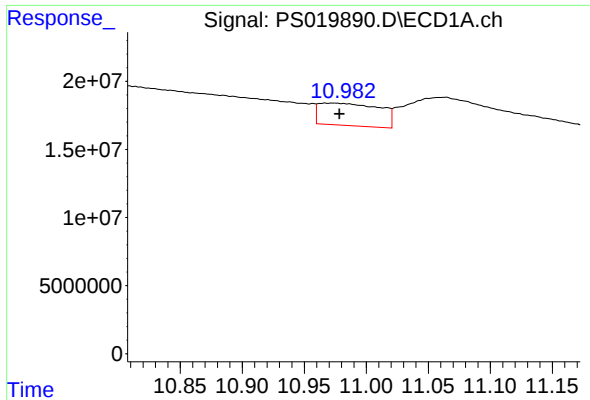

#15 Picloram

R.T.: 10.967 min
Delta R.T.: -0.012 min
Response: 55712099
Conc: 1.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

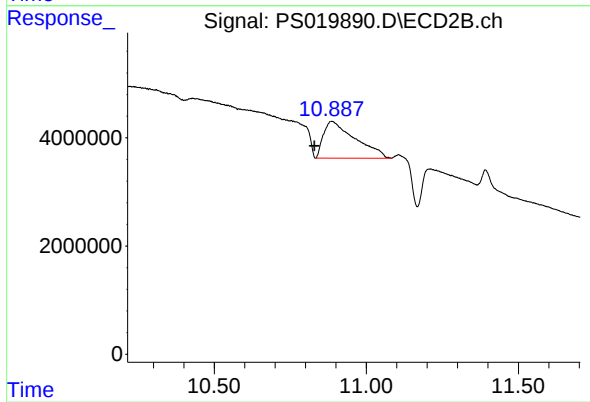

#15 Picloram

R.T.: 10.887 min
Delta R.T.: 0.057 min
Response: 49493973
Conc: 7.61 ng/ml