

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070720\
 Data File : PS011100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 11:28
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 17:53:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.491	0.000	29593663	0	23.523	N.D. #
5) T	DICAMBA	0.000	7.154	0	24515225	N.D.	10.794
6) T	MCP	0.000	7.154	0	24515225	N.D.	12.952
7) T	MCPA	7.684	0.000	11601879	0	2.913	N.D. #
8) T	DICHLORPROP	0.000	7.743	0	8549109	N.D.	14.561
9) T	2,4-D	0.000	8.049	0	62239326	N.D.	86.126
10) T	Pentachlo...	8.594	0.000	31675898	0	2.547	N.D. #
15) T	Picloram	11.043	11.013	14526784	14664440	2.591	3.500 #
16) T	DCPA	0.000	11.013	0	14664440	N.D.	3.937



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070720\
Data File : PS011100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 11:28
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 17:53:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

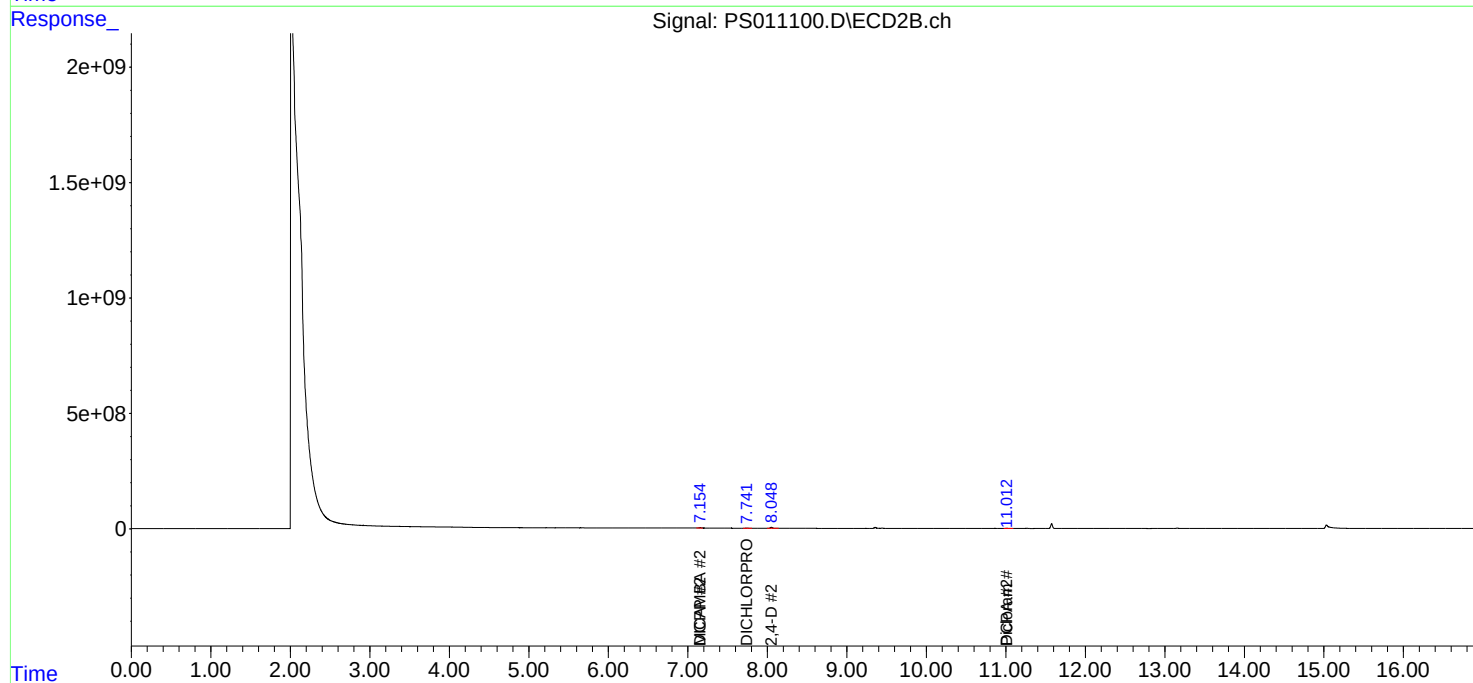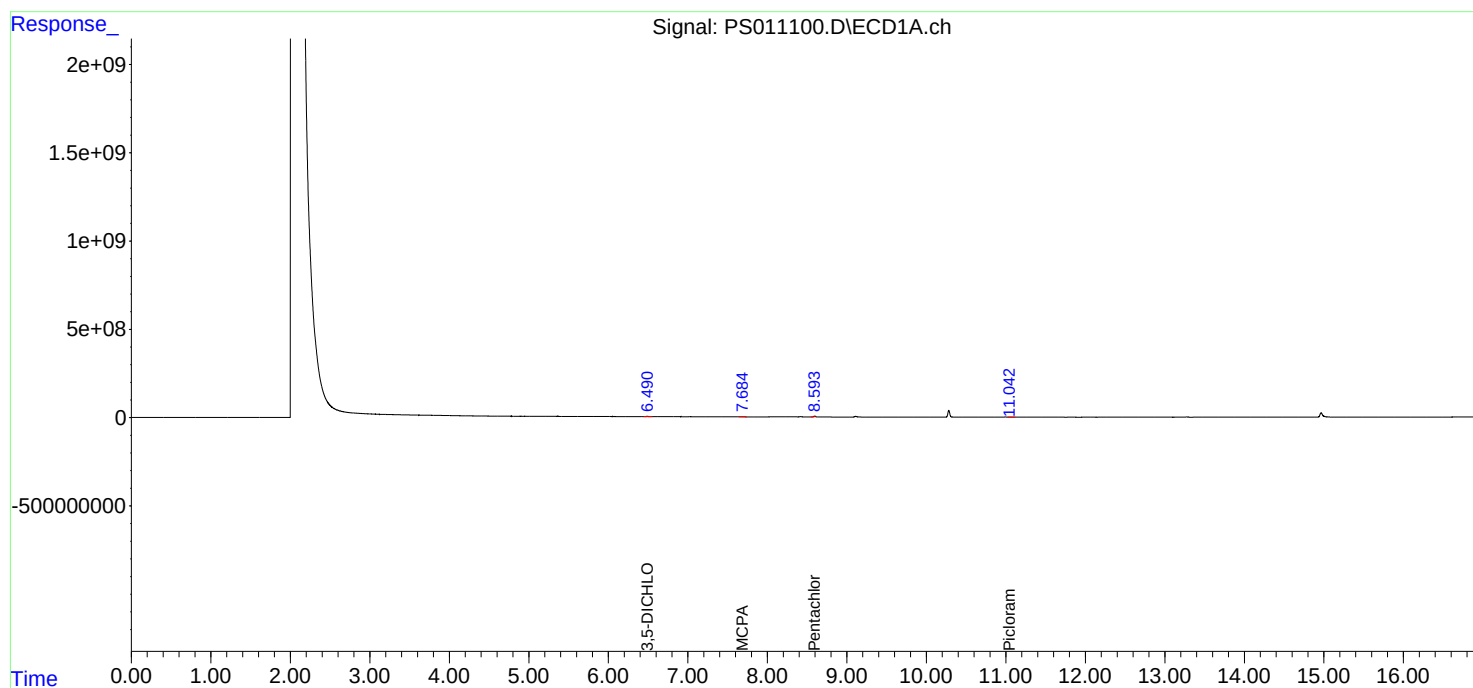


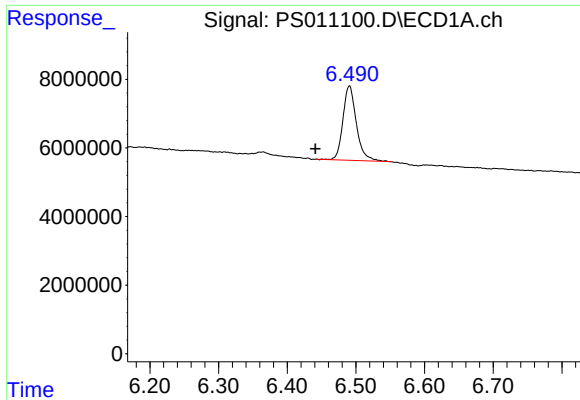

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.491 min
Delta R.T.: 0.049 min
Response: 29593663
Conc: 23.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

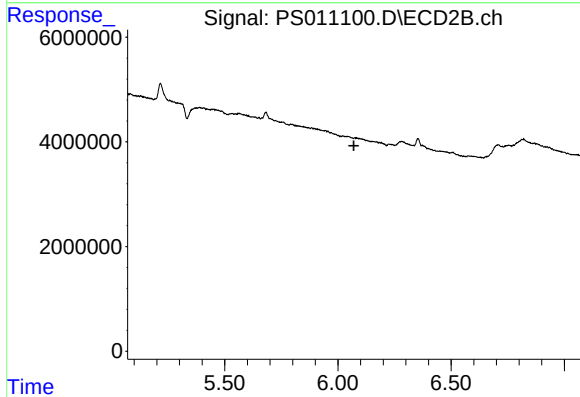


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

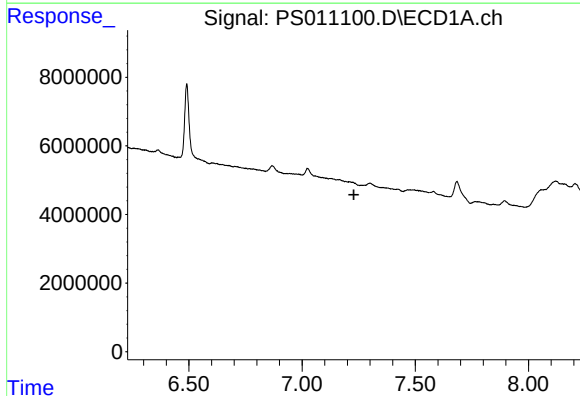


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

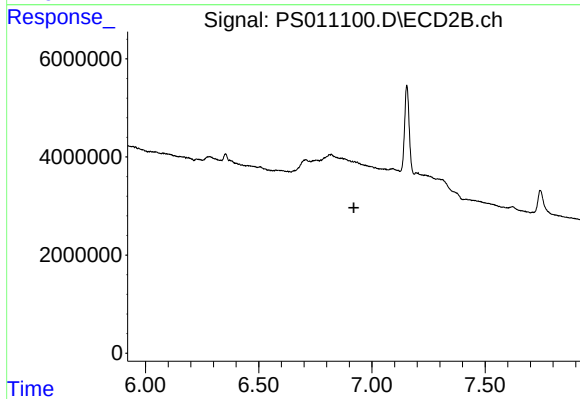

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

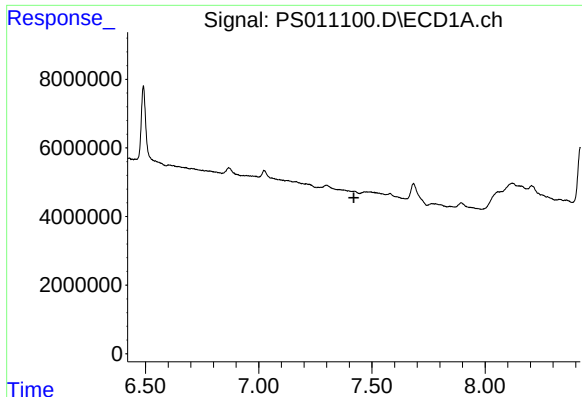

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

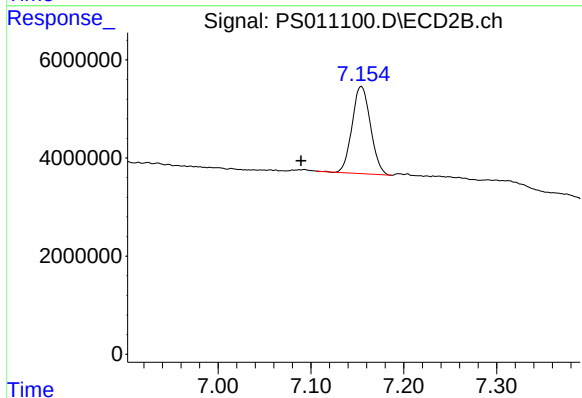


#5 DICAMBA

R.T.: 7.154 min
Delta R.T.: 0.065 min
Response: 24515225
Conc: 10.79 ng/ml

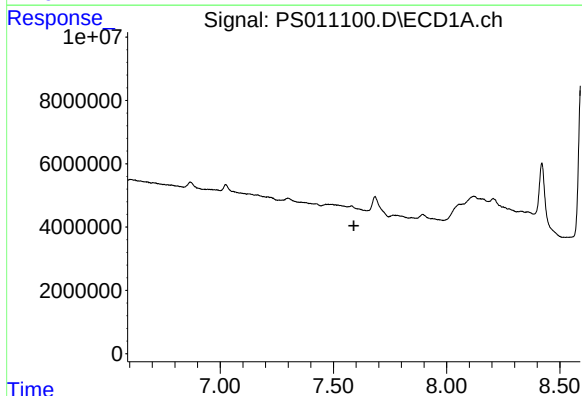


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.590 min
Response: 0
Conc: N.D.

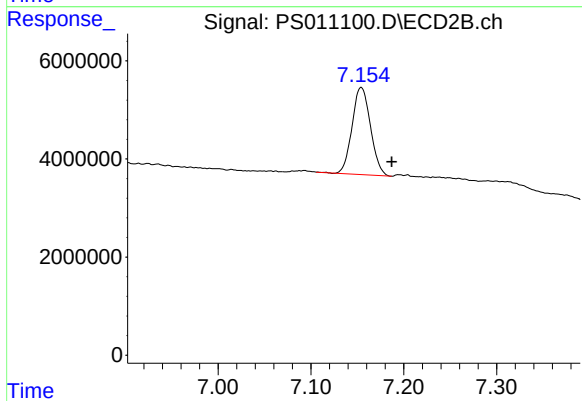

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.033 min
Response: 24515225
Conc: 12.95 ug/ml

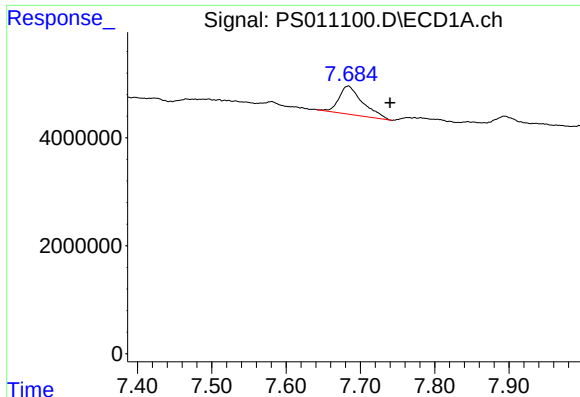

#7 MCPA


R.T.: 7.684 min
Delta R.T.: -0.056 min
Response: 11601879
Conc: 2.91 ug/ml

Instrument :
ECD_S
ClientSampleId :

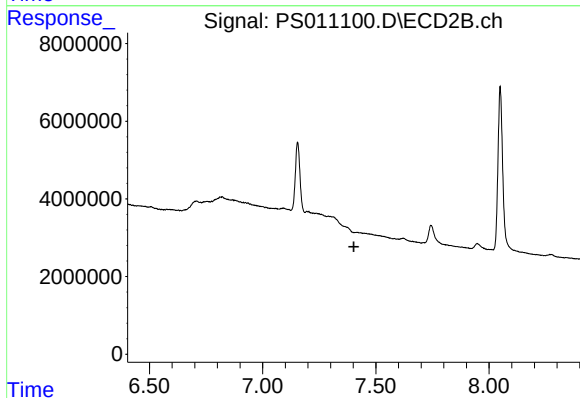


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

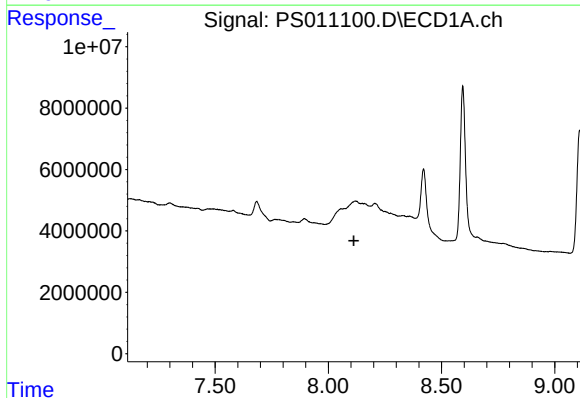


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

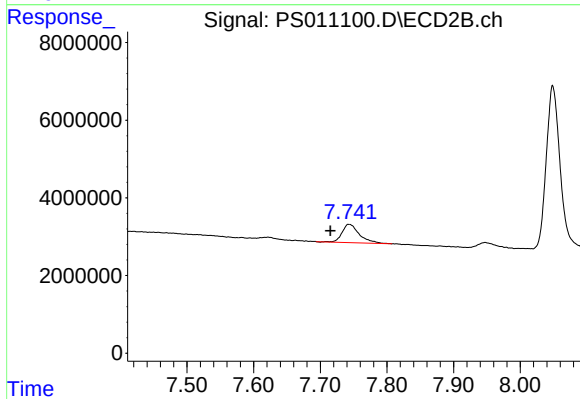

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.028 min
Response: 8549109
Conc: 14.56 ng/ml

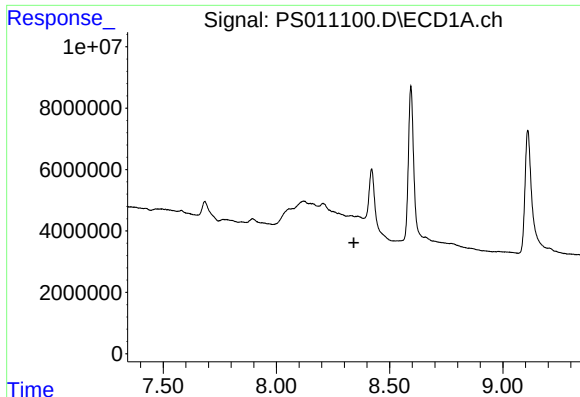

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

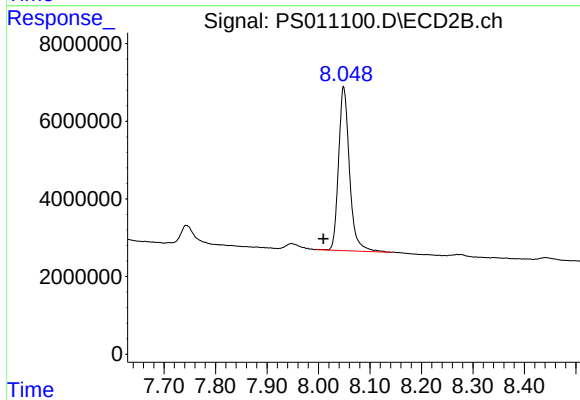


#9 2,4-D

R.T.: 8.049 min
Delta R.T.: 0.039 min
Response: 62239326
Conc: 86.13 ng/ml

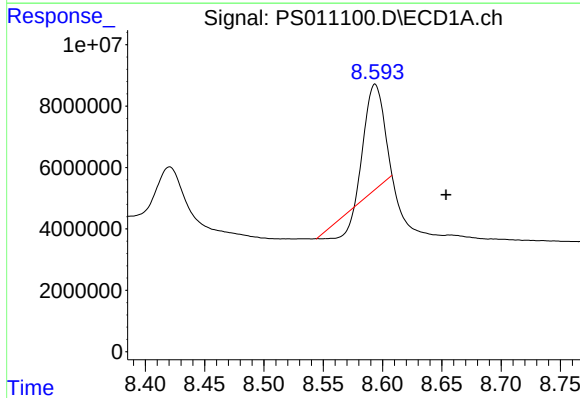


#10 Pentachlorophenol

R.T.: 8.594 min
Delta R.T.: -0.060 min
Response: 31675898
Conc: 2.55 ng/ml

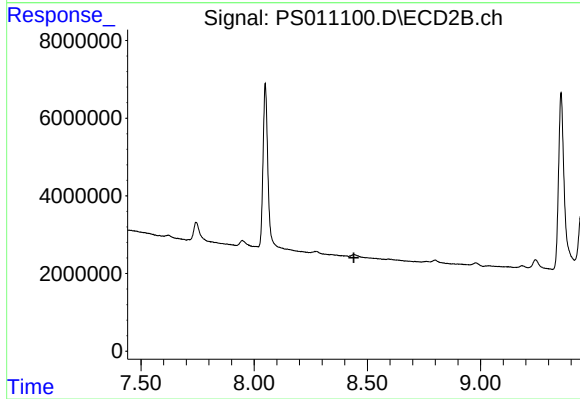

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.440 min
Response: 0
Conc: N.D.

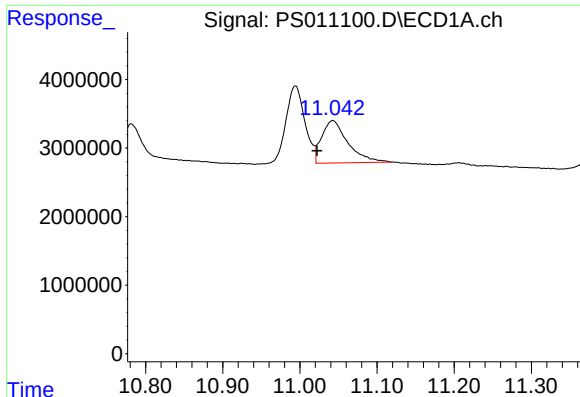

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.020 min
Response: 14526784
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

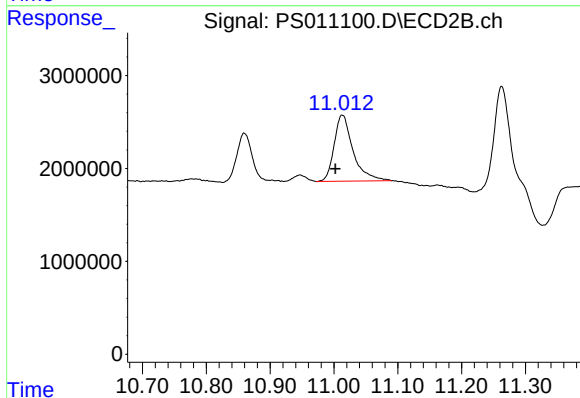


#15 Picloram

R.T.: 11.013 min
Delta R.T.: 0.011 min
Response: 14664440
Conc: 3.50 ng/ml

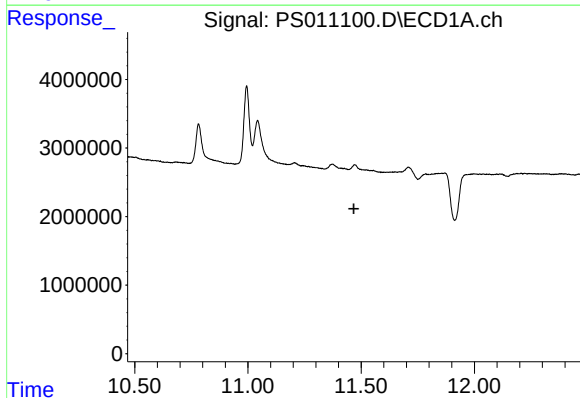

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

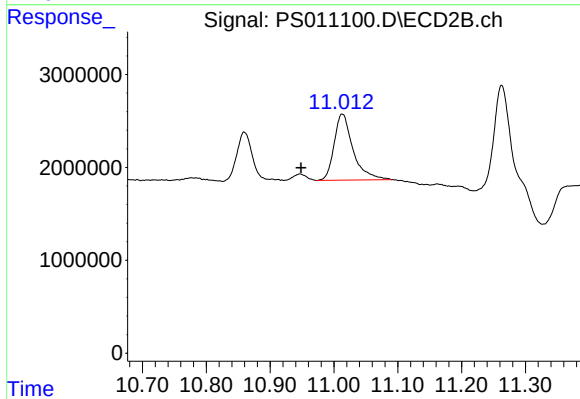

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.064 min
Response: 14664440
Conc: 3.94 ng/ml