

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070720\
 Data File : PS011103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2020 16:16
 Operator : DD\AJ
 Sample : PB130004BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 17:56:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.917	479.7E6	311.5E6	529.013	562.261
Target Compounds							
1) T	Dalapon	2.996	2.579	43958174	186.2E6	39.258	246.869 #
2) T	3,5-DICHL...	0.000	6.097	0	86398009	N.D.	103.741
6) T	MCPD	7.587	0.000	6249837	0	2.192	N.D. #
7) T	MCPA	7.780	7.381	21227987	15843994	5.330	5.741
8) T	DICHLORPROP	0.000	7.737	0	6733203	N.D.	11.468
10) T	Pentachlo...	8.712	8.509	16766537	6389236	1.348	<MDL #
12) T	2,4,5-T	9.512	9.233	12813924	31200895	2.751	10.478 #
14) T	DINOSEB	11.173	10.031	74025513	25985633	20.669	12.480 #
15) T	Picloram	11.031	11.004	140.2E6	132.1E6	25.013	31.528 #
16) T	DCPA	0.000	11.004	0	132.1E6	N.D.	35.466



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070720\
Data File : PS011103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2020 16:16
Operator : DD\AJ
Sample : PB130004BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 17:56:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

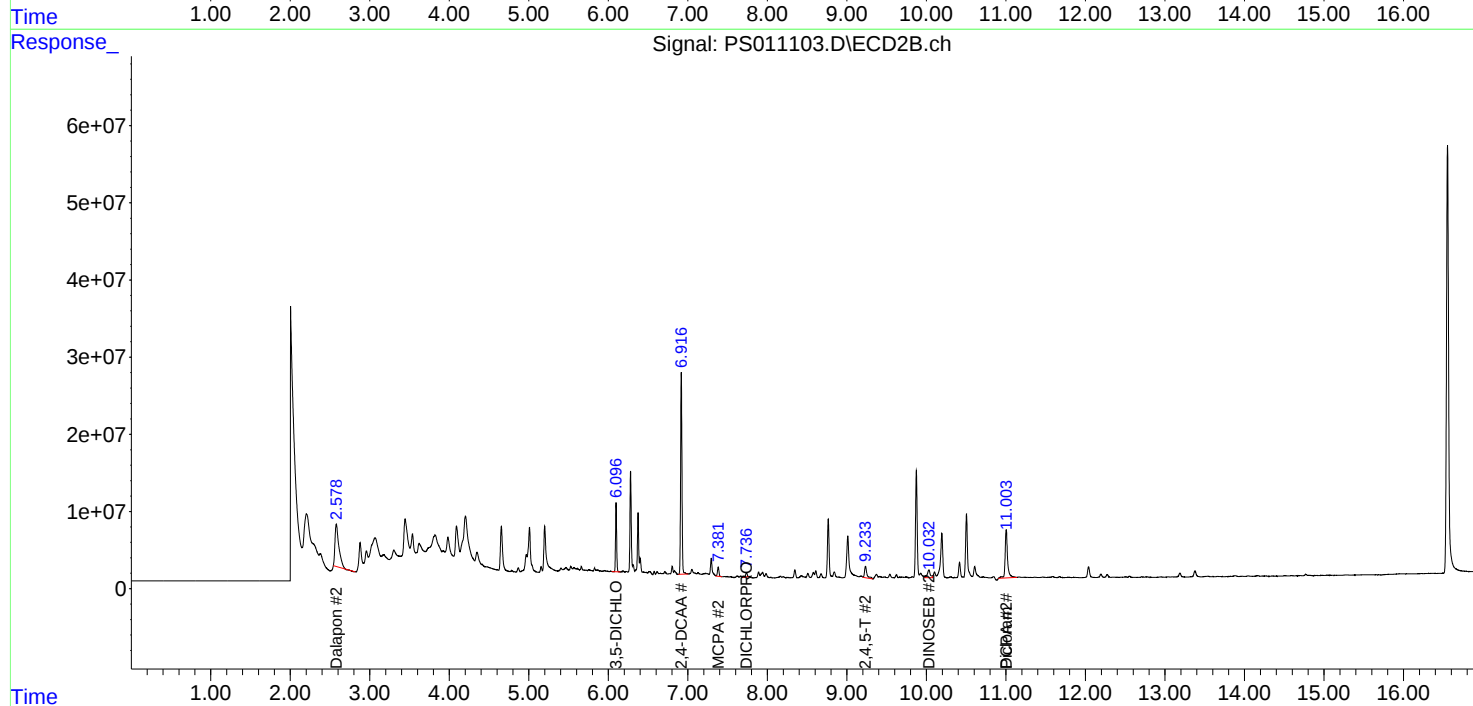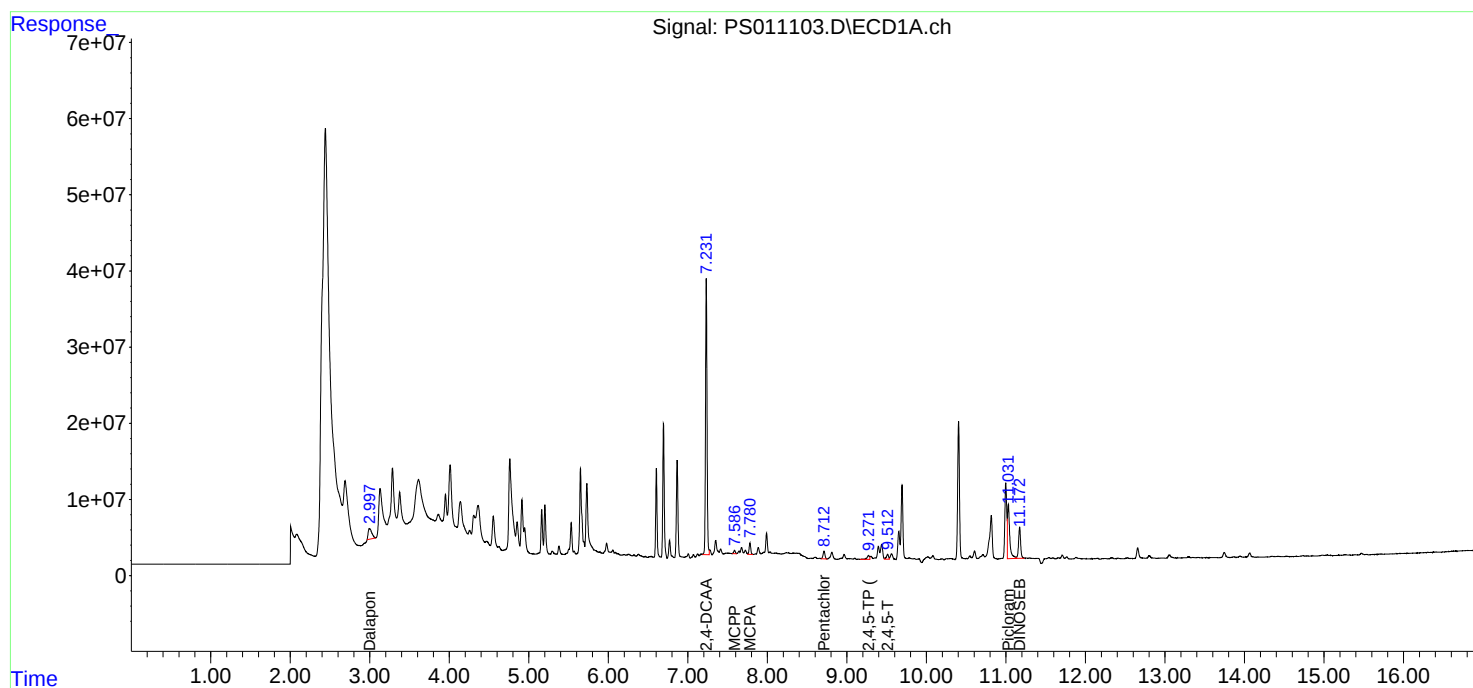


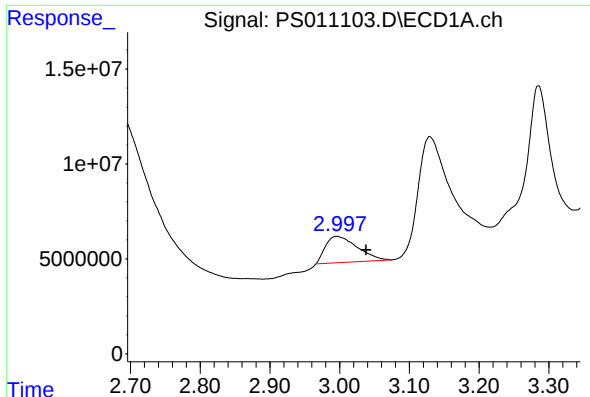

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 43958174
Conc: 39.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

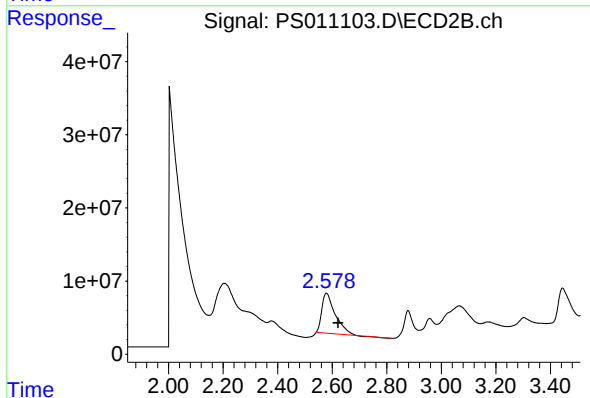


#1 Dalapon

R.T.: 2.579 min
Delta R.T.: -0.043 min
Response: 186227938
Conc: 246.87 ng/ml

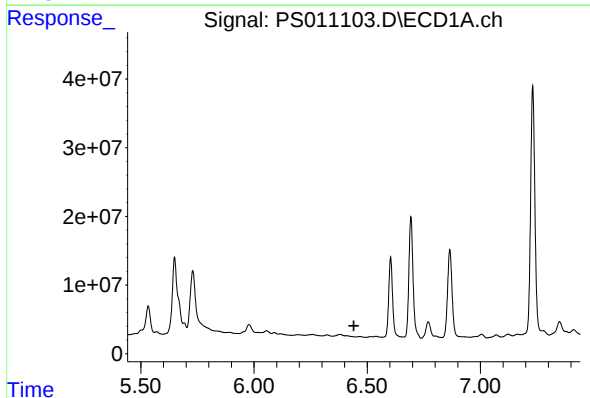


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

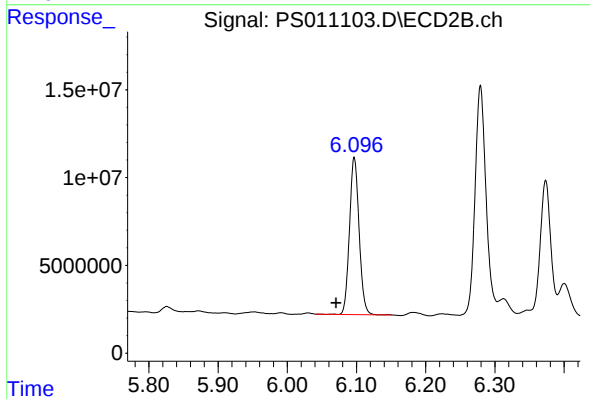

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.097 min
Delta R.T.: 0.027 min
Response: 86398009
Conc: 103.74 ng/ml

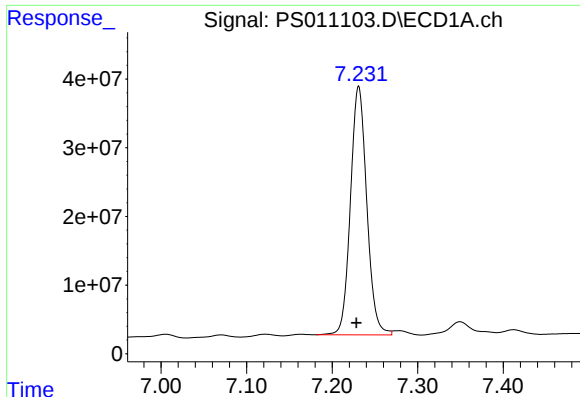

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: 0.003 min
Response: 479719186
Conc: 529.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

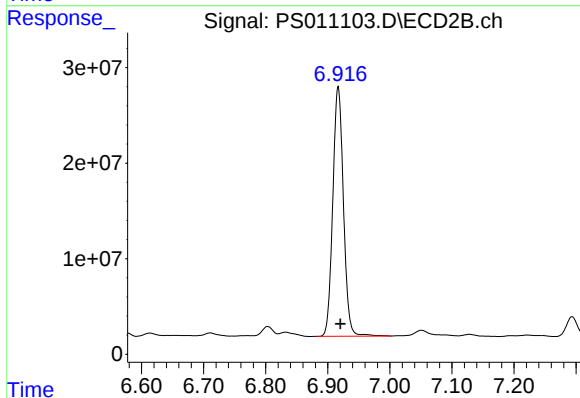


#4 2,4-DCAA

R.T.: 6.917 min
Delta R.T.: -0.004 min
Response: 311535548
Conc: 562.26 ng/ml

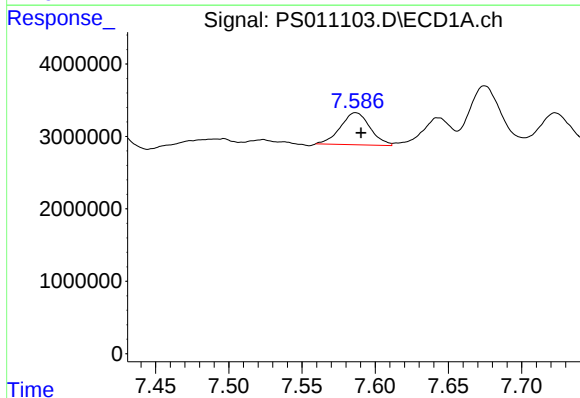


#6 MCP

R.T.: 7.587 min
Delta R.T.: -0.004 min
Response: 6249837
Conc: 2.19 ug/ml

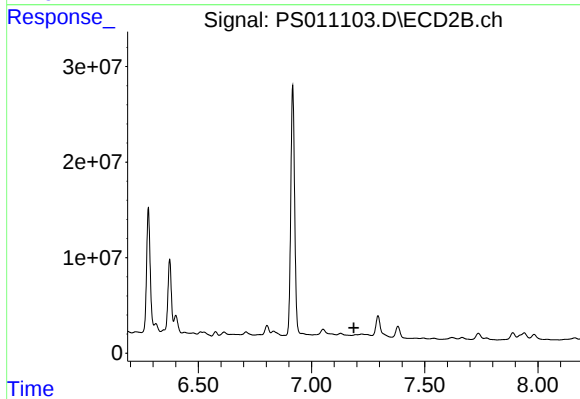

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

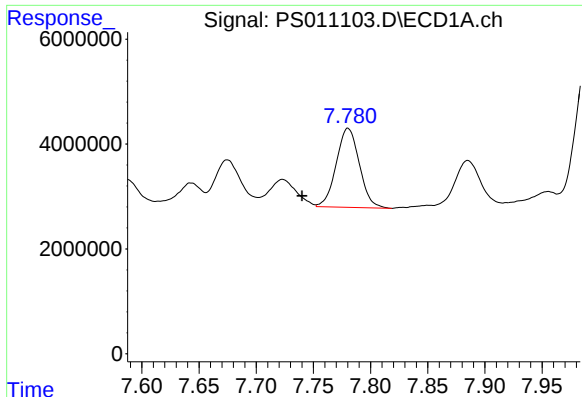

#7 MCPA


R.T.: 7.780 min
Delta R.T.: 0.040 min
Response: 21227987
Conc: 5.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

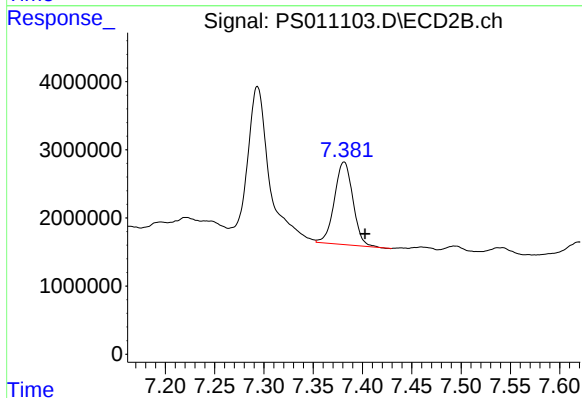


#7 MCPA

R.T.: 7.381 min
Delta R.T.: -0.022 min
Response: 15843994
Conc: 5.74 ug/ml

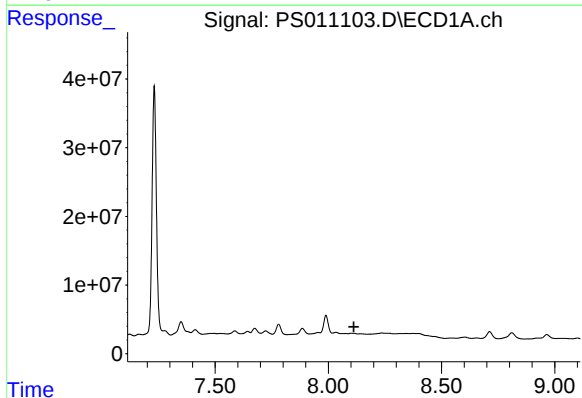


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

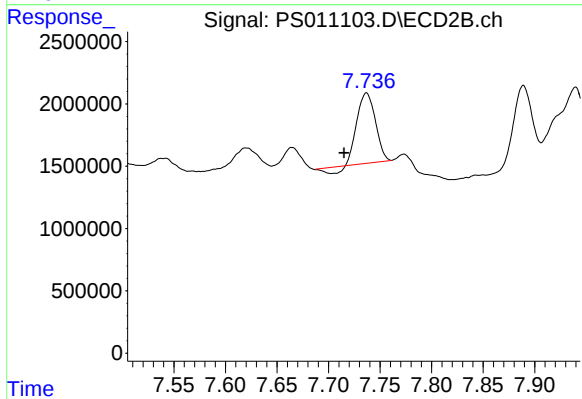

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.022 min
Response: 6733203
Conc: 11.47 ng/ml

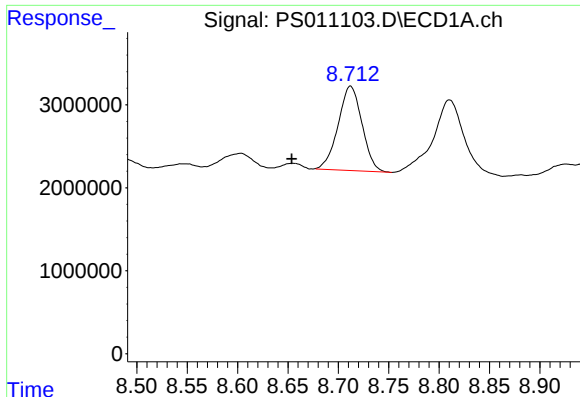

#10 Pentachlorophenol


R.T.: 8.712 min
Delta R.T.: 0.058 min
Response: 16766537
Conc: 1.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

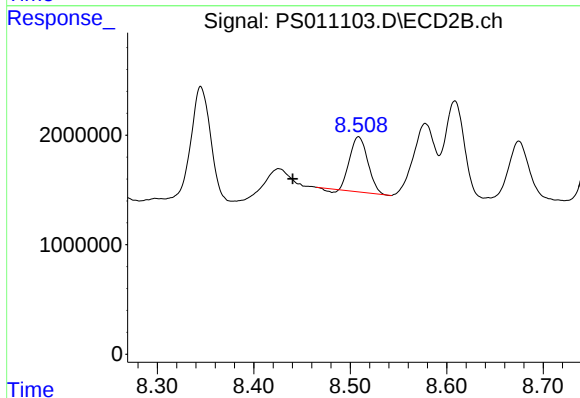


#10 Pentachlorophenol

R.T.: 8.509 min
Delta R.T.: 0.068 min
Response: 6389236
Conc: N.D.

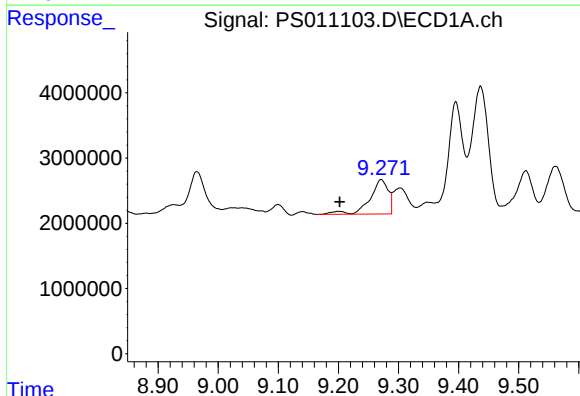


#11 2,4,5-TP (SILVEX)

R.T.: 9.271 min
Delta R.T.: 0.069 min
Response: 11234267
Conc: 2.26 ng/ml

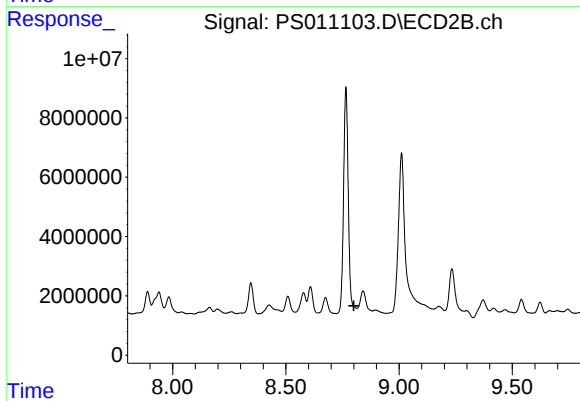

#11 2,4,5-TP (SILVEX)


R.T.: 8.841 min
Delta R.T.: 0.041 min
Response: -44263074
Conc: N.D.

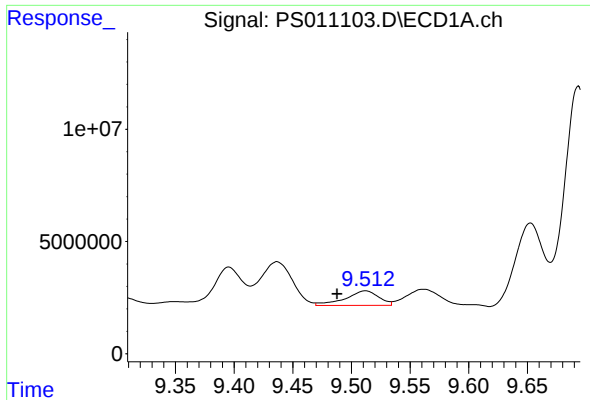

#12 2,4,5-T


R.T.: 9.512 min
Delta R.T.: 0.024 min
Response: 12813924
Conc: 2.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

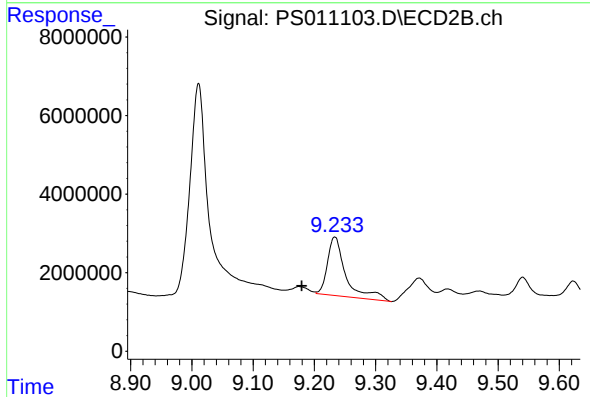


#12 2,4,5-T

R.T.: 9.233 min
Delta R.T.: 0.054 min
Response: 31200895
Conc: 10.48 ng/ml

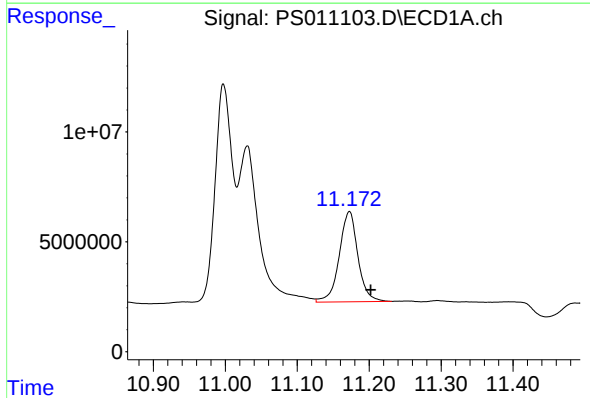


#14 DINOSEB

R.T.: 11.173 min
Delta R.T.: -0.029 min
Response: 74025513
Conc: 20.67 ng/ml

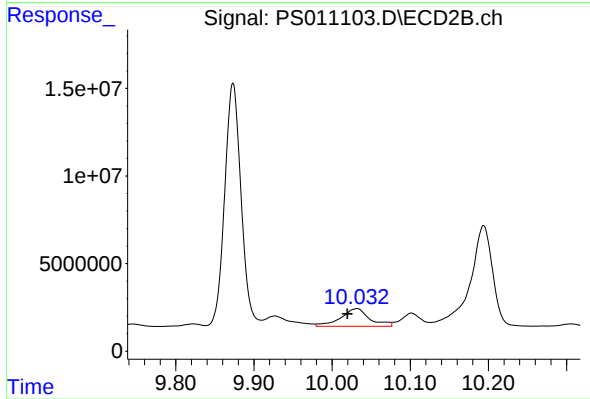

#14 DINOSEB


R.T.: 10.031 min
Delta R.T.: 0.012 min
Response: 25985633
Conc: 12.48 ng/ml

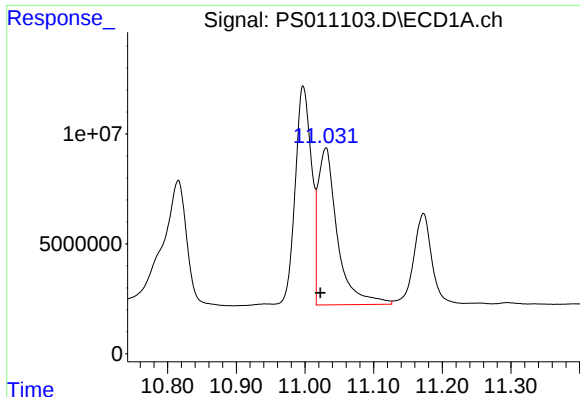

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.008 min
Response: 140224514
Conc: 25.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

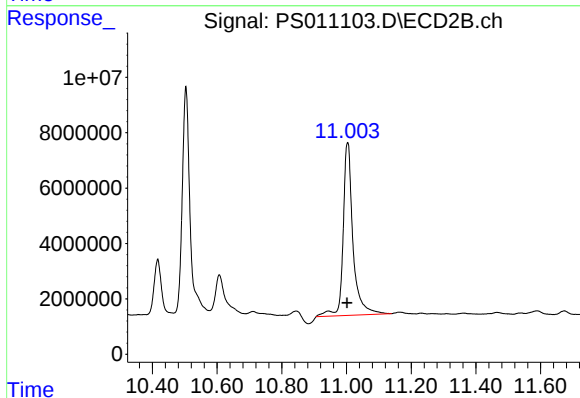


#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.001 min
Response: 132088690
Conc: 31.53 ng/ml

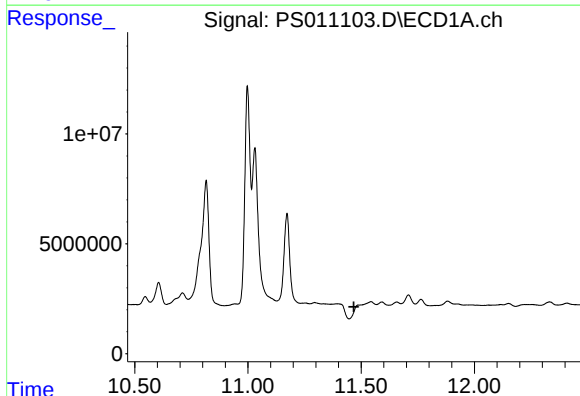

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

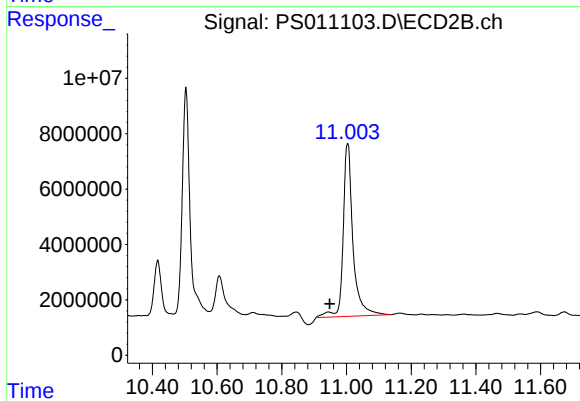

#16 DCPA

R.T.: 11.004 min
Delta R.T.: 0.055 min
Response: 132088690
Conc: 35.47 ng/ml