

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070722\
 Data File : PS019897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 09:49
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:06:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	6.780	1390.3E6	396.3E6	536.035	487.918
Target Compounds							
2) T	3,5-DICHL...	6.462f	0.000	2489626	0	<MDL	N.D. #
7) T	MCPA	7.671	0.000	1163353	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.610f	0	121240	N.D.	<MDL
10) T	Pentachlo...	8.625	8.285	381289	595557	<MDL	<MDL #
11) T	2,4,5-TP ...	9.196	0.000	2870826	0	<MDL	N.D. #
12) T	2,4,5-T	9.509f	0.000	8163471	0	<MDL	N.D. #
13) T	2,4-DB	9.948f	0.000	1928681	0	<MDL	N.D. #
14) T	DINOSEB	11.123	9.809	42068426	307378	2.588	<MDL #
15) T	Picloram	10.998	10.775f	20098293	6777093	<MDL	1.042 #
16) T	DCPA	11.422	10.775	1927552	6777093	<MDL	1.046 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070722\
Data File : PS019897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 09:49
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 01:06:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

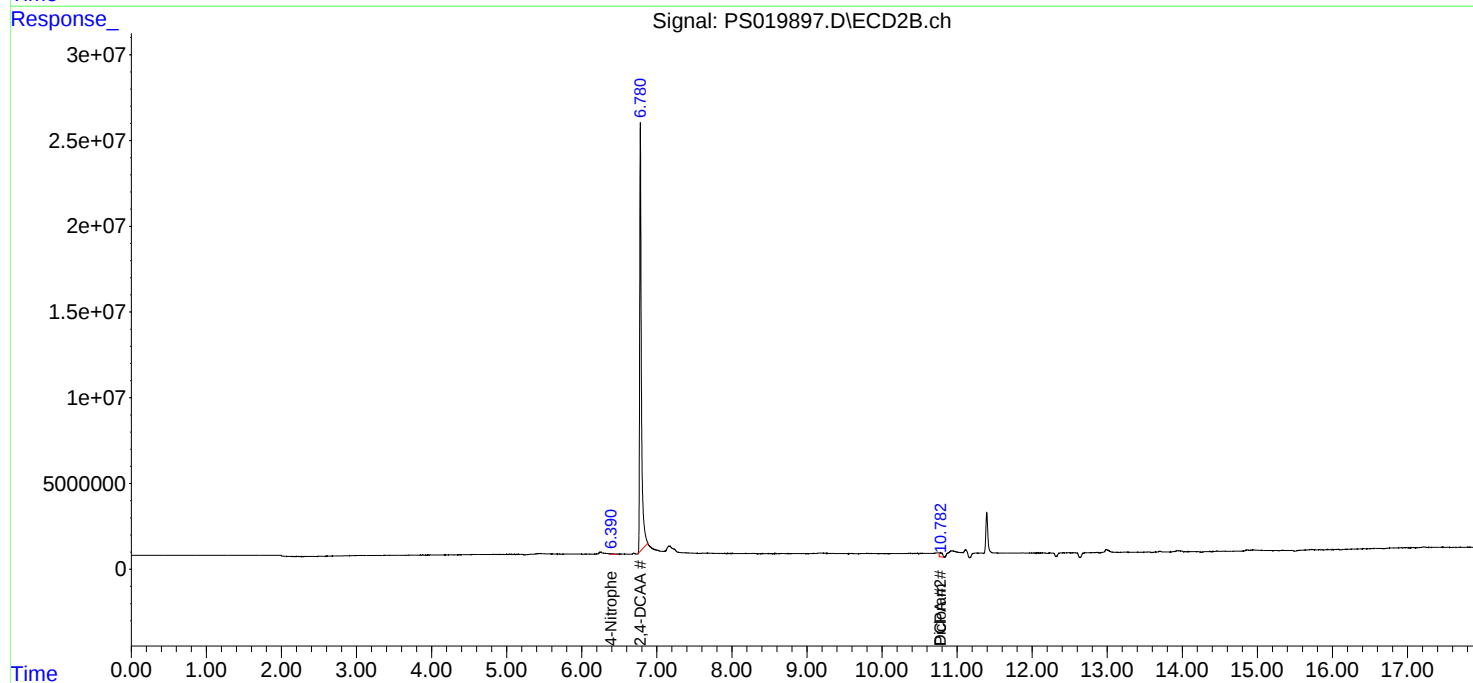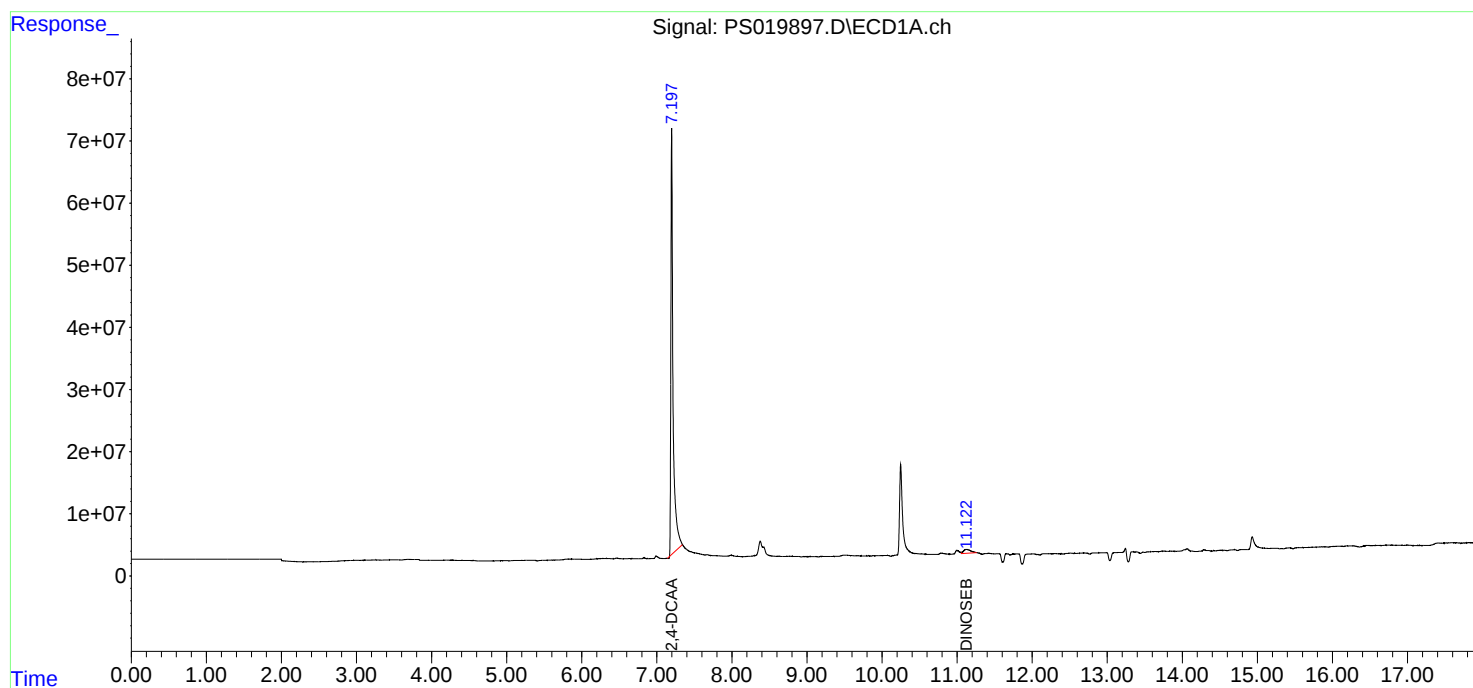


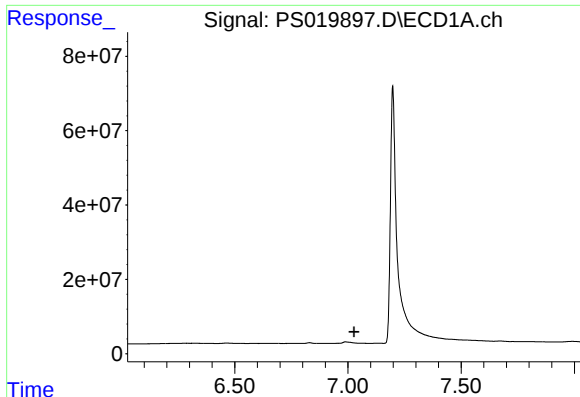

#3 4-Nitrophenol


R.T.: 6.989 min
Delta R.T.: -0.038 min
Response: -4576471
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

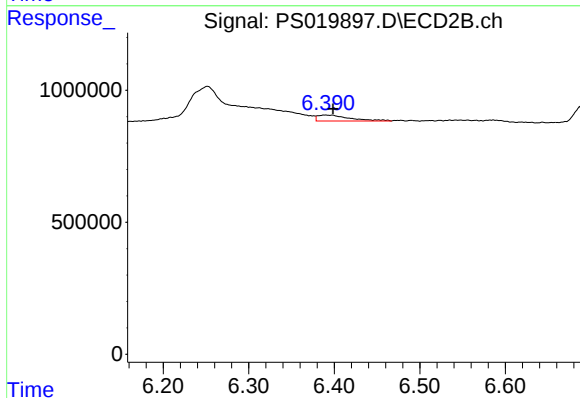


#3 4-Nitrophenol

R.T.: 6.389 min
Delta R.T.: -0.009 min
Response: 576879
Conc: 1.33 ng/ml

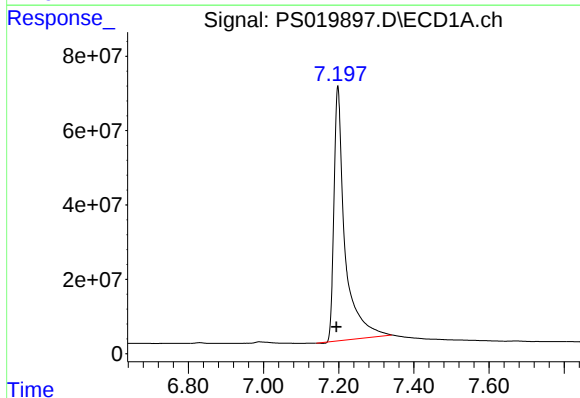


#4 2,4-DCAA

R.T.: 7.198 min
Delta R.T.: 0.004 min
Response: 1390287439
Conc: 536.03 ng/ml

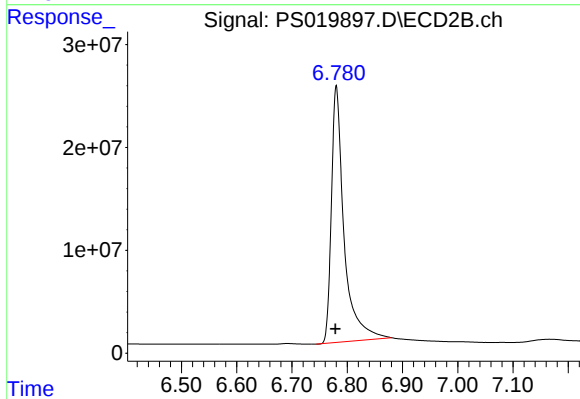

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: 0.002 min
Response: 396260688
Conc: 487.92 ng/ml

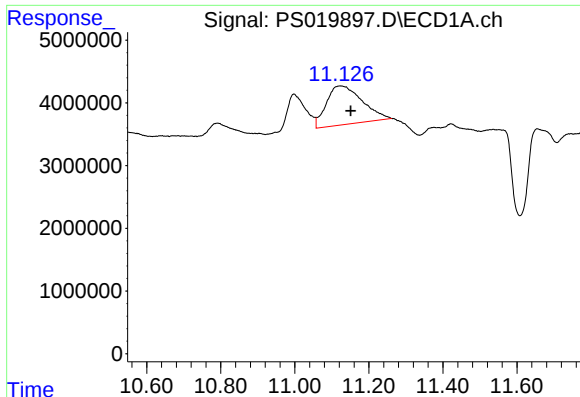

#14 DINOSEB


R.T.: 11.123 min
Delta R.T.: -0.028 min
Response: 42068426
Conc: 2.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

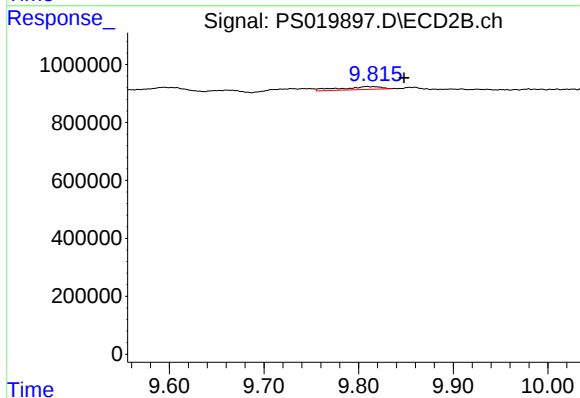


#14 DINOSEB

R.T.: 9.809 min
Delta R.T.: -0.039 min
Response: 307378
Conc: N.D.

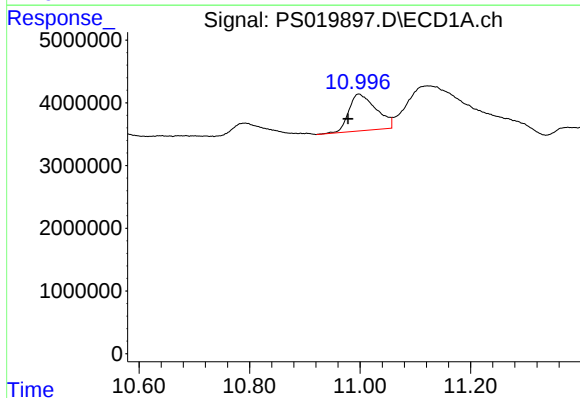


#15 Picloram

R.T.: 10.998 min
Delta R.T.: 0.019 min
Response: 20098293
Conc: N.D.

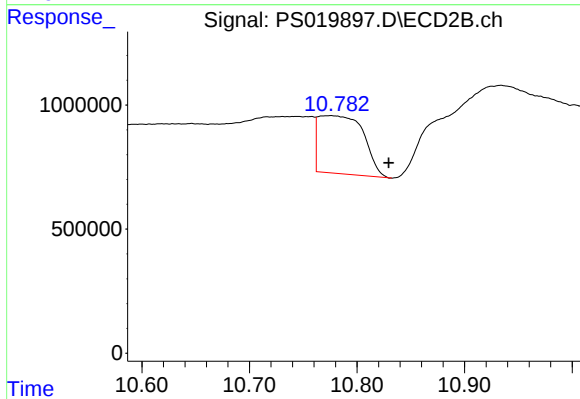

#15 Picloram


R.T.: 10.775 min
Delta R.T.: -0.054 min
Response: 6777093
Conc: 1.04 ng/ml

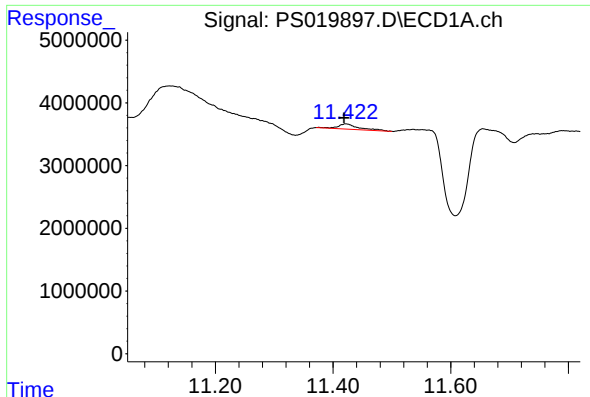

#16 DCPA

R.T.: 11.422 min
Delta R.T.: 0.003 min
Response: 1927552
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

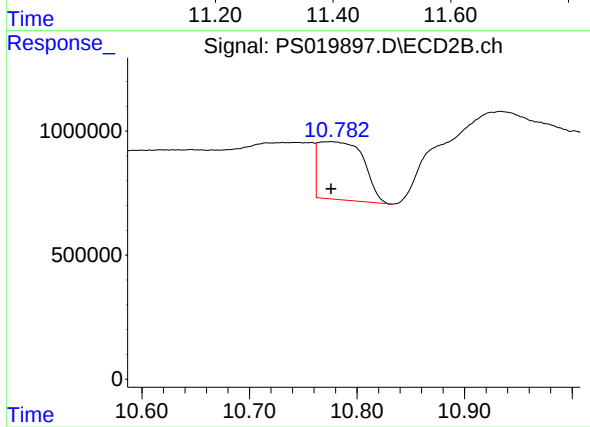

#16 DCPA

R.T.: 10.775 min
Delta R.T.: 0.000 min
Response: 6777093
Conc: 1.05 ng/ml