

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070723\
 Data File : PS023627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2023 16:22
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 02:36:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
 Quant Title : 8080.M
 QLast Update : Fri Jul 07 18:46:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.375	6.812	680.2E6	224.2E6	538.518	534.521
Target Compounds							
1) T	Dalapon	2.500	0.000	235377	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.712	0.000	8114754	0	4.188	N.D. #
3) T	4-Nitroph...	6.217	6.354f	3901689	16607	4.360	<MDL #
5) T	DICAMBA	6.518	6.975	272741	120527	<MDL	<MDL #
8) T	DICHLORPROP	7.060f	7.612	4303365	556051	2.910	1.195 #
10) T	Pentachlo...	7.536	8.310	472788	587466	<MDL	<MDL #
11) T	2,4,5-TP ...	8.062	0.000	2040829	0	<MDL	N.D. #
12) T	2,4,5-T	8.319	9.082f	951374	878262	<MDL	<MDL #
13) T	2,4-DB	8.769f	0.000	3813358	0	3.873	N.D. #
14) T	DINOSEB	9.881	0.000	1130291	0	<MDL	N.D. #
15) T	Picloram	9.709	10.834	14438020	4920985	1.231	1.163
16) T	DCPA	10.146	10.834	1643721	4920985	<MDL	1.774 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070723\
Data File : PS023627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2023 16:22
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 02:36:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070723.M
Quant Title : 8080.M
QLast Update : Fri Jul 07 18:46:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

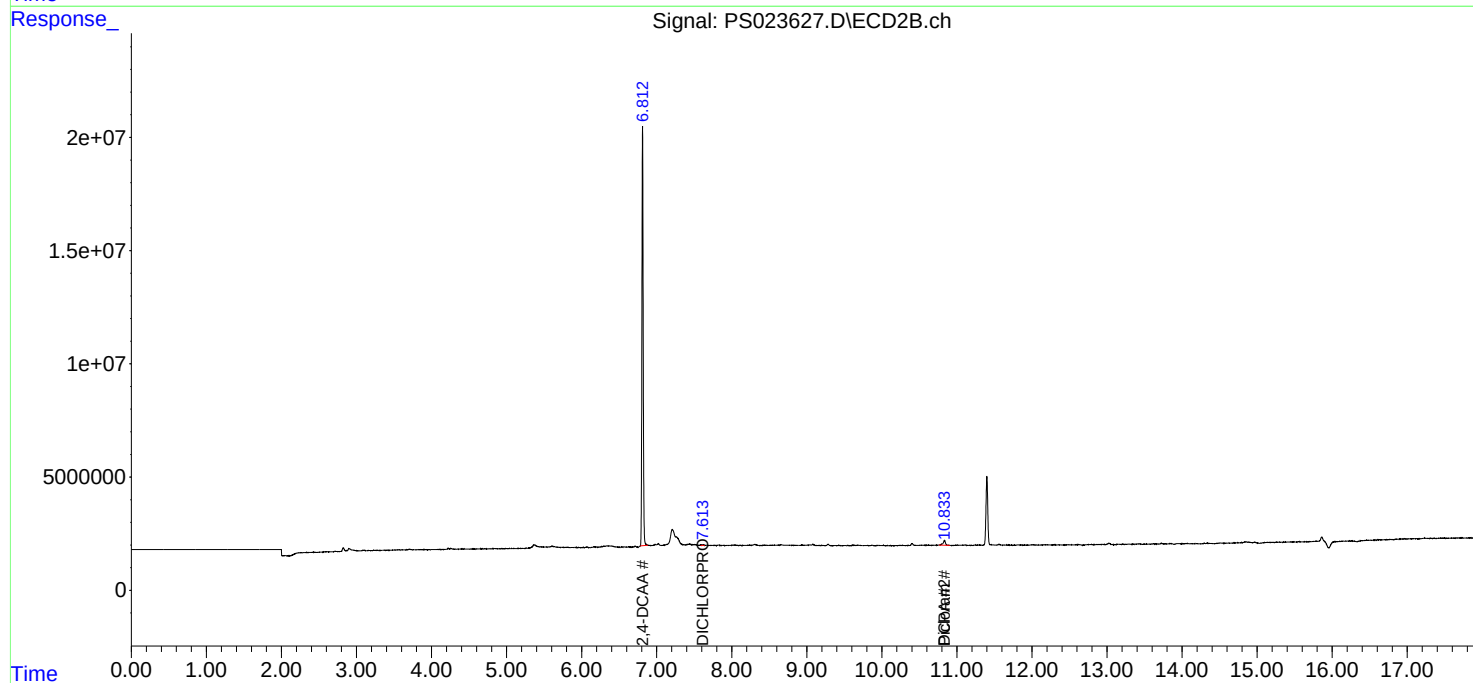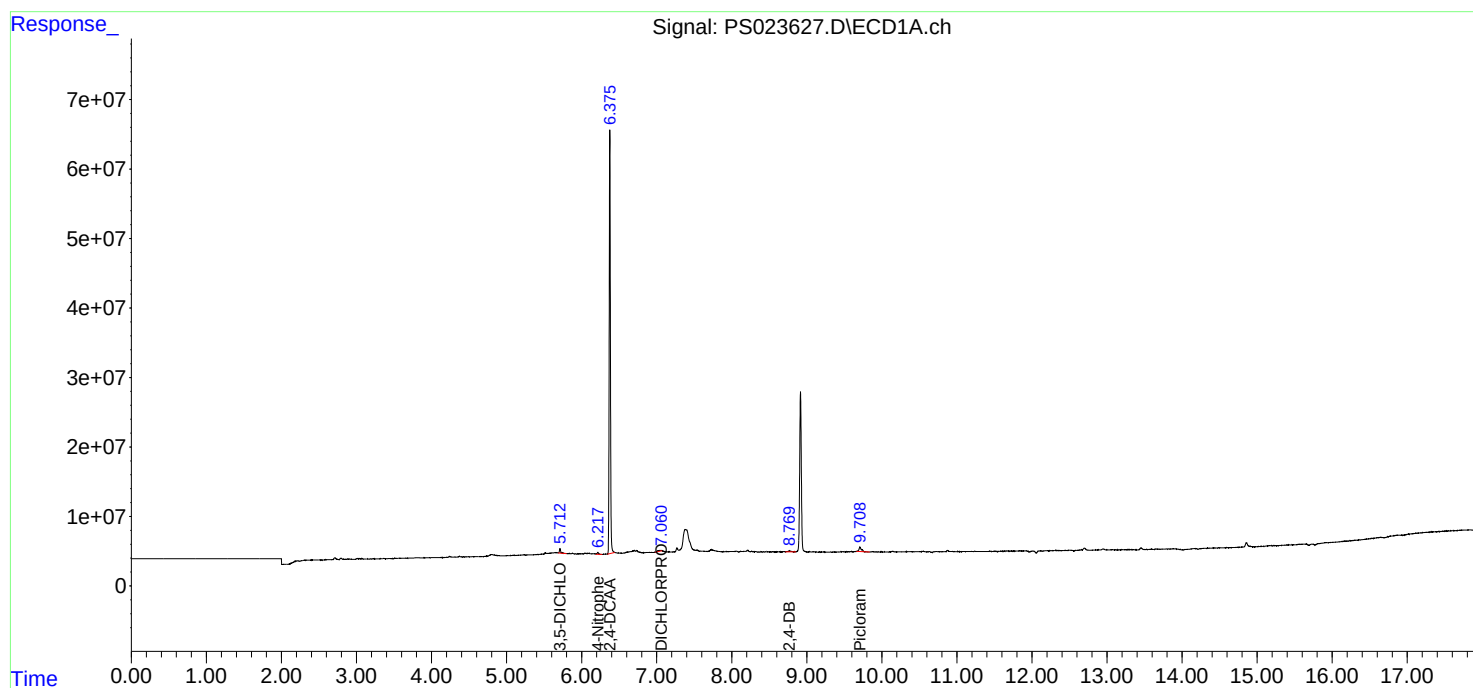


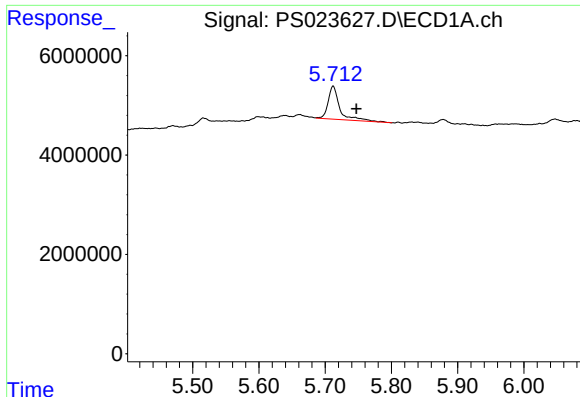

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.712 min
Delta R.T.: -0.035 min
Response: 8114754
Conc: 4.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

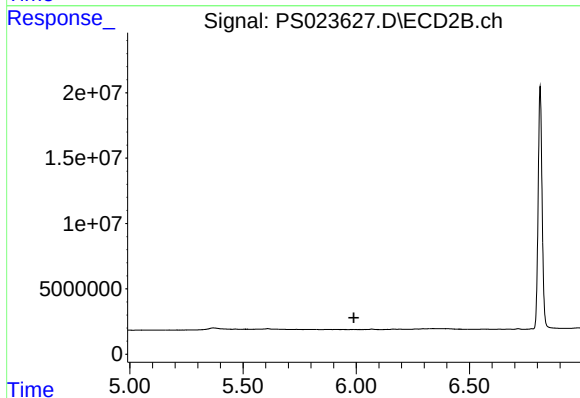


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.989 min
Response: 0
Conc: N.D.

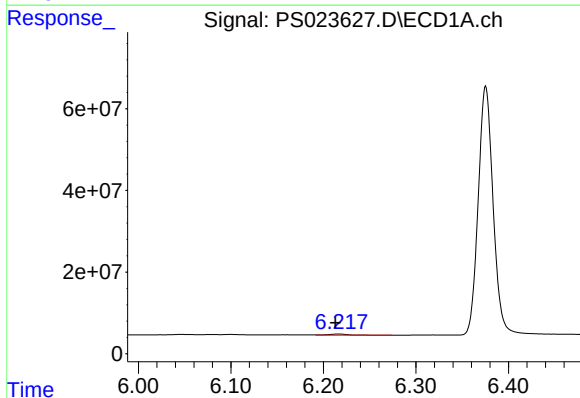


#3 4-Nitrophenol

R.T.: 6.217 min
Delta R.T.: 0.004 min
Response: 3901689
Conc: 4.36 ng/ml

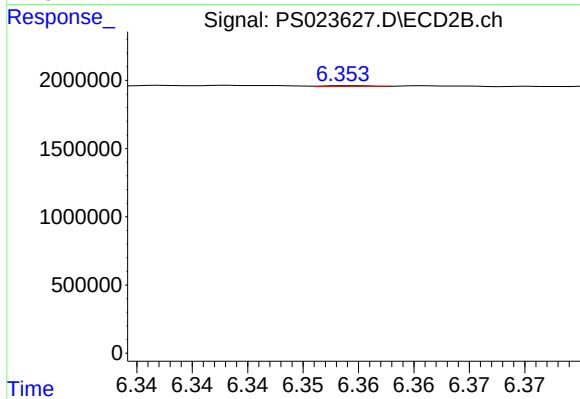

#3 4-Nitrophenol


R.T.: 6.354 min
Delta R.T.: -0.069 min
Response: 16607
Conc: N.D.

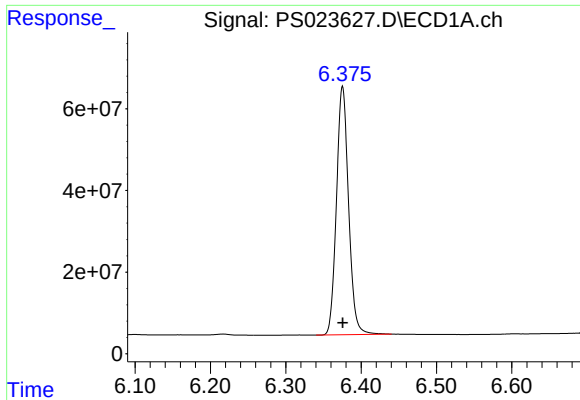

#4 2,4-DCAA


R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 680151341
Conc: 538.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

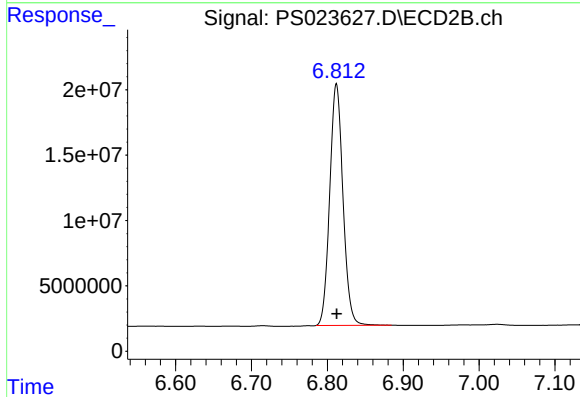


#4 2,4-DCAA

R.T.: 6.812 min
Delta R.T.: 0.000 min
Response: 224201023
Conc: 534.52 ng/ml

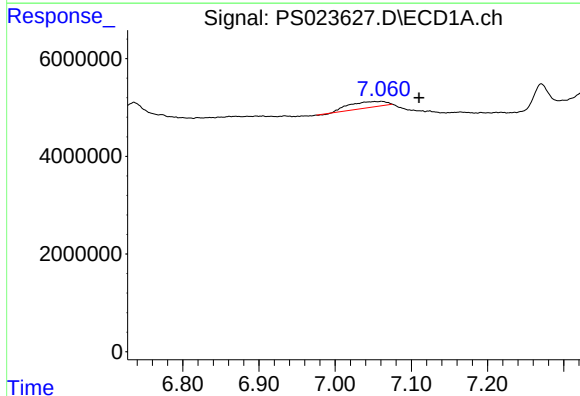


#8 DICHLORPROP

R.T.: 7.060 min
Delta R.T.: -0.050 min
Response: 4303365
Conc: 2.91 ng/ml

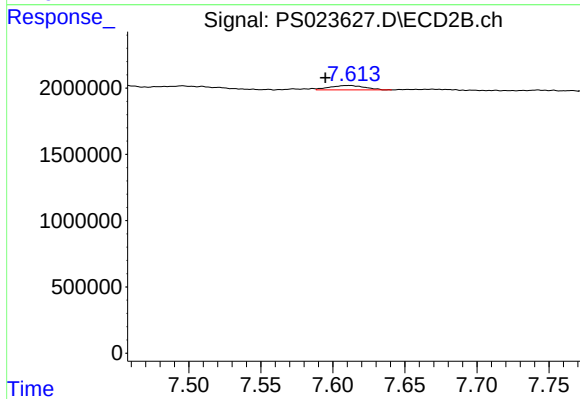

#8 DICHLORPROP


R.T.: 7.612 min
Delta R.T.: 0.018 min
Response: 556051
Conc: 1.19 ng/ml

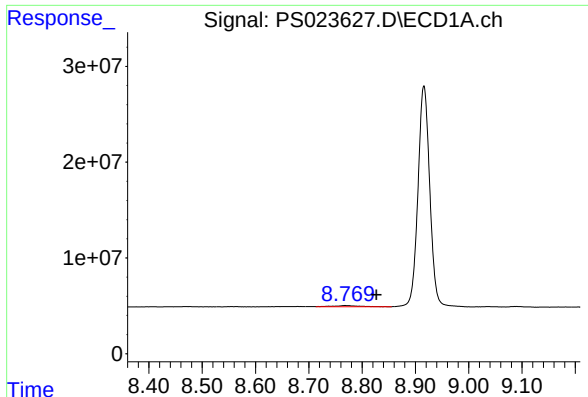

#13 2,4-DB


R.T.: 8.769 min
Delta R.T.: -0.057 min
Response: 3813358
Conc: 3.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

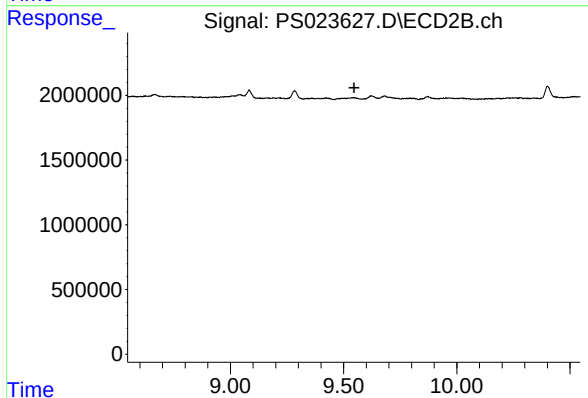


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.546 min
Response: 0
Conc: N.D.

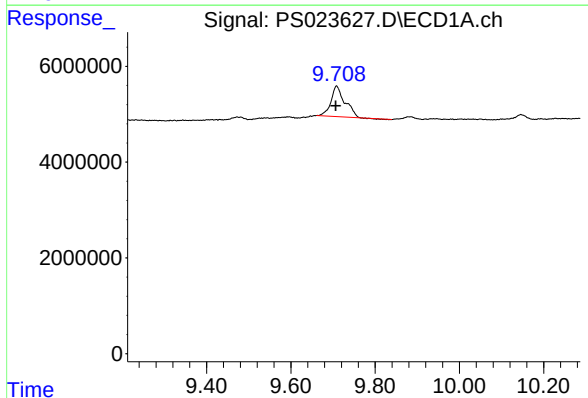


#15 Picloram

R.T.: 9.709 min
Delta R.T.: 0.002 min
Response: 14438020
Conc: 1.23 ng/ml

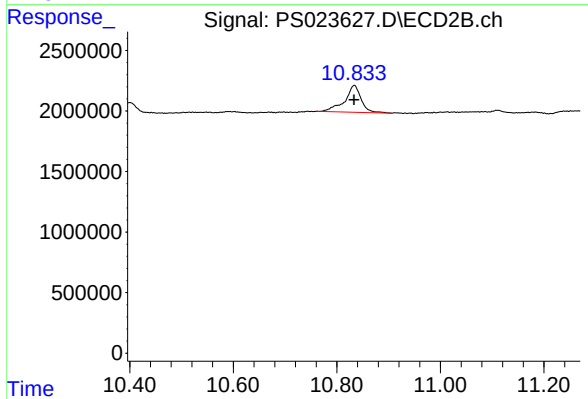

#15 Picloram


R.T.: 10.834 min
Delta R.T.: 0.000 min
Response: 4920985
Conc: 1.16 ng/ml

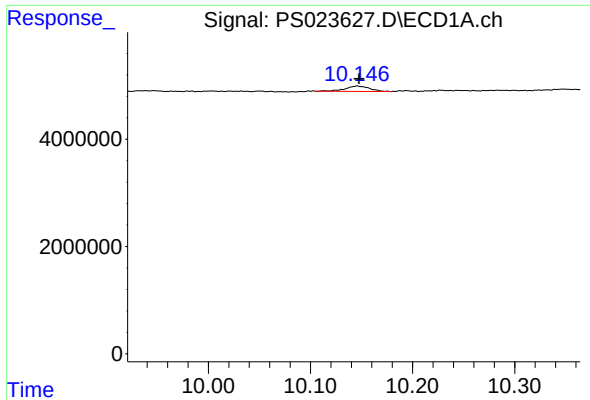

#16 DCPA

R.T.: 10.146 min
Delta R.T.: -0.002 min
Response: 1643721
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

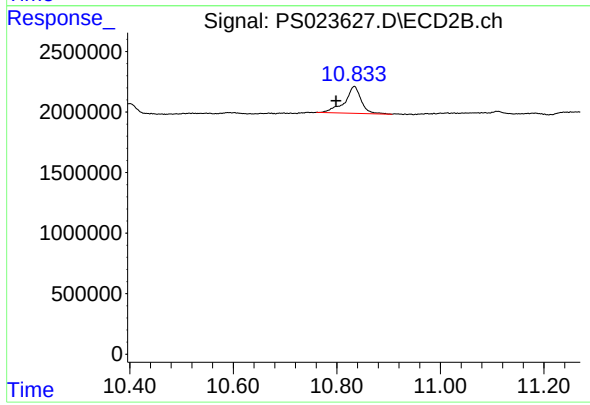

#16 DCPA

R.T.: 10.834 min
Delta R.T.: 0.035 min
Response: 4920985
Conc: 1.77 ng/ml