

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 03:36
 Operator : UA
 Sample : J3843-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:29:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.661	11.082	64130156	55951540	310.829	256.898
Target Compounds							
2) T	3,5-DICHL...	0.000	9.167	0	4565709	N.D.	15.522 #
3) T	4-Nitroph...	0.000	10.273	0	51759847	N.D.	428.955 #
5) T	DICAMBA	11.940	11.325	37367305	8370969	47.458	10.664 #
6) T	MCP	12.354	0.000	11574559	0	21.072	N.D. #
8) T	DICHLORPROP	0.000	12.449	0	2248854	N.D.	11.134 #
10) T	Pentachlo...	0.000	13.443	0	3378626	N.D.	1.077 #
11) T	2,4,5-TP ...	0.000	14.060	0	36756603	N.D.	29.290 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 03:36
Operator : UA
Sample : J3843-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:29:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

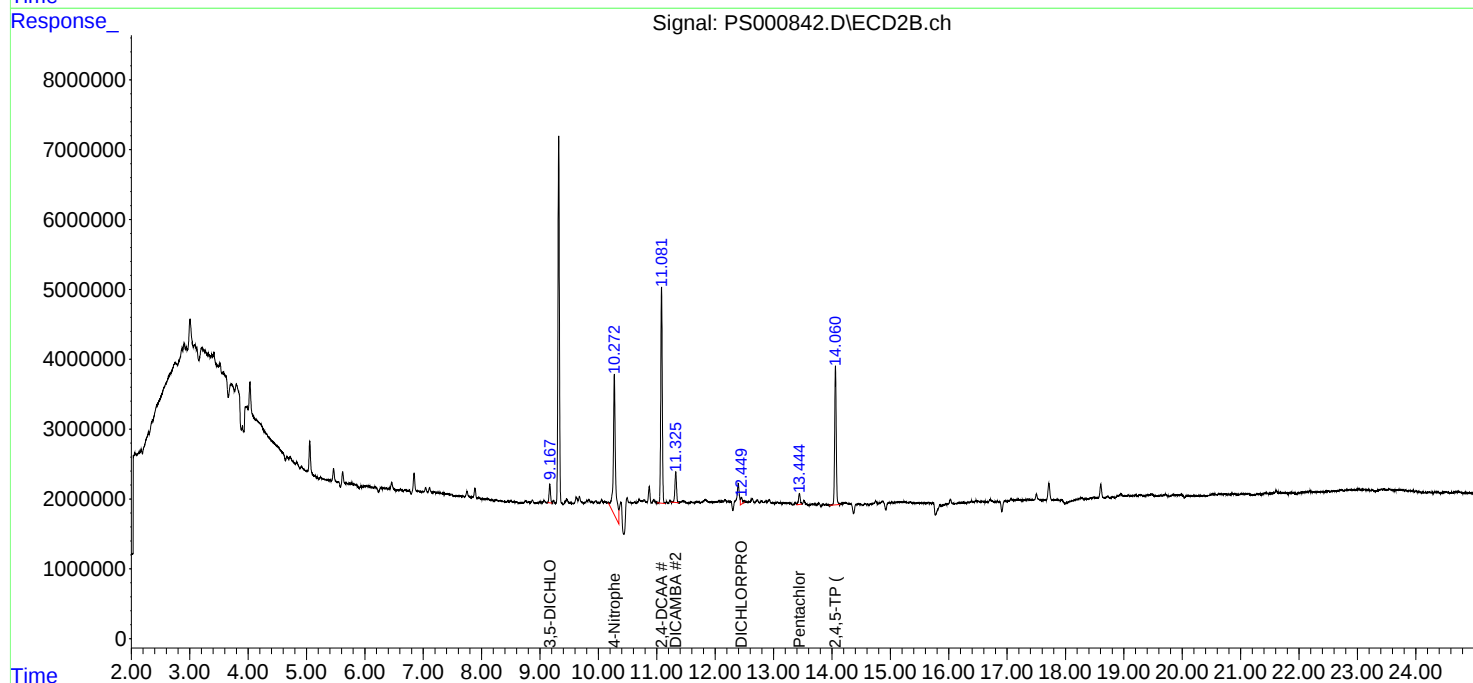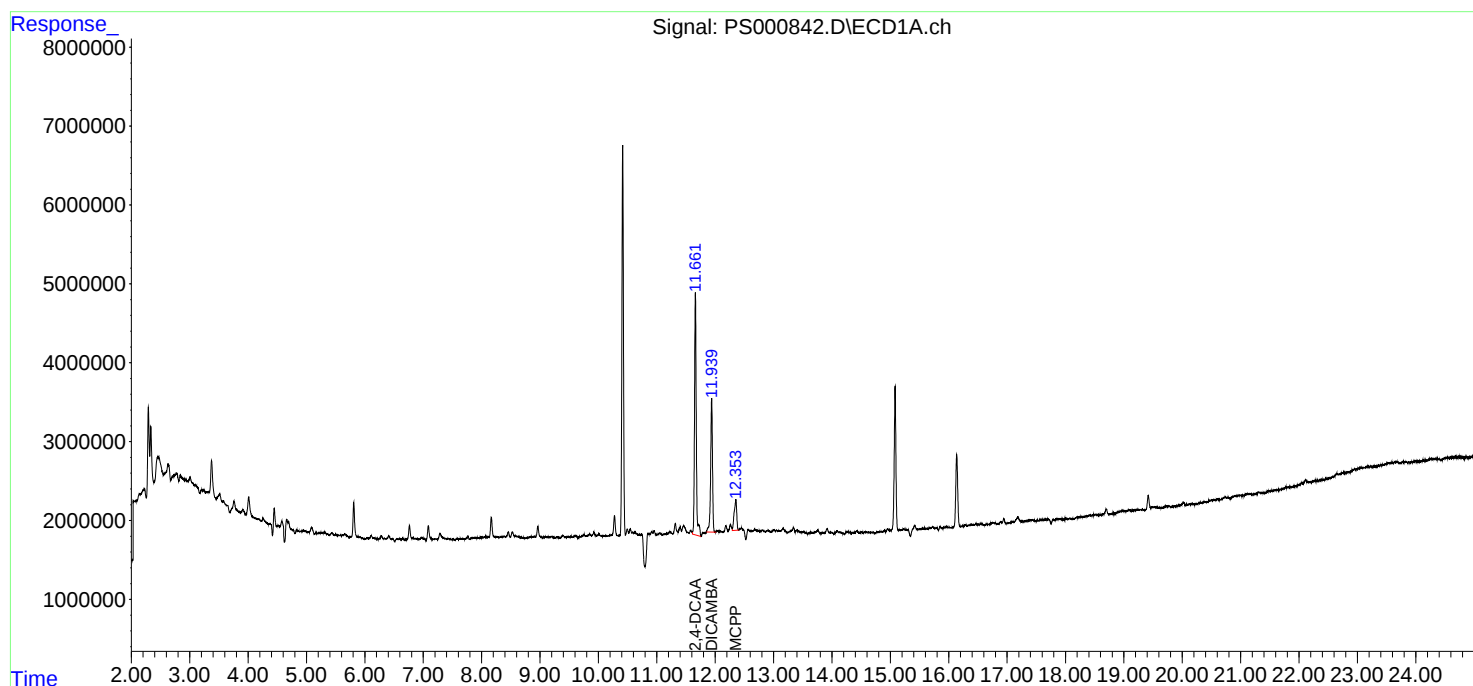


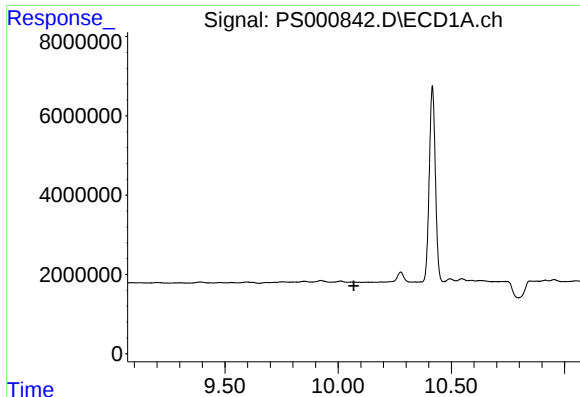

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

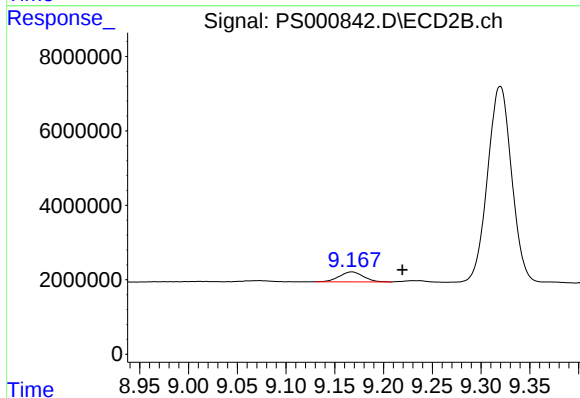


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.167 min
Delta R.T.: -0.052 min
Response: 4565709
Conc: 15.52 ng/ml

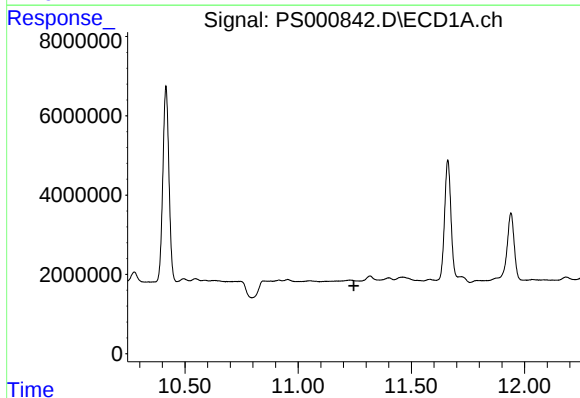


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

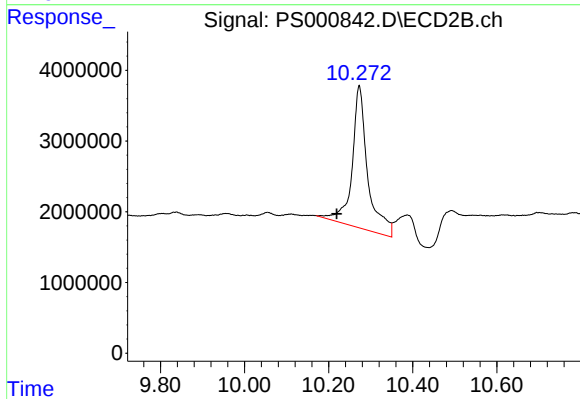

#3 4-Nitrophenol


R.T.: 10.273 min
Delta R.T.: 0.054 min
Response: 51759847
Conc: 428.95 ng/ml

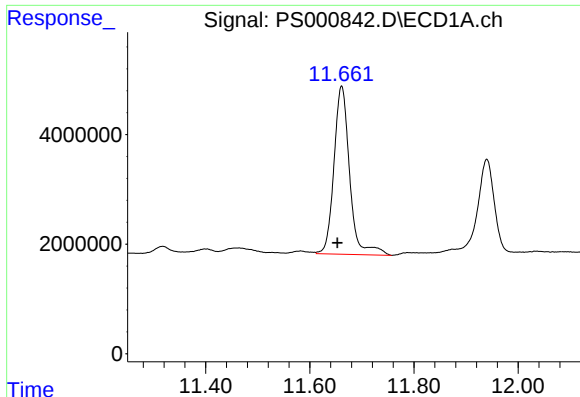

#4 2,4-DCAA


R.T.: 11.661 min
Delta R.T.: 0.008 min
Response: 64130156
Conc: 310.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

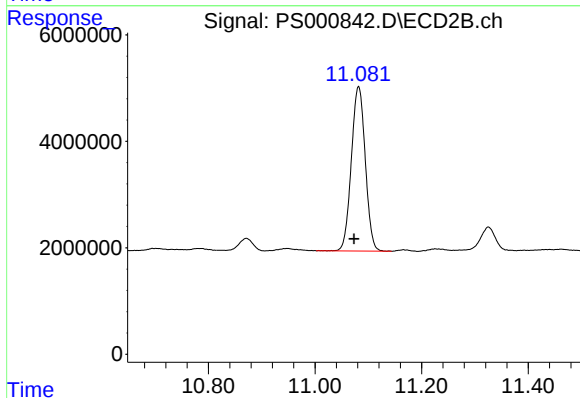


#4 2,4-DCAA

R.T.: 11.082 min
Delta R.T.: 0.008 min
Response: 55951540
Conc: 256.90 ng/ml

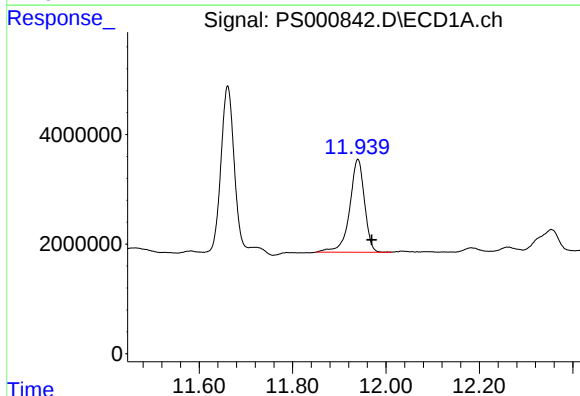


#5 DICAMBA

R.T.: 11.940 min
Delta R.T.: -0.030 min
Response: 37367305
Conc: 47.46 ng/ml

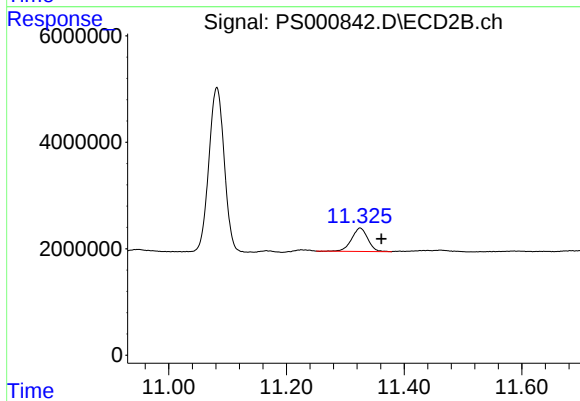

#5 DICAMBA


R.T.: 11.325 min
Delta R.T.: -0.036 min
Response: 8370969
Conc: 10.66 ng/ml

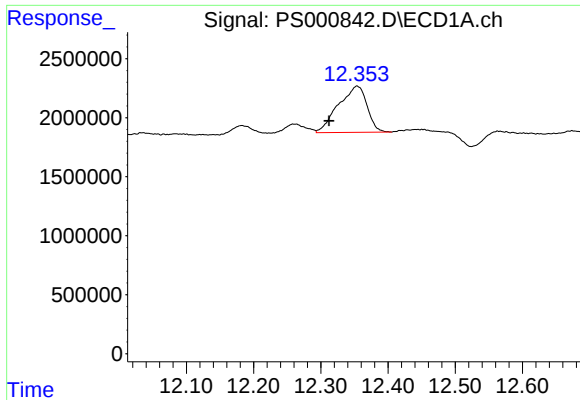

#6 MCP


R.T.: 12.354 min
Delta R.T.: 0.042 min
Response: 11574559
Conc: 21.07 ug/ml

Instrument :
ECD_S
ClientSampleId :

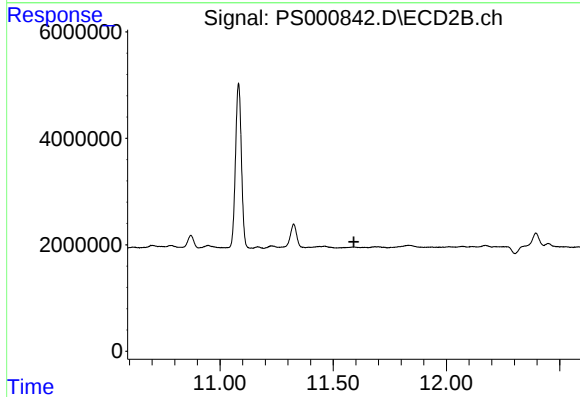


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

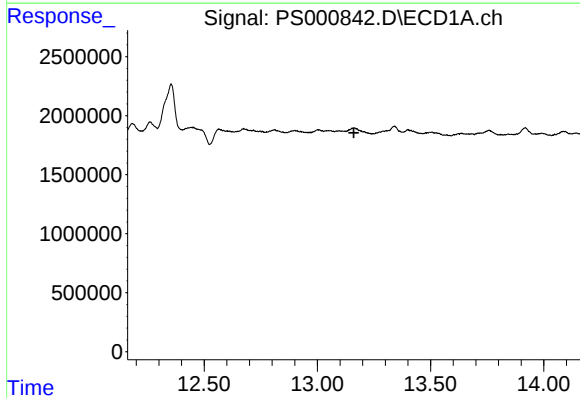


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

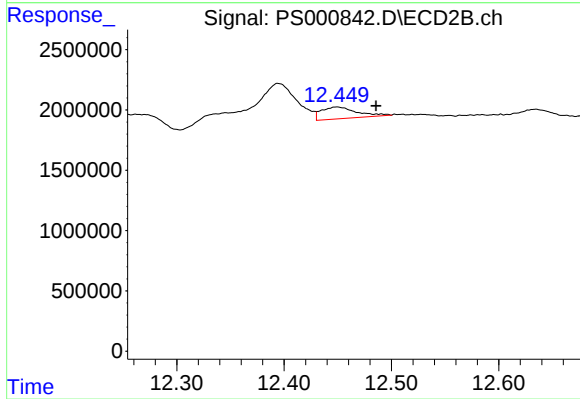

#8 DICHLORPROP


R.T.: 12.449 min
Delta R.T.: -0.037 min
Response: 2248854
Conc: 11.13 ng/ml

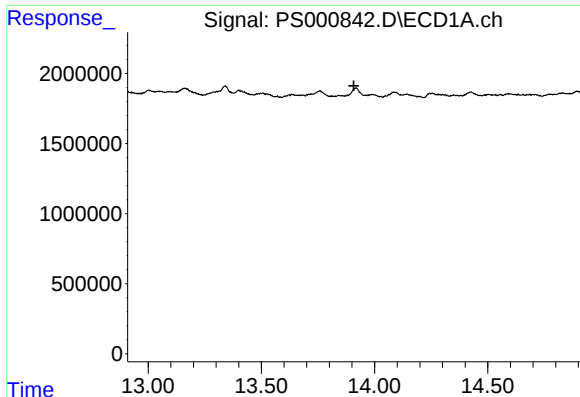

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

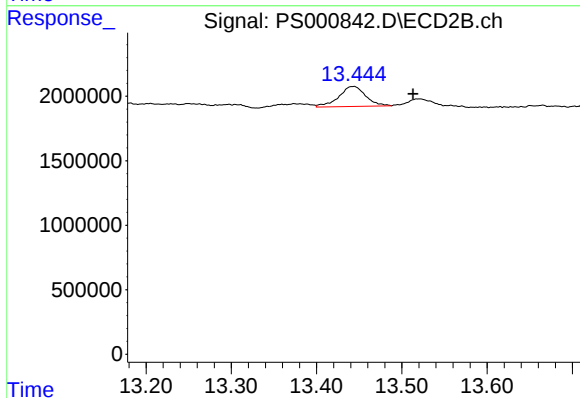


#10 Pentachlorophenol

R.T.: 13.443 min
Delta R.T.: -0.070 min
Response: 3378626
Conc: 1.08 ng/ml

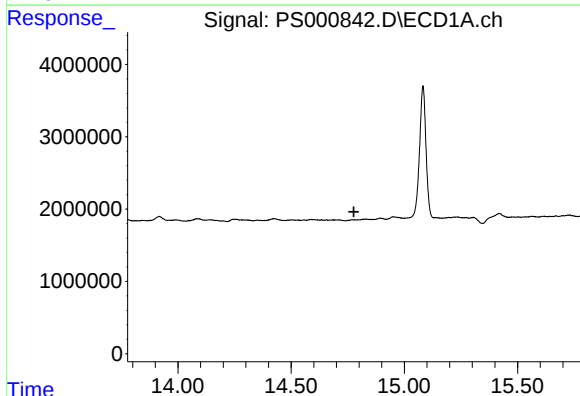

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

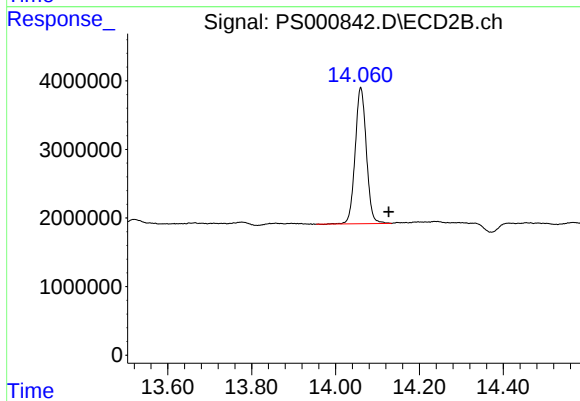

#11 2,4,5-TP (SILVEX)

R.T.: 14.060 min
Delta R.T.: -0.066 min
Response: 36756603
Conc: 29.29 ng/ml