

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000844.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 04:38
 Operator : UA
 Sample : J3852-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:30:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.649	11.068	66197571	58609070	320.849	269.099
Target Compounds							
1) T	Dalapon	0.000	2.443	0	1139302	N.D.	4.229 #
2) T	3,5-DICHL...	0.000	9.154	0	4889557	N.D.	16.622 #
3) T	4-Nitroph...	11.305	10.225	1730896	9112481	12.620	75.519 #
5) T	DICAMBA	11.901	11.312	3243983	7546461	4.120	9.614 #
6) T	MCP	12.342	0.000	12304528	0	22.401	N.D. #
8) T	DICHLORPROP	0.000	12.437	0	2443450	N.D.	12.098 #
11) T	2,4,5-TP ...	14.719	0.000	12346745	0	10.106	N.D. #
15) T	Picloram	0.000	17.009	0	9663524	N.D.	6.346 #
16) T	DCPA	0.000	17.009	0	9663524	N.D.	5.621 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000844.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 04:38
Operator : UA
Sample : J3852-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:30:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

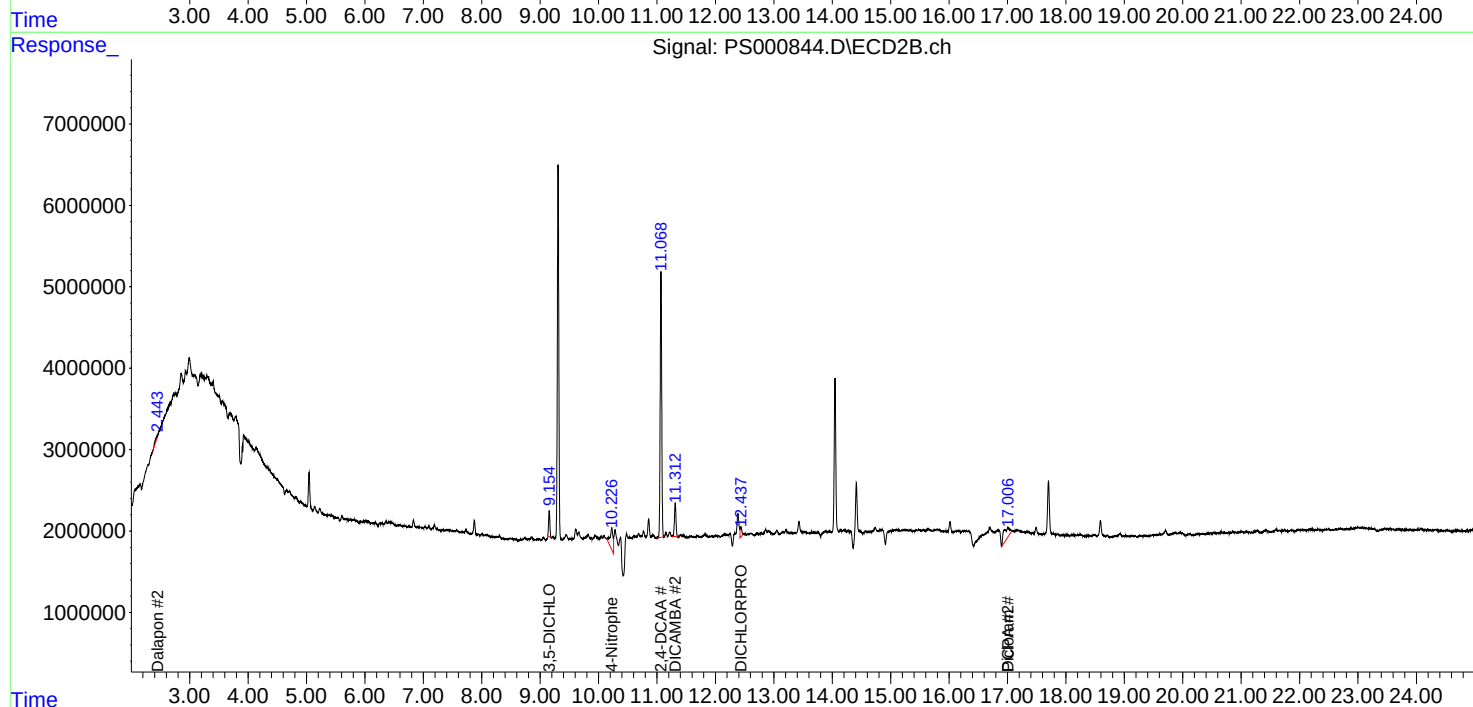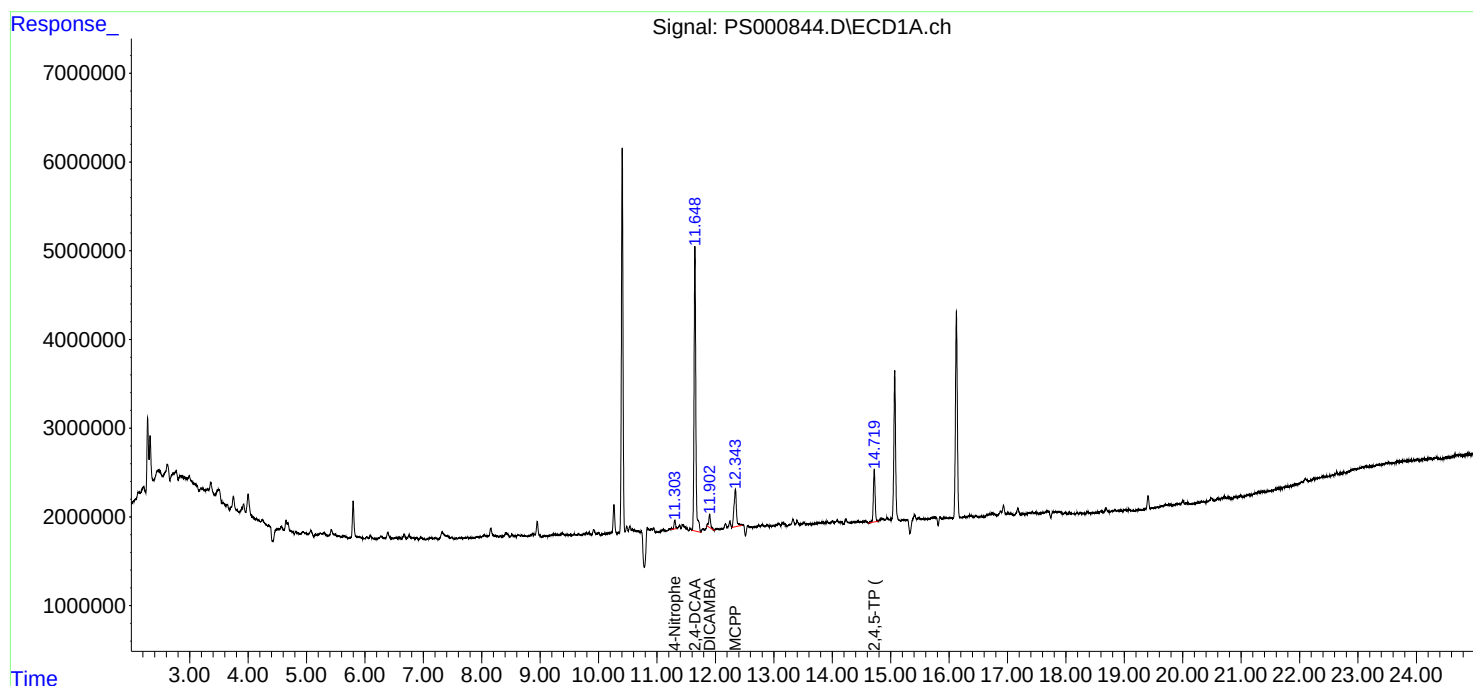


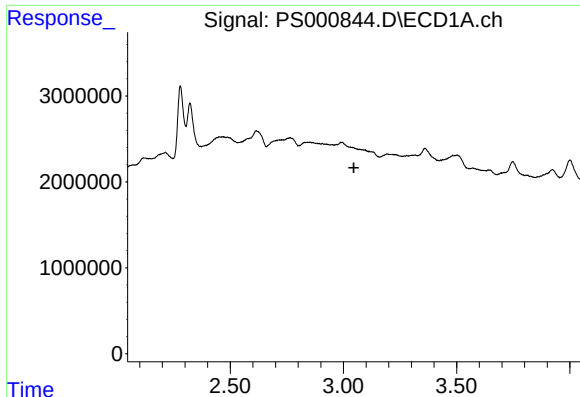

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.046 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

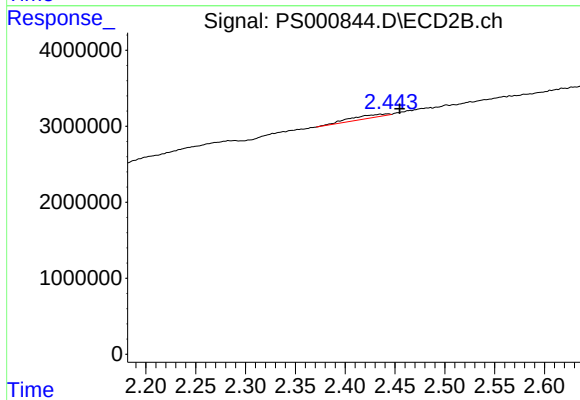


#1 Dalapon

R.T.: 2.443 min
Delta R.T.: -0.011 min
Response: 1139302
Conc: 4.23 ng/ml

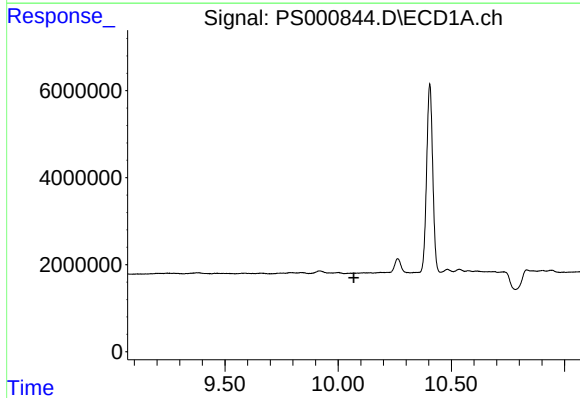


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.070 min
Response: 0
Conc: N.D.

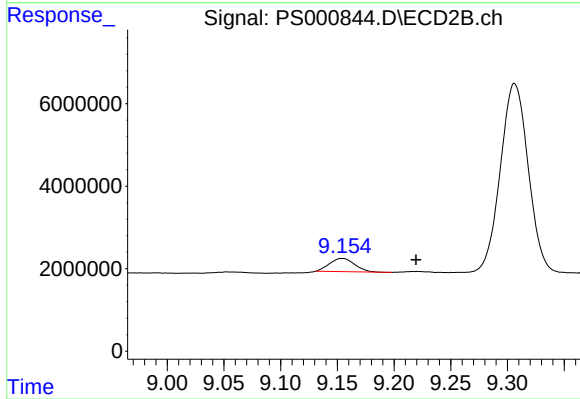

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.154 min
Delta R.T.: -0.065 min
Response: 4889557
Conc: 16.62 ng/ml

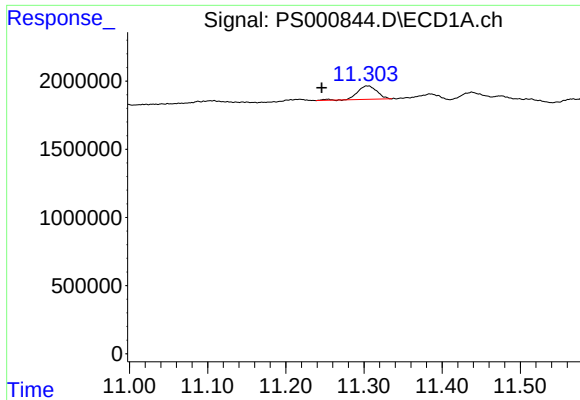

#3 4-Nitrophenol


R.T.: 11.305 min
Delta R.T.: 0.059 min
Response: 1730896
Conc: 12.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

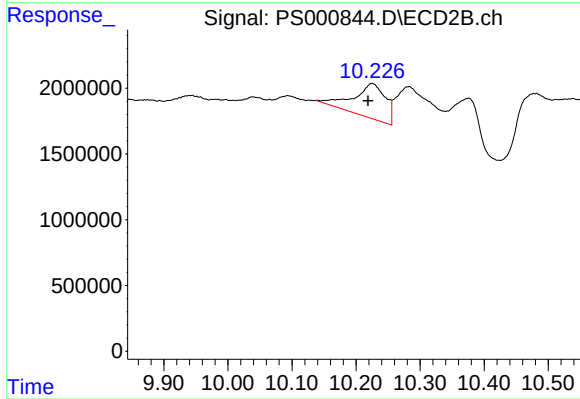


#3 4-Nitrophenol

R.T.: 10.225 min
Delta R.T.: 0.006 min
Response: 9112481
Conc: 75.52 ng/ml

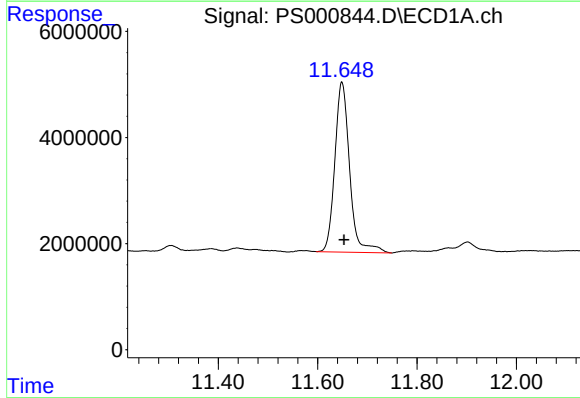


#4 2,4-DCAA

R.T.: 11.649 min
Delta R.T.: -0.004 min
Response: 66197571
Conc: 320.85 ng/ml

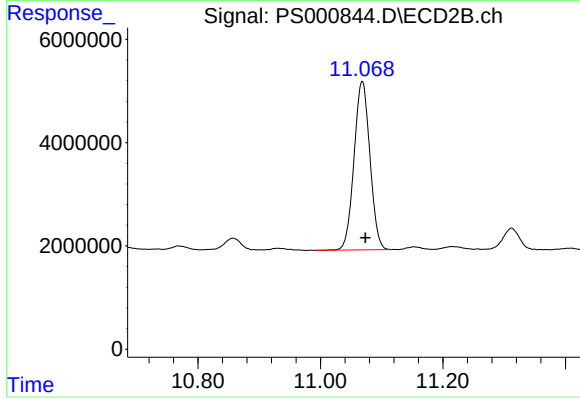

#4 2,4-DCAA


R.T.: 11.068 min
Delta R.T.: -0.005 min
Response: 58609070
Conc: 269.10 ng/ml

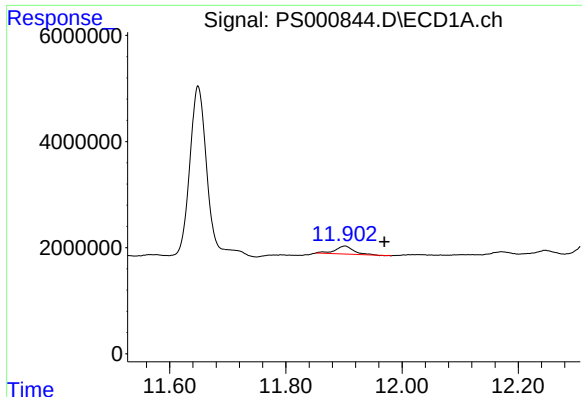

#5 DICAMBA


R.T.: 11.901 min
Delta R.T.: -0.068 min
Response: 3243983
Conc: 4.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

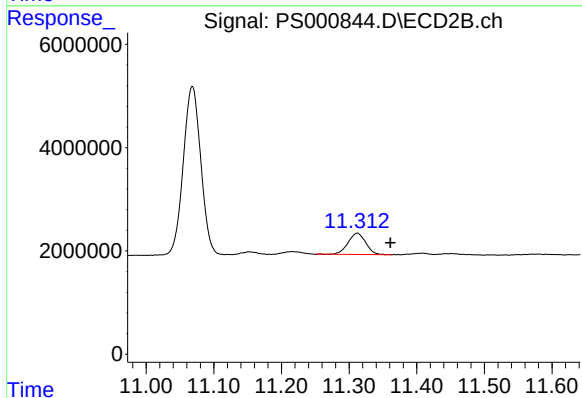


#5 DICAMBA

R.T.: 11.312 min
Delta R.T.: -0.049 min
Response: 7546461
Conc: 9.61 ng/ml

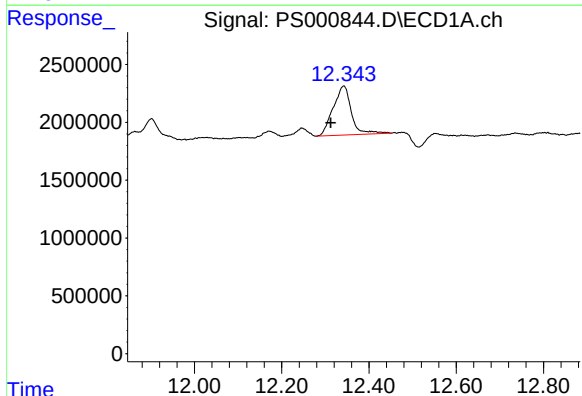


#6 MCP

R.T.: 12.342 min
Delta R.T.: 0.030 min
Response: 12304528
Conc: 22.40 ug/ml

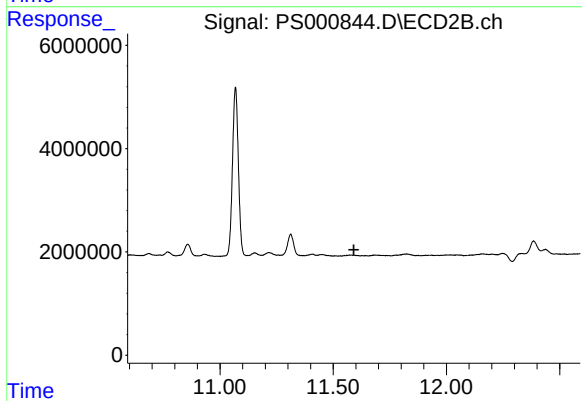

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

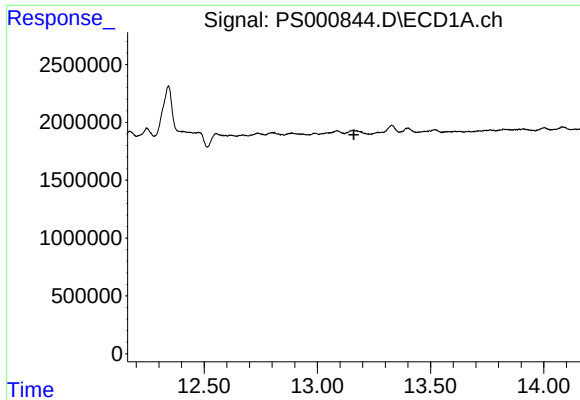

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

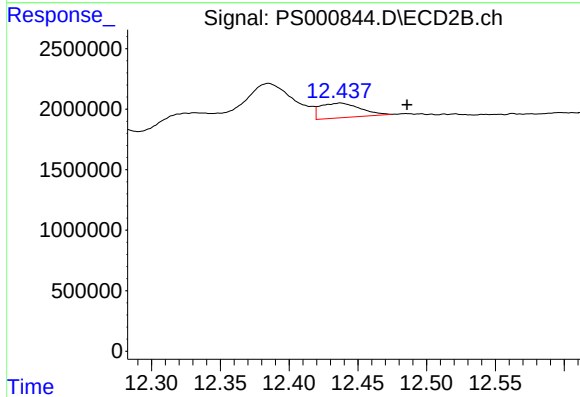


#8 DICHLORPROP

R.T.: 12.437 min
Delta R.T.: -0.048 min
Response: 2443450
Conc: 12.10 ng/ml

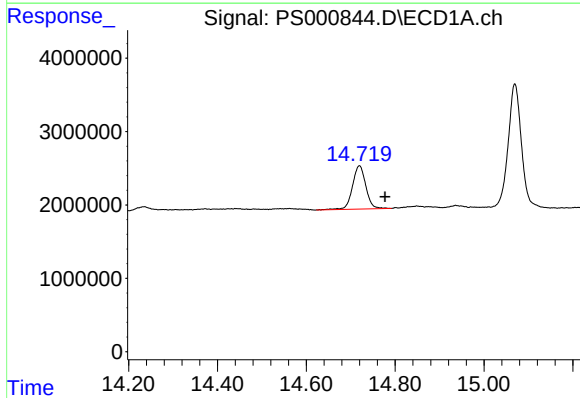


#11 2,4,5-TP (SILVEX)

R.T.: 14.719 min
Delta R.T.: -0.058 min
Response: 12346745
Conc: 10.11 ng/ml

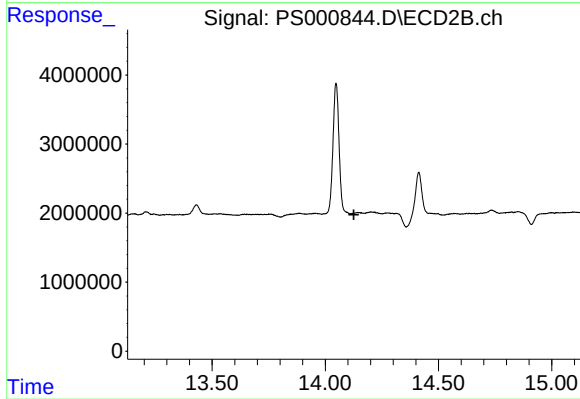

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.126 min
Response: 0
Conc: N.D.

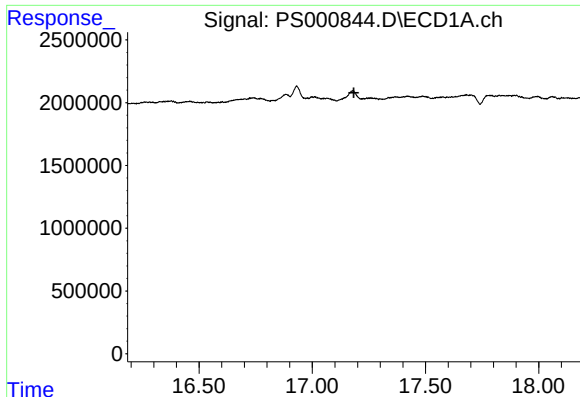

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

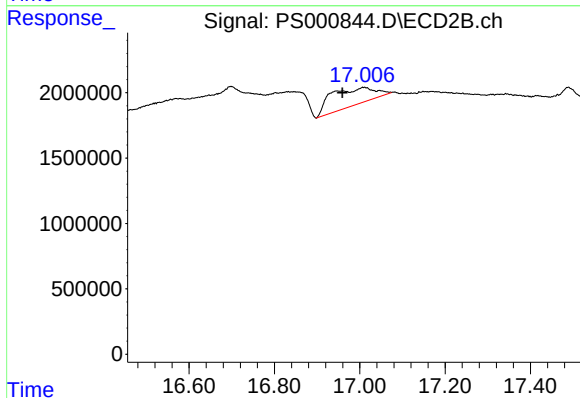


#15 Picloram

R.T.: 17.009 min
Delta R.T.: 0.050 min
Response: 9663524
Conc: 6.35 ng/ml

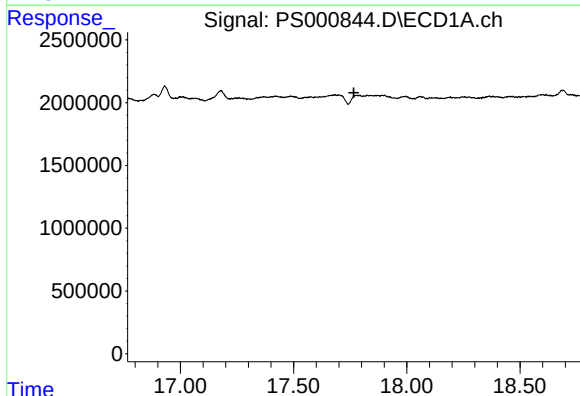

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

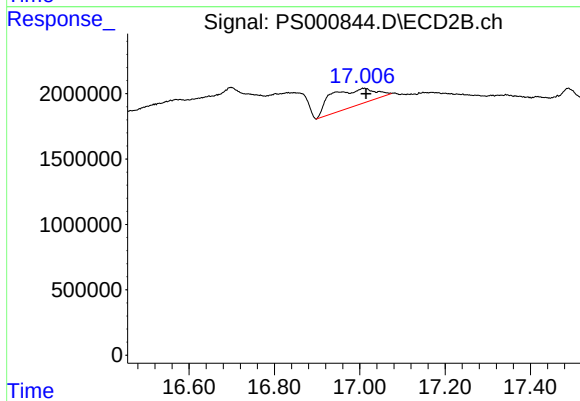

#16 DCPA

R.T.: 17.009 min
Delta R.T.: -0.006 min
Response: 9663524
Conc: 5.62 ng/ml