

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 05:40
 Operator : UA
 Sample : J3854-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:31:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.652	11.069	65993505	58775232	319.860	269.862
Target Compounds							
2) T	3,5-DICHL...	0.000	9.155	0	4390676	N.D.	14.926 #
5) T	DICAMBA	11.904	11.313	3142520	5755785	3.991	7.333 #
6) T	MCP	12.346	0.000	6278015	0	11.429	N.D. #
8) T	DICHLORPROP	0.000	12.435	0	2150549	N.D.	10.647 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 05:40
Operator : UA
Sample : J3854-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:31:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

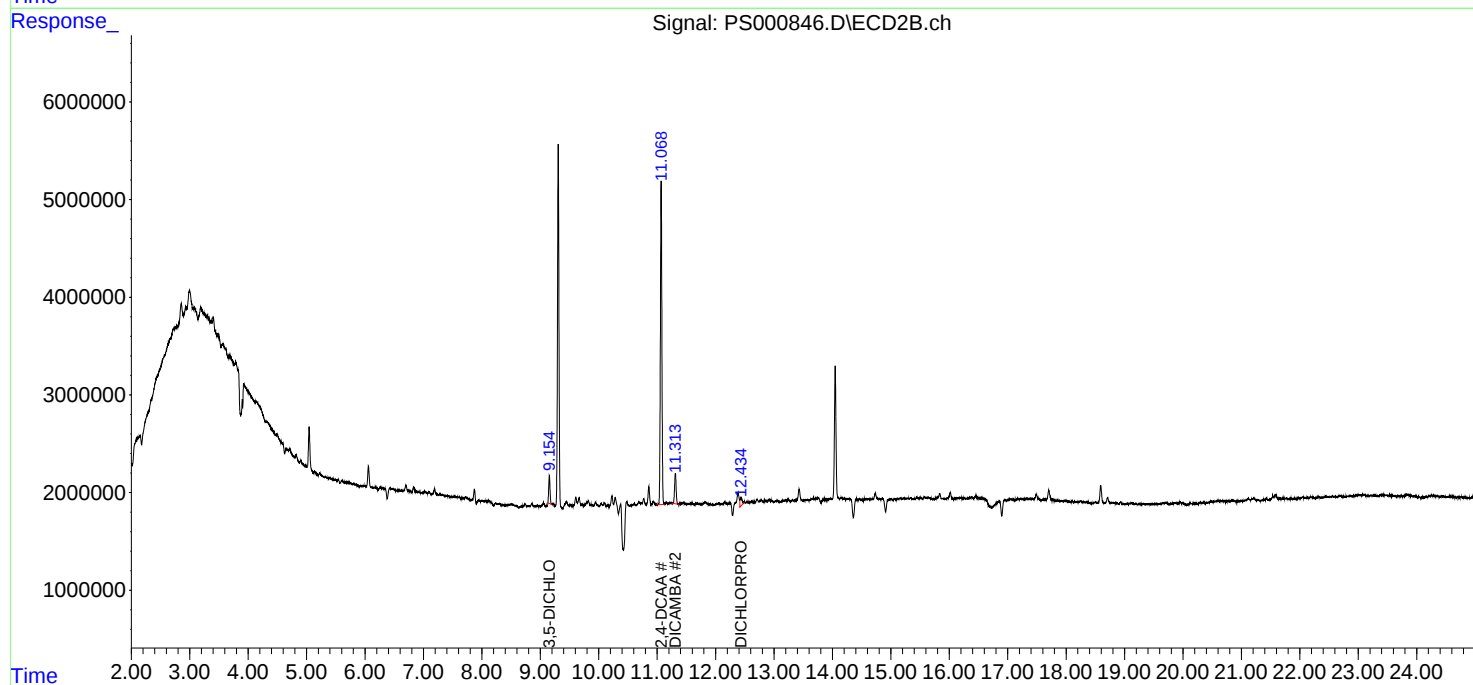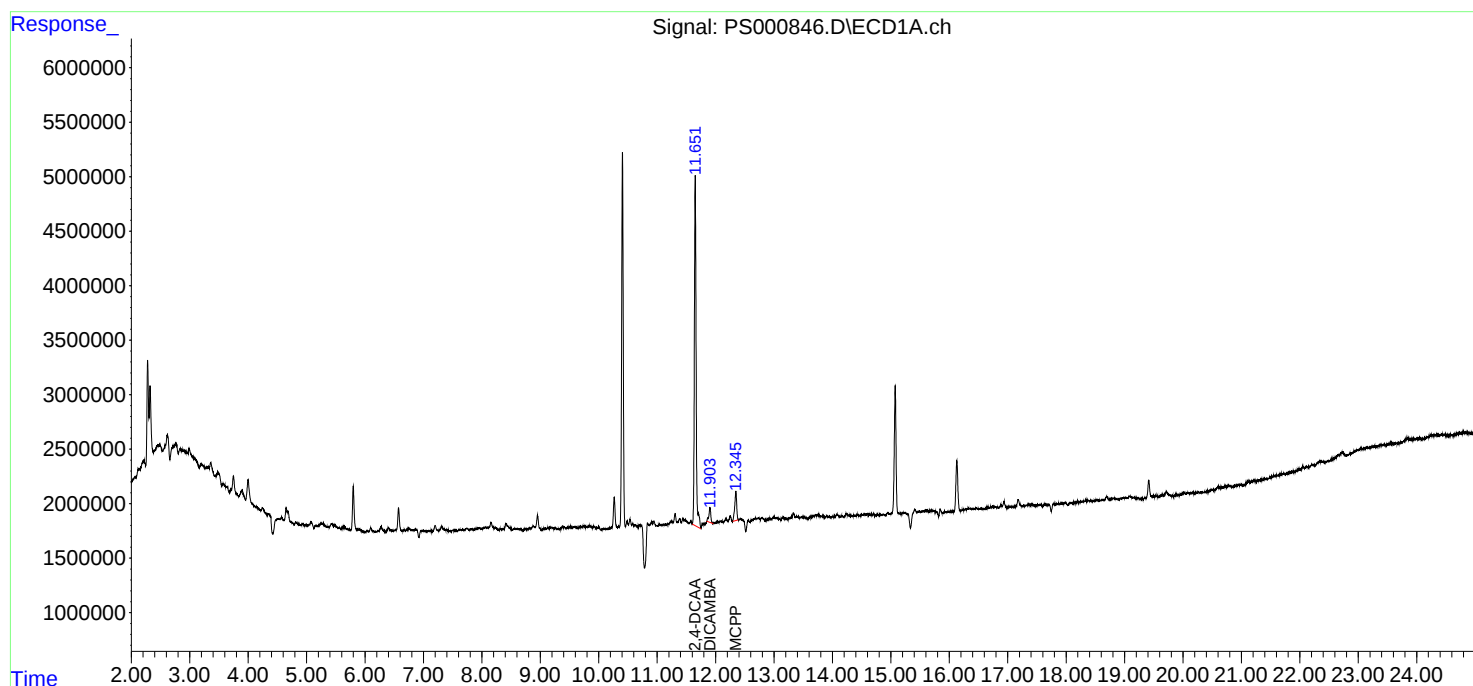


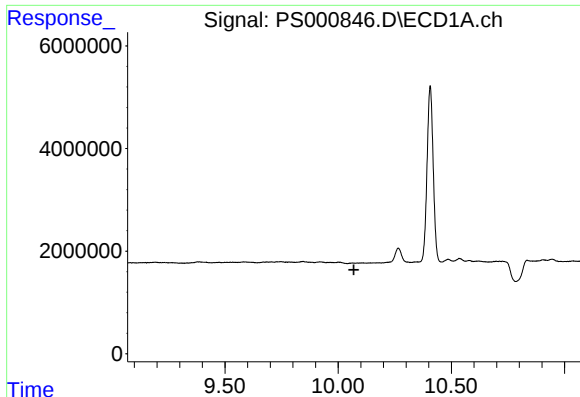

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

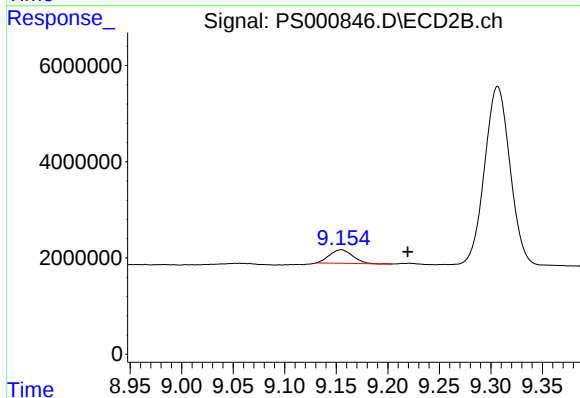


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.155 min
Delta R.T.: -0.065 min
Response: 4390676
Conc: 14.93 ng/ml

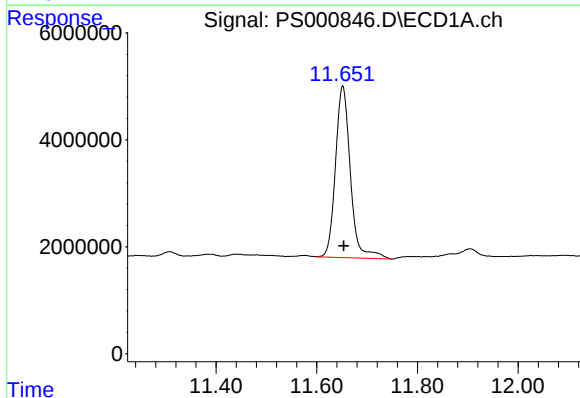


#4 2,4-DCAA

R.T.: 11.652 min
Delta R.T.: -0.002 min
Response: 65993505
Conc: 319.86 ng/ml

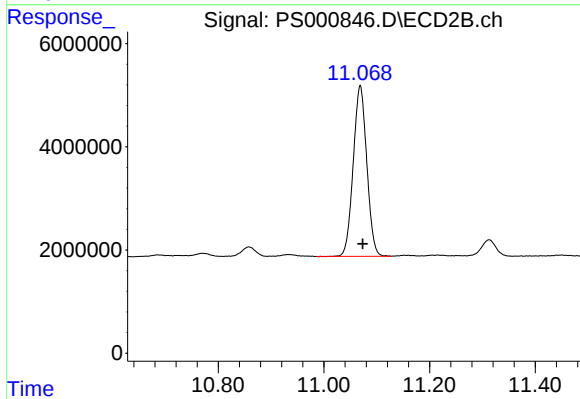

#4 2,4-DCAA


R.T.: 11.069 min
Delta R.T.: -0.005 min
Response: 58775232
Conc: 269.86 ng/ml

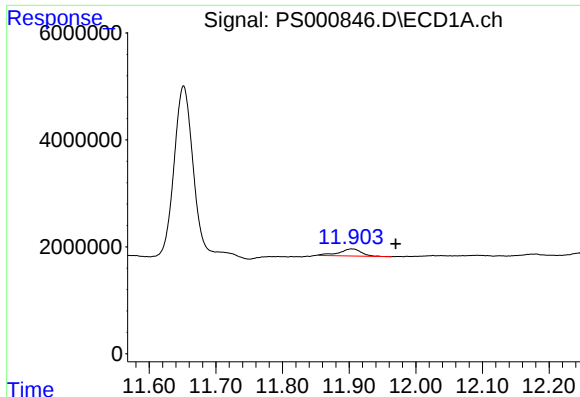

#5 DICAMBA


R.T.: 11.904 min
Delta R.T.: -0.066 min
Response: 3142520
Conc: 3.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

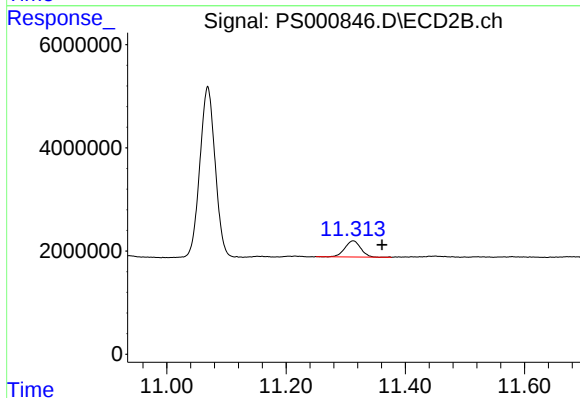


#5 DICAMBA

R.T.: 11.313 min
Delta R.T.: -0.048 min
Response: 5755785
Conc: 7.33 ng/ml

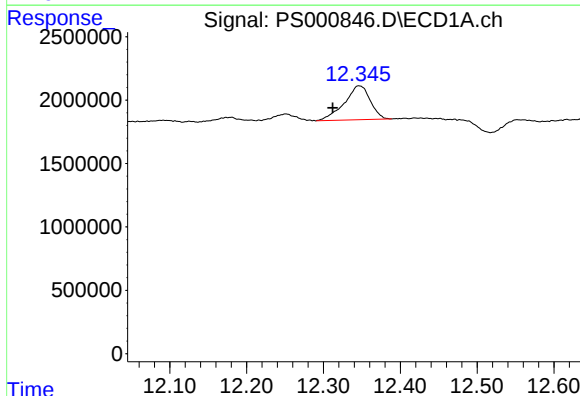


#6 MCP

R.T.: 12.346 min
Delta R.T.: 0.034 min
Response: 6278015
Conc: 11.43 ug/ml

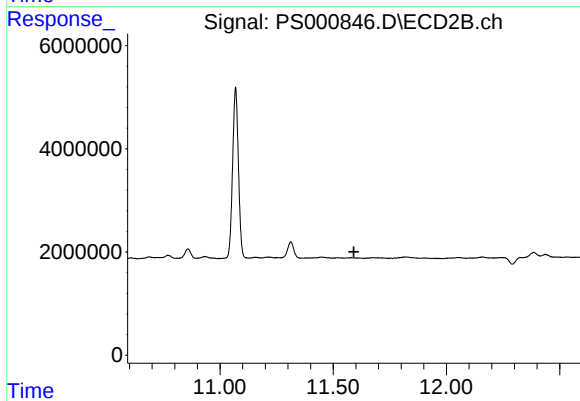

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

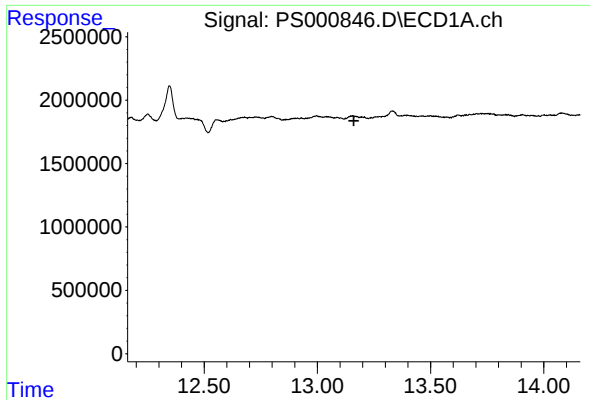

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

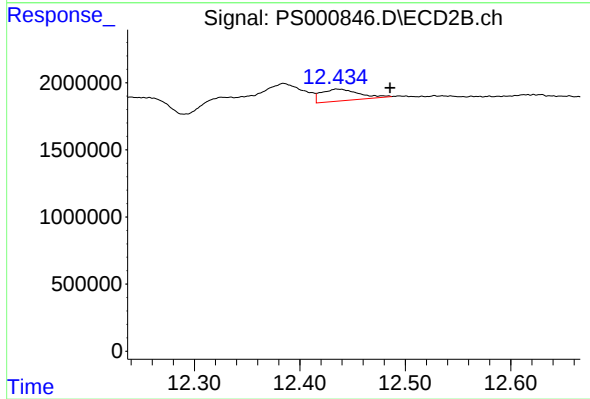

#8 DICHLORPROP

R.T.: 12.435 min
Delta R.T.: -0.050 min
Response: 2150549
Conc: 10.65 ng/ml