

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 06:11
 Operator : UA
 Sample : J3854-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:31:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.655	11.053	69940828	63143825	338.992	289.920
Target Compounds							
3) T	4-Nitroph...	0.000	10.209	0	4809820	N.D.	39.861 #
5) T	DICAMBA	11.908	11.297	3985109	6400239	5.061	8.154 #
6) T	MCP	12.351	0.000	7357555	0	13.395	N.D. #
8) T	DICHLORPROP	0.000	12.420	0	2291865	N.D.	11.347 #
12) T	2,4,5-T	0.000	14.718	0	3908025	N.D.	3.777 #
15) T	Picloram	0.000	17.010	0	8860742	N.D.	5.819 #
16) T	DCPA	0.000	17.010	0	8860742	N.D.	5.154 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 06:11
Operator : UA
Sample : J3854-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:31:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

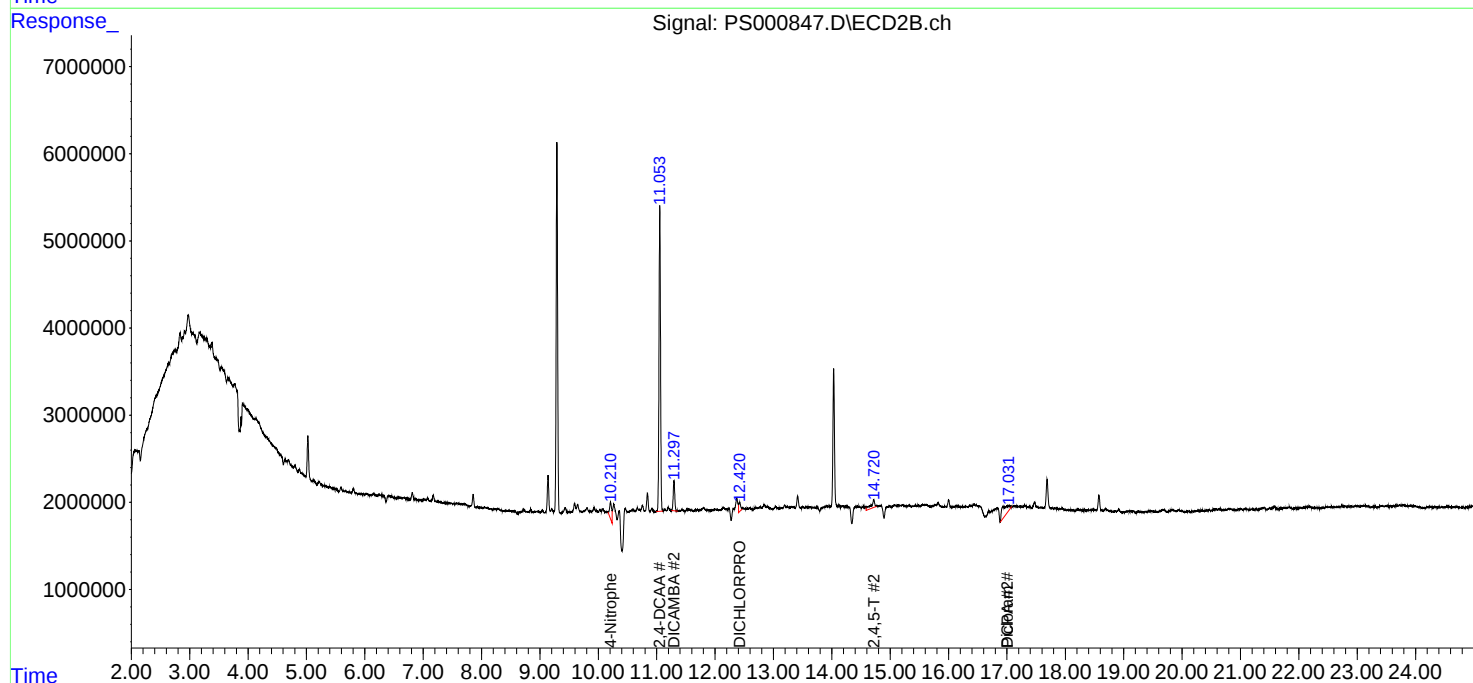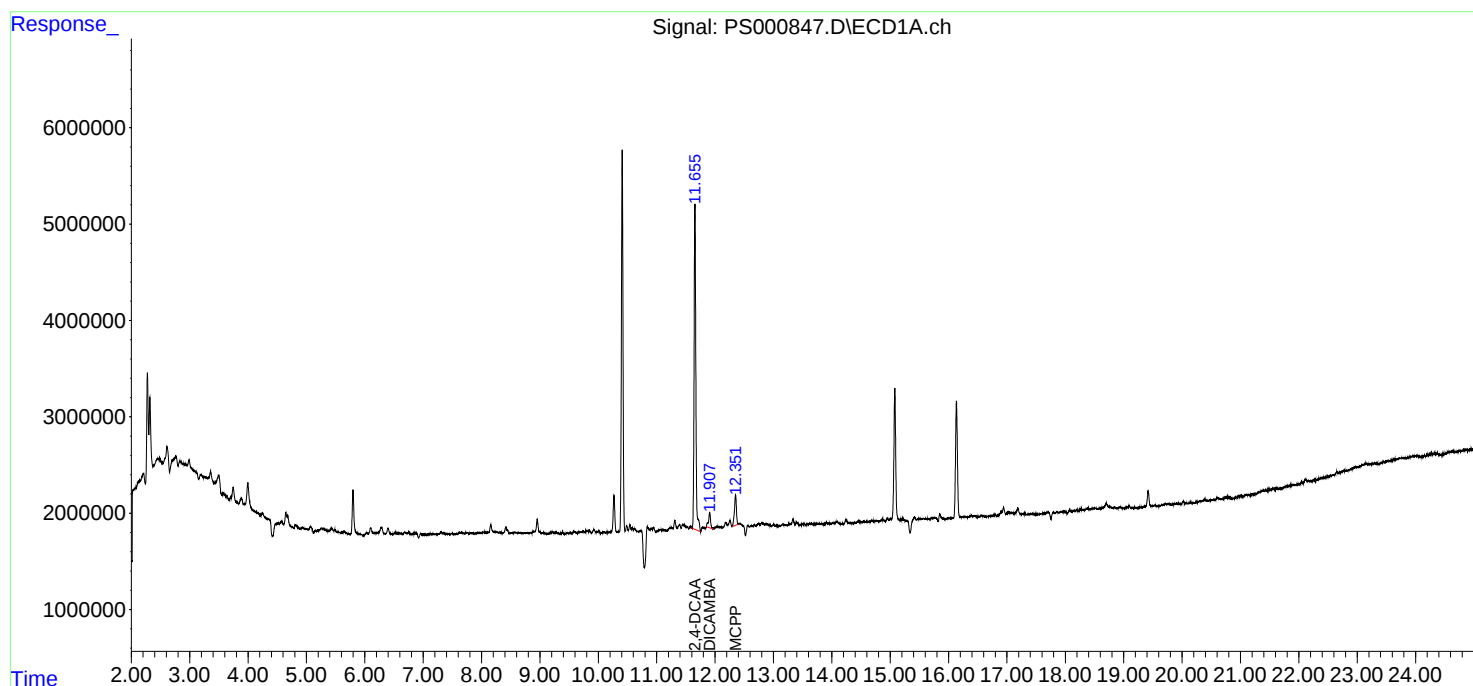


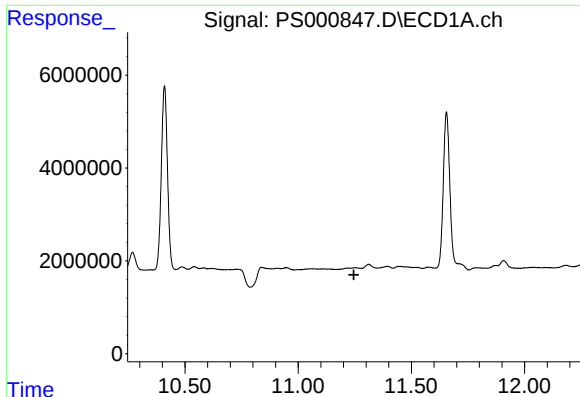

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

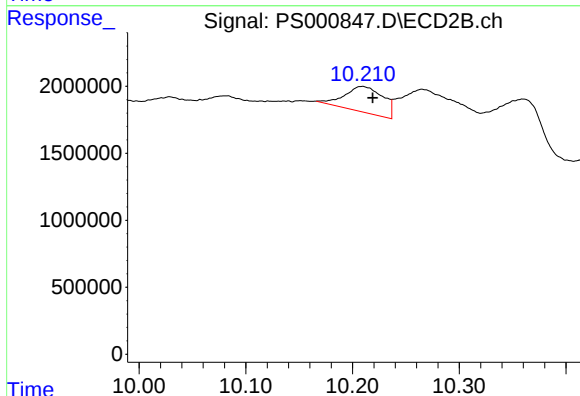


#3 4-Nitrophenol

R.T.: 10.209 min
Delta R.T.: -0.010 min
Response: 4809820
Conc: 39.86 ng/ml

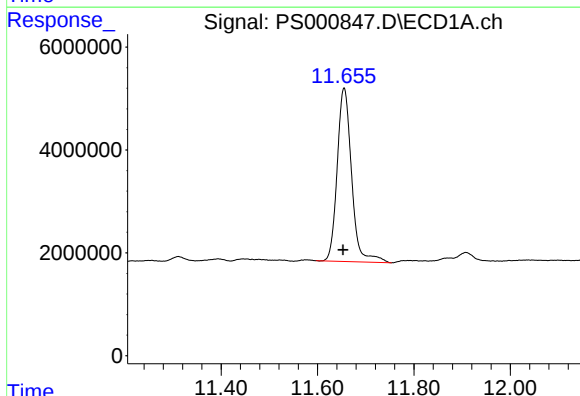


#4 2,4-DCAA

R.T.: 11.655 min
Delta R.T.: 0.002 min
Response: 69940828
Conc: 338.99 ng/ml

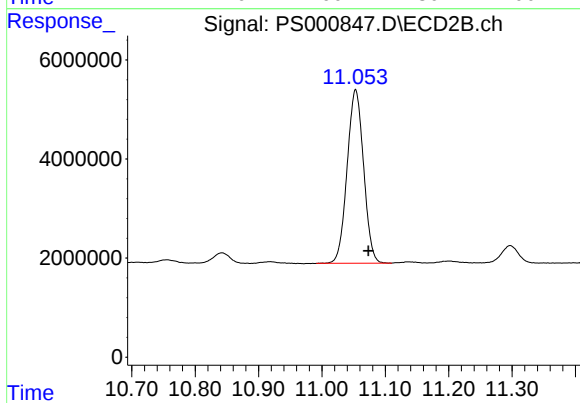

#4 2,4-DCAA


R.T.: 11.053 min
Delta R.T.: -0.020 min
Response: 63143825
Conc: 289.92 ng/ml

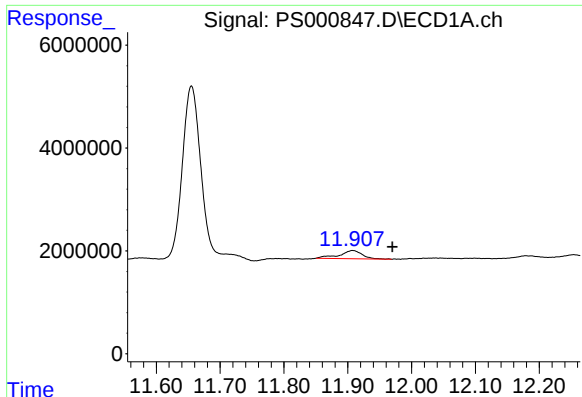

#5 DICAMBA


R.T.: 11.908 min
Delta R.T.: -0.062 min
Response: 3985109
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

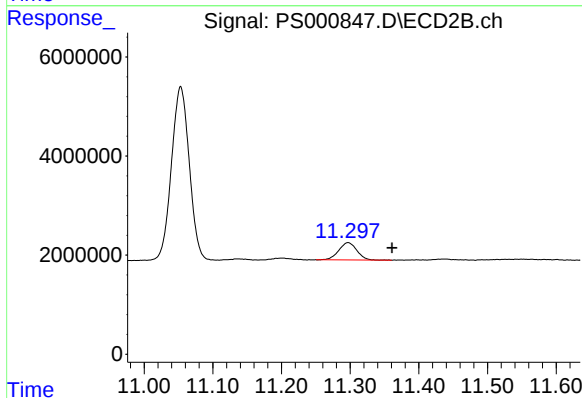


#5 DICAMBA

R.T.: 11.297 min
Delta R.T.: -0.064 min
Response: 6400239
Conc: 8.15 ng/ml

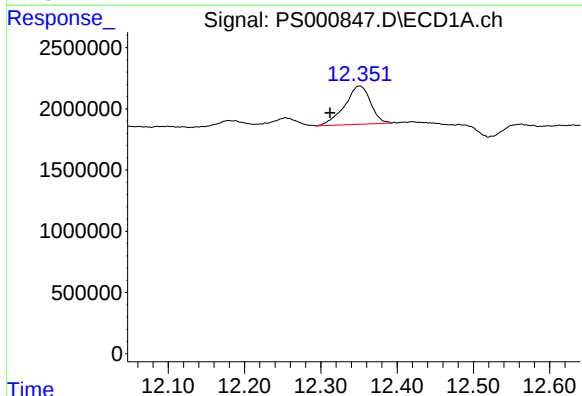


#6 MCP

R.T.: 12.351 min
Delta R.T.: 0.039 min
Response: 7357555
Conc: 13.39 ug/ml

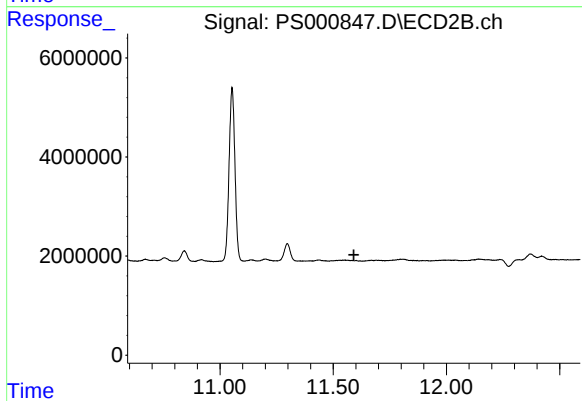

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

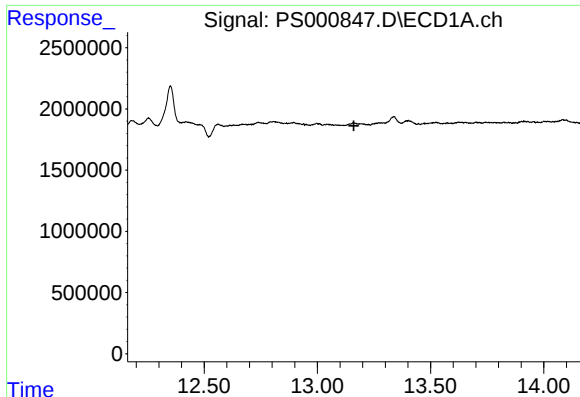

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

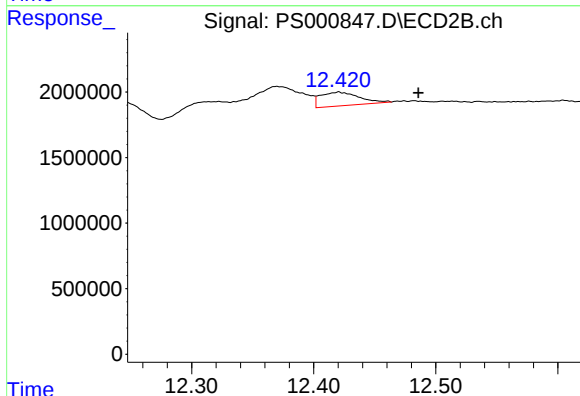


#8 DICHLORPROP

R.T.: 12.420 min
Delta R.T.: -0.065 min
Response: 2291865
Conc: 11.35 ng/ml

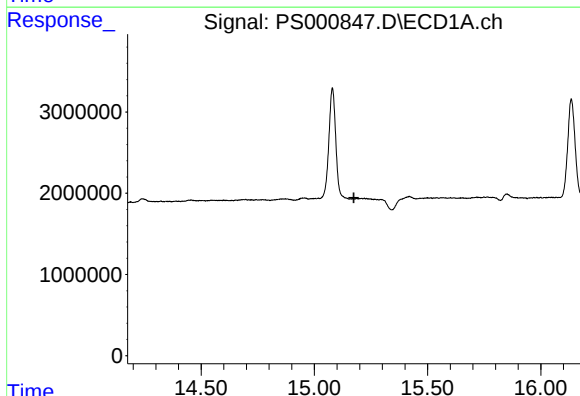


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.174 min
Response: 0
Conc: N.D.

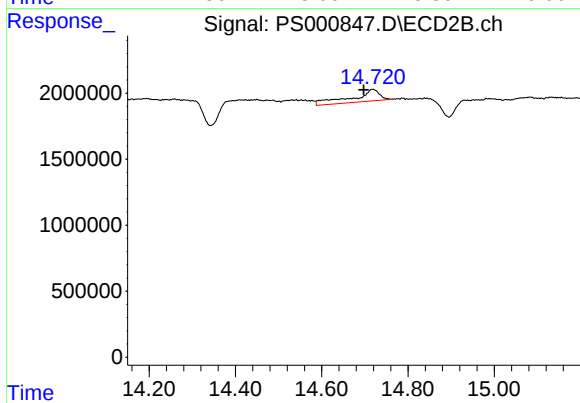

#12 2,4,5-T


R.T.: 14.718 min
Delta R.T.: 0.021 min
Response: 3908025
Conc: 3.78 ng/ml

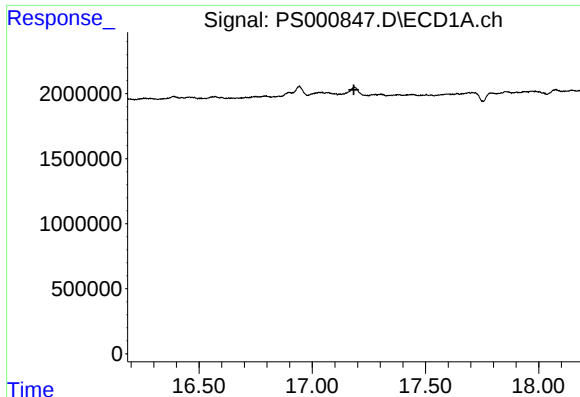

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

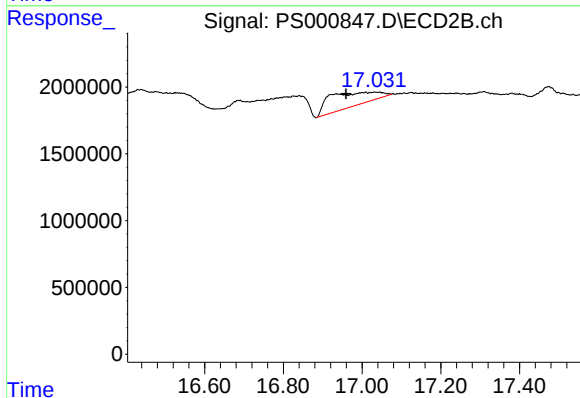


#15 Picloram

R.T.: 17.010 min
Delta R.T.: 0.051 min
Response: 8860742
Conc: 5.82 ng/ml

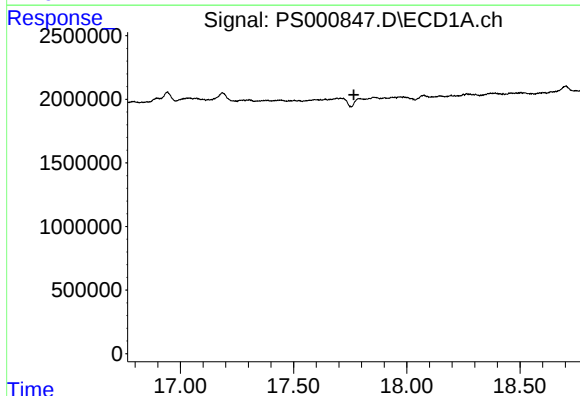

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

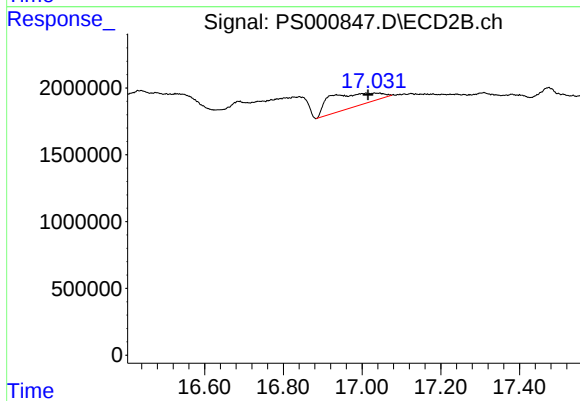

#16 DCPA

R.T.: 17.010 min
Delta R.T.: -0.005 min
Response: 8860742
Conc: 5.15 ng/ml