

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 07:44
 Operator : UA
 Sample : J3868-12
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:32:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.666	11.094	83451597	74843903	404.476	343.641
Target Compounds							
2) T	3,5-DICHL...	0.000	9.179	0	5759843	N.D.	19.581 #
3) T	4-Nitroph...	0.000	10.251	0	5284301	N.D.	43.793 #
5) T	DICAMBA	11.918	11.338	4458674	8180180	5.663	10.421 #
6) T	MCP	12.361	0.000	9123630	0	16.610	N.D. #
8) T	DICHLORPROP	0.000	12.462	0	2398095	N.D.	11.873 #
10) T	Pentachlo...	0.000	13.456	0	3468700	N.D.	1.105 #
11) T	2,4,5-TP ...	0.000	14.073	0	38684486	N.D.	30.826 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 07:44
Operator : UA
Sample : J3868-12
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:32:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

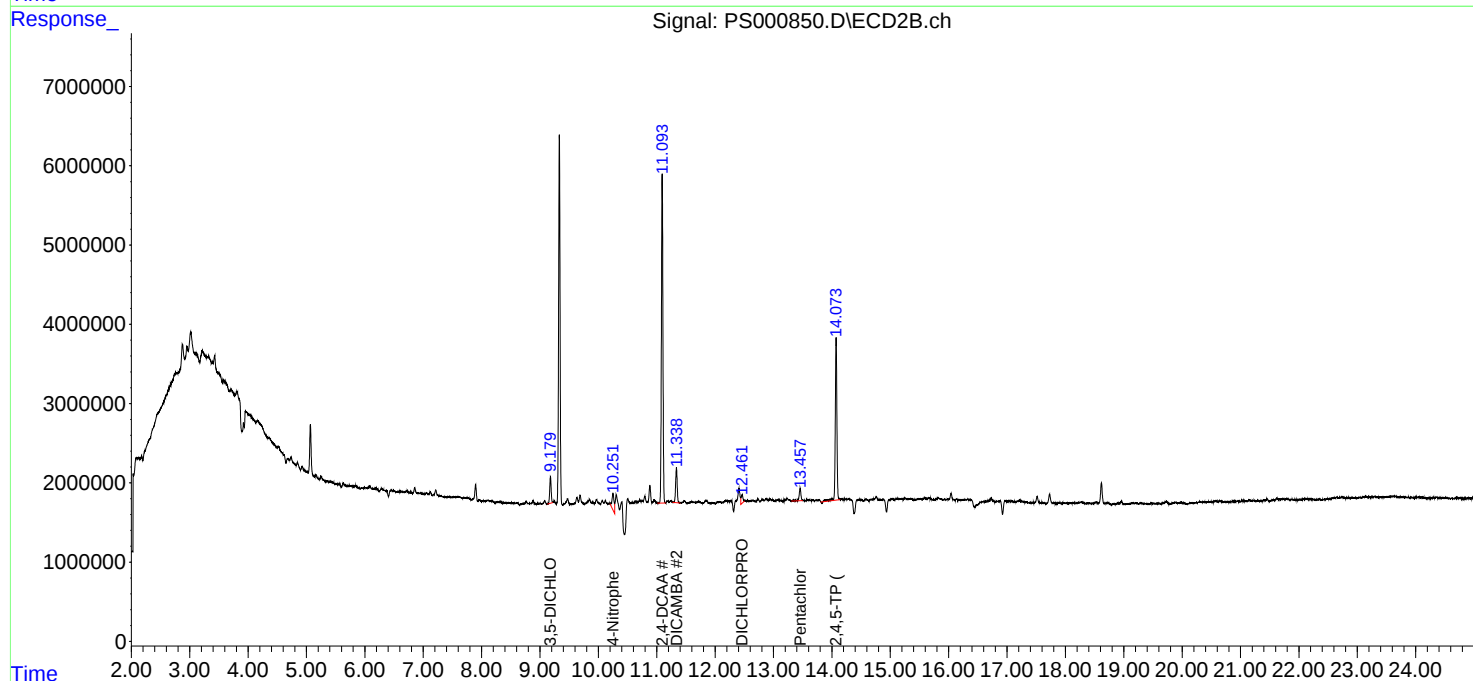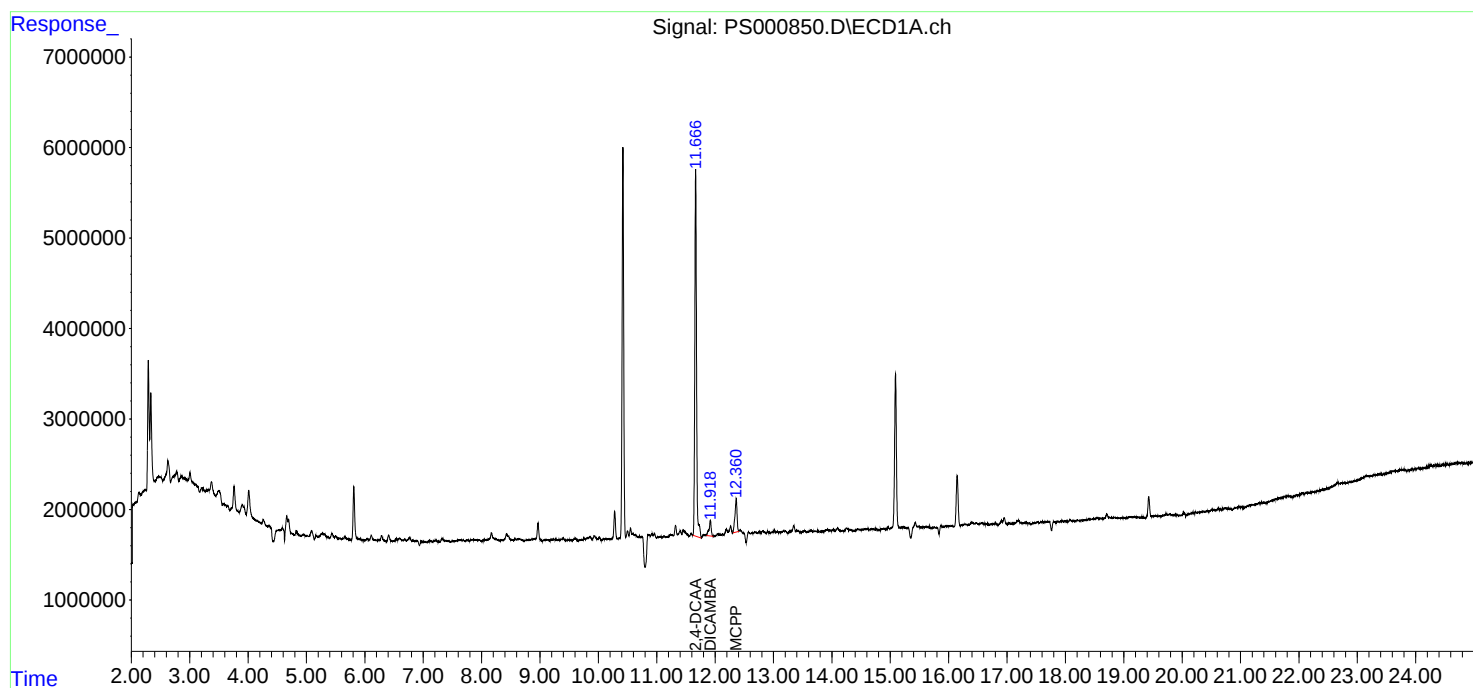


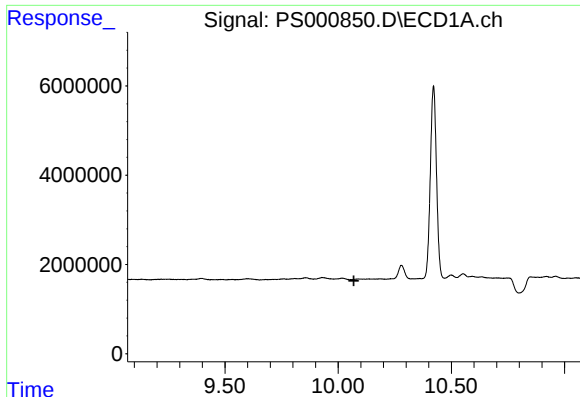

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

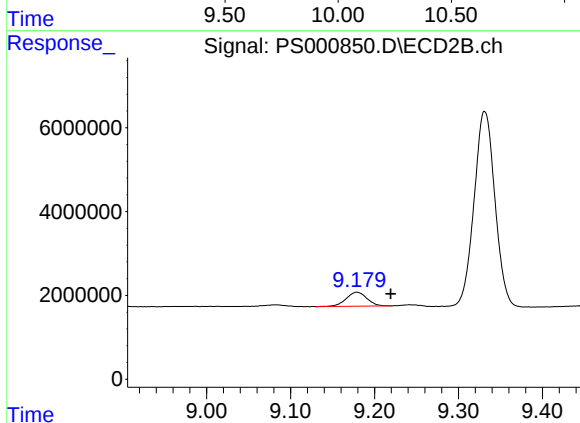


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.179 min
Delta R.T.: -0.040 min
Response: 5759843
Conc: 19.58 ng/ml

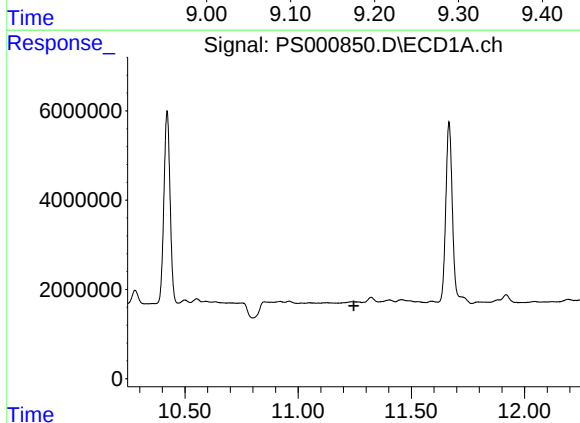


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

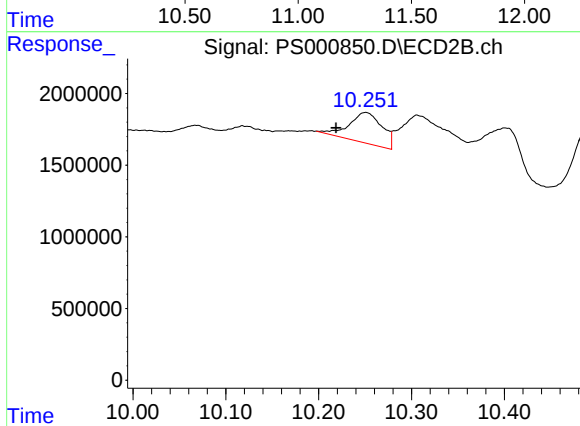

#3 4-Nitrophenol


R.T.: 10.251 min
Delta R.T.: 0.032 min
Response: 5284301
Conc: 43.79 ng/ml

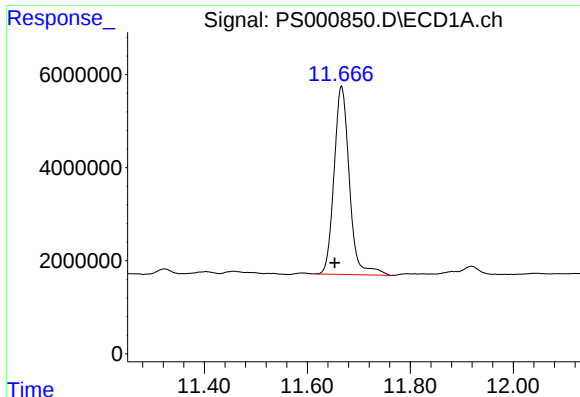

#4 2,4-DCAA


R.T.: 11.666 min
Delta R.T.: 0.013 min
Response: 83451597
Conc: 404.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

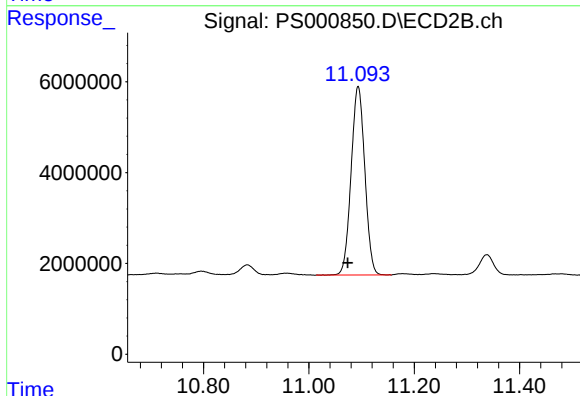


#4 2,4-DCAA

R.T.: 11.094 min
Delta R.T.: 0.020 min
Response: 74843903
Conc: 343.64 ng/ml

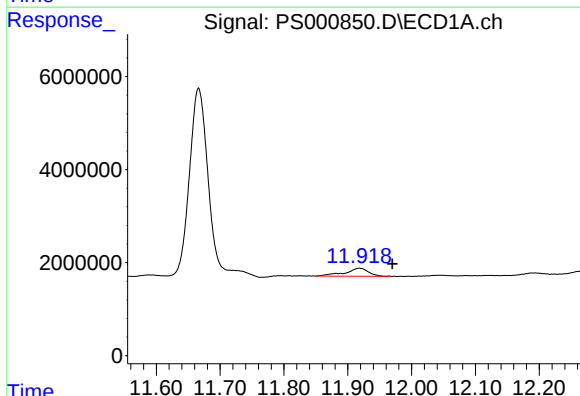


#5 DICAMBA

R.T.: 11.918 min
Delta R.T.: -0.051 min
Response: 4458674
Conc: 5.66 ng/ml

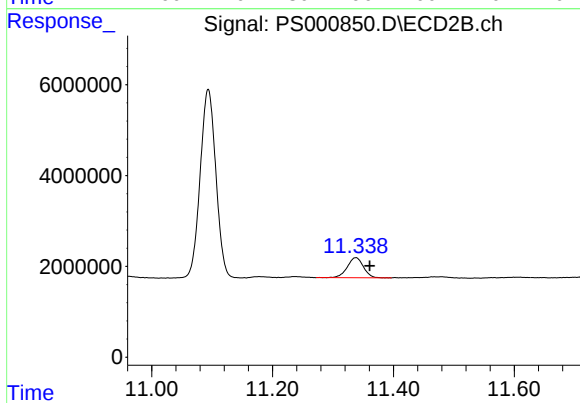

#5 DICAMBA


R.T.: 11.338 min
Delta R.T.: -0.024 min
Response: 8180180
Conc: 10.42 ng/ml

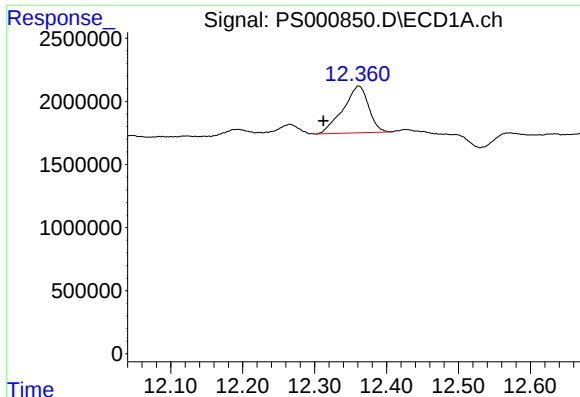

#6 MCP


R.T.: 12.361 min
Delta R.T.: 0.049 min
Response: 9123630
Conc: 16.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

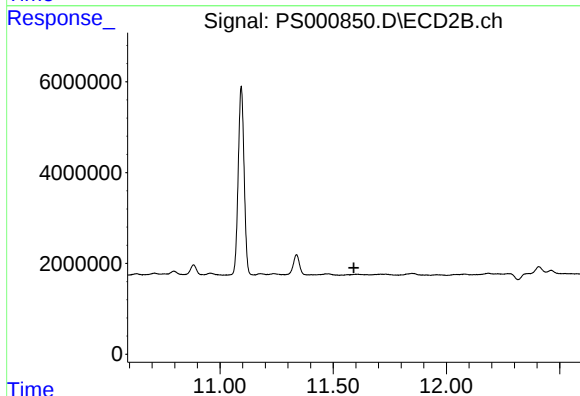


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

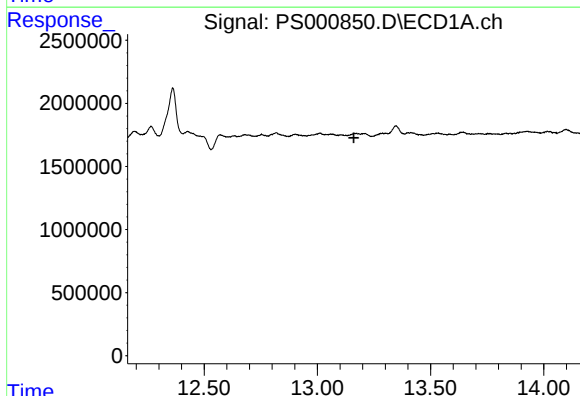


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

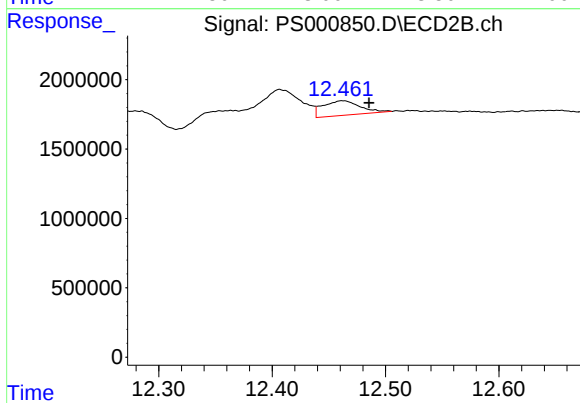

#8 DICHLORPROP


R.T.: 12.462 min
Delta R.T.: -0.023 min
Response: 2398095
Conc: 11.87 ng/ml

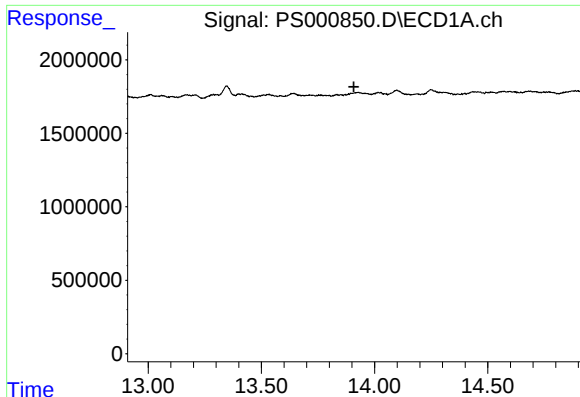

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

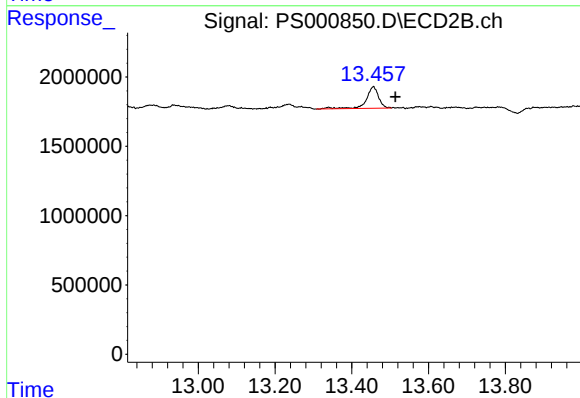


#10 Pentachlorophenol

R.T.: 13.456 min
Delta R.T.: -0.057 min
Response: 3468700
Conc: 1.11 ng/ml

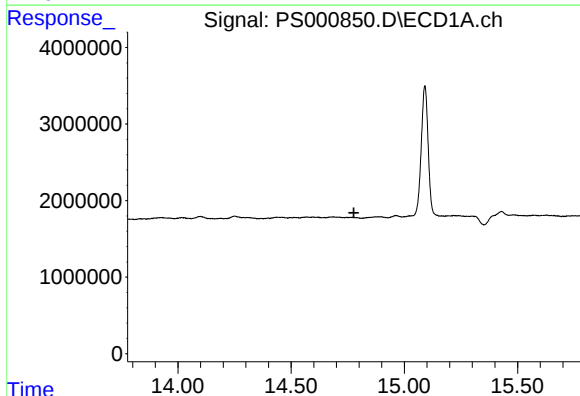

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

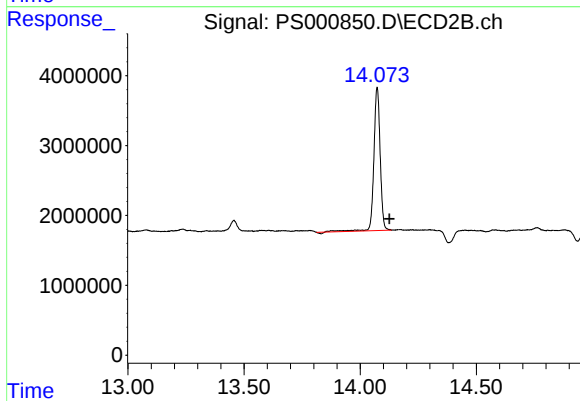

#11 2,4,5-TP (SILVEX)

R.T.: 14.073 min
Delta R.T.: -0.054 min
Response: 38684486
Conc: 30.83 ng/ml