

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 10:49
 Operator : UA
 Sample : J3887-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:34:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.684	11.097	65169419	58588871	315.866	269.007
Target Compounds							
2) T	3,5-DICHL...	0.000	9.181	0	9063971	N.D.	30.814 #
5) T	DICAMBA	11.936	11.341	3553675	6311762	4.513	8.041 #
6) T	MCP	12.379	0.000	6707866	0	12.212	N.D. #
8) T	DICHLORPROP	0.000	12.464	0	1815810	N.D.	8.990 #
10) T	Pentachlo...	0.000	13.459	0	2470082	N.D.	0.787 #
11) T	2,4,5-TP ...	0.000	14.076	0	18432959	N.D.	14.688 #
12) T	2,4,5-T	15.108	0.000	16906853	0	13.884	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 10:49
Operator : UA
Sample : J3887-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:34:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

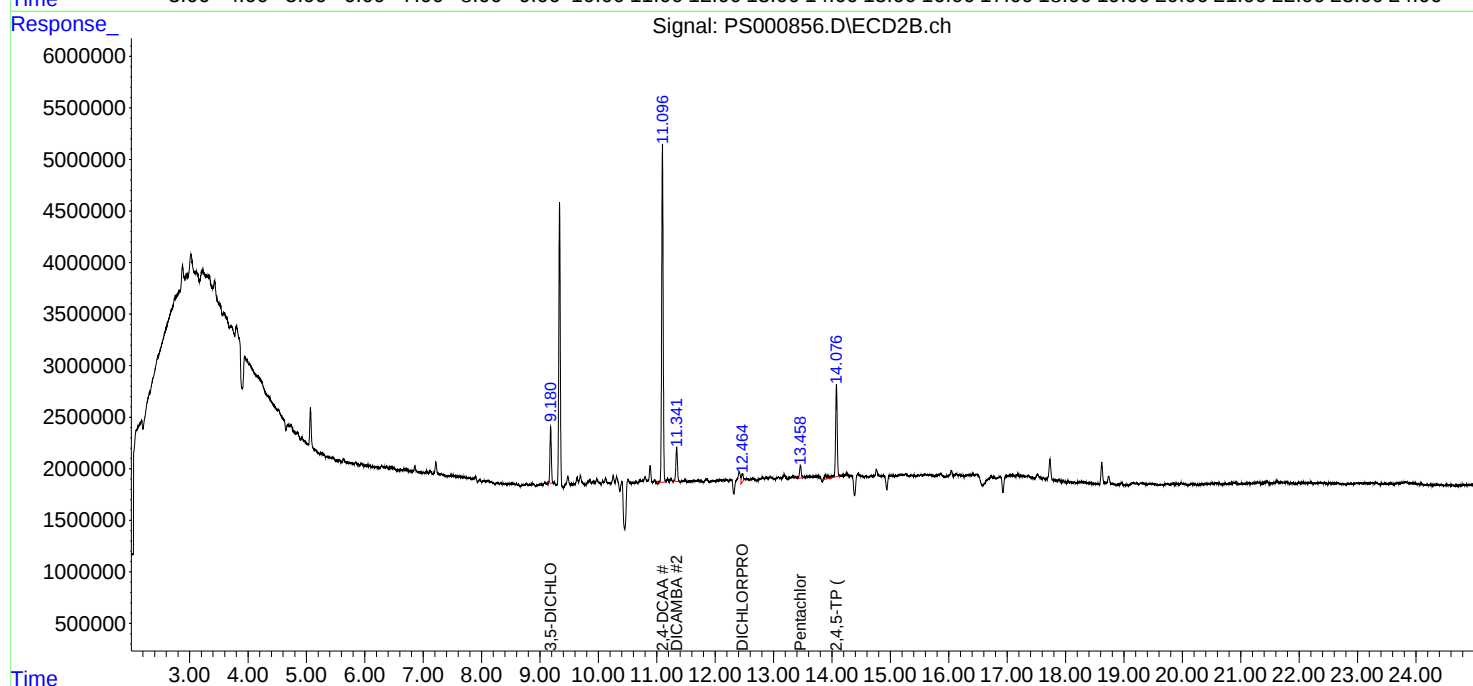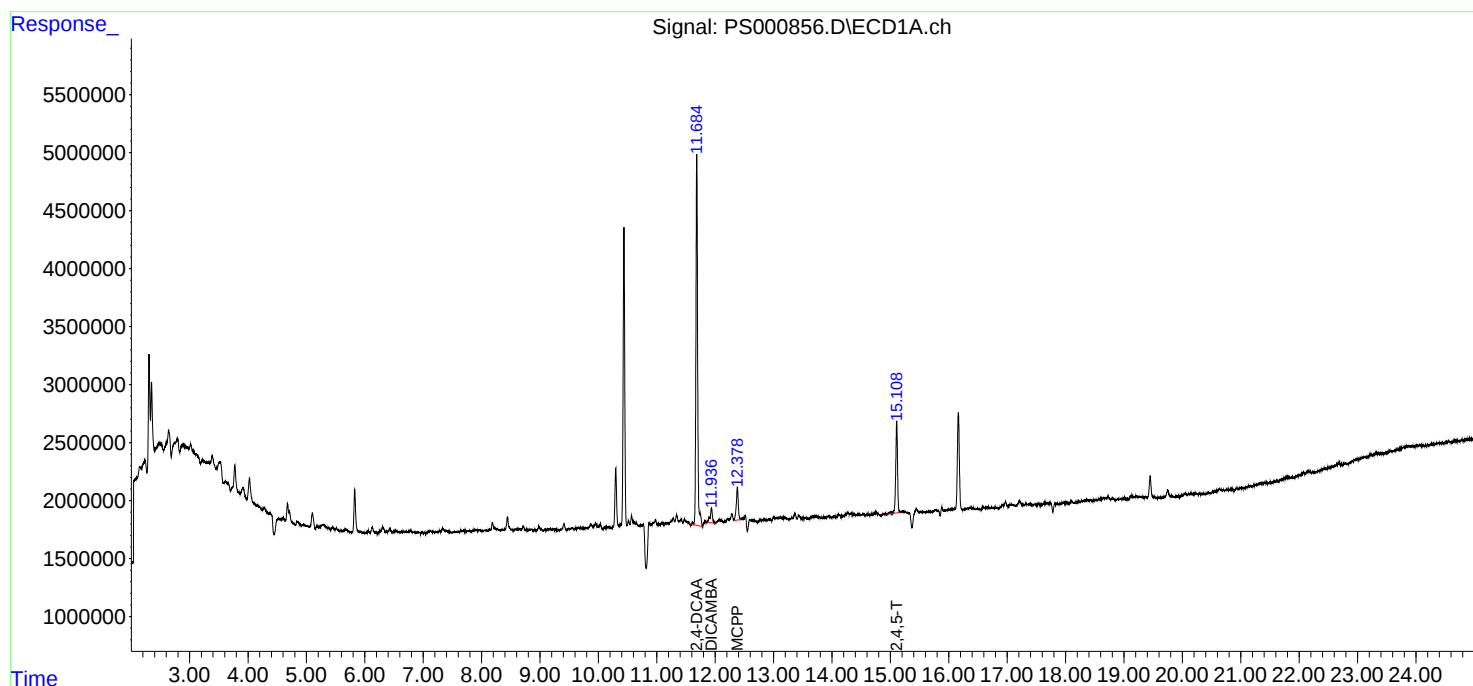


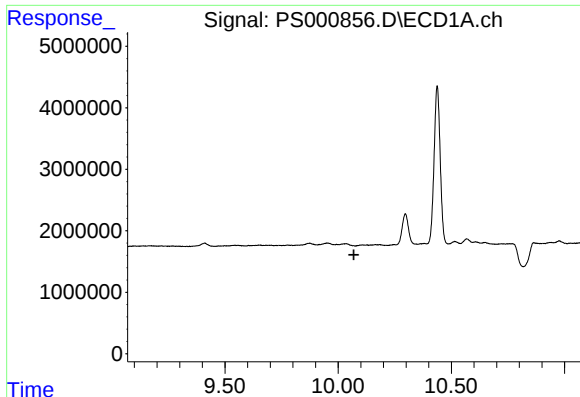

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

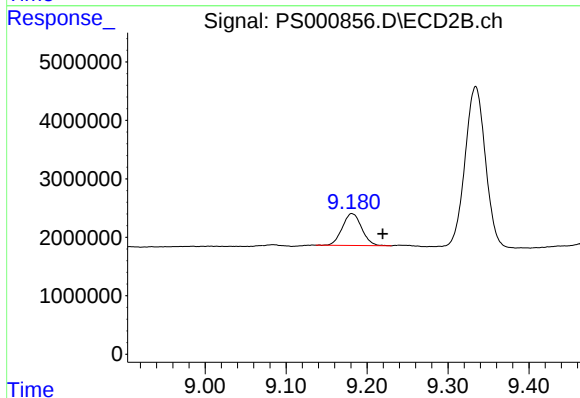


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.181 min
Delta R.T.: -0.038 min
Response: 9063971
Conc: 30.81 ng/ml

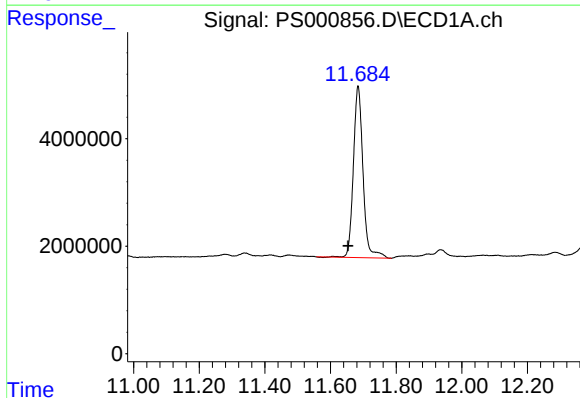


#4 2,4-DCAA

R.T.: 11.684 min
Delta R.T.: 0.031 min
Response: 65169419
Conc: 315.87 ng/ml

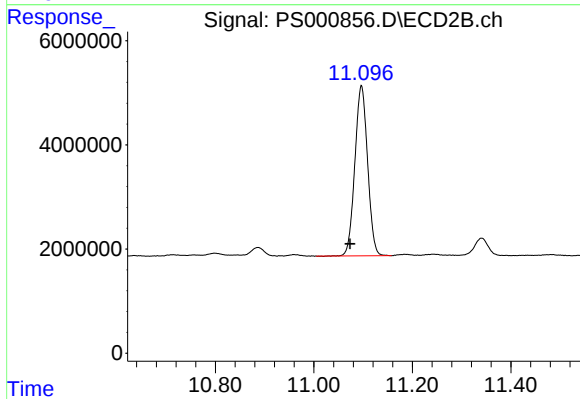

#4 2,4-DCAA


R.T.: 11.097 min
Delta R.T.: 0.023 min
Response: 58588871
Conc: 269.01 ng/ml

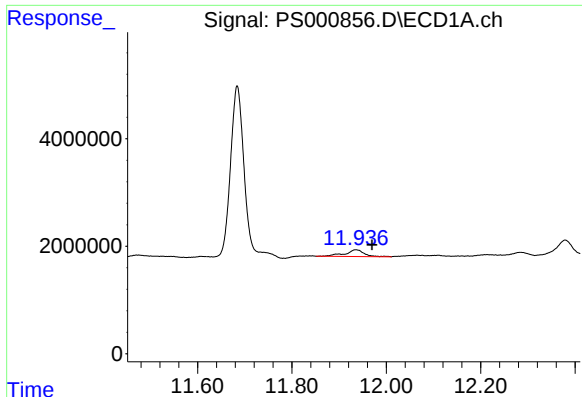

#5 DICAMBA


R.T.: 11.936 min
Delta R.T.: -0.034 min
Response: 3553675
Conc: 4.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

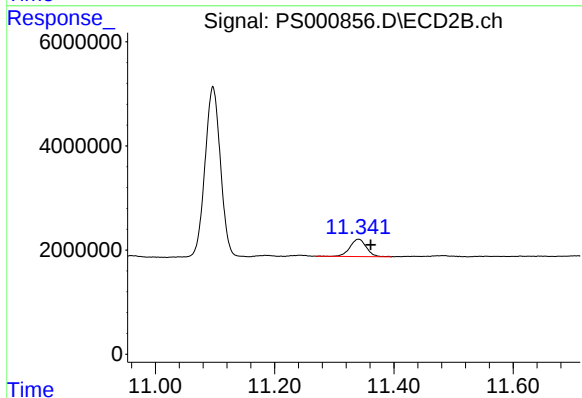


#5 DICAMBA

R.T.: 11.341 min
Delta R.T.: -0.021 min
Response: 6311762
Conc: 8.04 ng/ml

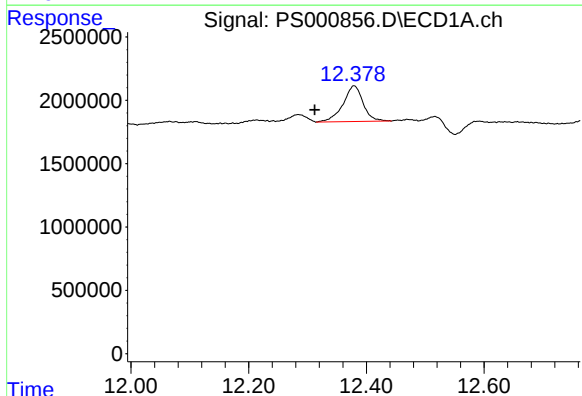


#6 MCP

R.T.: 12.379 min
Delta R.T.: 0.067 min
Response: 6707866
Conc: 12.21 ug/ml

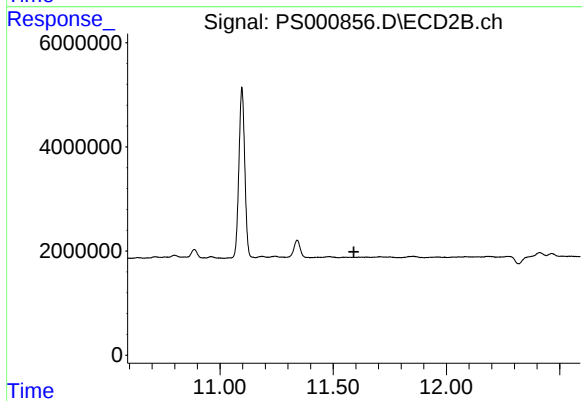

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.591 min
Response: 0
Conc: N.D.

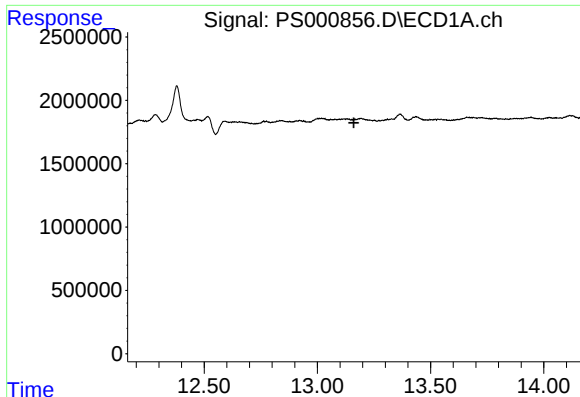

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

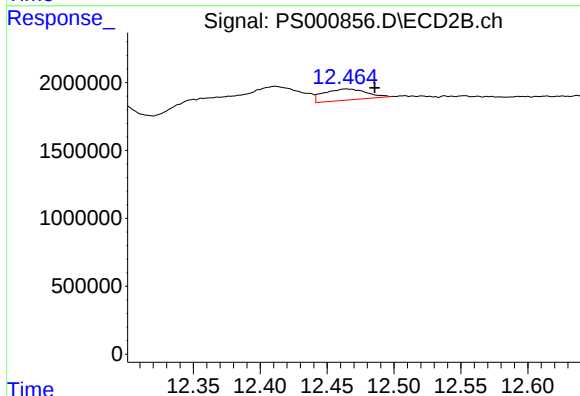


#8 DICHLORPROP

R.T.: 12.464 min
Delta R.T.: -0.022 min
Response: 1815810
Conc: 8.99 ng/ml

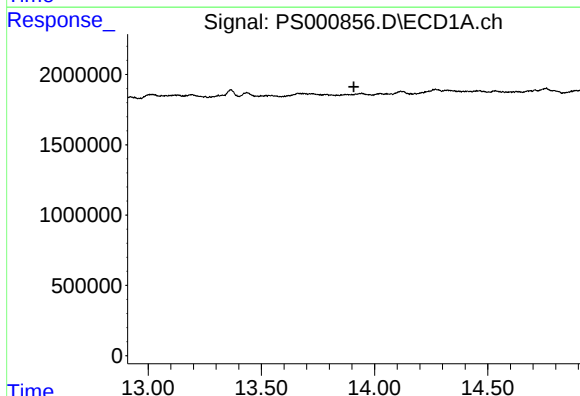


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

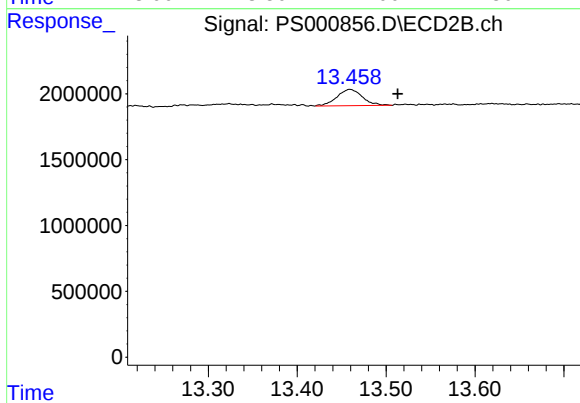

#10 Pentachlorophenol


R.T.: 13.459 min
Delta R.T.: -0.054 min
Response: 2470082
Conc: 0.79 ng/ml

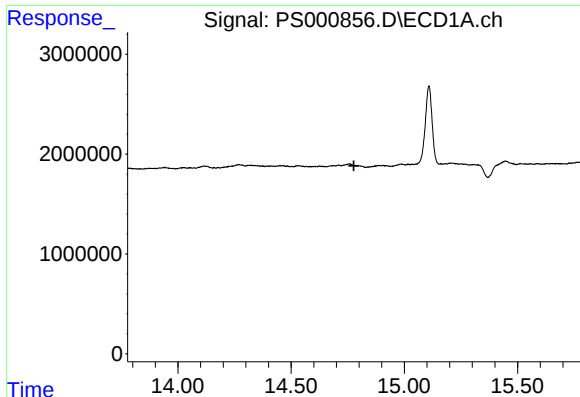

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

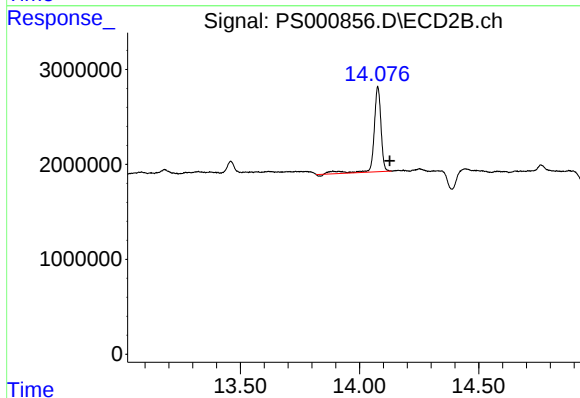


#11 2,4,5-TP (SILVEX)

R.T.: 14.076 min
Delta R.T.: -0.050 min
Response: 18432959
Conc: 14.69 ng/ml

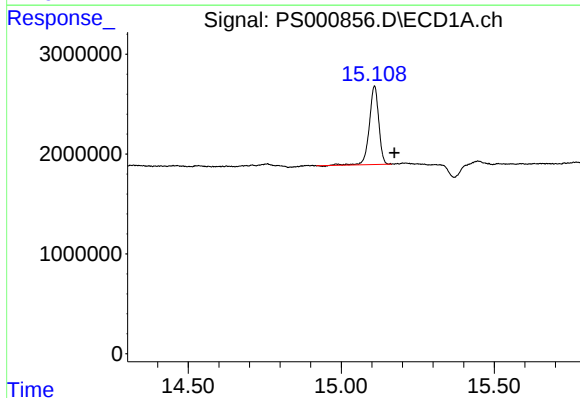

#12 2,4,5-T

R.T.: 15.108 min
Delta R.T.: -0.066 min
Response: 16906853
Conc: 13.88 ng/ml

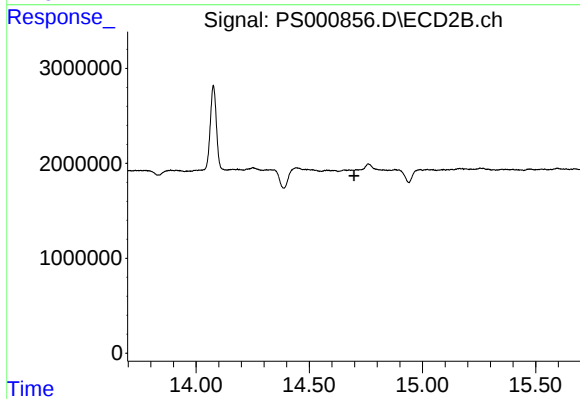

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.697 min
Response: 0
Conc: N.D.