

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 11:20
 Operator : UA
 Sample : J3887-08
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:35:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.658	11.072	63044067	57690193	305.564	264.880
Target Compounds							
5) T	DICAMBA	11.910	11.317	2862924	6425274	3.636	8.186 #
6) T	MCPD	12.353	0.000	6524289	0	11.878	N.D. #
8) T	DICHLORPROP	0.000	12.443	0	1325329	N.D.	6.562 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 11:20
Operator : UA
Sample : J3887-08
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:35:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

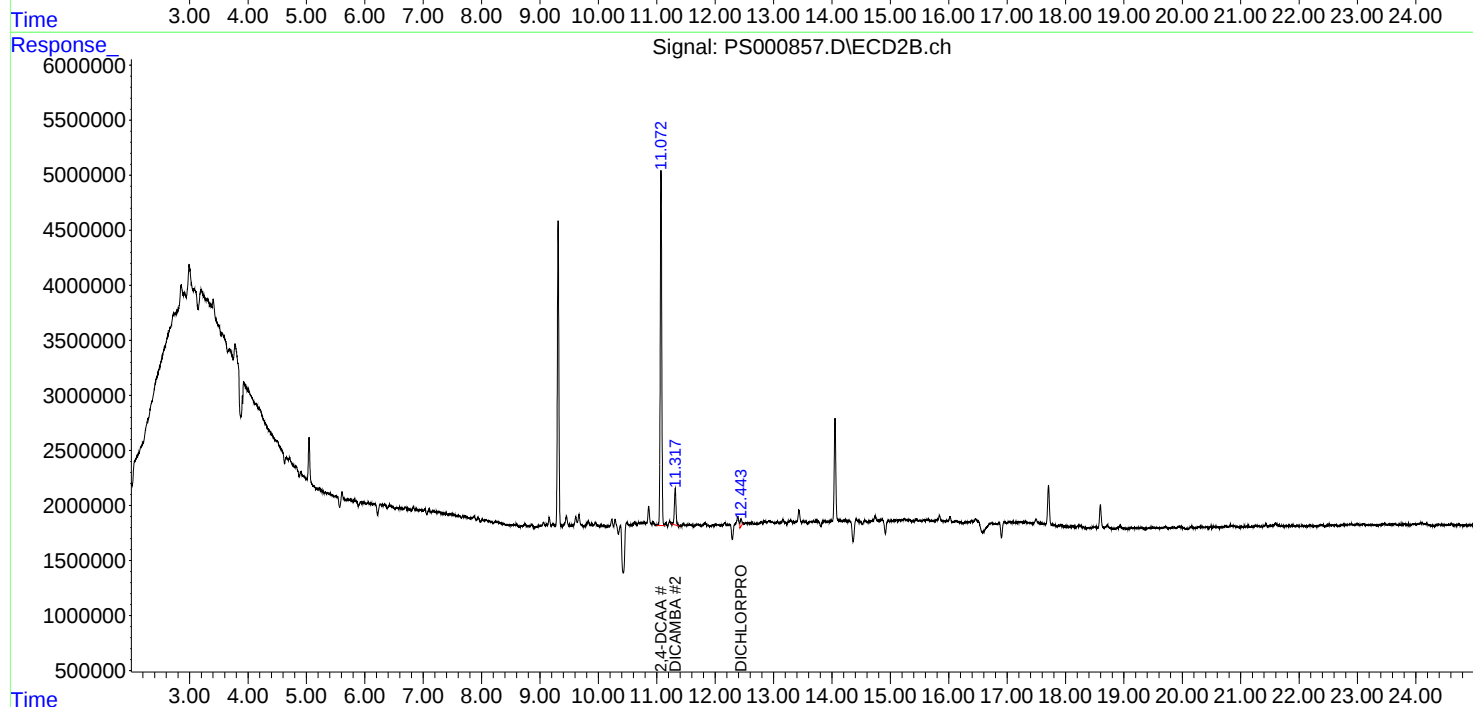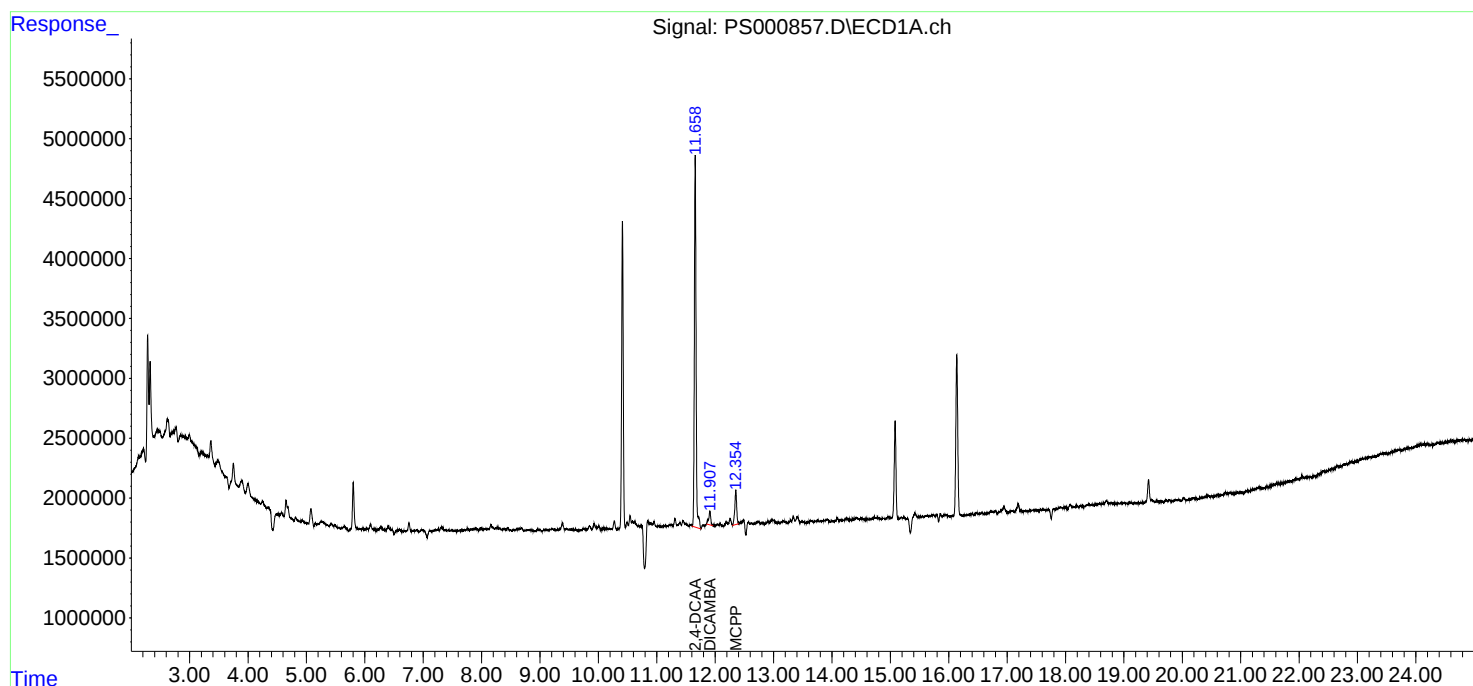


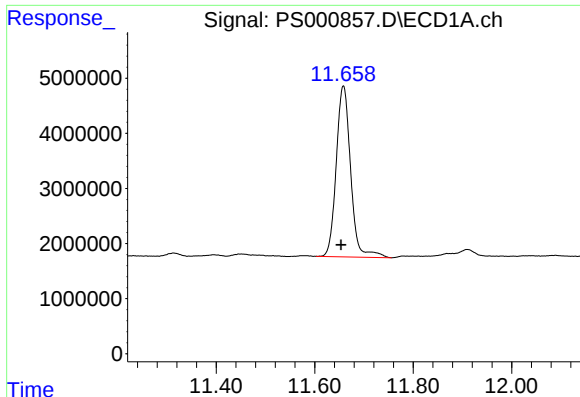

#4 2,4-DCAA


R.T.: 11.658 min
Delta R.T.: 0.005 min
Response: 63044067
Conc: 305.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

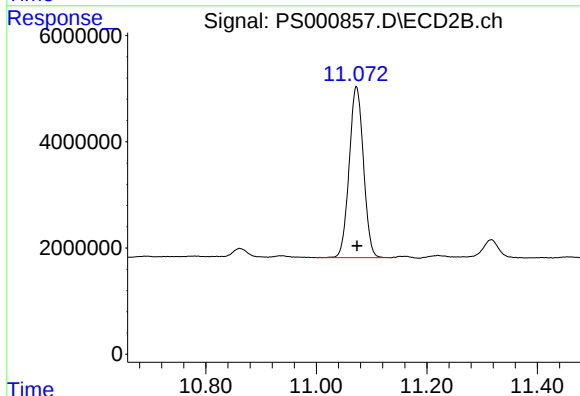


#4 2,4-DCAA

R.T.: 11.072 min
Delta R.T.: -0.001 min
Response: 57690193
Conc: 264.88 ng/ml

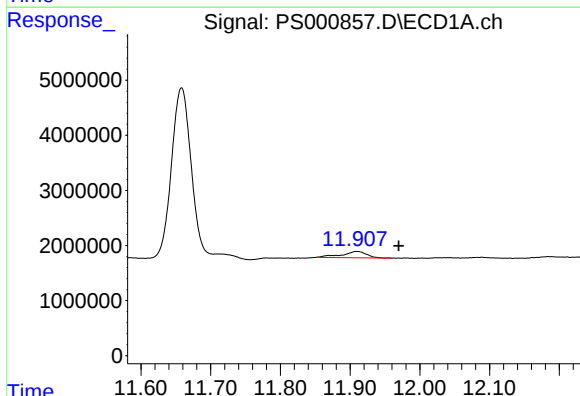


#5 DICAMBA

R.T.: 11.910 min
Delta R.T.: -0.060 min
Response: 2862924
Conc: 3.64 ng/ml

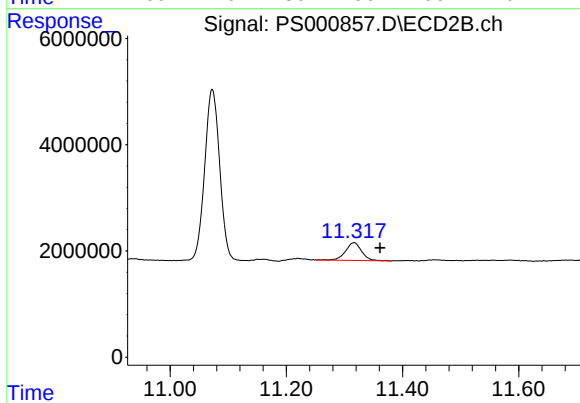

#5 DICAMBA


R.T.: 11.317 min
Delta R.T.: -0.045 min
Response: 6425274
Conc: 8.19 ng/ml

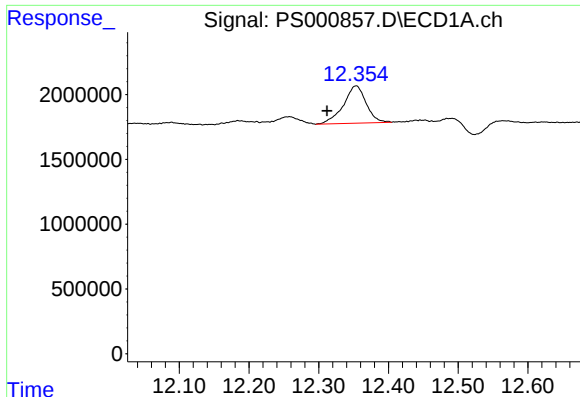

#6 MCP


R.T.: 12.353 min
Delta R.T.: 0.041 min
Response: 6524289
Conc: 11.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

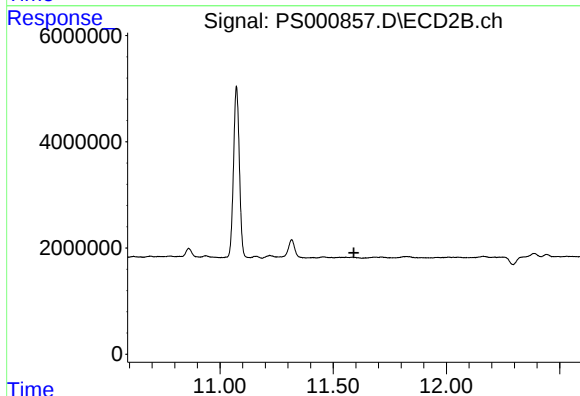


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

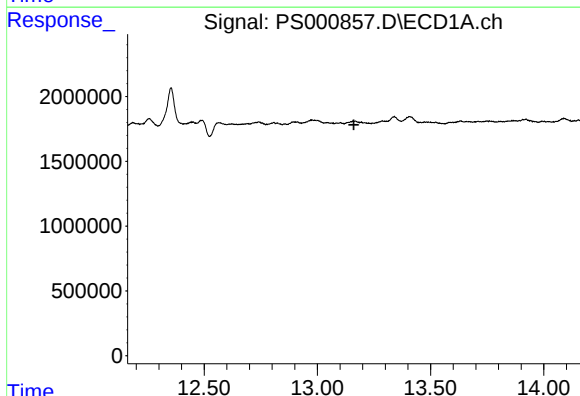

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.161 min
Response: 0
Conc: N.D.

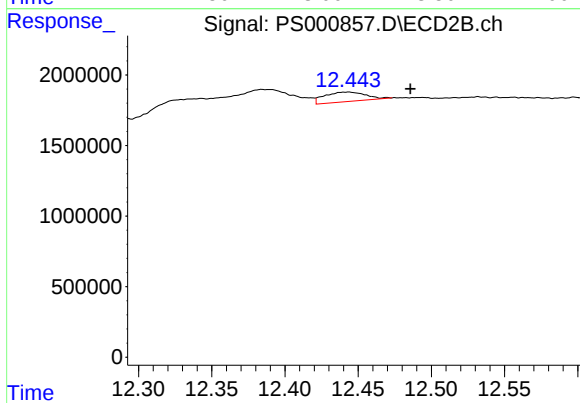

#8 DICHLORPROP

R.T.: 12.443 min
Delta R.T.: -0.043 min
Response: 1325329
Conc: 6.56 ng/ml