

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2018 12:53
 Operator : UA
 Sample : PB110896BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 03:36:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 02:00:25 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.674	11.087	97693833	94033916	473.506	431.750
Target Compounds							
2) T	3,5-DICHL...	0.000	9.173	0	2850742	N.D.	9.691 #
3) T	4-Nitroph...	0.000	10.244	0	5069834	N.D.	42.016 #
5) T	DICAMBA	11.927	11.331	4109975	7269497	5.220	9.261 #
6) T	MCP	12.368	0.000	12129419	0	22.082	N.D. #
7) T	MCPA	12.580	11.949	1460116	3179458	1.600	4.090 #
8) T	DICHLORPROP	0.000	12.454	0	1554519	N.D.	7.696 #
10) T	Pentachlo...	0.000	13.448	0	2176011	N.D.	0.693 #
11) T	2,4,5-TP ...	0.000	14.065	0	6560872	N.D.	5.228 #
14) T	DINOSEB	0.000	15.786	0	12279343	N.D.	14.662 #
15) T	Picloram	0.000	16.971	0	10839078	N.D.	7.118 #
16) T	DCPA	0.000	17.032	0	6982394	N.D.	4.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2018 12:53
Operator : UA
Sample : PB110896BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 03:36:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 02:00:25 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

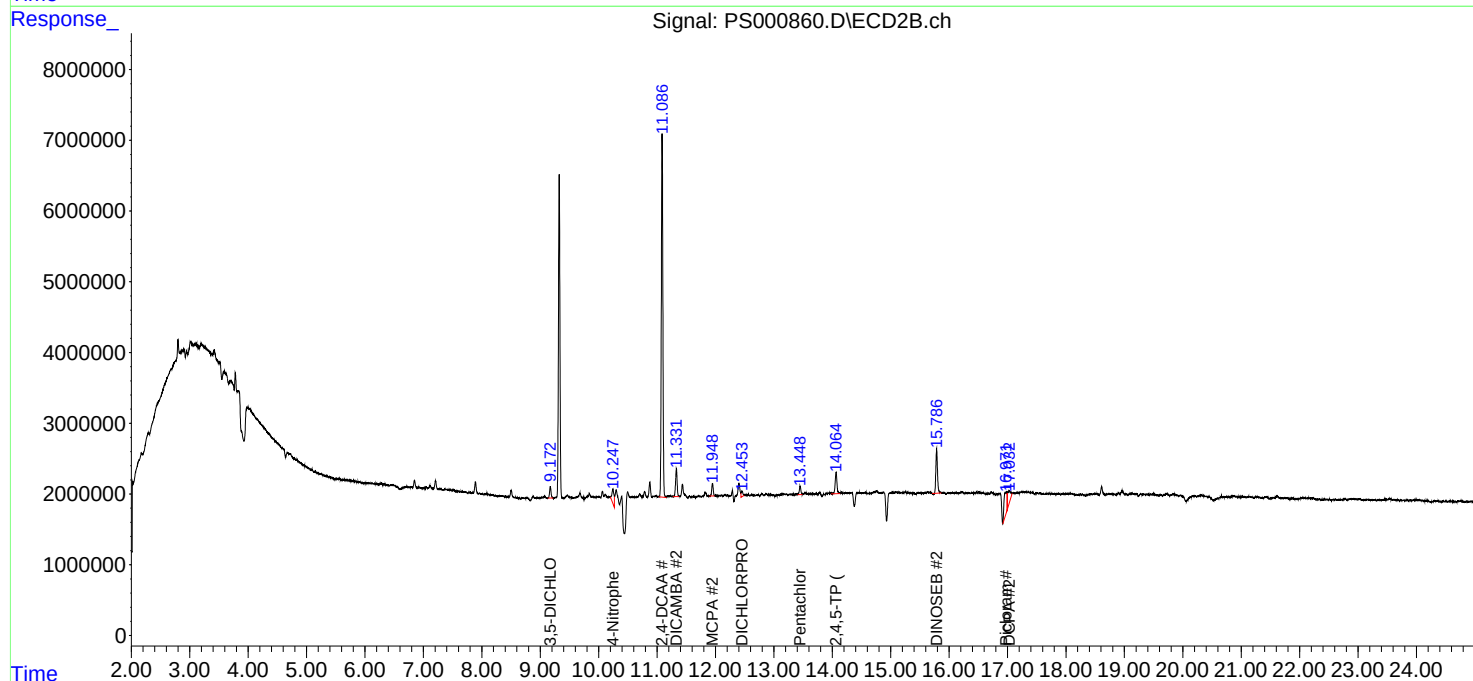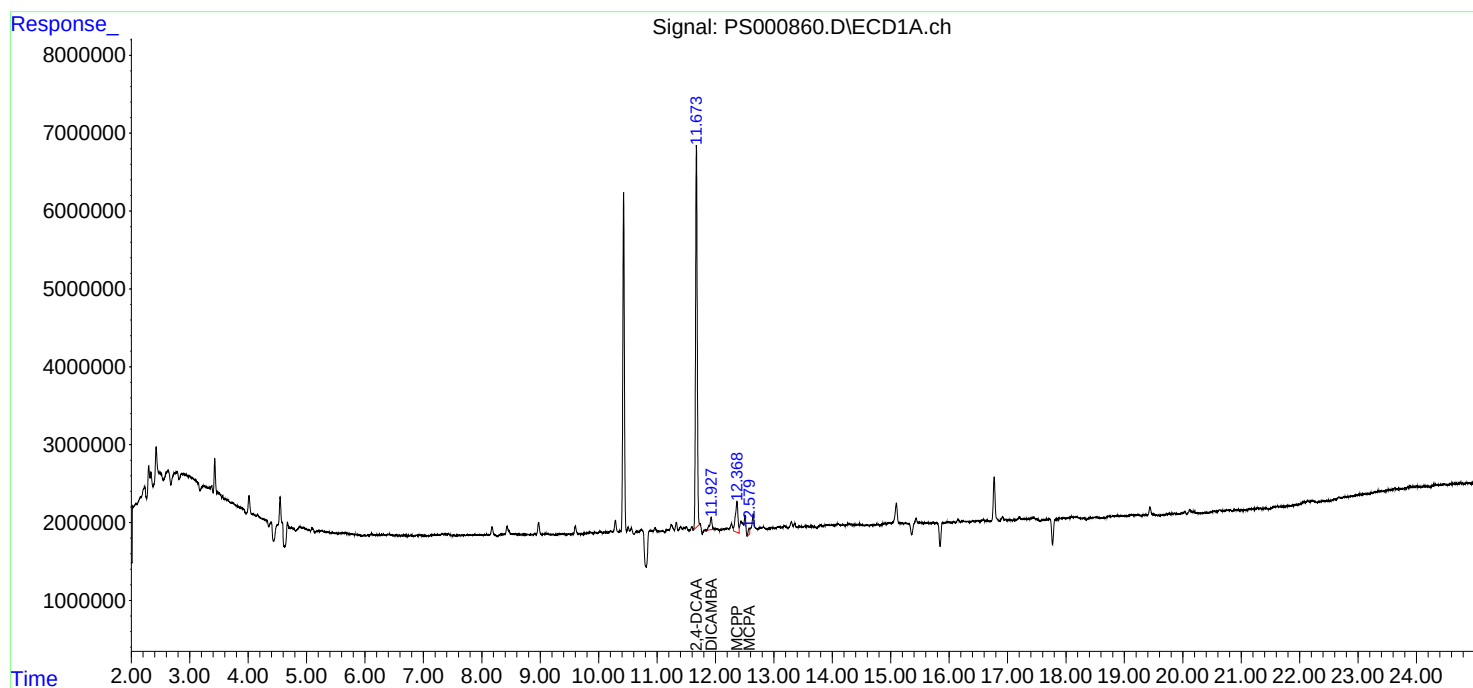


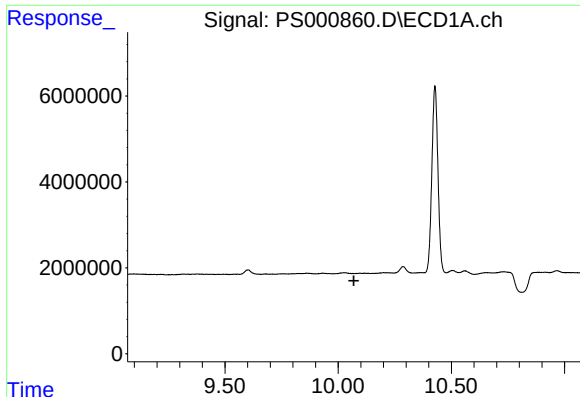

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.070 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

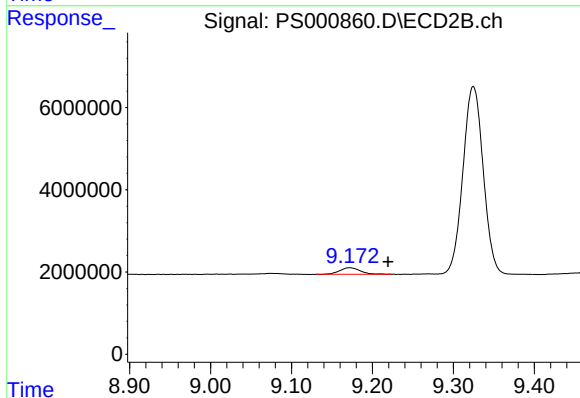


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.173 min
Delta R.T.: -0.047 min
Response: 2850742
Conc: 9.69 ng/ml

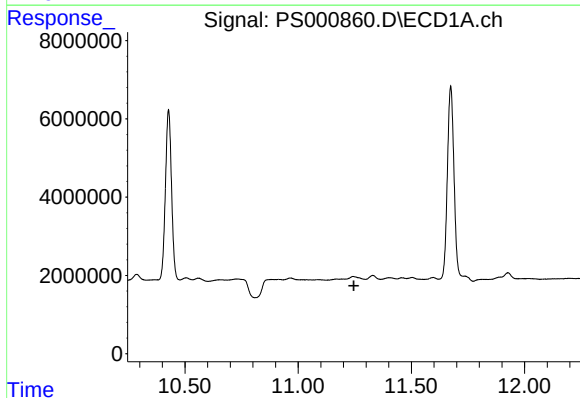


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.246 min
Response: 0
Conc: N.D.

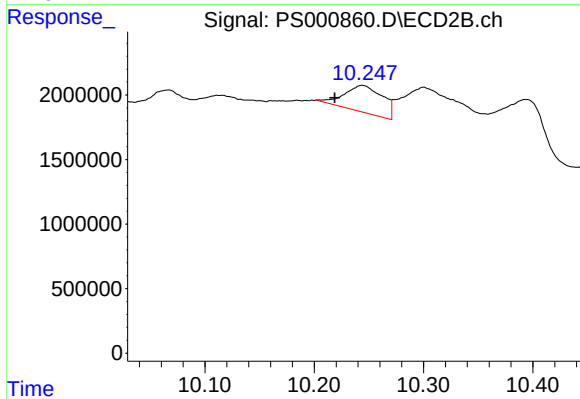

#3 4-Nitrophenol


R.T.: 10.244 min
Delta R.T.: 0.025 min
Response: 5069834
Conc: 42.02 ng/ml

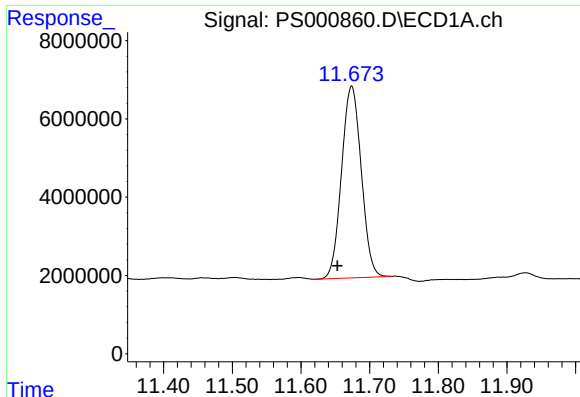

#4 2,4-DCAA


R.T.: 11.674 min
Delta R.T.: 0.020 min
Response: 97693833
Conc: 473.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

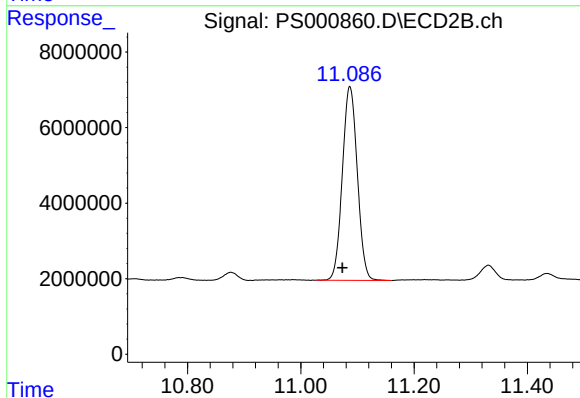


#4 2,4-DCAA

R.T.: 11.087 min
Delta R.T.: 0.013 min
Response: 94033916
Conc: 431.75 ng/ml

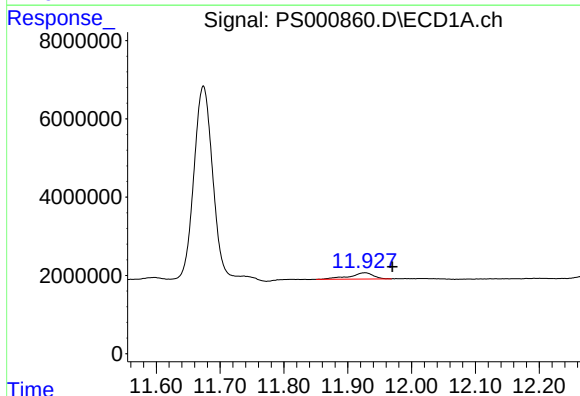


#5 DICAMBA

R.T.: 11.927 min
Delta R.T.: -0.043 min
Response: 4109975
Conc: 5.22 ng/ml

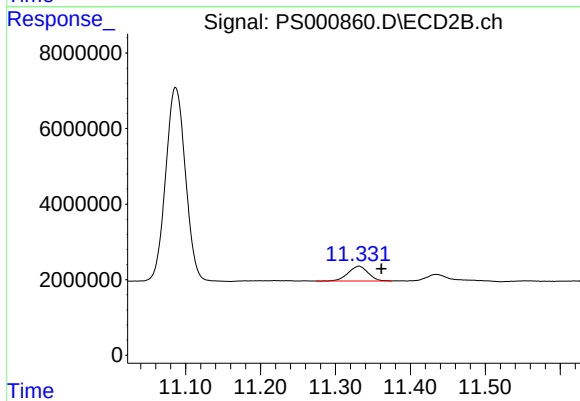

#5 DICAMBA


R.T.: 11.331 min
Delta R.T.: -0.030 min
Response: 7269497
Conc: 9.26 ng/ml

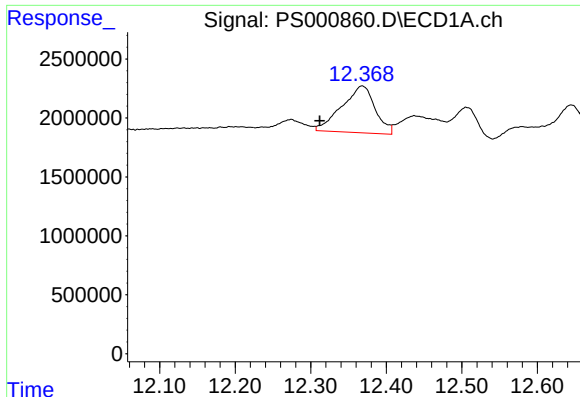

#6 MCPP


R.T.: 12.368 min
Delta R.T.: 0.056 min
Response: 12129419
Conc: 22.08 ug/ml

Instrument :
ECD_S
ClientSampleId :

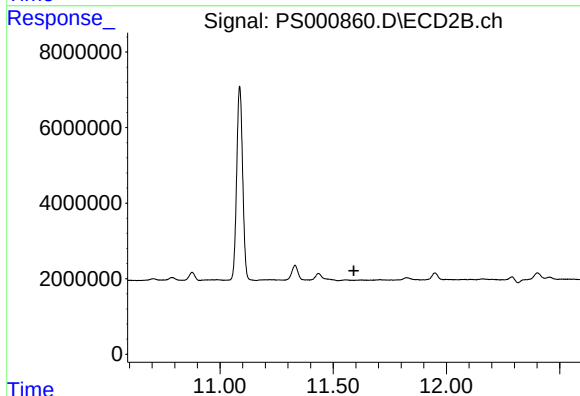


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.591 min
Response: 0
Conc: N.D.

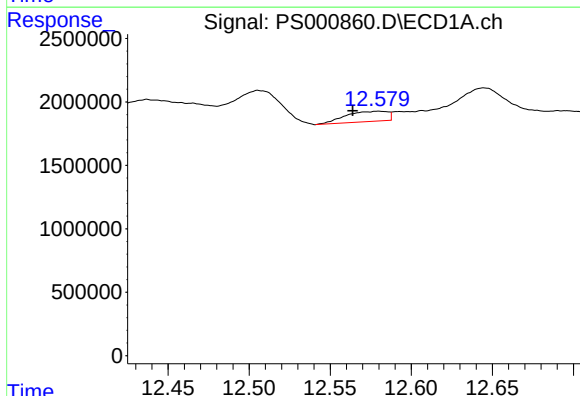


#7 MCPA

R.T.: 12.580 min
Delta R.T.: 0.016 min
Response: 1460116
Conc: 1.60 ug/ml

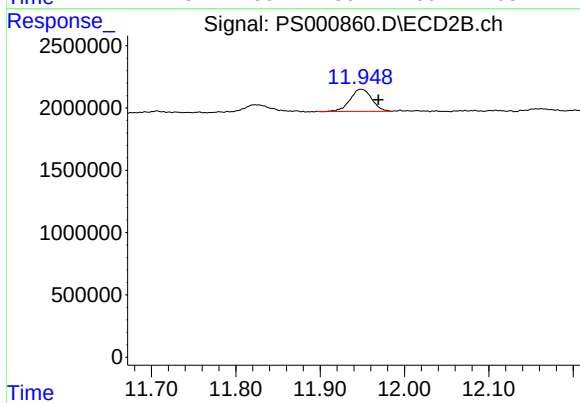

#7 MCPA


R.T.: 11.949 min
Delta R.T.: -0.021 min
Response: 3179458
Conc: 4.09 ug/ml

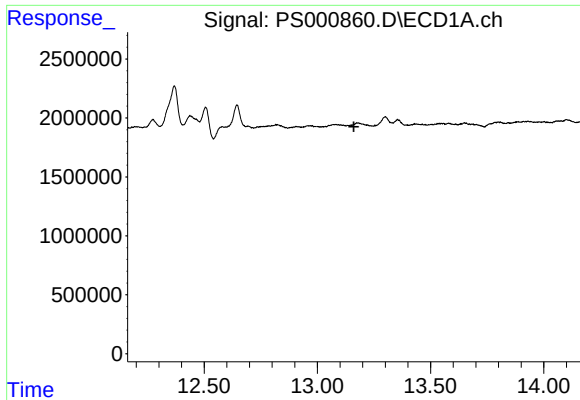

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.161 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

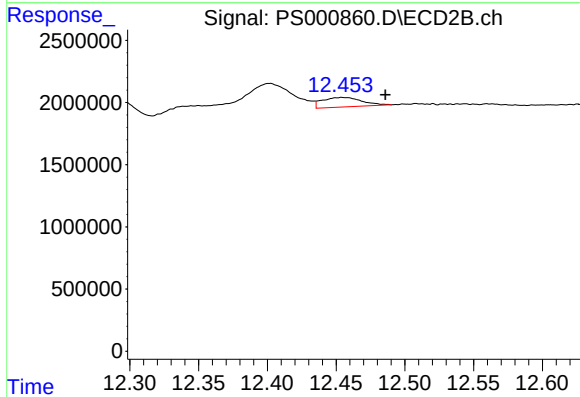


#8 DICHLORPROP

R.T.: 12.454 min
Delta R.T.: -0.032 min
Response: 1554519
Conc: 7.70 ng/ml

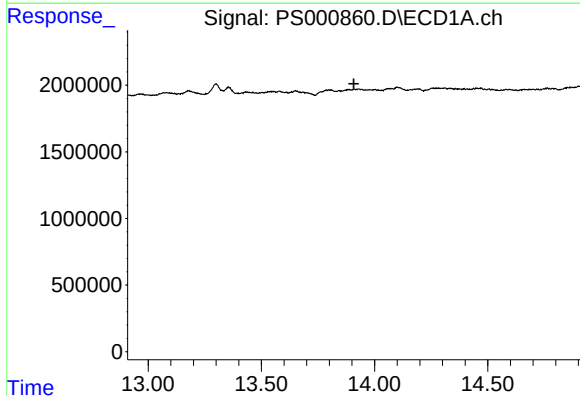


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.908 min
Response: 0
Conc: N.D.

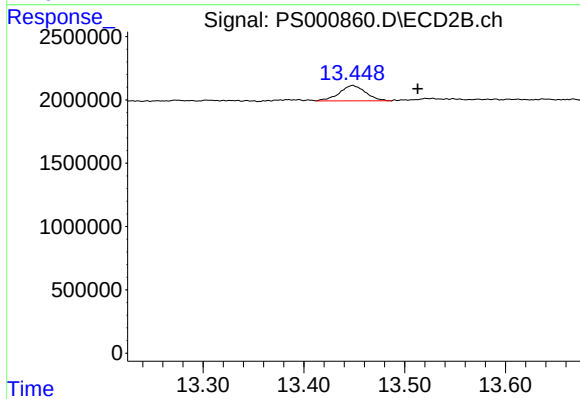

#10 Pentachlorophenol


R.T.: 13.448 min
Delta R.T.: -0.065 min
Response: 2176011
Conc: 0.69 ng/ml

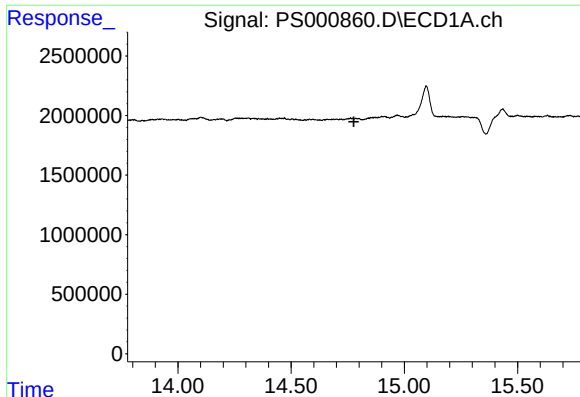

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.777 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

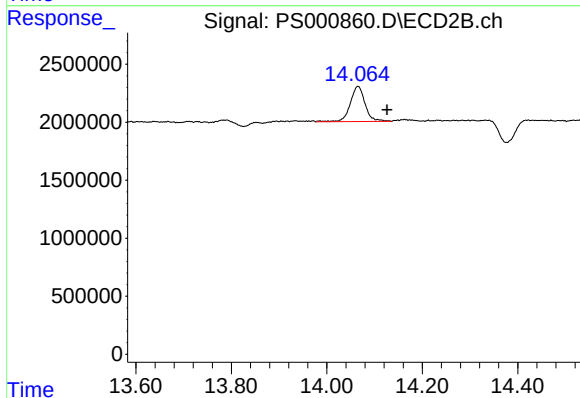


#11 2,4,5-TP (SILVEX)

R.T.: 14.065 min
Delta R.T.: -0.061 min
Response: 6560872
Conc: 5.23 ng/ml

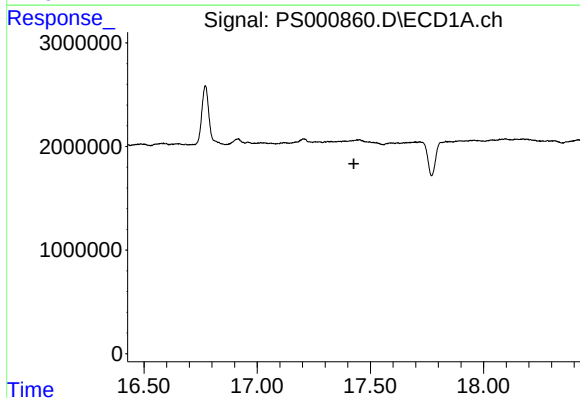


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.427 min
Response: 0
Conc: N.D.

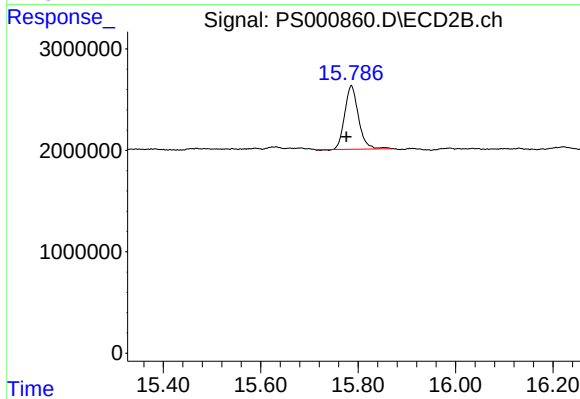

#14 DINOSEB


R.T.: 15.786 min
Delta R.T.: 0.010 min
Response: 12279343
Conc: 14.66 ng/ml

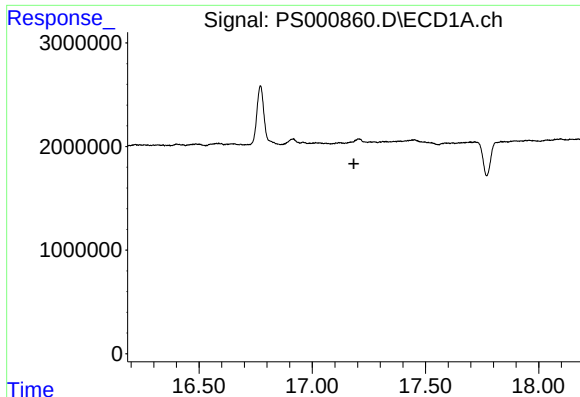

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

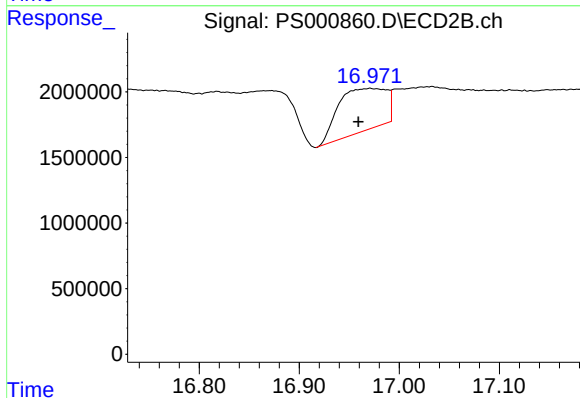


#15 Picloram

R.T.: 16.971 min
Delta R.T.: 0.012 min
Response: 10839078
Conc: 7.12 ng/ml

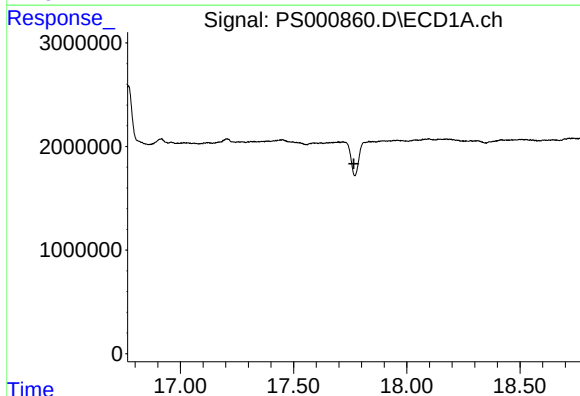

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.766 min
Response: 0
Conc: N.D.

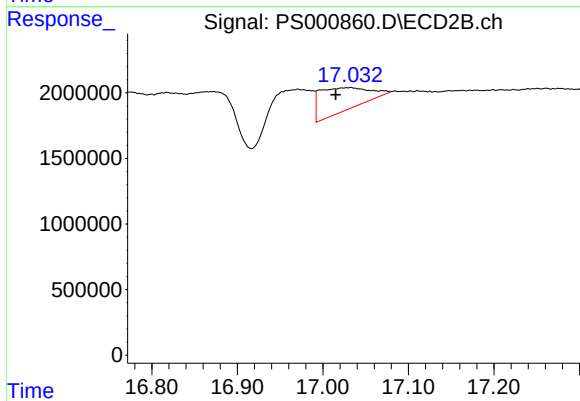

#16 DCPA

R.T.: 17.032 min
Delta R.T.: 0.017 min
Response: 6982394
Conc: 4.06 ng/ml