

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
 Data File : PS000822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2018 17:18
 Operator : UA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:45:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
 Quant Title : 8080.M
 QLast Update : Mon Jul 09 01:45:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.608	11.042	157.1E6	166.5E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.000	2.423	190.0E6	189.1E6	682.500	682.500
2) T	3,5-DICHL...	10.025	9.188	212.6E6	208.3E6	697.500	697.500
3) T	4-Nitroph...	11.201	10.188	91762793	83786486	682.500	682.500
5) T	DICAMBA	11.923	11.330	568.8E6	570.6E6	705.000	705.000
6) T	MCPD	12.263	11.555	43040796	40358896	70.500	70.500
7) T	MCPA	12.515	11.933	65818543	59399885	69.750	69.750
8) T	DICHLORPROP	13.115	12.455	145.4E6	144.1E6	705.000	705.000
9) T	2,4-D	13.473	12.925	194.5E6	198.9E6	705.000	705.000
10) T	Pentachlo...	13.863	13.482	2234.1E6	2319.1E6	712.500	712.500
11) T	2,4,5-TP ...	14.732	14.096	894.5E6	924.8E6	712.500	712.500
12) T	2,4,5-T	15.129	14.667	891.4E6	752.2E6	712.500	712.500
13) T	2,4-DB	15.880	15.313	119.3E6	112.5E6	712.500	712.500
14) T	DINOSEB	17.382	15.745	620.4E6	605.4E6	705.000	705.000
15) T	Picloram	17.139	16.929	1327.2E6	1119.3E6	712.500	712.500
16) T	DCPA	17.721	16.985	1073.6E6	1291.7E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070818\
Data File : PS000822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2018 17:18
Operator : UA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
Client Sampled :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:45:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS070818.M
Quant Title : 8080.M
QLast Update : Mon Jul 09 01:45:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

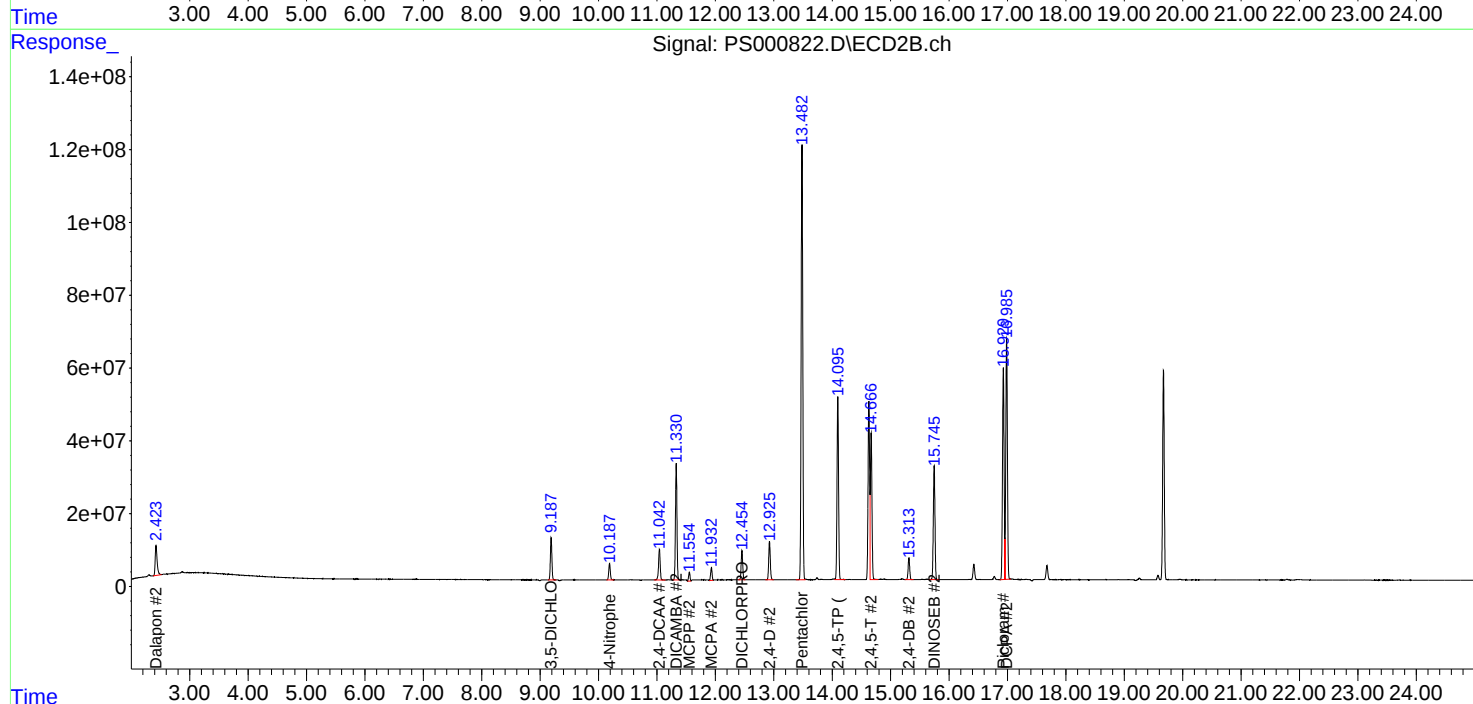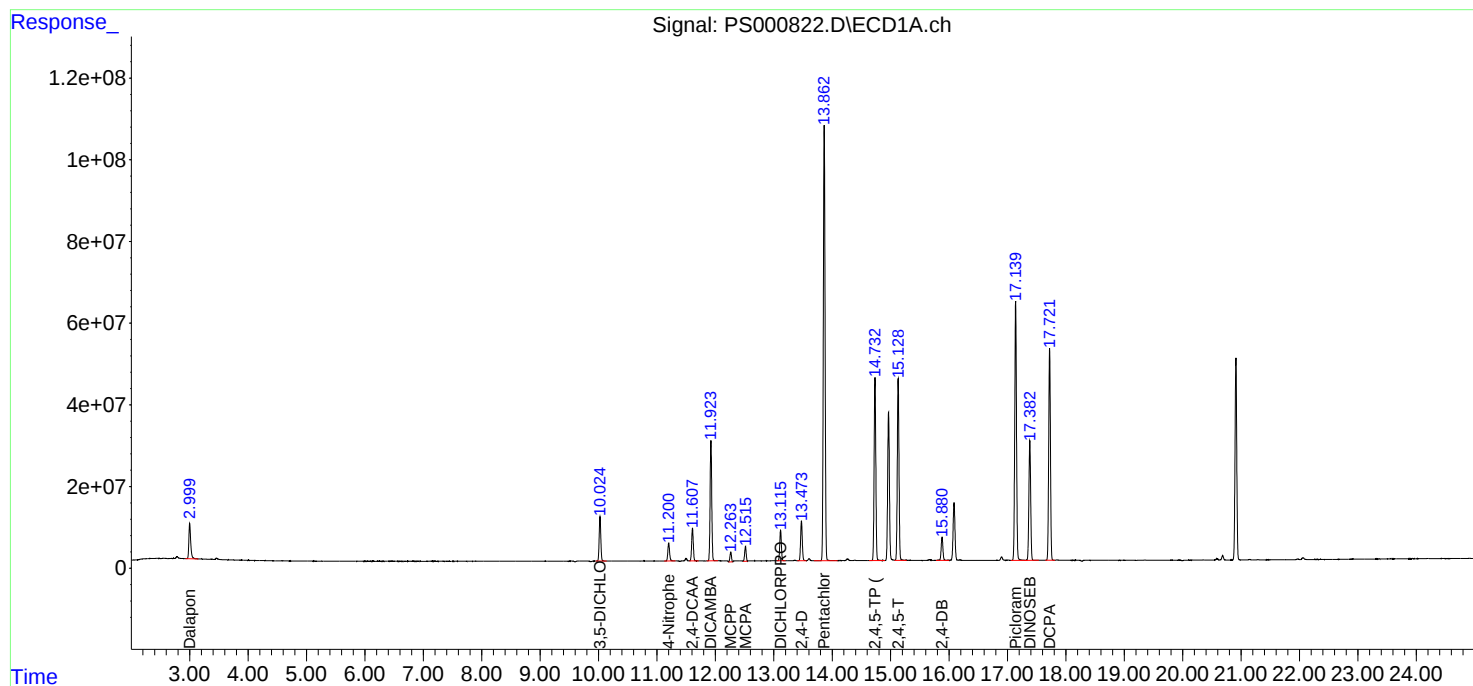


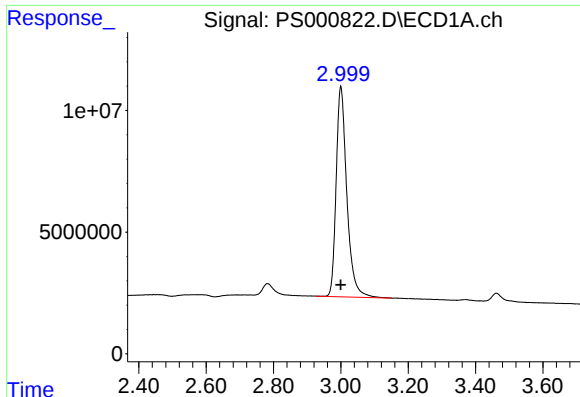

#1 Dalapon


R.T.: 3.000 min
Delta R.T.: 0.000 min
Response: 189977437
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

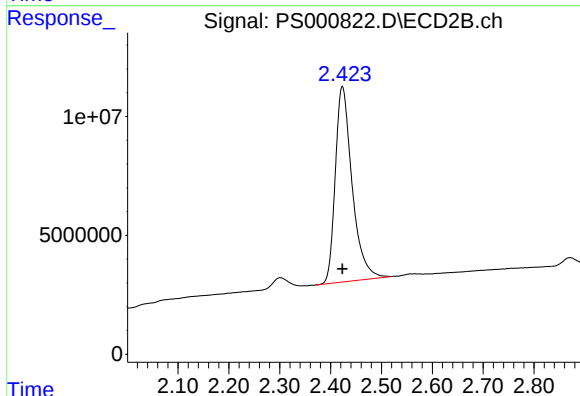


#1 Dalapon

R.T.: 2.423 min
Delta R.T.: 0.000 min
Response: 189112237
Conc: 682.50 ng/ml

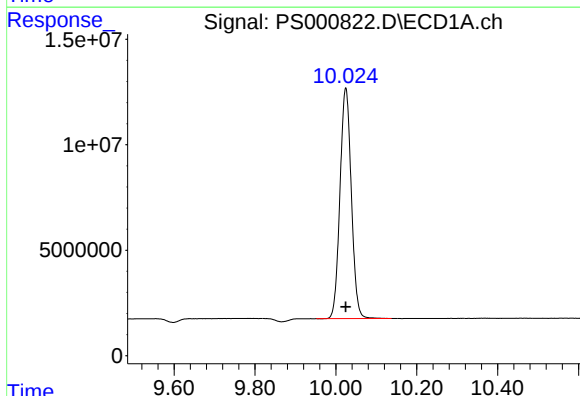


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.025 min
Delta R.T.: 0.000 min
Response: 212566246
Conc: 697.50 ng/ml

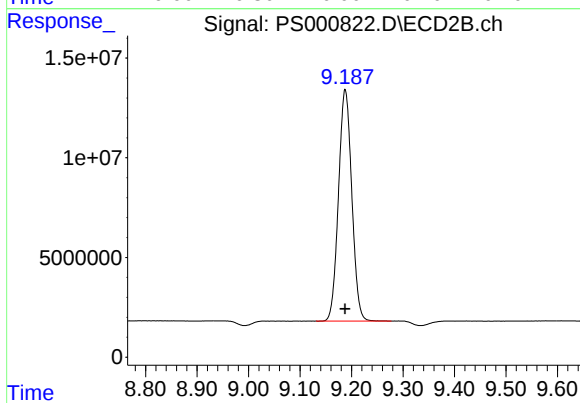

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.188 min
Delta R.T.: 0.000 min
Response: 208292710
Conc: 697.50 ng/ml

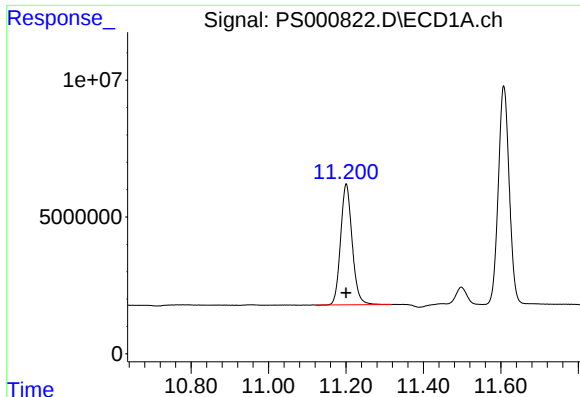

#3 4-Nitrophenol


R.T.: 11.201 min
Delta R.T.: 0.000 min
Response: 91762793
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

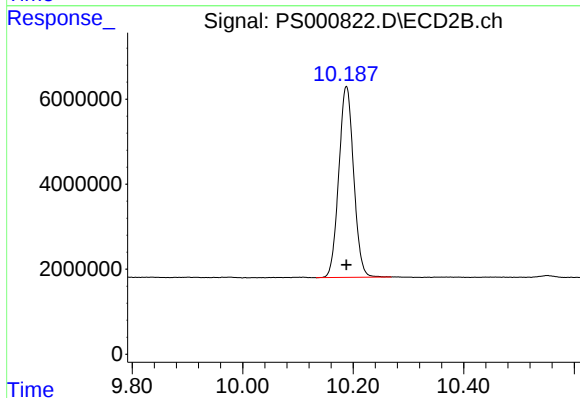


#3 4-Nitrophenol

R.T.: 10.188 min
Delta R.T.: 0.000 min
Response: 83786486
Conc: 682.50 ng/ml

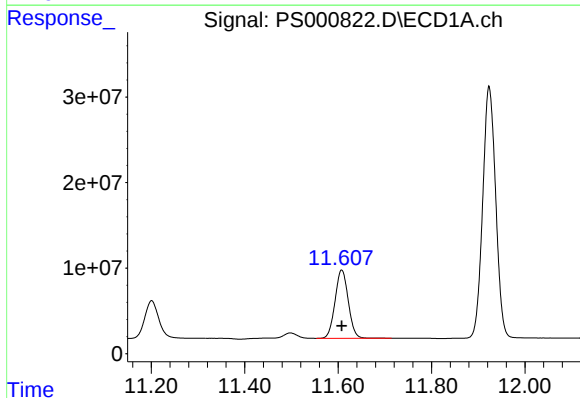


#4 2,4-DCAA

R.T.: 11.608 min
Delta R.T.: 0.000 min
Response: 157070347
Conc: 750.00 ng/ml

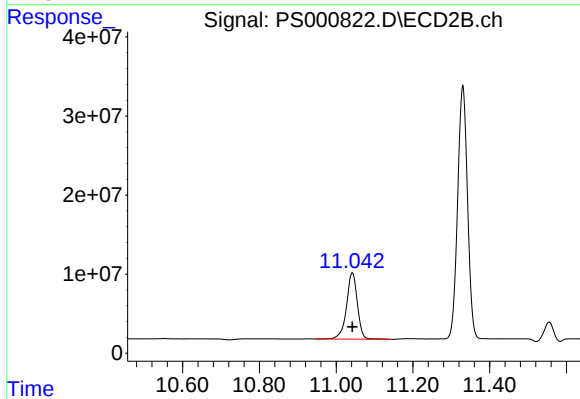

#4 2,4-DCAA


R.T.: 11.042 min
Delta R.T.: 0.000 min
Response: 166485317
Conc: 750.00 ng/ml

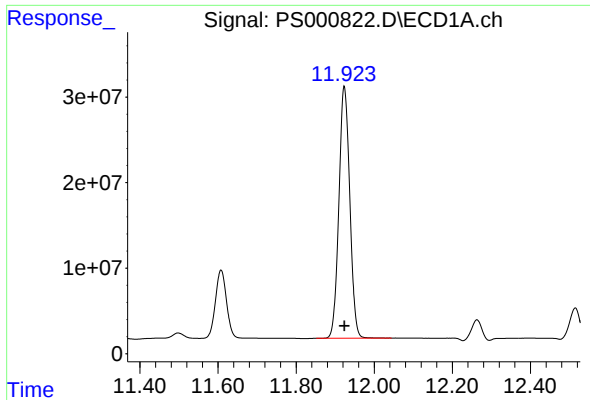

#5 DICAMBA


R.T.: 11.923 min
Delta R.T.: 0.000 min
Response: 568839999
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

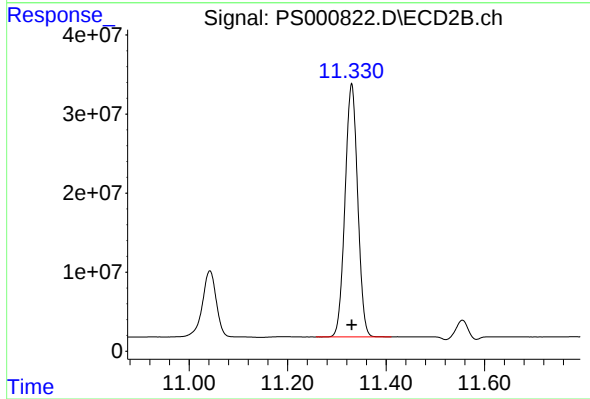


#5 DICAMBA

R.T.: 11.330 min
Delta R.T.: 0.000 min
Response: 570643991
Conc: 705.00 ng/ml

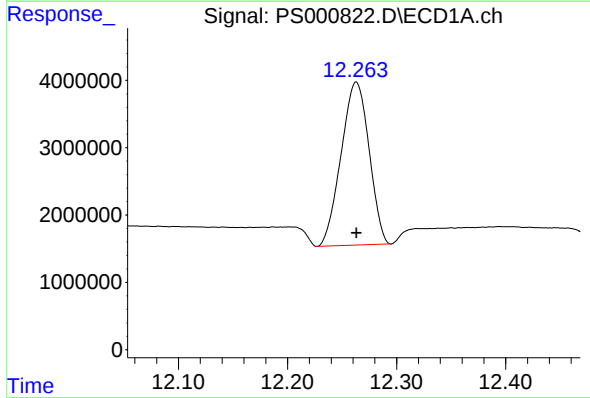


#6 MCP

R.T.: 12.263 min
Delta R.T.: 0.000 min
Response: 43040796
Conc: 70.50 ug/ml

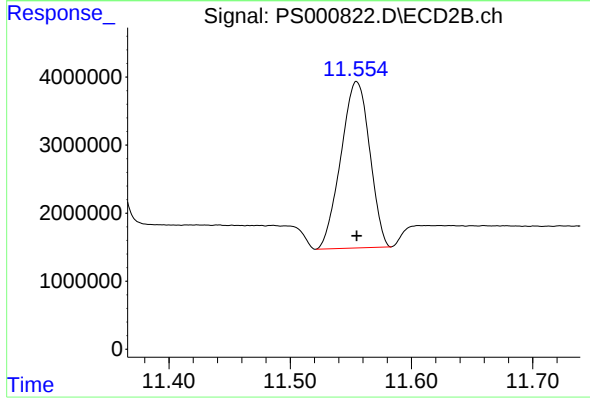

#6 MCP


R.T.: 11.555 min
Delta R.T.: 0.000 min
Response: 40358896
Conc: 70.50 ug/ml

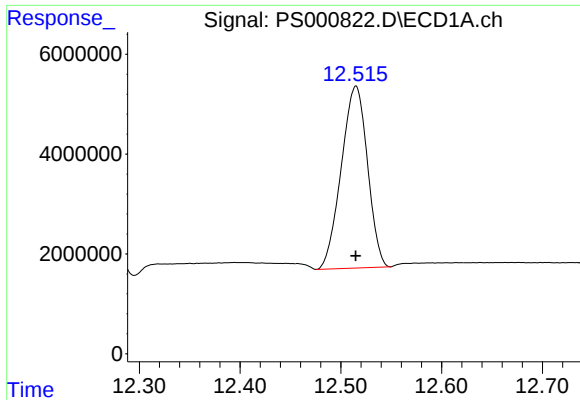

#7 MCPA


R.T.: 12.515 min
Delta R.T.: 0.000 min
Response: 65818543
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

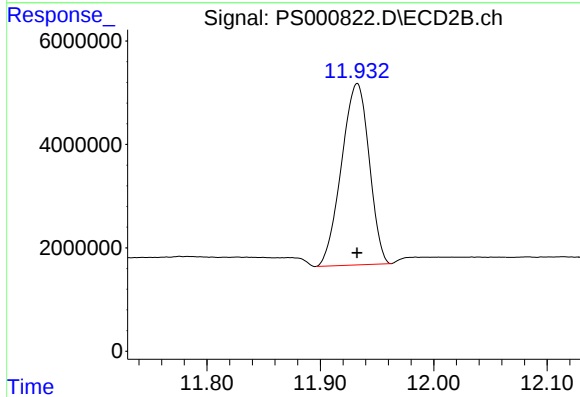


#7 MCPA

R.T.: 11.933 min
Delta R.T.: 0.000 min
Response: 59399885
Conc: 69.75 ug/ml

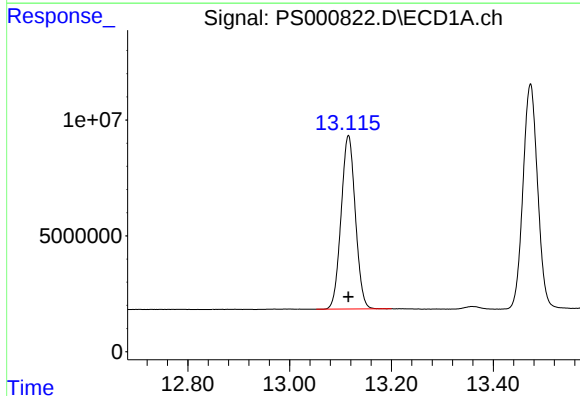


#8 DICHLORPROP

R.T.: 13.115 min
Delta R.T.: 0.000 min
Response: 145447482
Conc: 705.00 ng/ml

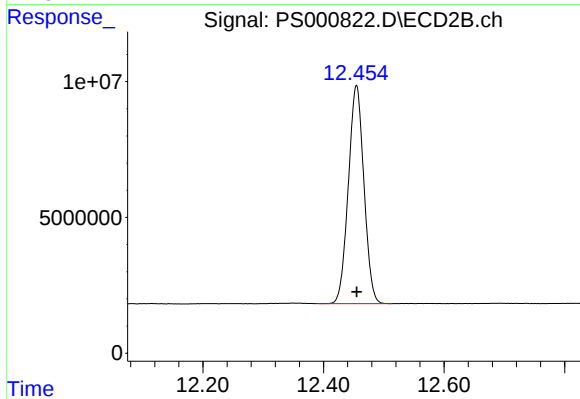

#8 DICHLORPROP


R.T.: 12.455 min
Delta R.T.: 0.000 min
Response: 144136361
Conc: 705.00 ng/ml

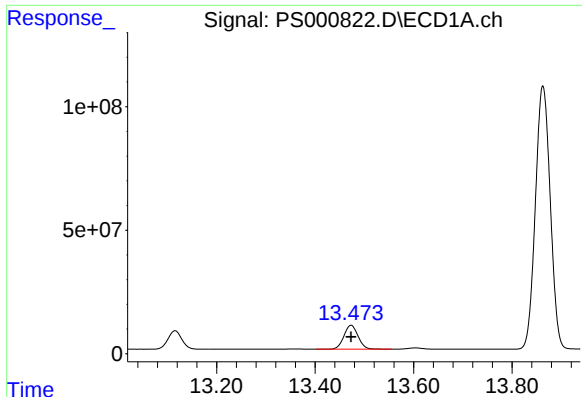

#9 2,4-D


R.T.: 13.473 min
Delta R.T.: 0.000 min
Response: 194499447
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

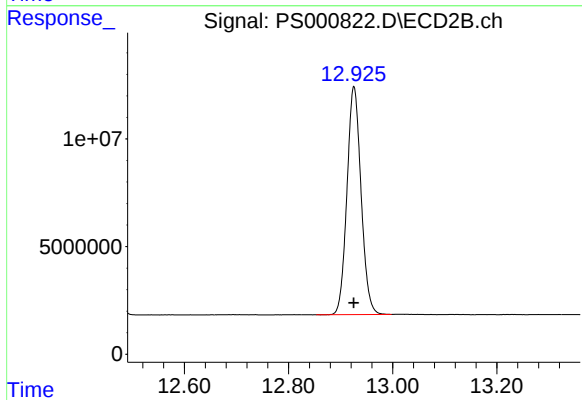


#9 2,4-D

R.T.: 12.925 min
Delta R.T.: 0.000 min
Response: 198876023
Conc: 705.00 ng/ml

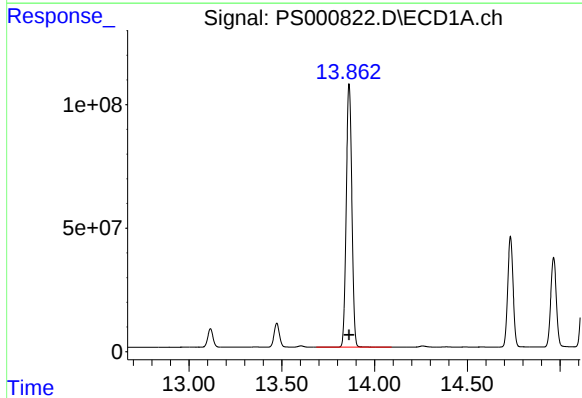


#10 Pentachlorophenol

R.T.: 13.863 min
Delta R.T.: 0.000 min
Response: 2234056667
Conc: 712.50 ng/ml

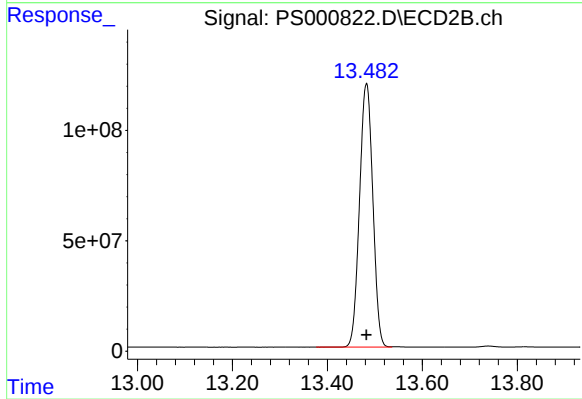

#10 Pentachlorophenol


R.T.: 13.482 min
Delta R.T.: 0.000 min
Response: 2319058998
Conc: 712.50 ng/ml

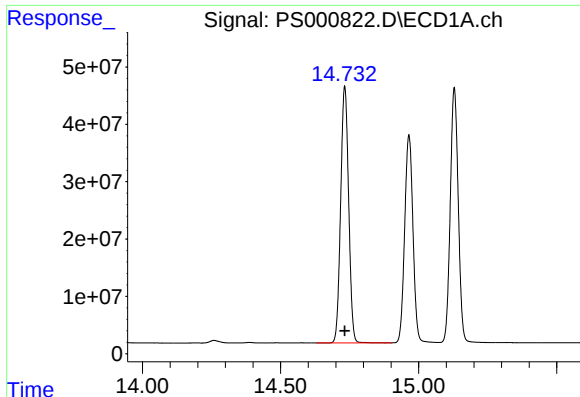

#11 2,4,5-TP (SILVEX)


R.T.: 14.732 min
Delta R.T.: 0.000 min
Response: 894543867
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

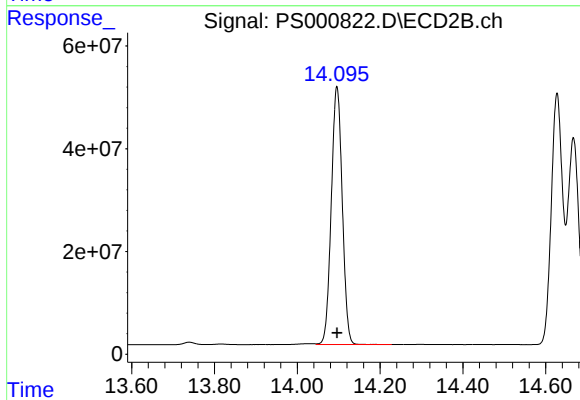


#11 2,4,5-TP (SILVEX)

R.T.: 14.096 min
Delta R.T.: 0.000 min
Response: 924784761
Conc: 712.50 ng/ml

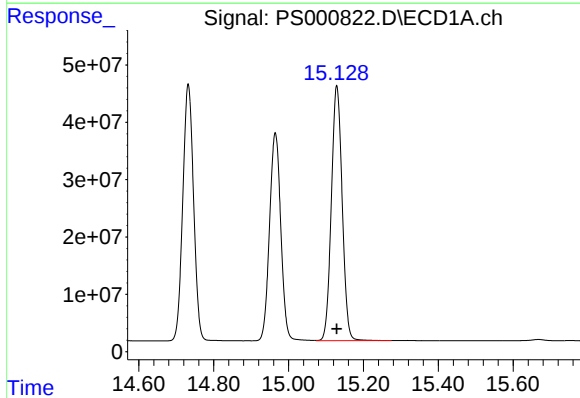


#12 2,4,5-T

R.T.: 15.129 min
Delta R.T.: 0.000 min
Response: 891408084
Conc: 712.50 ng/ml

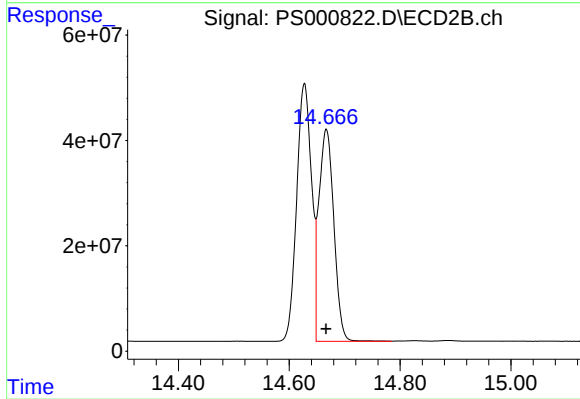

#12 2,4,5-T


R.T.: 14.667 min
Delta R.T.: 0.000 min
Response: 752244806
Conc: 712.50 ng/ml

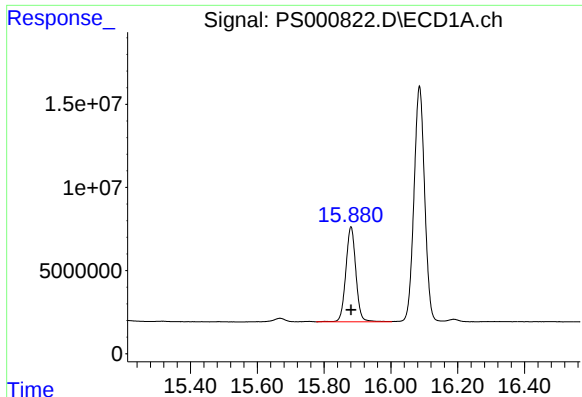

#13 2,4-DB


R.T.: 15.880 min
Delta R.T.: 0.000 min
Response: 119278888
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

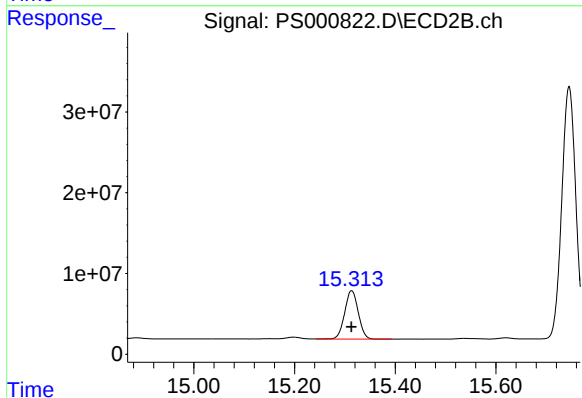


#13 2,4-DB

R.T.: 15.313 min
Delta R.T.: 0.000 min
Response: 112542387
Conc: 712.50 ng/ml

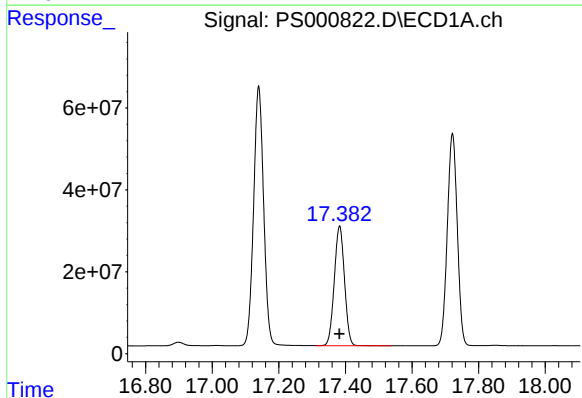


#14 DINOSEB

R.T.: 17.382 min
Delta R.T.: 0.000 min
Response: 620401774
Conc: 705.00 ng/ml

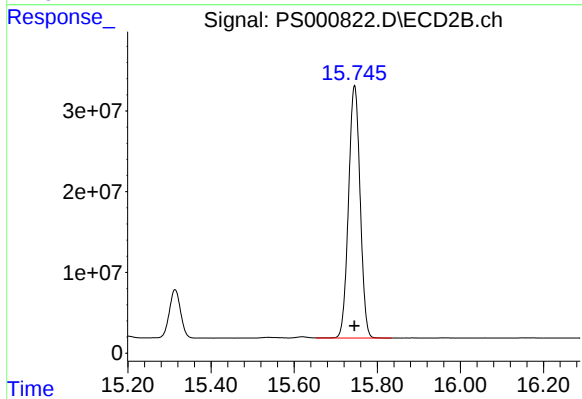

#14 DINOSEB


R.T.: 15.745 min
Delta R.T.: 0.000 min
Response: 605395549
Conc: 705.00 ng/ml

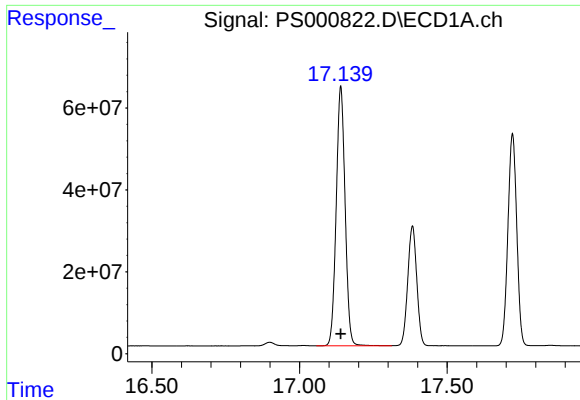

#15 Picloram


R.T.: 17.139 min
Delta R.T.: 0.000 min
Response: 1327190517
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

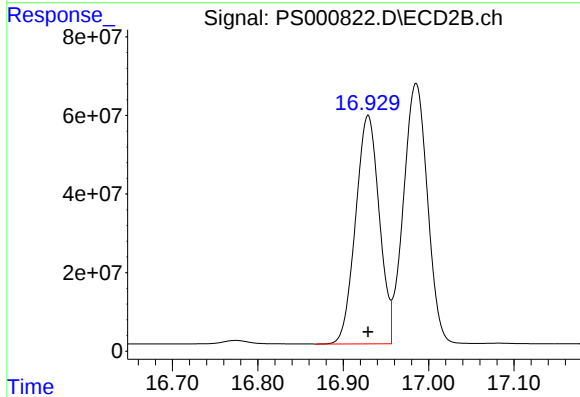


#15 Picloram

R.T.: 16.929 min
Delta R.T.: 0.000 min
Response: 1119281508
Conc: 712.50 ng/ml

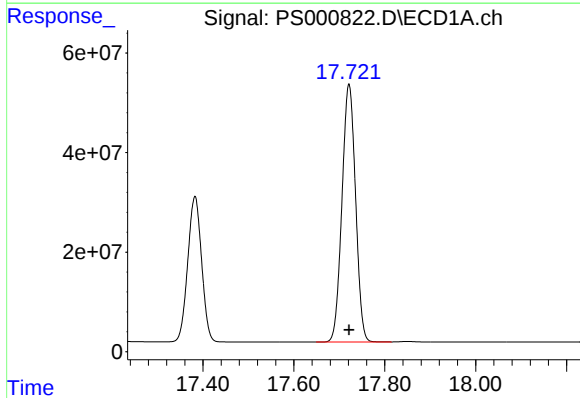

#16 DCPA

R.T.: 17.721 min
Delta R.T.: 0.000 min
Response: 1073644951
Conc: 720.00 ng/ml

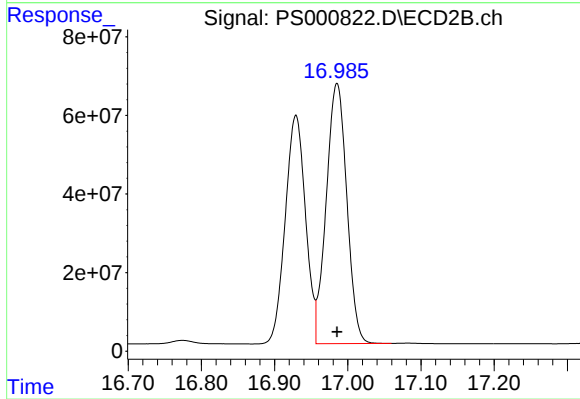

#16 DCPA

R.T.: 16.985 min
Delta R.T.: 0.000 min
Response: 1291665077
Conc: 720.00 ng/ml