

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070822\
 Data File : PS019820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jul 2022 20:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 01:05:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
 Quant Title : 8080.M
 QLast Update : Mon Jun 27 17:26:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.194	6.779	1199.2E6	411.8E6	462.360	507.072
Target Compounds							
2) T	3,5-DICHL...	6.356f	5.926	529132	69237	<MDL	<MDL #
7) T	MCPA	7.716	0.000	3022282	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.629f	0	2387255	N.D.	2.538
10) T	Pentachlo...	8.610	8.281	782936	1048248	<MDL	<MDL #
11) T	2,4,5-TP ...	9.174	8.610	1979464	346198	<MDL	<MDL #
12) T	2,4,5-T	9.419	9.048	9265669	318923	<MDL	<MDL #
13) T	2,4-DB	10.017	9.462f	4865896	1528047	1.216	2.353 #
14) T	DINOSEB	0.000	9.846	0	362345	N.D.	<MDL
15) T	Picloram	10.970	10.802	1625688	2623347	<MDL	<MDL #
16) T	DCPA	11.415	10.802	566614	2623347	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070822\
Data File : PS019820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jul 2022 20:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 01:05:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062722.M
Quant Title : 8080.M
QLast Update : Mon Jun 27 17:26:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

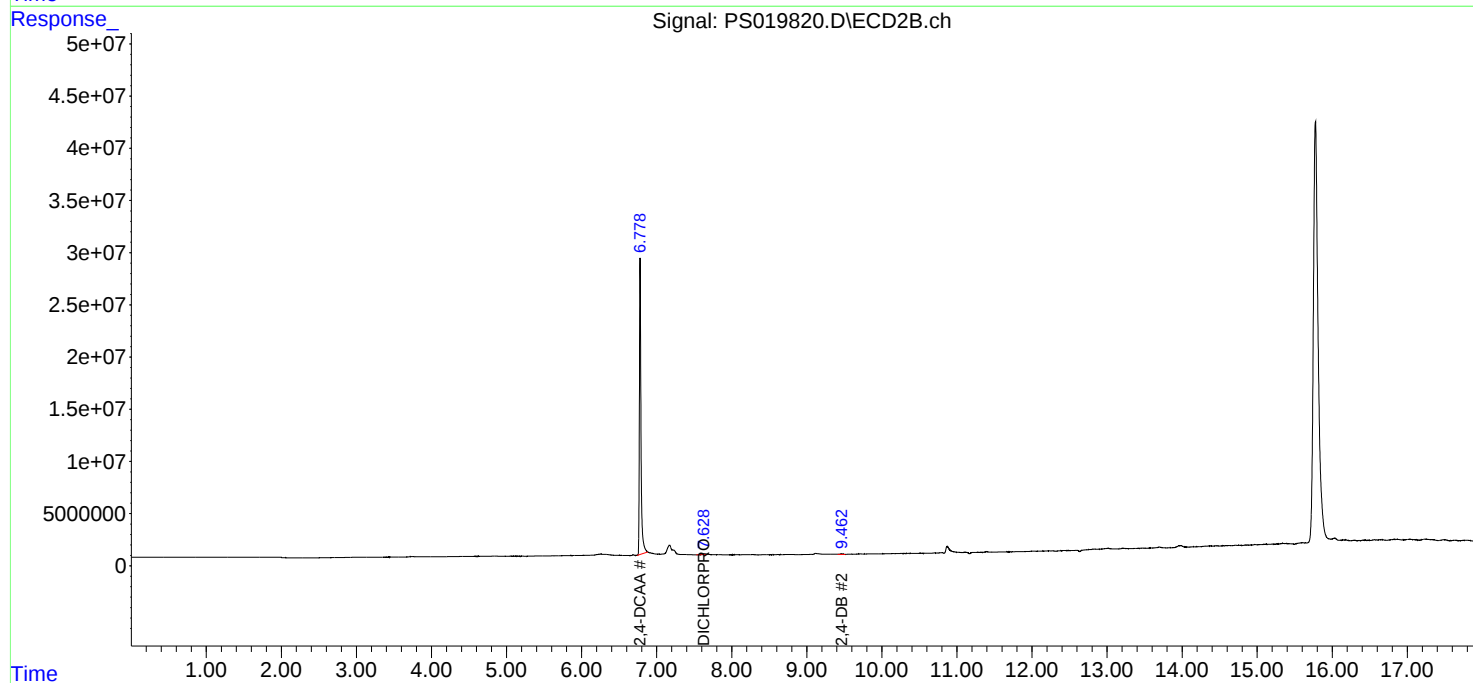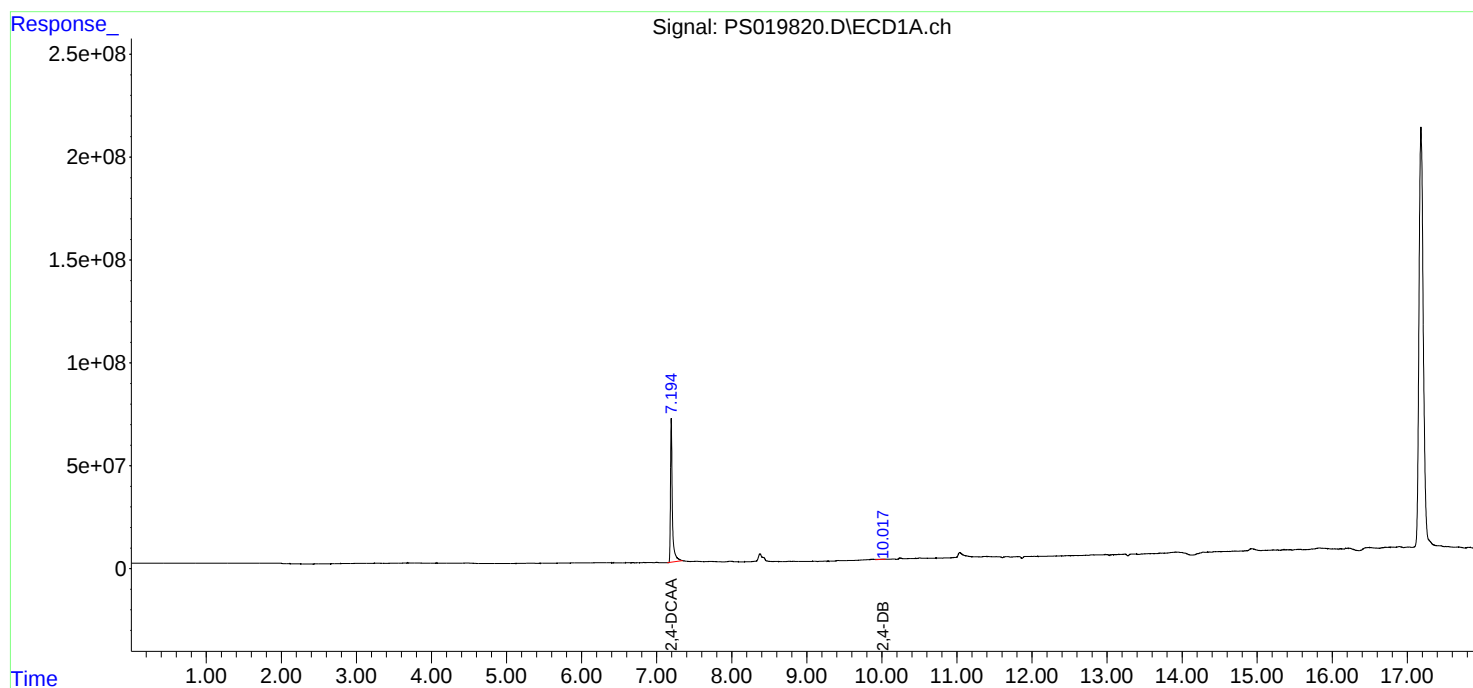


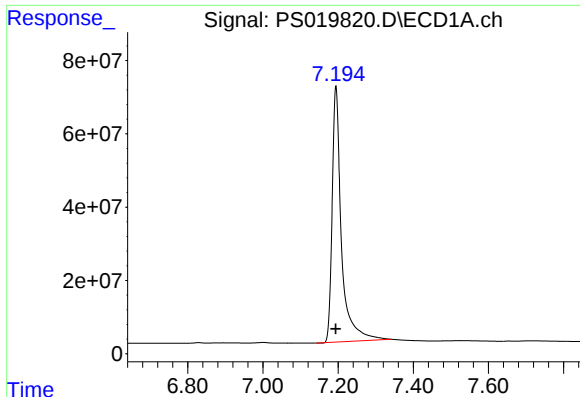

#4 2,4-DCAA


R.T.: 7.194 min
Delta R.T.: 0.000 min
Response: 1199201690
Conc: 462.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

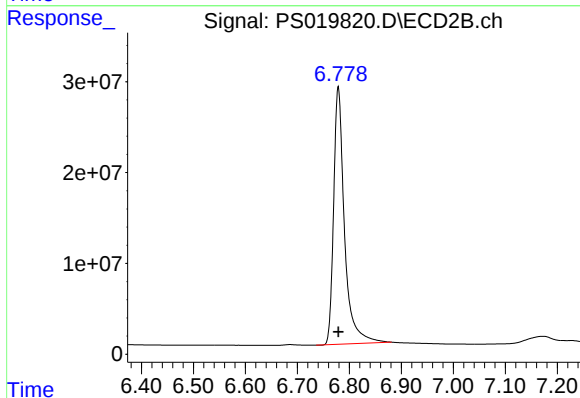


#4 2,4-DCAA

R.T.: 6.779 min
Delta R.T.: 0.000 min
Response: 411816378
Conc: 507.07 ng/ml

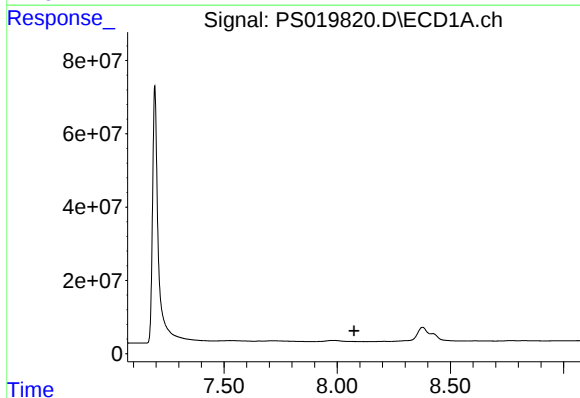


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.074 min
Response: 0
Conc: N.D.

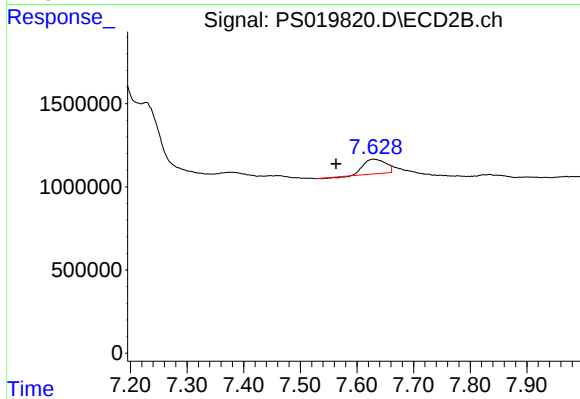

#8 DICHLORPROP


R.T.: 7.629 min
Delta R.T.: 0.066 min
Response: 2387255
Conc: 2.54 ng/ml

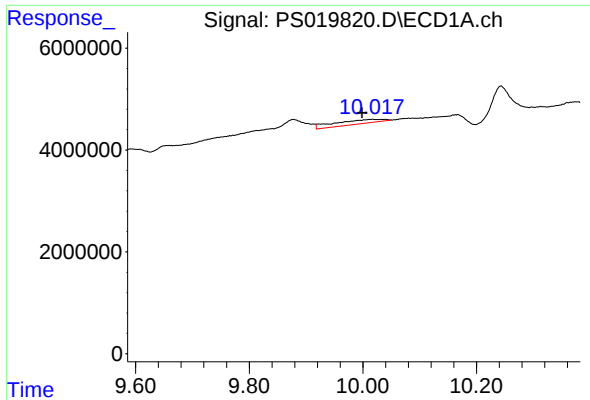

#13 2,4-DB

R.T.: 10.017 min
Delta R.T.: 0.018 min
Response: 4865896
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

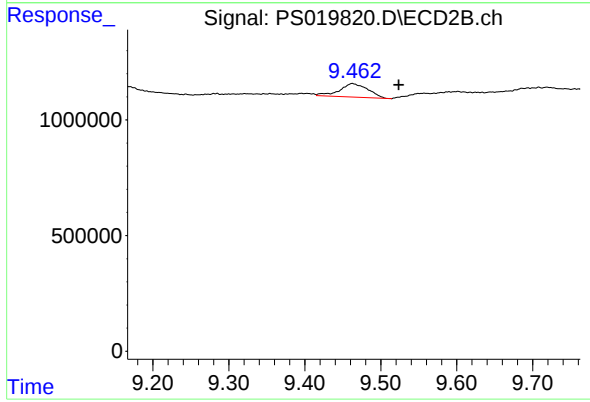

#13 2,4-DB

R.T.: 9.462 min
Delta R.T.: -0.061 min
Response: 1528047
Conc: 2.35 ng/ml