

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 08:37
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 12:35:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.489	0.000	38200159	0	30.365	N.D. #
5) T	DICAMBA	0.000	7.152	0	36863440	N.D.	16.230
6) T	MCPD	0.000	7.152	0	36863440	N.D.	19.476
7) T	MCPA	7.680	0.000	15614024	0	3.921	N.D. #
8) T	DICHLORPROP	0.000	7.740	0	12162799	N.D.	20.716
9) T	2,4-D	0.000	8.046	0	142.8E6	N.D.	197.670
10) T	Pentachlo...	8.591	0.000	115.3E6	0	9.276	N.D. #
15) T	Picloram	11.035	11.005	29469927	24304731	5.257	5.801
16) T	DCPA	0.000	11.005	0	24304731	N.D.	6.526



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 08:37
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 12:35:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

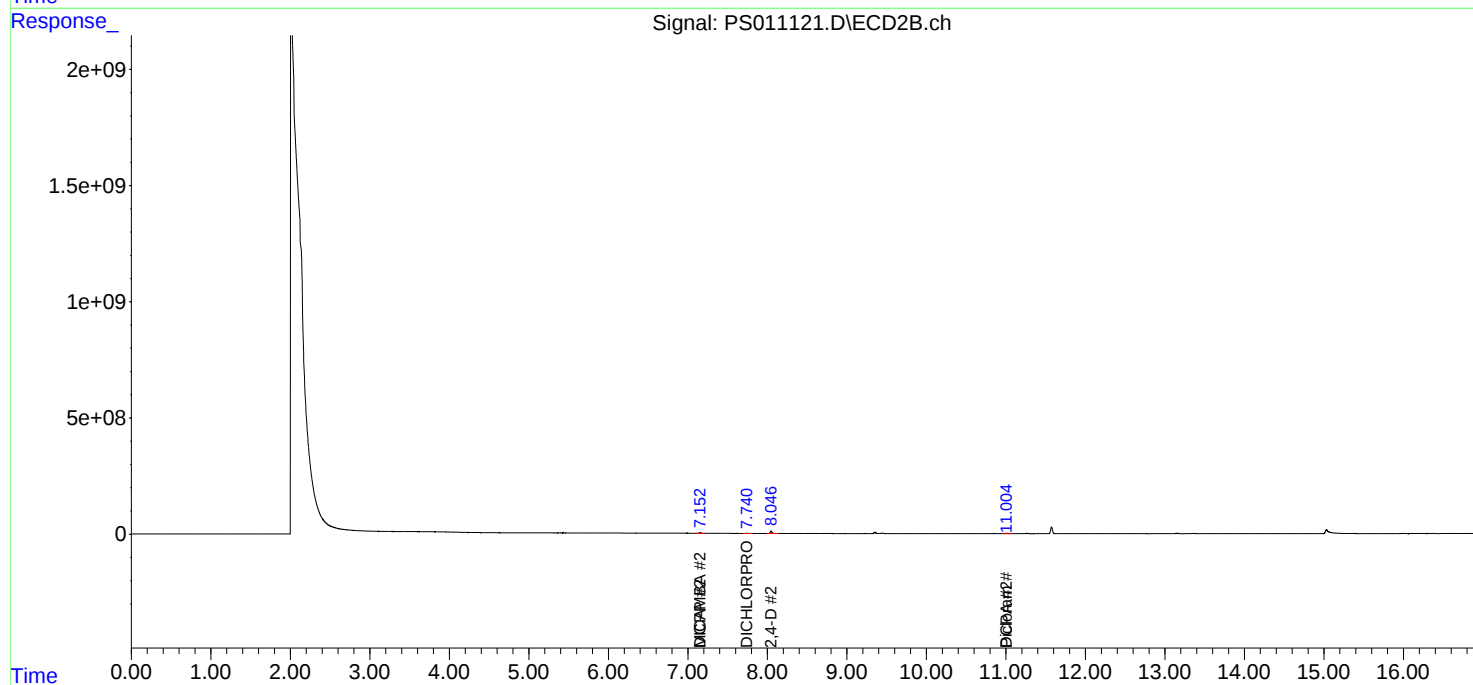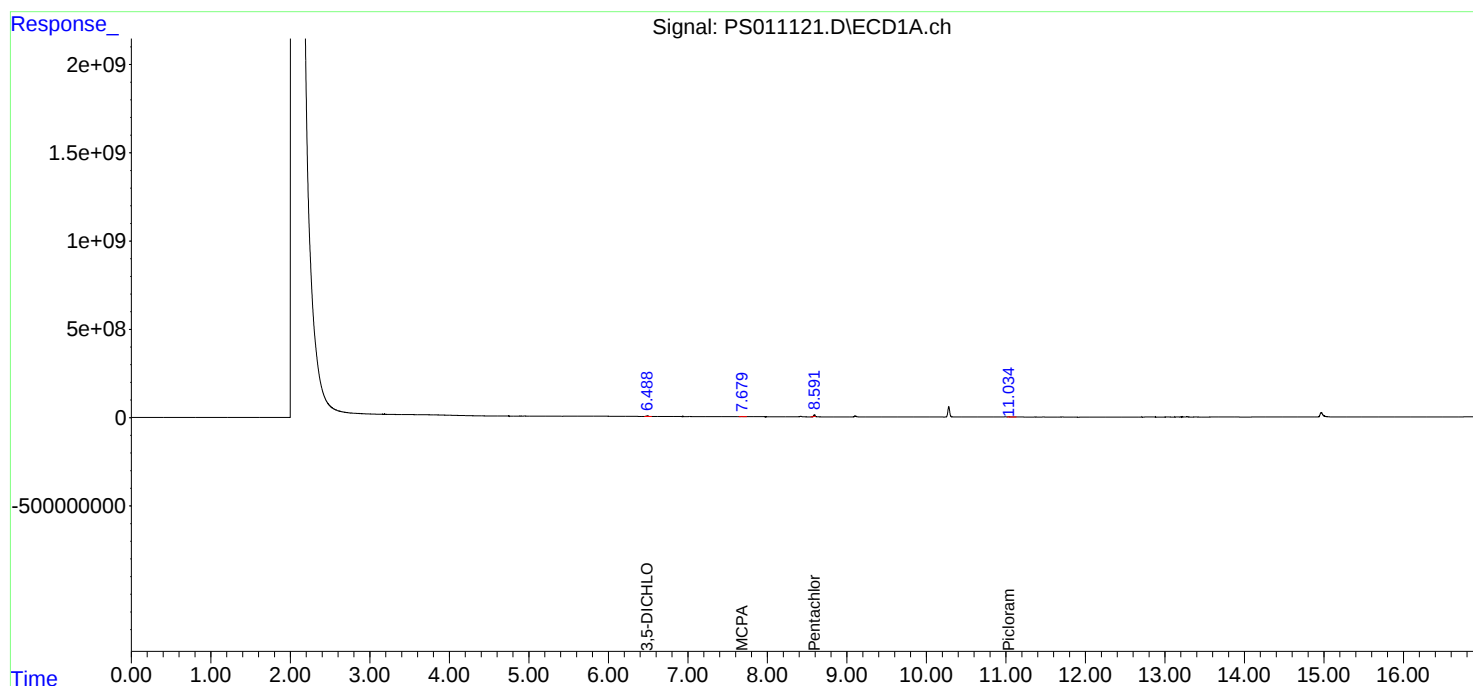


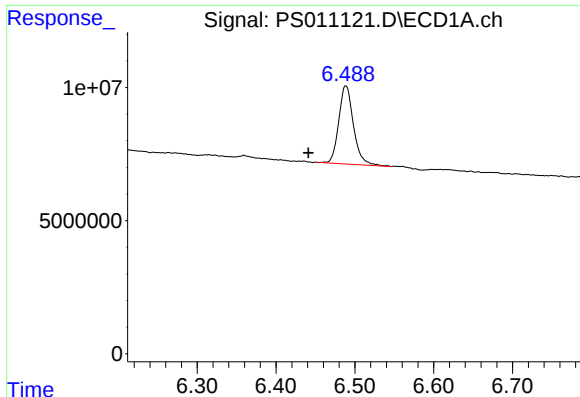

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.489 min
Delta R.T.: 0.047 min
Response: 38200159
Conc: 30.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

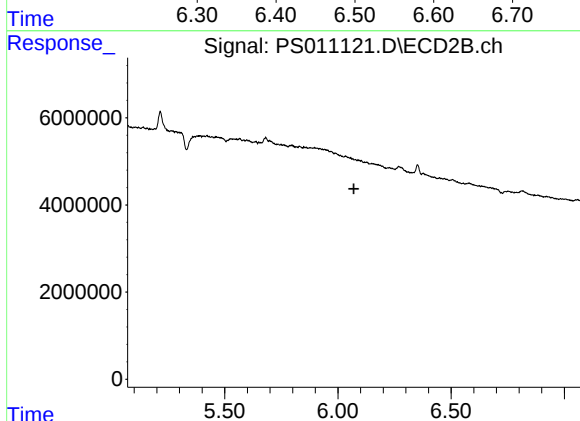


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

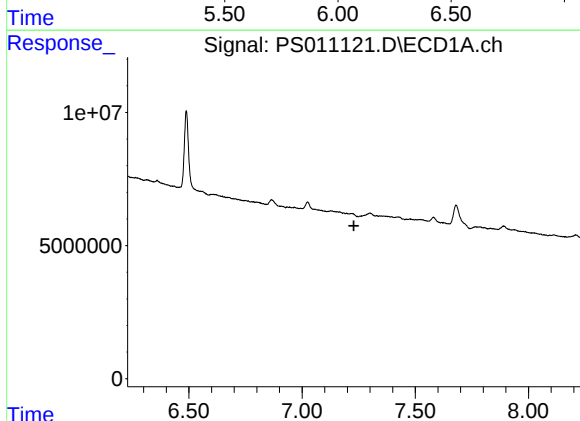


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

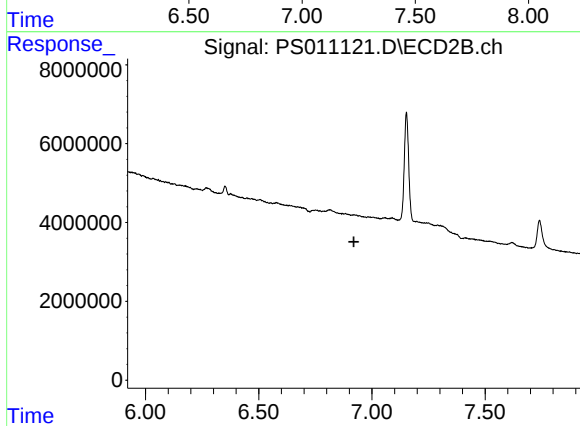

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

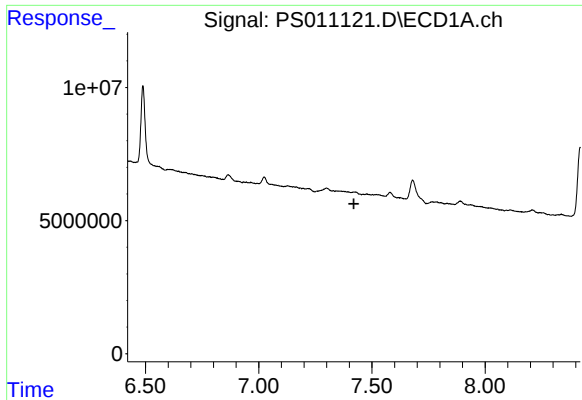

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

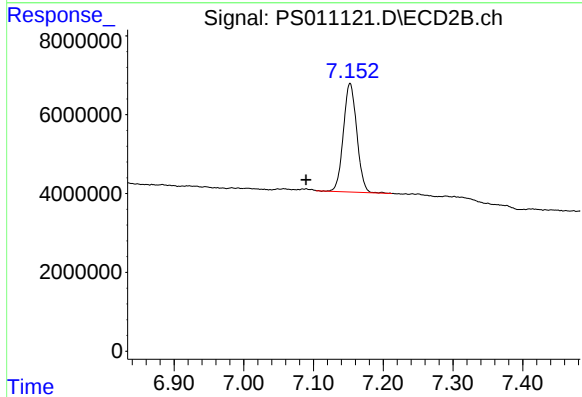


#5 DICAMBA

R.T.: 7.152 min
Delta R.T.: 0.063 min
Response: 36863440
Conc: 16.23 ng/ml

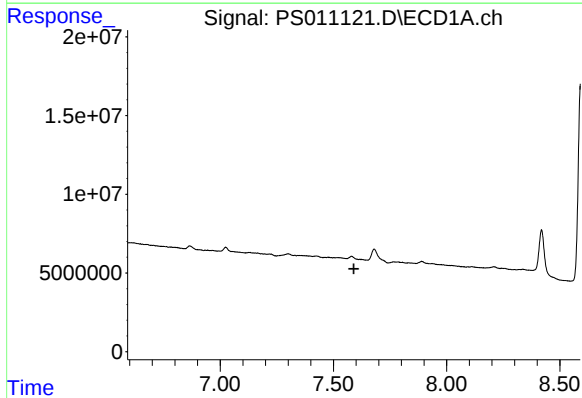


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.590 min
Response: 0
Conc: N.D.

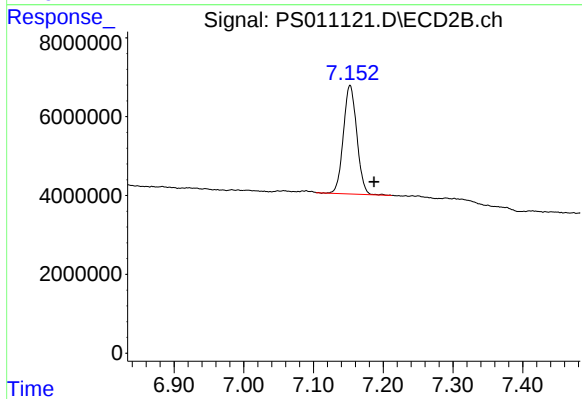

#6 MCP


R.T.: 7.152 min
Delta R.T.: -0.034 min
Response: 36863440
Conc: 19.48 ug/ml

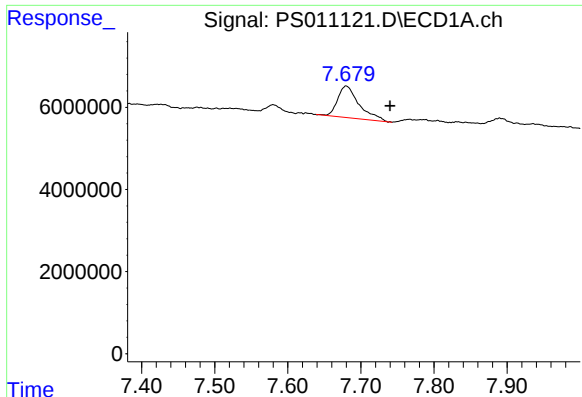

#7 MCPA


R.T.: 7.680 min
Delta R.T.: -0.060 min
Response: 15614024
Conc: 3.92 ug/ml

Instrument :
ECD_S
ClientSampleId :

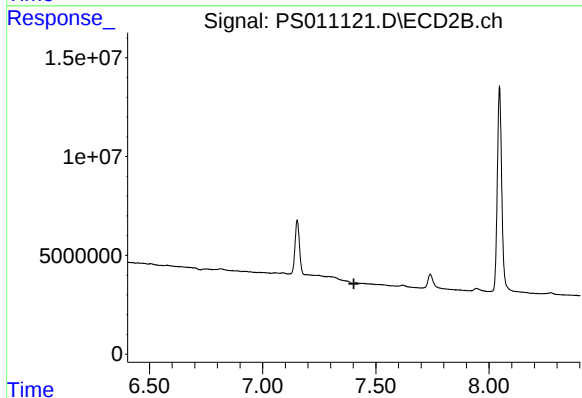


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

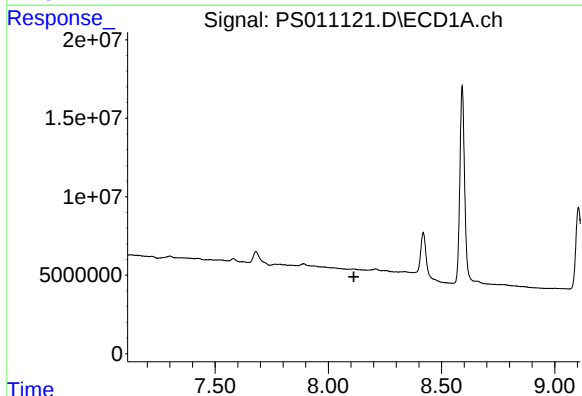


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

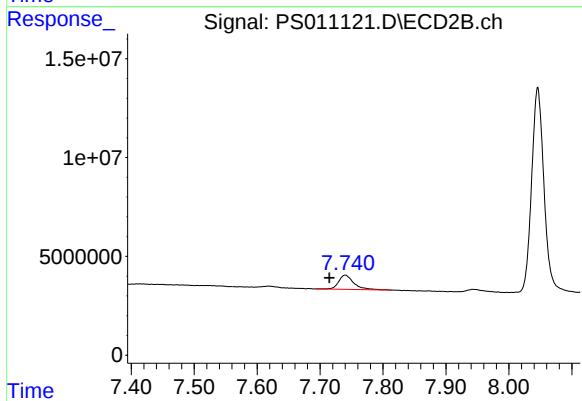

#8 DICHLORPROP


R.T.: 7.740 min
Delta R.T.: 0.025 min
Response: 12162799
Conc: 20.72 ng/ml

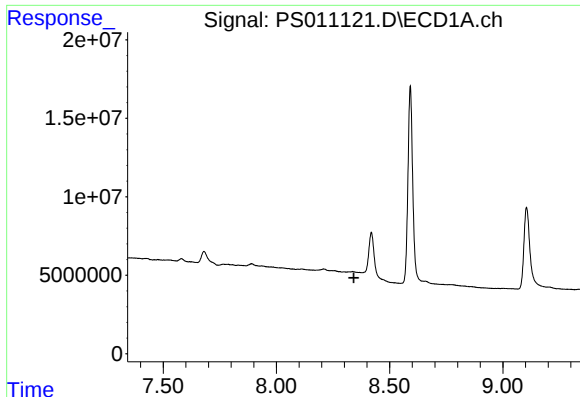

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

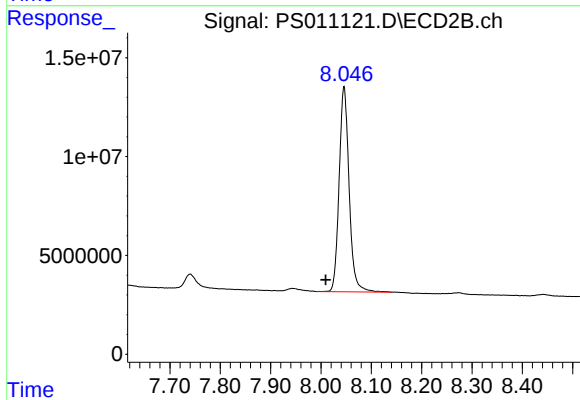


#9 2,4-D

R.T.: 8.046 min
Delta R.T.: 0.036 min
Response: 142846664
Conc: 197.67 ng/ml

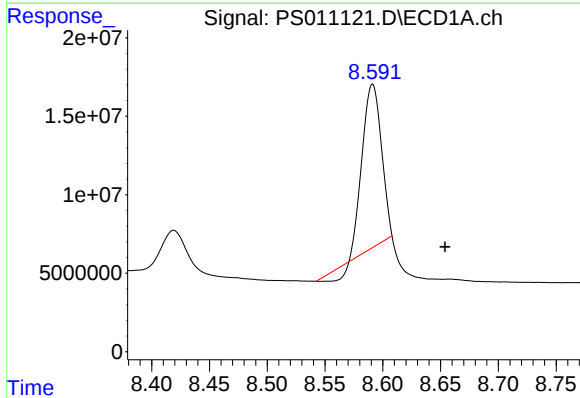


#10 Pentachlorophenol

R.T.: 8.591 min
Delta R.T.: -0.063 min
Response: 115339725
Conc: 9.28 ng/ml

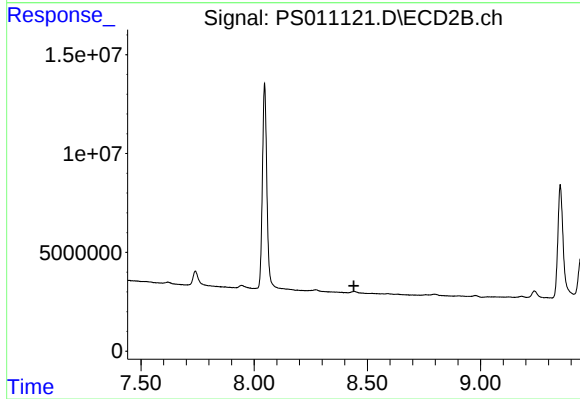

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.440 min
Response: 0
Conc: N.D.

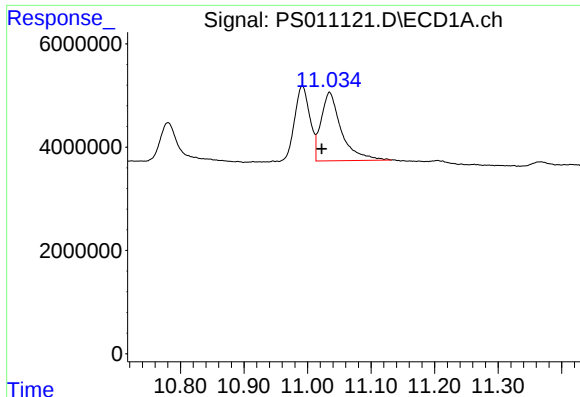

#15 Picloram


R.T.: 11.035 min
Delta R.T.: 0.012 min
Response: 29469927
Conc: 5.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

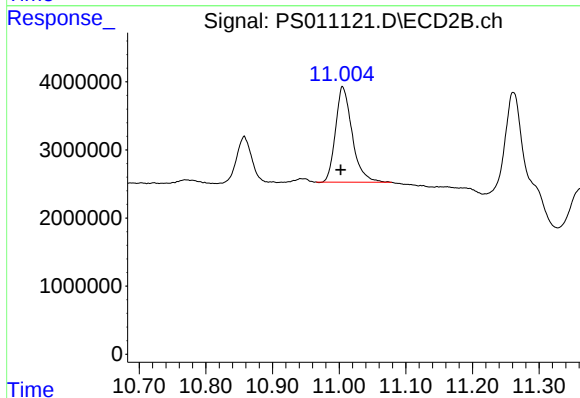


#15 Picloram

R.T.: 11.005 min
Delta R.T.: 0.003 min
Response: 24304731
Conc: 5.80 ng/ml

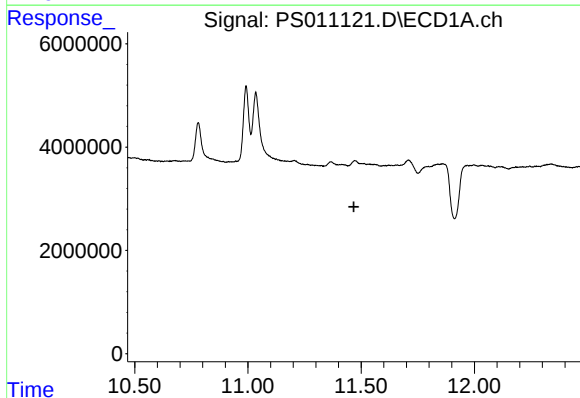

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

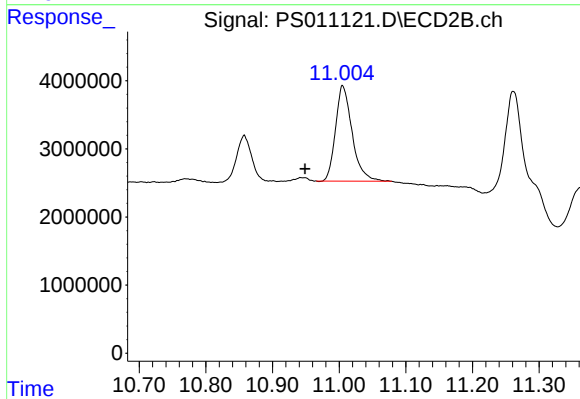

#16 DCPA

R.T.: 11.005 min
Delta R.T.: 0.057 min
Response: 24304731
Conc: 6.53 ng/ml