

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 16:35
 Operator : DD\AJ
 Sample : PB130049BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 19:05:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.917	397.0E6	276.1E6	437.759	498.257
Target Compounds							
1) T	Dalapon	2.996	2.581	45472673	241.0E6	40.611	319.414 #
2) T	3,5-DICHL...	0.000	6.097	0	100.8E6	N.D.	121.021
3) T	4-Nitroph...	6.999	0.000	7040118	0	17.637	N.D. #
5) T	DICAMBA	7.413	0.000	6170412	0	1.692	N.D. #
6) T	MCPD	7.644	0.000	5626892	0	1.973	N.D. #
7) T	MCPA	7.692	7.458	194.0E6	143.2E6	48.705	51.888
8) T	DICHLORPROP	0.000	7.738	0	23651101	N.D.	40.282
10) T	Pentachlo...	8.713	0.000	15545039	0	1.250	N.D. #
12) T	2,4,5-T	9.430	9.238	49756952	20518742	10.682	6.890 #
15) T	Picloram	11.033	11.004	94133500	75706599	16.791	18.070
16) T	DCPA	0.000	11.004	0	75706599	N.D.	20.327



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 16:35
Operator : DD\AJ
Sample : PB130049BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 19:05:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

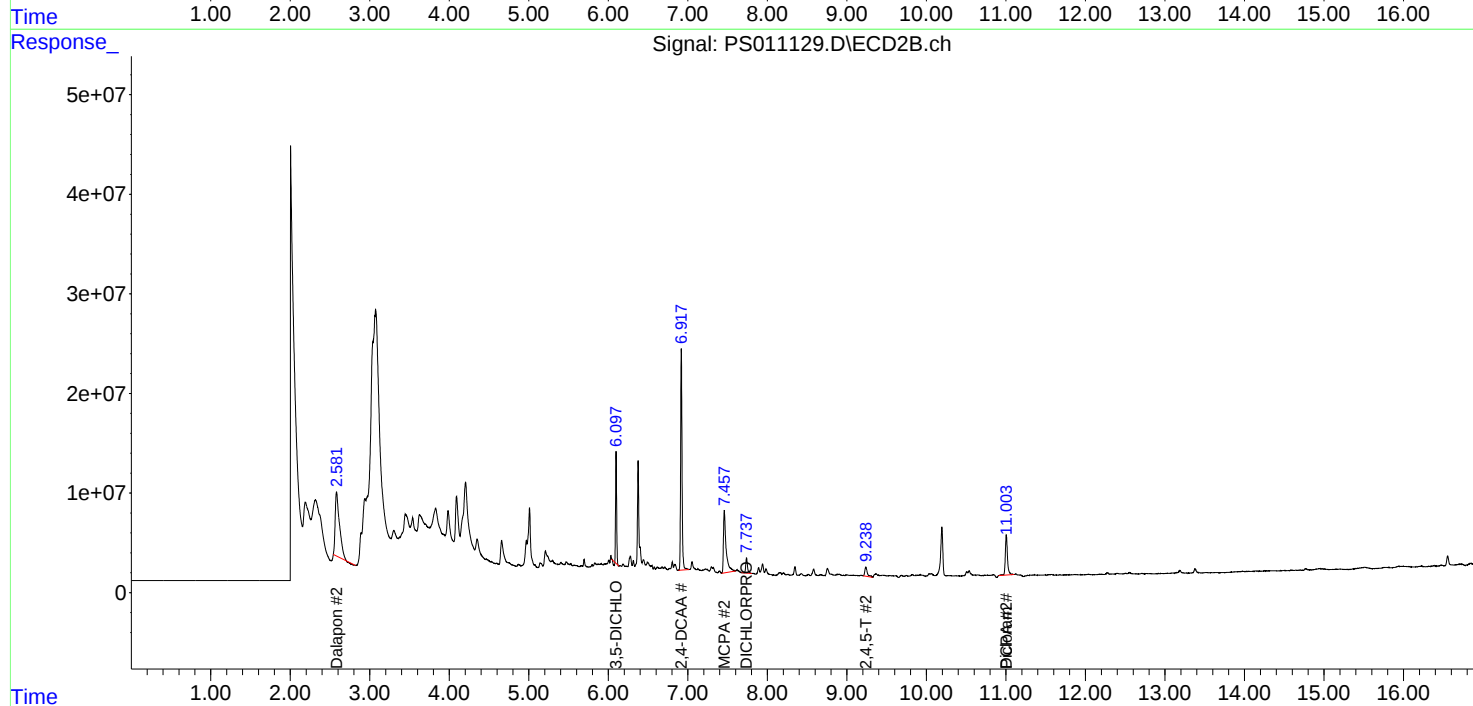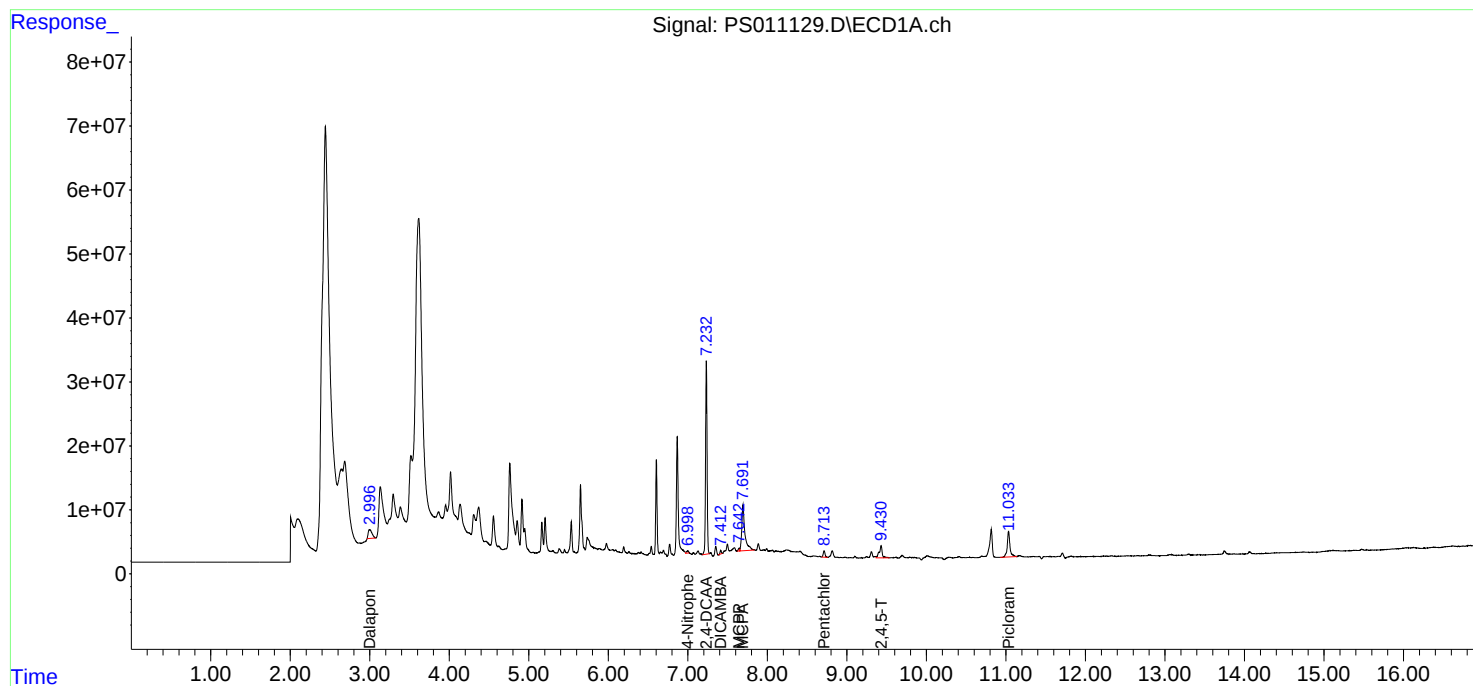


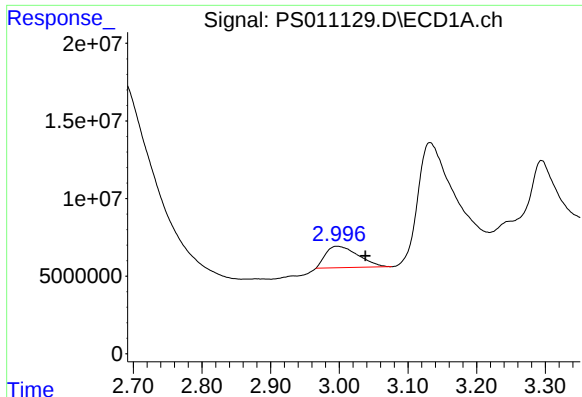

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 45472673
Conc: 40.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

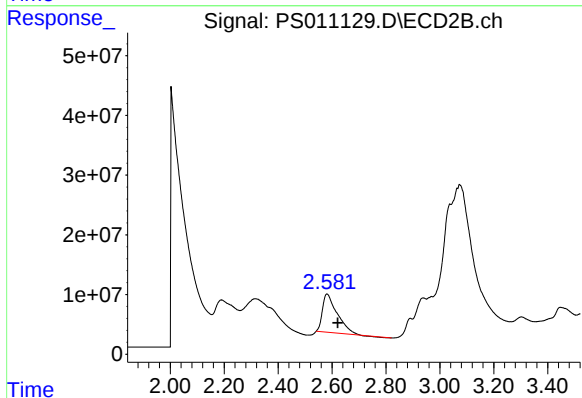


#1 Dalapon

R.T.: 2.581 min
Delta R.T.: -0.040 min
Response: 240953681
Conc: 319.41 ng/ml

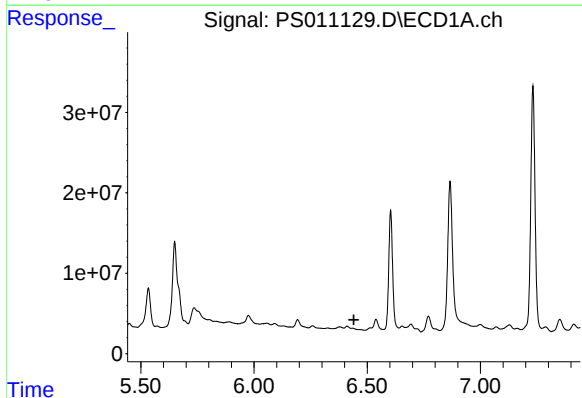


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

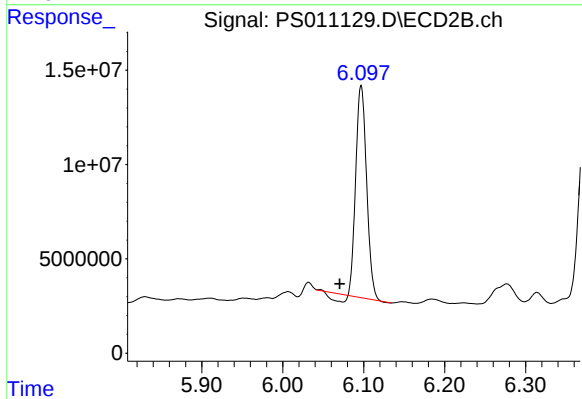

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.097 min
Delta R.T.: 0.027 min
Response: 100789224
Conc: 121.02 ng/ml

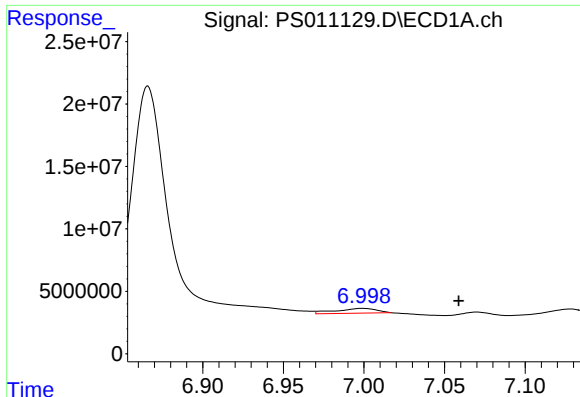

#3 4-Nitrophenol


R.T.: 6.999 min
Delta R.T.: -0.060 min
Response: 7040118
Conc: 17.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

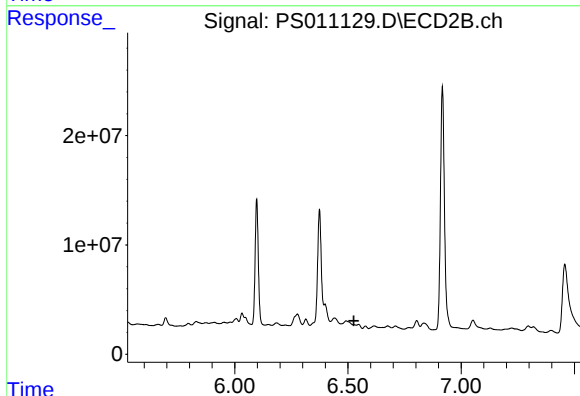


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

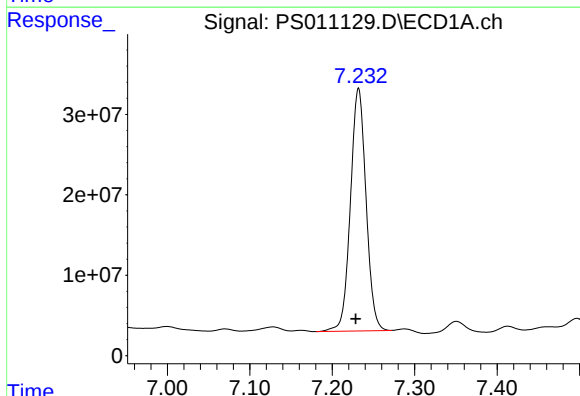


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: 0.004 min
Response: 396967526
Conc: 437.76 ng/ml

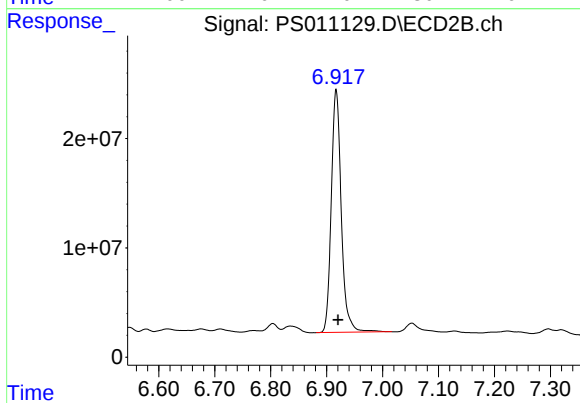

#4 2,4-DCAA


R.T.: 6.917 min
Delta R.T.: -0.003 min
Response: 276072349
Conc: 498.26 ng/ml

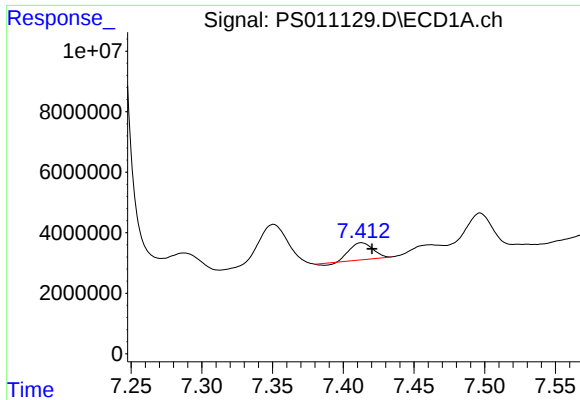

#5 DICAMBA


R.T.: 7.413 min
Delta R.T.: -0.007 min
Response: 6170412
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

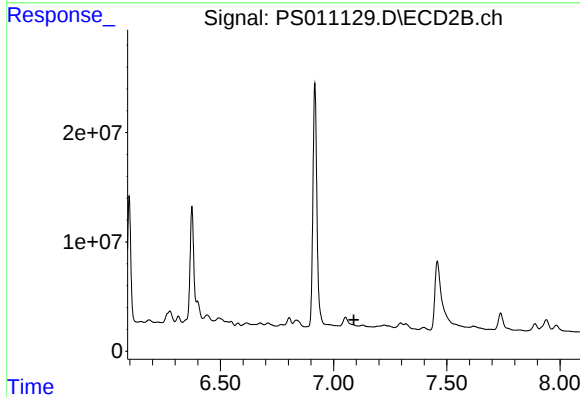


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

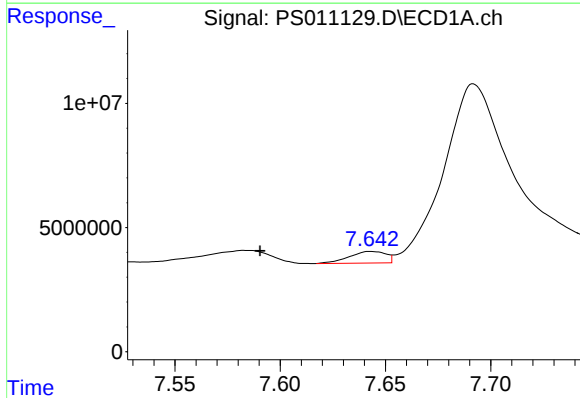


#6 MCP

R.T.: 7.644 min
Delta R.T.: 0.053 min
Response: 5626892
Conc: 1.97 ug/ml

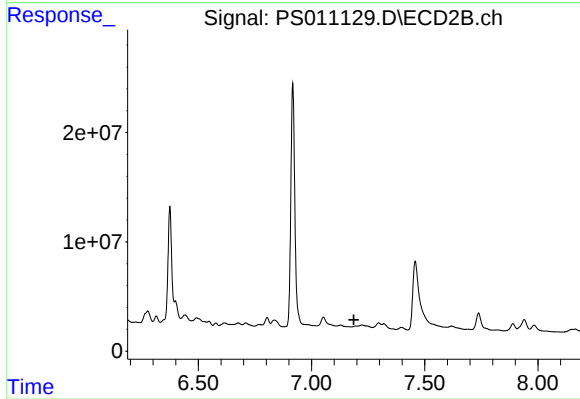

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

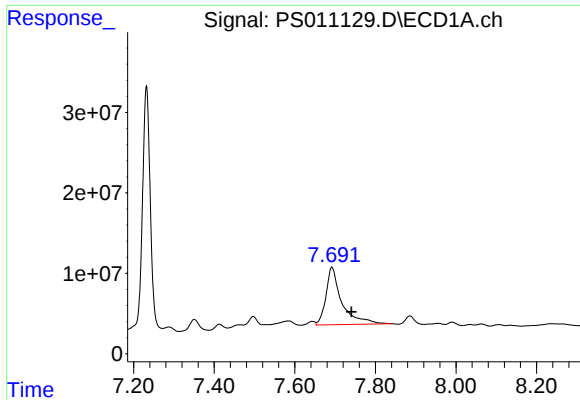

#7 MCPA


R.T.: 7.692 min
Delta R.T.: -0.048 min
Response: 193962685
Conc: 48.70 ug/ml

Instrument :
ECD_S
ClientSampleId :

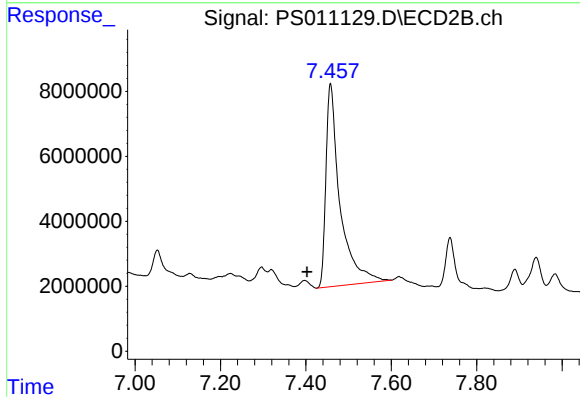


#7 MCPA

R.T.: 7.458 min
Delta R.T.: 0.055 min
Response: 143209029
Conc: 51.89 ug/ml

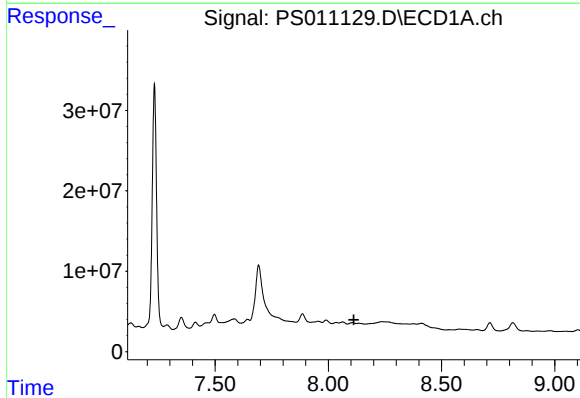


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

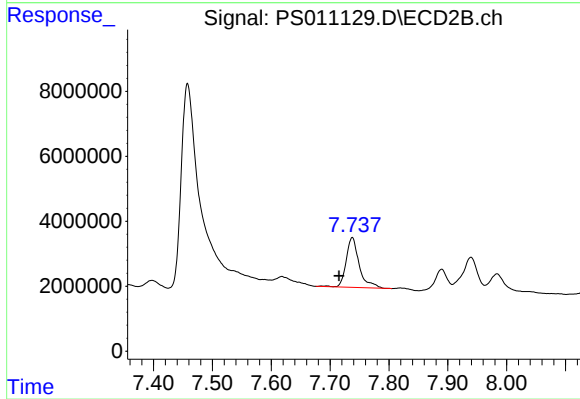

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.022 min
Response: 23651101
Conc: 40.28 ng/ml

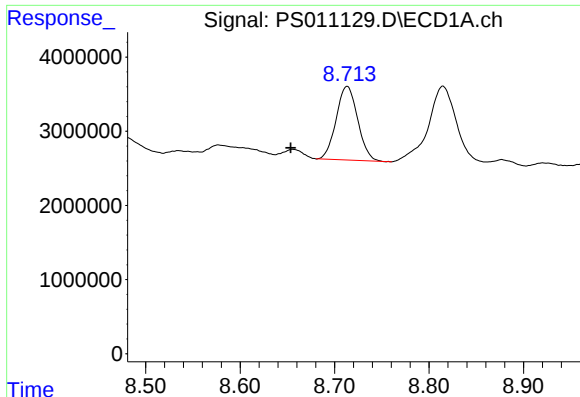

#10 Pentachlorophenol


R.T.: 8.713 min
Delta R.T.: 0.059 min
Response: 15545039
Conc: 1.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

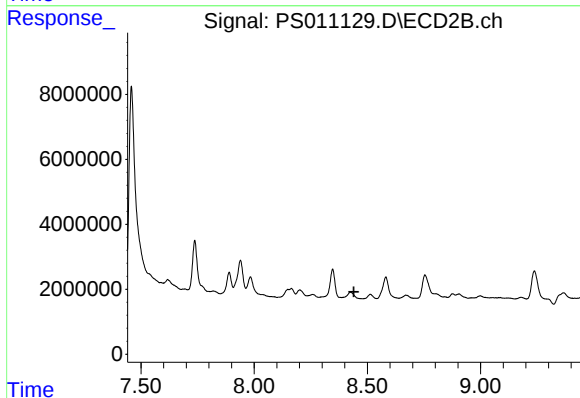


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

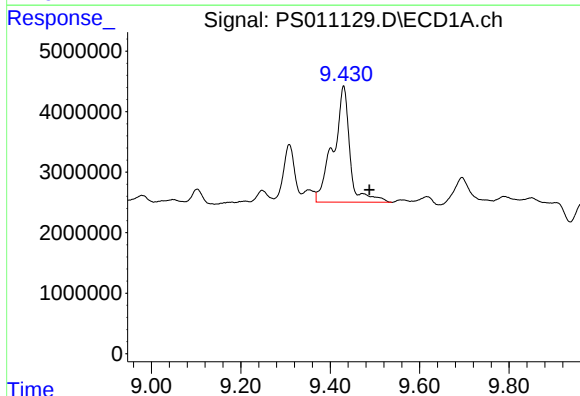


#12 2,4,5-T

R.T.: 9.430 min
Delta R.T.: -0.058 min
Response: 49756952
Conc: 10.68 ng/ml

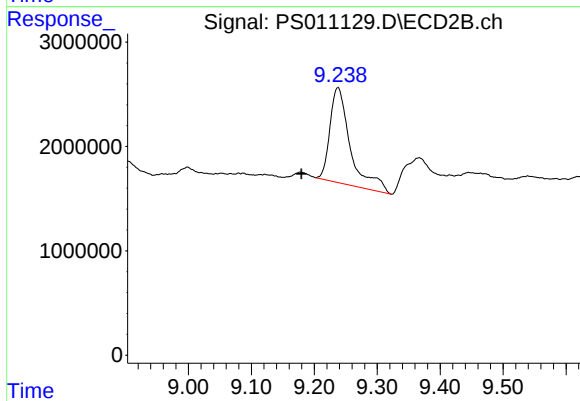

#12 2,4,5-T


R.T.: 9.238 min
Delta R.T.: 0.058 min
Response: 20518742
Conc: 6.89 ng/ml

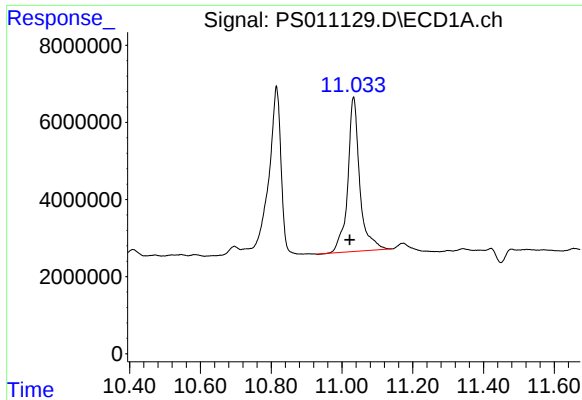

#15 Picloram


R.T.: 11.033 min
Delta R.T.: 0.010 min
Response: 94133500
Conc: 16.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

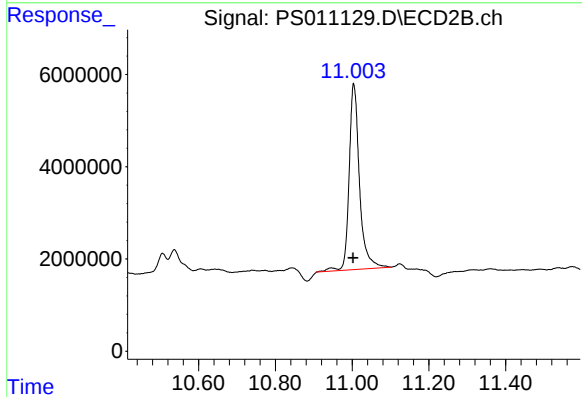


#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.002 min
Response: 75706599
Conc: 18.07 ng/ml

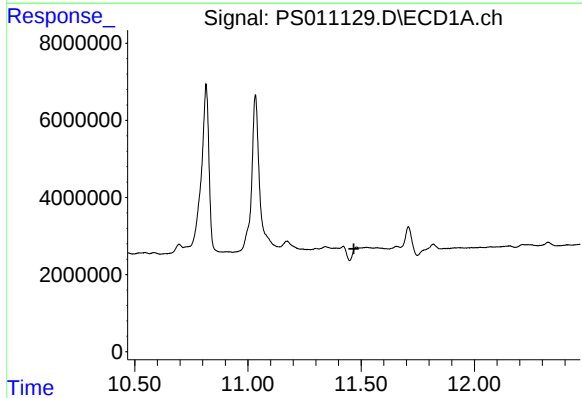

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

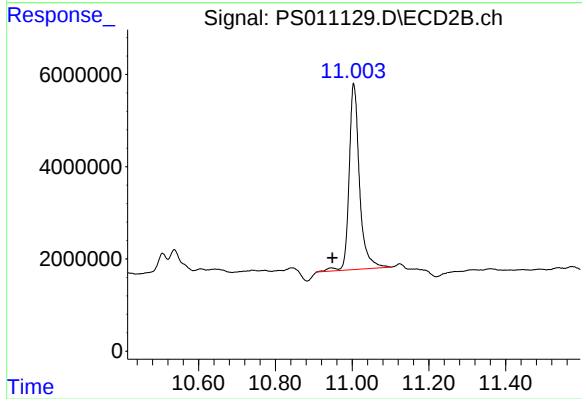

#16 DCPA

R.T.: 11.004 min
Delta R.T.: 0.056 min
Response: 75706599
Conc: 20.33 ng/ml