

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011134.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 18:30
 Operator : DD\AJ
 Sample : L3203-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 19:06:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.920	1817.4E6	168.0E6	2004.194	303.285 #
Target Compounds							
1) T	Dalapon	2.997	2.586	39069461	185.3E6	34.892	245.590 #
2) T	3,5-DICHL...	0.000	6.100	0	43497716	N.D.	52.229
3) T	4-Nitroph...	7.062	0.000	4635690	0	11.613	N.D. #
5) T	DICAMBA	0.000	7.128	0	7457835	N.D.	3.284
6) T	MCPD	7.584	7.212	7085636	11349691	2.485	5.996 #
7) T	MCPA	7.776	7.382	18854520	22687241	4.734	8.220 #
8) T	DICHLORPROP	0.000	7.736	0	13960510	N.D.	23.777
9) T	2,4-D	8.275	7.987	76350461	8987956	86.340	12.437 #
10) T	Pentachlo...	8.653	8.439	28777.2E6	13486.9E6	2314.363	1939.525
11) T	2,4,5-TP ...	9.137	8.782	52629418	106.5E6	10.599	35.408 #
12) T	2,4,5-T	9.432	0.000	52778188	0	11.331	N.D. #
13) T	2,4-DB	0.000	9.678	0	52063786	N.D.	126.680
14) T	DINOSEB	11.167	10.036	65328278	26105977	18.241	12.538 #
15) T	Picloram	10.992	10.993	166.4E6	16072185	29.677	3.836 #
16) T	DCPA	0.000	10.993	0	16072185	N.D.	4.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011134.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 18:30
Operator : DD\AJ
Sample : L3203-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 19:06:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

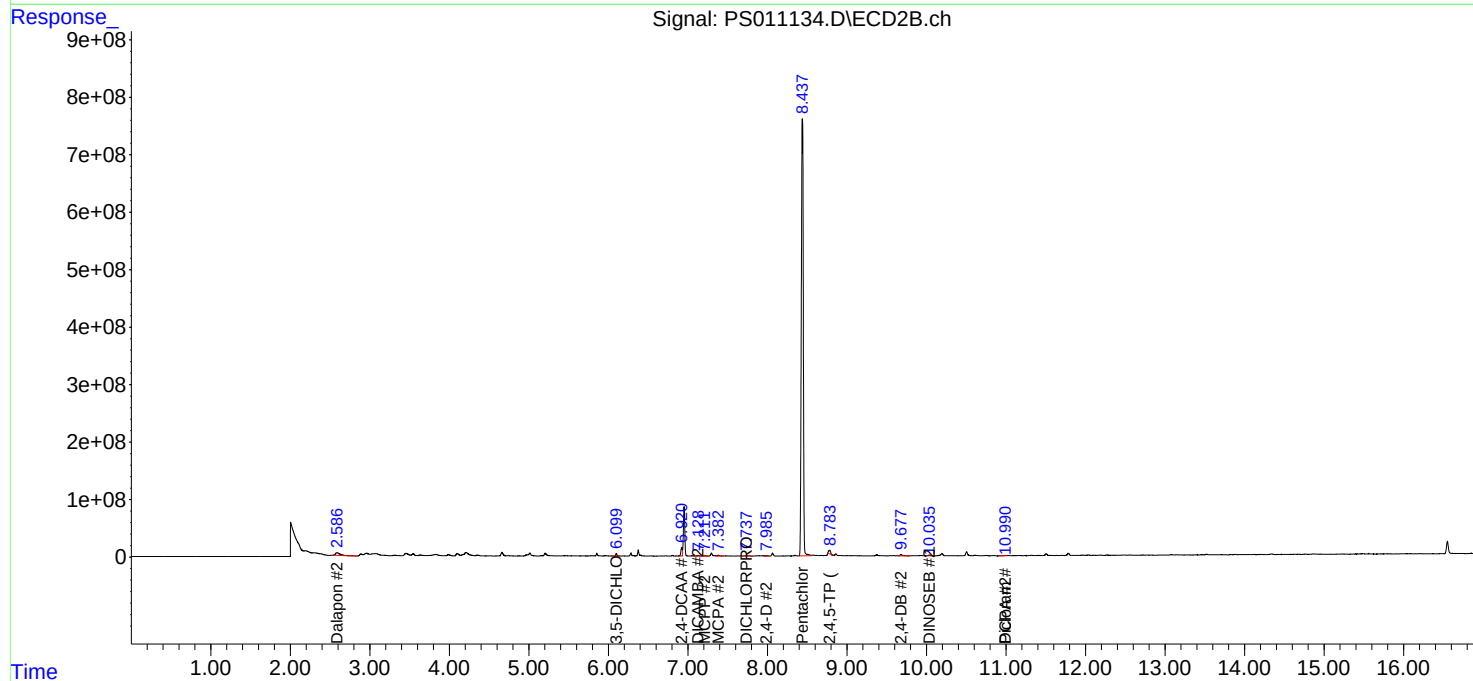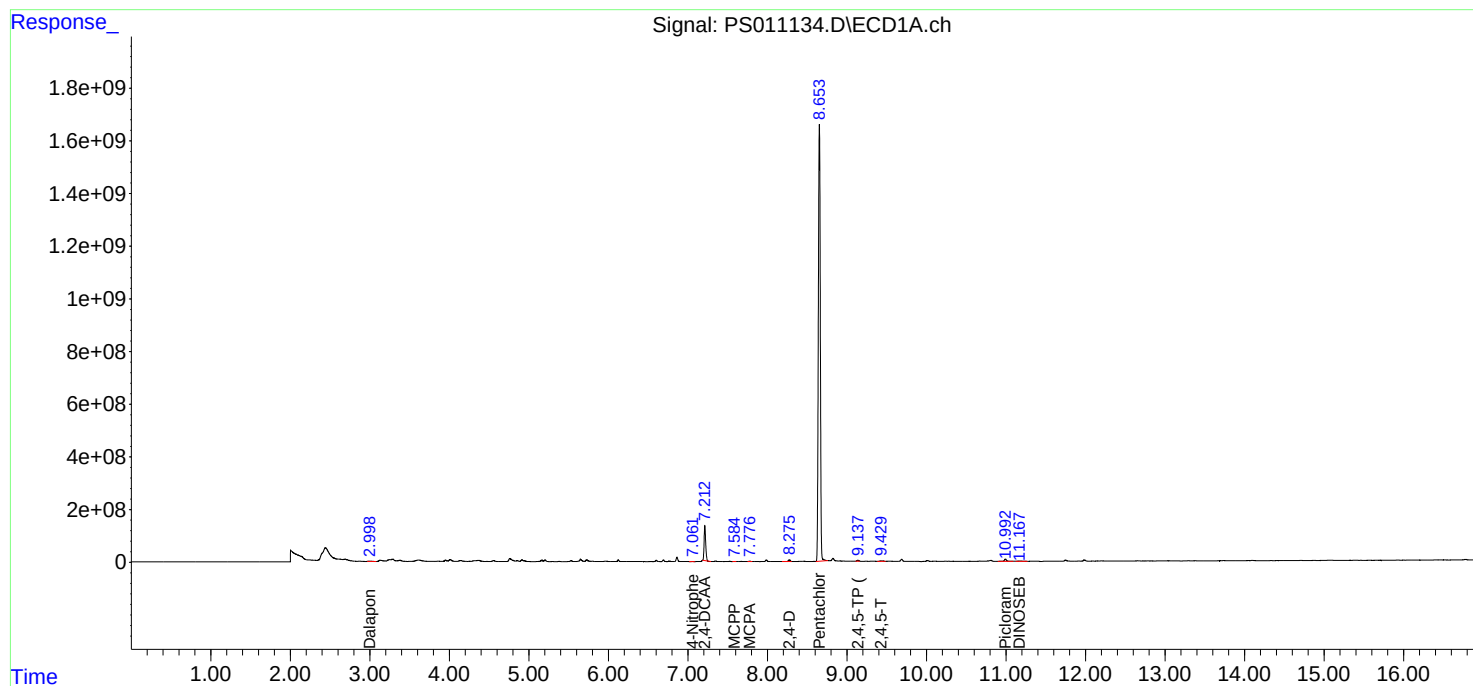


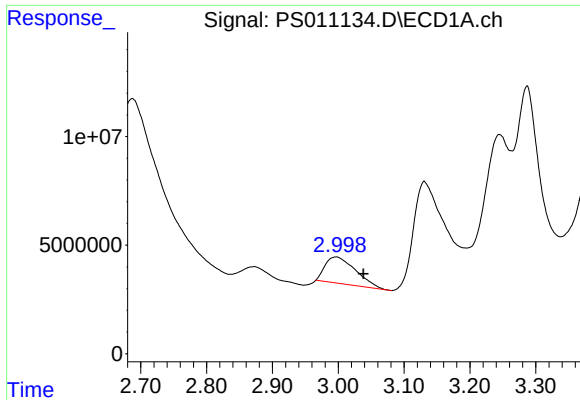

#1 Dalapon


R.T.: 2.997 min
Delta R.T.: -0.041 min
Response: 39069461
Conc: 34.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

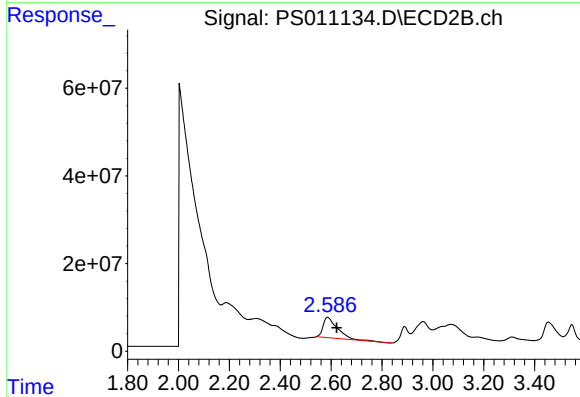


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 185263174
Conc: 245.59 ng/ml

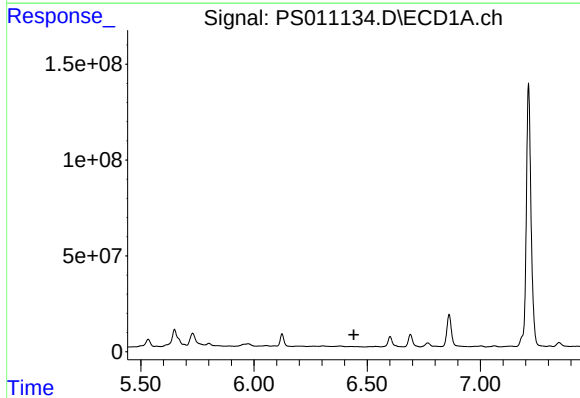


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

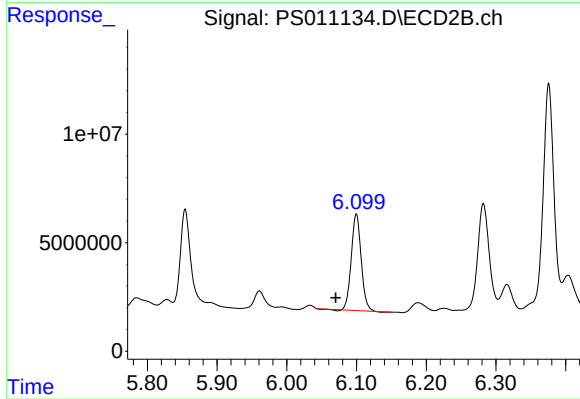

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 43497716
Conc: 52.23 ng/ml

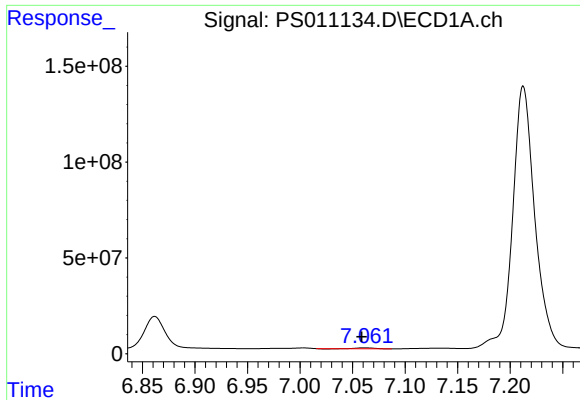

#3 4-Nitrophenol


R.T.: 7.062 min
Delta R.T.: 0.003 min
Response: 4635690
Conc: 11.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

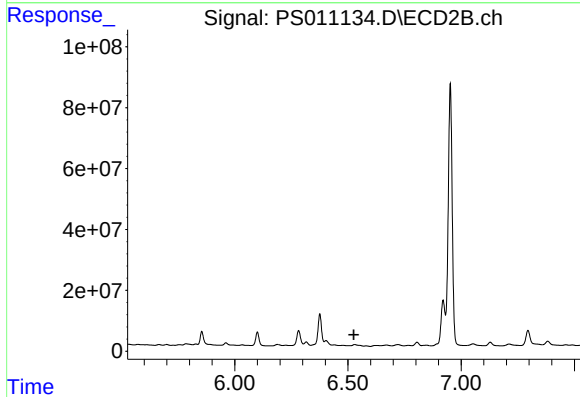


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

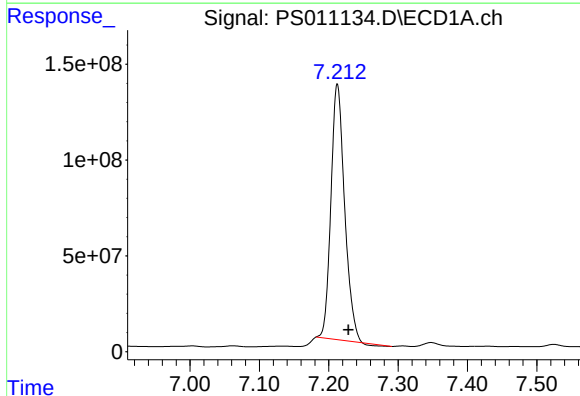


#4 2,4-DCAA

R.T.: 7.213 min
Delta R.T.: -0.016 min
Response: 1817440521
Conc: 2004.19 ng/ml

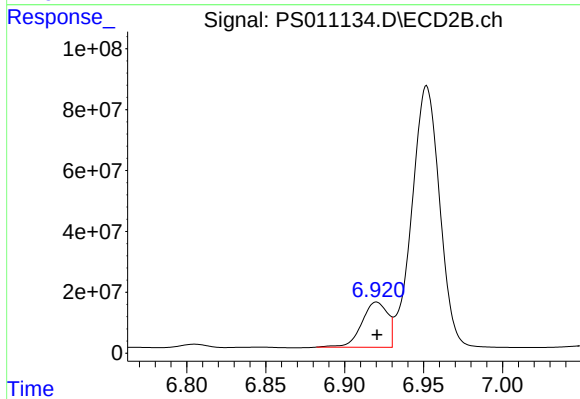

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 168042910
Conc: 303.28 ng/ml

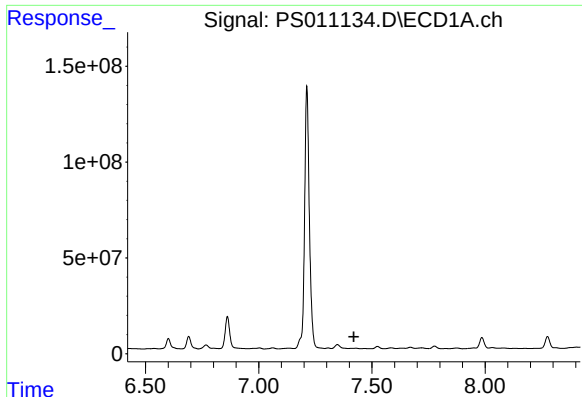

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

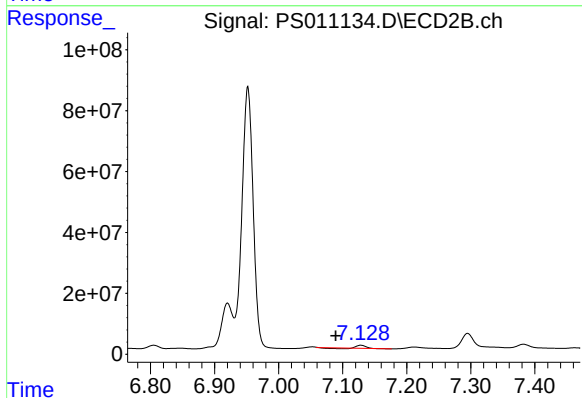


#5 DICAMBA

R.T.: 7.128 min
Delta R.T.: 0.039 min
Response: 7457835
Conc: 3.28 ng/ml

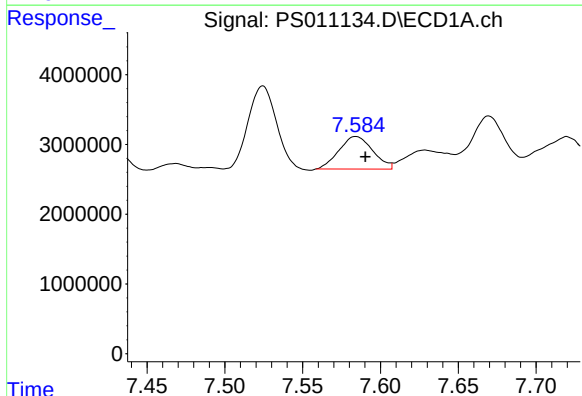


#6 MCP

R.T.: 7.584 min
Delta R.T.: -0.006 min
Response: 7085636
Conc: 2.48 ug/ml

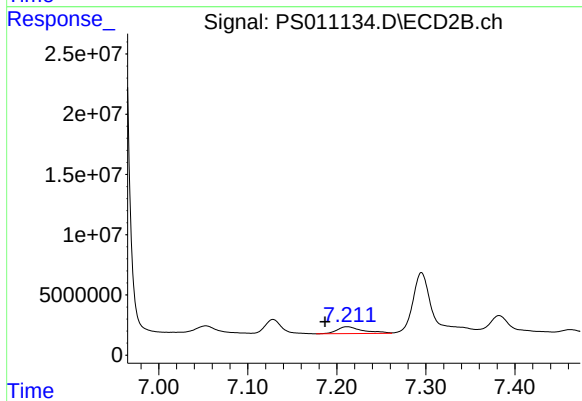

#6 MCP


R.T.: 7.212 min
Delta R.T.: 0.025 min
Response: 11349691
Conc: 6.00 ug/ml

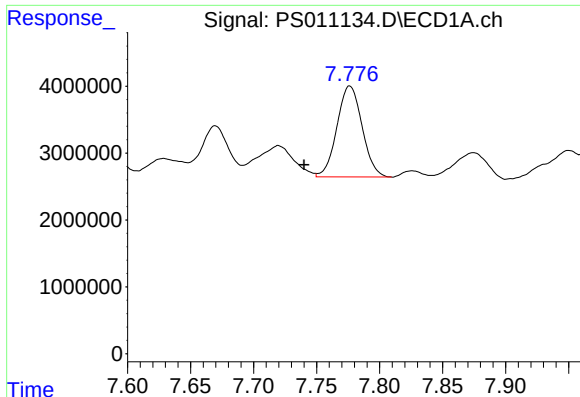

#7 MCPA


R.T.: 7.776 min
Delta R.T.: 0.036 min
Response: 18854520
Conc: 4.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

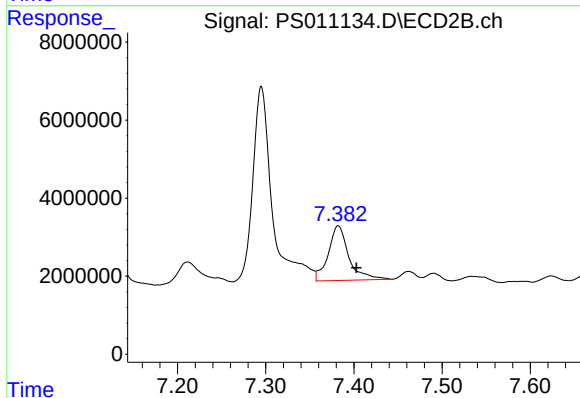


#7 MCPA

R.T.: 7.382 min
Delta R.T.: -0.021 min
Response: 22687241
Conc: 8.22 ug/ml

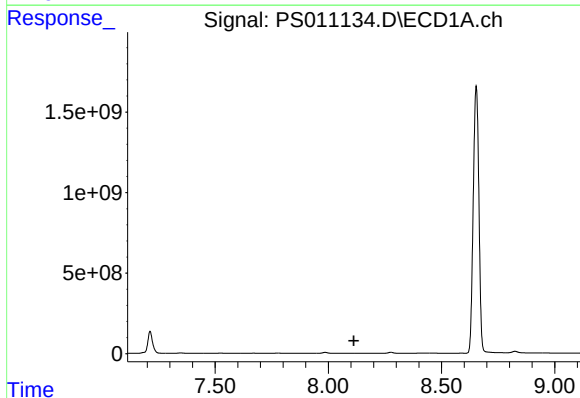


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

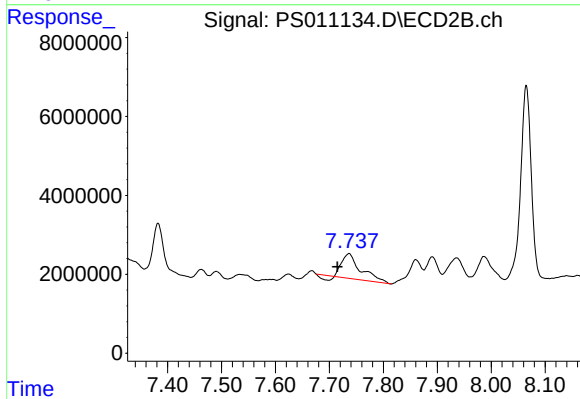

#8 DICHLORPROP


R.T.: 7.736 min
Delta R.T.: 0.021 min
Response: 13960510
Conc: 23.78 ng/ml

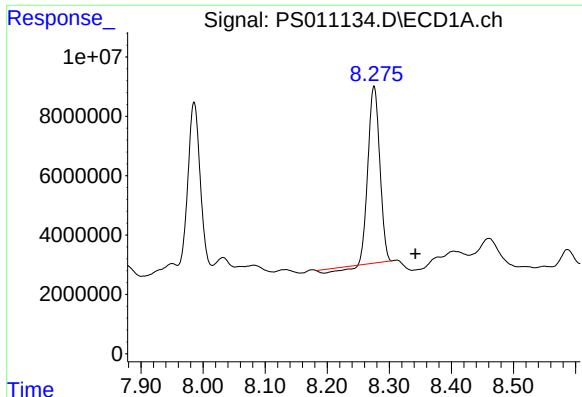

#9 2,4-D


R.T.: 8.275 min
Delta R.T.: -0.066 min
Response: 76350461
Conc: 86.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

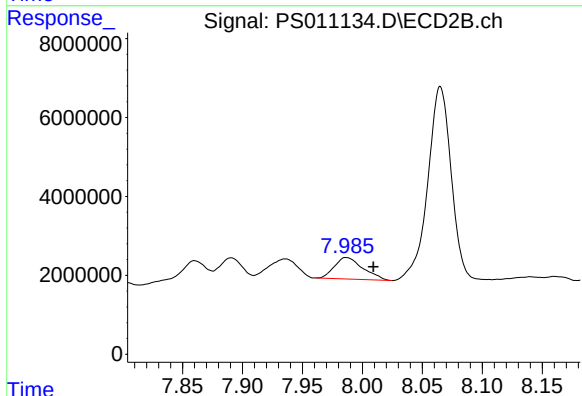


#9 2,4-D

R.T.: 7.987 min
Delta R.T.: -0.022 min
Response: 8987956
Conc: 12.44 ng/ml

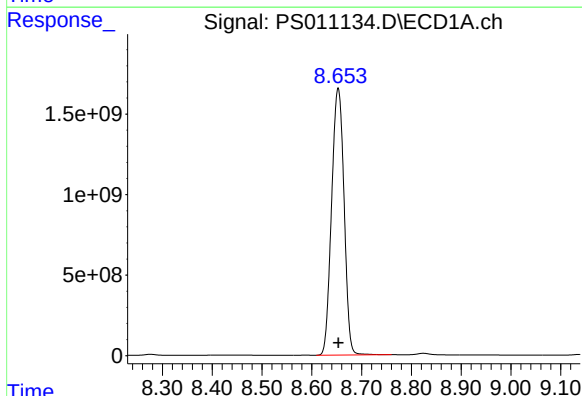


#10 Pentachlorophenol

R.T.: 8.653 min
Delta R.T.: 0.000 min
Response: 28777154129
Conc: 2314.36 ng/ml

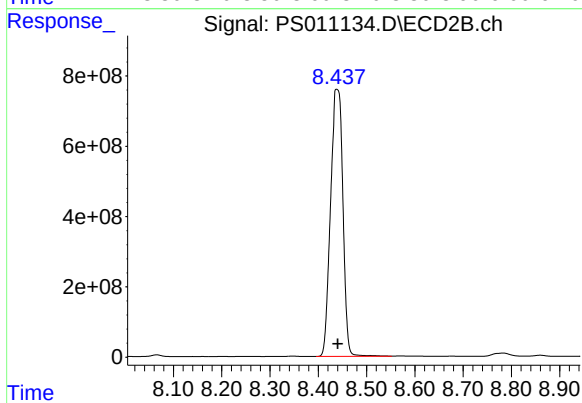

#10 Pentachlorophenol


R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 13486854583
Conc: 1939.53 ng/ml

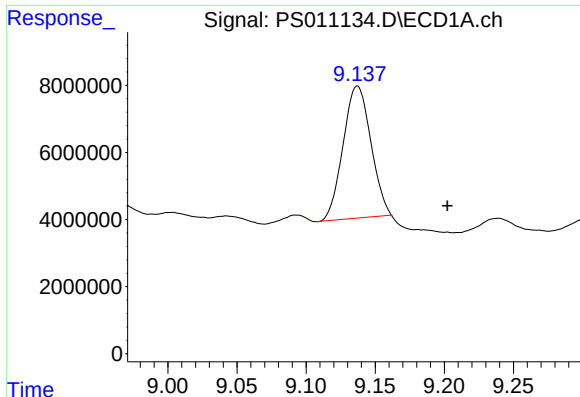

#11 2,4,5-TP (SILVEX)


R.T.: 9.137 min
Delta R.T.: -0.065 min
Response: 52629418
Conc: 10.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

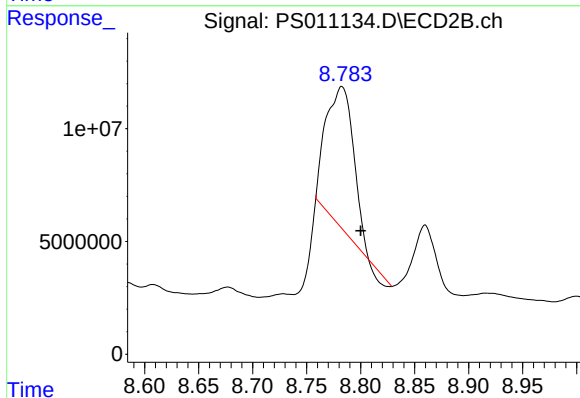


#11 2,4,5-TP (SILVEX)

R.T.: 8.782 min
Delta R.T.: -0.018 min
Response: 106538031
Conc: 35.41 ng/ml

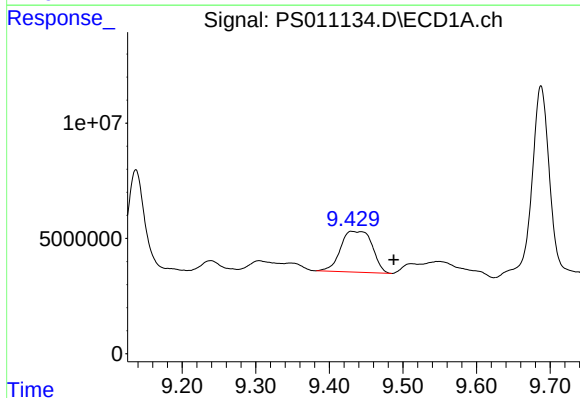


#12 2,4,5-T

R.T.: 9.432 min
Delta R.T.: -0.056 min
Response: 52778188
Conc: 11.33 ng/ml

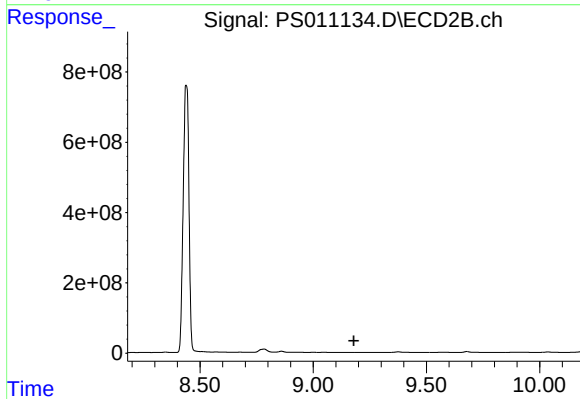

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

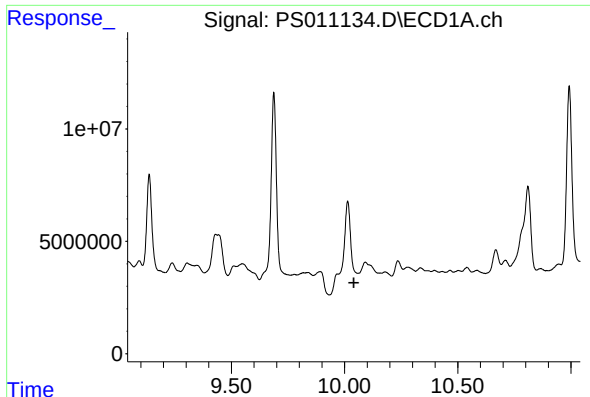

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

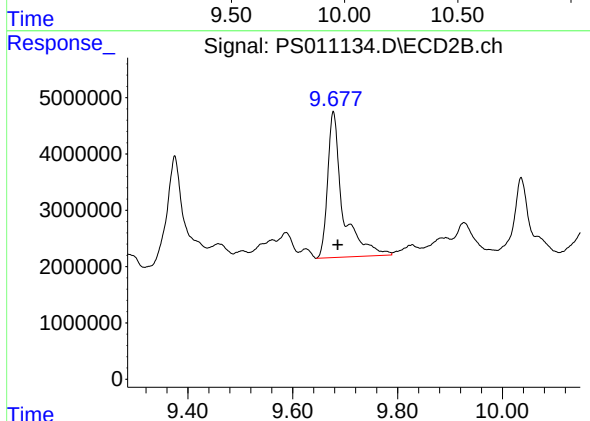


#13 2,4-DB

R.T.: 9.678 min
Delta R.T.: -0.009 min
Response: 52063786
Conc: 126.68 ng/ml

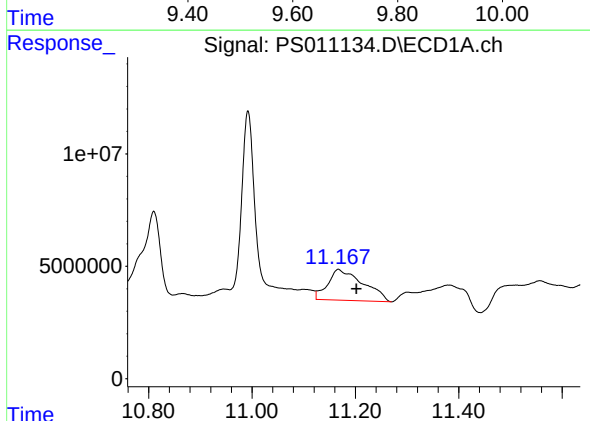


#14 DINOSEB

R.T.: 11.167 min
Delta R.T.: -0.035 min
Response: 65328278
Conc: 18.24 ng/ml

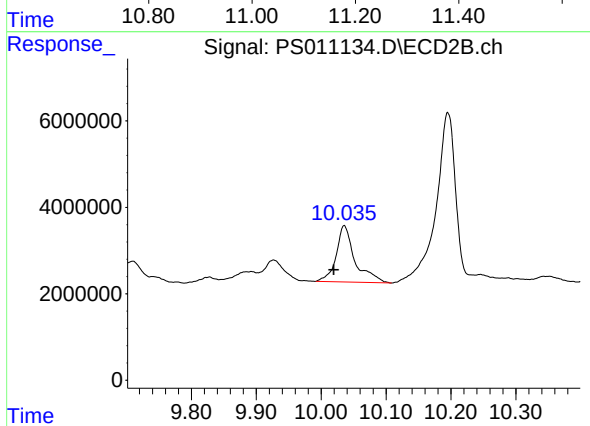

#14 DINOSEB


R.T.: 10.036 min
Delta R.T.: 0.016 min
Response: 26105977
Conc: 12.54 ng/ml

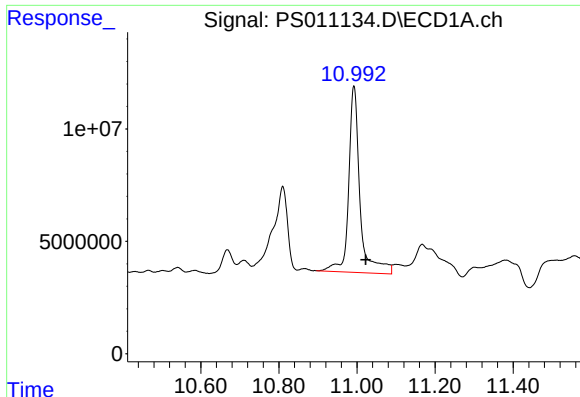

#15 Picloram


R.T.: 10.992 min
Delta R.T.: -0.030 min
Response: 166372015
Conc: 29.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

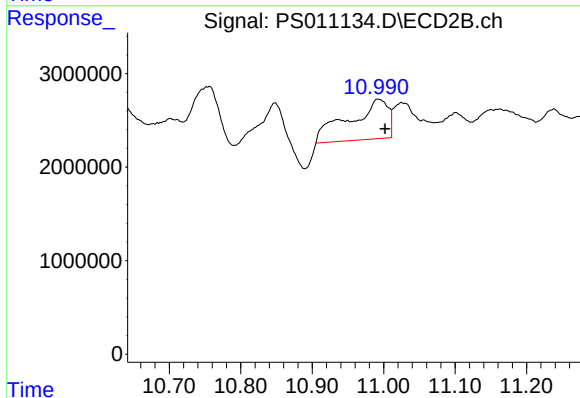


#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.009 min
Response: 16072185
Conc: 3.84 ng/ml

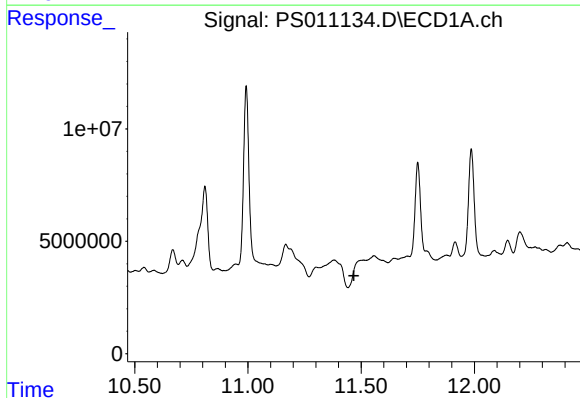

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.468 min
Response: 0
Conc: N.D.

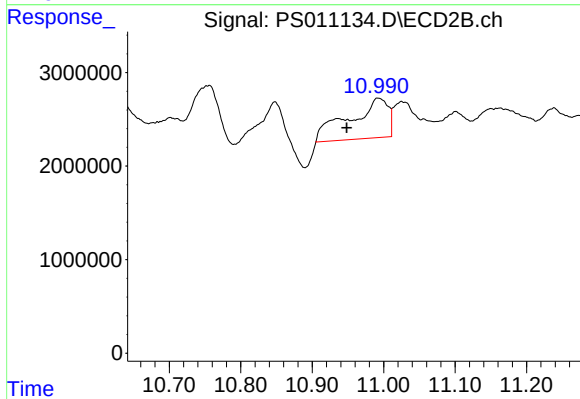

#16 DCPA

R.T.: 10.993 min
Delta R.T.: 0.044 min
Response: 16072185
Conc: 4.32 ng/ml