

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 20:02
 Operator : DD\AJ
 Sample : PB130072BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:50:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.919	459.3E6	308.7E6	506.462	557.167
Target Compounds							
1) T	Dalapon	2.999	2.587	50228179	199.4E6	44.858	264.324 #
2) T	3,5-DICHL...	0.000	6.100	0	75569842	N.D.	90.739
3) T	4-Nitroph...	7.003	0.000	7067957	0	17.706	N.D. #
5) T	DICAMBA	7.473	0.000	23007760	0	6.310	N.D. #
6) T	MCP	7.584	0.000	6604450	0	2.316	N.D. #
7) T	MCPA	7.777	7.383	22237786	20563660	5.584	7.451 #
10) T	Pentachlo...	8.709	0.000	13578571	0	1.092	N.D. #
12) T	2,4,5-T	9.509	0.000	7823989	0	1.680	N.D. #
14) T	DINOSEB	0.000	10.037	0	15123919	N.D.	7.264
16) T	DCPA	11.537	0.000	14683241	0	2.402	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 20:02
Operator : DD\AJ
Sample : PB130072BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:50:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

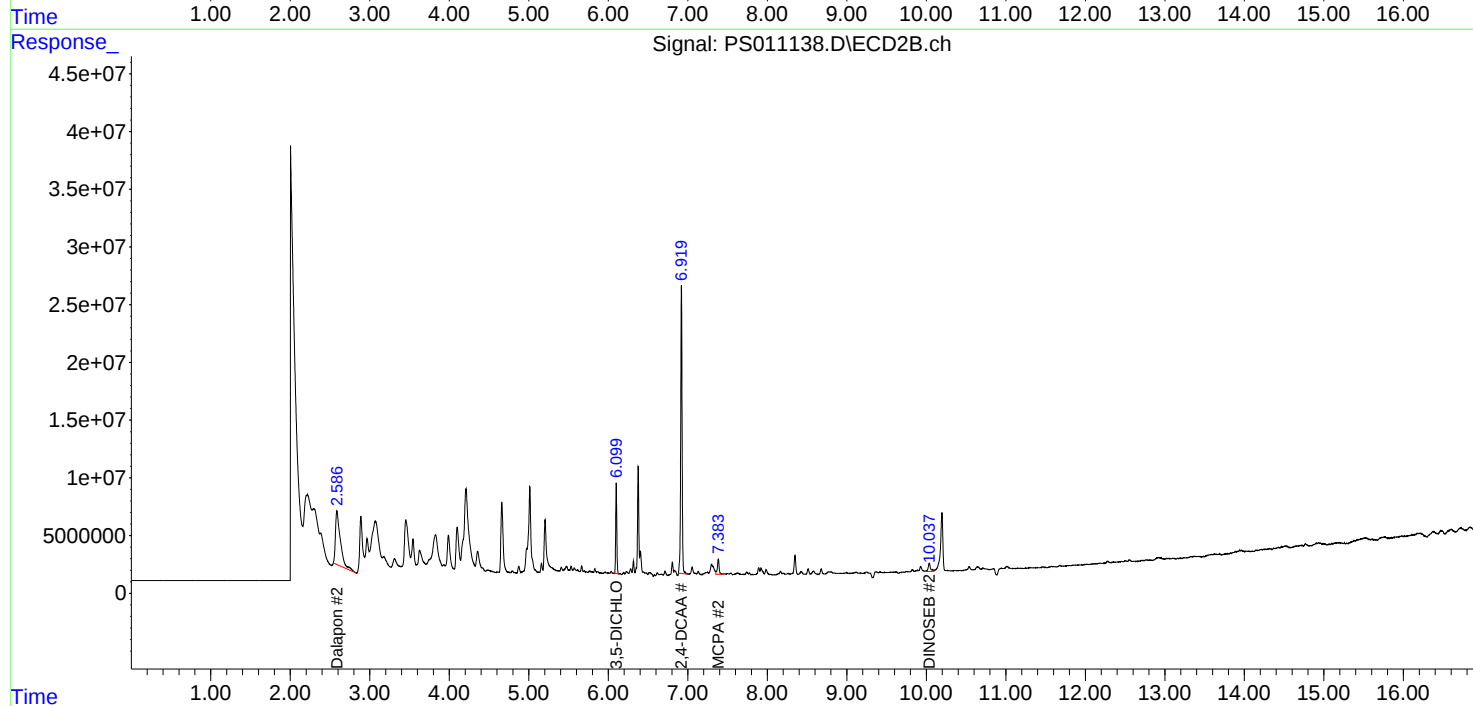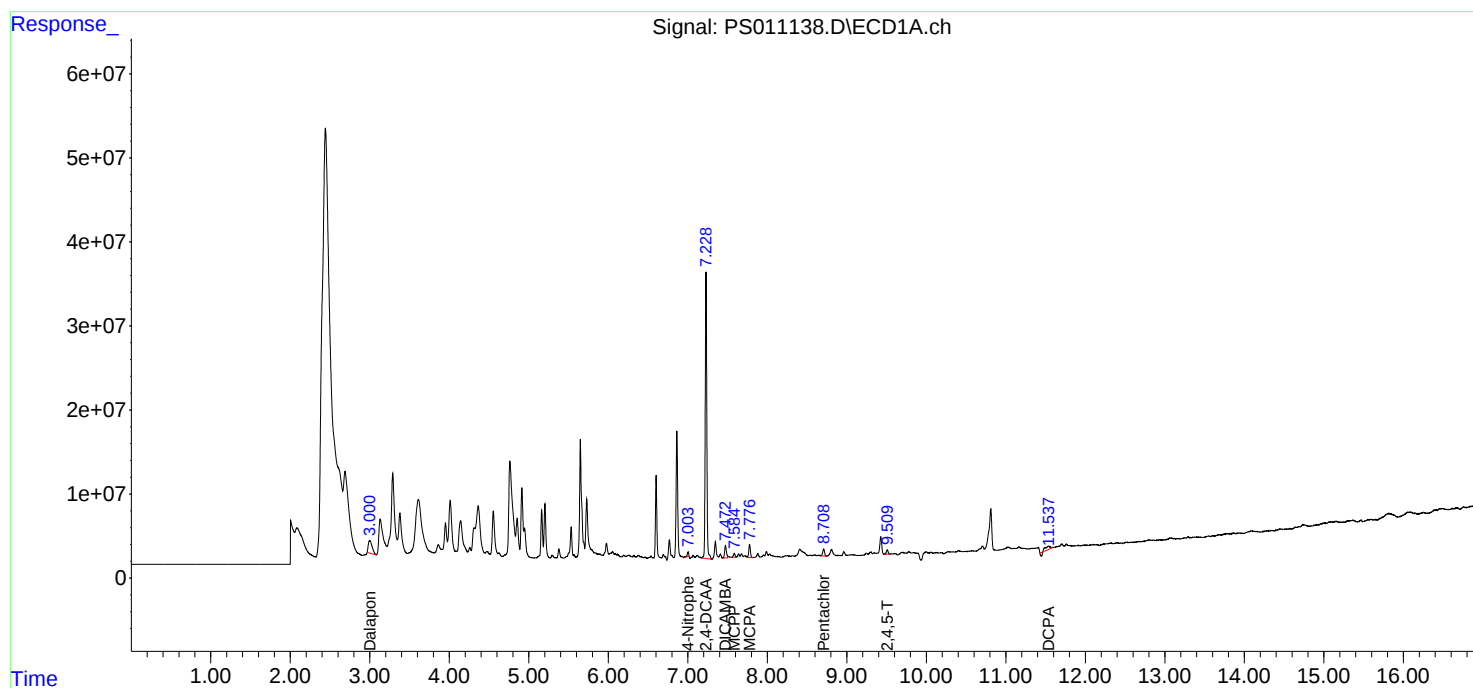


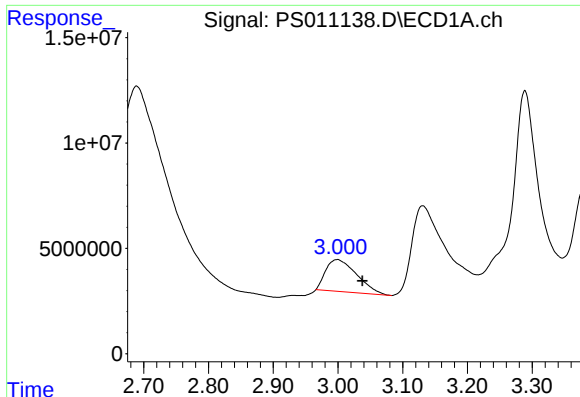

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: -0.039 min
Response: 50228179
Conc: 44.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

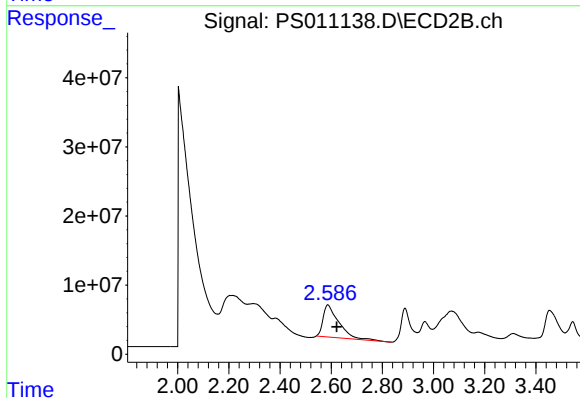


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.035 min
Response: 199395624
Conc: 264.32 ng/ml

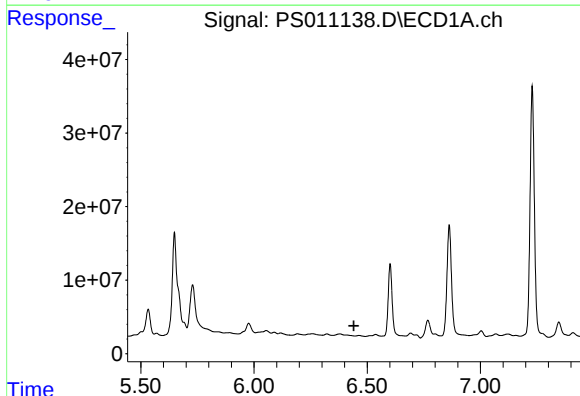


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

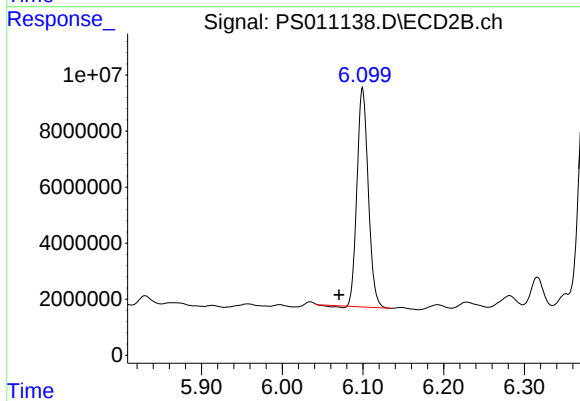

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 75569842
Conc: 90.74 ng/ml

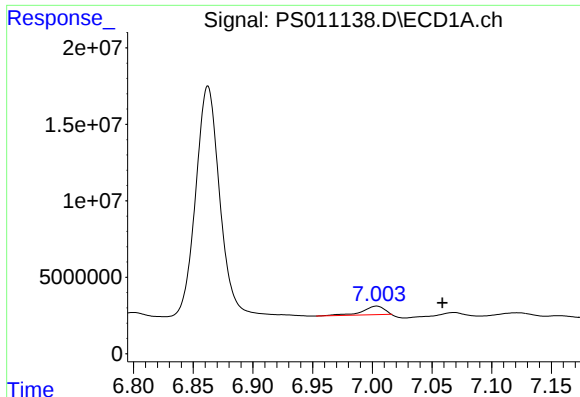

#3 4-Nitrophenol


R.T.: 7.003 min
Delta R.T.: -0.055 min
Response: 7067957
Conc: 17.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

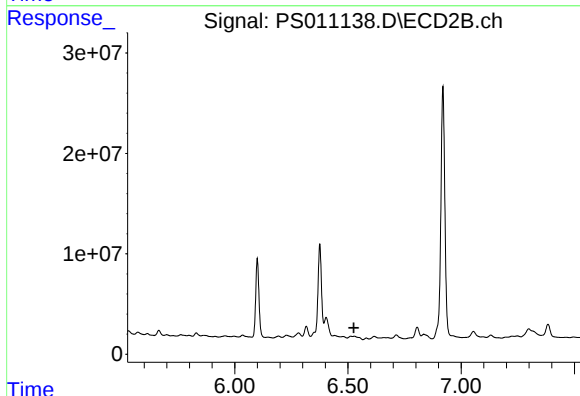


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

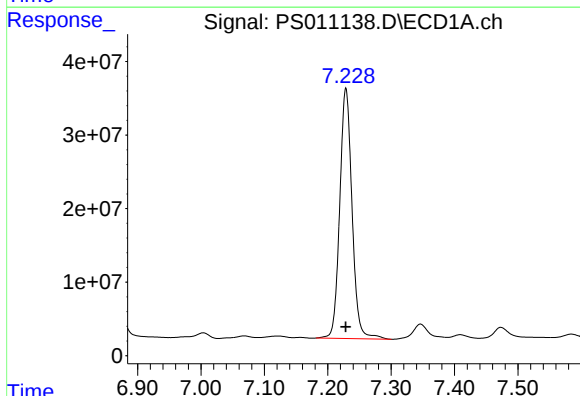


#4 2,4-DCAA

R.T.: 7.229 min
Delta R.T.: 0.000 min
Response: 459269333
Conc: 506.46 ng/ml

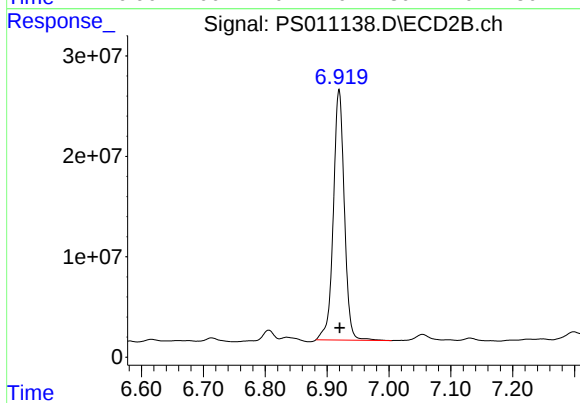

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 308712774
Conc: 557.17 ng/ml

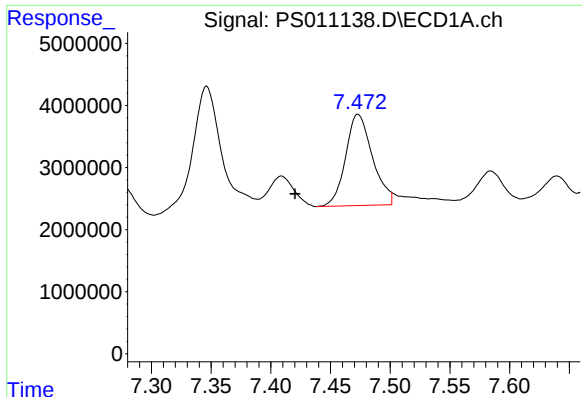

#5 DICAMBA


R.T.: 7.473 min
Delta R.T.: 0.053 min
Response: 23007760
Conc: 6.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

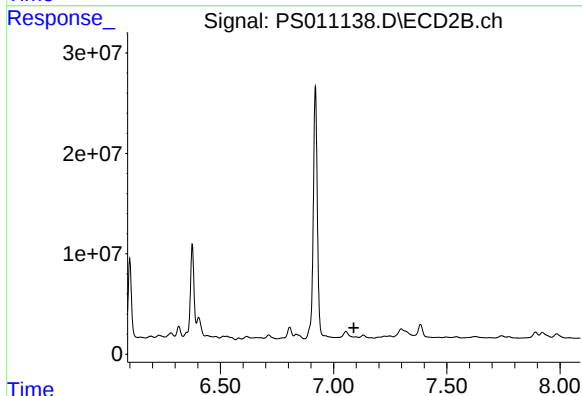


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

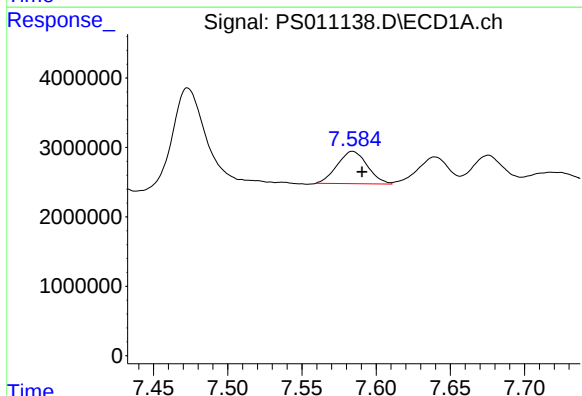


#6 MCPP

R.T.: 7.584 min
Delta R.T.: -0.006 min
Response: 6604450
Conc: 2.32 ug/ml

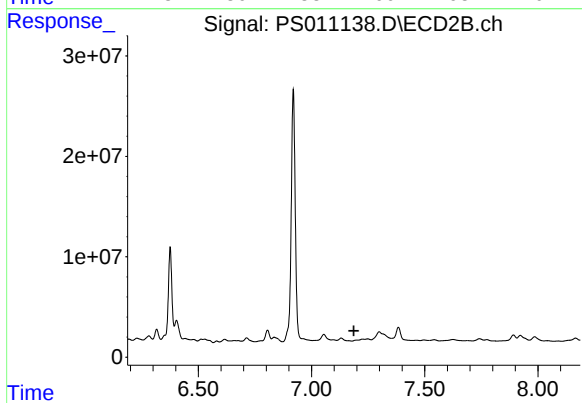

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

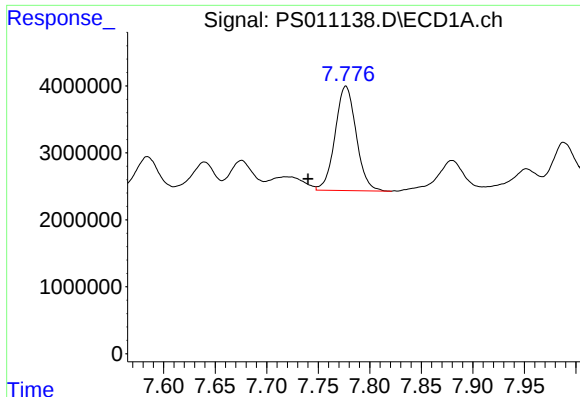

#7 MCPA


R.T.: 7.777 min
Delta R.T.: 0.037 min
Response: 22237786
Conc: 5.58 ug/ml

Instrument :
ECD_S
ClientSampleId :

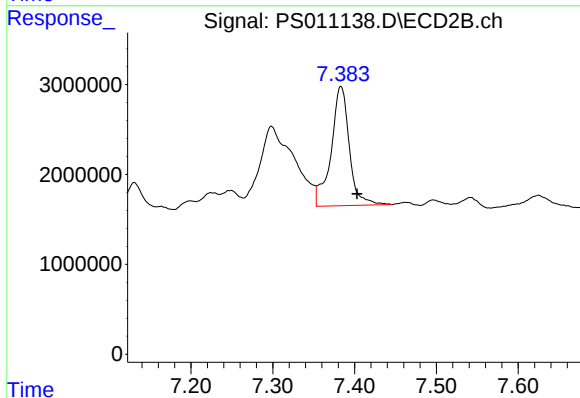


#7 MCPA

R.T.: 7.383 min
Delta R.T.: -0.019 min
Response: 20563660
Conc: 7.45 ug/ml

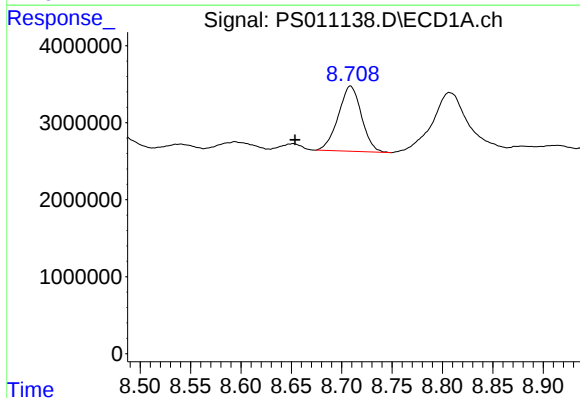


#10 Pentachlorophenol

R.T.: 8.709 min
Delta R.T.: 0.055 min
Response: 13578571
Conc: 1.09 ng/ml

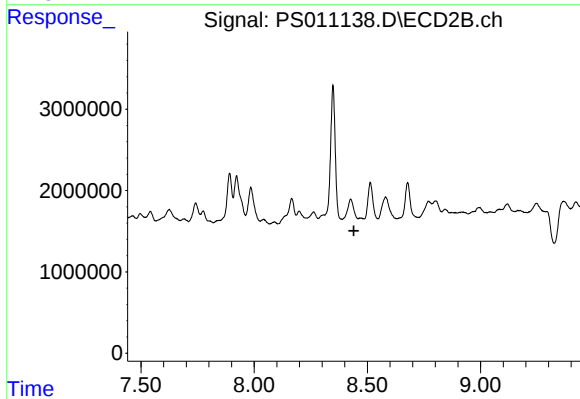

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

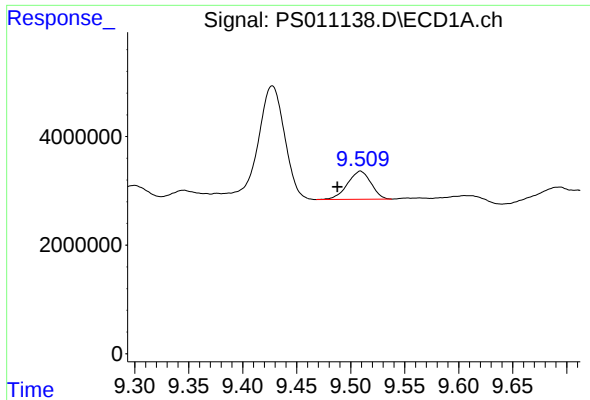

#12 2,4,5-T


R.T.: 9.509 min
Delta R.T.: 0.021 min
Response: 7823989
Conc: 1.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

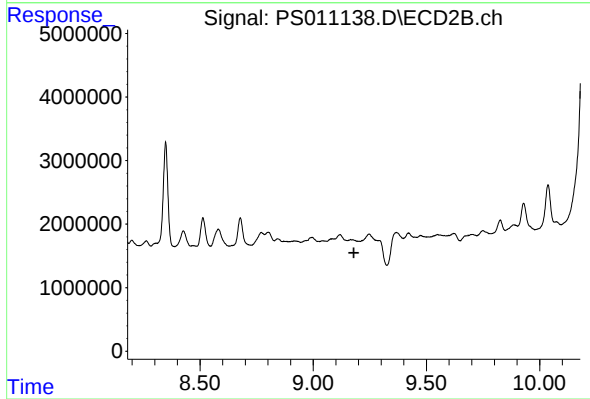


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

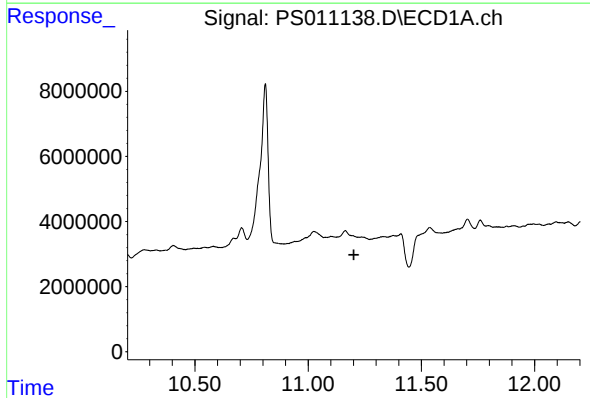


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.202 min
Response: 0
Conc: N.D.

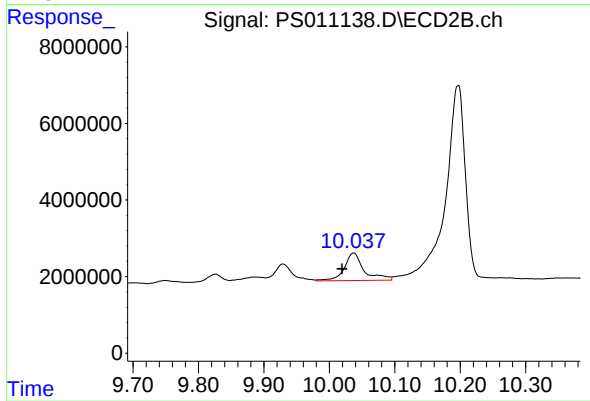

#14 DINOSEB


R.T.: 10.037 min
Delta R.T.: 0.017 min
Response: 15123919
Conc: 7.26 ng/ml

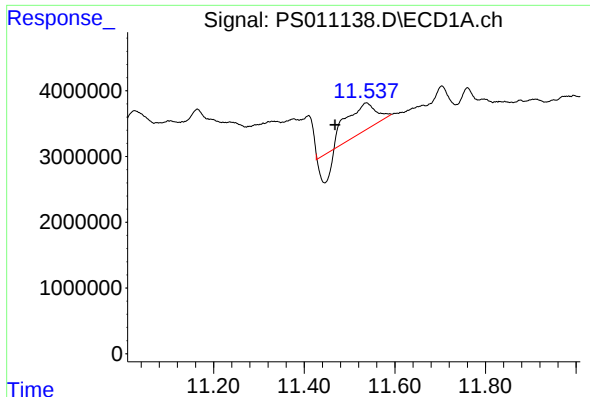

#16 DCPA

R.T.: 11.537 min
Delta R.T.: 0.069 min
Response: 14683241
Conc: 2.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

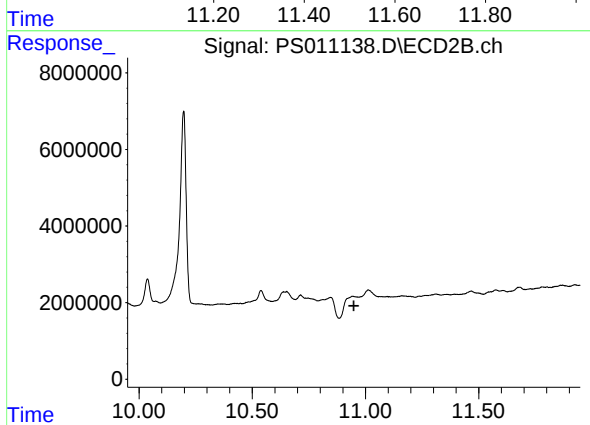

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.949 min
Response: 0
Conc: N.D.