

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011142.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 21:34
 Operator : DD\AJ
 Sample : PB130072TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:52:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.919	263.1E6	199.0E6	290.186	359.209
Target Compounds							
1) T	Dalapon	2.996	2.586	47710800	178.0E6	42.609	236.022 #
2) T	3,5-DICHL...	0.000	6.100	0	78826580	N.D.	94.650
3) T	4-Nitroph...	6.996	0.000	6895657	0	17.275	N.D. #
5) T	DICAMBA	7.407	0.000	7252745	0	1.989	N.D. #
6) T	MCPD	7.639	0.000	5690405	0	1.996	N.D. #
7) T	MCPA	7.690	7.460	160.6E6	129.4E6	40.315	46.867
8) T	DICHLORPROP	0.000	7.739	0	18397427	N.D.	31.334
10) T	Pentachlo...	8.707	0.000	10672769	0	<MDL	N.D. #
12) T	2,4,5-T	9.425	0.000	25939637	0	5.569	N.D. #
15) T	Picloram	11.030	11.009	21490553	14146466	3.833	3.377
16) T	DCPA	0.000	11.009	0	14146466	N.D.	3.798



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011142.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 21:34
Operator : DD\AJ
Sample : PB130072TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:52:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

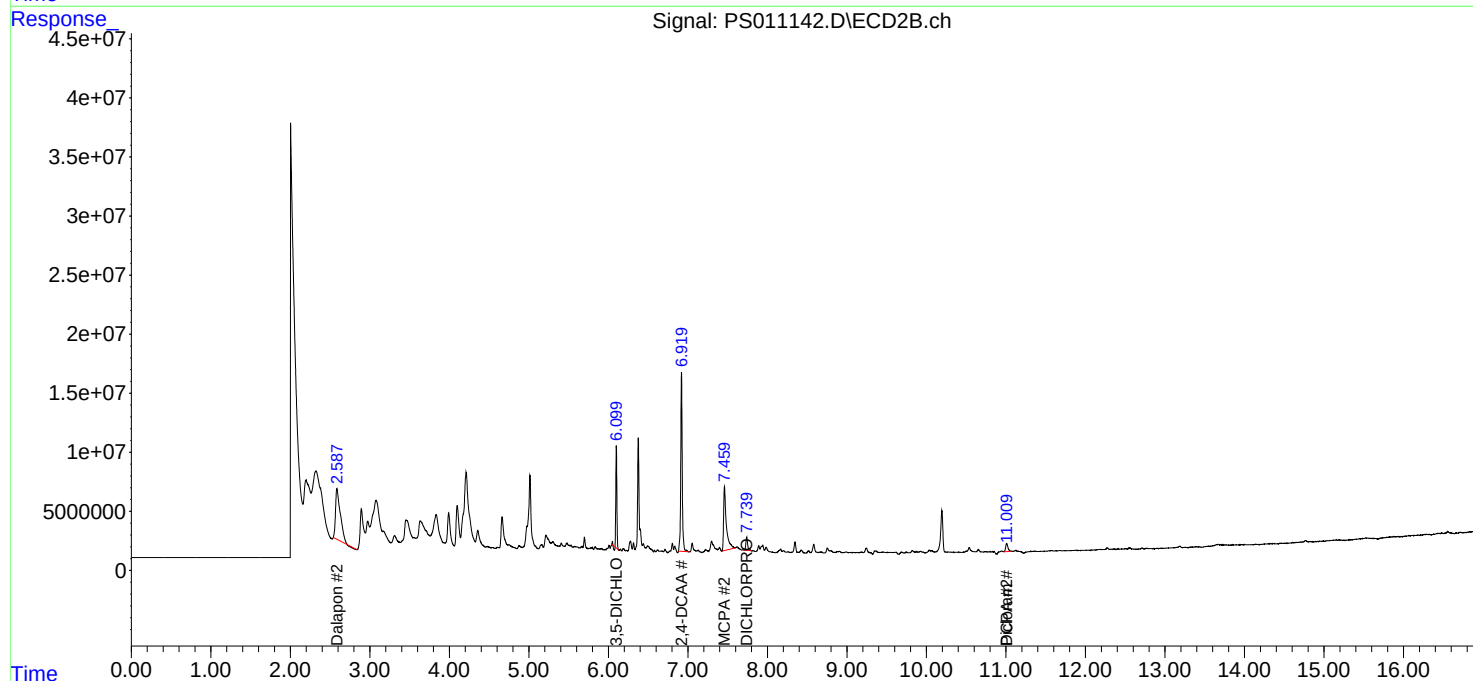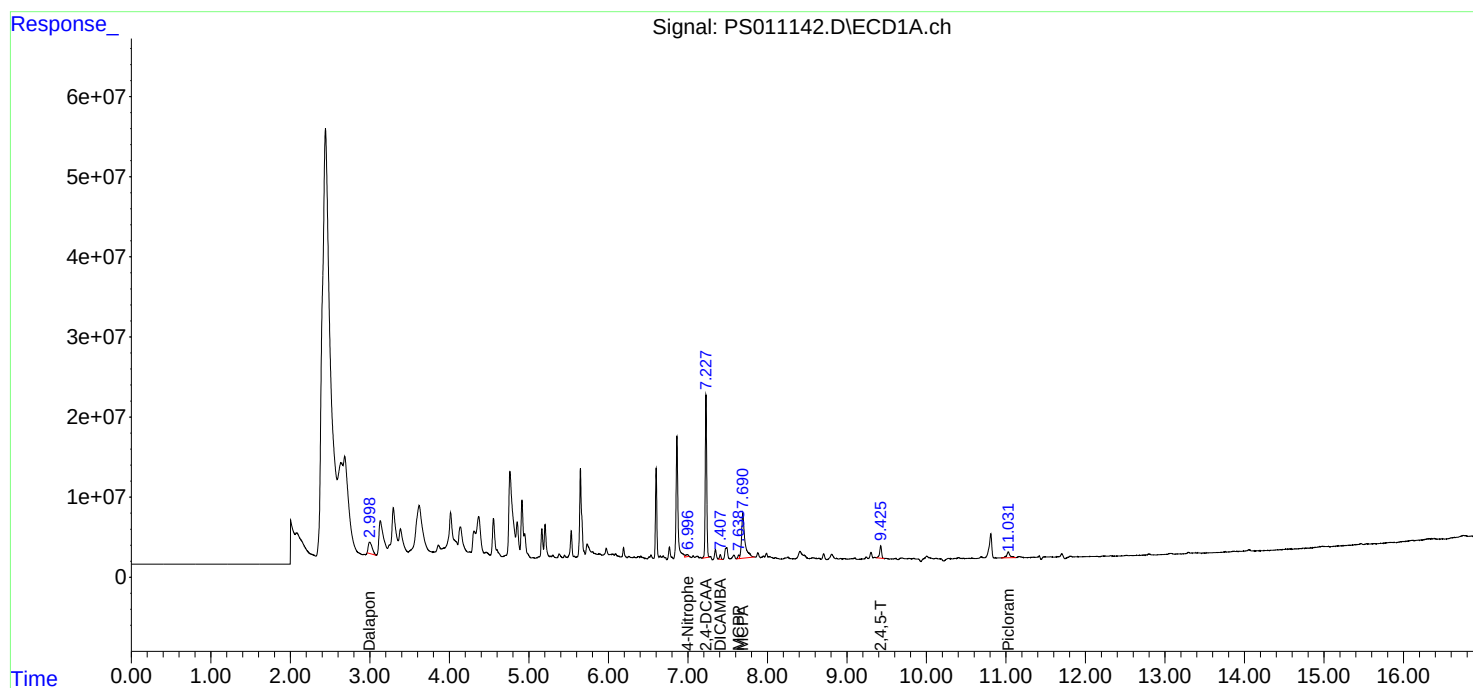


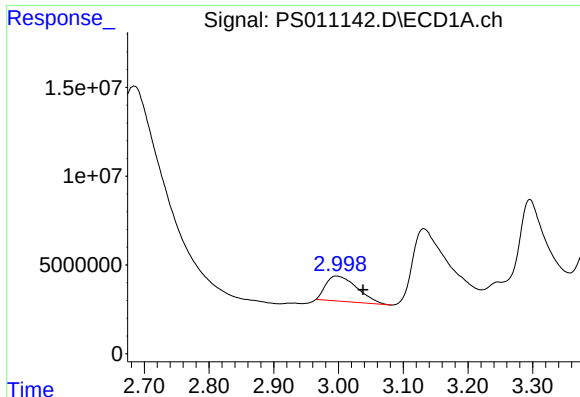

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 47710800
Conc: 42.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

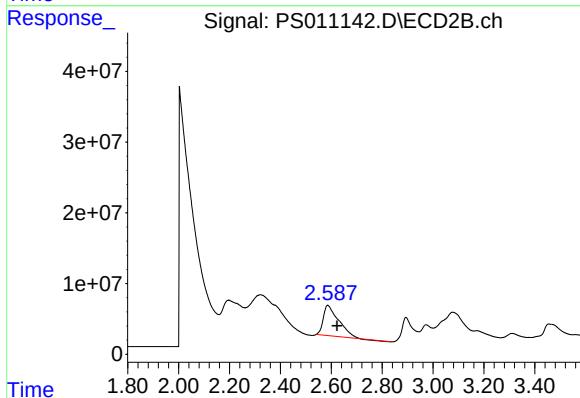


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 178045489
Conc: 236.02 ng/ml

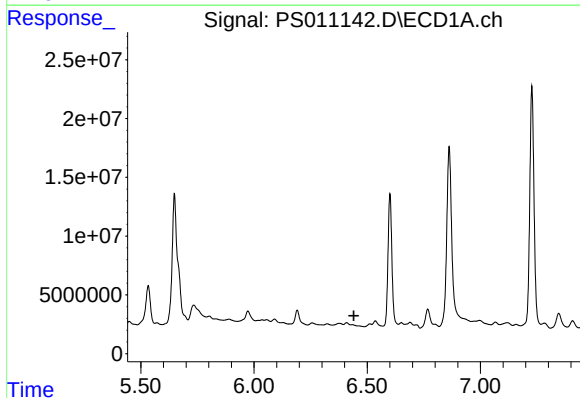


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

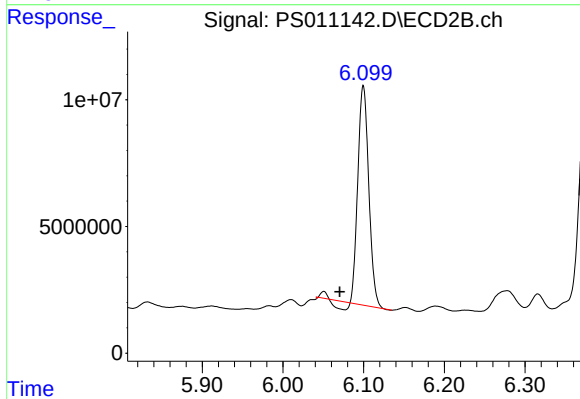

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 78826580
Conc: 94.65 ng/ml

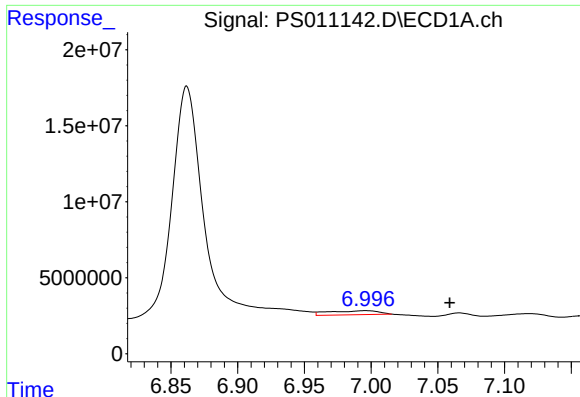

#3 4-Nitrophenol


R.T.: 6.996 min
Delta R.T.: -0.063 min
Response: 6895657
Conc: 17.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

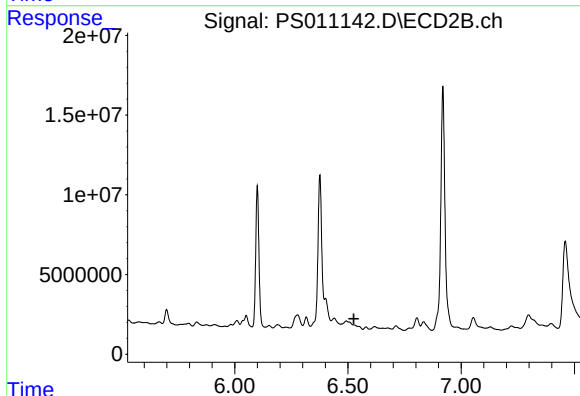


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.526 min
Response: 0
Conc: N.D.

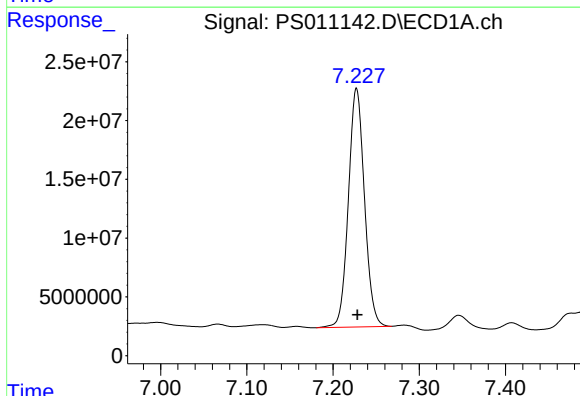


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: -0.001 min
Response: 263145674
Conc: 290.19 ng/ml

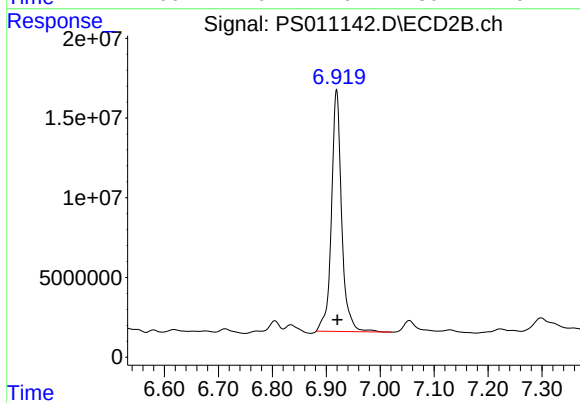

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 199029420
Conc: 359.21 ng/ml

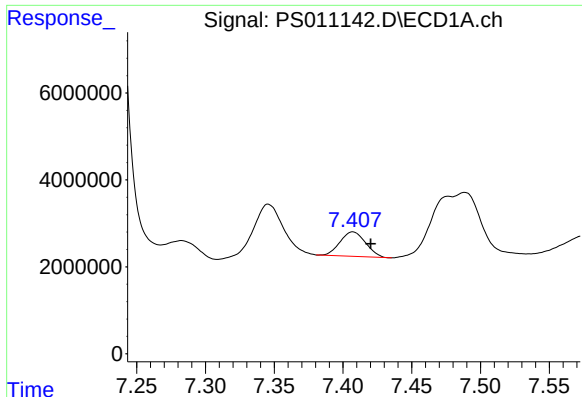

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: -0.013 min
Response: 7252745
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

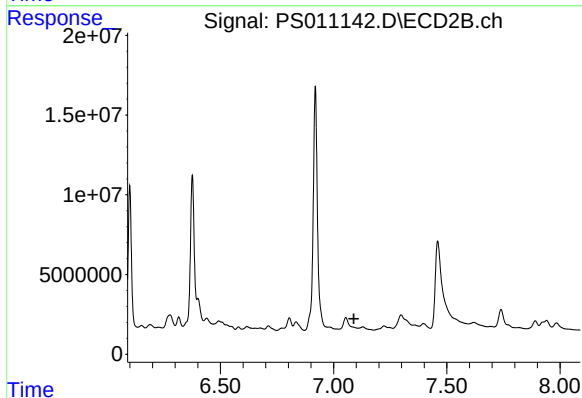


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.089 min
Response: 0
Conc: N.D.

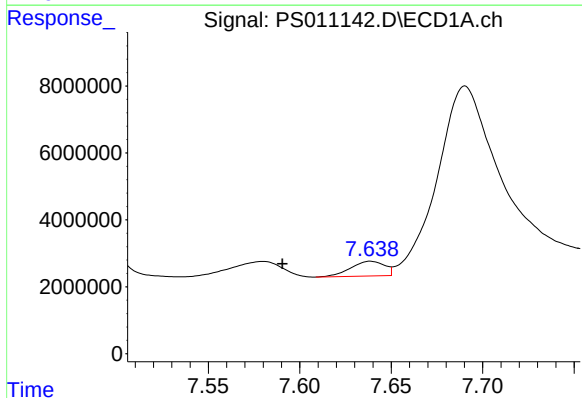


#6 MCP

R.T.: 7.639 min
Delta R.T.: 0.048 min
Response: 5690405
Conc: 2.00 ug/ml

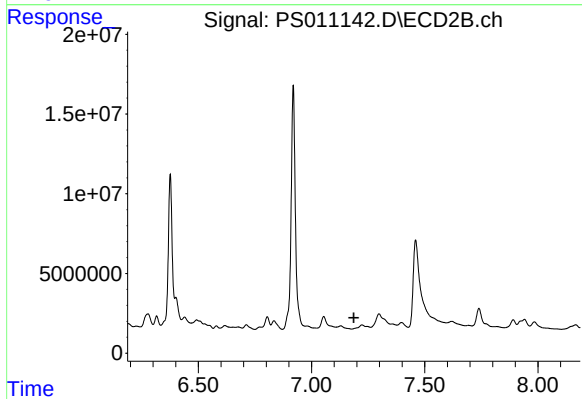

#6 MCP


R.T.: 0.000 min
Exp R.T. : 7.187 min
Response: 0
Conc: N.D.

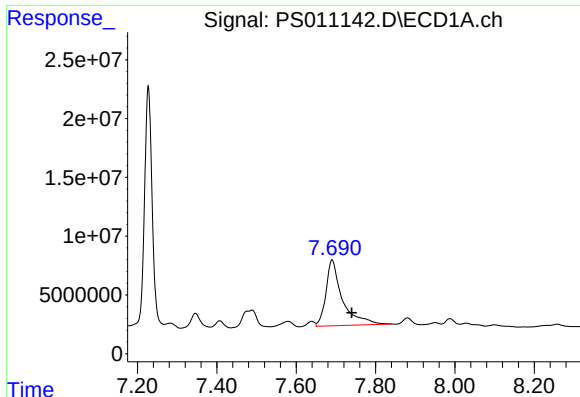

#7 MCPA


R.T.: 7.690 min
Delta R.T.: -0.050 min
Response: 160553562
Conc: 40.32 ug/ml

Instrument :
ECD_S
ClientSampleId :

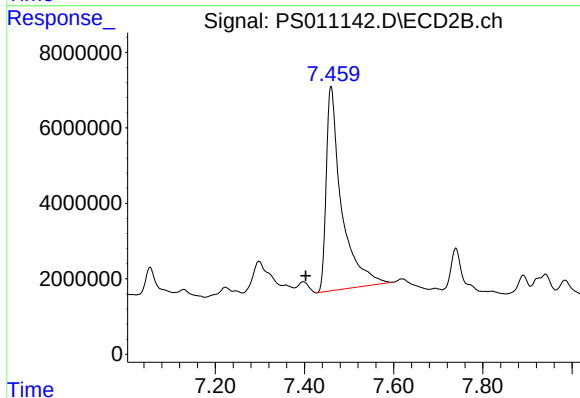


#7 MCPA

R.T.: 7.460 min
Delta R.T.: 0.057 min
Response: 129352144
Conc: 46.87 ug/ml

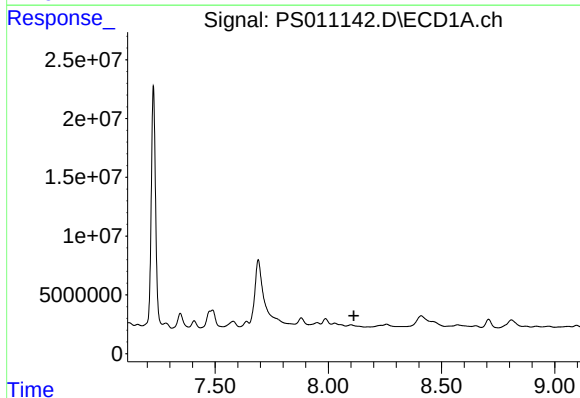


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

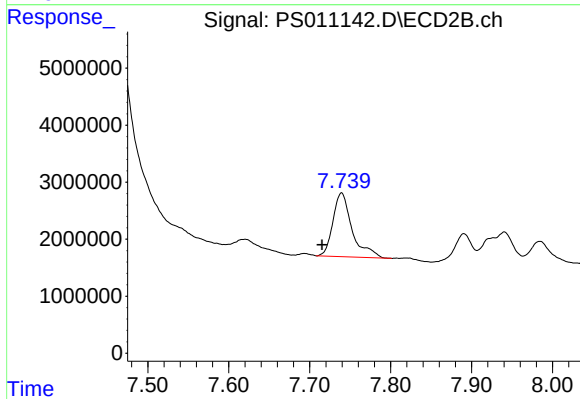

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.024 min
Response: 18397427
Conc: 31.33 ng/ml

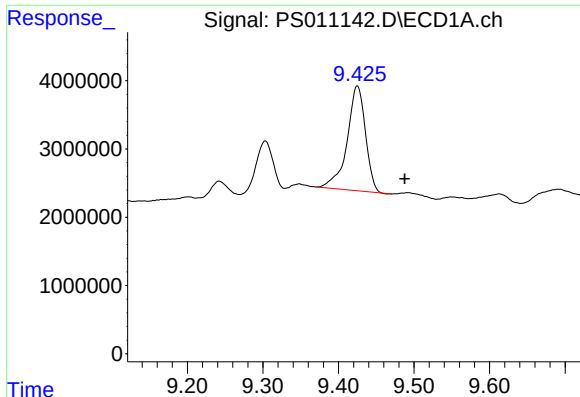

#12 2,4,5-T


R.T.: 9.425 min
Delta R.T.: -0.063 min
Response: 25939637
Conc: 5.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

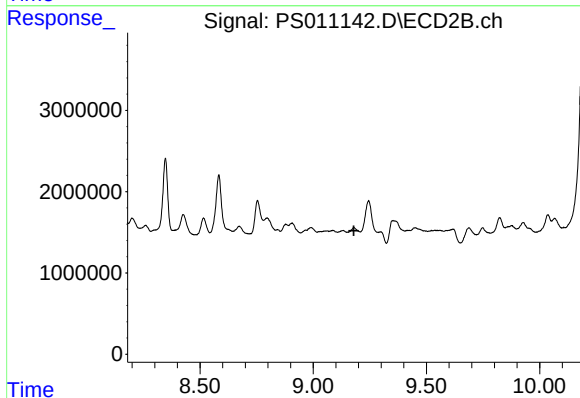


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

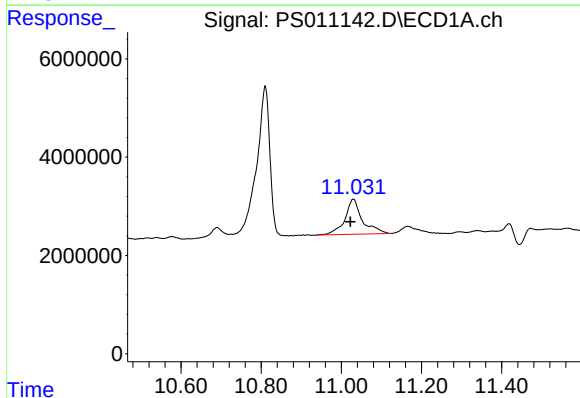


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.007 min
Response: 21490553
Conc: 3.83 ng/ml

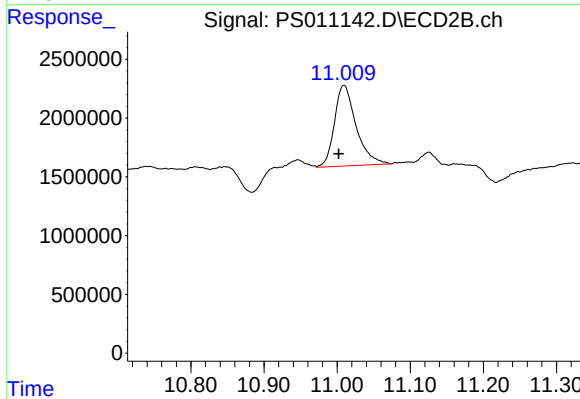

#15 Picloram


R.T.: 11.009 min
Delta R.T.: 0.007 min
Response: 14146466
Conc: 3.38 ng/ml

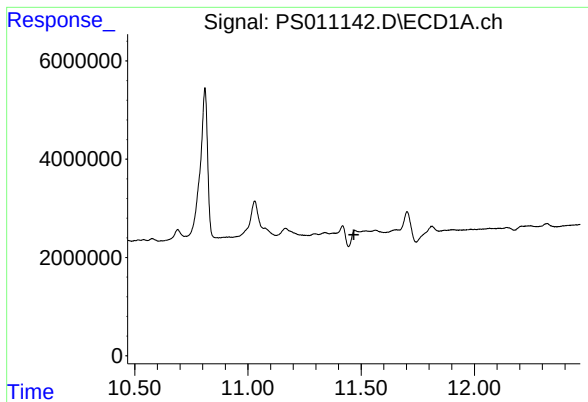

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

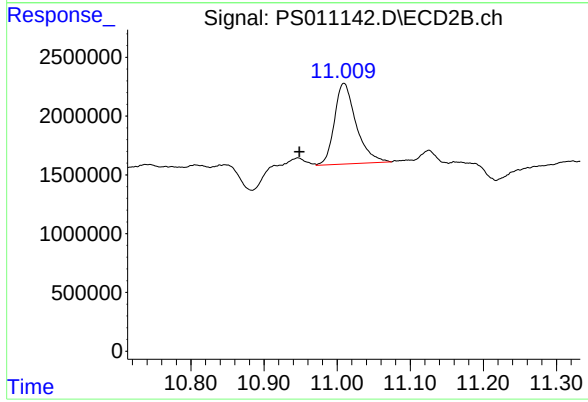

#16 DCPA

R.T.: 11.009 min
Delta R.T.: 0.061 min
Response: 14146466
Conc: 3.80 ng/ml