

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 21:57
 Operator : DD\AJ
 Sample : L3183-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:52:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.920	269.3E6	192.4E6	297.013	347.263
Target Compounds							
1) T	Dalapon	2.999	2.586	46243893	171.9E6	41.299	227.893 #
2) T	3,5-DICHL...	0.000	6.100	0	113.6E6	N.D.	136.399
3) T	4-Nitroph...	6.998	6.551	10788991	6371385	27.028	19.828 #
5) T	DICAMBA	7.408	7.054	8989274	6428242	2.465	2.830
6) T	MCP	7.640	0.000	8521881	0	2.989	N.D. #
7) T	MCPA	7.689	7.458	202.7E6	173.3E6	50.900	62.801
8) T	DICHLORPROP	8.060	7.739	9532635	21800003	10.870	37.129 #
10) T	Pentachlo...	8.708	0.000	13012926	0	1.047	N.D. #
11) T	2,4,5-TP ...	9.242	0.000	5830447	0	1.174	N.D. #
12) T	2,4,5-T	9.426	0.000	40366159	0	8.666	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 21:57
Operator : DD\AJ
Sample : L3183-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:52:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

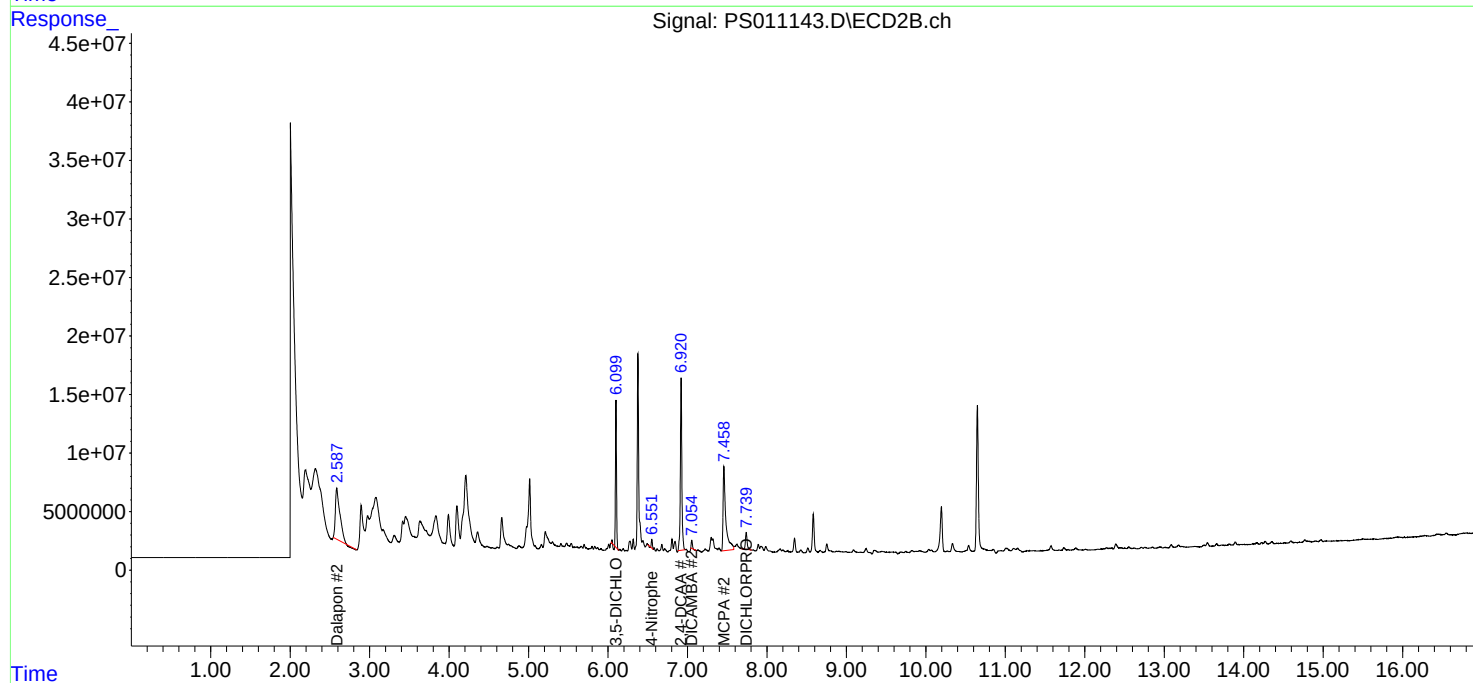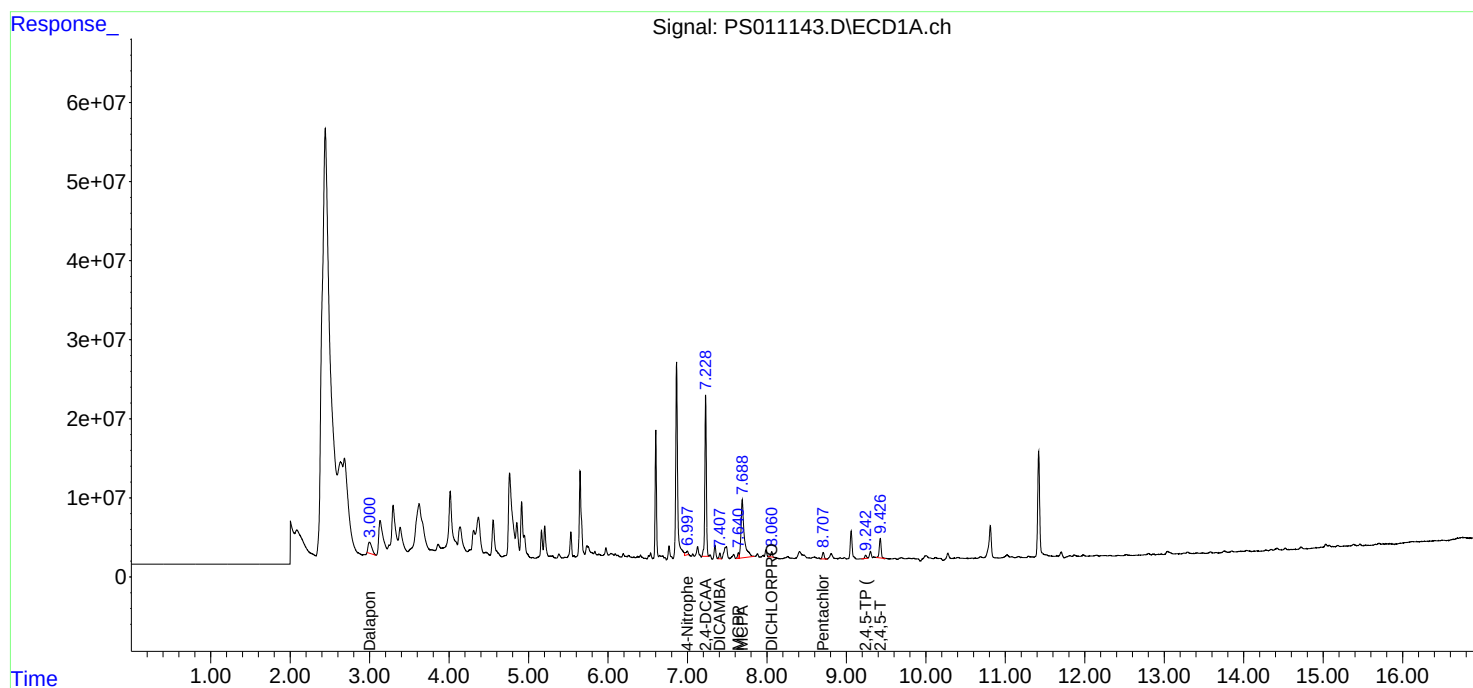


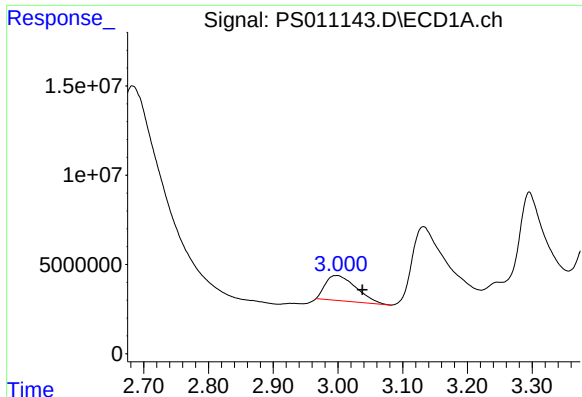

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: -0.039 min
Response: 46243893
Conc: 41.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

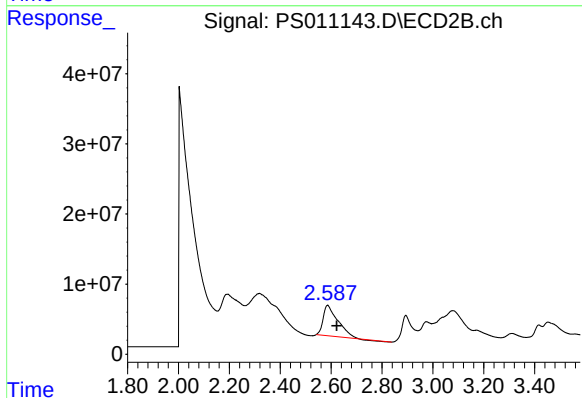


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 171913432
Conc: 227.89 ng/ml

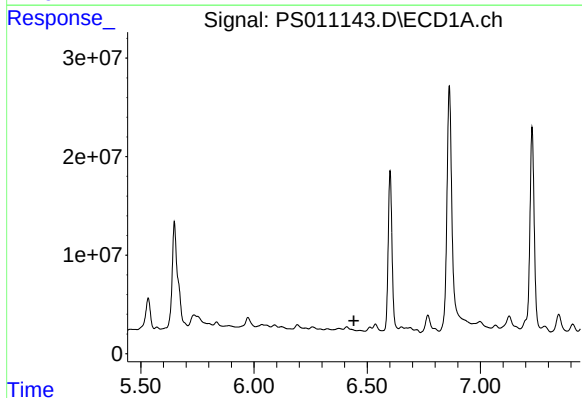


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

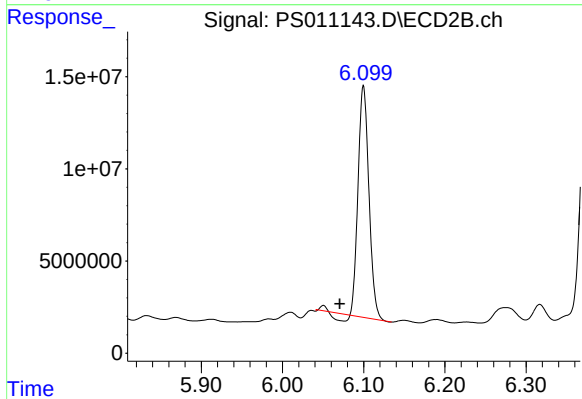

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 113596064
Conc: 136.40 ng/ml

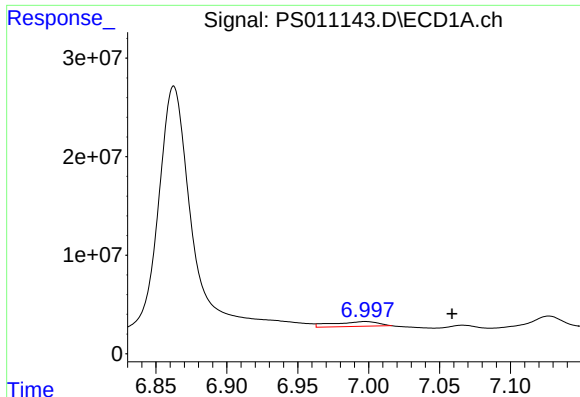

#3 4-Nitrophenol


R.T.: 6.998 min
Delta R.T.: -0.061 min
Response: 10788991
Conc: 27.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

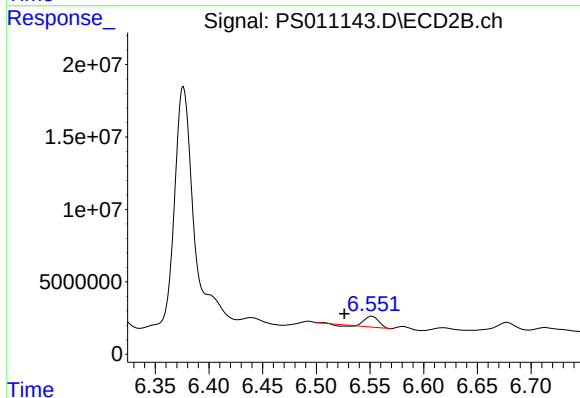


#3 4-Nitrophenol

R.T.: 6.551 min
Delta R.T.: 0.025 min
Response: 6371385
Conc: 19.83 ng/ml

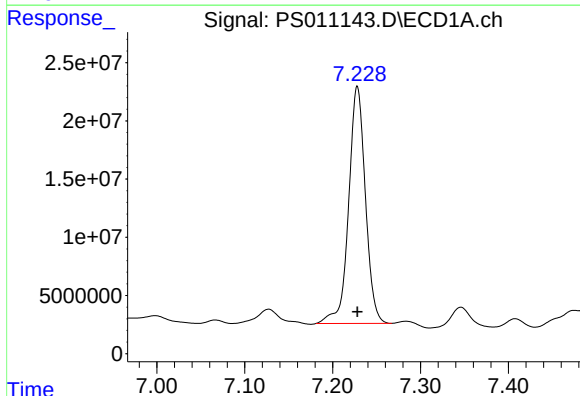


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 269336503
Conc: 297.01 ng/ml

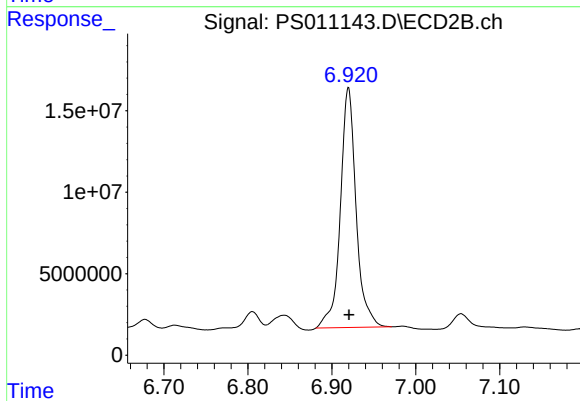

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 192410317
Conc: 347.26 ng/ml

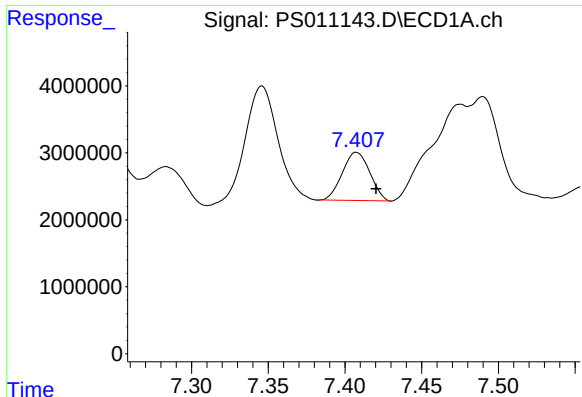

#5 DICAMBA


R.T.: 7.408 min
Delta R.T.: -0.013 min
Response: 8989274
Conc: 2.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

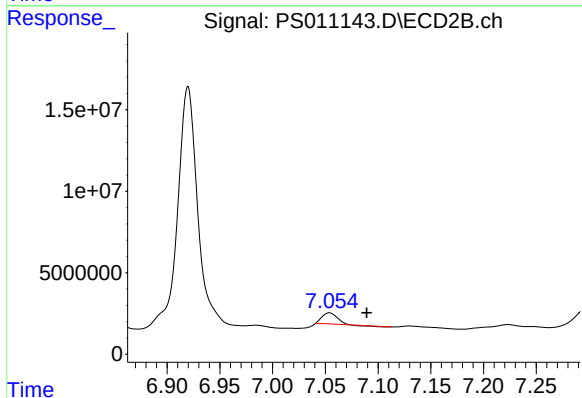


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.035 min
Response: 6428242
Conc: 2.83 ng/ml

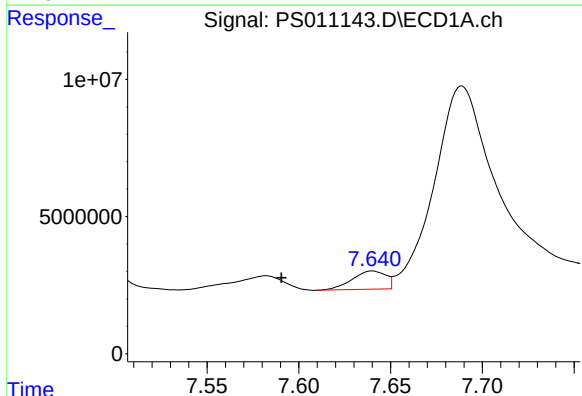


#6 MCP

R.T.: 7.640 min
Delta R.T.: 0.050 min
Response: 8521881
Conc: 2.99 ug/ml

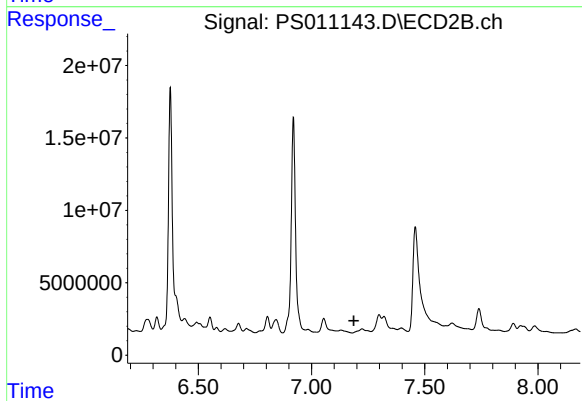

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

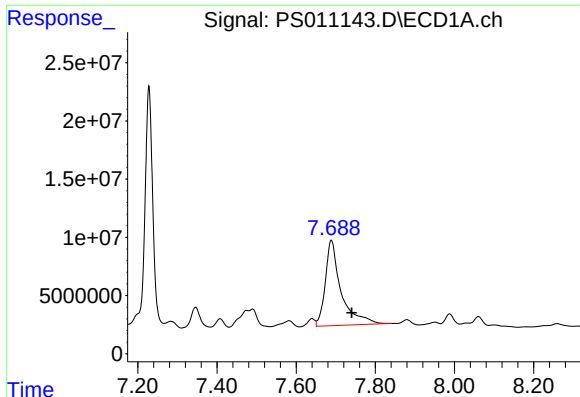

#7 MCPA


R.T.: 7.689 min
Delta R.T.: -0.051 min
Response: 202706361
Conc: 50.90 ug/ml

Instrument :
ECD_S
ClientSampleId :

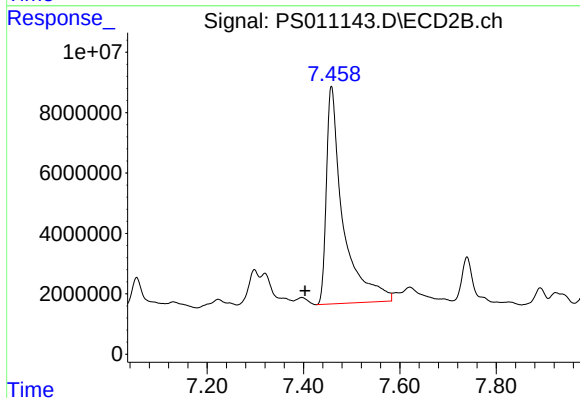


#7 MCPA

R.T.: 7.458 min
Delta R.T.: 0.055 min
Response: 173330343
Conc: 62.80 ug/ml

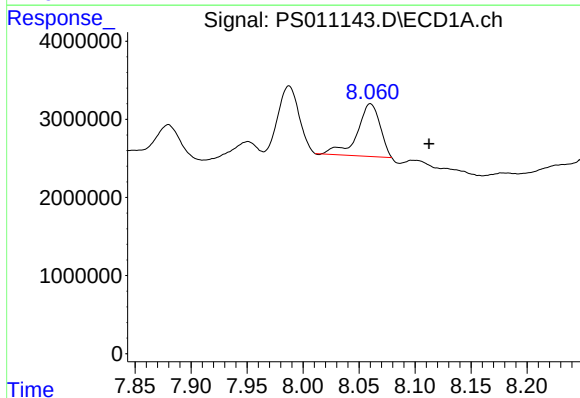


#8 DICHLORPROP

R.T.: 8.060 min
Delta R.T.: -0.052 min
Response: 9532635
Conc: 10.87 ng/ml

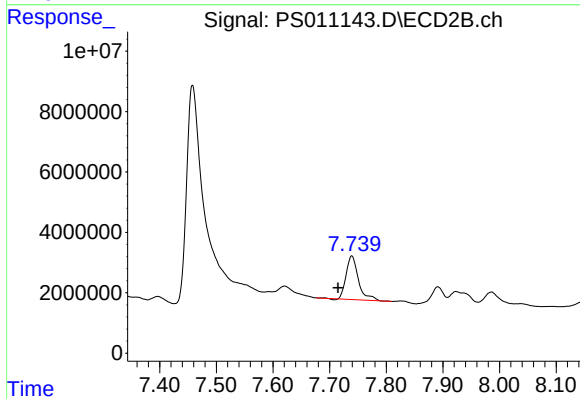

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.024 min
Response: 21800003
Conc: 37.13 ng/ml

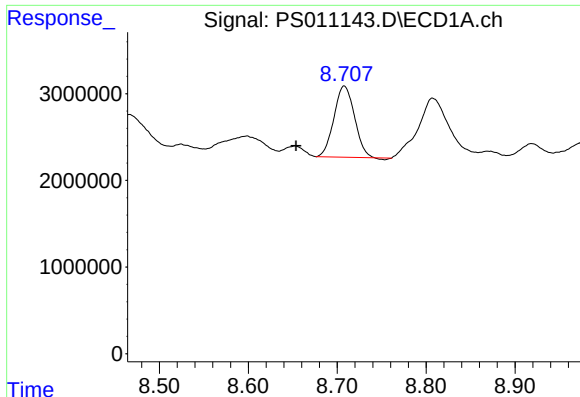

#10 Pentachlorophenol


R.T.: 8.708 min
Delta R.T.: 0.054 min
Response: 13012926
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

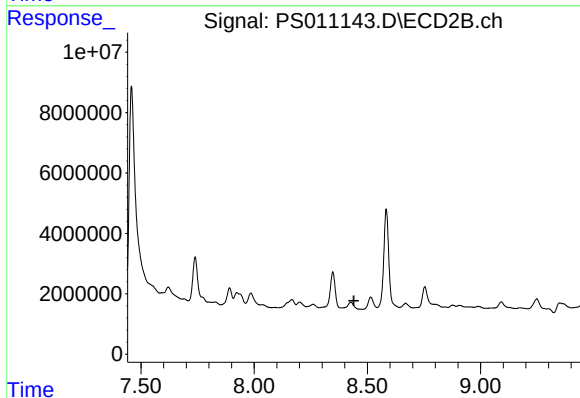


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

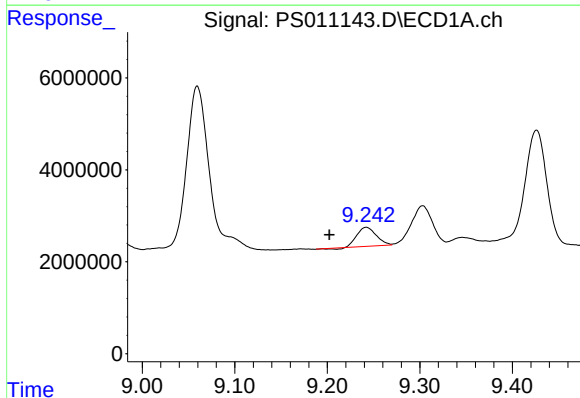


#11 2,4,5-TP (SILVEX)

R.T.: 9.242 min
Delta R.T.: 0.040 min
Response: 5830447
Conc: 1.17 ng/ml

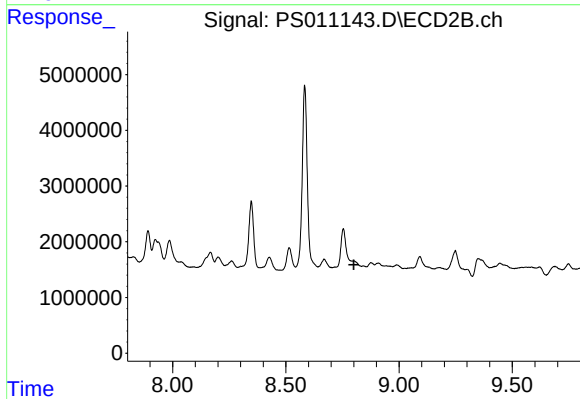

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.800 min
Response: 0
Conc: N.D.

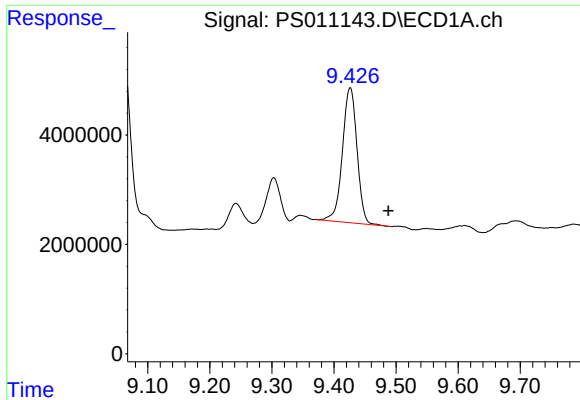

#12 2,4,5-T

R.T.: 9.426 min
Delta R.T.: -0.062 min
Response: 40366159
Conc: 8.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

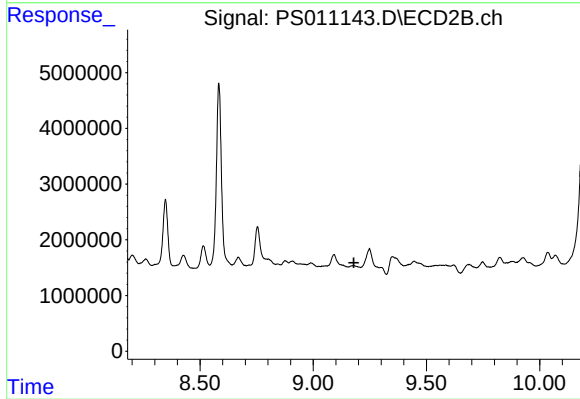

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.