

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 23:06
 Operator : DD\AJ
 Sample : L3186-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:53:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	309.3E6	222.2E6	341.042	401.027
Target Compounds							
1) T	Dalapon	2.998	2.587	49330758	180.3E6	44.056	239.067 #
2) T	3,5-DICHL...	0.000	6.099	0	110.6E6	N.D.	132.854
3) T	4-Nitroph...	6.995	6.551	9083635	15132092	22.756	47.091 #
5) T	DICAMBA	7.407	7.053	8199833	7258830	2.249	3.196 #
6) T	MCPD	7.639	0.000	11355067	0	3.982	N.D. #
7) T	MCPA	7.691	7.460	149.9E6	124.8E6	37.635	45.205
8) T	DICHLORPROP	8.059	7.739	19840471	9072806	22.625	15.453 #
9) T	2,4-D	8.277	0.000	8026038	0	9.076	N.D. #
10) T	Pentachlo...	8.707	0.000	14686958	0	1.181	N.D. #
11) T	2,4,5-TP ...	0.000	8.788	0	29410410	N.D.	9.774
12) T	2,4,5-T	9.425	0.000	42872339	0	9.204	N.D. #
15) T	Picloram	11.022	0.000	17360406	0	3.097	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 23:06
Operator : DD\AJ
Sample : L3186-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:53:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

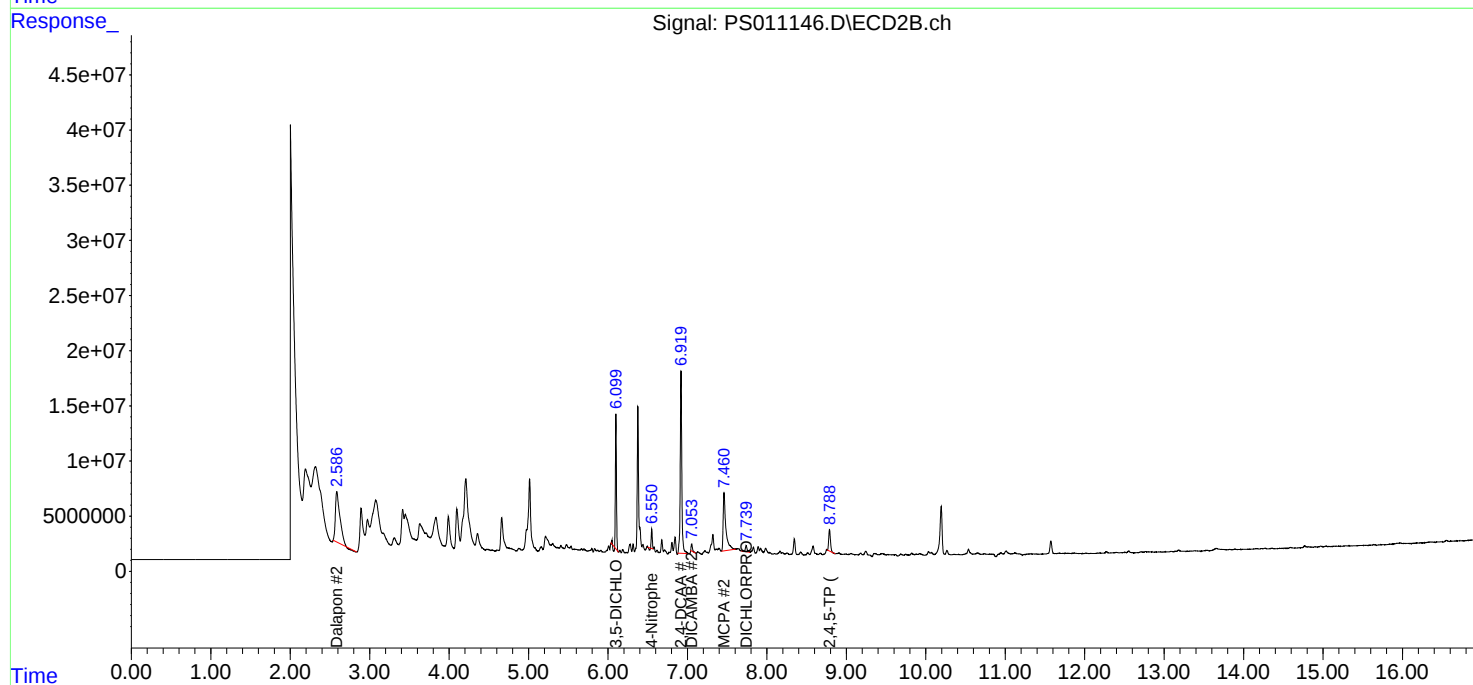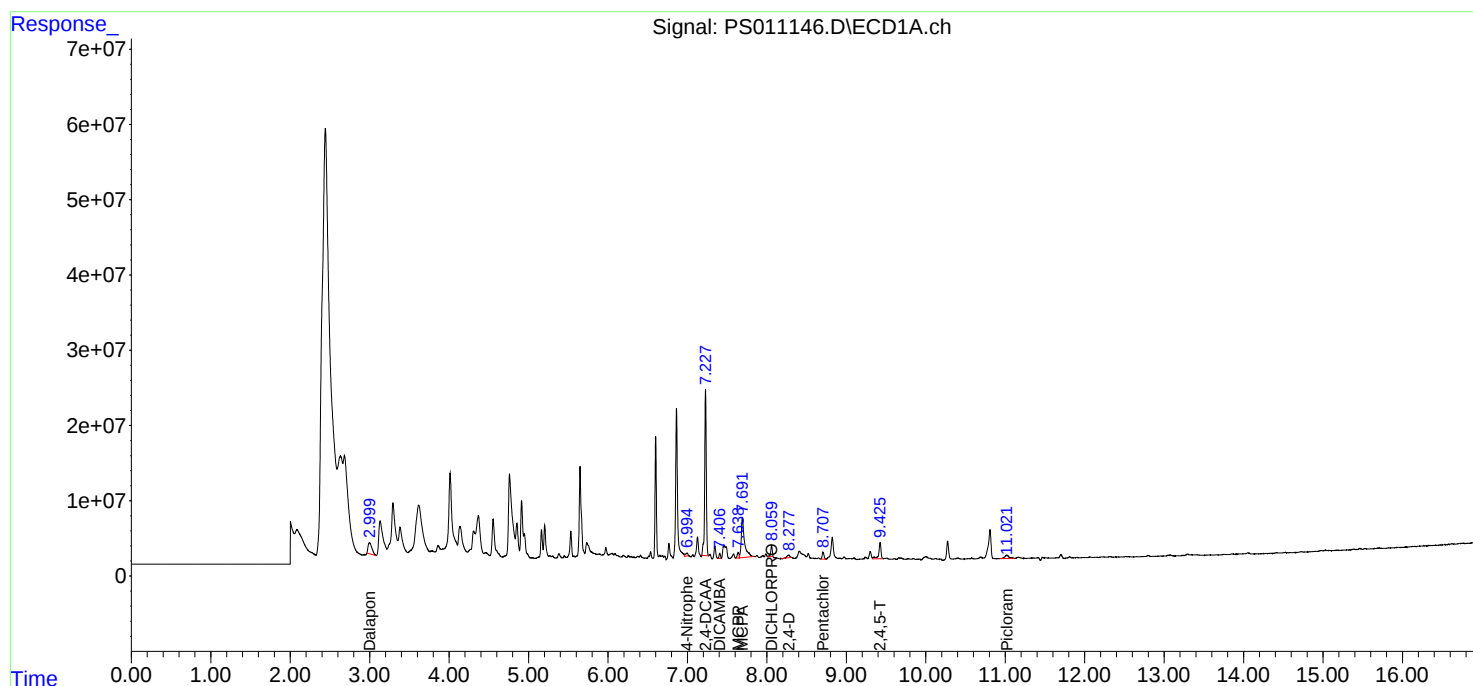


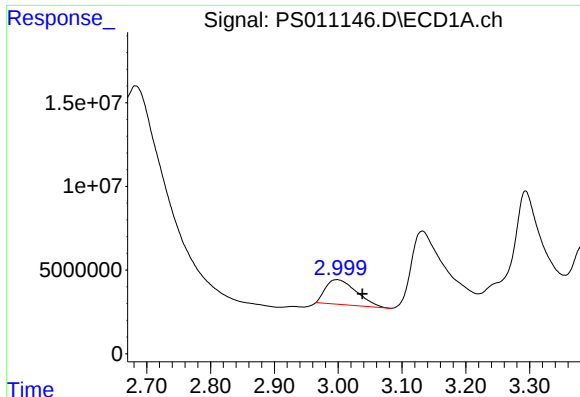

#1 Dalapon


R.T.: 2.998 min
Delta R.T.: -0.040 min
Response: 49330758
Conc: 44.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

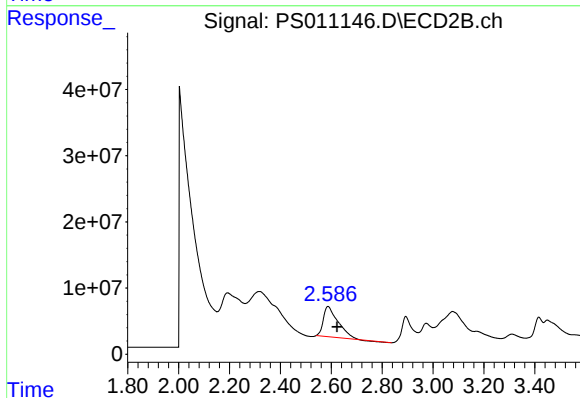


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.035 min
Response: 180343020
Conc: 239.07 ng/ml

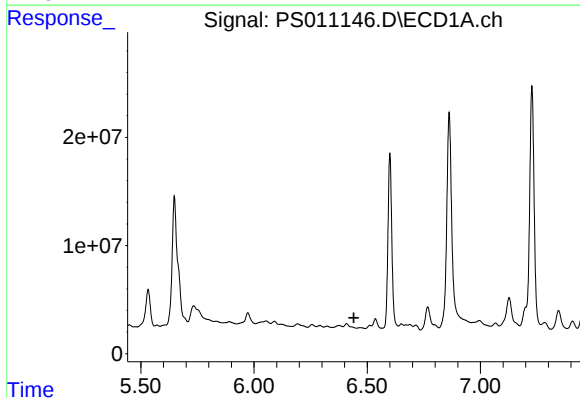


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

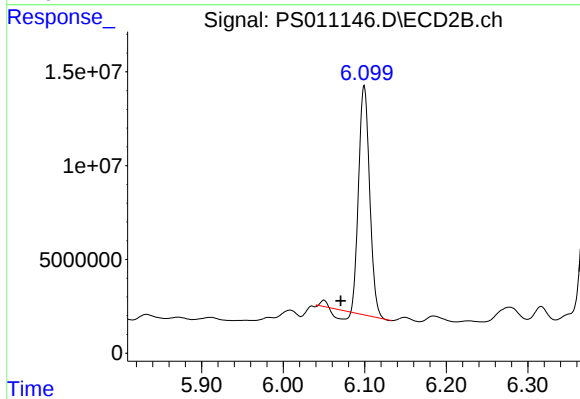

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.099 min
Delta R.T.: 0.029 min
Response: 110643952
Conc: 132.85 ng/ml

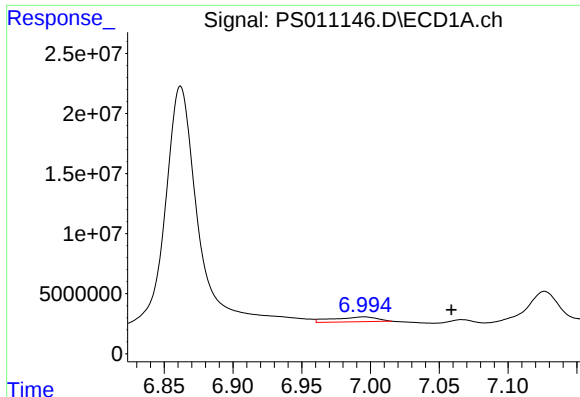

#3 4-Nitrophenol


R.T.: 6.995 min
Delta R.T.: -0.064 min
Response: 9083635
Conc: 22.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

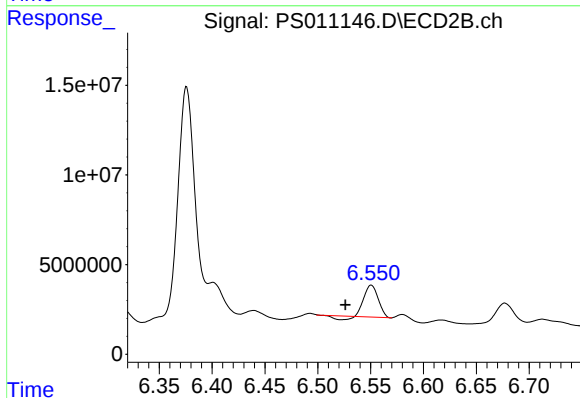


#3 4-Nitrophenol

R.T.: 6.551 min
Delta R.T.: 0.024 min
Response: 15132092
Conc: 47.09 ng/ml

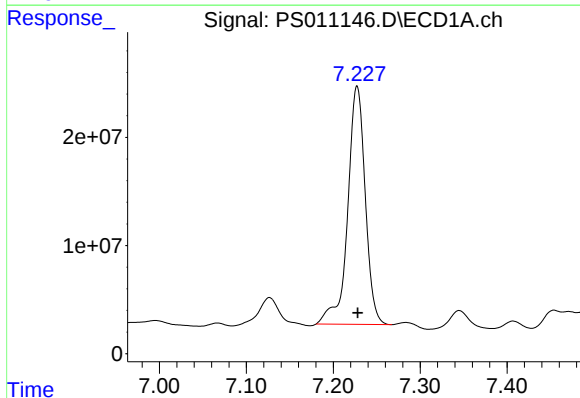


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 309263524
Conc: 341.04 ng/ml

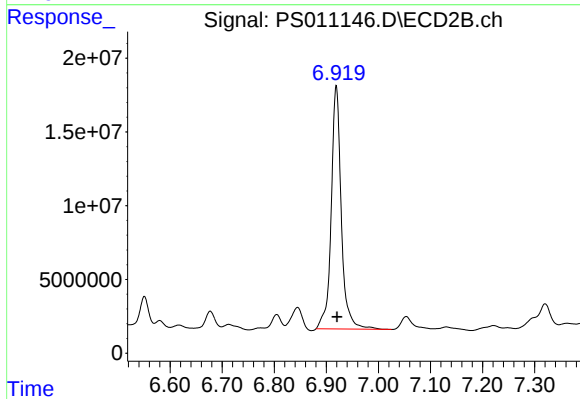

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 222199352
Conc: 401.03 ng/ml

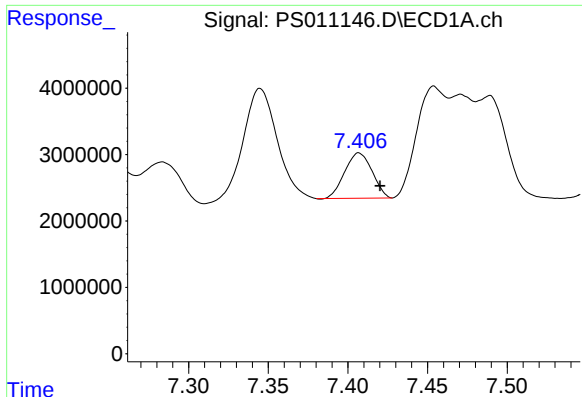

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: -0.013 min
Response: 8199833
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

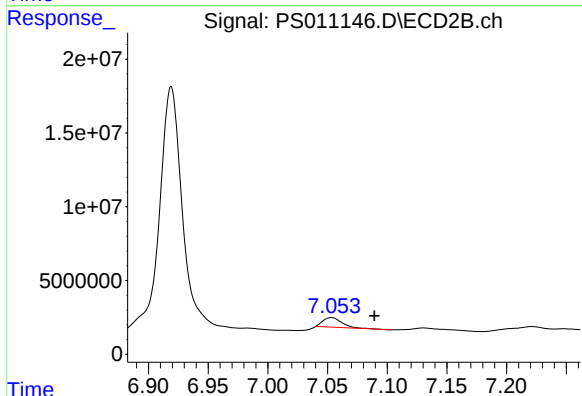


#5 DICAMBA

R.T.: 7.053 min
Delta R.T.: -0.036 min
Response: 7258830
Conc: 3.20 ng/ml

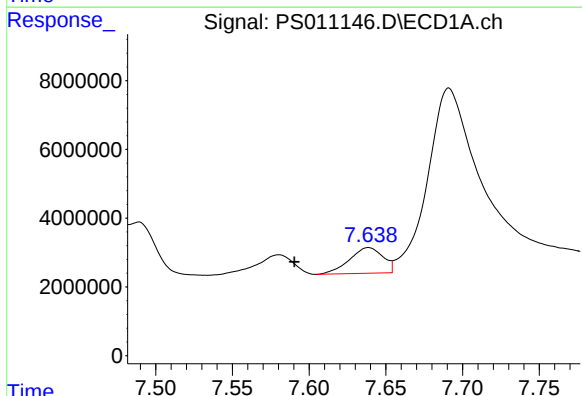


#6 MCP

R.T.: 7.639 min
Delta R.T.: 0.048 min
Response: 11355067
Conc: 3.98 ug/ml

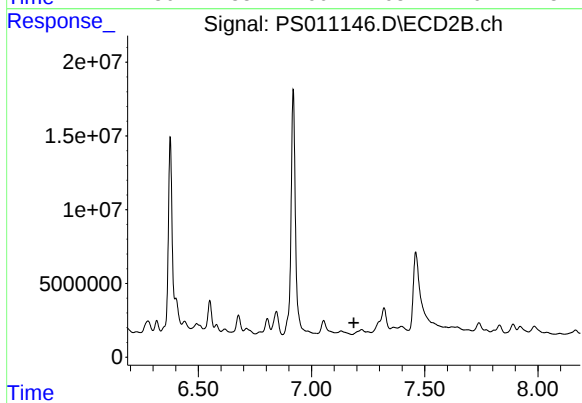

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

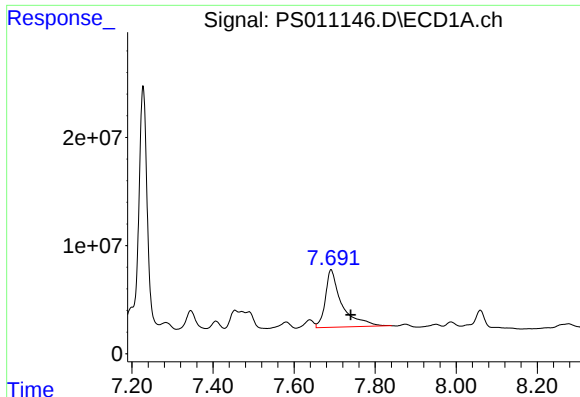

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.049 min
Response: 149878499
Conc: 37.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

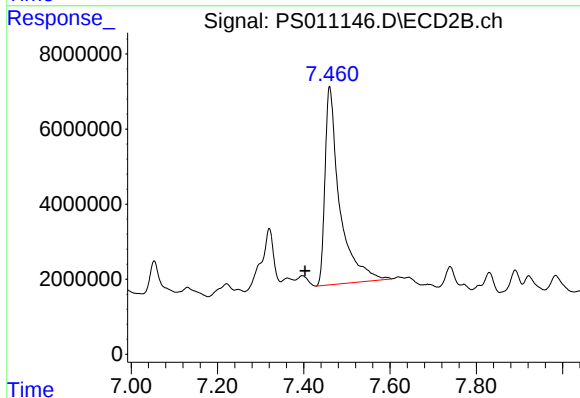


#7 MCPA

R.T.: 7.460 min
Delta R.T.: 0.058 min
Response: 124766568
Conc: 45.21 ug/ml

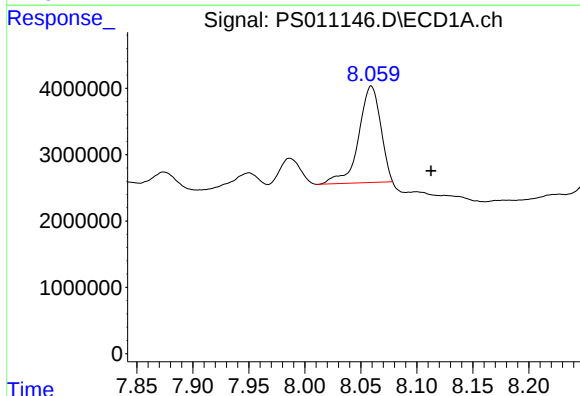


#8 DICHLORPROP

R.T.: 8.059 min
Delta R.T.: -0.053 min
Response: 19840471
Conc: 22.62 ng/ml

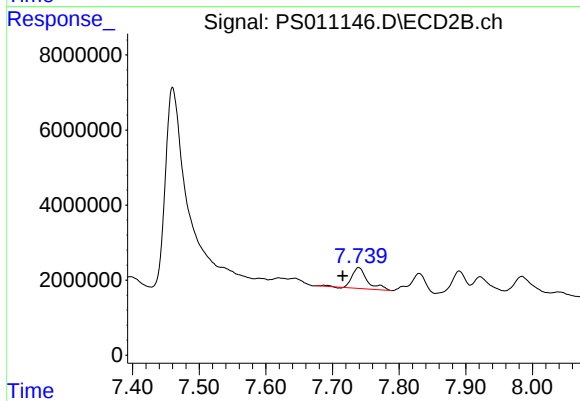

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.024 min
Response: 9072806
Conc: 15.45 ng/ml

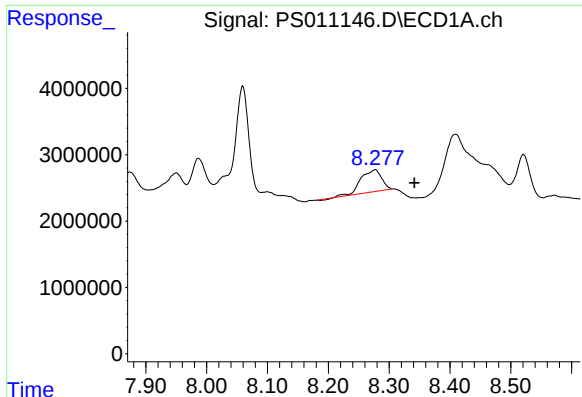

#9 2,4-D


R.T.: 8.277 min
Delta R.T.: -0.065 min
Response: 8026038
Conc: 9.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

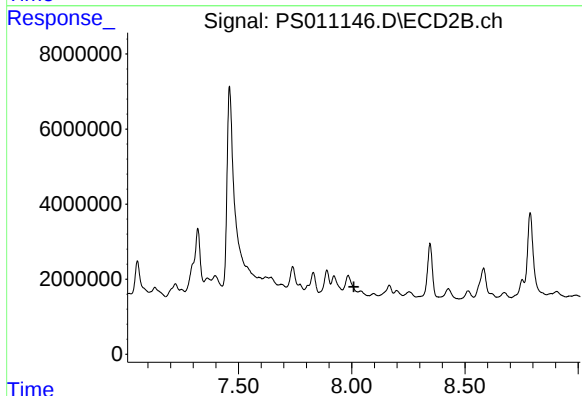


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.009 min
Response: 0
Conc: N.D.

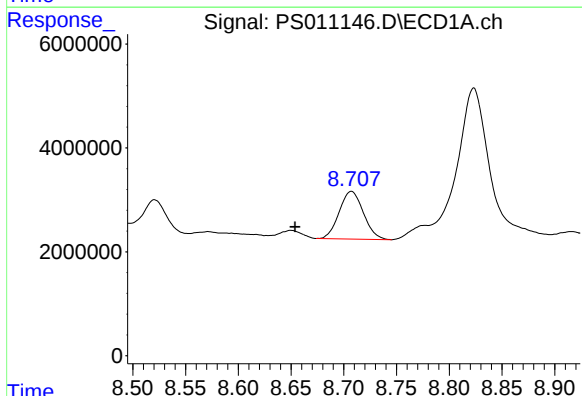


#10 Pentachlorophenol

R.T.: 8.707 min
Delta R.T.: 0.053 min
Response: 14686958
Conc: 1.18 ng/ml

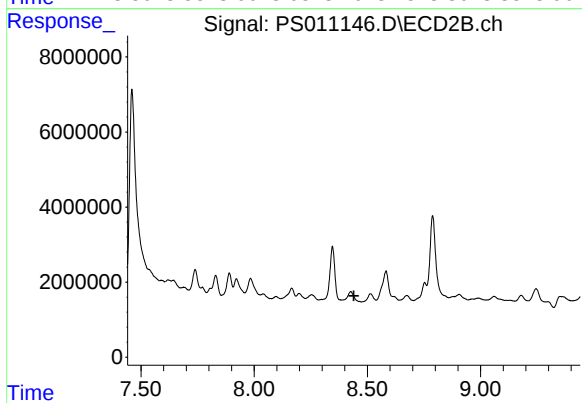

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

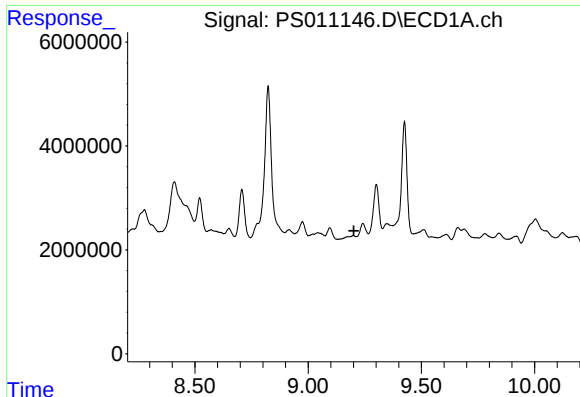

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.202 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

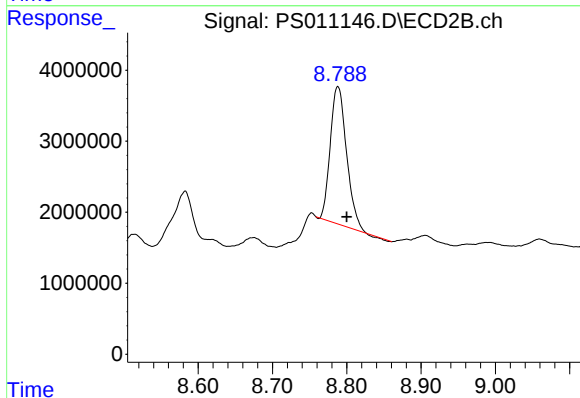


#11 2,4,5-TP (SILVEX)

R.T.: 8.788 min
Delta R.T.: -0.012 min
Response: 29410410
Conc: 9.77 ng/ml

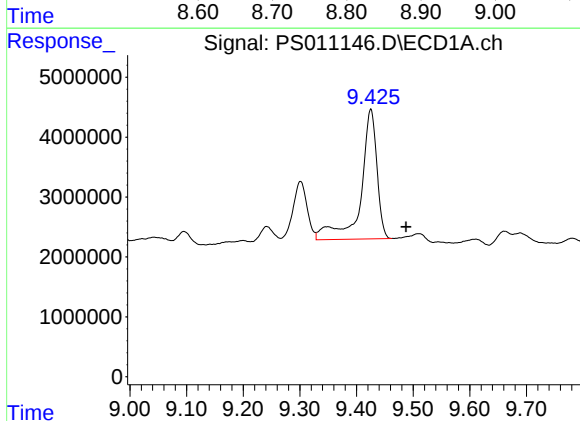


#12 2,4,5-T

R.T.: 9.425 min
Delta R.T.: -0.063 min
Response: 42872339
Conc: 9.20 ng/ml

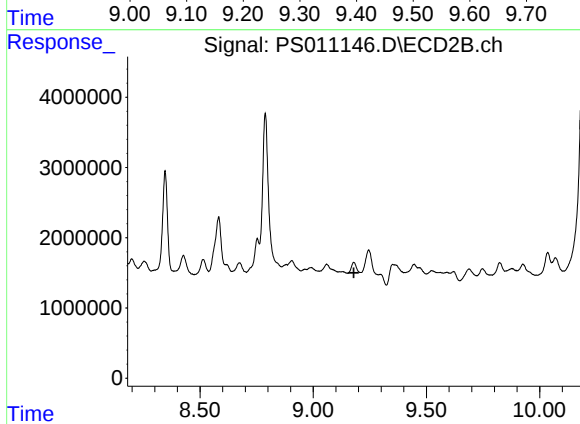

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

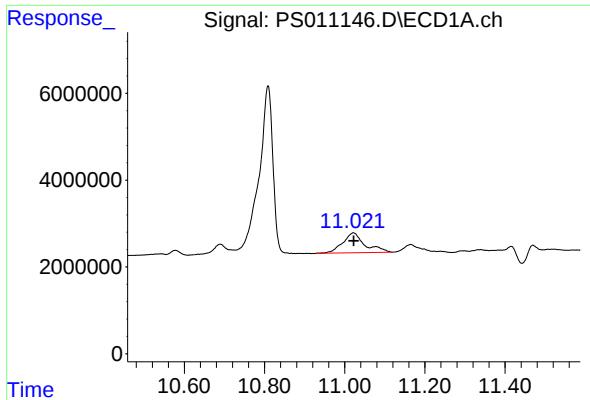

#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.000 min
Response: 17360406
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

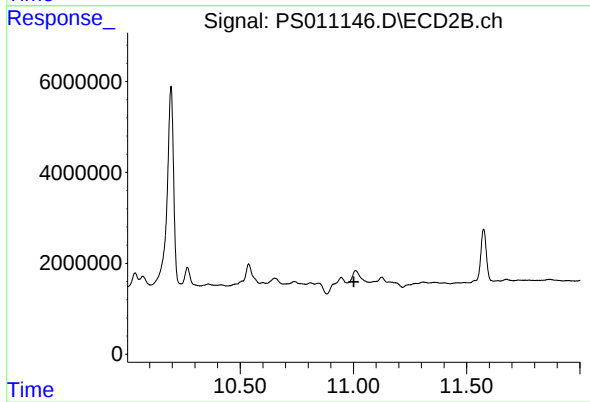

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.