

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
 Data File : PS011147.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2020 23:29
 Operator : DD\AJ
 Sample : L3187-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 03:54:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.919	343.5E6	243.7E6	378.824	439.905
Target Compounds							
1) T	Dalapon	2.996	2.586	50699266	168.3E6	45.278	223.114 #
2) T	3,5-DICHL...	0.000	6.100	0	77387817	N.D.	92.922
3) T	4-Nitroph...	6.994	6.551	8998227	11473093	22.542	35.705 #
5) T	DICAMBA	7.407	7.054	6162418	5571508	1.690	2.453 #
6) T	MCPD	7.639	0.000	6850959	0	2.403	N.D. #
7) T	MCPA	7.695	7.467	86786048	69573451	21.792	25.208
8) T	DICHLORPROP	8.059	0.000	13466159	0	15.356	N.D. #
10) T	Pentachlo...	8.707	0.000	14477744	0	1.164	N.D. #
12) T	2,4,5-T	9.425	0.000	27931553	0	5.997	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS070920\
Data File : PS011147.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2020 23:29
Operator : DD\AJ
Sample : L3187-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 03:54:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

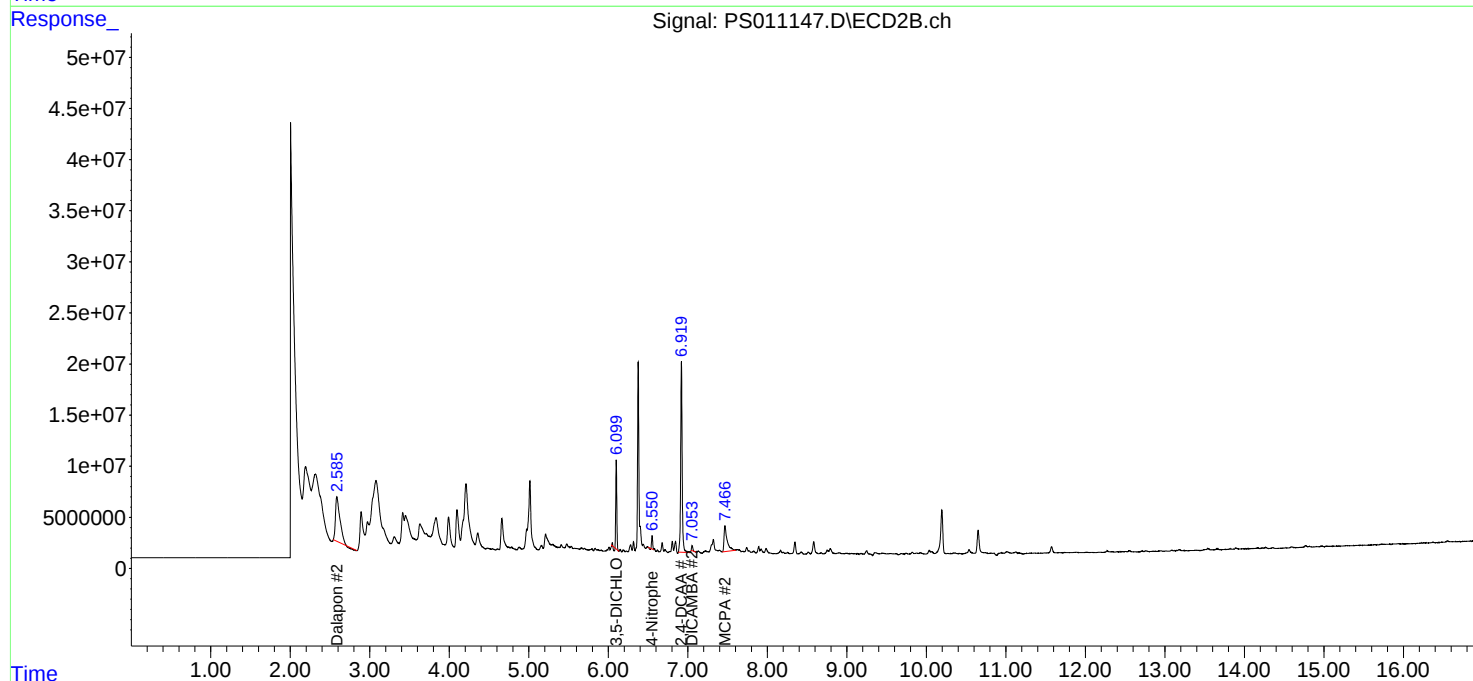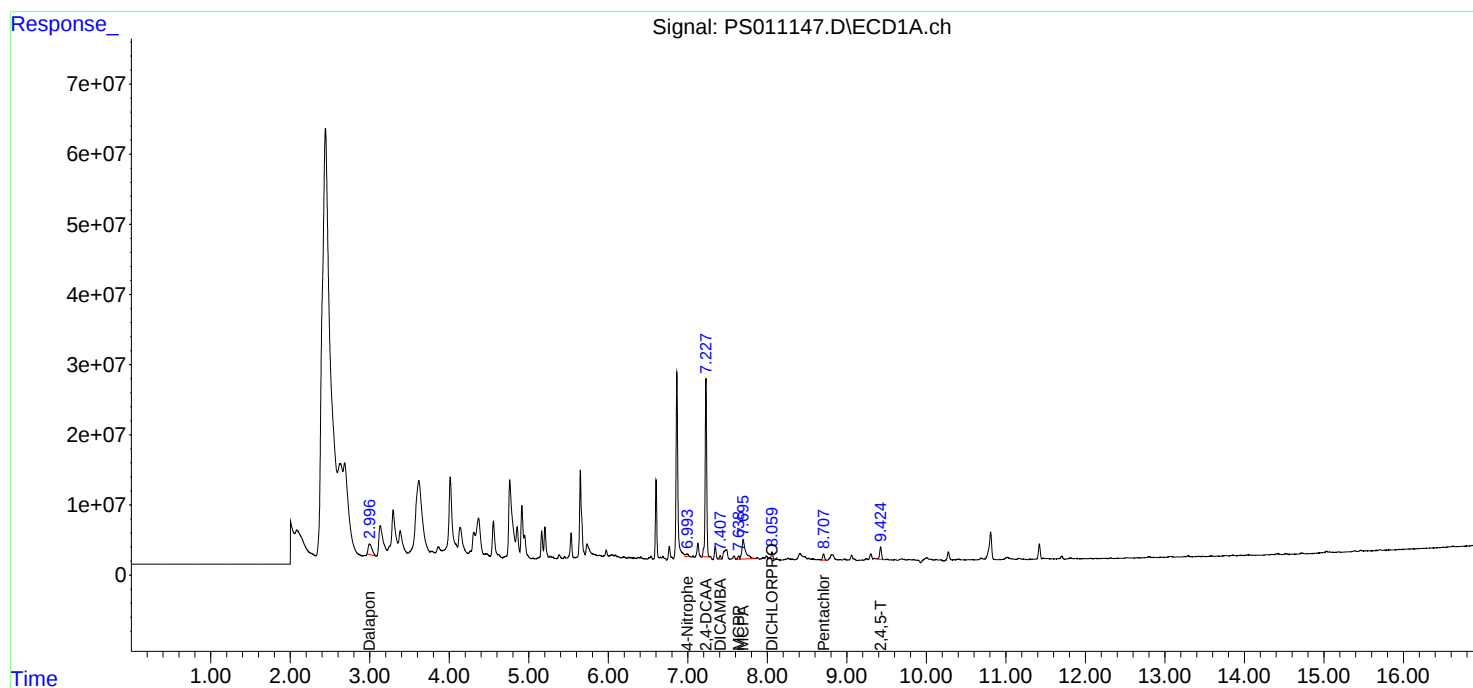


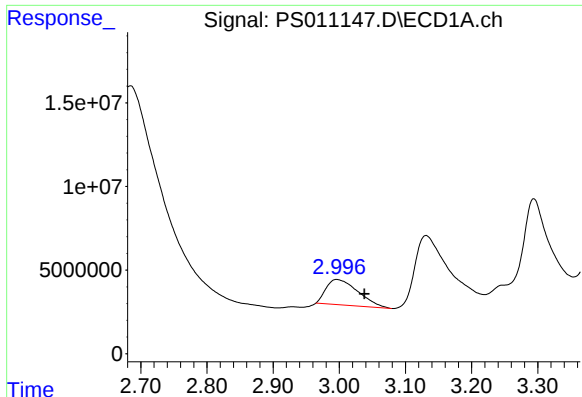

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.042 min
Response: 50699266
Conc: 45.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

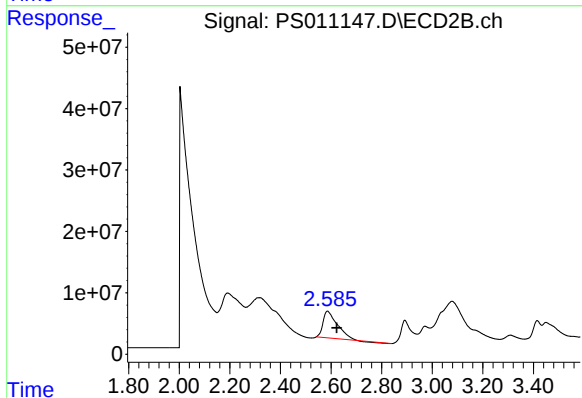


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.036 min
Response: 168308582
Conc: 223.11 ng/ml

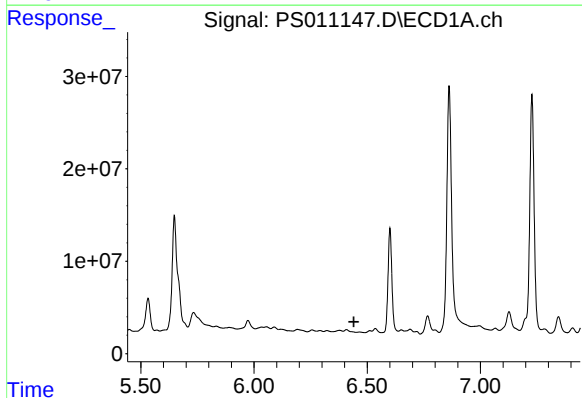


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.441 min
Response: 0
Conc: N.D.

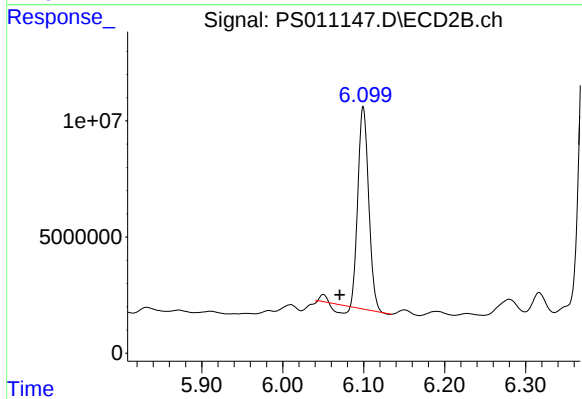

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.100 min
Delta R.T.: 0.029 min
Response: 77387817
Conc: 92.92 ng/ml

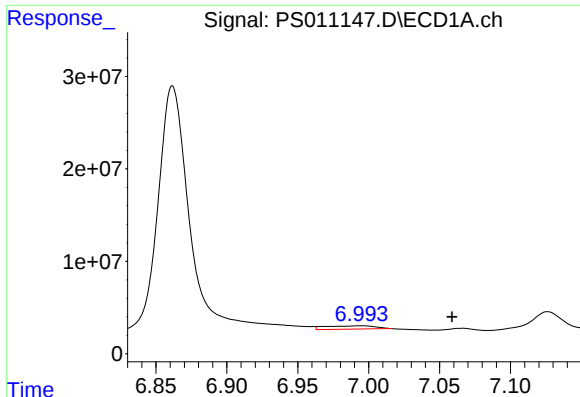

#3 4-Nitrophenol


R.T.: 6.994 min
Delta R.T.: -0.065 min
Response: 8998227
Conc: 22.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

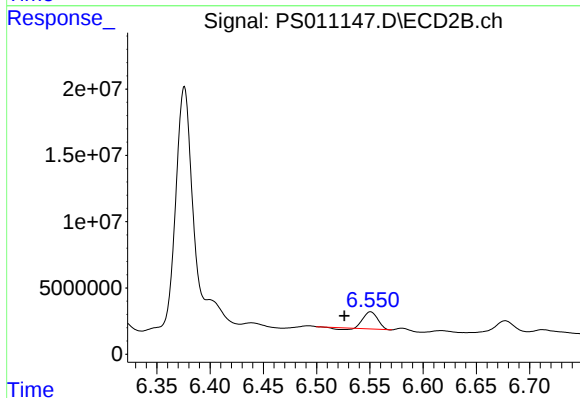


#3 4-Nitrophenol

R.T.: 6.551 min
Delta R.T.: 0.025 min
Response: 11473093
Conc: 35.70 ng/ml

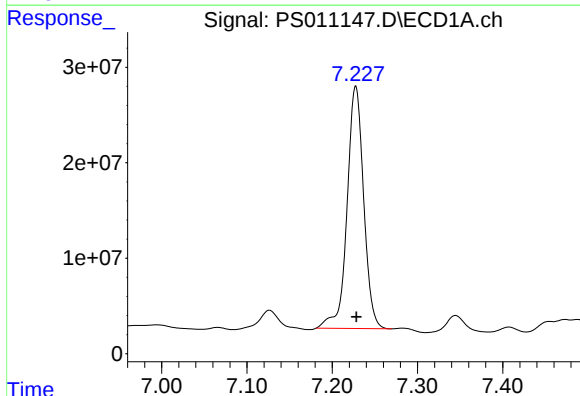


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 343524895
Conc: 378.82 ng/ml

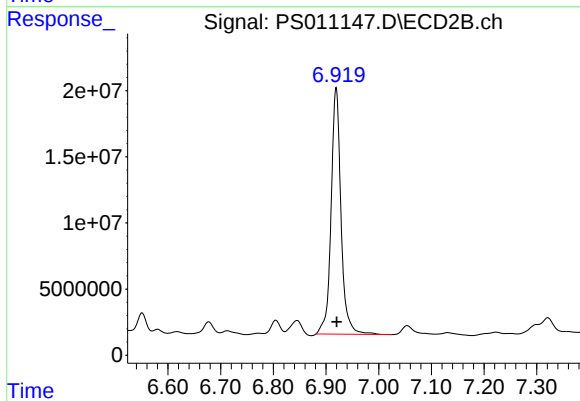

#4 2,4-DCAA


R.T.: 6.919 min
Delta R.T.: -0.001 min
Response: 243740803
Conc: 439.90 ng/ml

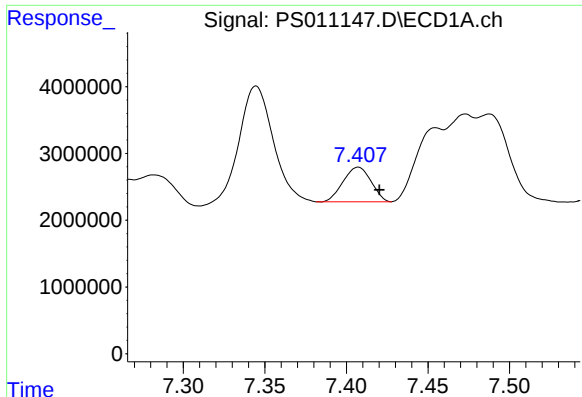

#5 DICAMBA


R.T.: 7.407 min
Delta R.T.: -0.013 min
Response: 6162418
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

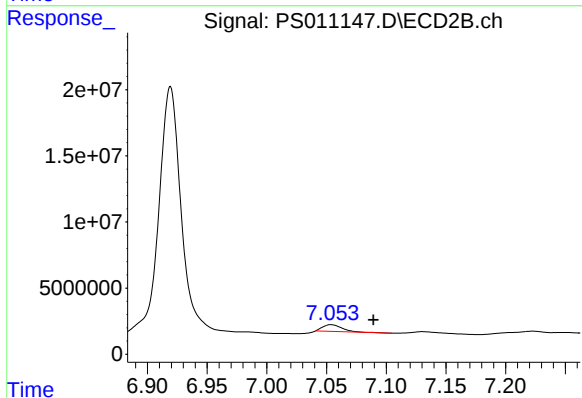


#5 DICAMBA

R.T.: 7.054 min
Delta R.T.: -0.035 min
Response: 5571508
Conc: 2.45 ng/ml

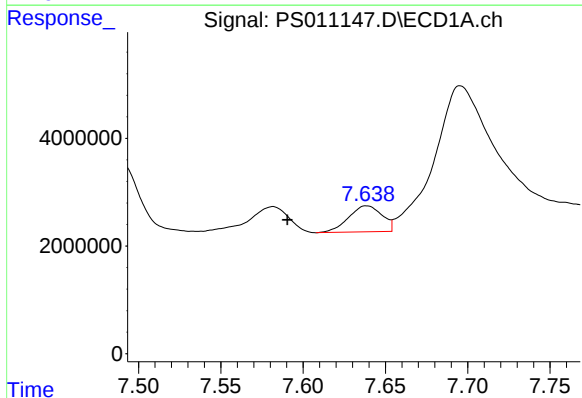


#6 MCP

R.T.: 7.639 min
Delta R.T.: 0.048 min
Response: 6850959
Conc: 2.40 ug/ml

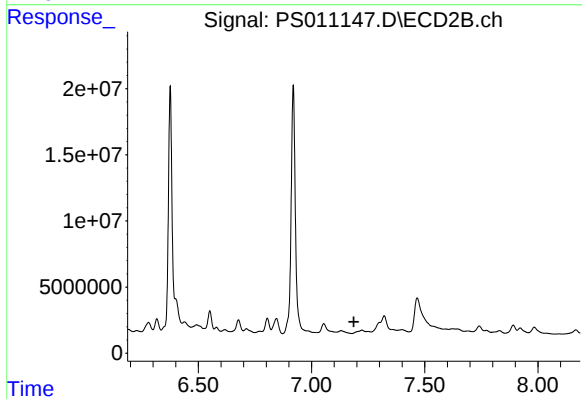

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.187 min
Response: 0
Conc: N.D.

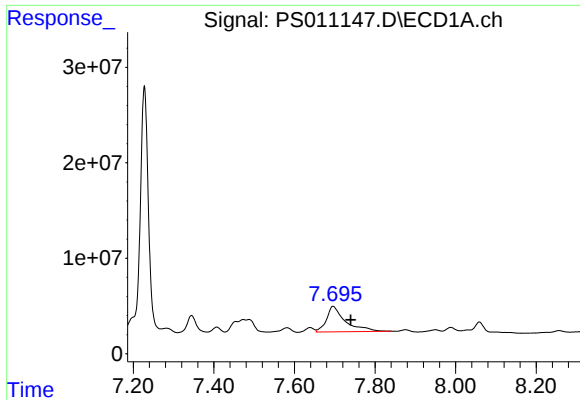

#7 MCPA


R.T.: 7.695 min
Delta R.T.: -0.045 min
Response: 86786048
Conc: 21.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

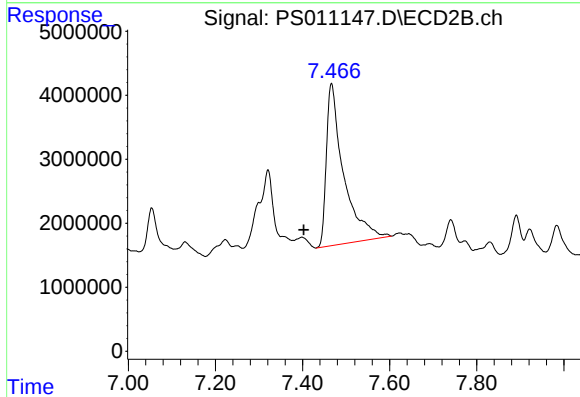


#7 MCPA

R.T.: 7.467 min
Delta R.T.: 0.064 min
Response: 69573451
Conc: 25.21 ug/ml

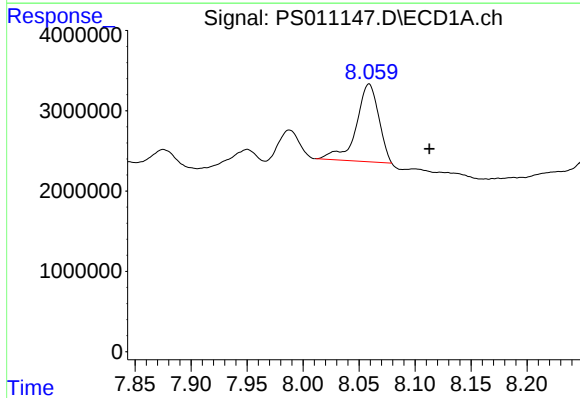


#8 DICHLORPROP

R.T.: 8.059 min
Delta R.T.: -0.054 min
Response: 13466159
Conc: 15.36 ng/ml

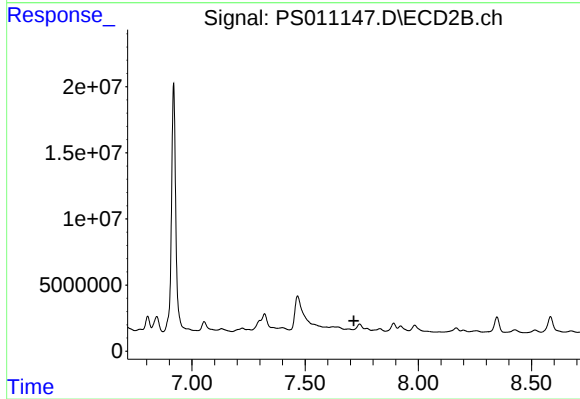

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.715 min
Response: 0
Conc: N.D.

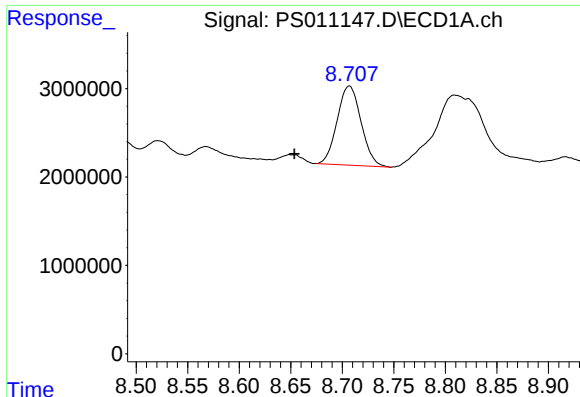

#10 Pentachlorophenol


R.T.: 8.707 min
Delta R.T.: 0.053 min
Response: 14477744
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

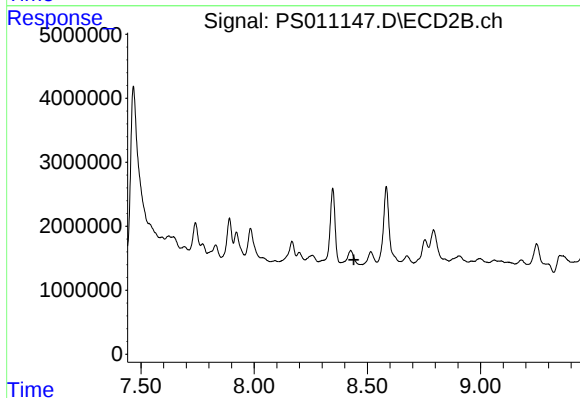


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.440 min
Response: 0
Conc: N.D.

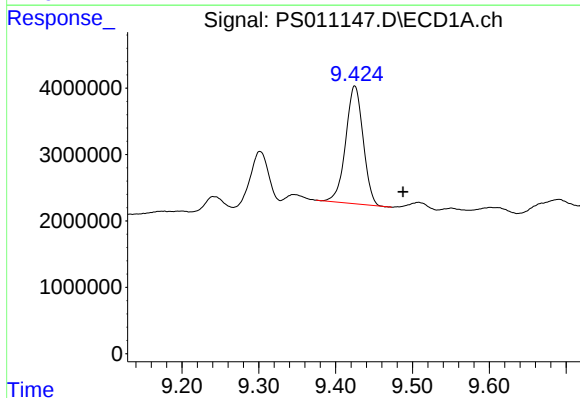

#12 2,4,5-T

R.T.: 9.425 min
Delta R.T.: -0.063 min
Response: 27931553
Conc: 6.00 ng/ml

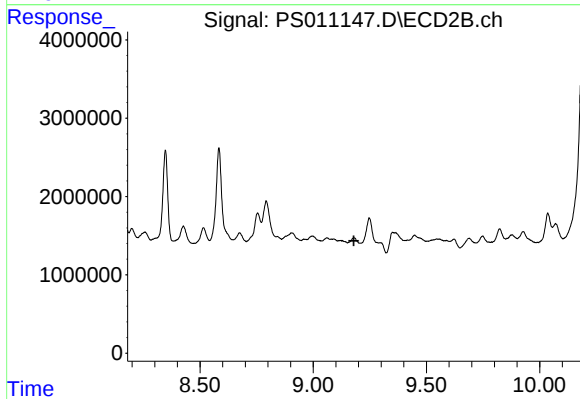

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.