

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
 Data File : PS005440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2019 12:07
 Operator : SM\AJ
 Sample : PB121229BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121229BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 15:20:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.571	5.285	649.5E6	430.5E6	442.495	429.474
Target Compounds							
1) T	Dalapon	2.076	0.000	41117521	0	22.307	N.D. #
2) T	3,5-DICHL...	0.000	4.604	0	126.4E6	N.D.	95.851
3) T	4-Nitroph...	5.374	0.000	20387032	0	28.147	N.D. #
5) T	DICAMBA	5.669	0.000	17704435	0	3.103	N.D. #
7) T	MCPA	6.061	5.675	30186005	27929801	4.807	6.895 #
10) T	Pentachlo...	0.000	6.550	0	43386437	N.D.	3.375
11) T	2,4,5-TP ...	0.000	6.942	0	74608860	N.D.	14.010
15) T	Picloram	0.000	9.114	0	9430522	N.D.	1.250
16) T	DCPA	0.000	9.114	0	9430522	N.D.	1.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
Data File : PS005440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2019 12:07
Operator : SM\AJ
Sample : PB121229BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB121229BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 15:20:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

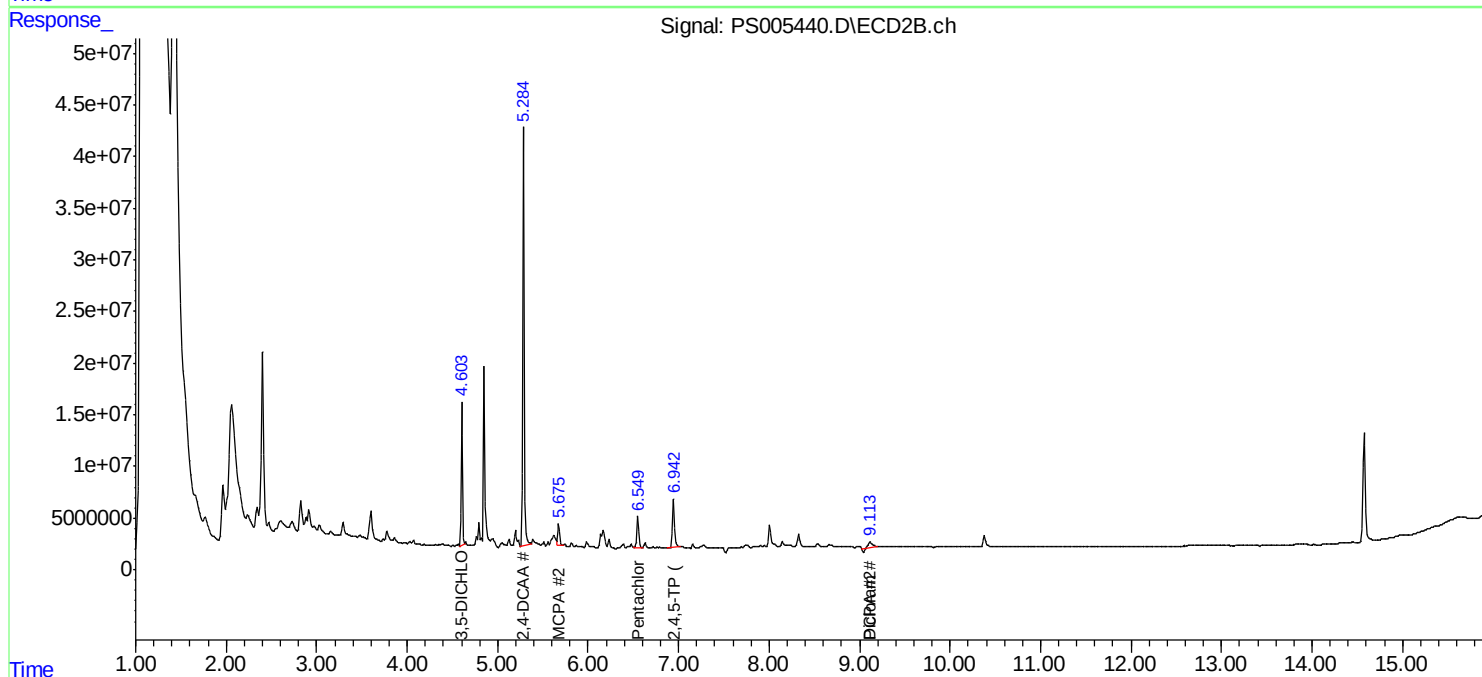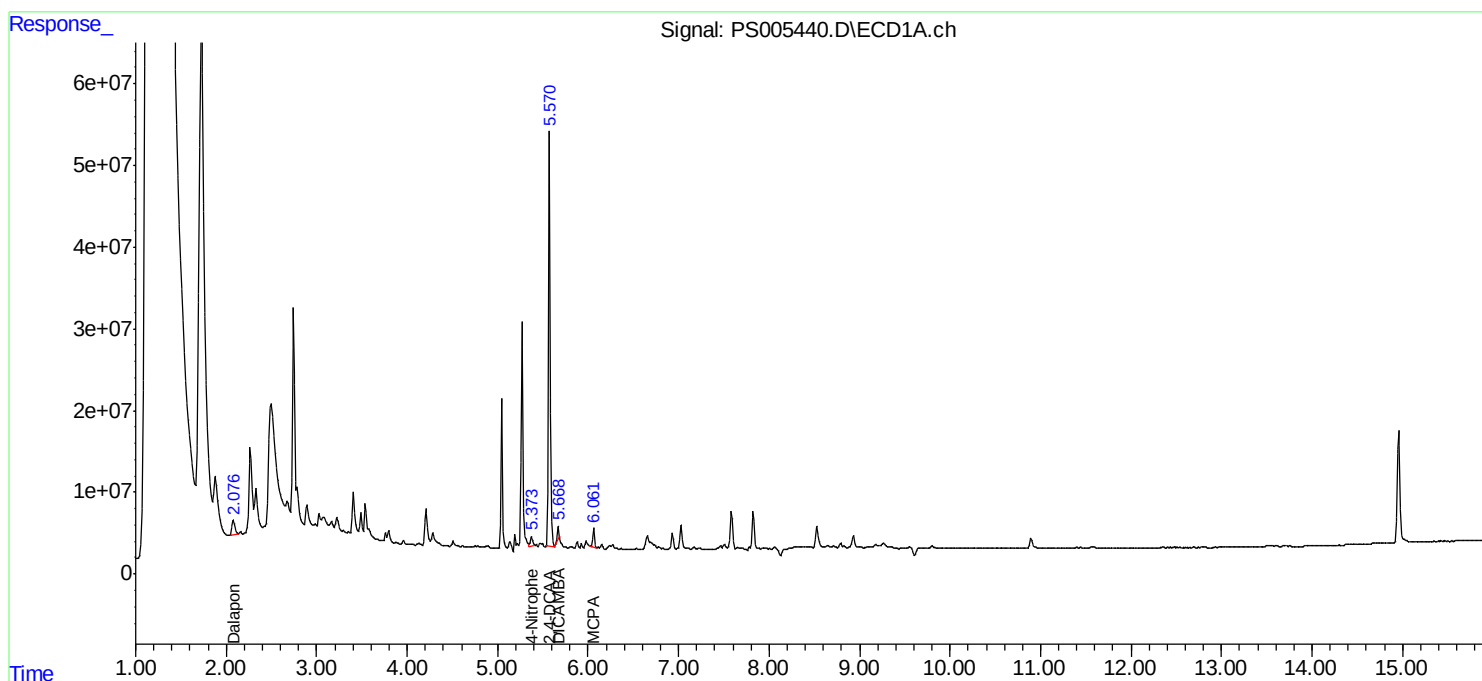


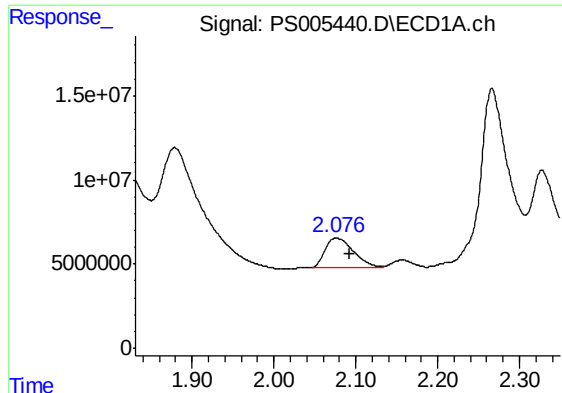

#1 Dalapon


R.T.: 2.076 min
Delta R.T.: -0.016 min
Response: 41117521
Conc: 22.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121229BL

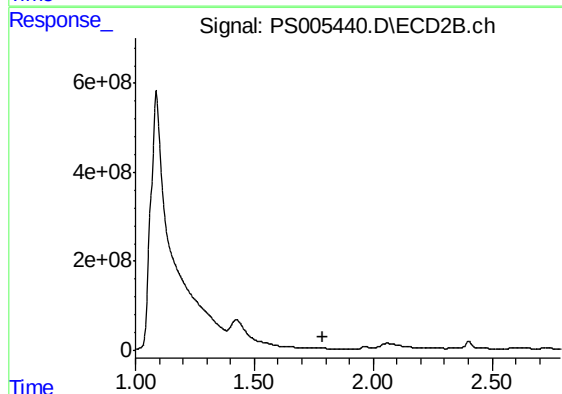


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

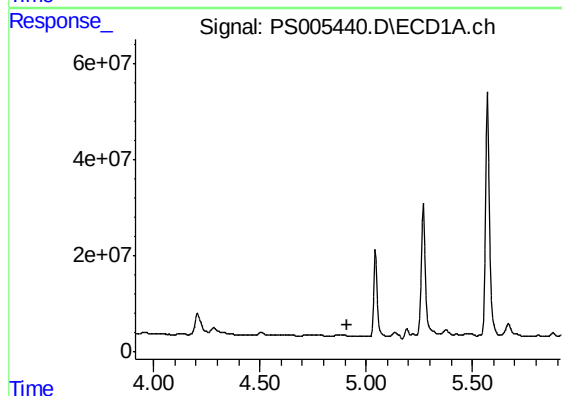


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

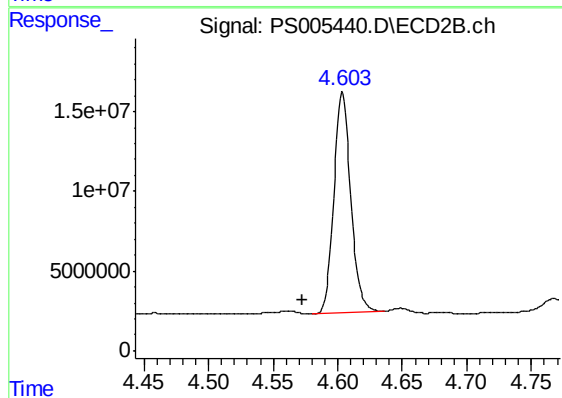

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.031 min
Response: 126399572
Conc: 95.85 ng/ml

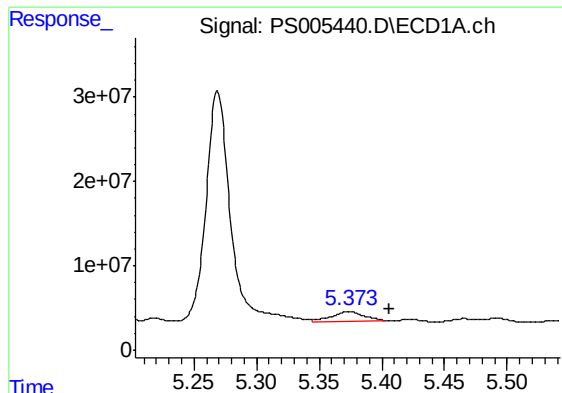

#3 4-Nitrophenol


R.T.: 5.374 min
Delta R.T.: -0.032 min
Response: 20387032
Conc: 28.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121229BL

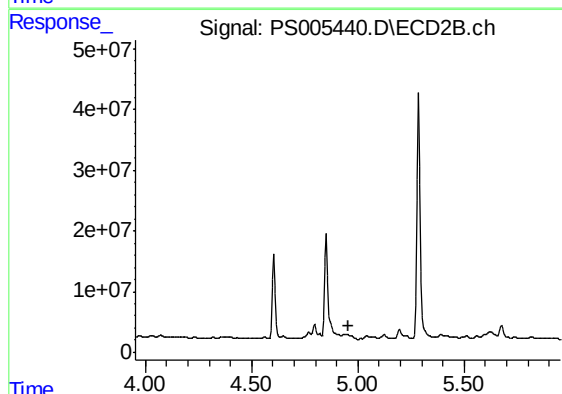


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

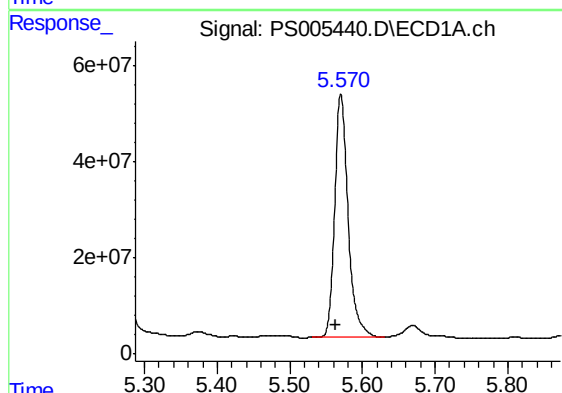


#4 2,4-DCAA

R.T.: 5.571 min
Delta R.T.: 0.007 min
Response: 649535372
Conc: 442.50 ng/ml

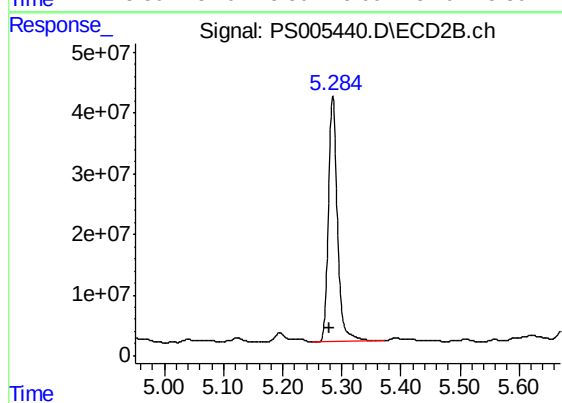

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: 0.005 min
Response: 430491535
Conc: 429.47 ng/ml

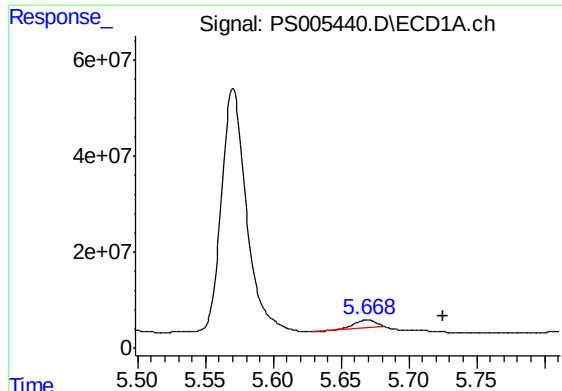

#5 DICAMBA


R.T.: 5.669 min
Delta R.T.: -0.056 min
Response: 17704435
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121229BL

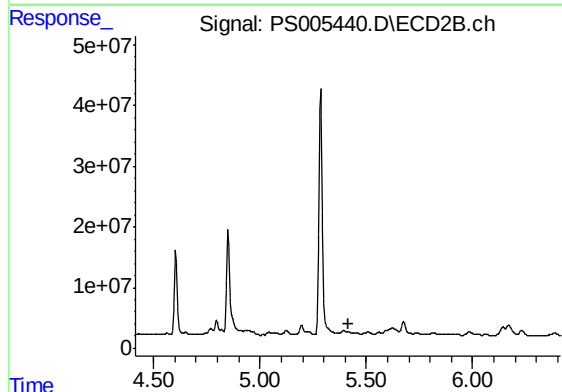


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.414 min
Response: 0
Conc: N.D.

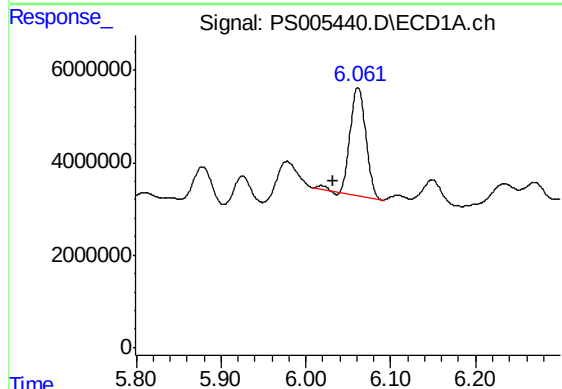


#7 MCPA

R.T.: 6.061 min
Delta R.T.: 0.029 min
Response: 30186005
Conc: 4.81 ug/ml

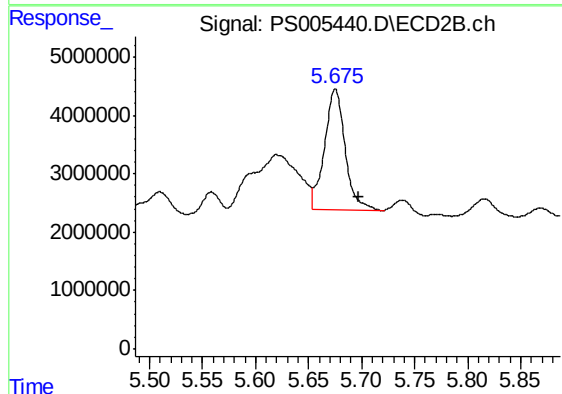

#7 MCPA


R.T.: 5.675 min
Delta R.T.: -0.023 min
Response: 27929801
Conc: 6.89 ug/ml

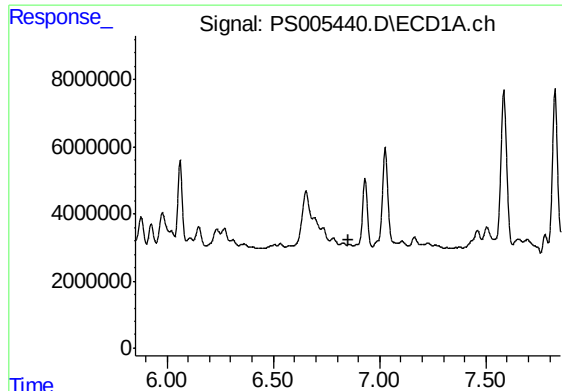

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121229BL

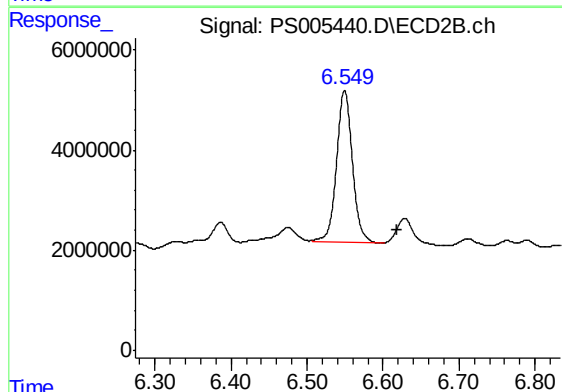


#10 Pentachlorophenol

R.T.: 6.550 min
Delta R.T.: -0.070 min
Response: 43386437
Conc: 3.37 ng/ml

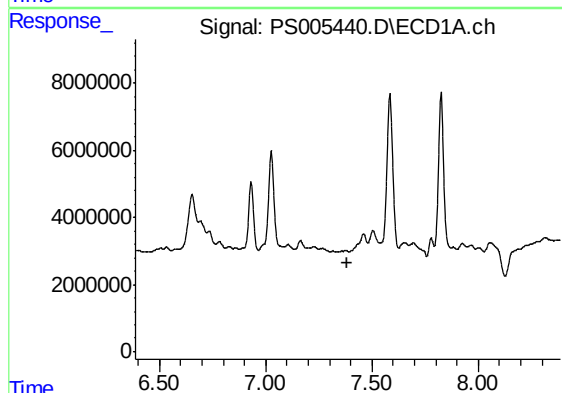


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

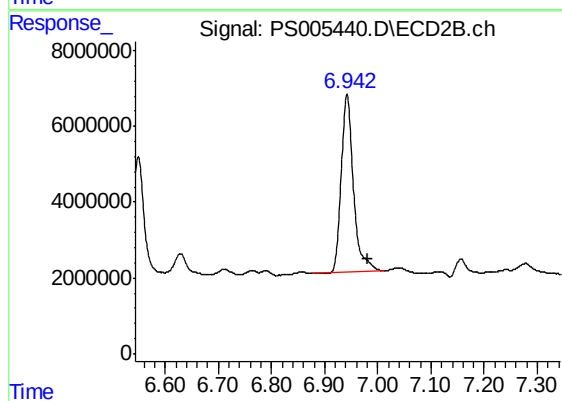

#11 2,4,5-TP (SILVEX)


R.T.: 6.942 min
Delta R.T.: -0.038 min
Response: 74608860
Conc: 14.01 ng/ml

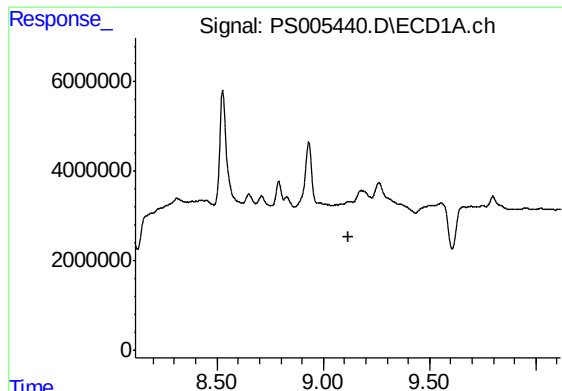

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.117 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121229BL

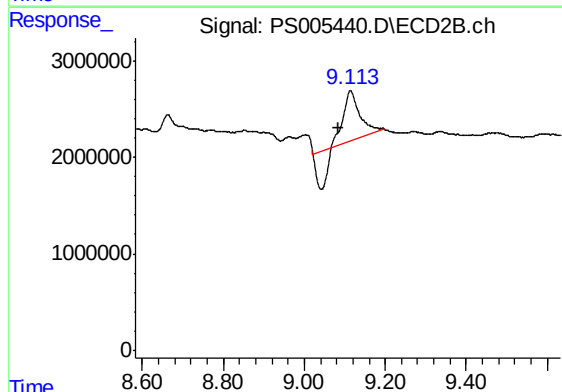


#15 Picloram

R.T.: 9.114 min
Delta R.T.: 0.029 min
Response: 9430522
Conc: 1.25 ng/ml

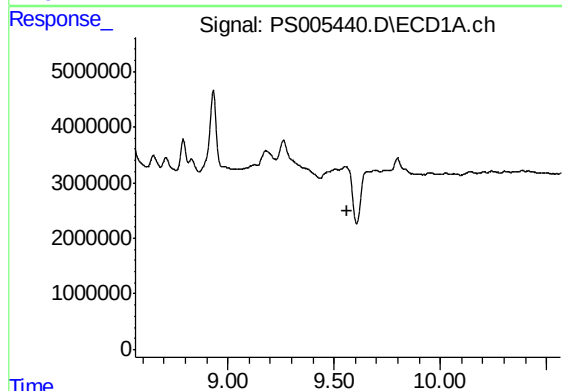

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.565 min
Response: 0
Conc: N.D.

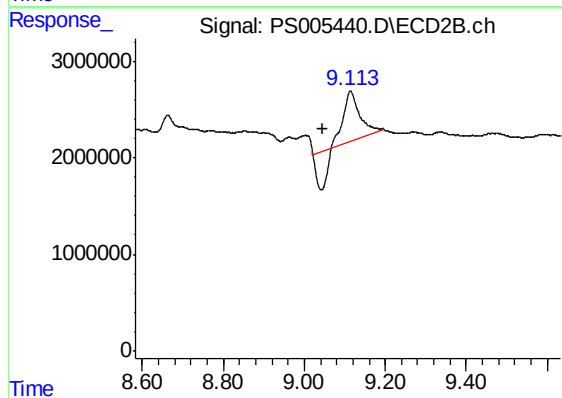

#16 DCPA

R.T.: 9.114 min
Delta R.T.: 0.068 min
Response: 9430522
Conc: 1.39 ng/ml