

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
 Data File : PS005450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2019 15:53
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 17:12:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.303	614.0E6	410.2E6	418.310	409.267
Target Compounds							
7) T	MCPA	0.000	5.641	0	78975572	N.D.	19.496
15) T	Picloram	9.127	0.000	194.1E6	0	16.895	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
Data File : PS005450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2019 15:53
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 17:12:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

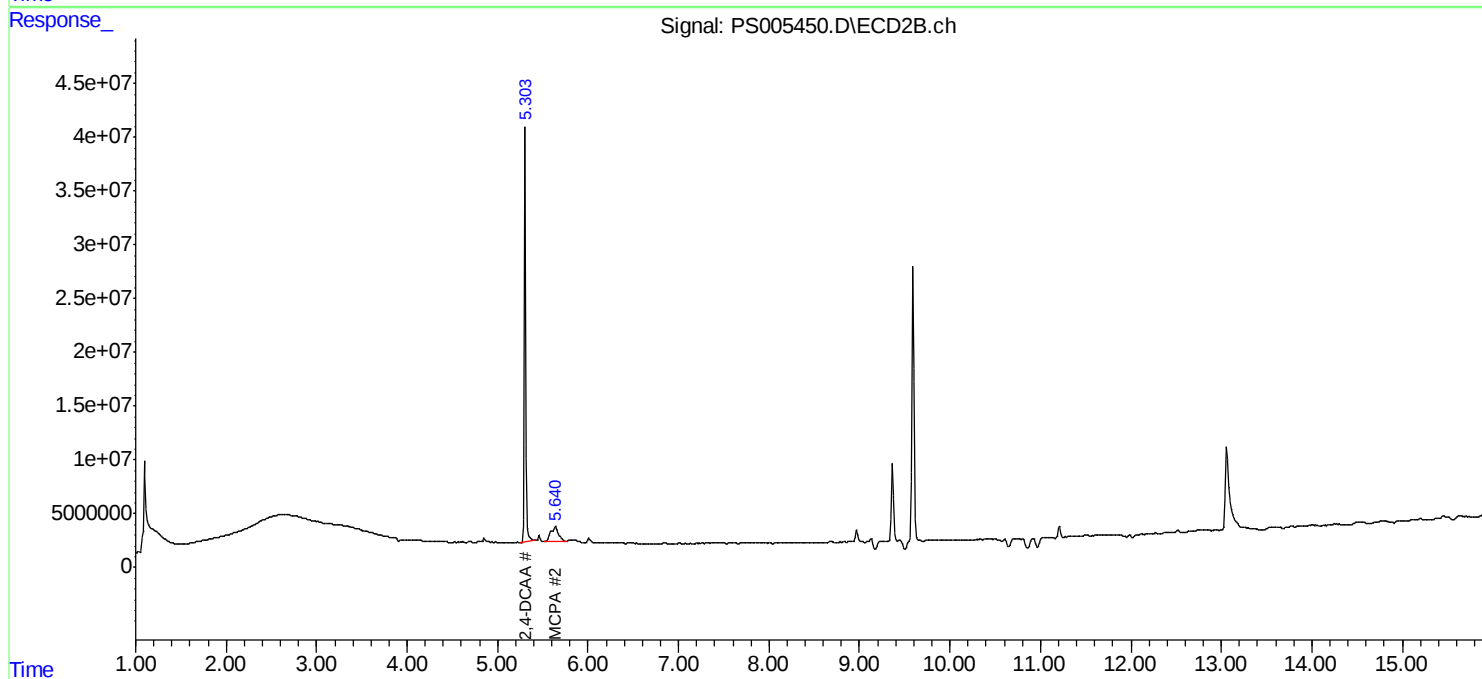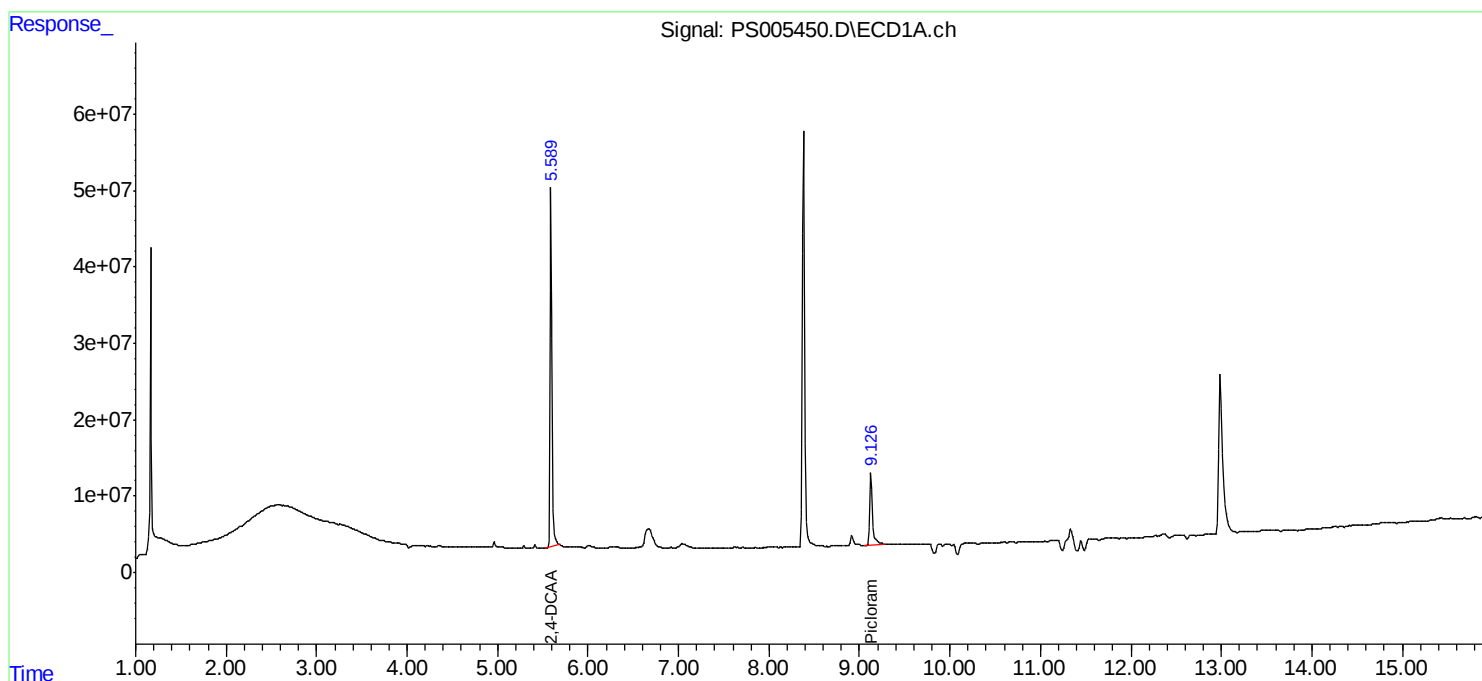


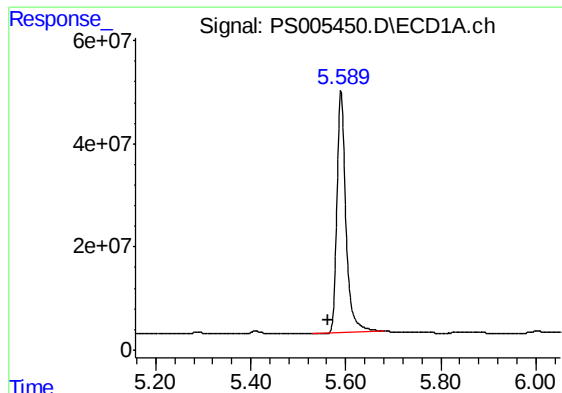

#4 2,4-DCAA


R.T.: 5.590 min
Delta R.T.: 0.026 min
Response: 614034334
Conc: 418.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

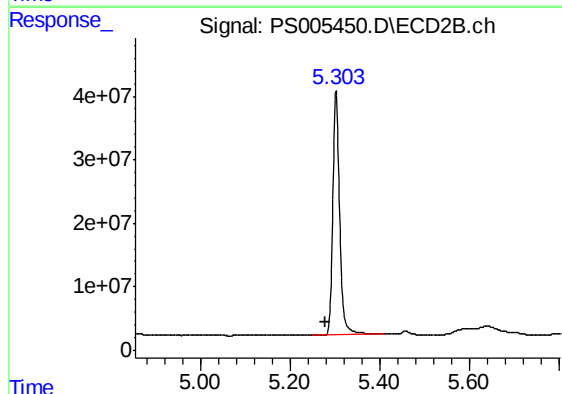


#4 2,4-DCAA

R.T.: 5.303 min
Delta R.T.: 0.024 min
Response: 410236477
Conc: 409.27 ng/ml

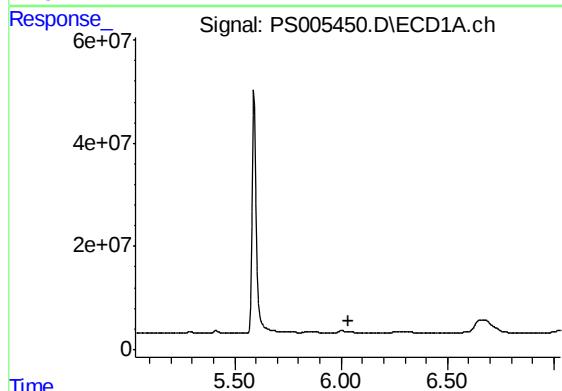


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.032 min
Response: 0
Conc: N.D.

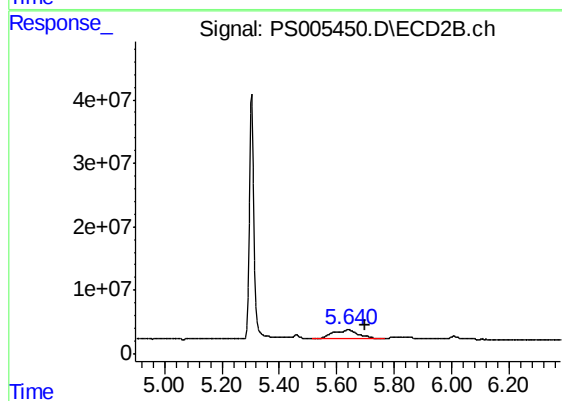

#7 MCPA


R.T.: 5.641 min
Delta R.T.: -0.057 min
Response: 78975572
Conc: 19.50 ug/ml

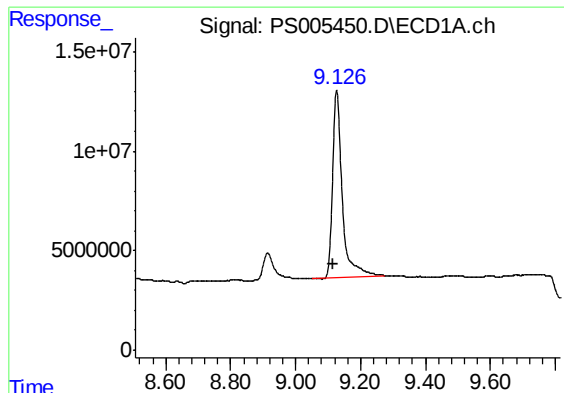

#15 Picloram

R.T.: 9.127 min
Delta R.T.: 0.010 min
Response: 194140684
Conc: 16.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

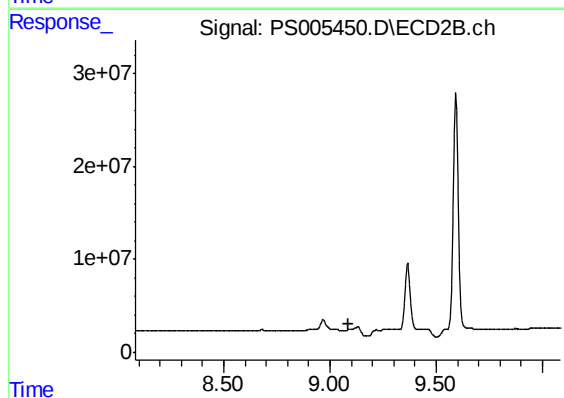

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.