

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
 Data File : PS005452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2019 16:44
 Operator : SM\AJ
 Sample : PB121263BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB121263BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 17:40:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 20 11:04:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.576	5.288	775.3E6	506.3E6	528.201	505.077
Target Compounds							
1) T	Dalapon	2.083	0.000	41503876	0	22.516	N.D. #
2) T	3,5-DICHL...	0.000	4.606	0	103.0E6	N.D.	78.133
3) T	4-Nitroph...	5.380	0.000	11813141	0	16.310	N.D. #
6) T	MCPD	0.000	5.562	0	19792838	N.D.	7.106
7) T	MCPA	6.069	5.679	9949878	24280653	1.584	5.994 #
9) T	2,4-D	0.000	6.173	0	33735422	N.D.	30.248
10) T	Pentachlo...	0.000	6.553	0	32877630	N.D.	2.557
11) T	2,4,5-TP ...	0.000	6.943	0	22228329	N.D.	4.174
12) T	2,4,5-T	7.591	7.400	104.8E6	24573898	13.028	4.818 #
15) T	Picloram	9.153	9.105	211.0E6	140.8E6	18.358	18.659
16) T	DCPA	0.000	9.105	0	140.8E6	N.D.	20.685



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071019\
Data File : PS005452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2019 16:44
Operator : SM\AJ
Sample : PB121263BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
PB121263BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 17:40:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS061919.M
Quant Title : 8080.M
QLast Update : Thu Jun 20 11:04:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

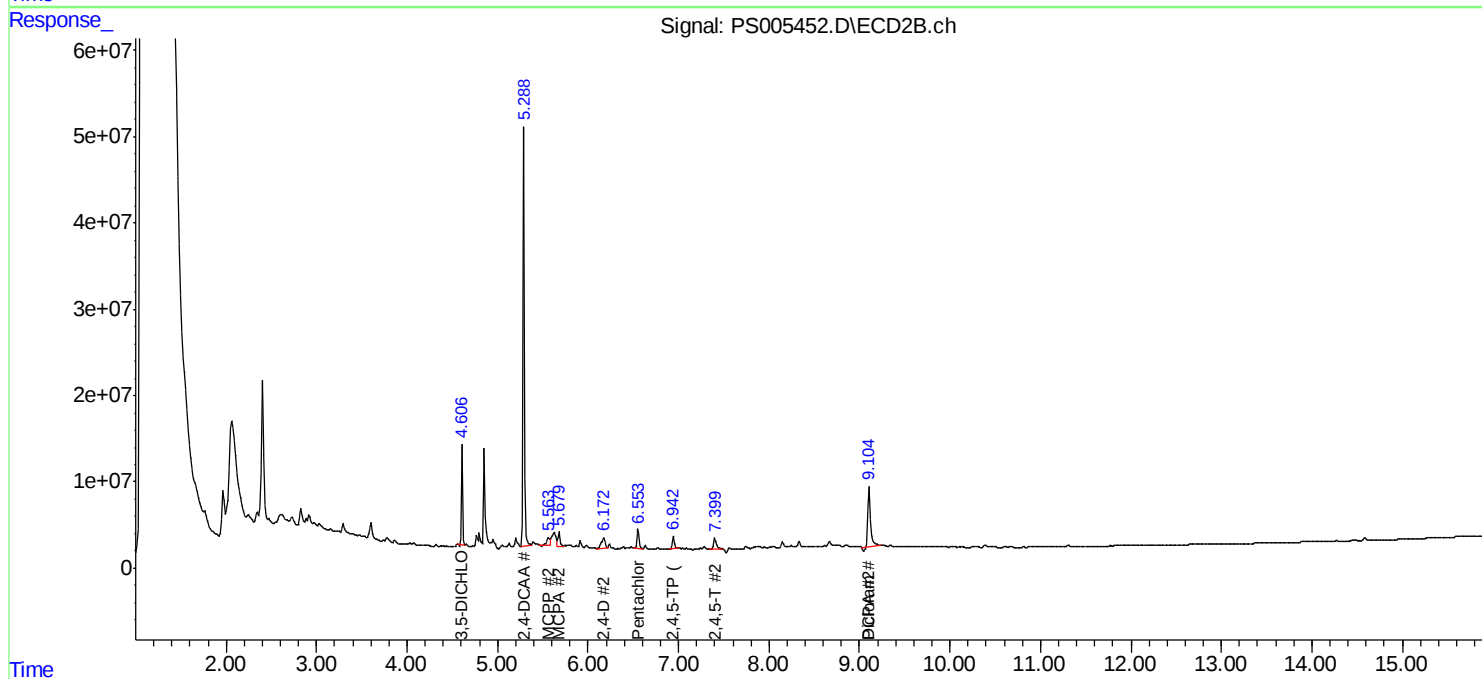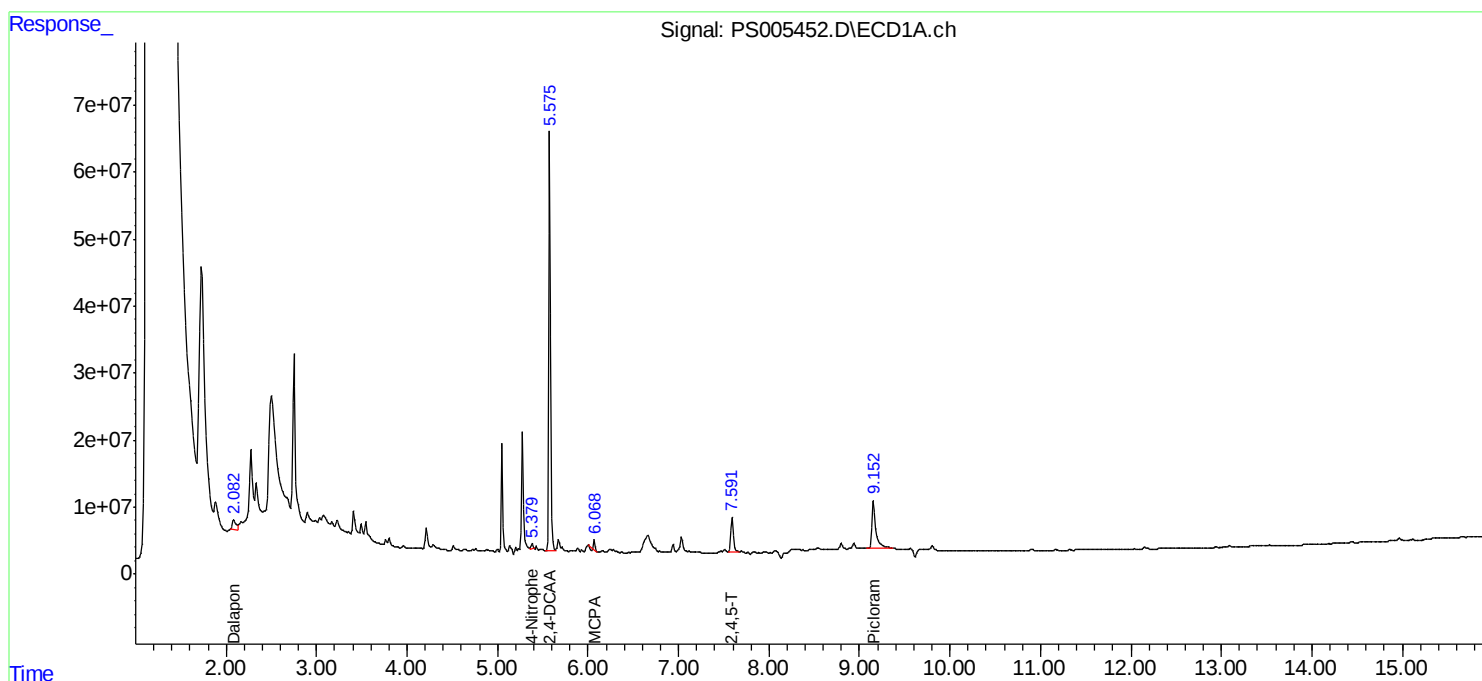


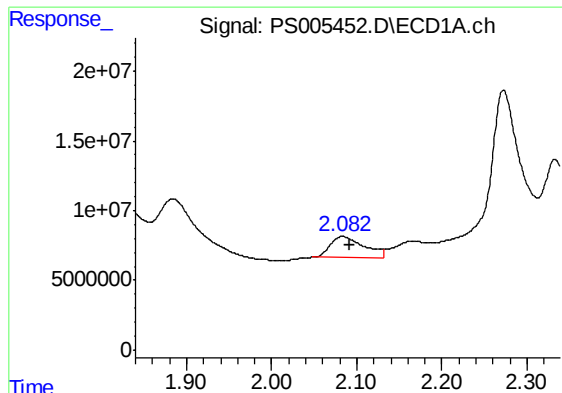

#1 Dalapon


R.T.: 2.083 min
Delta R.T.: -0.009 min
Response: 41503876
Conc: 22.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121263BL

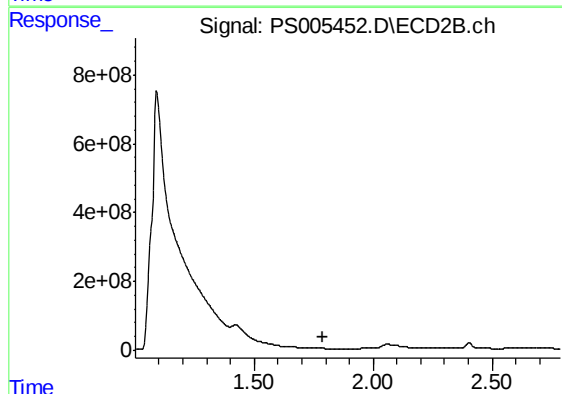


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.788 min
Response: 0
Conc: N.D.

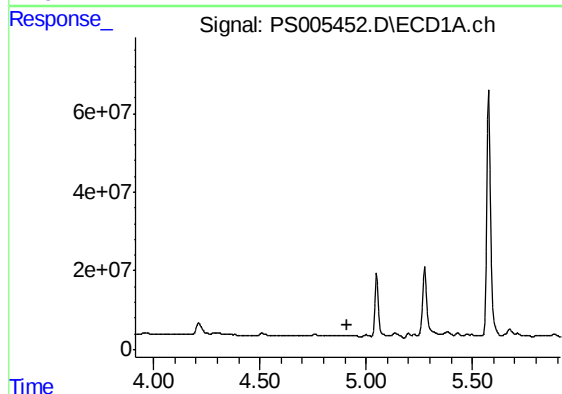


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.914 min
Response: 0
Conc: N.D.

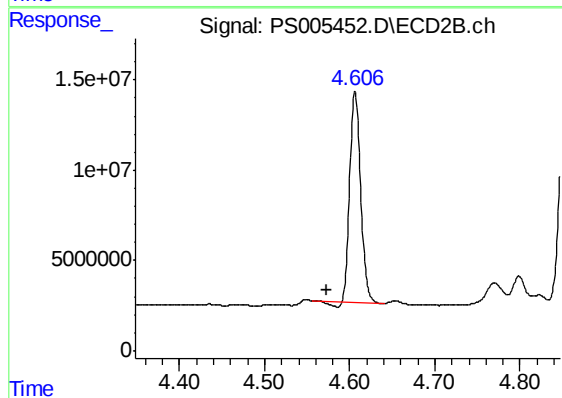

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.606 min
Delta R.T.: 0.034 min
Response: 103034325
Conc: 78.13 ng/ml

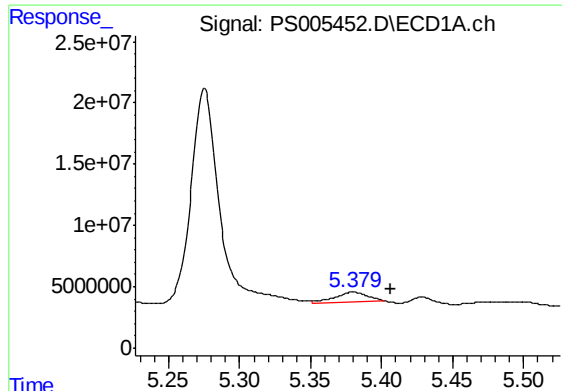

#3 4-Nitrophenol


R.T.: 5.380 min
Delta R.T.: -0.026 min
Response: 11813141
Conc: 16.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121263BL

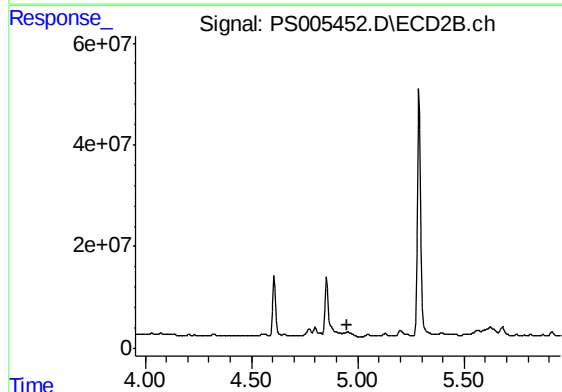


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.953 min
Response: 0
Conc: N.D.

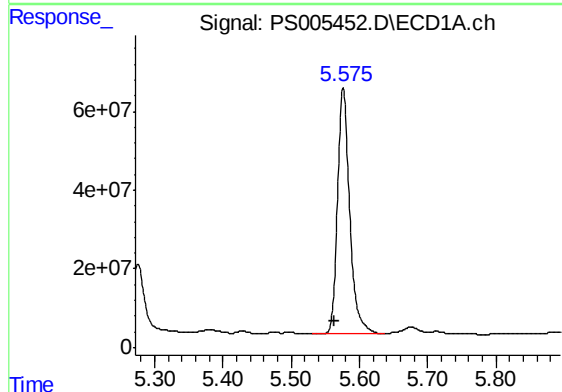


#4 2,4-DCAA

R.T.: 5.576 min
Delta R.T.: 0.012 min
Response: 775342830
Conc: 528.20 ng/ml

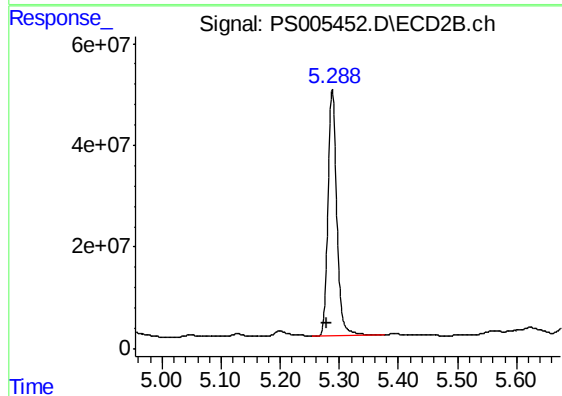

#4 2,4-DCAA


R.T.: 5.288 min
Delta R.T.: 0.009 min
Response: 506272955
Conc: 505.08 ng/ml

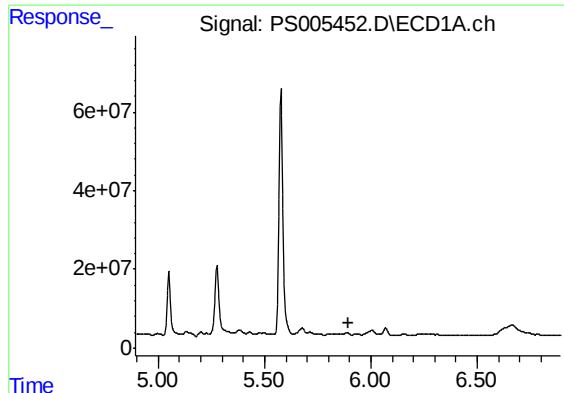

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.892 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121263BL

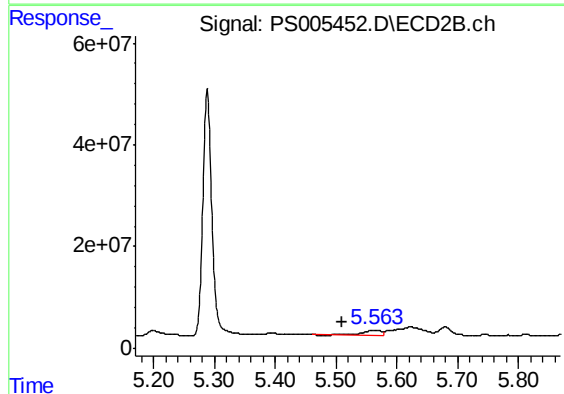


#6 MCPP

R.T.: 5.562 min
Delta R.T.: 0.052 min
Response: 19792838
Conc: 7.11 ug/ml

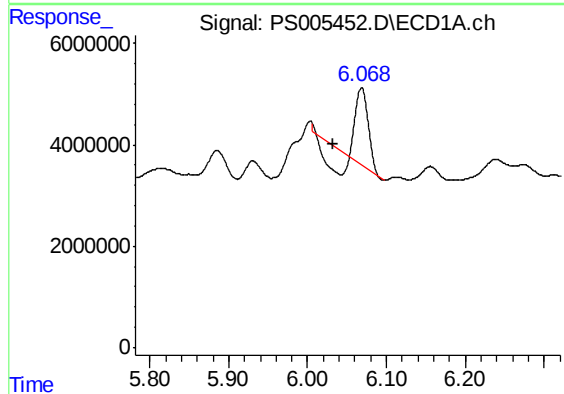


#7 MCPA

R.T.: 6.069 min
Delta R.T.: 0.036 min
Response: 9949878
Conc: 1.58 ug/ml

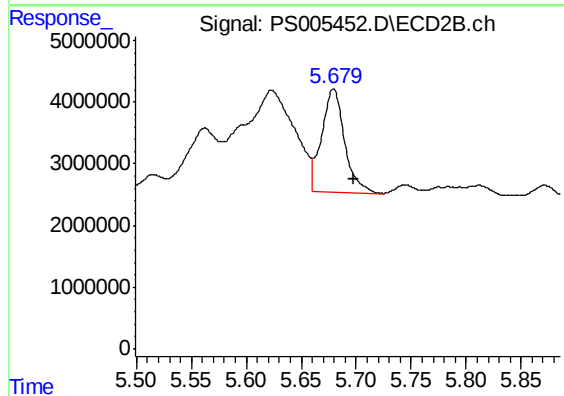

#7 MCPA


R.T.: 5.679 min
Delta R.T.: -0.018 min
Response: 24280653
Conc: 5.99 ug/ml

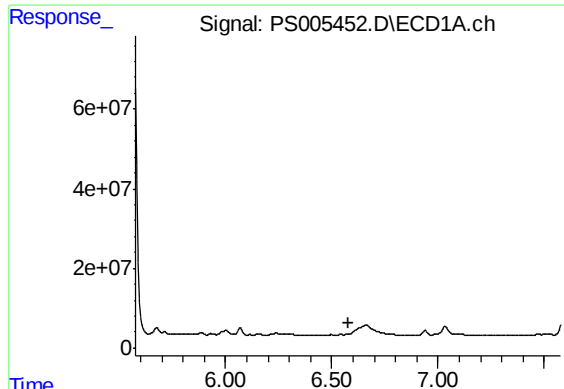

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.576 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121263BL

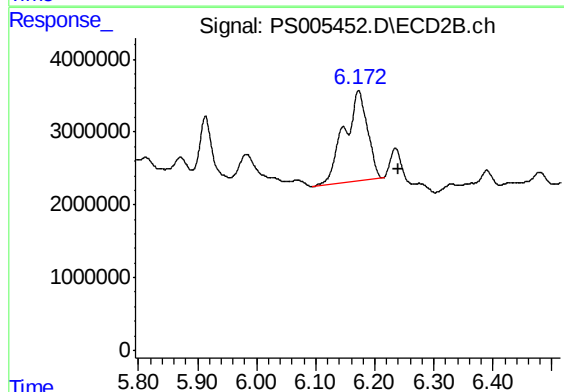


#9 2,4-D

R.T.: 6.173 min
Delta R.T.: -0.067 min
Response: 33735422
Conc: 30.25 ng/ml

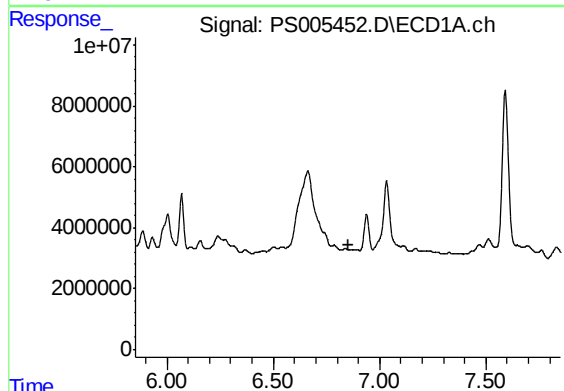


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.852 min
Response: 0
Conc: N.D.

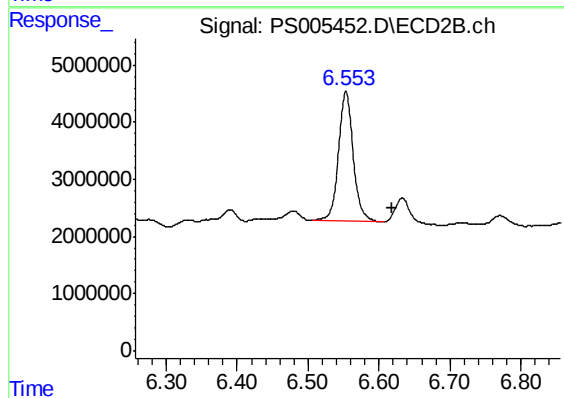

#10 Pentachlorophenol


R.T.: 6.553 min
Delta R.T.: -0.066 min
Response: 32877630
Conc: 2.56 ng/ml

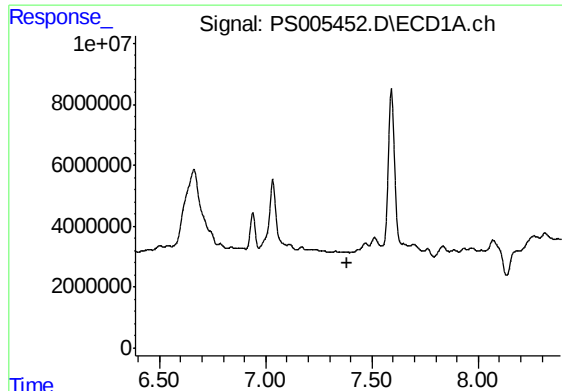

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB121263BL

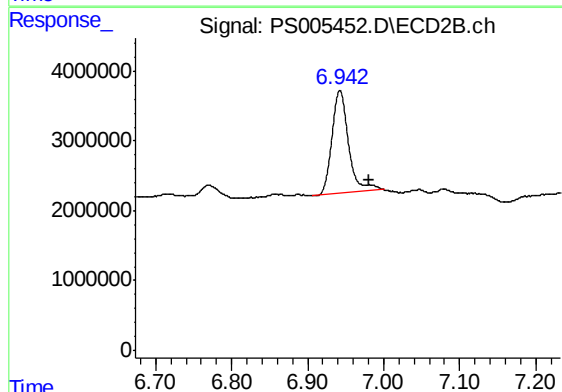


#11 2,4,5-TP (SILVEX)

R.T.: 6.943 min
Delta R.T.: -0.038 min
Response: 22228329
Conc: 4.17 ng/ml

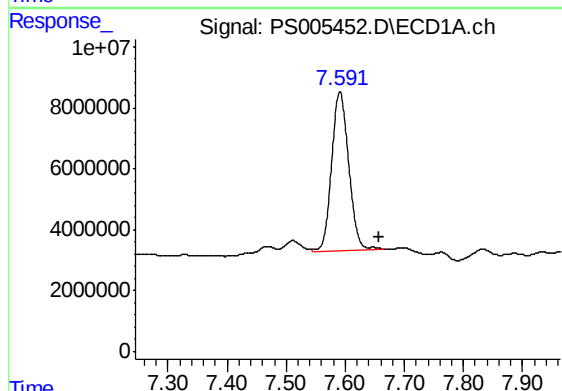


#12 2,4,5-T

R.T.: 7.591 min
Delta R.T.: -0.067 min
Response: 104844219
Conc: 13.03 ng/ml

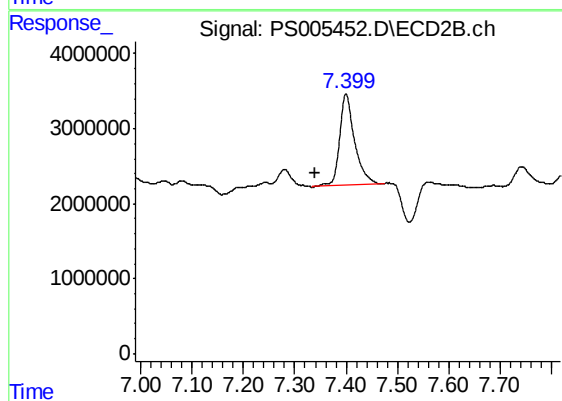

#12 2,4,5-T


R.T.: 7.400 min
Delta R.T.: 0.060 min
Response: 24573898
Conc: 4.82 ng/ml

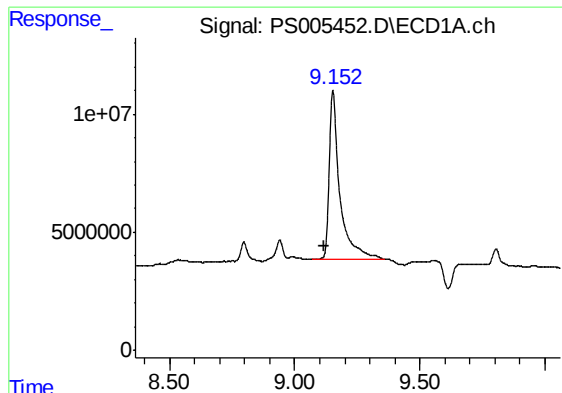

#15 Picloram


R.T.: 9.153 min
Delta R.T.: 0.036 min
Response: 210953389
Conc: 18.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB121263BL

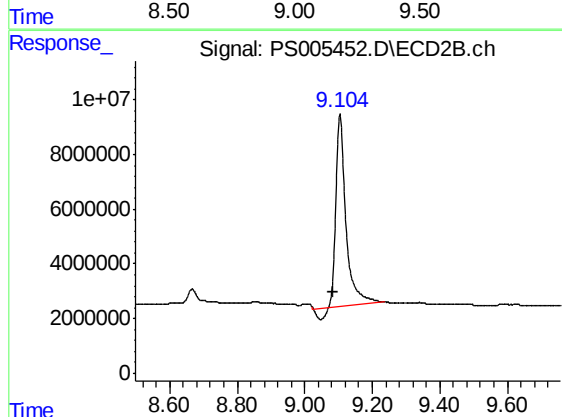


#15 Picloram

R.T.: 9.105 min
Delta R.T.: 0.020 min
Response: 140811937
Conc: 18.66 ng/ml

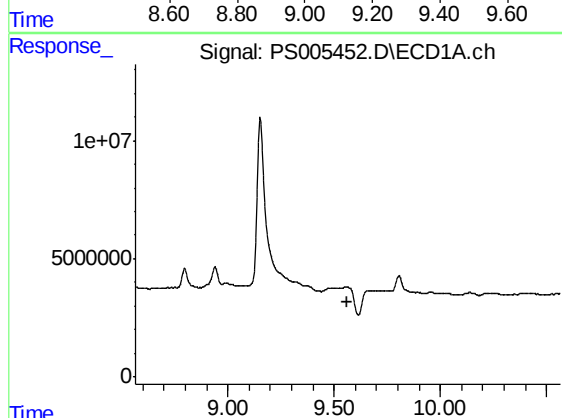

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.565 min
Response: 0
Conc: N.D.

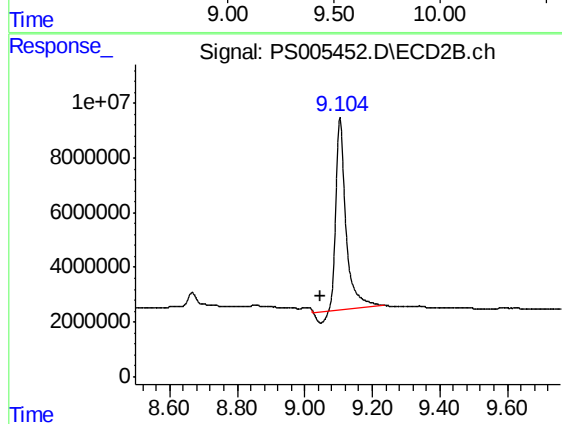

#16 DCPA

R.T.: 9.105 min
Delta R.T.: 0.059 min
Response: 140811937
Conc: 20.69 ng/ml