

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
 Data File : PS011157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 07:58
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 13:48:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.488	0.000	53471563	0	42.504	N.D. #
5) T	DICAMBA	0.000	7.152	0	49504337	N.D.	21.796
6) T	MCCP	0.000	7.152	0	49504337	N.D.	26.154
7) T	MCPA	7.683	0.000	22802692	0	5.726	N.D. #
8) T	DICHLORPROP	0.000	7.742	0	19321752	N.D.	32.909
9) T	2,4-D	0.000	8.047	0	245.0E6	N.D.	338.979
10) T	Pentachlo...	8.592	0.000	195.2E6	0	15.701	N.D. #
12) T	2,4,5-T	0.000	9.240	0	19387311	N.D.	6.510
15) T	Picloram	11.037	11.007	130.6E6	118.8E6	23.303	28.366
16) T	DCPA	0.000	11.007	0	118.8E6	N.D.	31.908



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
Data File : PS011157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 07:58
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 13:48:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

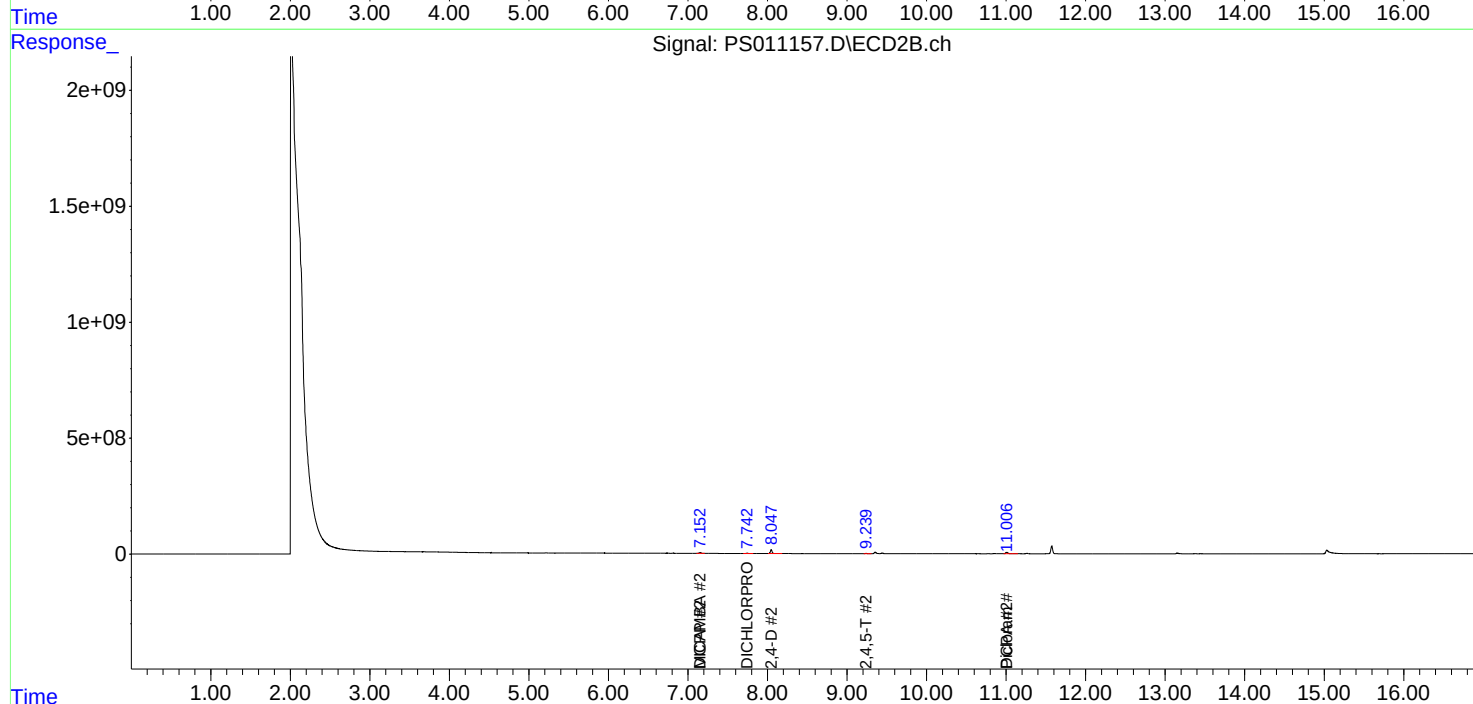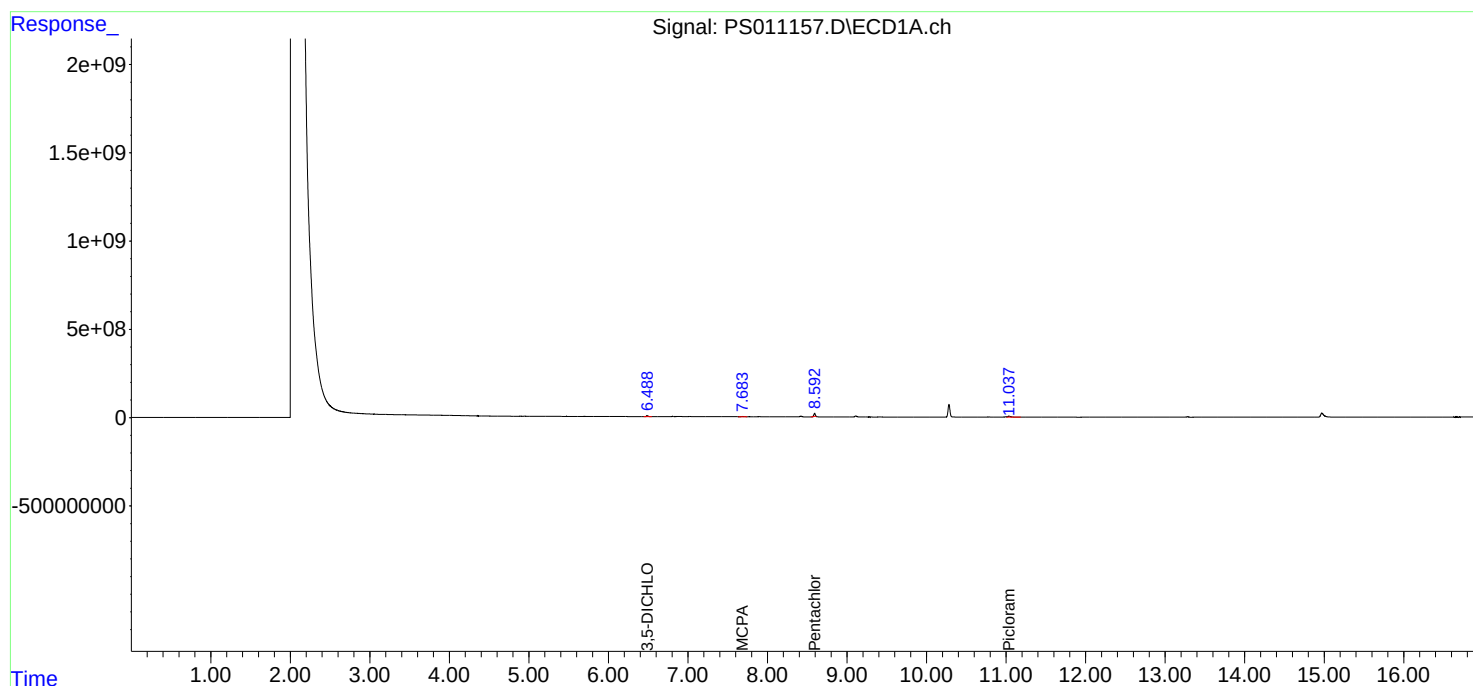


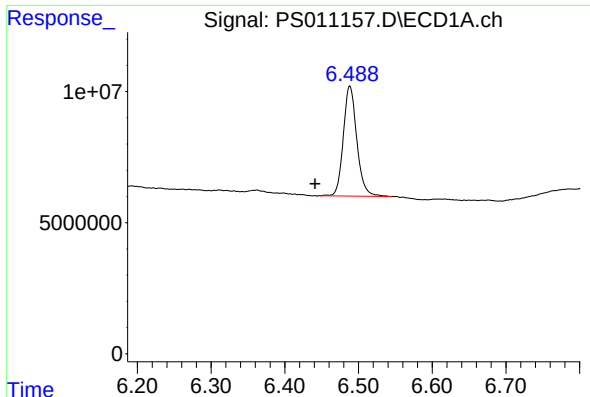

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.488 min
Delta R.T.: 0.047 min
Response: 53471563
Conc: 42.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

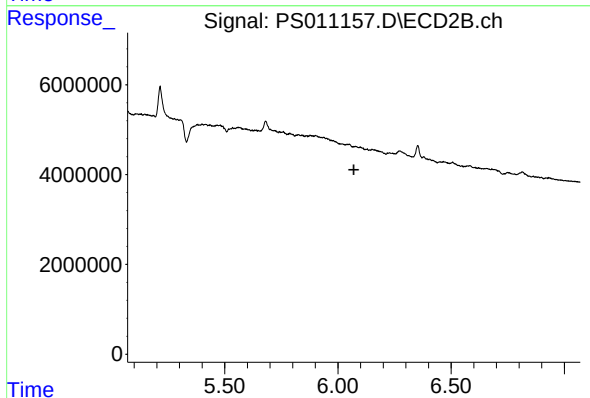


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

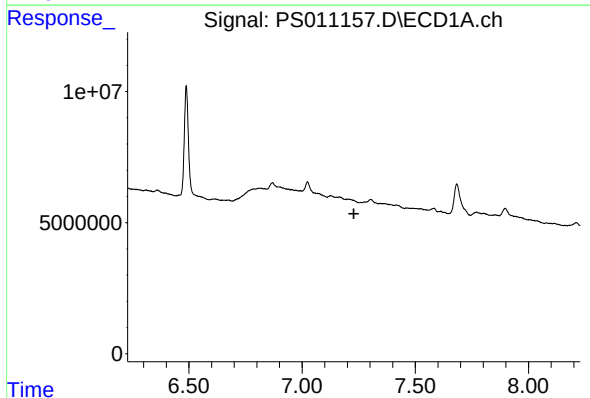


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.228 min
Response: 0
Conc: N.D.

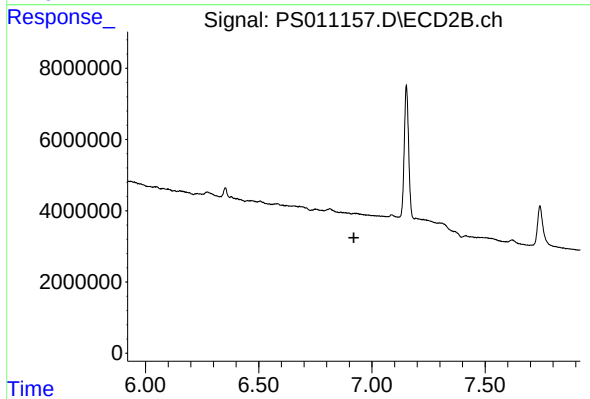

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.920 min
Response: 0
Conc: N.D.

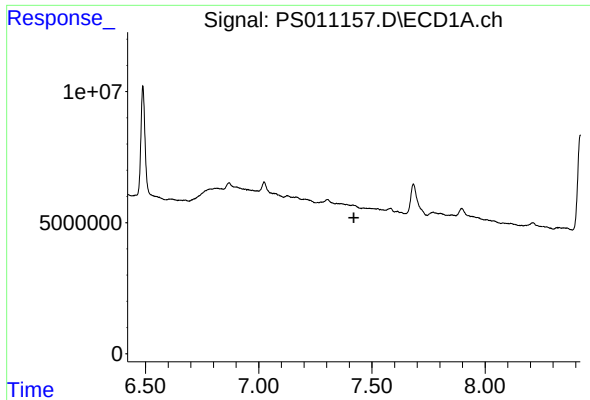

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

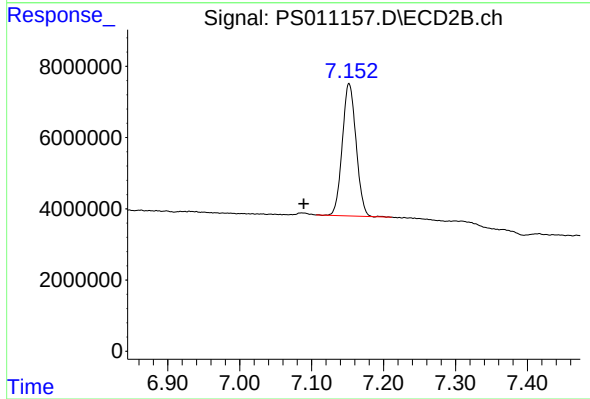


#5 DICAMBA

R.T.: 7.152 min
Delta R.T.: 0.063 min
Response: 49504337
Conc: 21.80 ng/ml

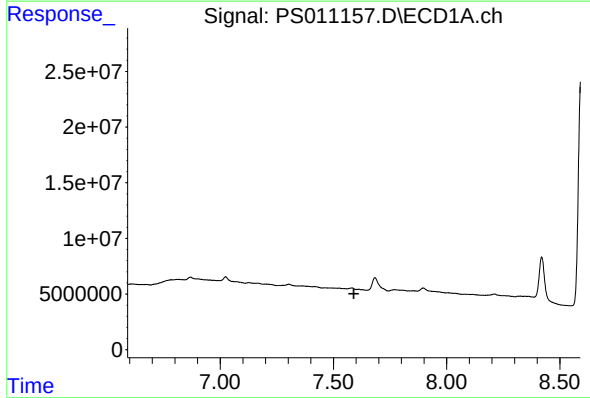


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.590 min
Response: 0
Conc: N.D.

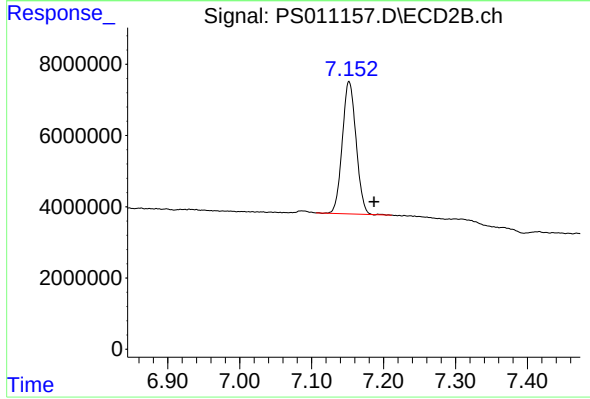

#6 MCP


R.T.: 7.152 min
Delta R.T.: -0.035 min
Response: 49504337
Conc: 26.15 ug/ml

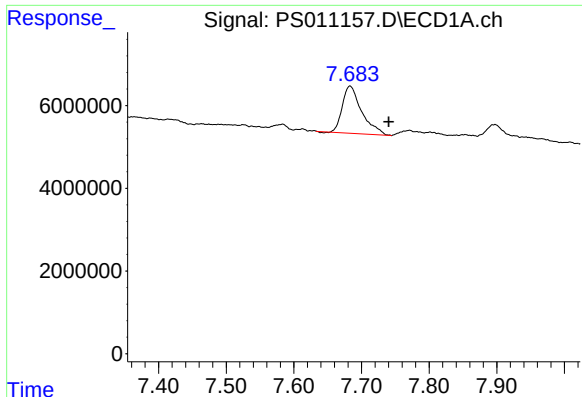

#7 MCPA


R.T.: 7.683 min
Delta R.T.: -0.057 min
Response: 22802692
Conc: 5.73 ug/ml

Instrument :
ECD_S
ClientSampleId :

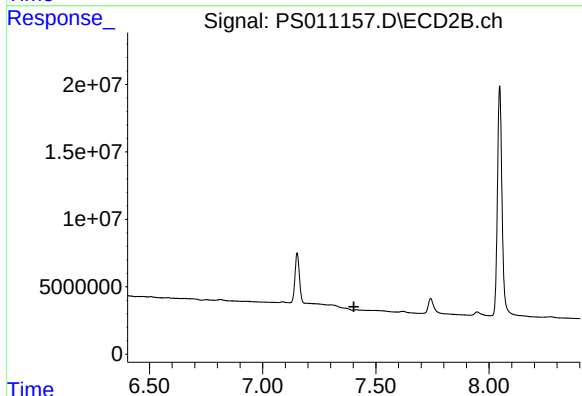


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.403 min
Response: 0
Conc: N.D.

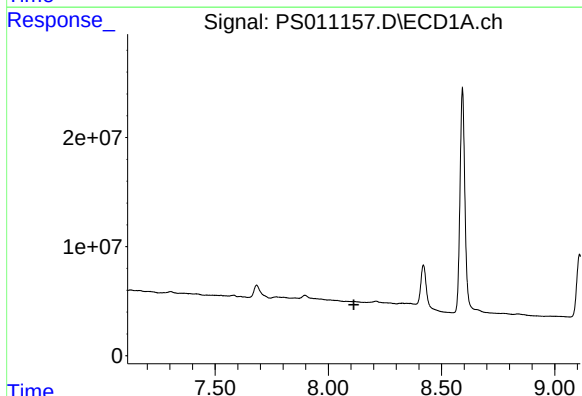


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.113 min
Response: 0
Conc: N.D.

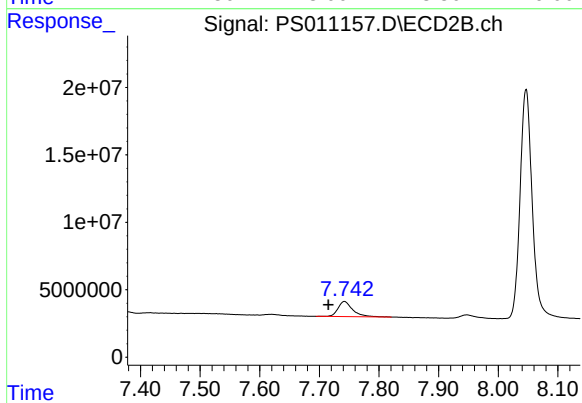

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.027 min
Response: 19321752
Conc: 32.91 ng/ml

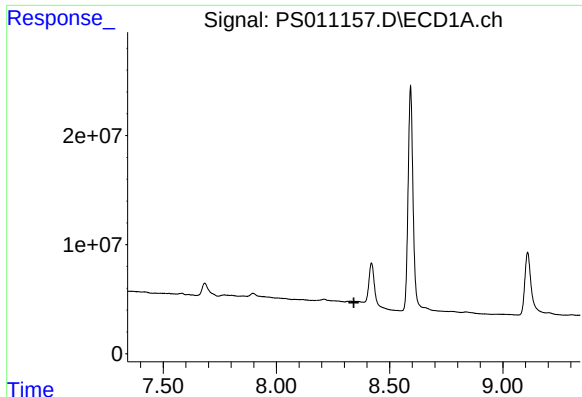

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

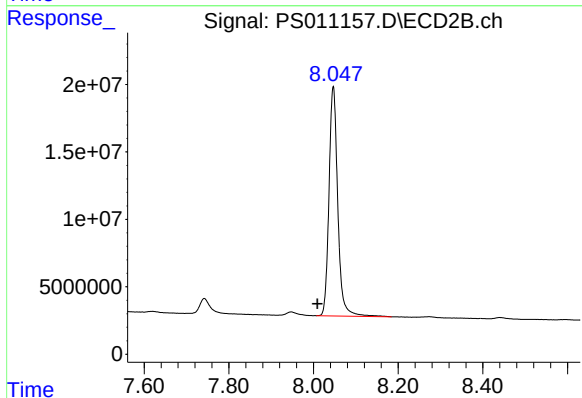


#9 2,4-D

R.T.: 8.047 min
Delta R.T.: 0.037 min
Response: 244964119
Conc: 338.98 ng/ml

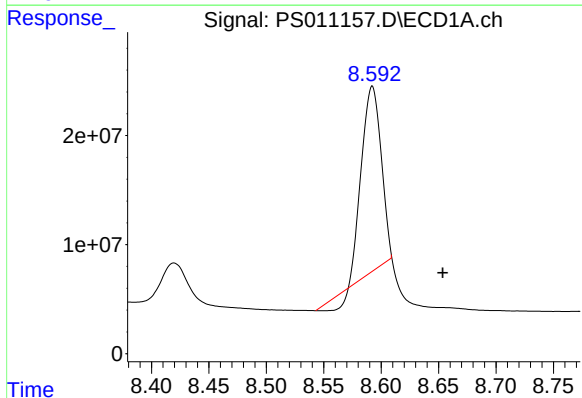


#10 Pentachlorophenol

R.T.: 8.592 min
Delta R.T.: -0.061 min
Response: 195233371
Conc: 15.70 ng/ml

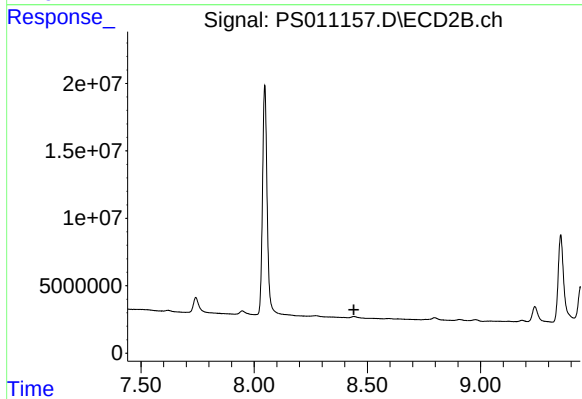

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.440 min
Response: 0
Conc: N.D.

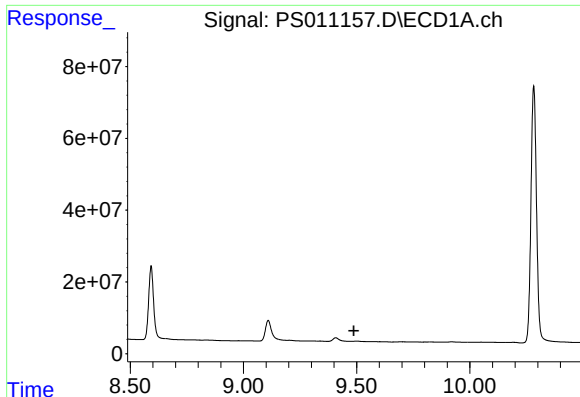

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.488 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

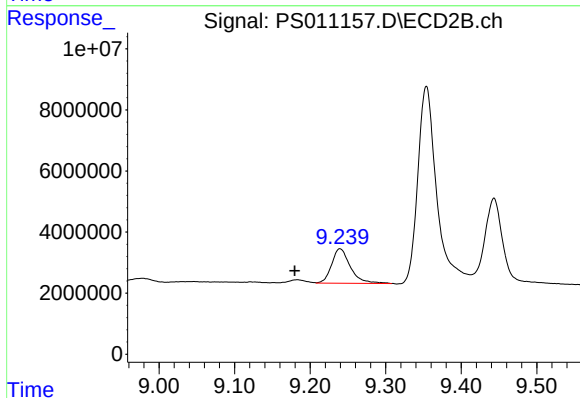


#12 2,4,5-T

R.T.: 9.240 min
Delta R.T.: 0.060 min
Response: 19387311
Conc: 6.51 ng/ml

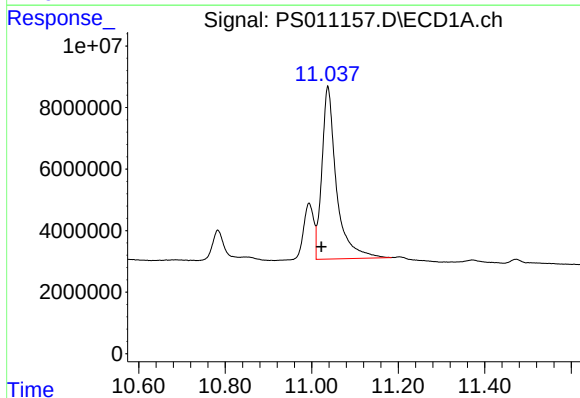


#15 Picloram

R.T.: 11.037 min
Delta R.T.: 0.015 min
Response: 130640996
Conc: 23.30 ng/ml

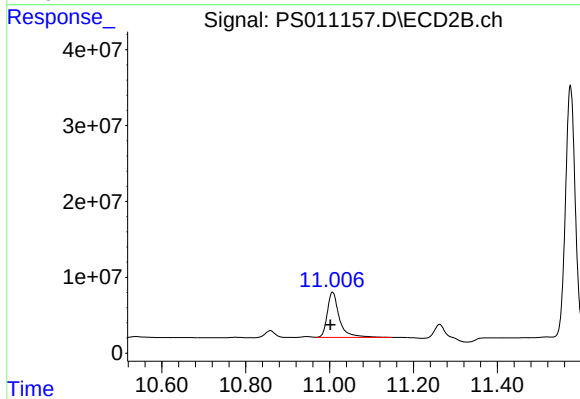

#15 Picloram


R.T.: 11.007 min
Delta R.T.: 0.005 min
Response: 118839353
Conc: 28.37 ng/ml

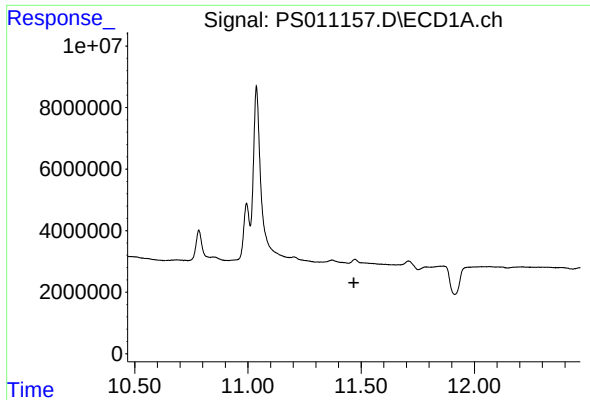

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.468 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

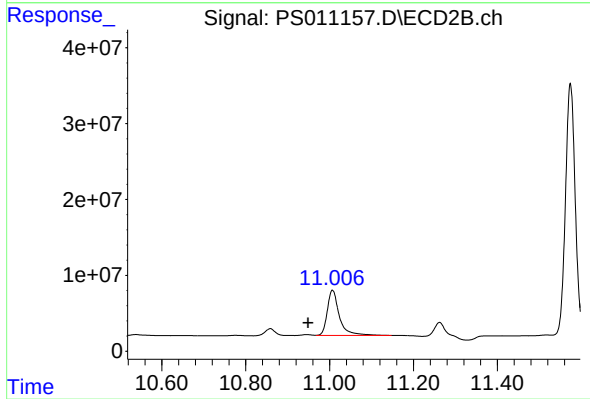

#16 DCPA

R.T.: 11.007 min
Delta R.T.: 0.058 min
Response: 118839353
Conc: 31.91 ng/ml