

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
 Data File : PS011161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 13:12
 Operator : DD\AJ
 Sample : L3203-13RE (Sig #1); L3203-13 RE (Sig #2)
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-06RE

Manual Integrations
 APPROVED

Ankita
 7/13/2020 11:39:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 00:21:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.920	1918.7E6	165.8E6	2115.906m	299.281 #
Target Compounds							
10) T	Pentachlo...	8.653	8.440	28033.0E6	12803.5E6	2254.516	1841.251

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
Data File : PS011161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 13:12
Operator : DD\AJ
Sample : L3203-13RE (Sig #1); L3203-13 RE (Sig #2)
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
RO-06RE


Manual Integrations
APPROVED

Ankita
7/13/2020 11:39:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 00:21:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

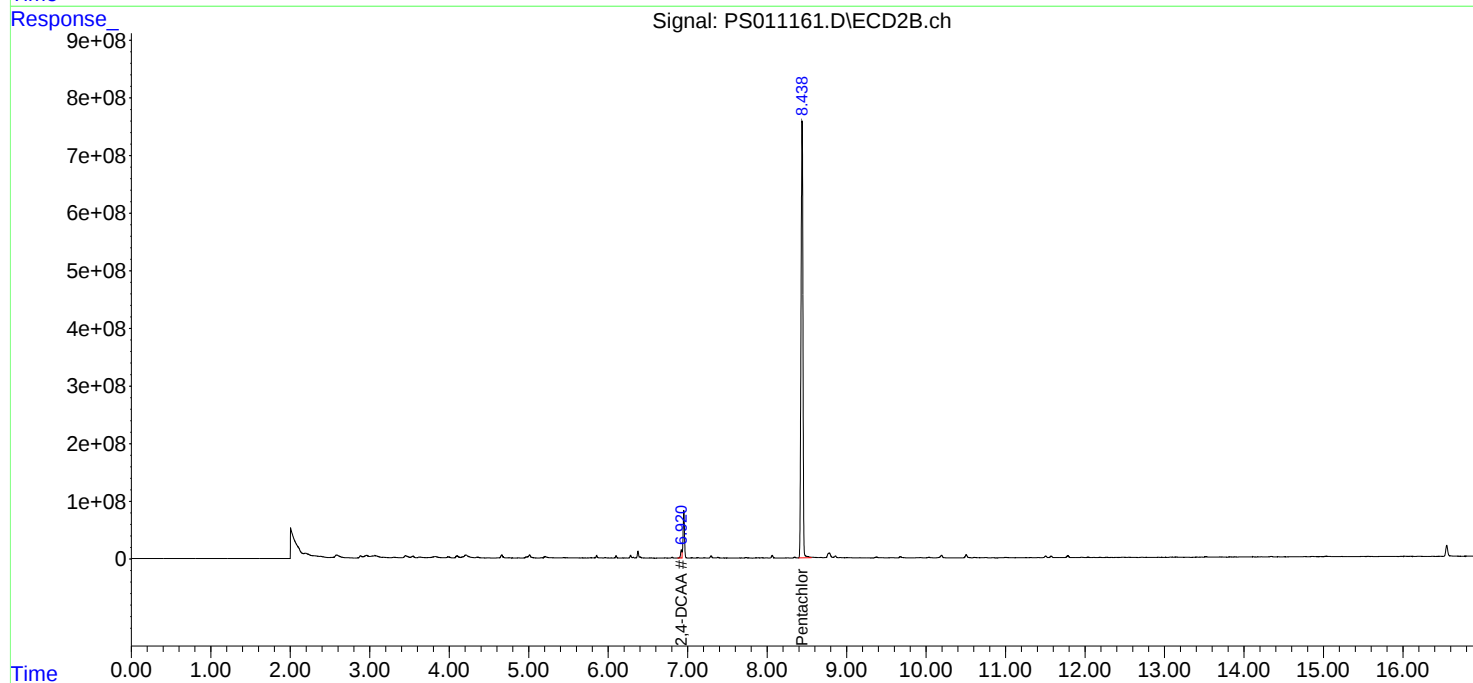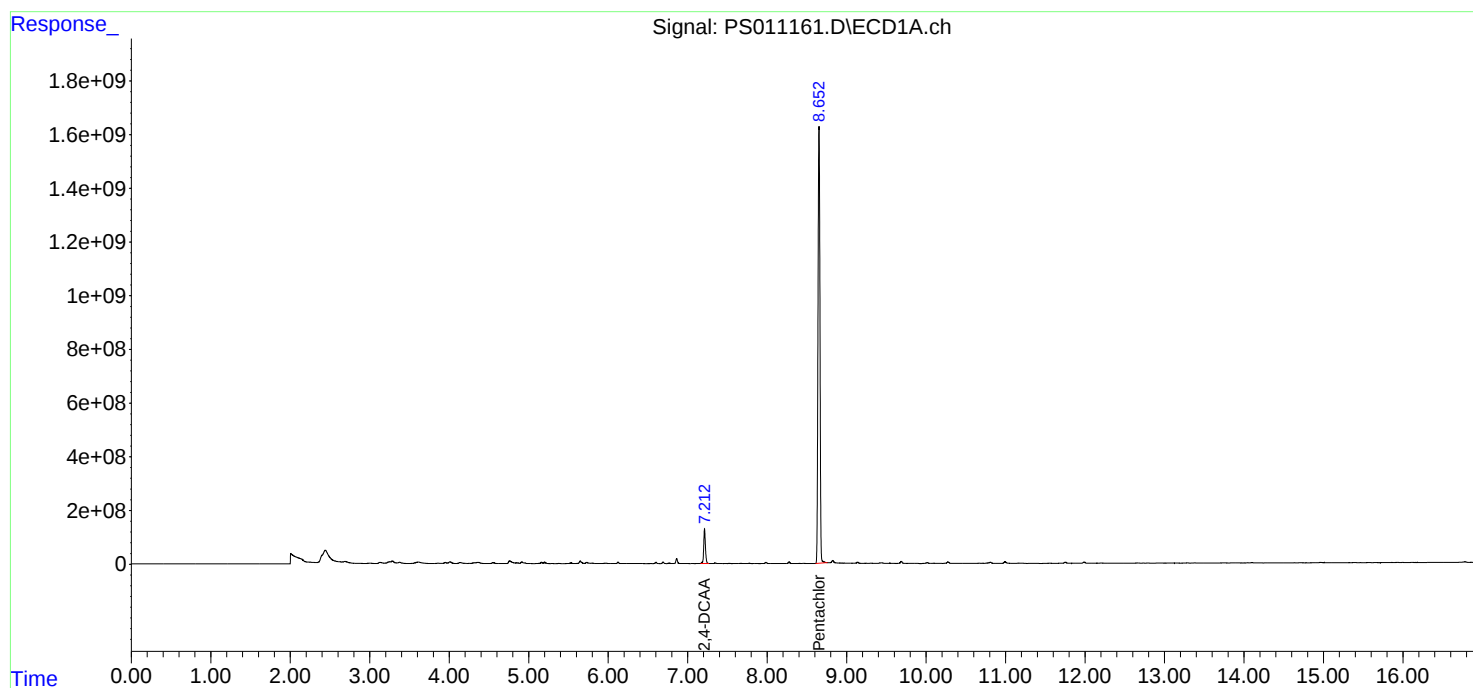

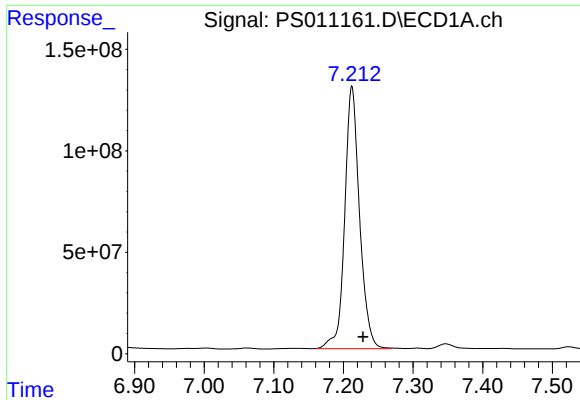


#4 2,4-DCAA

R.T.: 7.212 min
Delta R.T.: -0.017 min
Response: 1918742817
Conc: 2115.91 ng/ml m

Instrument :
ECD_S
ClientSampleId :
RO-06RE


Manual Integrations
APPROVED

Ankita
7/13/2020 11:39:18 AM

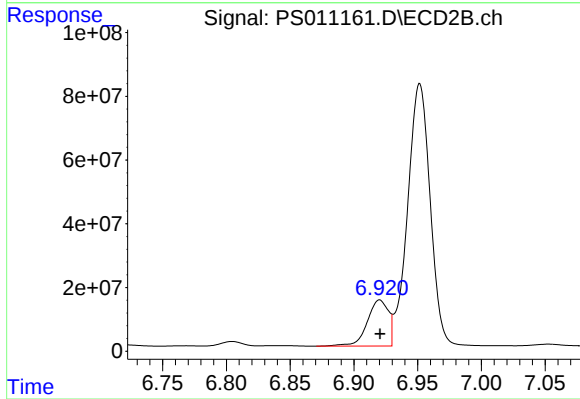


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 165824219
Conc: 299.28 ng/ml

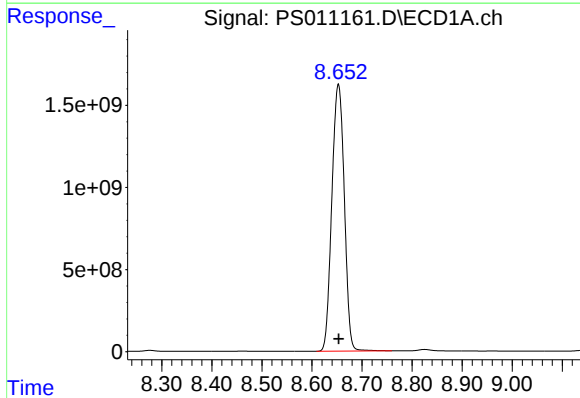

#10 Pentachlorophenol

R.T.: 8.653 min
Delta R.T.: 0.000 min
Response: 28033010087
Conc: 2254.52 ng/ml

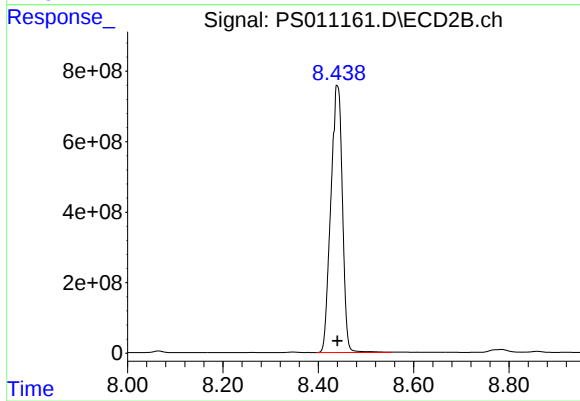

#10 Pentachlorophenol

R.T.: 8.440 min
Delta R.T.: 0.000 min
Response: 12803488020
Conc: 1841.25 ng/ml