

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
 Data File : PS011162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2020 13:35
 Operator : DD\AJ
 Sample : L3203-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-06

Manual Integrations
 APPROVED

Ankita
 7/13/2020 11:39:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 00:40:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
 Quant Title : 8080.M
 QLast Update : Thu Jun 25 02:45:12 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.920	756.1E6	285.9E6	833.772m	515.923 #
Target Compounds							
10) T	Pentachlo...	8.653	8.441	15349.0E6	7430.5E6	1234.419	1068.569

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS071020\
Data File : PS011162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2020 13:35
Operator : DD\AJ
Sample : L3203-15
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
7/13/2020 11:39:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 00:40:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS062420.M
Quant Title : 8080.M
QLast Update : Thu Jun 25 02:45:12 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

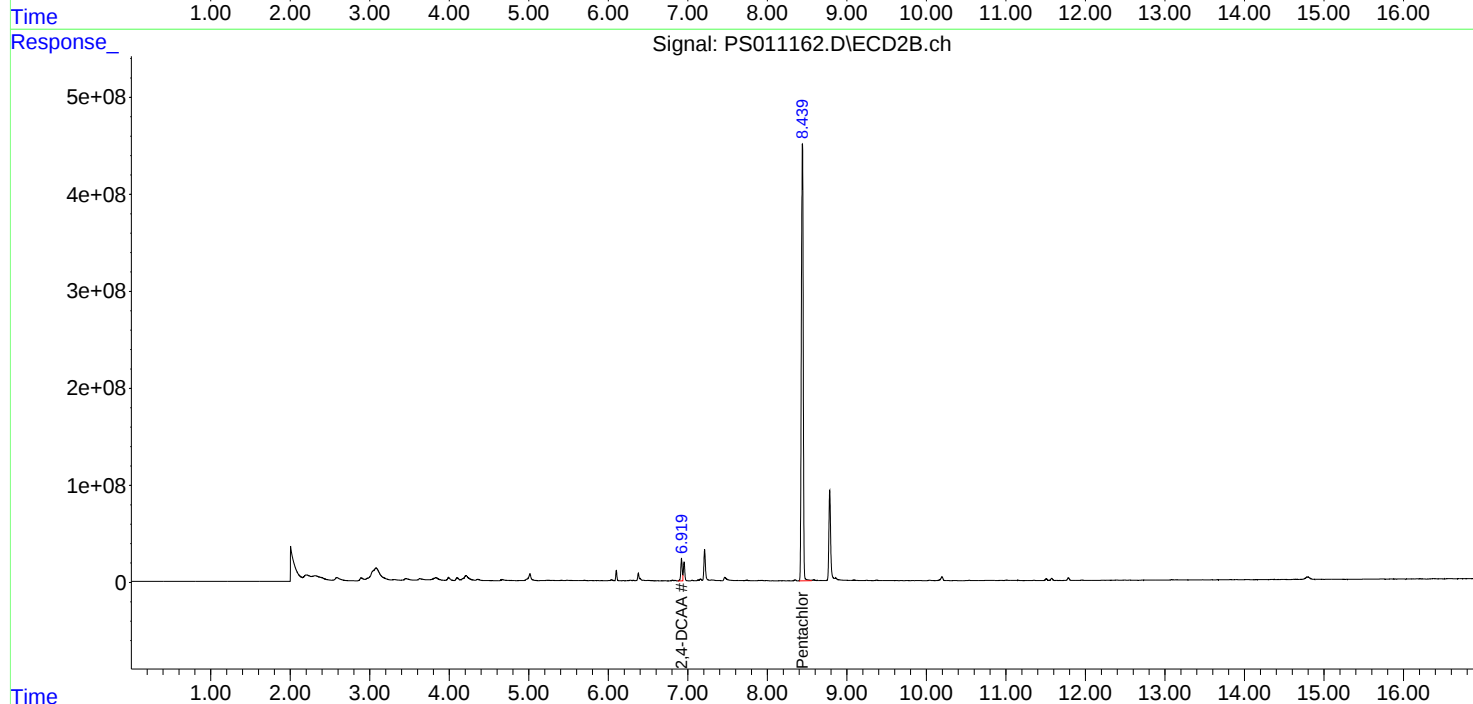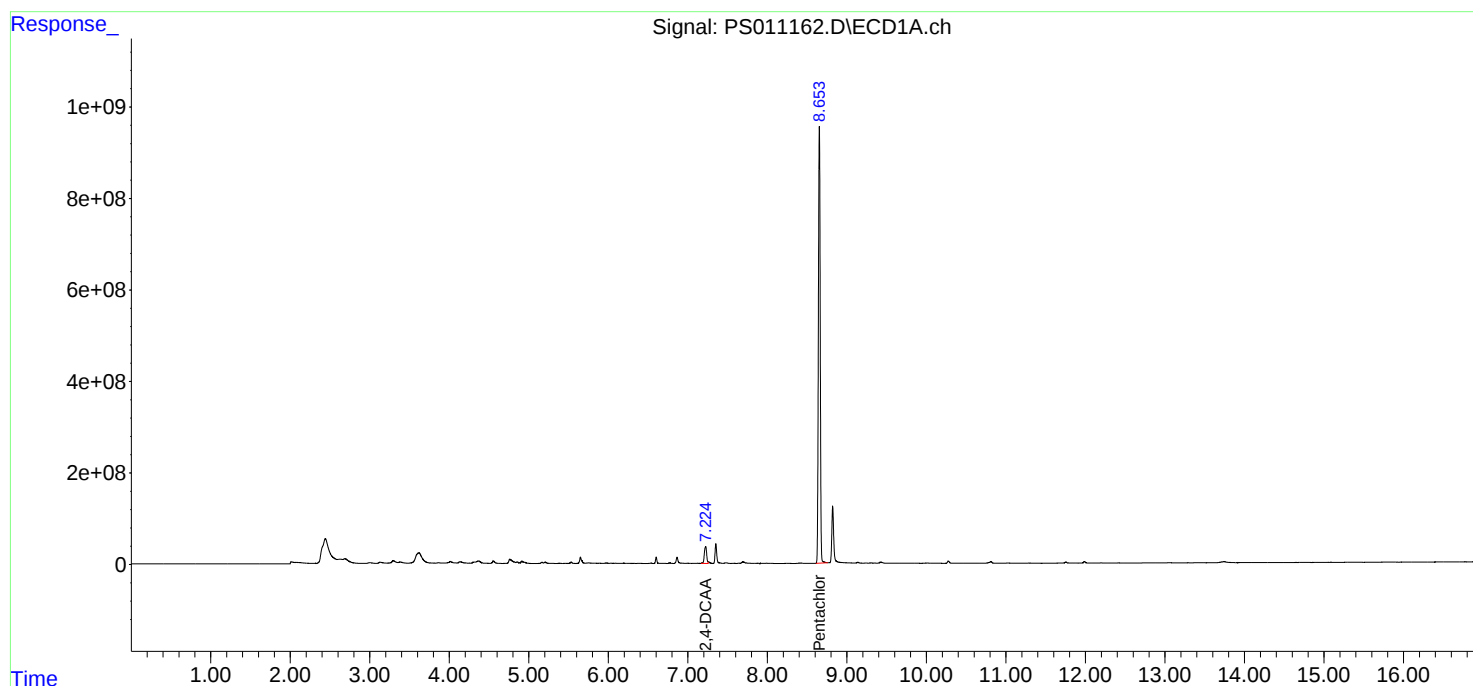

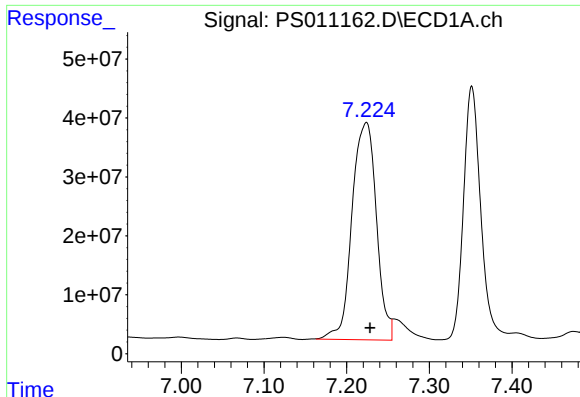


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: -0.005 min
Response: 756080305
Conc: 833.77 ng/ml m

Instrument :
ECD_S
ClientSampleId :
RO-06


Manual Integrations
APPROVED

Ankita
7/13/2020 11:39:20 AM

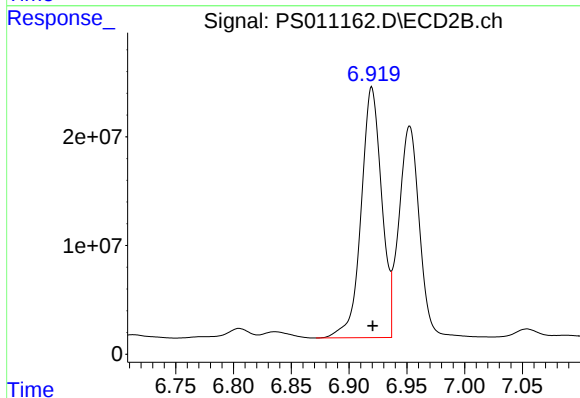


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 285860750
Conc: 515.92 ng/ml

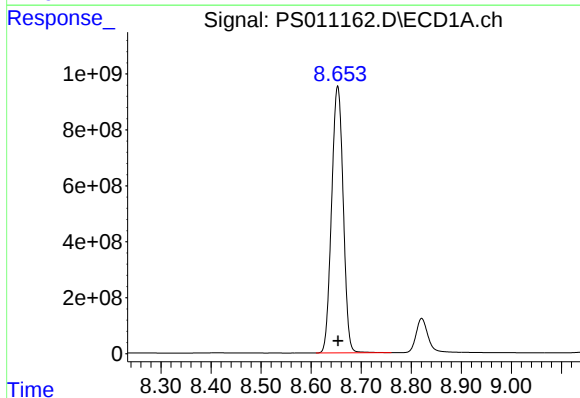

#10 Pentachlorophenol

R.T.: 8.653 min
Delta R.T.: 0.000 min
Response: 15348959136
Conc: 1234.42 ng/ml

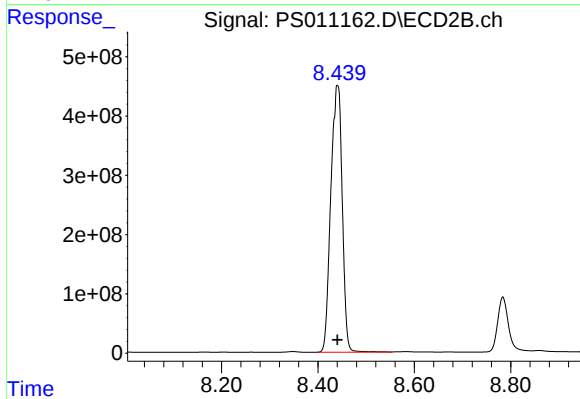

#10 Pentachlorophenol

R.T.: 8.441 min
Delta R.T.: 0.000 min
Response: 7430496027
Conc: 1068.57 ng/ml