

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071118\
Data File : FG001628.D
Signal(s) : FID1A.ch
Acq On : 11 Jul 2018 12:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 12 07:58:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.279	2736033	20.800 ug/ml
12)	N-OCTACOSANE	16.694	2688796	20.567 ug/ml
13)	N-TRIACONTANE	17.581	204238	1.568 ug/ml
14)	N-DOTRIACONTANE	18.416	279434	2.195 ug/ml
15)	N-TETRATRIACONTANE	19.202	202574	1.609 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG071118\
Data File : FG001628.D
Signal(s) : FID1A.ch
Acq On : 11 Jul 2018 12:31
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 12 07:58:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

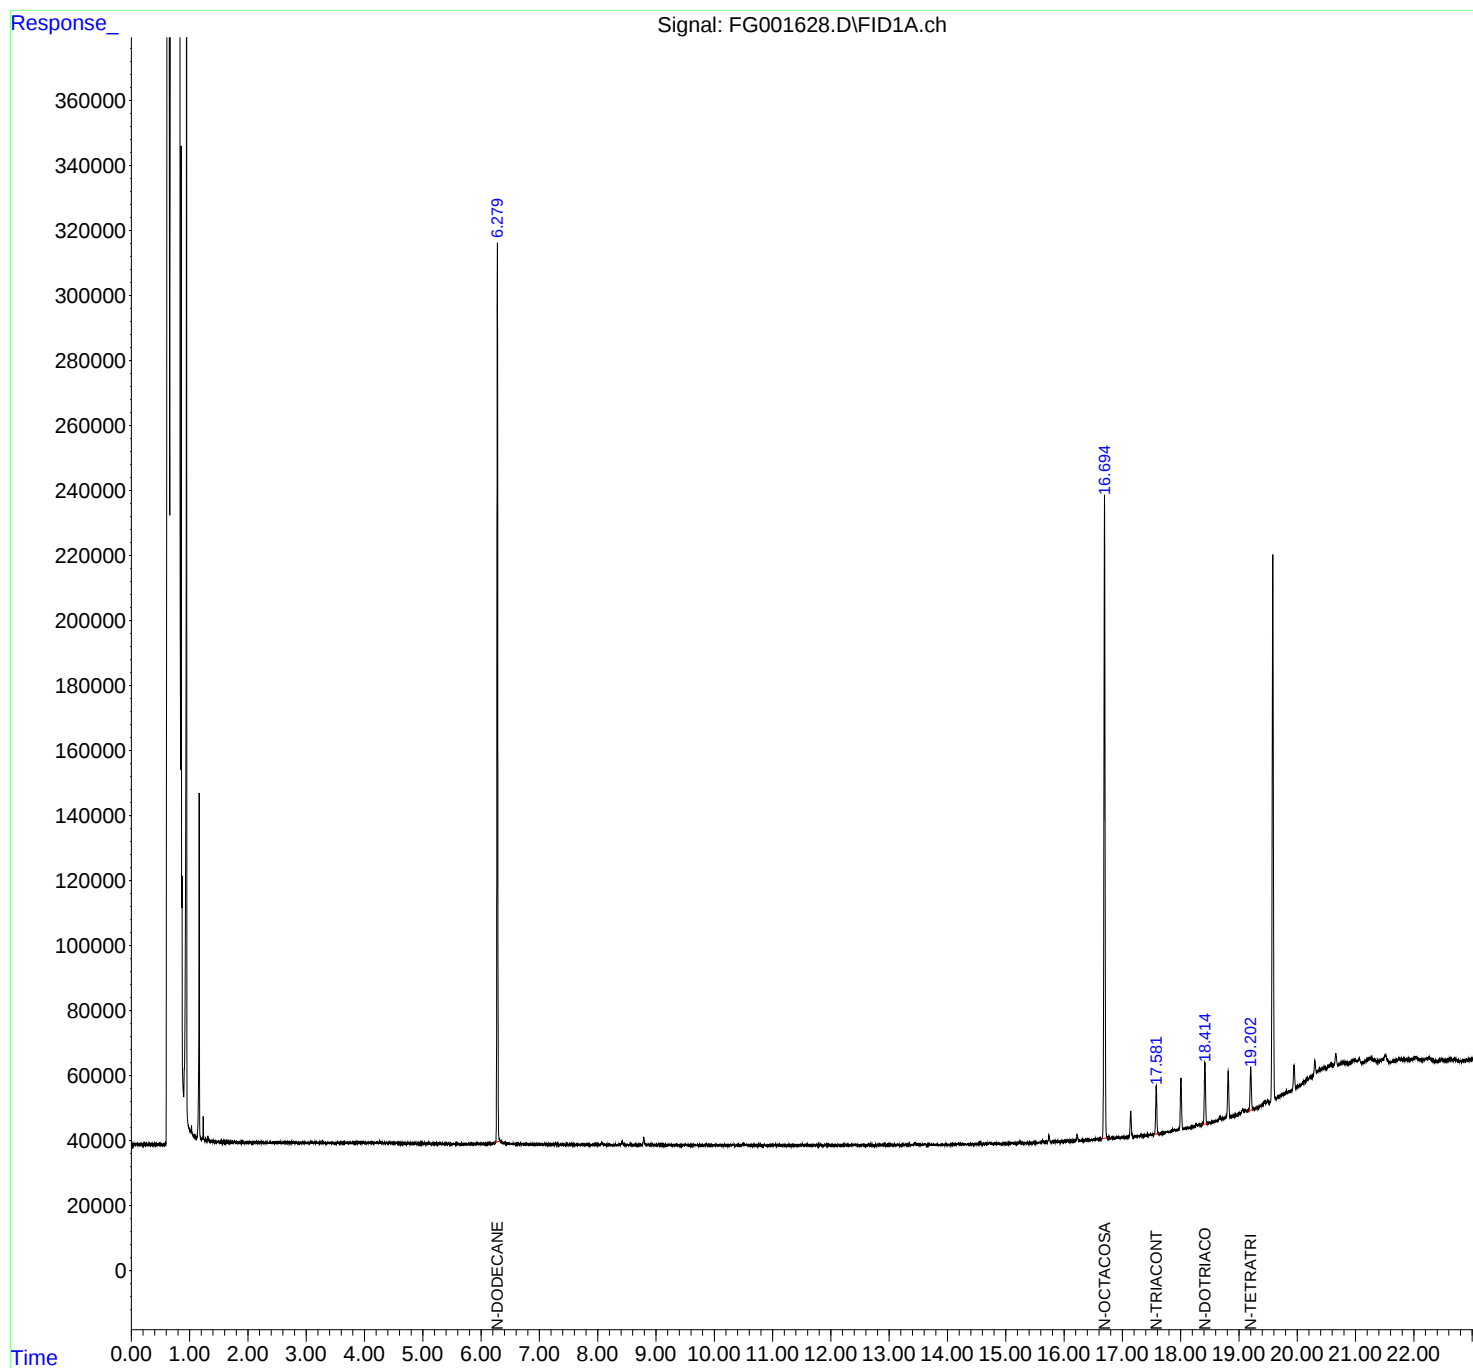


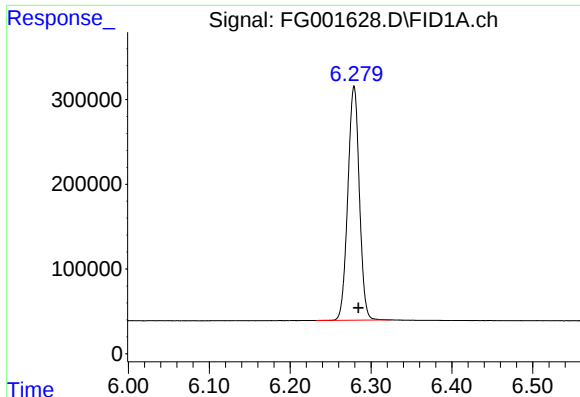

#3 N-DODECANE


R.T.: 6.279 min
Delta R.T.: -0.005 min
Response: 2736033
Conc: 20.80 ug/ml

Instrument :
ECD_S
ClientSampleId :

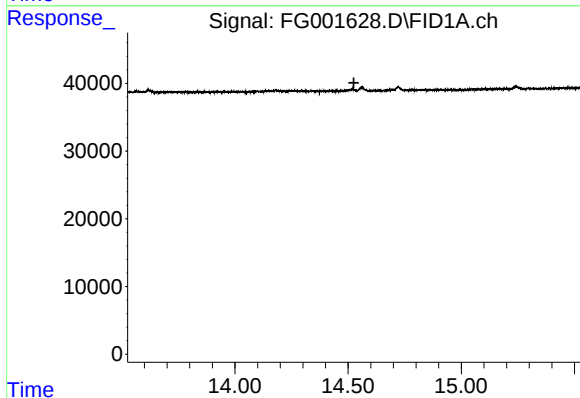


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.525 min
Response: 0
Conc: N.D.

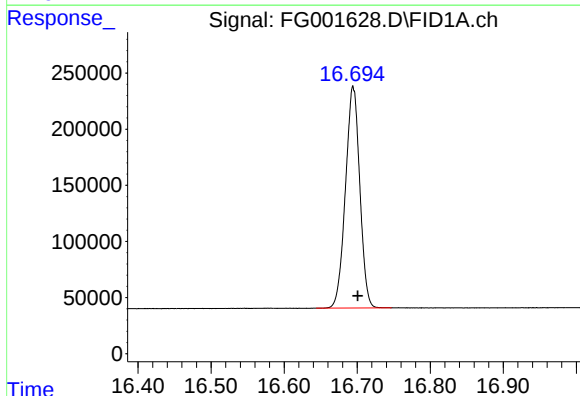


#12 N-OCTACOSANE

R.T.: 16.694 min
Delta R.T.: -0.006 min
Response: 2688796
Conc: 20.57 ug/ml

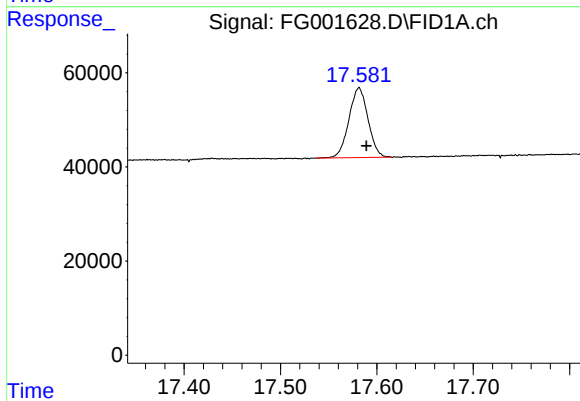

#13 N-TRIACONTANE


R.T.: 17.581 min
Delta R.T.: -0.008 min
Response: 204238
Conc: 1.57 ug/ml

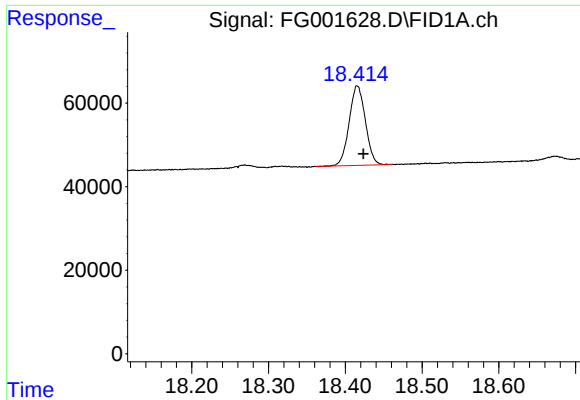

#14 N-DOTRIACONTANE

R.T.: 18.416 min
Delta R.T.: -0.008 min
Response: 279434
Conc: 2.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

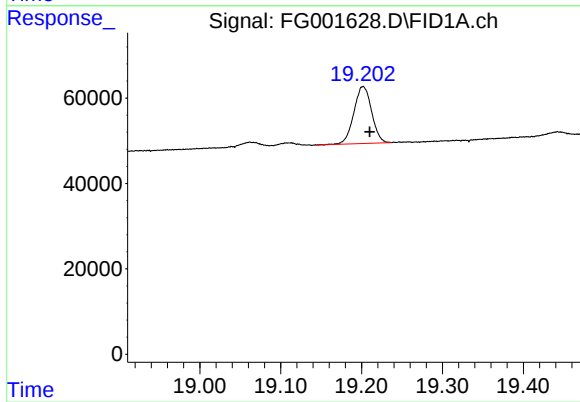

#15 N-TETRATRIACONTANE

R.T.: 19.202 min
Delta R.T.: -0.008 min
Response: 202574
Conc: 1.61 ug/ml